

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010725\
 Data File : VX044602.D
 Acq On : 07 Jan 2025 12:23
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Jan 08 05:52:12 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010725W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 08 03:57:12 2025
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 01/08/2025
 Supervised By : Mahesh Dadoda 01/08/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	167454	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	306306	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	275086	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	127489	50.000	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	5.946	65	141098	52.259	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	104.520%
35) Dibromofluoromethane	5.379	113	103080	49.077	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.160%
50) Toluene-d8	8.647	98	379423	52.885	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	105.780%
62) 4-Bromofluorobenzene	11.079	95	145063	57.285	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	114.560%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.167	85	873	0.360	ug/l	71
3) Chloromethane	1.295	50	964	0.399	ug/l	98
4) Vinyl Chloride	1.374	62	937	0.414	ug/l	94
5) Bromomethane	1.599	94	1089	0.928	ug/l	91
7) Trichlorofluoromethane	1.874	101	1216	0.361	ug/l #	68
9) 1,1,2-Trichlorotrifluo...	2.325	101	760	0.393	ug/l #	76
10) Methyl Iodide	2.447	142	1454	0.539	ug/l #	88
12) 1,1-Dichloroethene	2.313	96	1178	0.629	ug/l #	92
13) Acrolein	2.233	56	1073	2.441	ug/l	99
14) Allyl chloride	2.660	41	1302	0.418	ug/l	90
15) Acrylonitrile	3.069	53	2357	2.462	ug/l	97
16) Acetone	2.374	43	2223	2.612	ug/l #	88
17) Carbon Disulfide	2.502	76	7335	1.894	ug/l	99
18) Methyl Acetate	2.709	43	1333	0.531	ug/l #	79
20) Methylene Chloride	2.788	84	890	0.410	ug/l #	86
21) trans-1,2-Dichloroethene	3.093	96	1777	0.924	ug/l #	77
29) Tetrahydrofuran	5.038	42	1399m	1.663	ug/l	
30) Chloroform	5.087	83	1141	0.284	ug/l	84
31) Cyclohexane	5.465	56	817	0.267	ug/l #	80
36) 1,1-Dichloropropene	5.702	75	1609	0.592	ug/l #	53
39) Methylcyclohexane	7.379	83	999	0.288	ug/l	86
40) Benzene	6.044	78	2278	0.266	ug/l	91
44) Trichloroethene	7.123	130	1311m	0.600	ug/l	
46) Dibromomethane	7.586	93	717	0.442	ug/l	94
51) 4-Methyl-2-Pentanone	8.586	43	2802	1.046	ug/l	96
52) Toluene	8.720	92	1859	0.360	ug/l	90
53) t-1,3-Dichloropropene	8.994	75	1282	0.455	ug/l #	88
54) cis-1,3-Dichloropropene	8.379	75	1243	0.392	ug/l #	79
55) 1,1,2-Trichloroethane	9.165	97	540	0.267	ug/l #	81
57) 1,3-Dichloropropane	9.317	76	890	0.262	ug/l #	78
58) 2-Chloroethyl Vinyl ether	8.257	63	1166	0.800	ug/l #	69
59) 2-Hexanone	9.445	43	1881	0.993	ug/l	87
61) 1,2-Dibromoethane	9.622	107	722	0.353	ug/l	98
64) Tetrachloroethene	9.275	164	1363	0.701	ug/l	88
65) Chlorobenzene	10.073	112	2848	0.488	ug/l	97
67) Ethyl Benzene	10.195	91	4025	0.401	ug/l #	82

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010725\
 Data File : VX044602.D
 Acq On : 07 Jan 2025 12:23
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Manual Integrations
 APPROVED

Reviewed By : John Carlone 01/08/2025
 Supervised By : Mahesh Dadoda 01/08/2025

Quant Time: Jan 08 05:52:12 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010725W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 08 03:57:12 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

68) m/p-Xylenes	10.305	106	3323	0.902	ug/l	93
69) o-Xylene	10.647	106	1604	0.431	ug/l	86
70) Styrene	10.665	104	2627	0.442	ug/l	95
73) Isopropylbenzene	10.964	105	3650	0.386	ug/l	93
74) N-amyl acetate	10.854	43	1166	0.304	ug/l #	80
75) 1,1,2,2-Tetrachloroethane	11.213	83	1108	0.364	ug/l #	87
77) Bromobenzene	11.195	156	1502	0.655	ug/l	95
78) n-propylbenzene	11.305	91	5695	0.535	ug/l	84
79) 2-Chlorotoluene	11.366	91	3274	0.475	ug/l	83
80) 1,3,5-Trimethylbenzene	11.451	105	3965	0.506	ug/l	99
82) 4-Chlorotoluene	11.463	91	5023	0.648	ug/l	95
83) tert-Butylbenzene	11.713	119	3594	0.461	ug/l	92
84) 1,2,4-Trimethylbenzene	11.750	105	4316	0.549	ug/l	99
85) sec-Butylbenzene	11.890	105	5402	0.569	ug/l	94
86) p-Isopropyltoluene	12.006	119	4207	0.528	ug/l	86
87) 1,3-Dichlorobenzene	11.969	146	4050	0.976	ug/l	90
88) 1,4-Dichlorobenzene	12.043	146	3956m	0.915	ug/l	
89) n-Butylbenzene	12.335	91	5045	0.750	ug/l	97
90) Hexachloroethane	12.536	117	431	0.337	ug/l	86
91) 1,2-Dichlorobenzene	12.335	146	2605	0.621	ug/l	87
93) 1,2,4-Trichlorobenzene	13.591	180	4274	1.734	ug/l	91
94) Hexachlorobutadiene	13.725	225	878	0.855	ug/l	96
95) Naphthalene	13.780	128	19349	2.433	ug/l	99
96) 1,2,3-Trichlorobenzene	13.963	180	4130	1.639	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010725\
Data File : VX044602.D
Acq On : 07 Jan 2025 12:23
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Jan 08 05:52:12 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010725W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 08 03:57:12 2025
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : John Carlone 01/08/2025
Supervised By : Mahesh Dadoda 01/08/2025

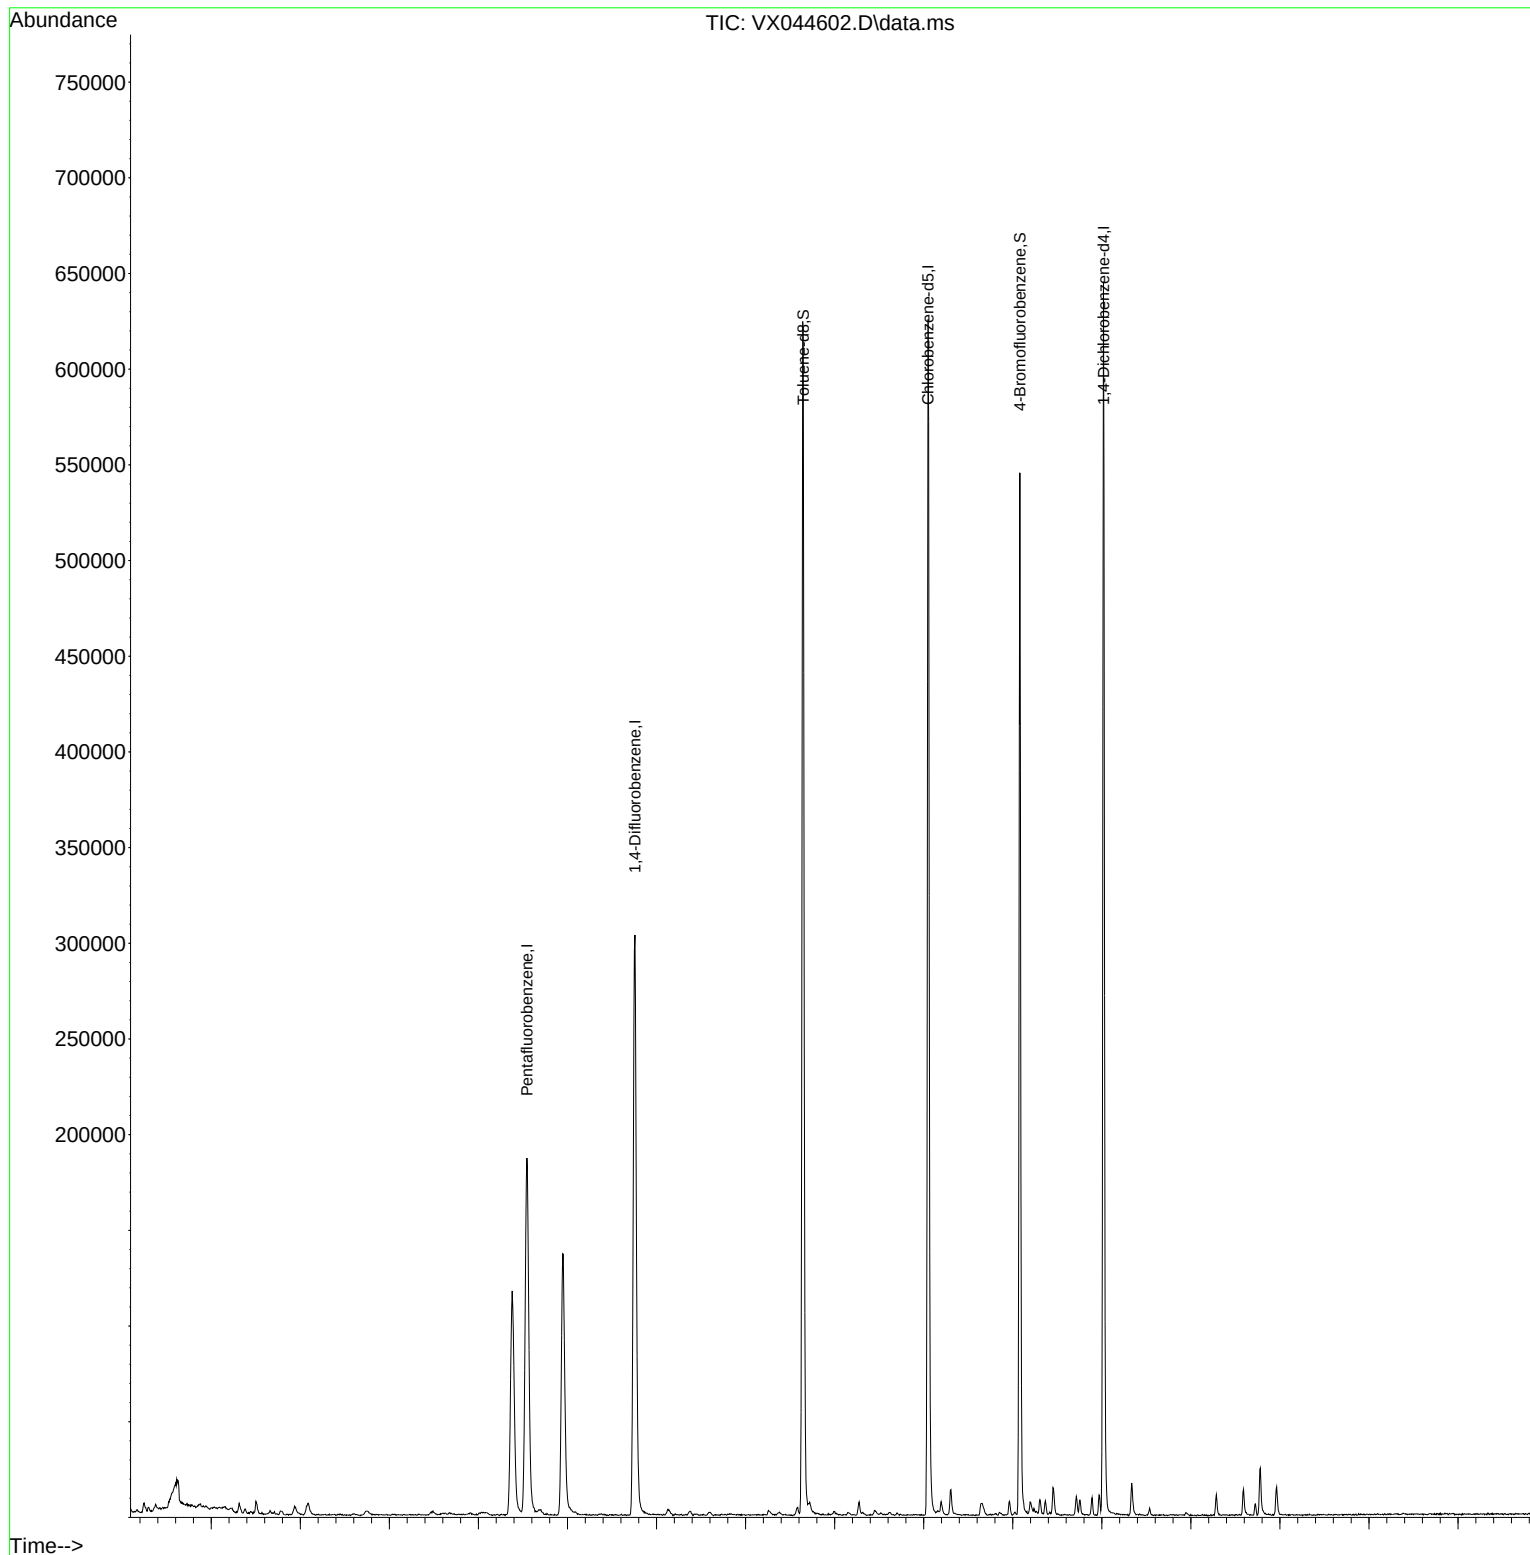



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23




Instrument :
MSVOA_X
ClientSampleId :
IBLK

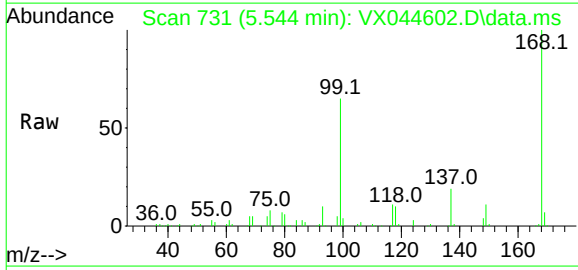

Tgt Ion: 168 Resp: 167454
Ion Ratio Lower Upper
168 100
99 65.1 53.5 80.3




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025



#2
Dichlorodifluoromethane
Concen: 0.360 ug/l
RT: 1.167 min Scan# 13
Delta R.T. 0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23


Tgt Ion: 85 Resp: 873
Ion Ratio Lower Upper
85 100
87 17.4 17.2 51.5

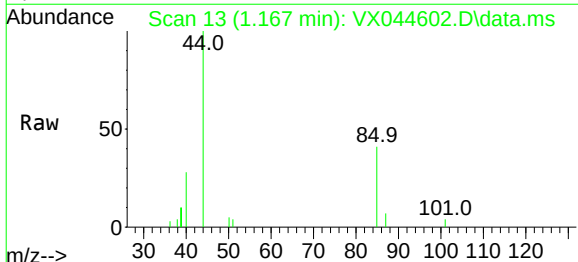



#3
Chloromethane
Concen: 0.399 ug/l
RT: 1.295 min Scan# 34
Delta R.T. 0.001 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23




Instrument :
MSVOA_X
ClientSampleId :
IBLK



Tgt Ion: 50 Resp: 964
Ion Ratio Lower Upper
50 100
52 32.3 27.0 40.4




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025

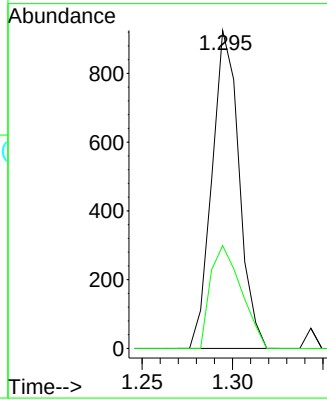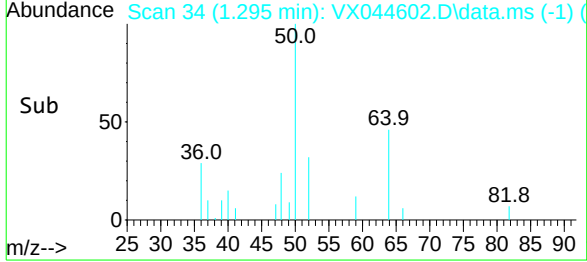

#4
Vinyl Chloride
Concen: 0.414 ug/l
RT: 1.374 min Scan# 47
Delta R.T. 0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Tgt Ion: 62 Resp: 937
Ion Ratio Lower Upper
62 100
64 35.6 26.0 39.0

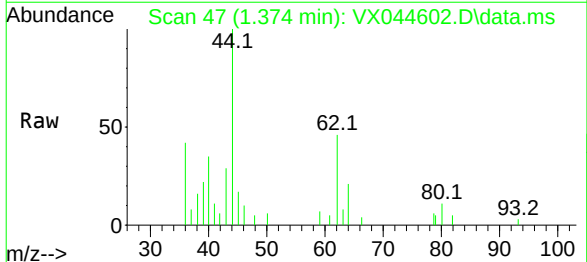



#5

Bromomethane

Concen: 0.928 ug/l

RT: 1.599 min Scan# 84

Delta R.T. 0.000 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23

Instrument :

MSVOA_X

ClientSampleId :

IBLK

Tgt Ion: 94 Resp: 1089

Ion Ratio Lower Upper

94 100





96 84.4 74.6 112.0

Manual Integrations

APPROVED

Reviewed By :John Carlone 01/08/2025

Supervised By :Mahesh Dadoda 01/08/2025

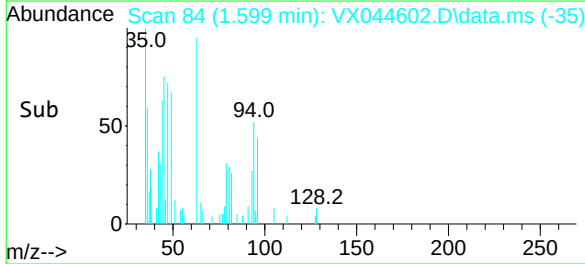

#7

Trichlorofluoromethane

Concen: 0.361 ug/l

RT: 1.874 min Scan# 129

Delta R.T. 0.000 min

Lab File: VX044602.D




Acq: 07 Jan 2025 12:23


Tgt Ion:101 Resp: 1216

Ion Ratio Lower Upper

101 100


103 41.4 53.3 79.9

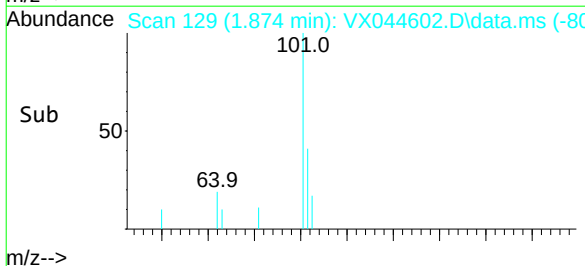



#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.393 ug/l
RT: 2.325 min Scan# 202
Delta R.T. 0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23




Instrument :
MSVOA_X
ClientSampleId :
IBLK

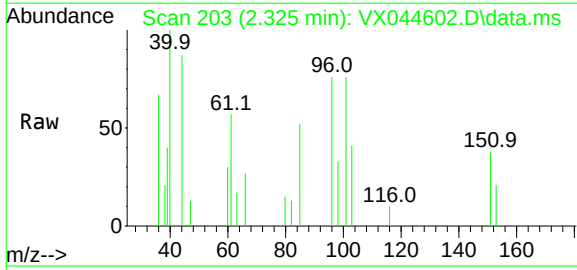


Tgt Ion:101 Resp: 760
Ion Ratio Lower Upper
101 100
85 58.9 36.5 54.7#
151 51.3 58.6 87.8#

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025




#10
Methyl Iodide
Concen: 0.539 ug/l
RT: 2.447 min Scan# 223
Delta R.T. 0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23



Tgt Ion:142 Resp: 1454
Ion Ratio Lower Upper
142 100
127 47.5 41.9 62.9
141 1.7 11.8 17.6#

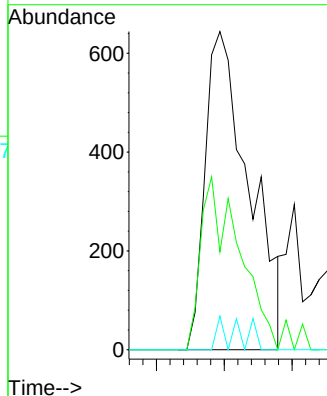







#12
1,1-Dichloroethene
Concen: 0.629 ug/l
RT: 2.313 min Scan# 201
Delta R.T. 0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion: 96 Resp: 1178
Ion Ratio Lower Upper
96 100
61 177.4 143.3 214.9
98 41.2 50.6 76.0#




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025

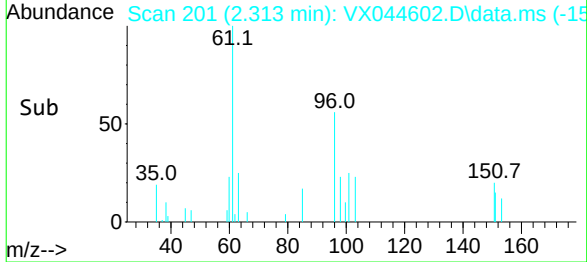

#13
Acrolein
Concen: 2.441 ug/l
RT: 2.233 min Scan# 188
Delta R.T. 0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Tgt Ion: 56 Resp: 1073
Ion Ratio Lower Upper
56 100
55 70.6 55.8 83.8

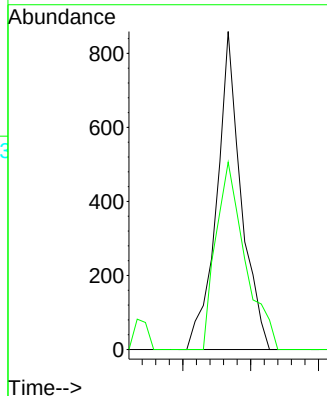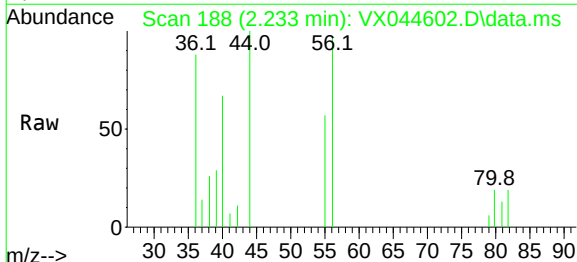



#14

Allyl chloride

Concen: 0.418 ug/l

RT: 2.660 min Scan# 258

Delta R.T. 0.000 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt Ion:	41	Resp:	1302
Ion	Ratio	Lower	Upper
41	100		
39	85.3	60.2	90.2
76	29.6	25.9	38.9

Manual Integrations

APPROVED

Reviewed By :John Carlone 01/08/2025

Supervised By :Mahesh Dadoda 01/08/2025

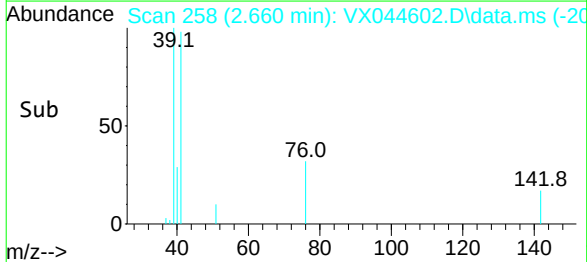

#15

Acrylonitrile

Concen: 2.462 ug/l




RT: 3.069 min Scan# 325


Delta R.T. 0.006 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23


Tgt Ion:	53	Resp:	2357
Ion	Ratio	Lower	Upper
53	100		
52	86.8	67.0	100.6
51	38.9	29.4	44.0





#16
Acetone
Concen: 2.612 ug/l
RT: 2.374 min Scan# 211
Delta R.T. -0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23




Instrument :
MSVOA_X
ClientSampleId :
IBLK

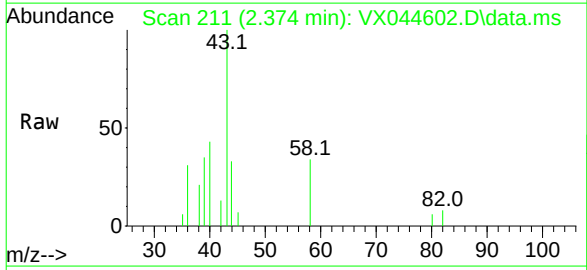

Tgt Ion: 43 Resp: 2223
Ion Ratio Lower Upper
43 100
58 33.9 22.0 33.0#




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025



#17
Carbon Disulfide
Concen: 1.894 ug/l
RT: 2.502 min Scan# 232
Delta R.T. -0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Tgt Ion: 76 Resp: 7335
Ion Ratio Lower Upper
76 100
78 8.4 7.1 10.7









#18
Methyl Acetate
Concen: 0.531 ug/l
RT: 2.709 min Scan# 265
Delta R.T. 0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion: 43 Resp: 1333
Ion Ratio Lower Upper
43 100
74 14.0 19.3 28.9#




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025

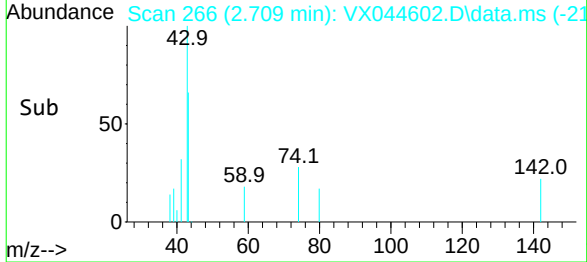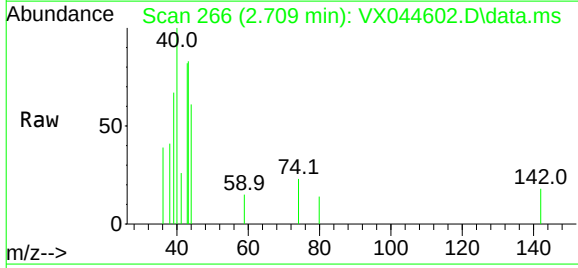

#20
Methylene Chloride
Concen: 0.410 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Tgt Ion: 84 Resp: 890
Ion Ratio Lower Upper
84 100
49 121.4 104.4 156.6
51 32.4 32.0 48.0
86 84.7 51.4 77.0#

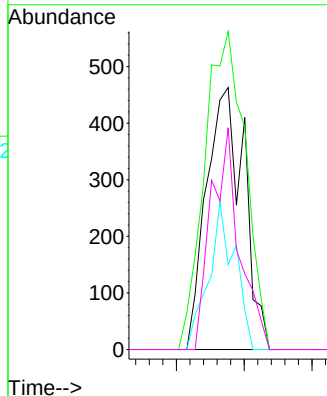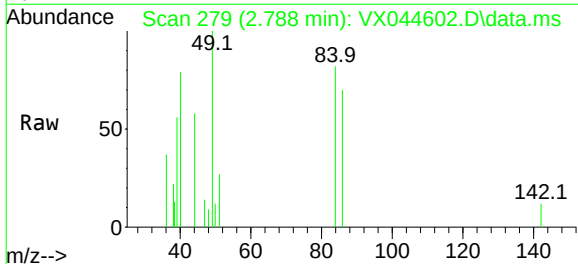







#21
trans-1,2-Dichloroethene
Concen: 0.924 ug/l
RT: 3.093 min Scan# 32
Delta R.T. 0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion: 96 Resp: 1777
Ion Ratio Lower Upper
96 100
61 124.1 118.5 177.7
98 41.7 53.4 80.0#




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025

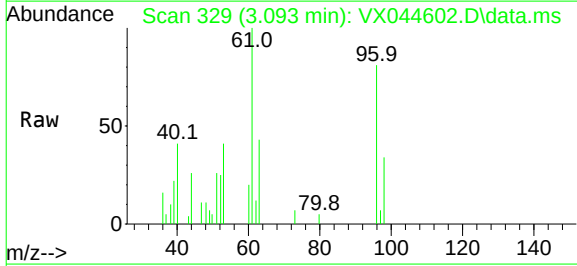

#29
Tetrahydrofuran
Concen: 1.663 ug/l m
RT: 5.038 min Scan# 648
Delta R.T. 0.037 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Tgt Ion: 42 Resp: 1399
Ion Ratio Lower Upper
42 100
72 0.0 36.1 54.1#
71 17.1 33.0 49.6#

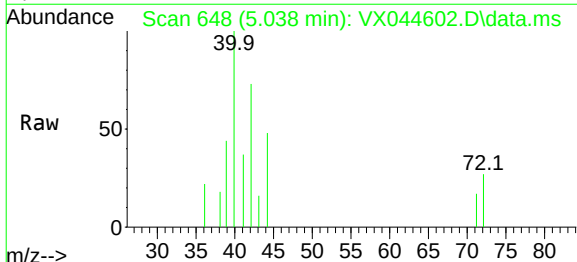







#30
Chloroform
Concen: 0.284 ug/l
RT: 5.087 min Scan# 656
Delta R.T. 0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion: 83 Resp: 1141
Ion Ratio Lower Upper
83 100
85 52.7 52.3 78.5




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025



#31
Cyclohexane
Concen: 0.267 ug/l
RT: 5.465 min Scan# 718
Delta R.T. 0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Tgt Ion: 56 Resp: 817
Ion Ratio Lower Upper
56 100
69 16.8 22.2 33.4#
84 65.7 66.6 100.0#









#33
1,2-Dichloroethane-d4
Concen: 52.259 ug/l
RT: 5.946 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion: 65 Resp: 141098
Ion Ratio Lower Upper
65 100
67 50.0 0.0 99.0




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025

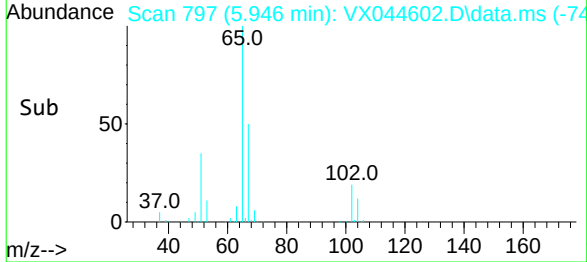

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. 0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Tgt Ion:114 Resp: 306306
Ion Ratio Lower Upper
114 100
63 21.4 0.0 42.6
88 16.4 0.0 32.6

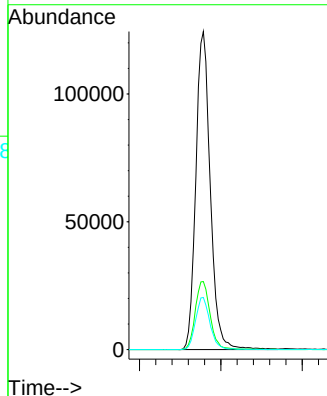



#35

Dibromofluoromethane

Concen: 49.077 ug/l

RT: 5.379 min Scan# 704

Delta R.T. 0.000 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23

Instrument :

MSVOA_X

ClientSampleId :

IBLK

Tgt Ion:113 Resp: 103080

Ion Ratio Lower Upper

113 100

111 101.8 83.3 124.9





192 17.0 14.3 21.5

Manual Integrations

APPROVED

Reviewed By :John Carlone 01/08/2025

Supervised By :Mahesh Dadoda 01/08/2025

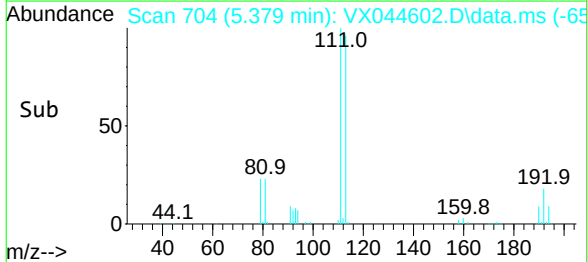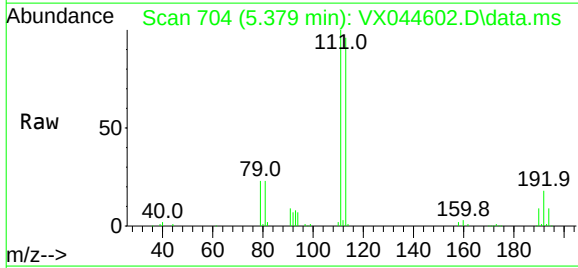

#36

1,1-Dichloropropene

Concen: 0.592 ug/l

RT: 5.702 min Scan# 757

Delta R.T. 0.012 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23




Tgt Ion: 75 Resp: 1609


Ion Ratio Lower Upper

75 100

110 0.0 17.3 51.9#

77 13.0 24.7 37.1#

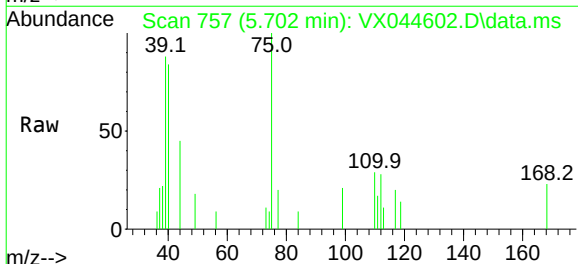







#39
Methylcyclohexane
Concen: 0.288 ug/l
RT: 7.379 min Scan# 1031
Delta R.T. 0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion	Ratio	Lower	Upper
83	100		
55	64.8	64.1	96.1
98	54.7	38.9	58.3




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025

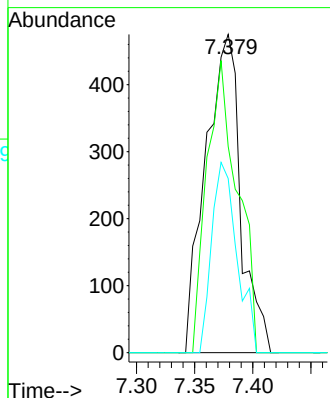

#40
Benzene
Concen: 0.266 ug/l
RT: 6.044 min Scan# 813
Delta R.T. 0.012 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23


Tgt Ion	Ratio	Lower	Upper
78	100		
77	18.9	18.8	28.2

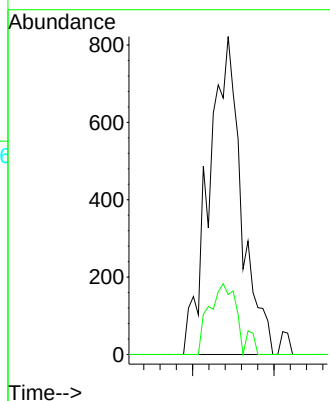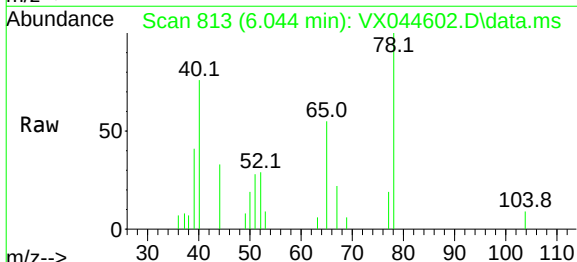



#44
Trichloroethene
Concen: 0.600 ug/l m
RT: 7.123 min Scan# 99
Delta R.T. 0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23




Instrument :
MSVOA_X
ClientSampleId :
IBLK




Tgt Ion: 130 Resp: 1311
Ion Ratio Lower Upper
130 100
95 79.3 0.0 195.6

Manual Integrations
APPROVED



Reviewed By : John Carlone 01/08/2025
Supervised By : Mahesh Dadoda 01/08/2025

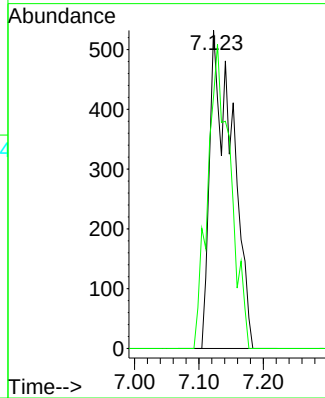


#46
Dibromomethane
Concen: 0.442 ug/l
RT: 7.586 min Scan# 1066
Delta R.T. 0.012 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23



Tgt Ion: 93 Resp: 717
Ion Ratio Lower Upper
93 100
95 90.1 65.8 98.6
174 87.6 73.4 110.0

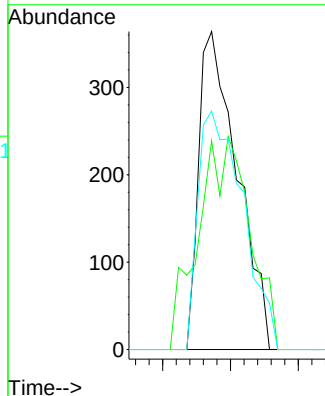







#50
Toluene-d8
Concen: 52.885 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion: 98 Resp: 379423
Ion Ratio Lower Upper
98 100
100 64.6 52.5 78.7




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025



#51
4-Methyl-2-Pentanone
Concen: 1.046 ug/l
RT: 8.586 min Scan# 1230
Delta R.T. 0.012 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23


Tgt Ion: 43 Resp: 2802
Ion Ratio Lower Upper
43 100
58 35.2 30.0 45.0

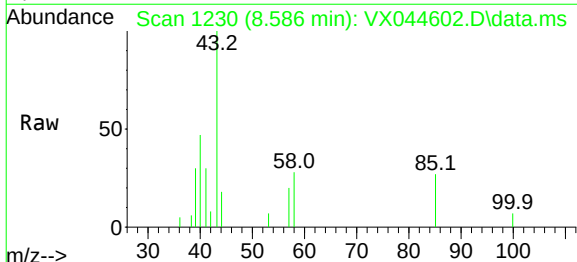

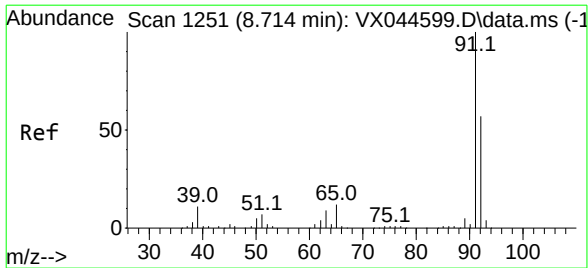

#52
Toluene
Concen: 0.360 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23




Instrument :
MSVOA_X
ClientSampleId :
IBLK

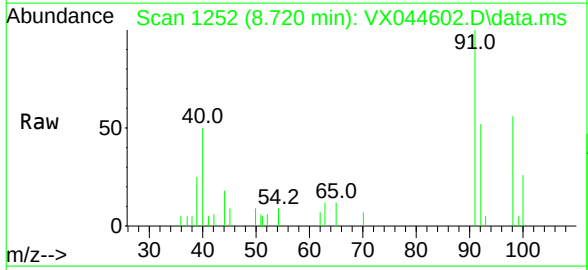

Tgt Ion: 92 Resp: 1859
Ion Ratio Lower Upper
92 100
91 189.8 140.6 210.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025

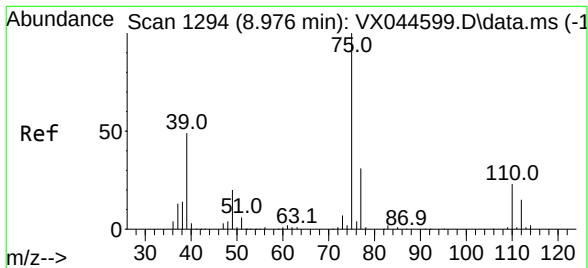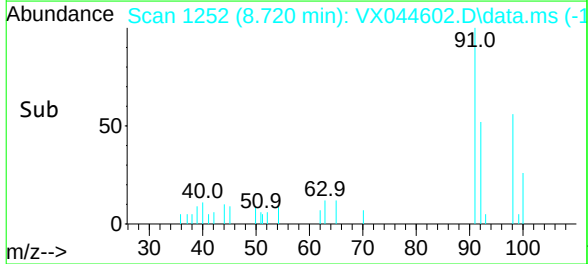

#53
t-1,3-Dichloropropene
Concen: 0.455 ug/l
RT: 8.994 min Scan# 1297
Delta R.T. 0.018 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23


Tgt Ion: 75 Resp: 1282
Ion Ratio Lower Upper
75 100
77 24.1 24.8 37.2#

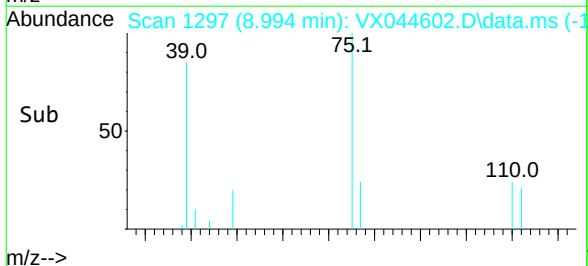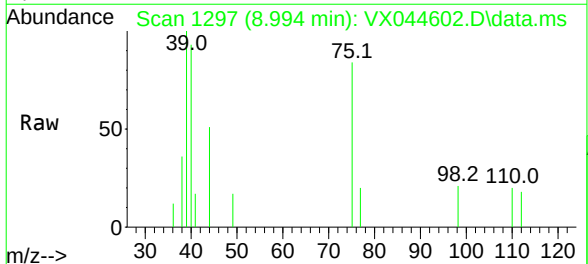

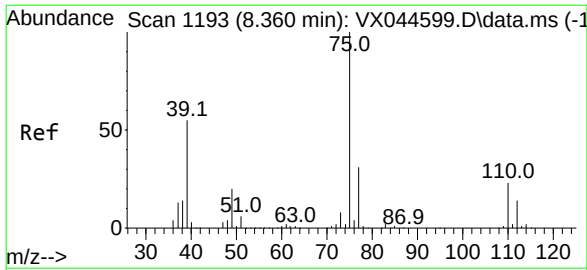

#54
 cis-1,3-Dichloropropene
 Concen: 0.392 ug/l
 RT: 8.379 min Scan# 1193
 Delta R.T. 0.018 min
 Lab File: VX044602.D
 Acq: 07 Jan 2025 12:23




Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

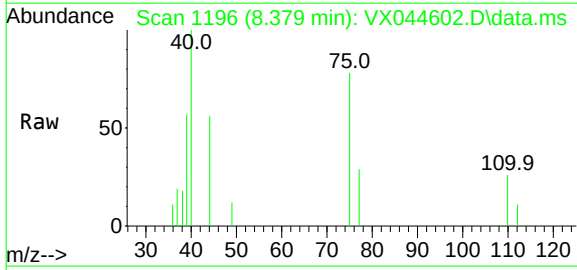


Tgt Ion:	75	Resp:	1243
Ion	Ratio	Lower	Upper
75	100		
77	37.2	24.5	36.7#
39	37.0	44.3	66.5#

Manual Integrations
 APPROVED



Reviewed By :John Carlone 01/08/2025
 Supervised By :Mahesh Dadoda 01/08/2025

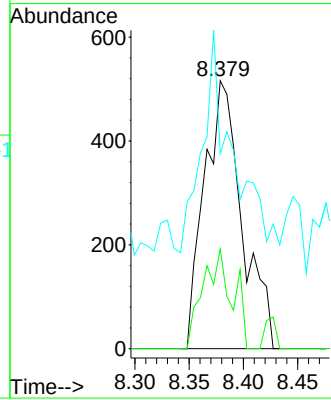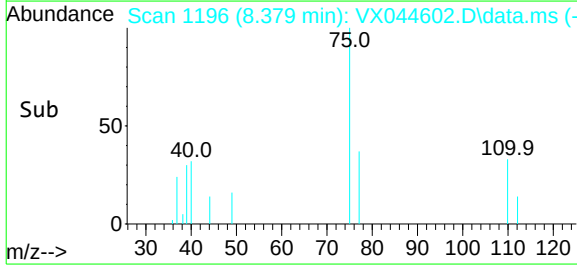


#55
 1,1,2-Trichloroethane
 Concen: 0.267 ug/l
 RT: 9.165 min Scan# 1325
 Delta R.T. 0.018 min
 Lab File: VX044602.D
 Acq: 07 Jan 2025 12:23

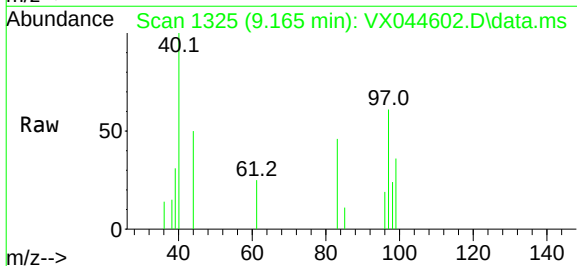

Tgt Ion:	97	Resp:	540
Ion	Ratio	Lower	Upper
97	100		
83	75.5	68.0	102.0
85	18.7	45.4	68.0#
99	59.7	48.4	72.6

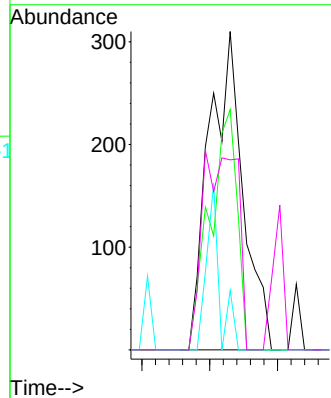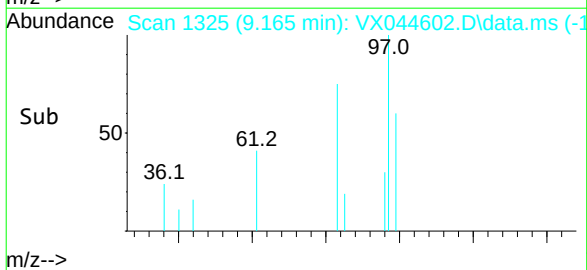



#57

1,3-Dichloropropane

Concen: 0.262 ug/l

RT: 9.317 min Scan# 13

Delta R.T. 0.012 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23

Instrument :

MSVOA_X

ClientSampleId :

IBLK

Tgt Ion: 76 Resp: 890

Ion Ratio Lower Upper

76 100





78 20.2 25.8 38.8#

Manual Integrations

APPROVED

Reviewed By :John Carlone 01/08/2025

Supervised By :Mahesh Dadoda 01/08/2025

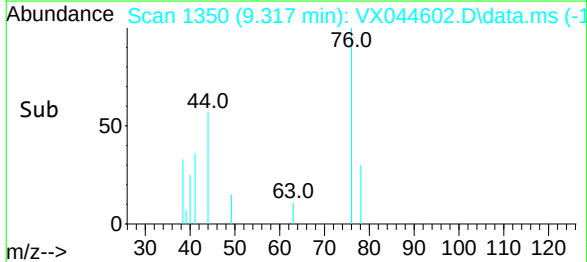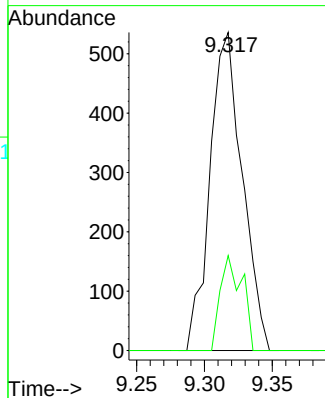

#58

2-Chloroethyl Vinyl ether

Concen: 0.800 ug/l

RT: 8.257 min Scan# 1176

Delta R.T. 0.018 min

Lab File: VX044602.D




Acq: 07 Jan 2025 12:23


Tgt Ion: 63 Resp: 1166

Ion Ratio Lower Upper

63 100

106 11.9 22.4 33.6#

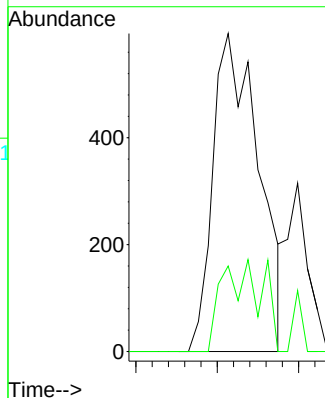

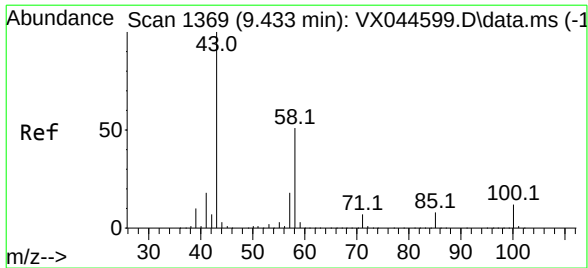





#59
2-Hexanone
Concen: 0.993 ug/l
RT: 9.445 min Scan# 13
Delta R.T. 0.012 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion: 43 Resp: 1881
Ion Ratio Lower Upper
43 100
58 59.7 25.4 76.4




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025

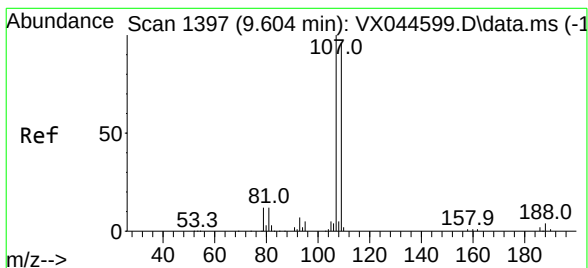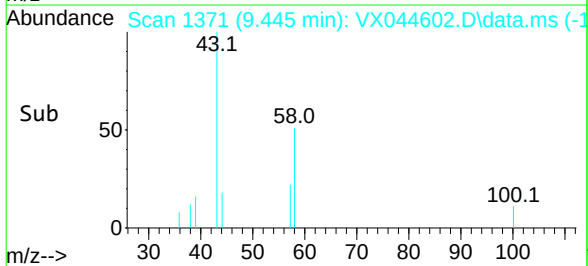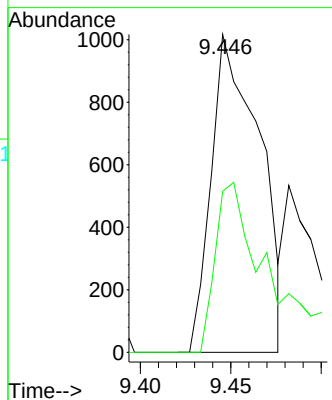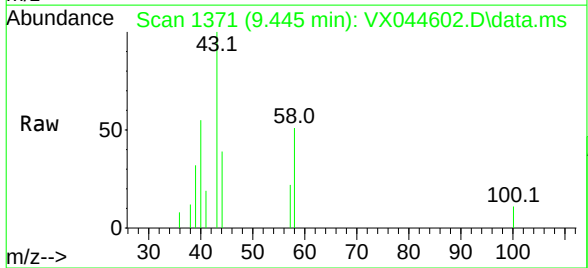

#61
1,2-Dibromoethane
Concen: 0.353 ug/l
RT: 9.622 min Scan# 1400
Delta R.T. 0.018 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23


Tgt Ion:107 Resp: 722
Ion Ratio Lower Upper
107 100
109 97.5 76.7 115.1

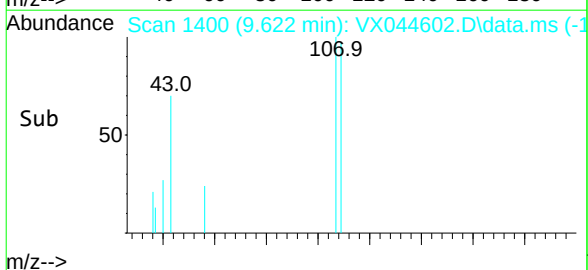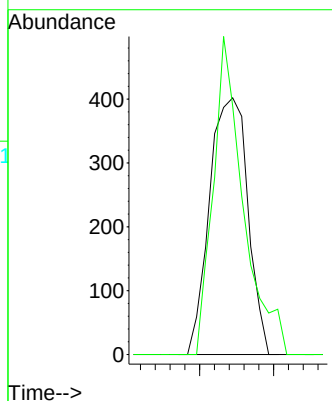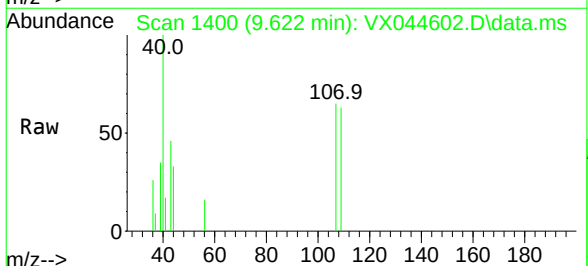

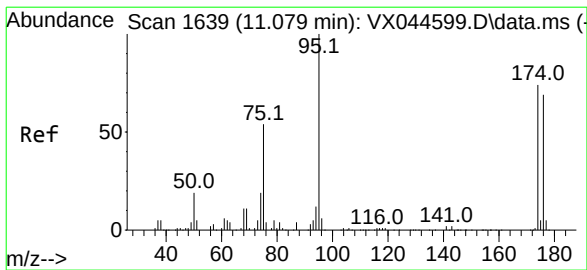

#62
4-Bromofluorobenzene
Concen: 57.285 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23




Instrument :
MSVOA_X
ClientSampleId :
IBLK




Tgt Ion: 95 Resp: 145063
Ion Ratio Lower Upper
95 100
174 73.3 0.0 148.8
176 71.4 0.0 139.8

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025

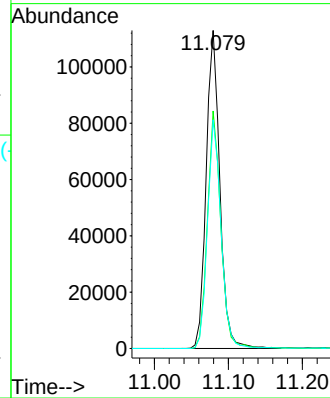


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23




Tgt Ion:117 Resp: 275086
Ion Ratio Lower Upper
117 100
82 59.7 47.8 71.6
119 32.5 25.0 37.6

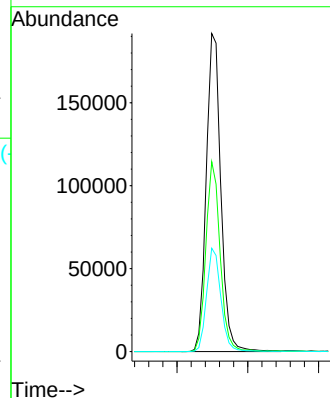

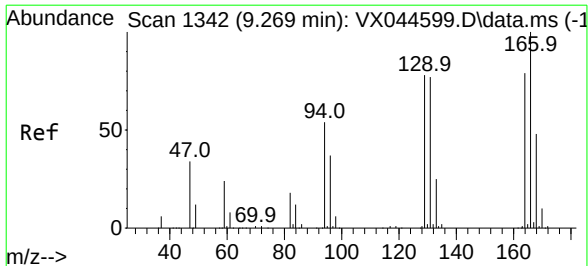

#64
Tetrachloroethene
Concen: 0.701 ug/l
RT: 9.275 min Scan# 1313
Delta R.T. 0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23




Instrument :
MSVOA_X
ClientSampleId :
IBLK

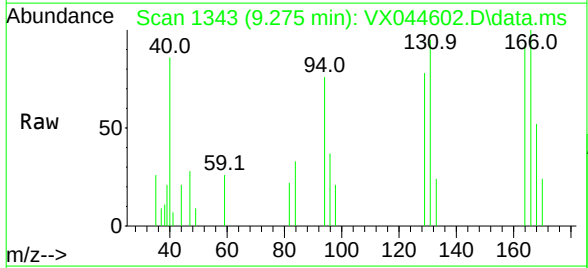

Tgt Ion:	164	Resp:	1363
Ion	Ratio	Lower	Upper
164	100		
166	108.7	101.5	152.3
129	84.6	78.9	118.3
131	102.9	77.9	116.9




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025

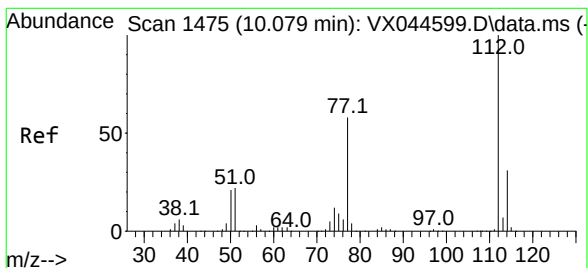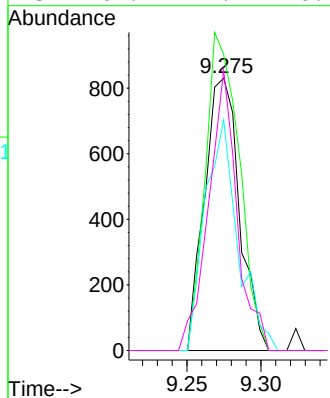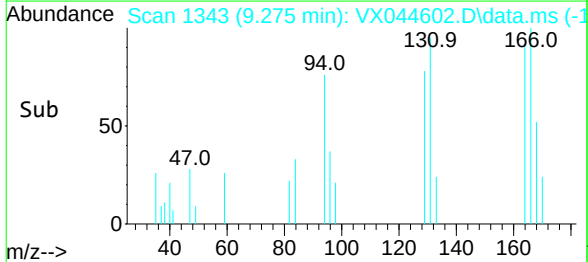

#65
Chlorobenzene
Concen: 0.488 ug/l
RT: 10.073 min Scan# 1474
Delta R.T. -0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Tgt Ion:	112	Resp:	2848
Ion	Ratio	Lower	Upper
112	100		
114	29.6	25.0	37.4

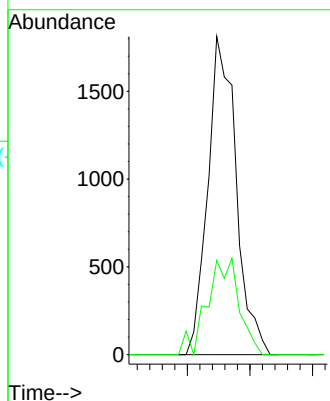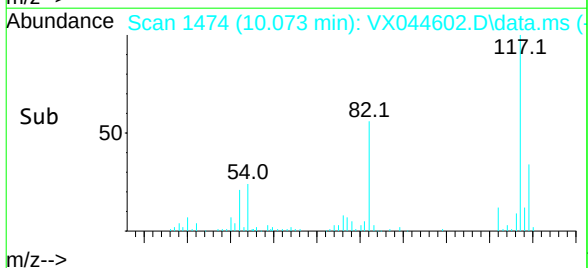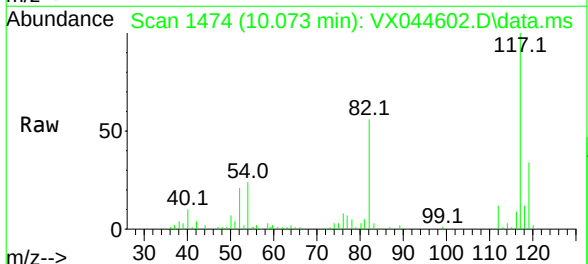







#67
Ethyl Benzene
Concen: 0.401 ug/l
RT: 10.195 min Scan# 1493
Delta R.T. 0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion: 91 Resp: 4025
Ion Ratio Lower Upper
91 100
106 39.4 23.8 35.8#




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025

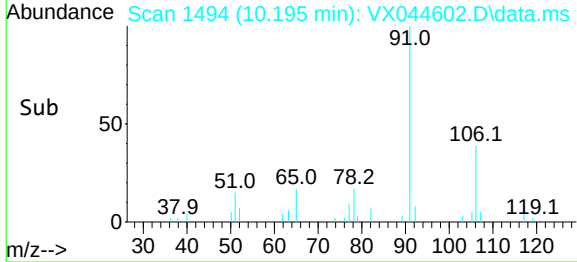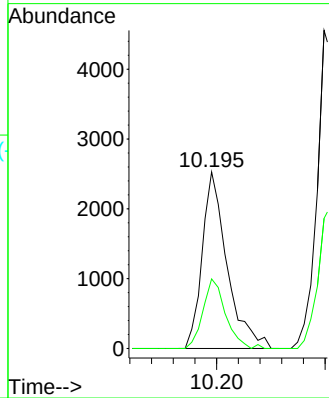

#68
m/p-Xylenes
Concen: 0.902 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Tgt Ion:106 Resp: 3323
Ion Ratio Lower Upper
106 100
91 224.8 170.4 255.6

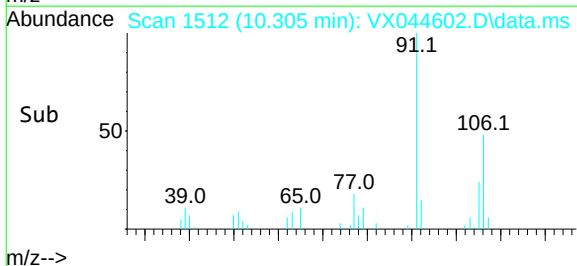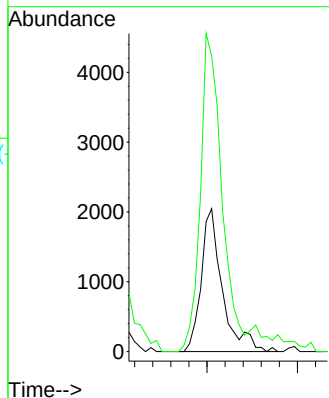







#69
o-Xylene
Concen: 0.431 ug/l
RT: 10.647 min Scan# 1570
Delta R.T. 0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion:106 Resp: 1604
Ion Ratio Lower Upper
106 100
91 201.4 112.3 336.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025

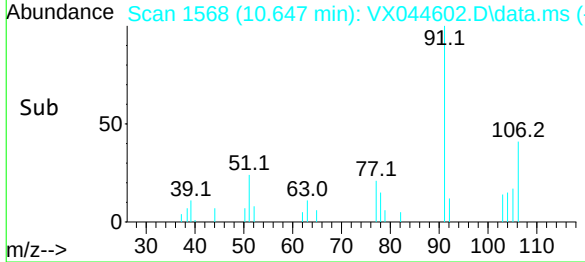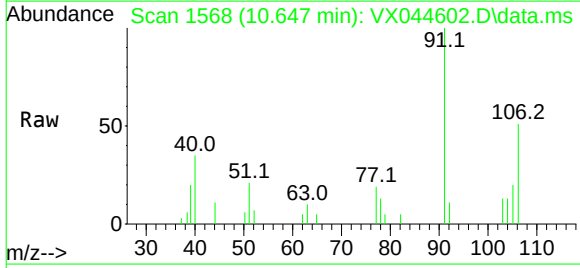

#70
Styrene
Concen: 0.442 ug/l
RT: 10.665 min Scan# 1571
Delta R.T. 0.012 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Tgt Ion:104 Resp: 2627
Ion Ratio Lower Upper
104 100
78 54.2 44.0 66.0
103 61.4 43.8 65.6

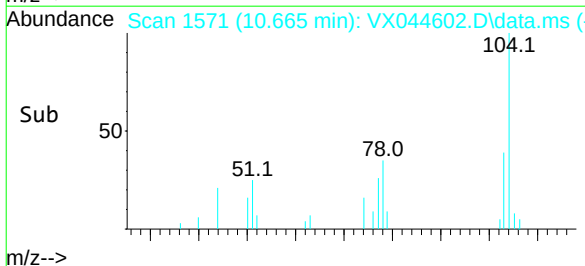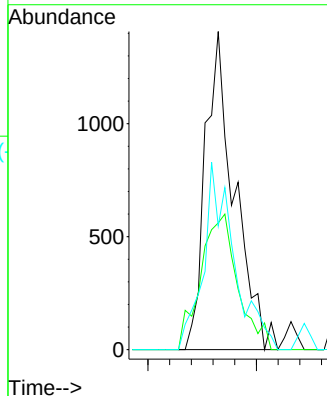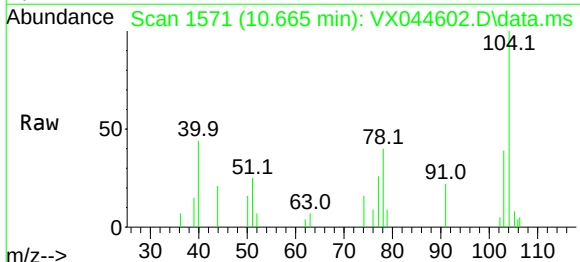



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 17

Delta R.T. 0.000 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23

Instrument :

MSVOA_X

ClientSampleId :

IBLK

Tgt Ion:152 Resp: 127489

Ion Ratio Lower Upper

152 100

115 63.8 44.4 133.1





150 155.5 0.0 355.0

Manual Integrations

APPROVED

Reviewed By :John Carlone 01/08/2025

Supervised By :Mahesh Dadoda 01/08/2025

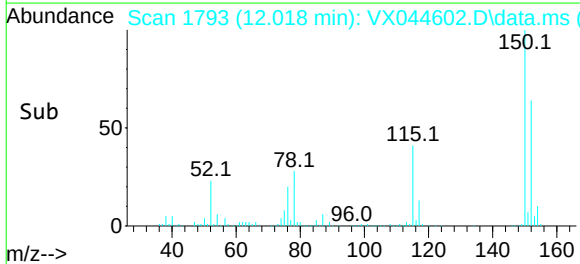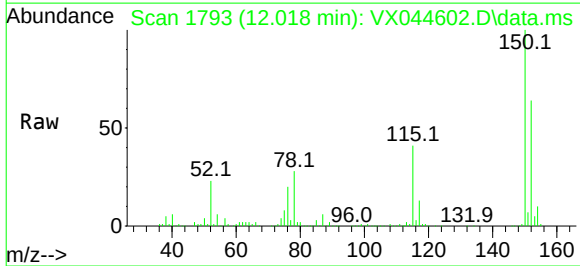

#73

Isopropylbenzene

Concen: 0.386 ug/l

RT: 10.964 min Scan# 1620

Delta R.T. 0.006 min

Lab File: VX044602.D




Acq: 07 Jan 2025 12:23


Tgt Ion:105 Resp: 3650

Ion Ratio Lower Upper

105 100

120 29.5 13.0 38.9

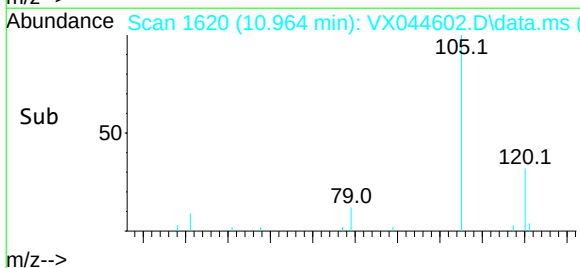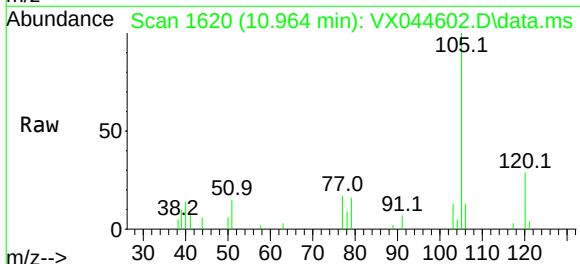



#74

N-amyI acetate

Concen: 0.304 ug/l

RT: 10.854 min Scan# 16

Delta R.T. 0.012 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt Ion:	43	Resp:	1166
Ion	Ratio	Lower	Upper
43	100		
70	32.2	32.9	49.3#
55	26.2	19.0	28.6
61	0.0	18.5	27.7#

Manual Integrations

APPROVED

Reviewed By :John Carlone 01/08/2025

Supervised By :Mahesh Dadoda 01/08/2025

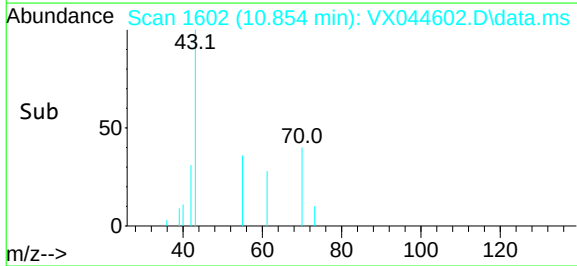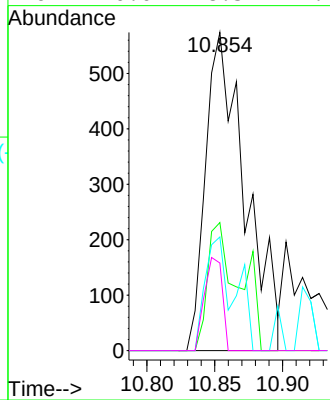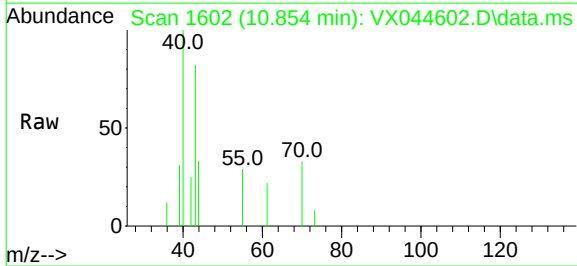

#75

1,1,2,2-Tetrachloroethane

Concen: 0.364 ug/l




RT: 11.213 min Scan# 1661


Delta R.T. 0.006 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23


Tgt Ion:	83	Resp:	1108
Ion	Ratio	Lower	Upper
83	100		
131	0.0	5.0	15.0#
85	55.5	31.9	95.5

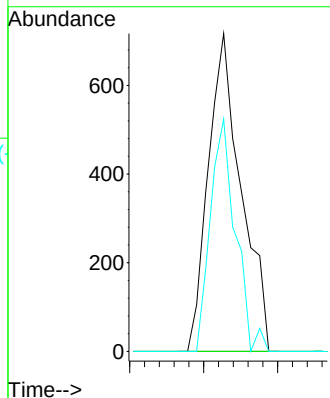



#77
Bromobenzene
Concen: 0.655 ug/l
RT: 11.195 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23




Instrument :
MSVOA_X
ClientSampleId :
IBLK

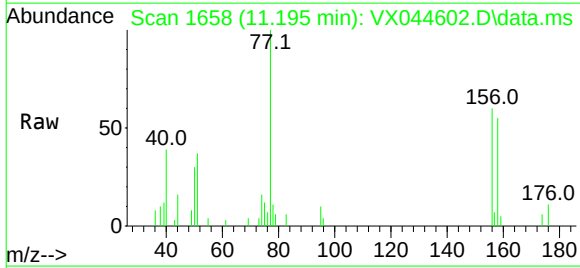


Tgt Ion: 156 Resp: 1502
Ion Ratio Lower Upper
156 100
77 166.6 85.7 257.1
158 90.8 49.9 149.6

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025

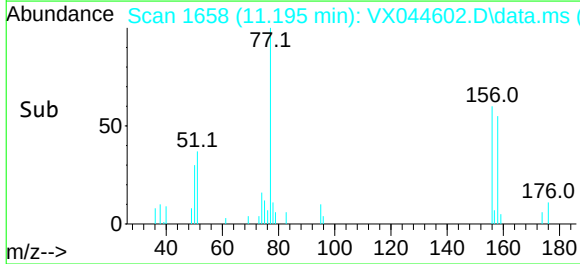


#78
n-propylbenzene
Concen: 0.535 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

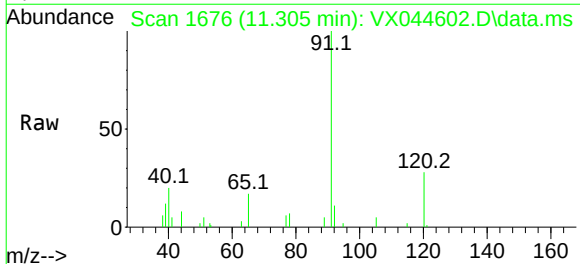

Tgt Ion: 91 Resp: 5695
Ion Ratio Lower Upper
91 100
120 30.1 11.2 33.5

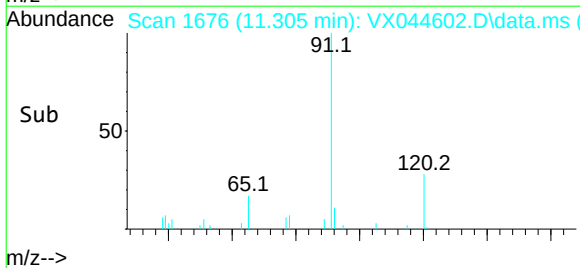







#79
2-Chlorotoluene
Concen: 0.475 ug/l
RT: 11.366 min Scan# 1685
Delta R.T. 0.006 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion: 91 Resp: 3274
Ion Ratio Lower Upper
91 100
126 42.5 16.4 49.2




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025

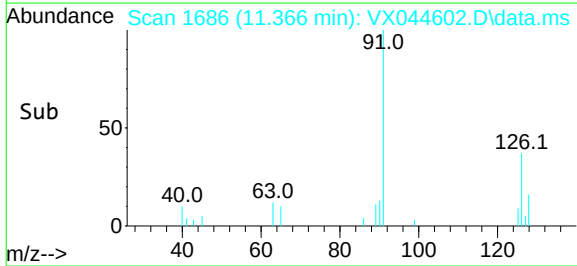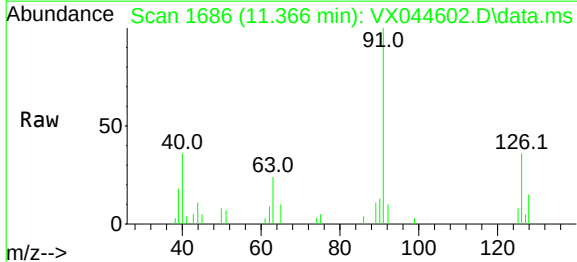

#80
1,3,5-Trimethylbenzene
Concen: 0.506 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Tgt Ion:105 Resp: 3965
Ion Ratio Lower Upper
105 100
120 46.2 23.5 70.5

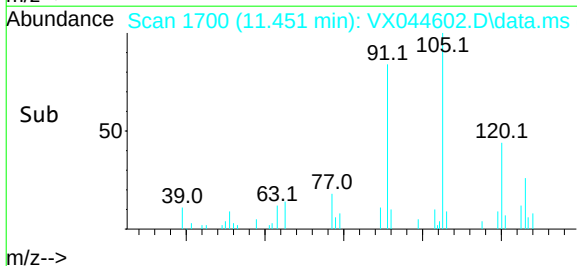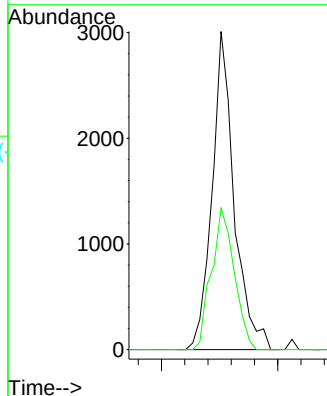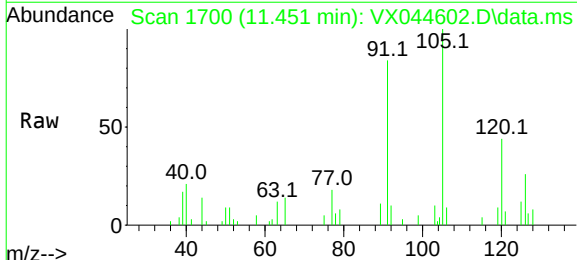



#82

4-Chlorotoluene

Concen: 0.648 ug/l

RT: 11.463 min Scan# 1700

Delta R.T. 0.012 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23

Instrument :

MSVOA_X

ClientSampleId :

IBLK

Tgt Ion: 91 Resp: 5023

Ion Ratio Lower Upper

91 100





126 30.5 14.0 42.0

Manual Integrations

APPROVED

Reviewed By :John Carlone 01/08/2025

Supervised By :Mahesh Dadoda 01/08/2025

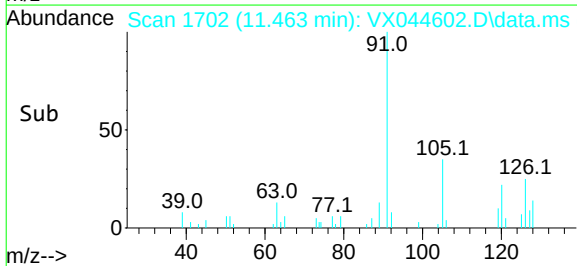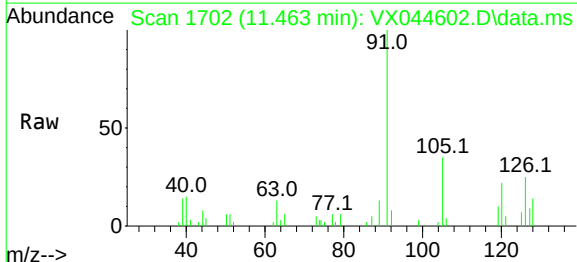

#83

tert-Butylbenzene

Concen: 0.461 ug/l

RT: 11.713 min Scan# 1743

Delta R.T. 0.000 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23




Tgt Ion:119 Resp: 3594


Ion Ratio Lower Upper

119 100

91 67.0 30.9 92.8

134 28.2 11.7 35.0

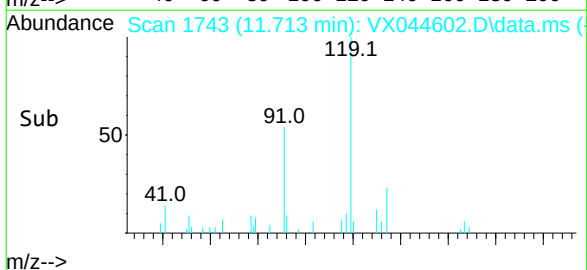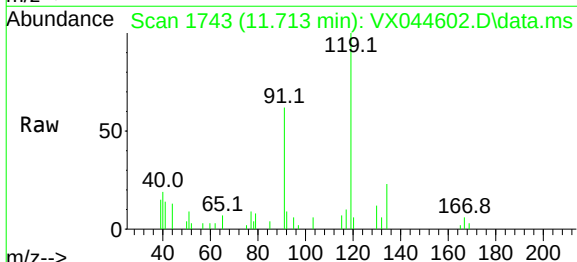



#84

1,2,4-Trimethylbenzene

Concen: 0.549 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt Ion:105 Resp: 4316
 Ion Ratio Lower Upper
 105 100
 120 44.4 21.9 65.7

Manual Integrations

APPROVED

Reviewed By :John Carlone 01/08/2025

Supervised By :Mahesh Dadoda 01/08/2025

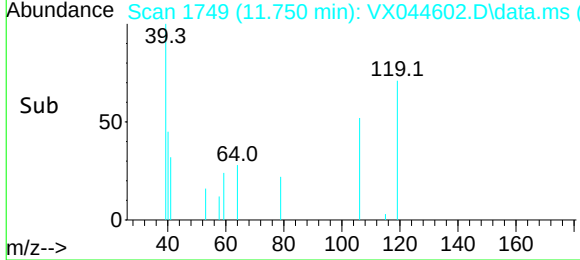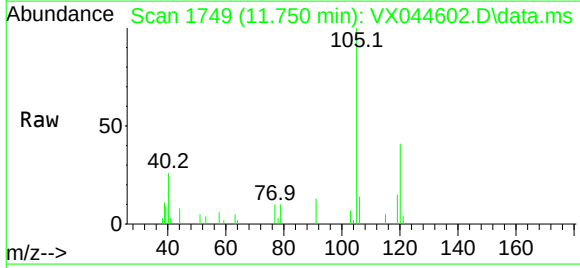

#85

sec-Butylbenzene

Concen: 0.569 ug/l




RT: 11.890 min Scan# 1772


Delta R.T. 0.000 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23


Tgt Ion:105 Resp: 5402
 Ion Ratio Lower Upper
 105 100
 134 17.1 9.9 29.7

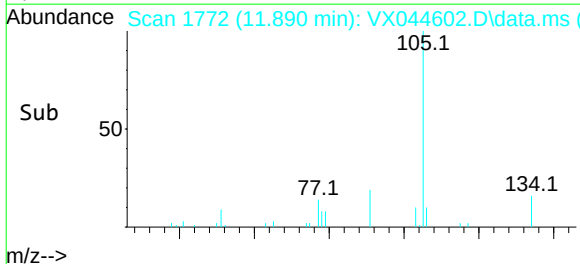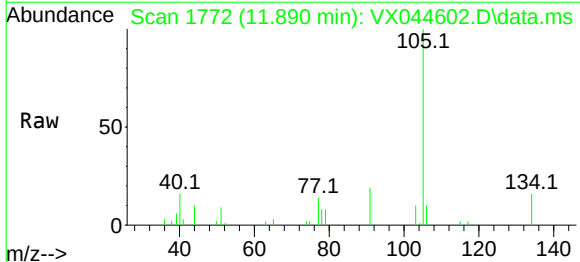



#86
p-Isopropyltoluene
Concen: 0.528 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. 0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23




Instrument :
MSVOA_X
ClientSampleId :
IBLK



Tgt Ion:119 Resp: 4207
Ion Ratio Lower Upper
119 100
134 30.6 12.6 37.8
91 35.1 13.1 39.1




Manual Integrations
APPROVED


Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025

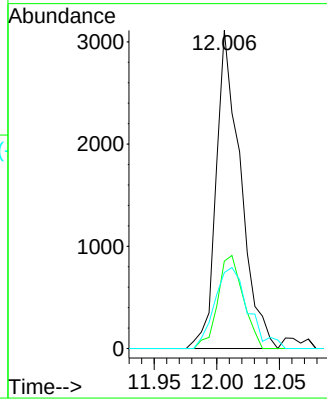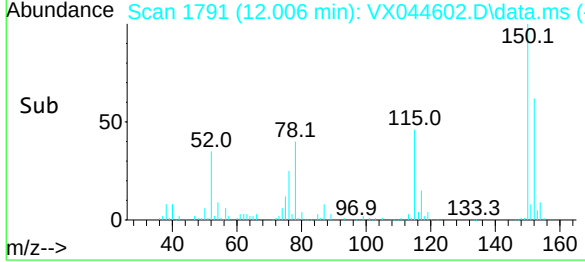

#87
1,3-Dichlorobenzene
Concen: 0.976 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. 0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

Tgt Ion:146 Resp: 4050
Ion Ratio Lower Upper
146 100
111 33.5 21.0 63.0
148 57.2 31.6 95.0

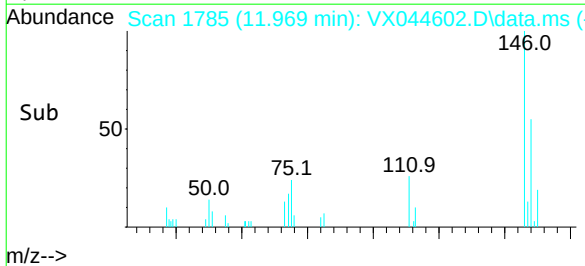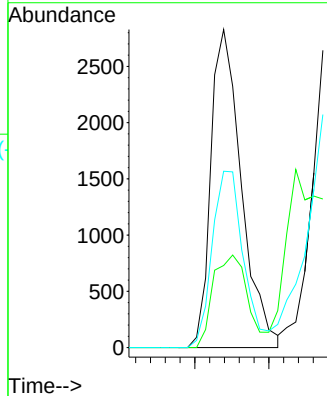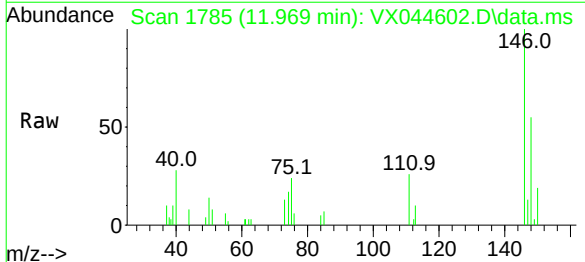



#88

1,4-Dichlorobenzene

Concen: 0.915 ug/l m

RT: 12.043 min Scan# 17

Delta R.T. 0.006 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt	Ion:146	Resp:	3956
Ion	Ratio	Lower	Upper
146	100		
111	34.3	20.7	62.1
148	58.6	31.8	95.4

Manual Integrations

APPROVED

Reviewed By :John Carlone 01/08/2025

Supervised By :Mahesh Dadoda 01/08/2025

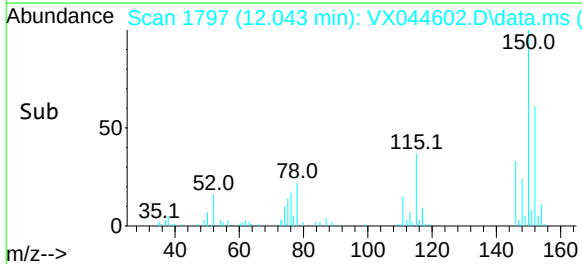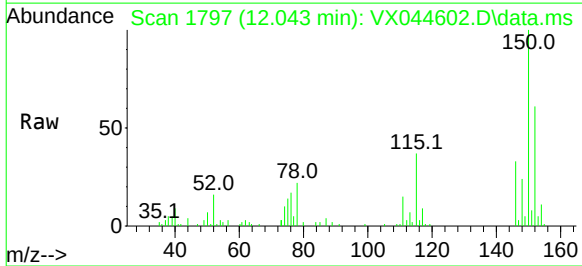

#89

n-Butylbenzene

Concen: 0.750 ug/l




RT: 12.335 min Scan# 1845


Delta R.T. 0.006 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23


Tgt	Ion: 91	Resp:	5045
Ion	Ratio	Lower	Upper
91	100		
92	55.9	26.5	79.4
134	25.3	12.4	37.2

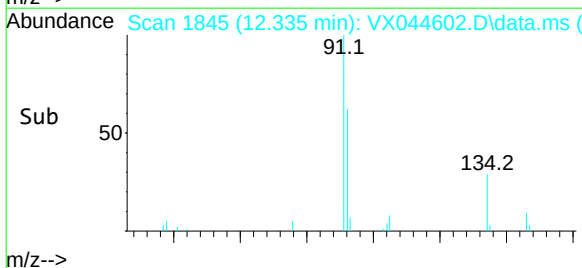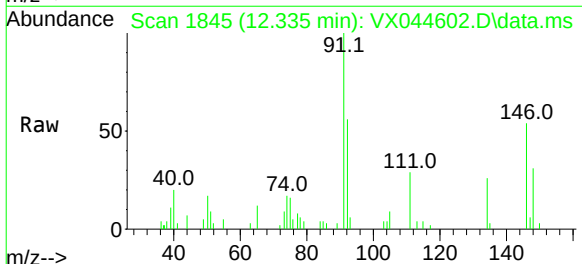



#90
Hexachloroethane
Concen: 0.337 ug/l
RT: 12.536 min Scan# 1878
Delta R.T. 0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23




Instrument :
MSVOA_X
ClientSampleId :
IBLK

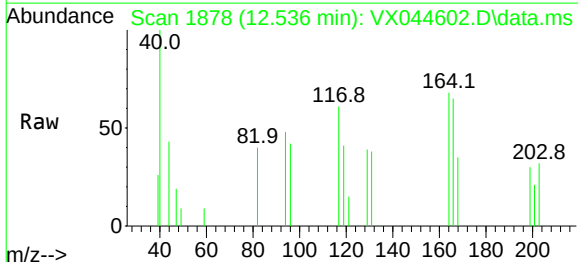


Tgt Ion:117 Resp: 431
Ion Ratio Lower Upper
117 100
201 56.1 33.6 100.6

Manual Integrations
APPROVED



Reviewed By :John Carlone 01/08/2025
Supervised By :Mahesh Dadoda 01/08/2025

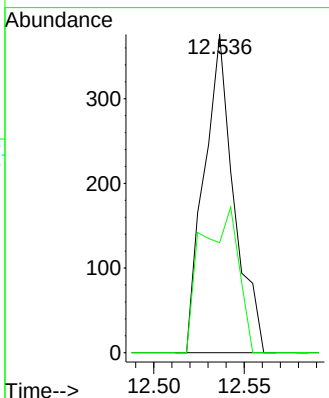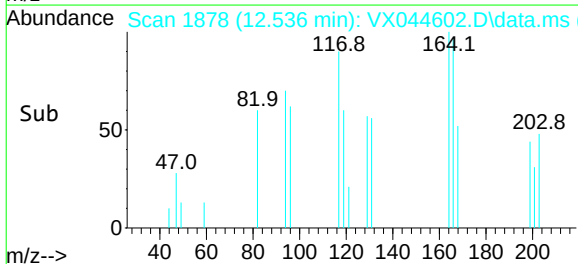


#91
1,2-Dichlorobenzene
Concen: 0.621 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX044602.D
Acq: 07 Jan 2025 12:23

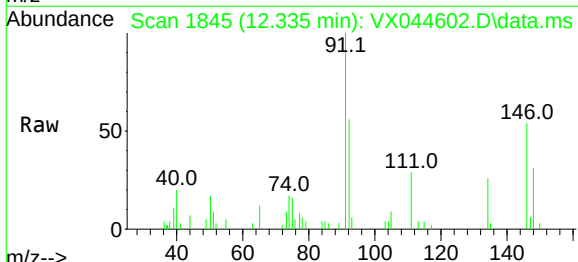

Tgt Ion:146 Resp: 2605
Ion Ratio Lower Upper
146 100
111 57.1 21.8 65.4
148 68.3 31.1 93.3

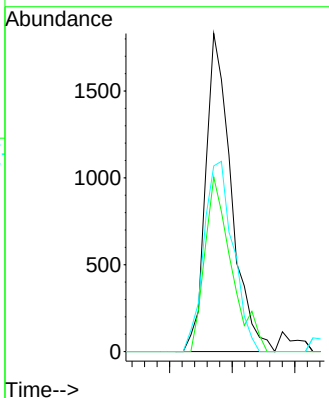



#93

1,2,4-Trichlorobenzene

Concen: 1.734 ug/l

RT: 13.591 min Scan# 2050

Delta R.T. 0.006 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt	Ion:180	Resp:	4274
Ion	Ratio	Lower	Upper
180	100		
182	85.2	47.9	143.6
145	31.3	16.3	48.9

Manual Integrations

APPROVED

Reviewed By :John Carlone 01/08/2025

Supervised By :Mahesh Dadoda 01/08/2025



#94

Hexachlorobutadiene

Concen: 0.855 ug/l




RT: 13.725 min Scan# 2073


Delta R.T. 0.000 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23

Tgt	Ion:225	Resp:	878
Ion	Ratio	Lower	Upper
225	100		
223	58.2	31.6	94.8
227	65.0	31.9	95.9





#95

Naphthalene

Concen: 2.433 ug/l

RT: 13.780 min Scan# 2081

Delta R.T. 0.006 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt	Ion:128	Resp:	19349
Ion	Ratio	Lower	Upper
128	100		
127	12.6	10.5	15.7
129	10.4	8.6	13.0

Manual Integrations

APPROVED

Reviewed By :John Carlone 01/08/2025

Supervised By :Mahesh Dadoda 01/08/2025



#96

1,2,3-Trichlorobenzene

Concen: 1.639 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. 0.006 min

Lab File: VX044602.D

Acq: 07 Jan 2025 12:23

Tgt	Ion:180	Resp:	4130
Ion	Ratio	Lower	Upper
180	100		
182	95.3	47.6	142.9
145	31.4	17.6	52.9

