

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010725\
 Data File : VX044602.D
 Acq On : 07 Jan 2025 12:23
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010725W.M
 Title : SW846 8260

Signal : TIC: VX044602.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	69	84	85	rBV7	12753	42446	4.16%	0.737%
2	2.502	228	232	242	rVB2	6480	10536	1.03%	0.183%
3	2.934	297	303	314	rBV	4421	10841	1.06%	0.188%
4	3.087	319	328	337	rBV6	6228	17680	1.73%	0.307%
5	5.379	694	704	721	rBV	116830	346558	33.97%	6.014%
6	5.544	721	731	746	rVV	185048	534004	52.35%	9.267%
7	5.946	786	797	817	rBV	136766	380157	37.27%	6.597%
8	6.757	920	930	945	rBV	303107	740688	72.61%	12.854%
9	8.641	1233	1239	1248	rBV	622877	1020079	100.00%	17.702%
10	9.275	1337	1343	1347	rBV	6983	10785	1.06%	0.187%
11	10.049	1465	1470	1484	rBV	624578	893285	87.57%	15.502%
12	10.195	1491	1494	1503	rVB2	6840	10814	1.06%	0.188%
13	10.305	1505	1512	1517	rBV	13211	20776	2.04%	0.361%
14	10.647	1563	1568	1579	rBV5	6184	17004	1.67%	0.295%
15	11.079	1634	1639	1651	rBV	544201	686741	67.32%	11.918%
16	11.195	1653	1658	1664	rBV2	6160	11247	1.10%	0.195%
17	11.305	1672	1676	1682	rVB2	7455	10525	1.03%	0.183%
18	11.451	1696	1700	1707	rVB2	14050	21551	2.11%	0.374%
19	11.713	1737	1743	1747	rBV3	9685	14392	1.41%	0.250%
20	11.890	1765	1772	1778	rBV2	9163	11604	1.14%	0.201%
21	11.969	1781	1785	1788	rBV2	10547	14260	1.40%	0.247%
22	12.018	1788	1793	1804	rVB	642732	814536	79.85%	14.135%
23	12.335	1839	1845	1853	rBV	17132	26620	2.61%	0.462%
24	13.286	1997	2001	2010	rVB	10808	14545	1.43%	0.252%
25	13.591	2047	2051	2059	rBV	13452	19226	1.88%	0.334%
26	13.780	2076	2082	2090	rBV	24744	39125	3.84%	0.679%
27	13.963	2106	2112	2118	rBV	14833	22427	2.20%	0.389%




Sum of corrected areas: 5762452

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010725\
Data File : VX044602.D
Acq On : 07 Jan 2025 12:23
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

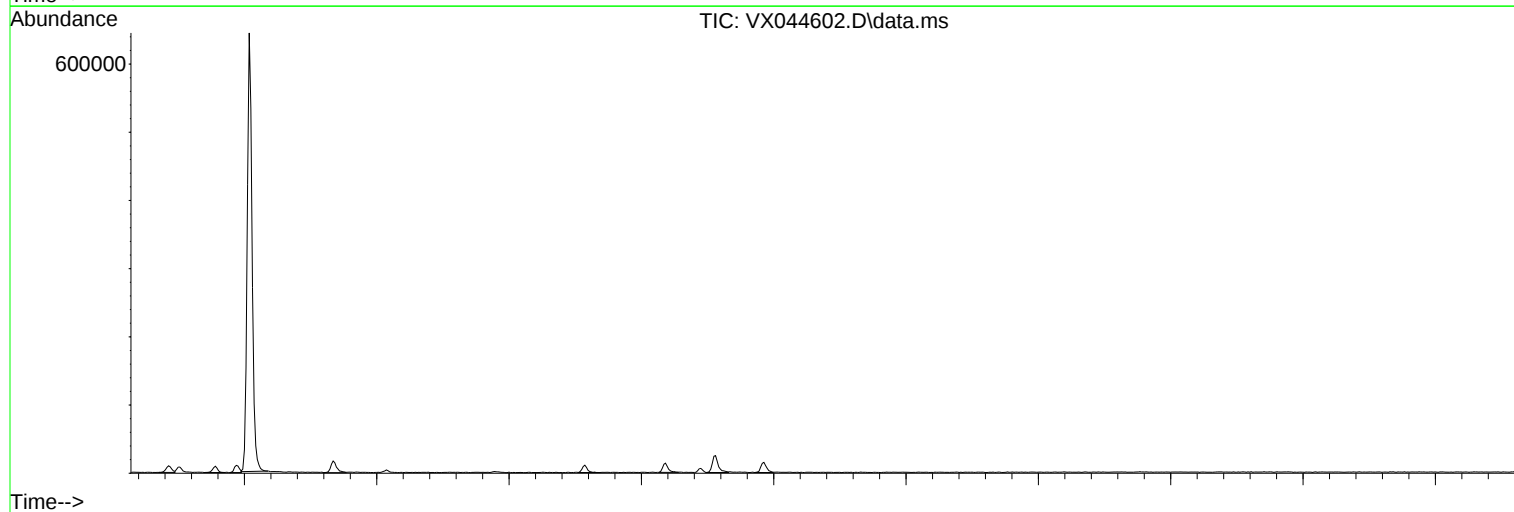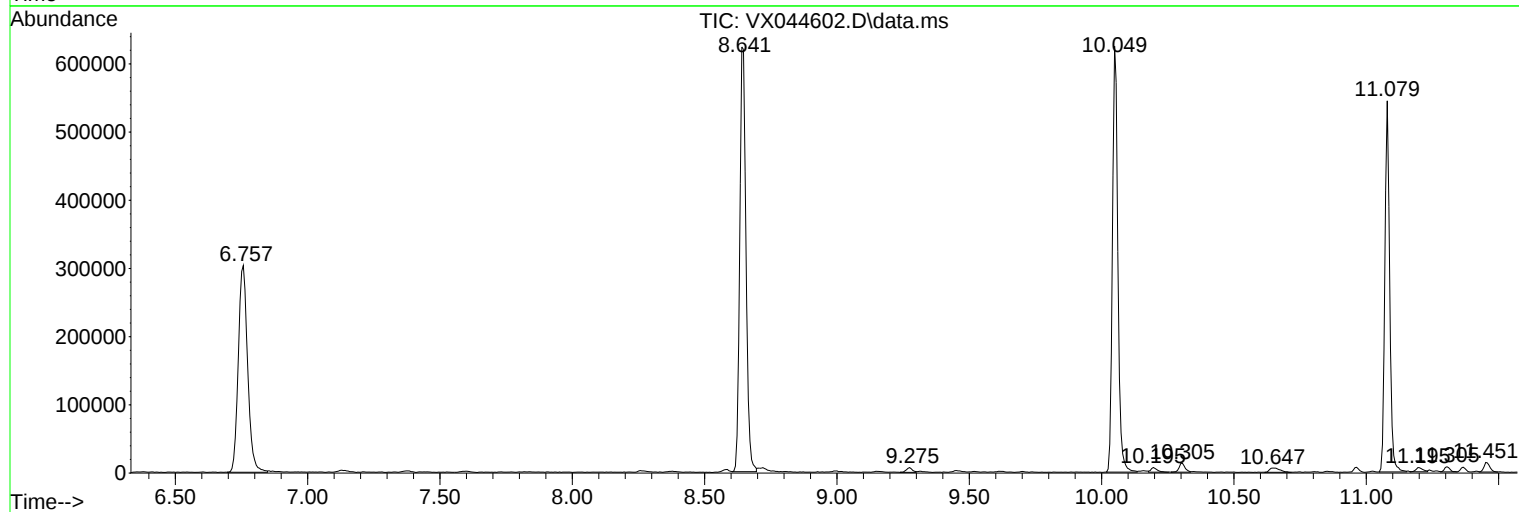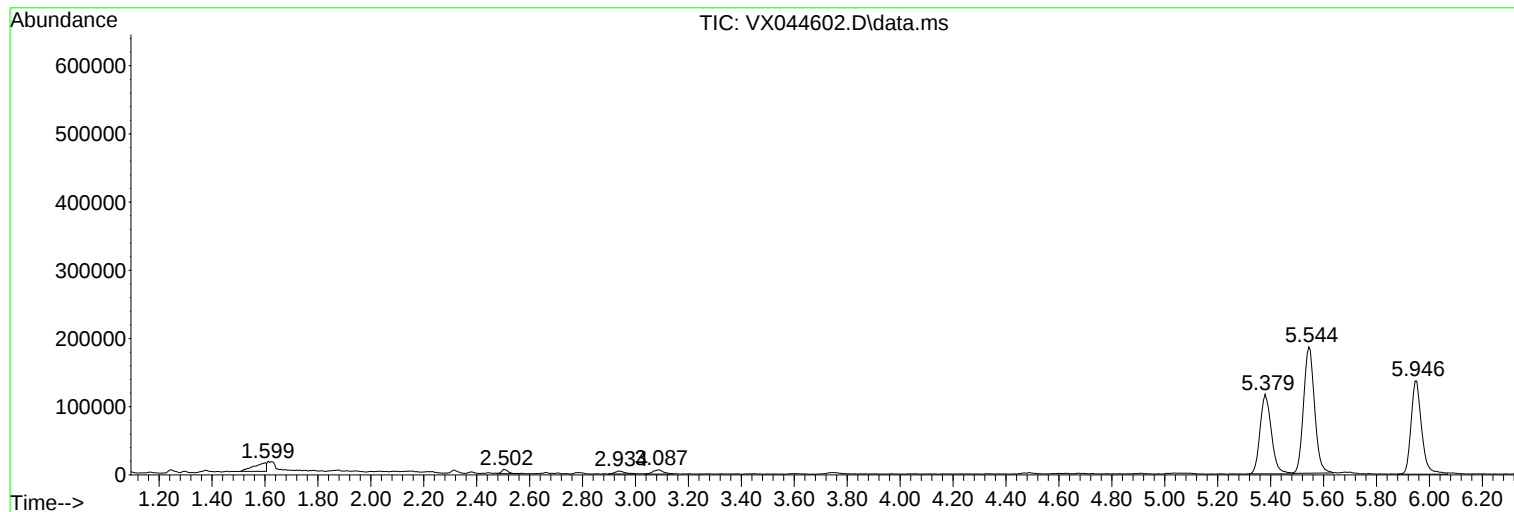

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010725\
Data File : VX044602.D
Acq On : 07 Jan 2025 12:23
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010725\
Data File : VX044602.D
Acq On : 07 Jan 2025 12:23
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010725W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc