




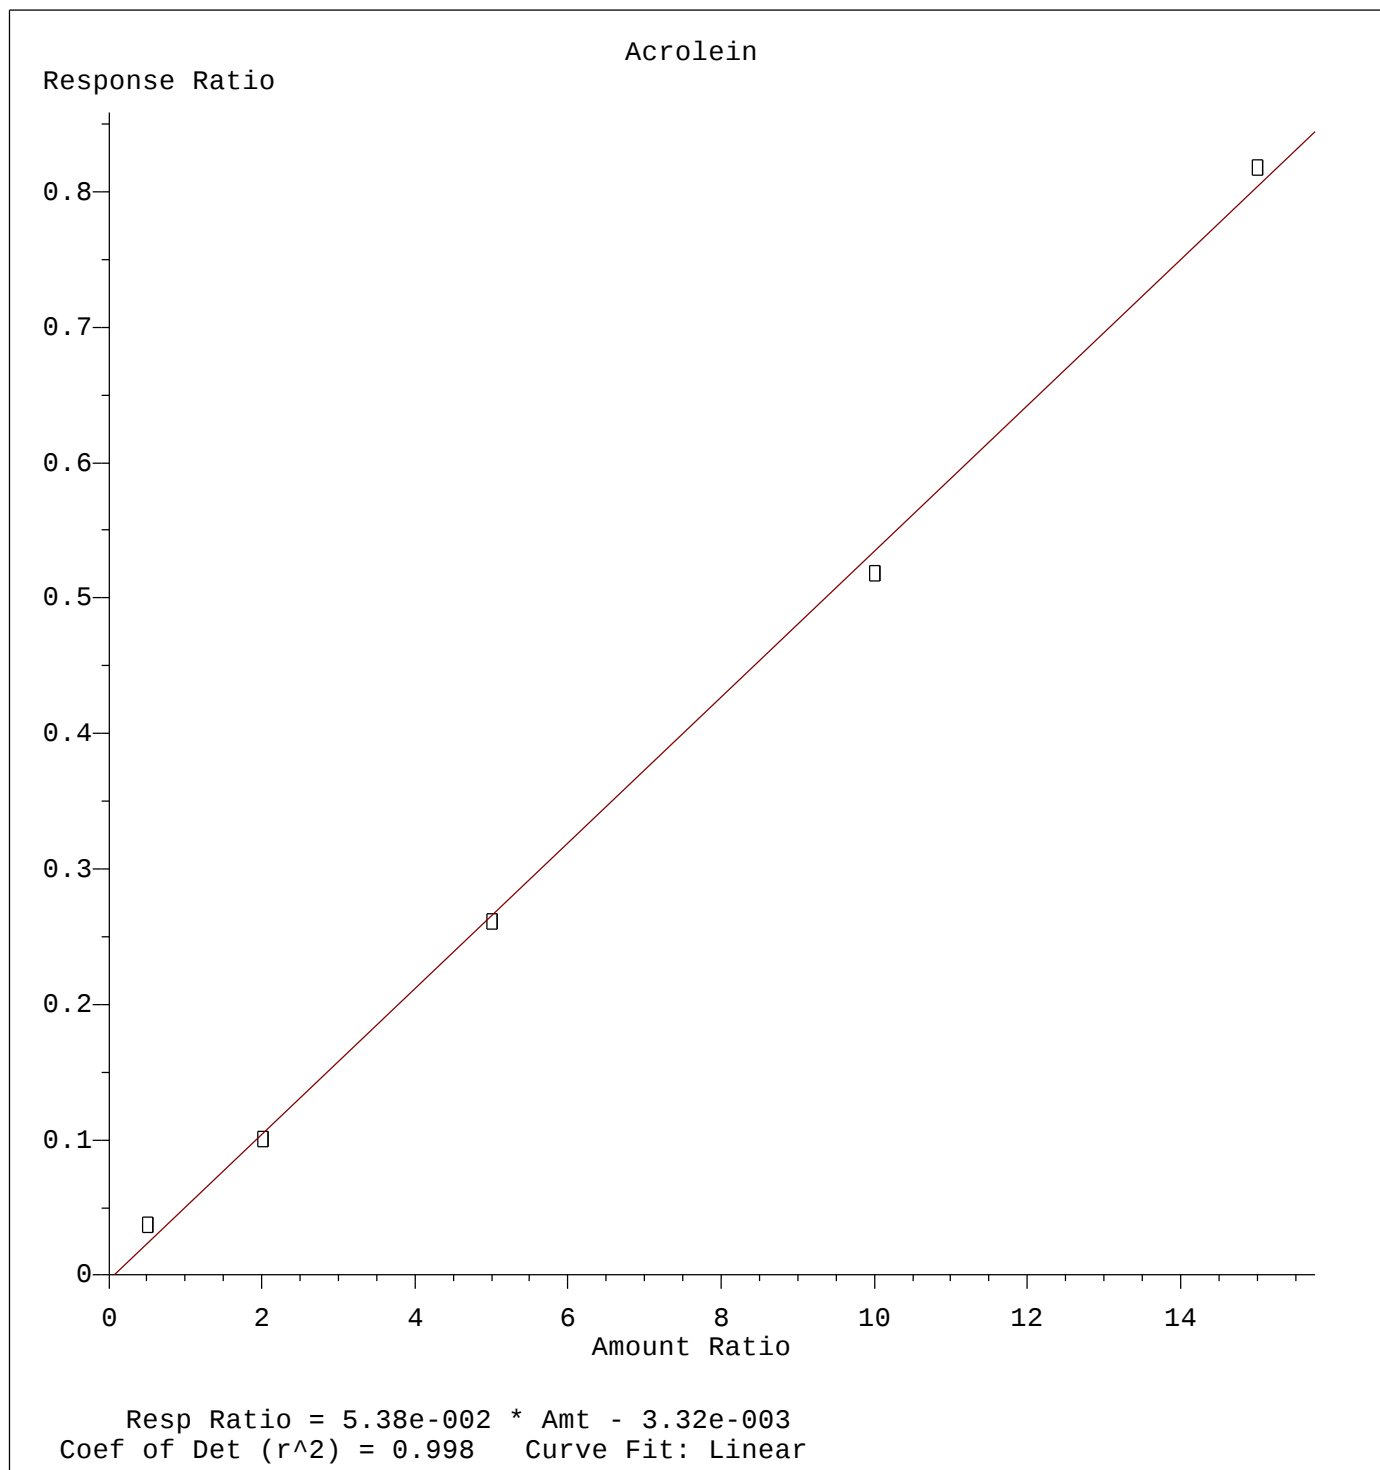


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Calibration Table Last Updated: Tue Jan 08 14:06:59 2019

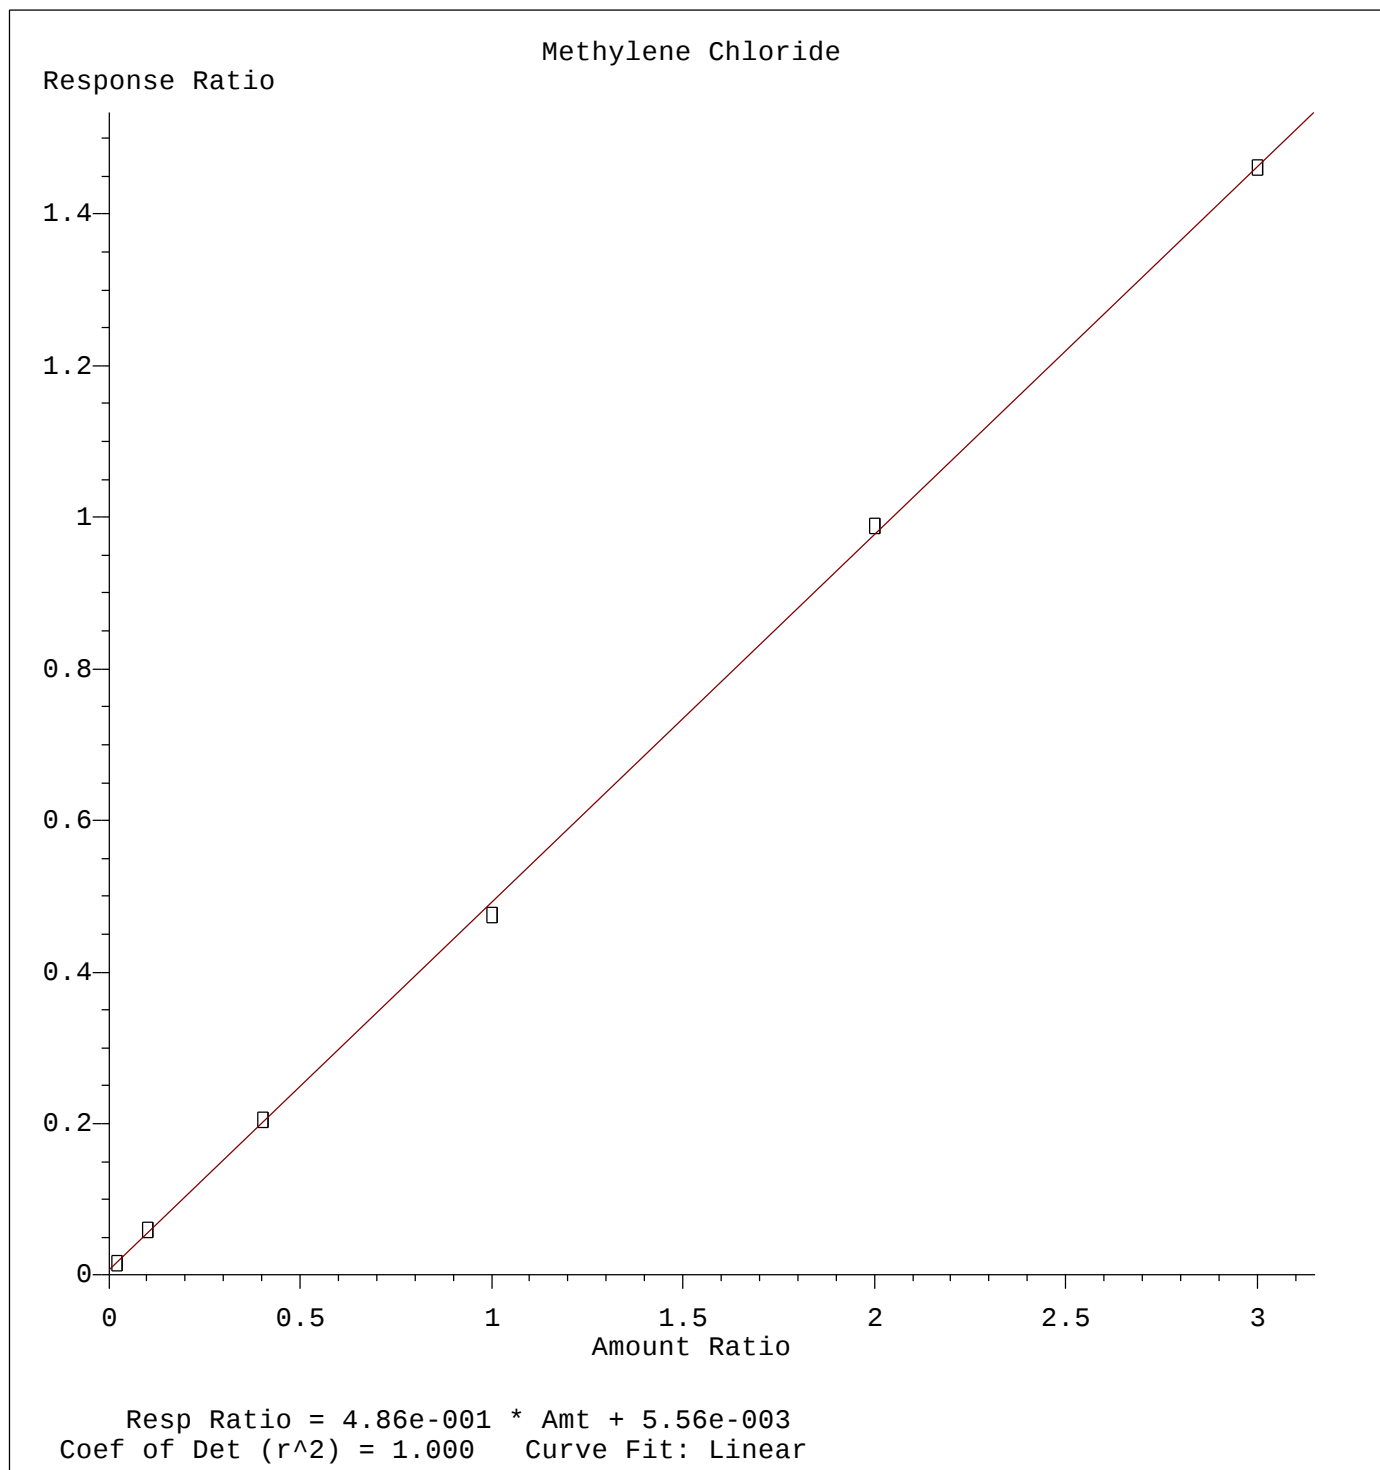

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Calibration Table Last Updated: Tue Jan 08 14:06:59 2019

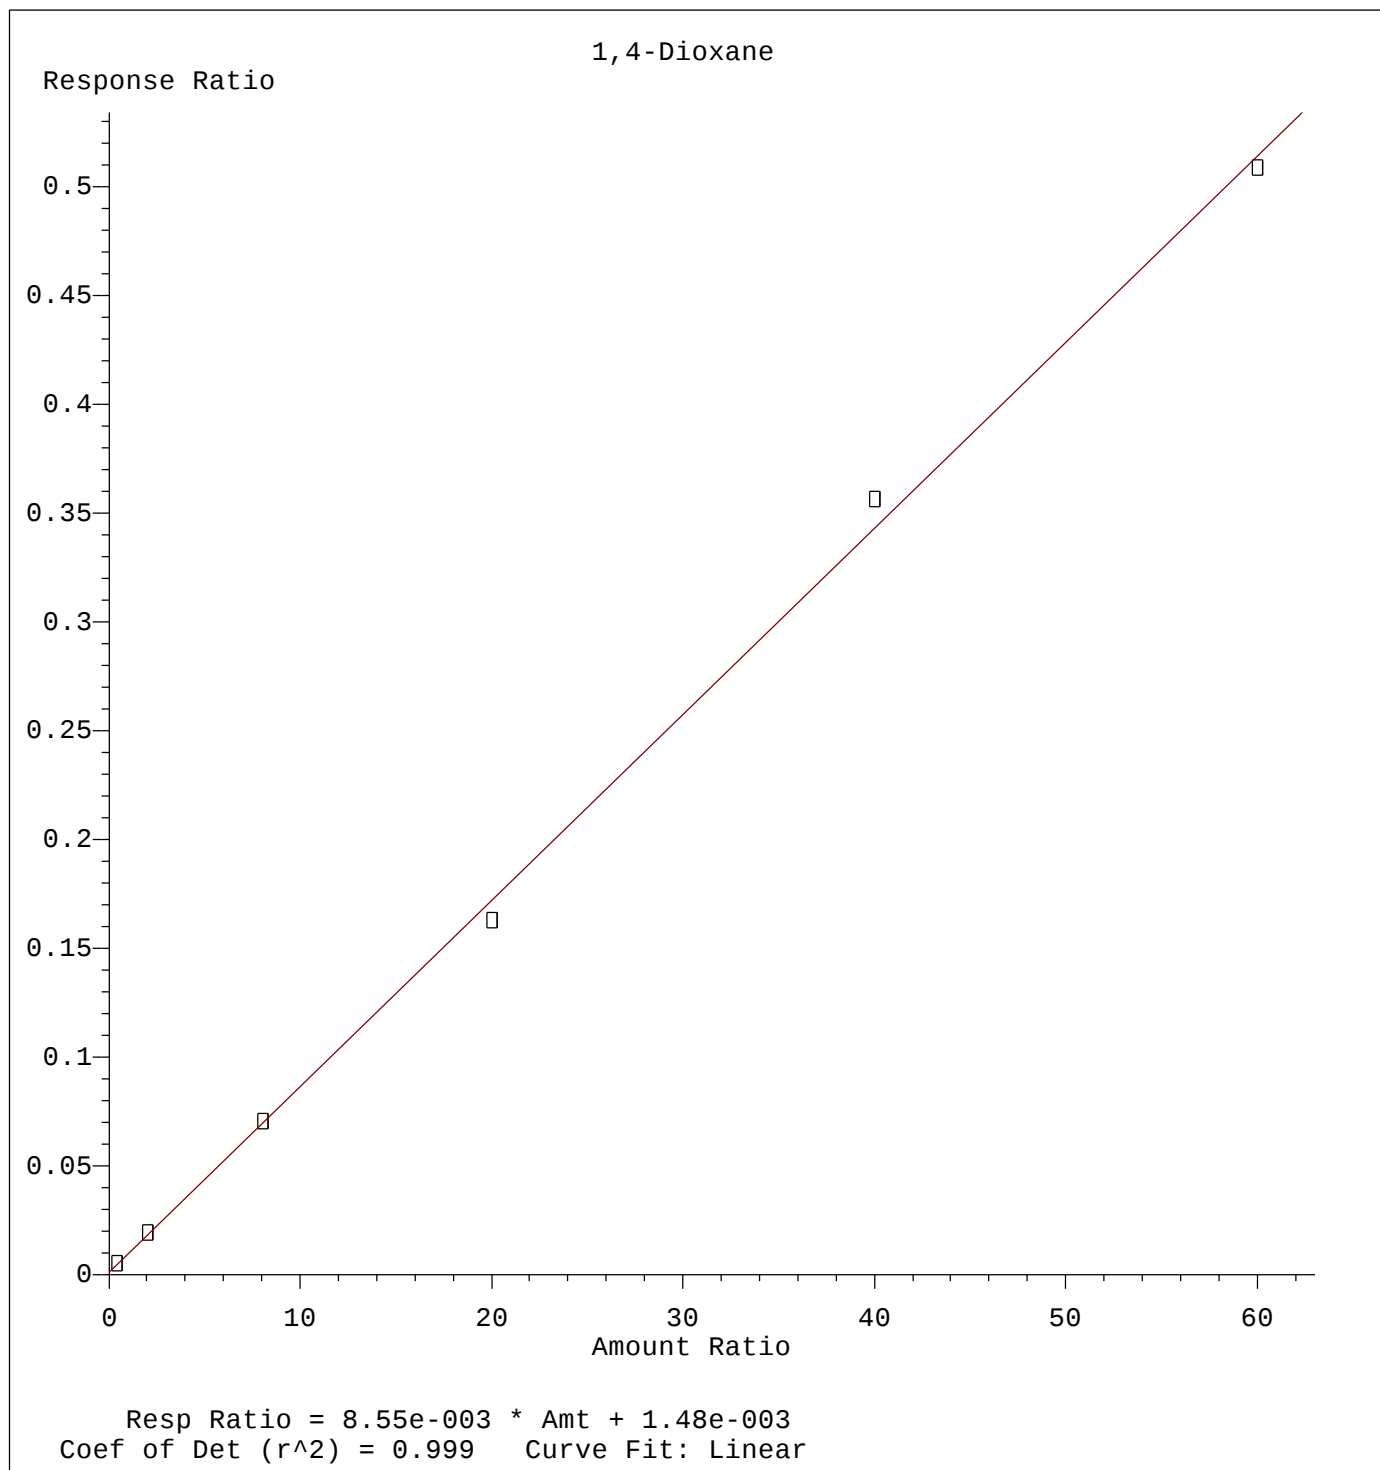


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Calibration Table Last Updated: Tue Jan 08 14:06:59 2019

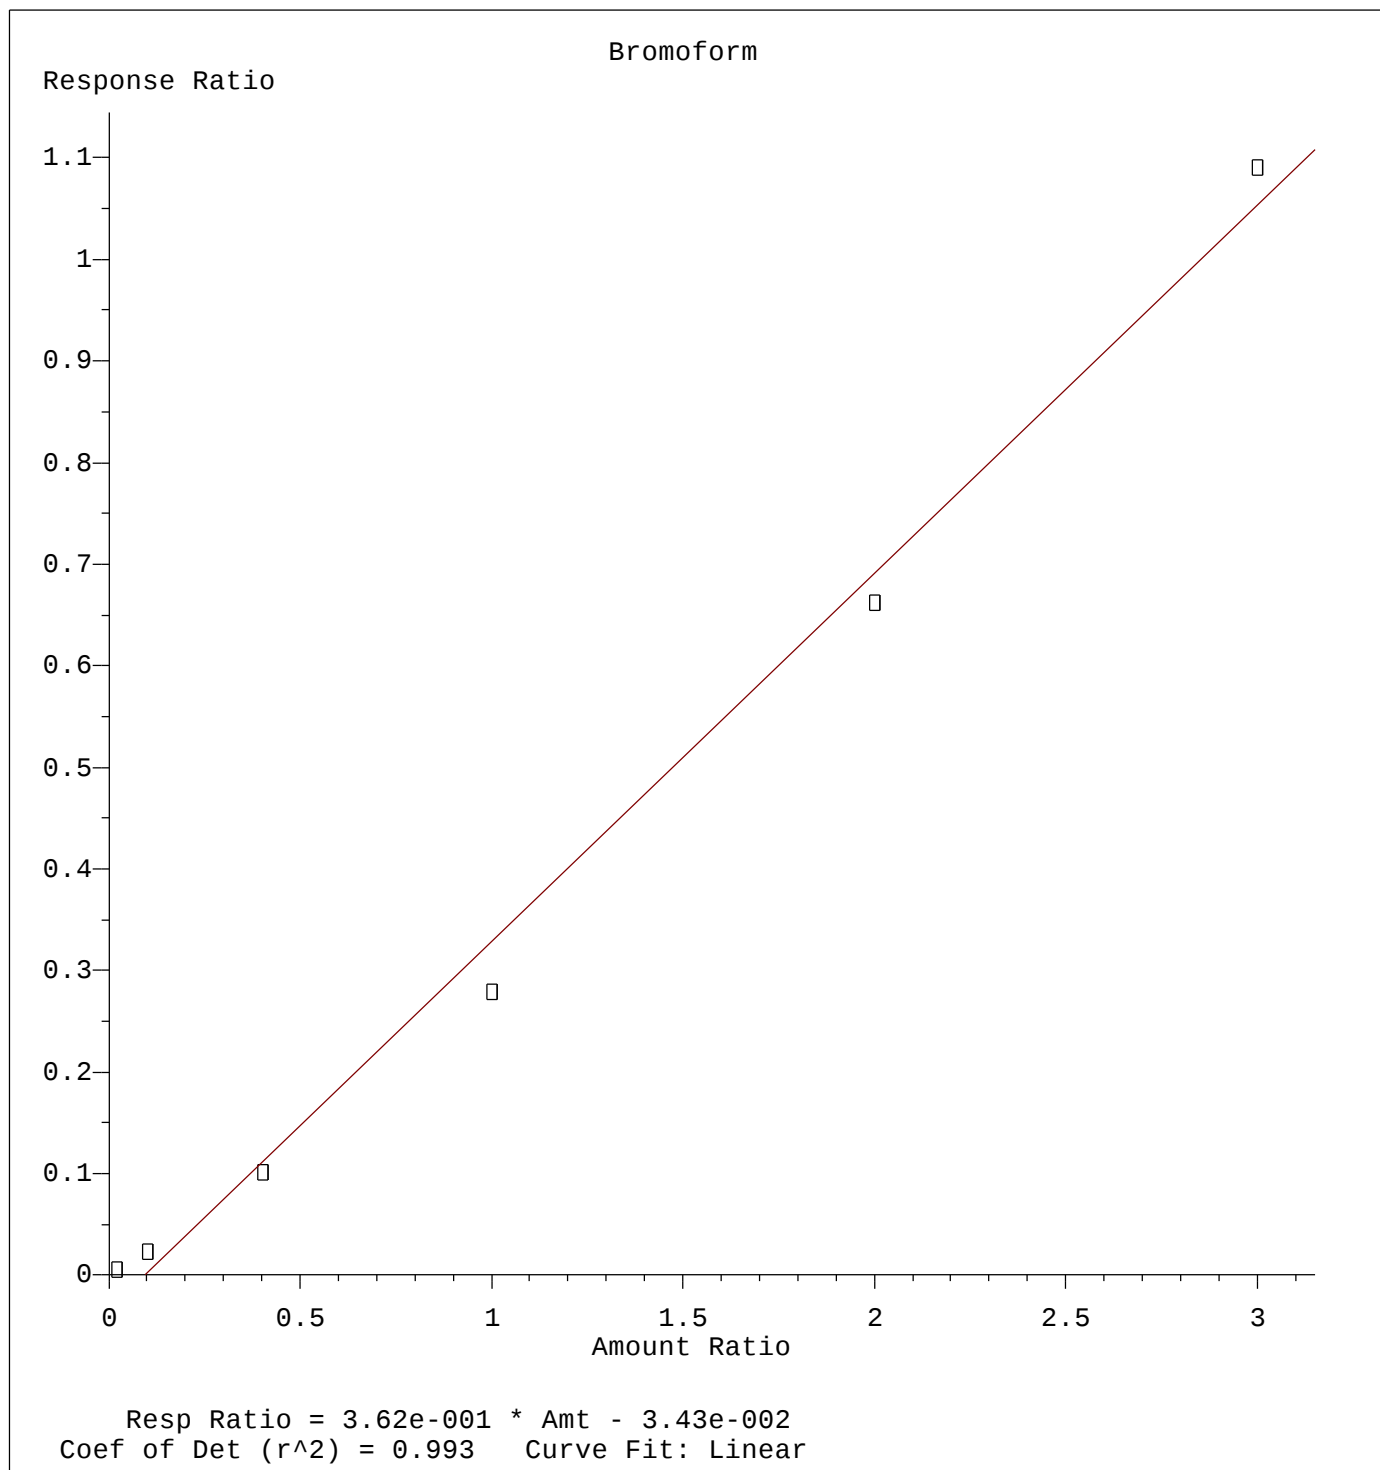

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Calibration Table Last Updated: Tue Jan 08 14:06:59 2019


trans-1,4-Dichloro-2-butene

Response Ratio

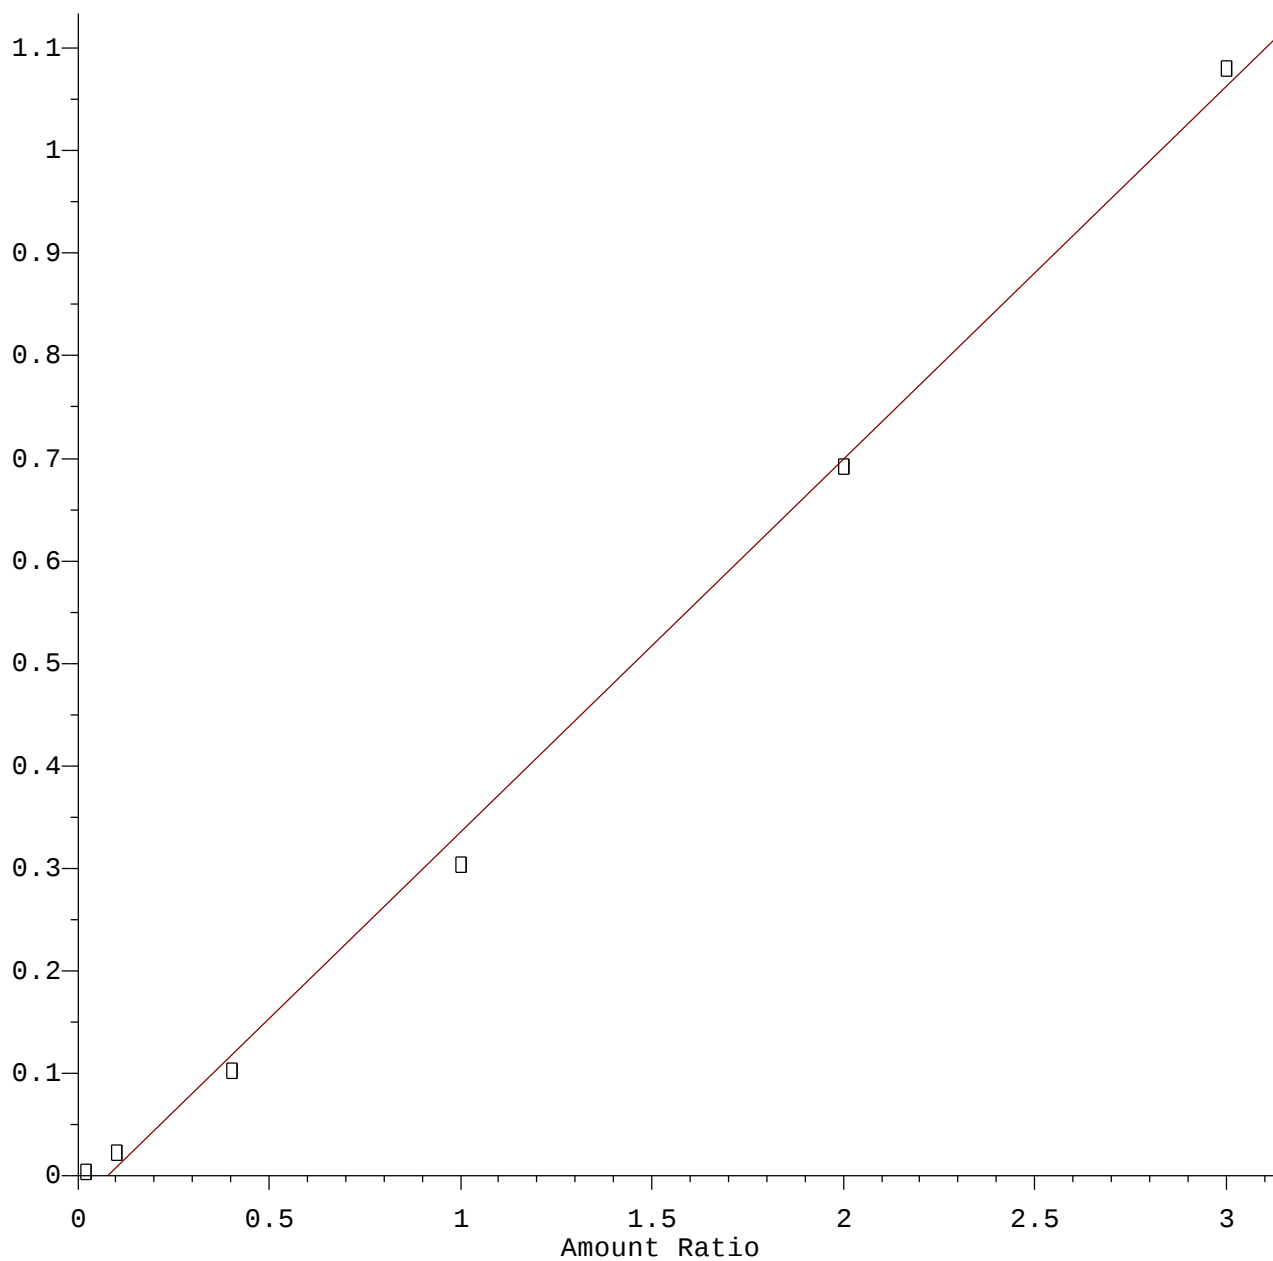


Resp Ratio = $3.63 \times 10^{-1} \times \text{Amt} - 2.75 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Calibration Table Last Updated: Tue Jan 08 14:06:59 2019

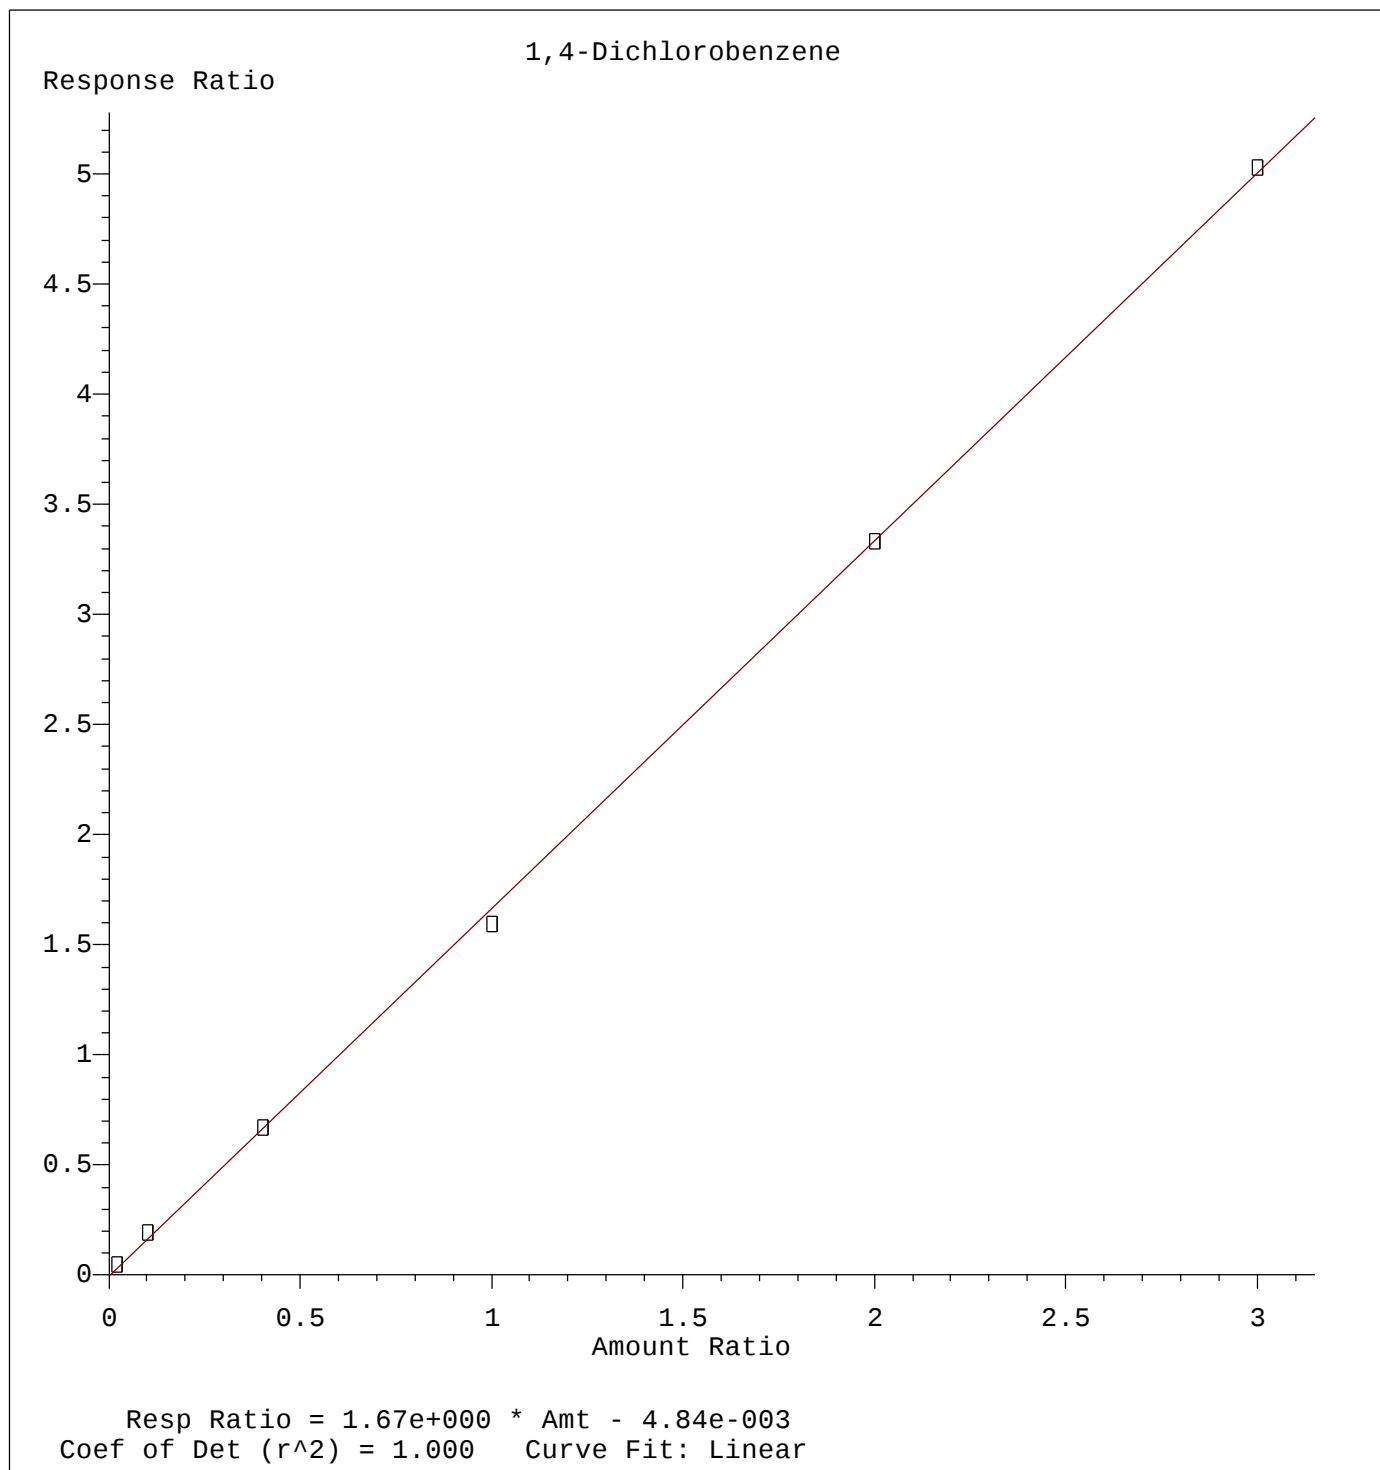

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Calibration Table Last Updated: Tue Jan 08 14:06:59 2019

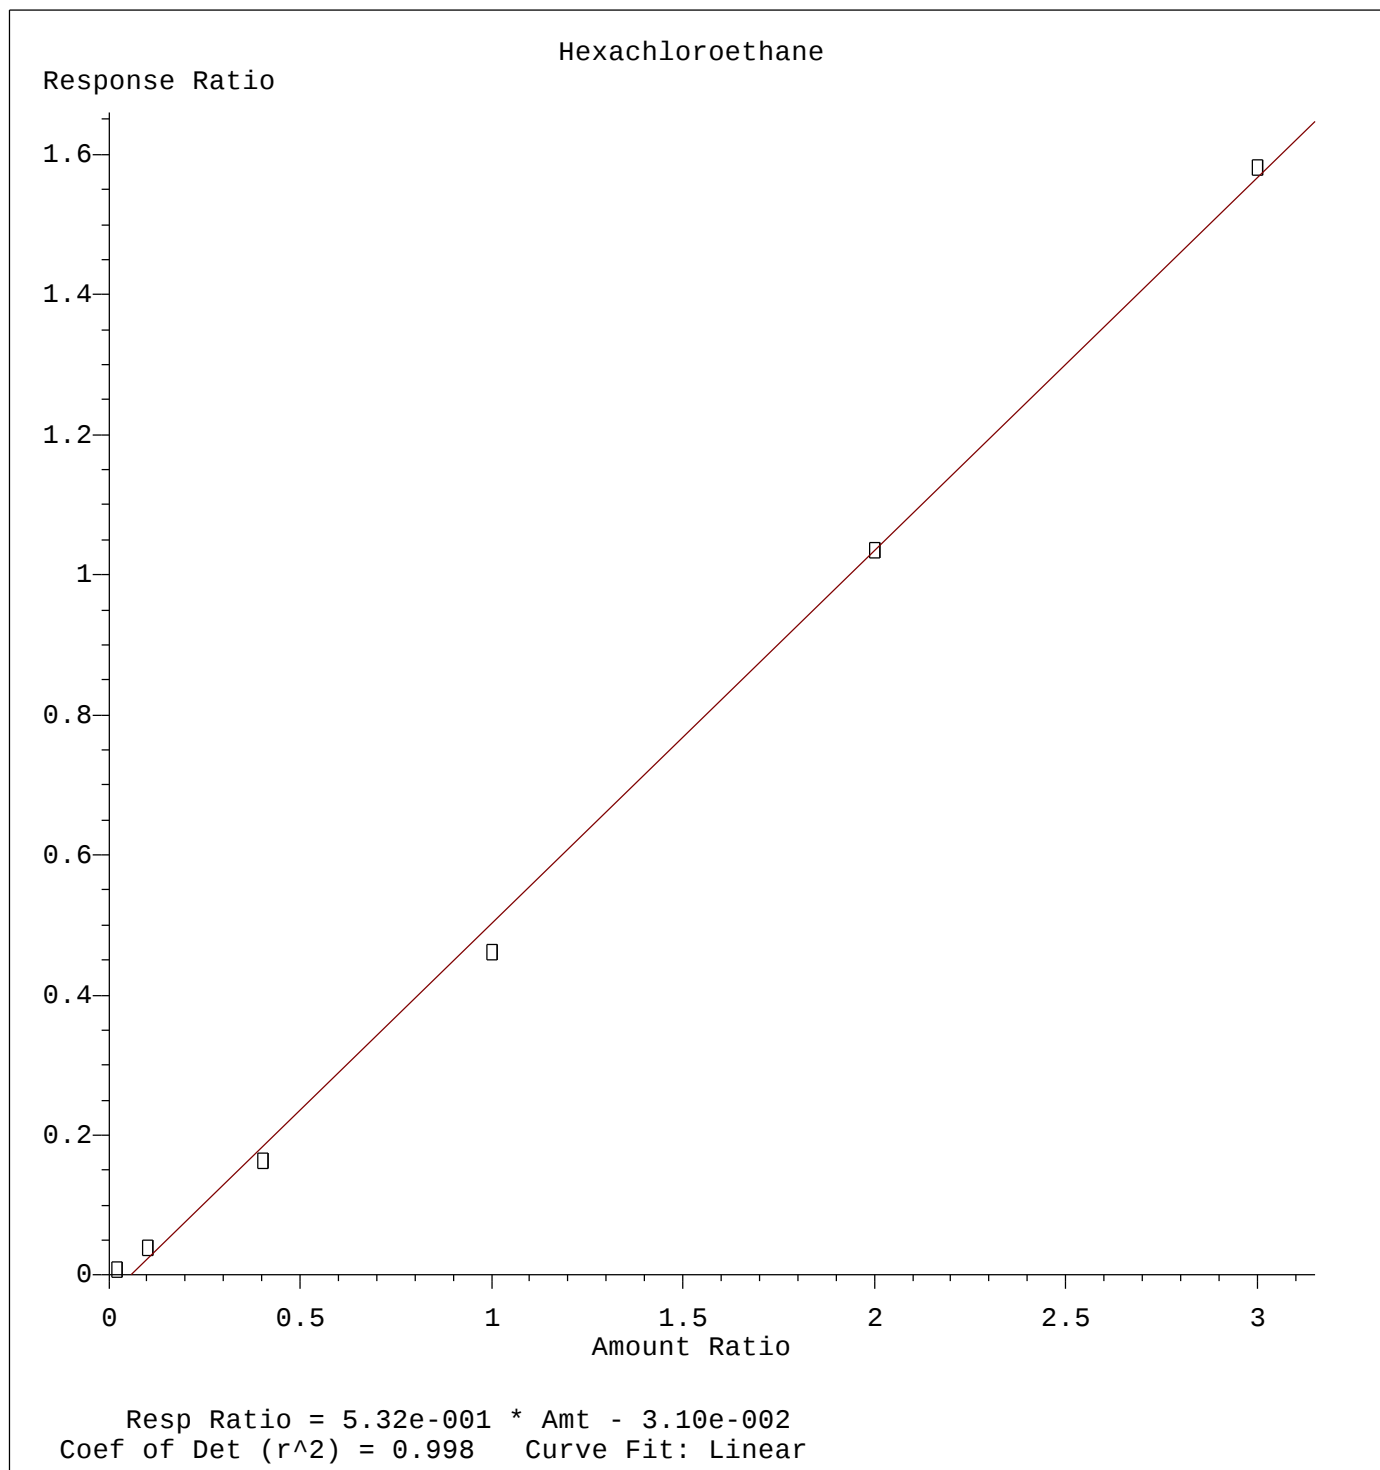

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Calibration Table Last Updated: Tue Jan 08 14:06:59 2019