

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010821\
 Data File : VX020537.D
 Acq On : 08 Jan 2021 14:13
 Operator : JC/MD
 Sample : M1050-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 X2X33

Quant Time: Jan 09 04:42:42 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML010721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jan 09 04:41:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.830	114	389457	50.00	ug/L	0.00
28) Chlorobenzene-d5	10.098	117	358150	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.061	152	178306	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.386	65	125909	40.24	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.48%
7) Chloroethane-d5	1.691	69	83564	34.17	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	68.34%#
11) 1,1-Dichloroethene-d2	2.343	63	228570	39.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.22%
21) 2-Butanone-d5	4.532	46	179545	93.65	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.65%
24) Chloroform-d	5.135	84	250445	46.52	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.04%
26) 1,2-Dichloroethane-d4	6.025	65	162118	45.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.94%
32) Benzene-d6	6.044	84	507592	47.12	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.24%
36) 1,2-Dichloropropane-d6	7.367	67	161290	48.42	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.84%
41) Toluene-d8	8.696	98	465833	47.70	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.40%
43) trans-1,3-Dichloroprop...	8.994	79	73976	45.65	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.30%
47) 2-Hexanone-d5	9.427	63	135552	92.12	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.12%
56) 1,1,2,2-Tetrachloroeth...	11.232	84	218827	47.29	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.58%
66) 1,2-Dichlorobenzene-d4	12.360	152	163290	46.72	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.44%
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.392	62	141564	39.05	ug/L	100
8) Chloroethane	1.709	64	93407	43.02	ug/L	99
12) 1,1-Dichloroethene	2.355	96	89828	32.37	ug/L	97
14) Carbon disulfide	2.550	76	426016	47.84	ug/L	98
15) Methyl Acetate	2.746	43	183568	58.67	ug/L	98
16) Methylene chloride	2.831	84	100925	30.42	ug/L	100
18) Methyl tert-butyl Ether	3.166	73	361901	40.09	ug/L	100
19) 1,1-Dichloroethane	3.666	63	115482	21.37	ug/L	98
20) cis-1,2-Dichloroethene	4.562	96	64789	19.84	ug/L	98
27) 1,2-Dichloroethane	6.160	62	249952	57.48	ug/L	98
30) 1,1,1-Trichloroethane	5.465	97	190585	41.64	ug/L	100
34) Trichloroethene	7.184	95	213240	70.73	ug/L	98
37) 1,2-Dichloropropane	7.489	63	77103	25.68	ug/L	99
40) 4-Methyl-2-pentanone	8.623	43	197107	49.96	ug/L	98
42) Toluene	8.763	91	404635	32.63	ug/L	99
44) trans-1,3-Dichloropropene	9.019	75	69013	15.65	ug/L	99
45) 1,1,2-Trichloroethane	9.196	97	116638	39.25	ug/L	98
46) Tetrachloroethene	9.318	164	86832	37.16	ug/L	98
48) 2-Hexanone	9.476	43	142187	45.61	ug/L	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010821\
 Data File : VX020537.D
 Acq On : 08 Jan 2021 14:13
 Operator : JC/MD
 Sample : M1050-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 X2X33

Quant Time: Jan 09 04:42:42 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML010721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jan 09 04:41:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


50) 1,2-Dibromoethane	9.653	107	118285	38.42	ug/L	100
51) Chlorobenzene	10.122	112	389161	49.57	ug/L	98
52) Ethylbenzene	10.232	91	819798	61.82	ug/L	99
53) m,p-Xylene	10.336	106	215650	43.53	ug/L	97
54) o-Xylene	10.683	106	101318	21.07	ug/L	92
55) Styrene	10.695	104	289041	35.51	ug/L	99
57) 1,1,2,2-Tetrachloroethane	11.250	83	317289	67.28	ug/L	99
59) Bromoform	10.842	173	40467	18.17	ug/L	99
60) Isopropylbenzene	11.000	105	545428	43.38	ug/L	100
64) 1,3-Dichlorobenzene	12.006	146	116051	19.79	ug/L	96
65) 1,4-Dichlorobenzene	12.079	146	238137	40.18	ug/L	99
67) 1,2-Dichlorobenzene	12.372	146	359983	61.56	ug/L	98
68) 1,2-Dibromo-3-chloropr...	12.982	75	70806	71.97	ug/L	99
72) 1,2,3-Trichlorobenzene	14.000	180	134660	37.76	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010821\
Data File : VX020537.D
Acq On : 08 Jan 2021 14:13
Operator : JC/MD
Sample : M1050-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
X2X33

Quant Time: Jan 09 04:42:42 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML010721WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jan 09 04:41:43 2021
Response via : Initial Calibration




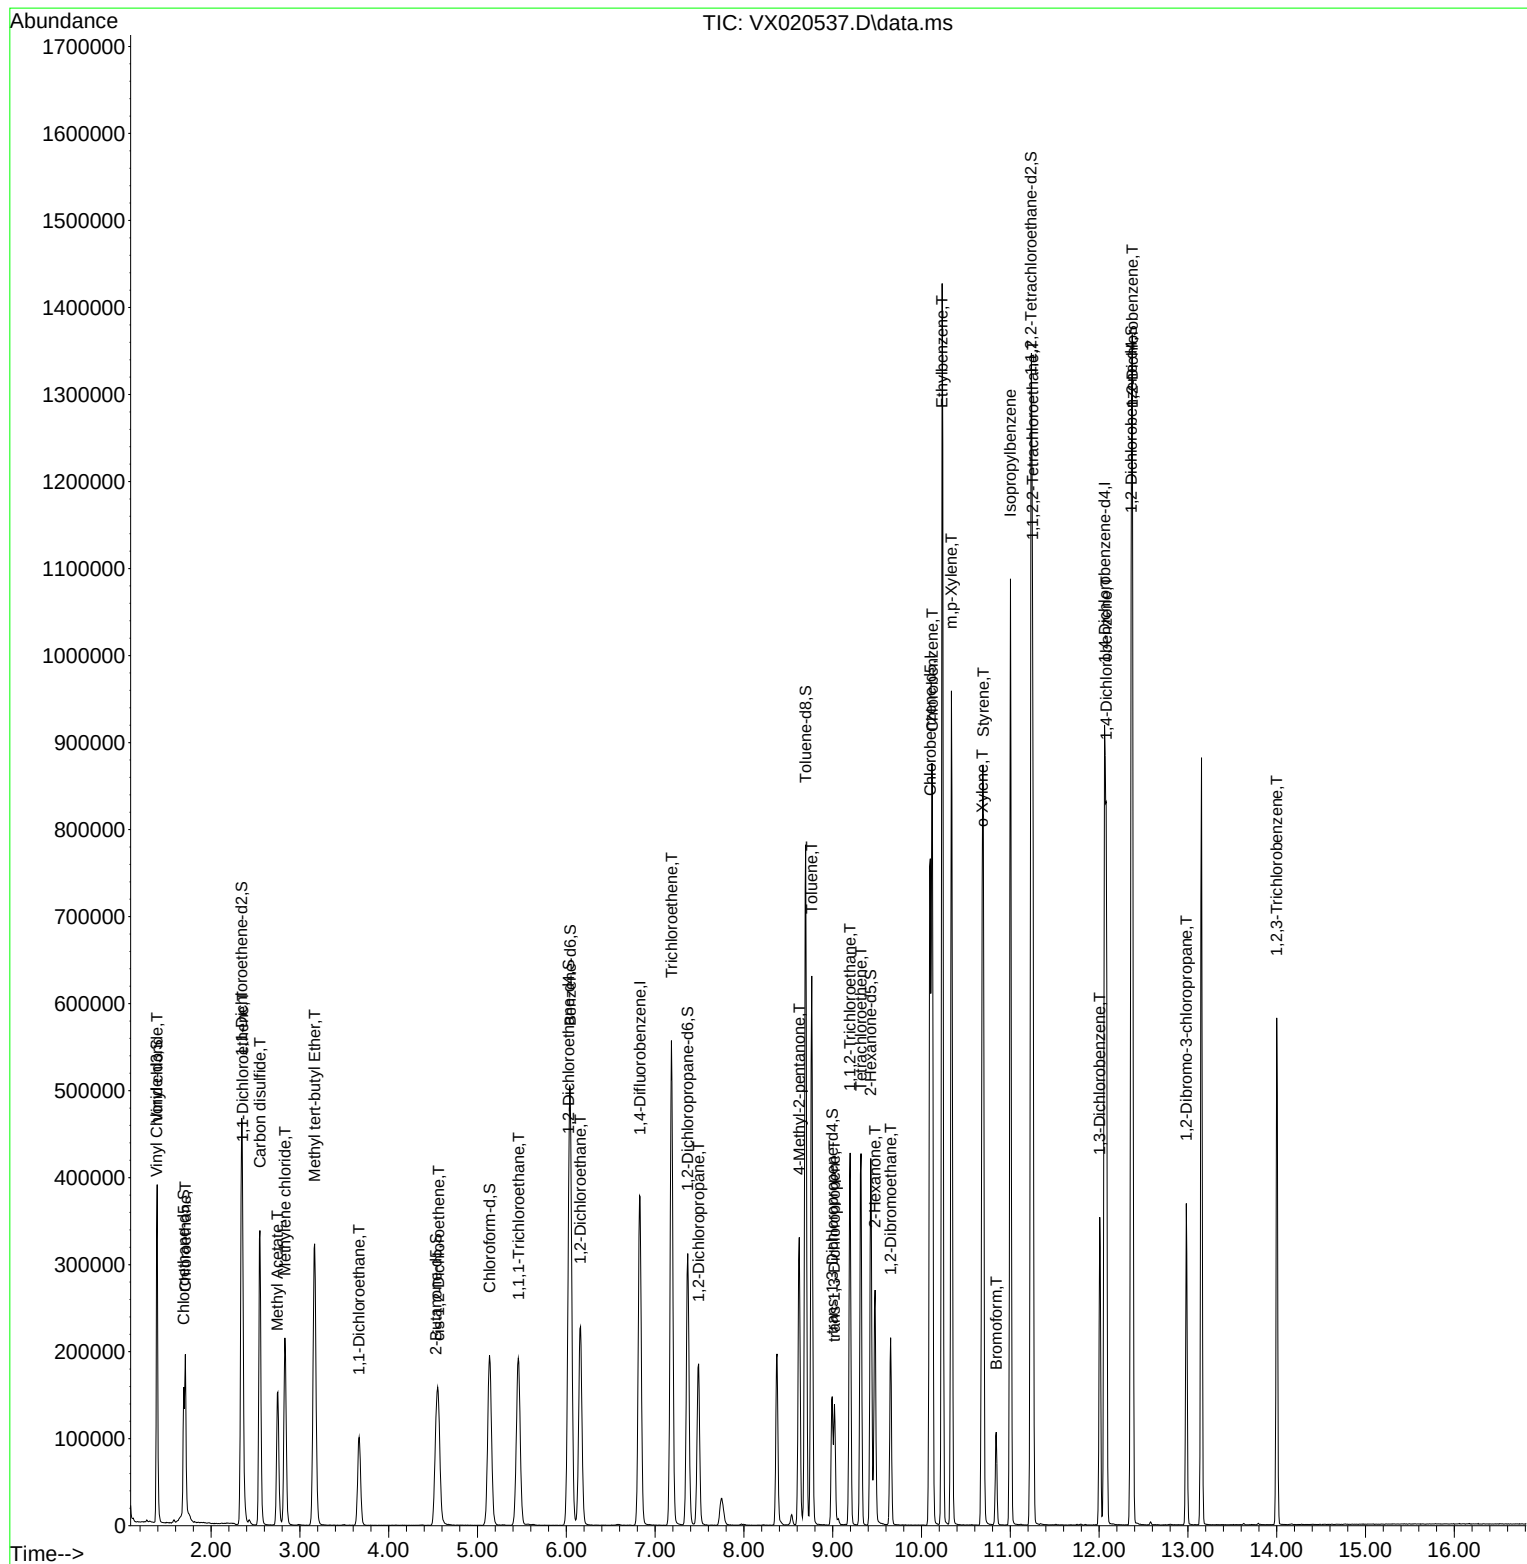


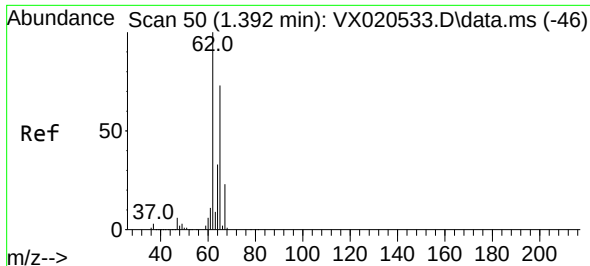

#5
 Vinyl chloride
 Concen: 39.05 ug/L
 RT: 1.392 min Scan# 50
 Delta R.T. 0.000 min
 Lab File: VX020537.D
 Acq: 08 Jan 2021 14:13




Instrument :
 MSVOA_X
 ClientSampleId :
 X2X33


Tgt Ion: 62 Resp: 141564
 Ion Ratio Lower Upper
 62 100
 64 32.3 22.7 42.3

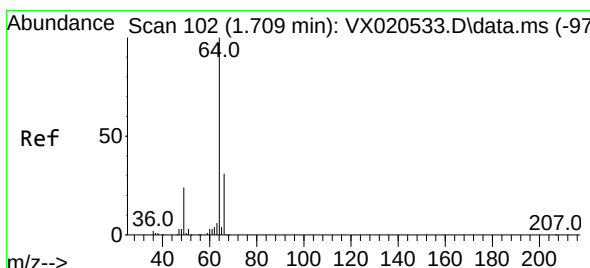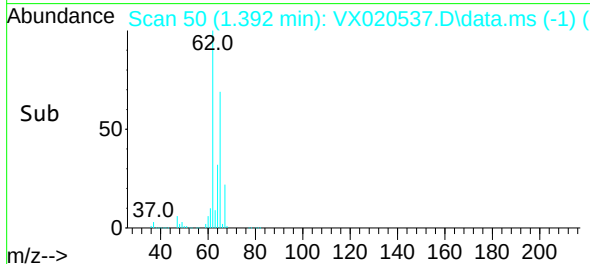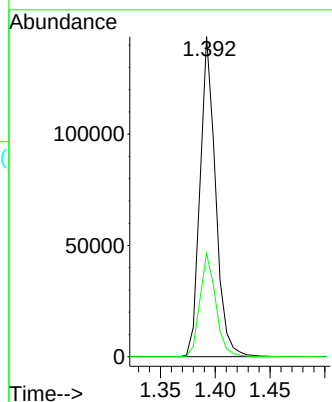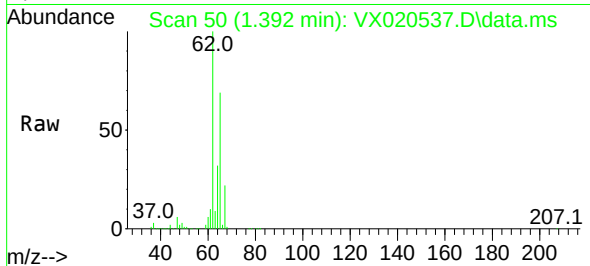

#8
 Chloroethane
 Concen: 43.02 ug/L
 RT: 1.709 min Scan# 102
 Delta R.T. 0.000 min
 Lab File: VX020537.D
 Acq: 08 Jan 2021 14:13

Tgt Ion: 64 Resp: 93407
 Ion Ratio Lower Upper
 64 100
 66 31.0 22.0 41.0


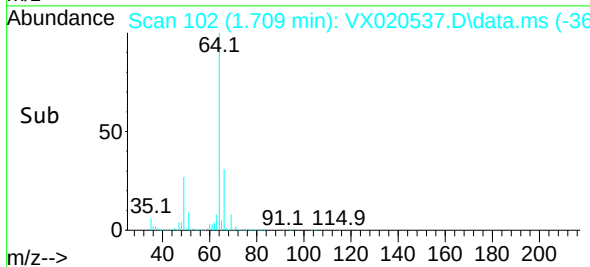
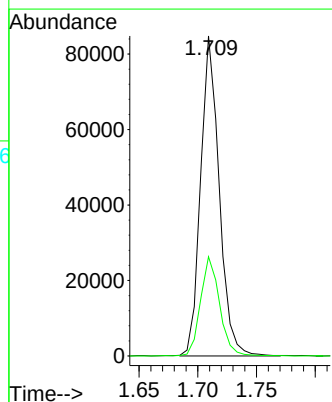
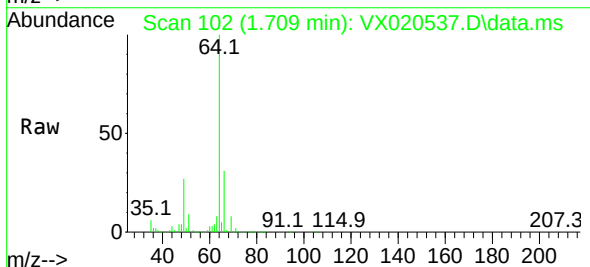


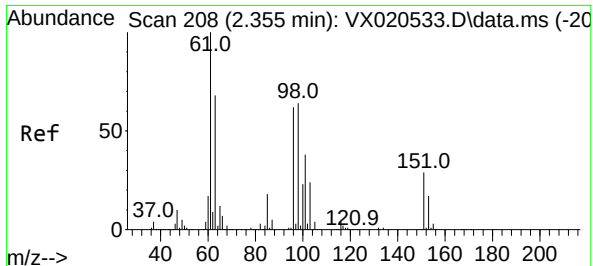

#12
1,1-Dichloroethene
Concen: 32.37 ug/L
RT: 2.355 min Scan# 208
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13




Instrument :
MSVOA_X
ClientSampled :
X2X33


Tgt Ion: 96 Resp: 89828
Ion Ratio Lower Upper
96 100
61 167.0 115.5 214.5
63 117.0 77.3 143.7

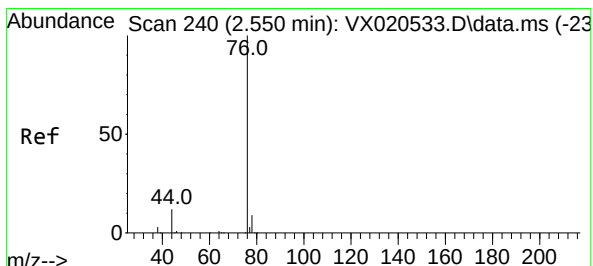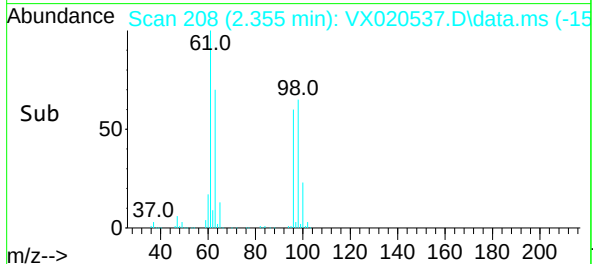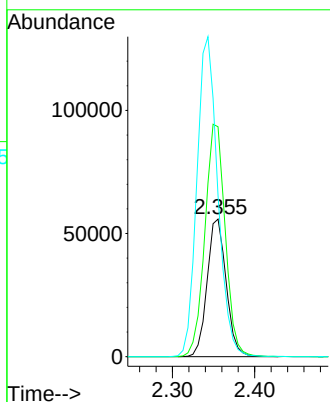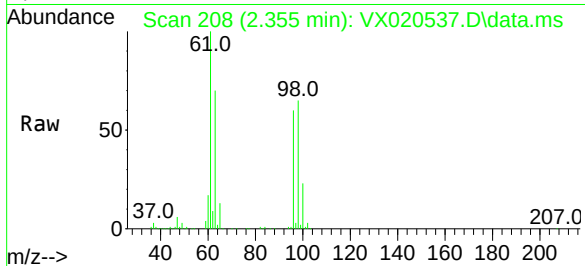

#14
Carbon disulfide
Concen: 47.84 ug/L
RT: 2.550 min Scan# 240
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13

Tgt Ion: 76 Resp: 426016
Ion Ratio Lower Upper
76 100
78 8.8 7.6 11.4


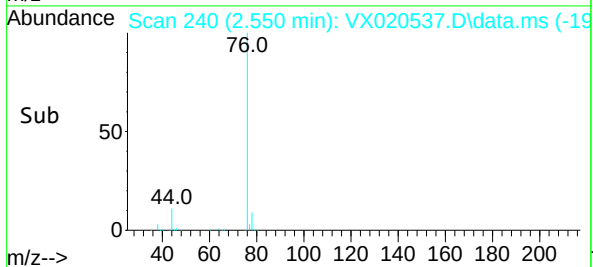
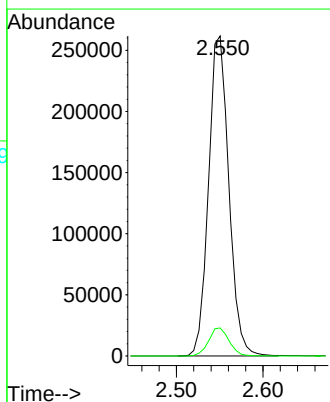
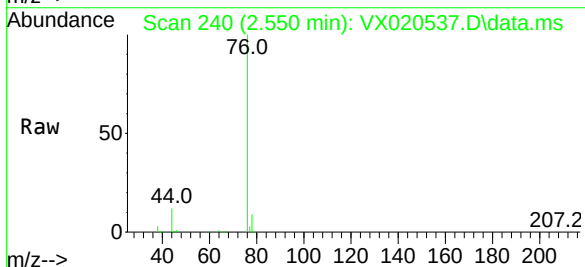




#15
Methyl Acetate
Concen: 58.67 ug/L
RT: 2.746 min Scan# 272
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13




Instrument :
MSVOA_X
ClientSampled :
X2X33


Tgt Ion: 43 Resp: 183568
Ion Ratio Lower Upper
43 100
74 26.0 21.7 32.5

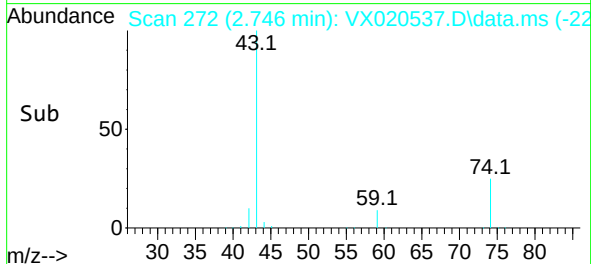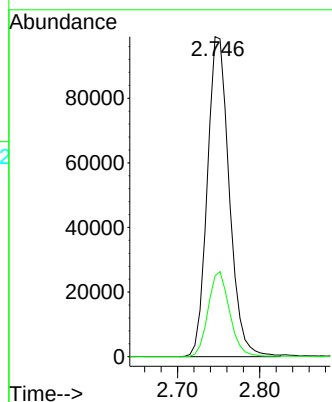

#16
Methylene chloride
Concen: 30.42 ug/L
RT: 2.831 min Scan# 286
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13


Tgt Ion: 84 Resp: 100925
Ion Ratio Lower Upper
84 100
86 62.9 44.2 82.0
49 111.8 77.8 144.6

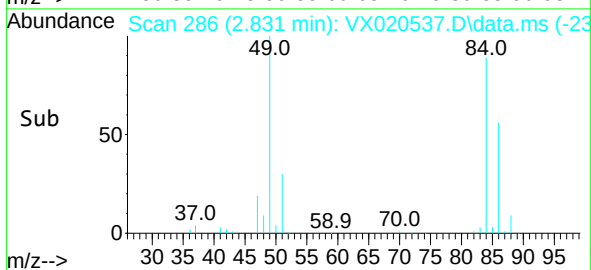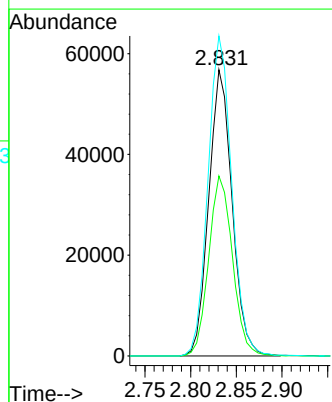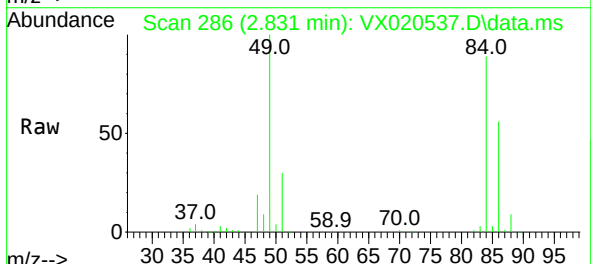






#18
Methyl tert-butyl Ether
Concen: 40.09 ug/L
RT: 3.166 min Scan# 341
Delta R.T. 0.006 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13

Instrument :
MSVOA_X
ClientSampleId :
X2X33







Tgt Ion: 73 Resp: 361901
Ion Ratio Lower Upper
73 100
43 19.1 15.1 22.7
57 21.8 17.4 26.2

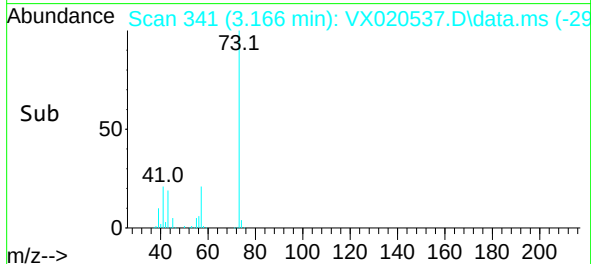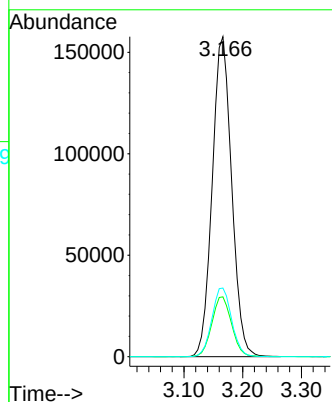

#19
1,1-Dichloroethane
Concen: 21.37 ug/L
RT: 3.666 min Scan# 423
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13

Tgt Ion: 63 Resp: 115482
Ion Ratio Lower Upper
63 100
65 30.6 22.4 41.6
83 12.8 9.5 17.7


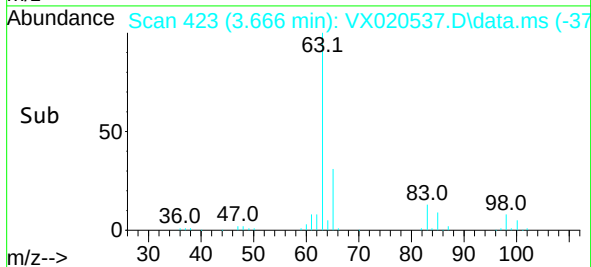
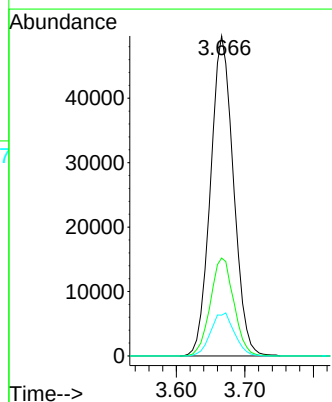
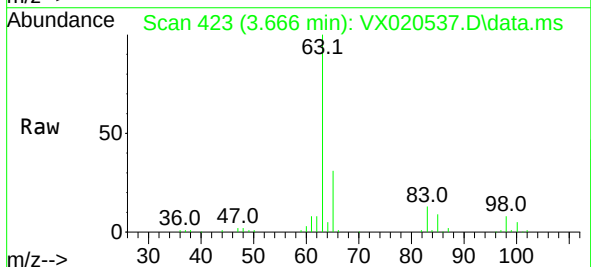




#20
cis-1,2-Dichloroethene
Concen: 19.84 ug/L
RT: 4.562 min Scan# 570
Delta R.T. 0.006 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13




Instrument :
MSVOA_X
ClientSampled :
X2X33


Tgt Ion: 96 Resp: 64789
Ion Ratio Lower Upper
96 100
61 123.4 87.8 163.0
68 0.0 0.0 0.0

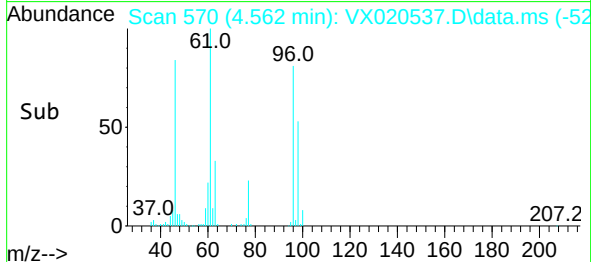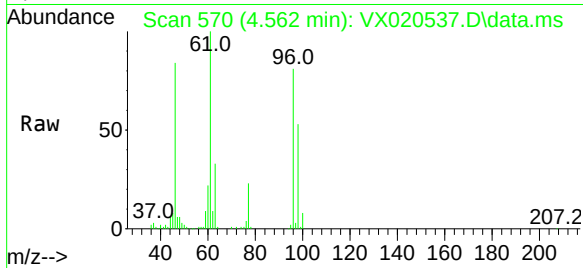

#27
1,2-Dichloroethane
Concen: 57.48 ug/L
RT: 6.160 min Scan# 832
Delta R.T. 0.006 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13

Tgt Ion: 62 Resp: 249952
Ion Ratio Lower Upper
62 100
98 10.7 7.9 11.9


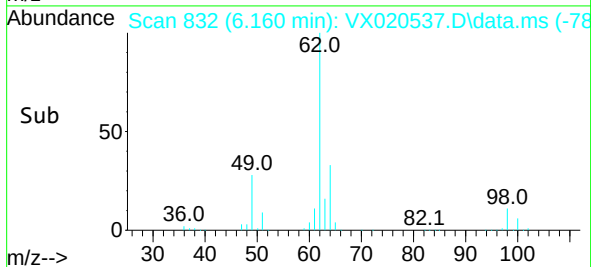

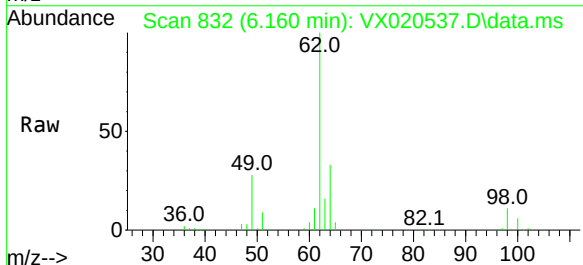


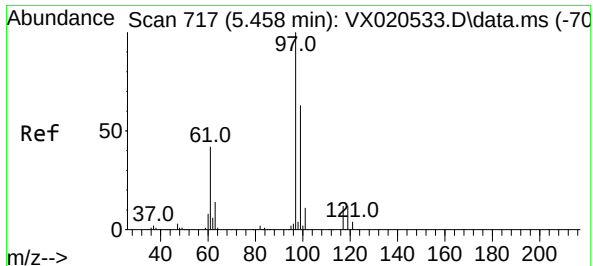

#30
1,1,1-Trichloroethane
Concen: 41.64 ug/L
RT: 5.465 min Scan# 718
Delta R.T. 0.006 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13




Instrument :
MSVOA_X
ClientSampleId :
X2X33


Tgt Ion: 97 Resp: 190585
Ion Ratio Lower Upper
97 100
99 64.5 52.1 78.1
61 44.1 35.3 52.9

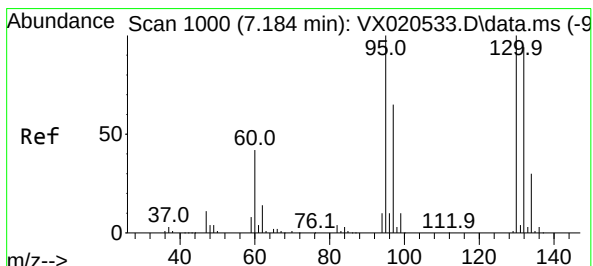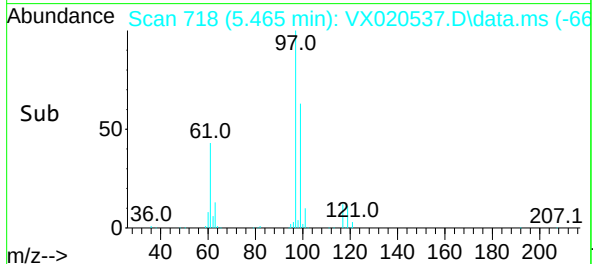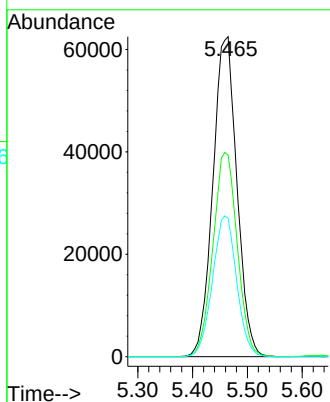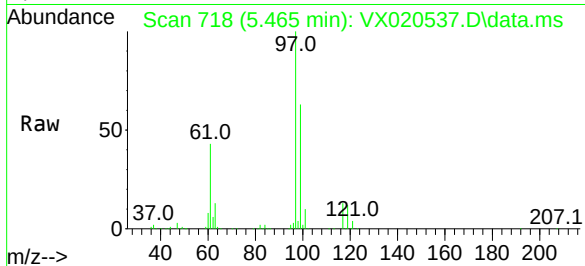

#34
Trichloroethene
Concen: 70.73 ug/L
RT: 7.184 min Scan# 1000
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13

Tgt Ion: 95 Resp: 213240
Ion Ratio Lower Upper
95 100
97 65.3 44.5 82.7
132 93.5 65.2 121.0
130 100.1 67.7 125.7


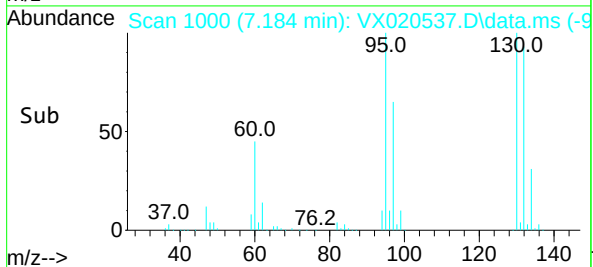
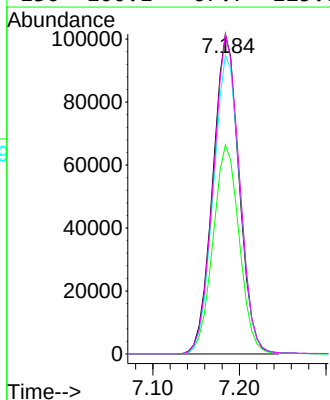
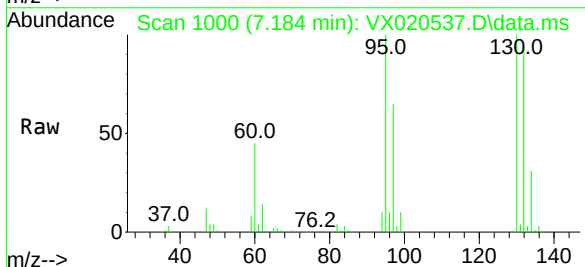


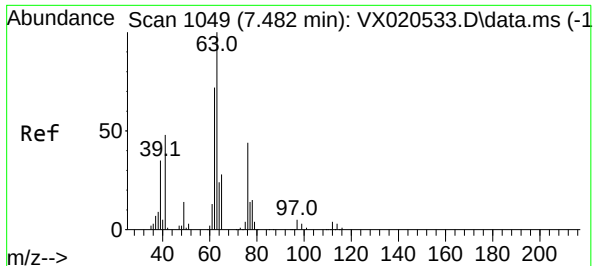

#37
1,2-Dichloropropane
Concen: 25.68 ug/L
RT: 7.489 min Scan# 1050
Delta R.T. 0.006 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13




Instrument :
MSVOA_X
ClientSampled :
X2X33


Tgt Ion: 63 Resp: 77103
Ion Ratio Lower Upper
63 100
112 4.7 3.6 5.4

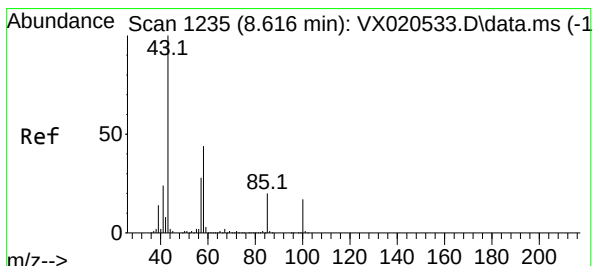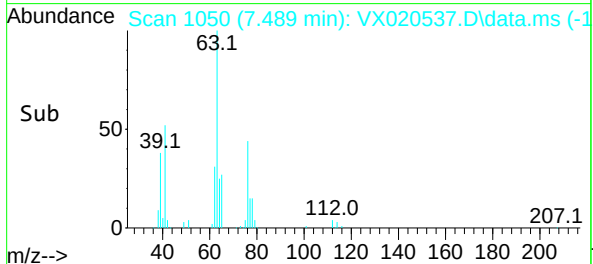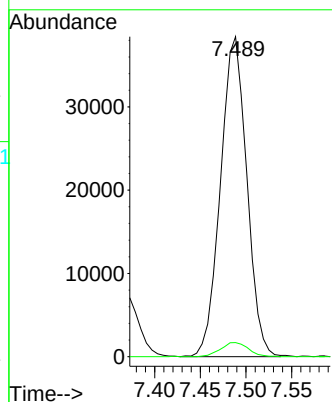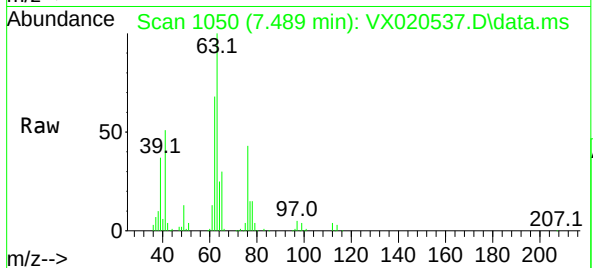

#40
4-Methyl-2-pentanone
Concen: 49.96 ug/L
RT: 8.623 min Scan# 1236
Delta R.T. 0.006 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13

Tgt Ion: 43 Resp: 197107
Ion Ratio Lower Upper
43 100
58 42.7 35.0 52.4
100 16.9 14.2 21.4


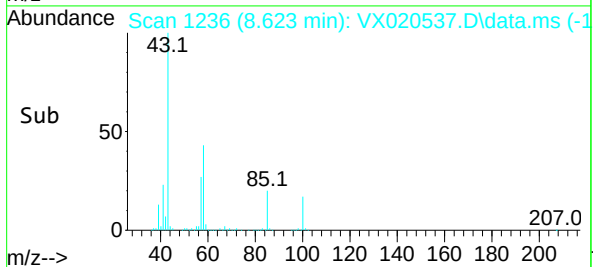
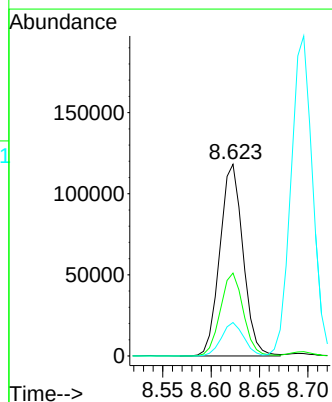
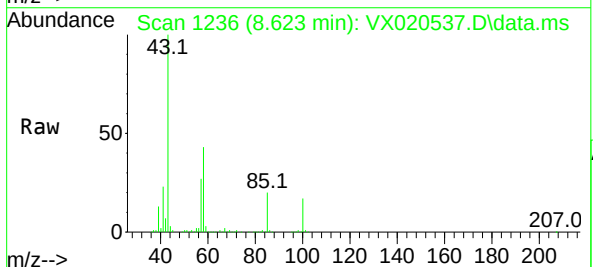




#42
Toluene
Concen: 32.63 ug/L
RT: 8.763 min Scan# 1259
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13




Instrument :
MSVOA_X
ClientSampled :
X2X33


Tgt Ion: 91 Resp: 404635
Ion Ratio Lower Upper
91 100
92 58.6 40.5 75.1

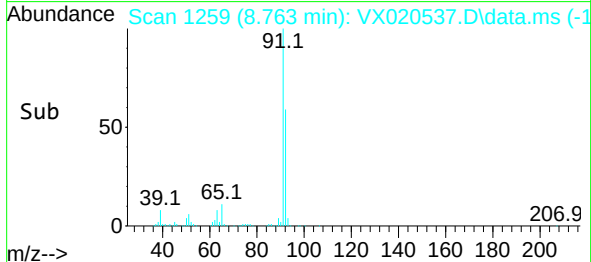

#44
trans-1,3-Dichloropropene
Concen: 15.65 ug/L
RT: 9.019 min Scan# 1301
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13

Tgt Ion: 75 Resp: 69013
Ion Ratio Lower Upper
75 100
77 31.7 22.4 41.6

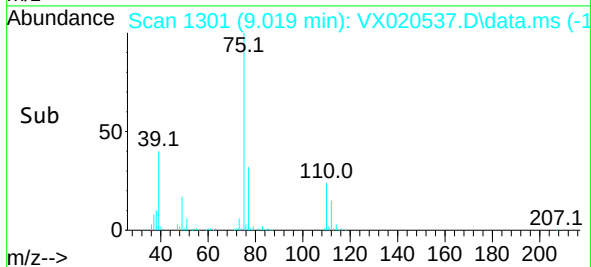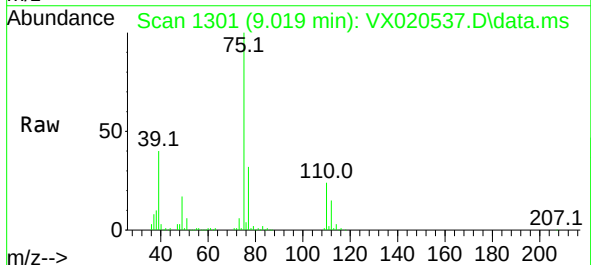




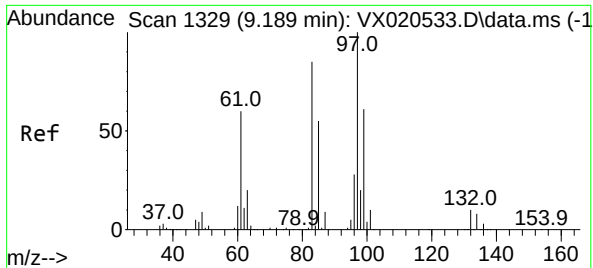


#45
1,1,2-Trichloroethane
Concen: 39.25 ug/L
RT: 9.196 min Scan# 1330
Delta R.T. 0.006 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13

Instrument :
MSVOA_X
ClientSampled :
X2X33

Tgt Ion: 97 Resp: 116638




Ion	Ratio	Lower	Upper
97	100		
99	62.5	44.0	81.6
83	85.4	60.8	113.0
85	54.2	39.4	73.2

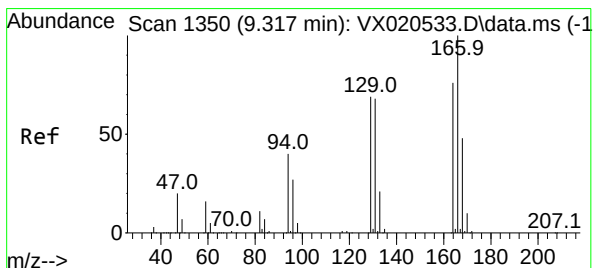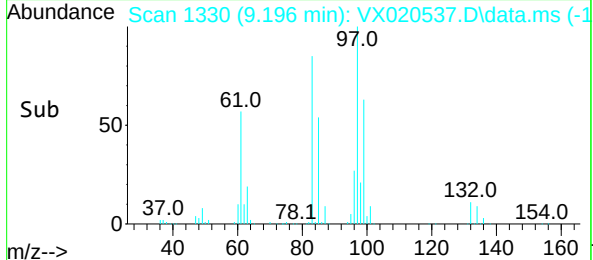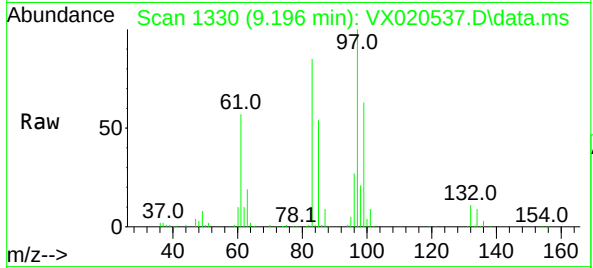


#46
Tetrachloroethene
Concen: 37.16 ug/L
RT: 9.318 min Scan# 1350
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13

Tgt Ion: 164 Resp: 86832

Ion	Ratio	Lower	Upper
164	100		
129	93.5	65.6	121.8
131	89.7	63.7	118.3
166	128.7	93.0	172.6


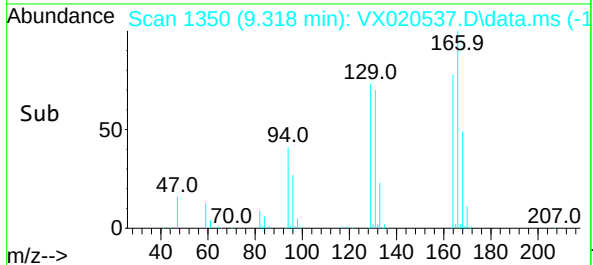
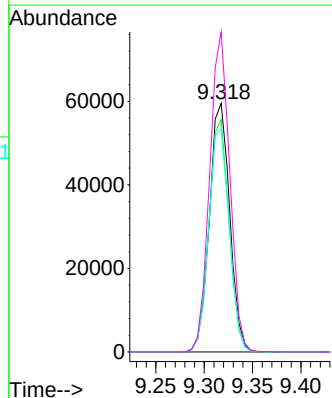
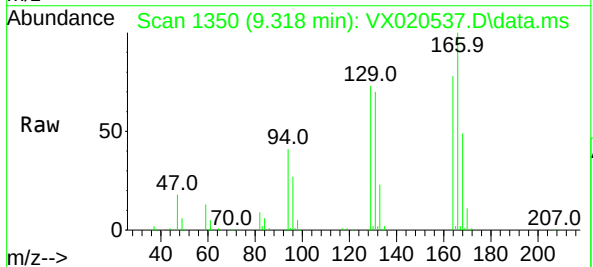




#48
2-Hexanone
Concen: 45.61 ug/L
RT: 9.476 min Scan# 1376
Delta R.T. 0.006 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13




Instrument :
MSVOA_X
ClientSampleId :
X2X33


Tgt Ion: 43 Resp: 142187
Ion Ratio Lower Upper
43 100
58 62.7 50.1 75.1
57 21.2 17.3 25.9
100 14.4 11.4 17.2

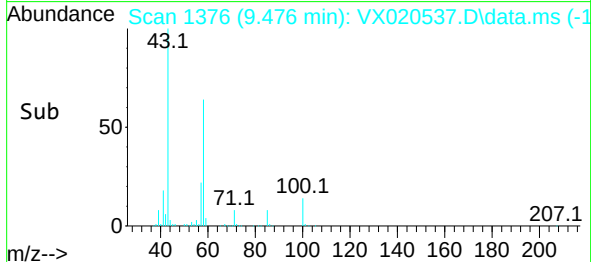

#50
1,2-Dibromoethane
Concen: 38.42 ug/L
RT: 9.653 min Scan# 1405
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13

Tgt Ion: 107 Resp: 118285
Ion Ratio Lower Upper
107 100
109 95.4 66.4 123.4
188 4.2 3.2 4.8


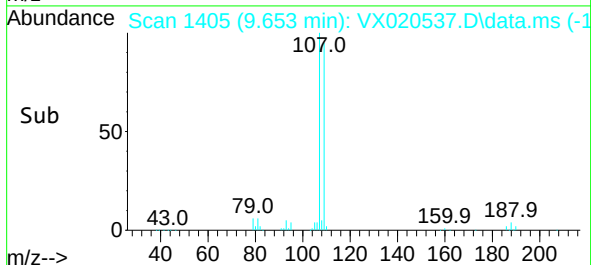
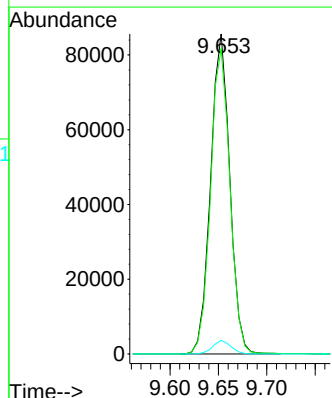
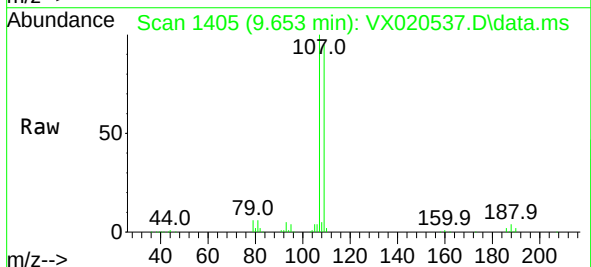




#51
Chlorobenzene
Concen: 49.57 ug/L
RT: 10.122 min Scan# 1482
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13




Instrument :
MSVOA_X
ClientSampled :
X2X33


Tgt Ion:112 Resp: 389161
Ion Ratio Lower Upper
112 100
114 32.2 23.2 43.2
77 59.0 48.4 72.6

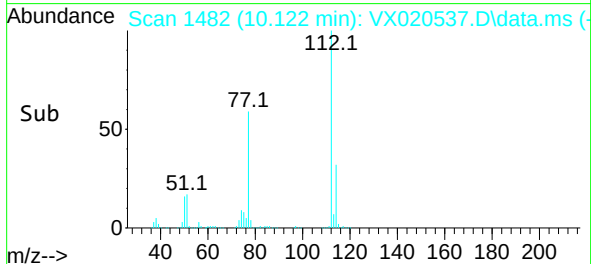

#52
Ethylbenzene
Concen: 61.82 ug/L
RT: 10.232 min Scan# 1500
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13

Tgt Ion: 91 Resp: 819798
Ion Ratio Lower Upper
91 100
106 30.5 21.0 39.0




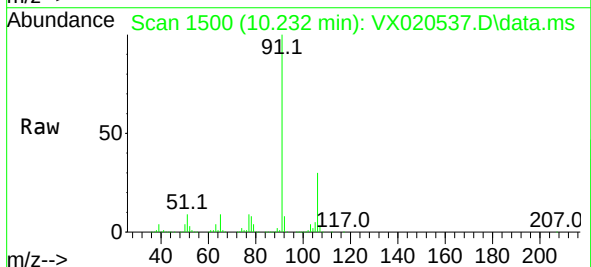




#53
m,p-Xylene
Concen: 43.53 ug/L
RT: 10.336 min Scan# 1517
Delta R.T. -0.006 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13




Instrument :
MSVOA_X
ClientSampleId :
X2X33


Tgt Ion:106 Resp: 215650
Ion Ratio Lower Upper
106 100
91 207.5 142.5 264.6

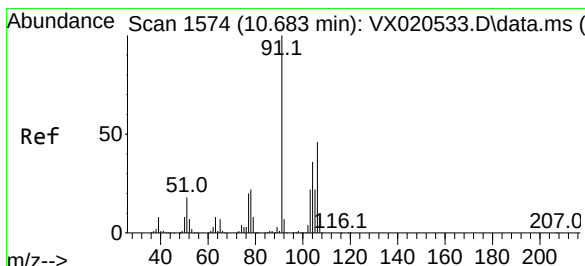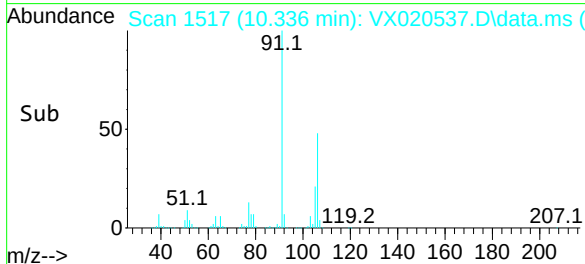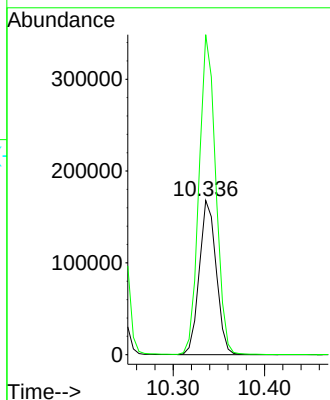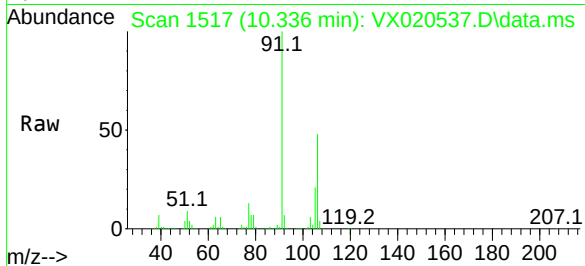

#54
o-Xylene
Concen: 21.07 ug/L
RT: 10.683 min Scan# 1574
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13

Tgt Ion:106 Resp: 101318
Ion Ratio Lower Upper
106 100
91 209.3 156.2 290.0

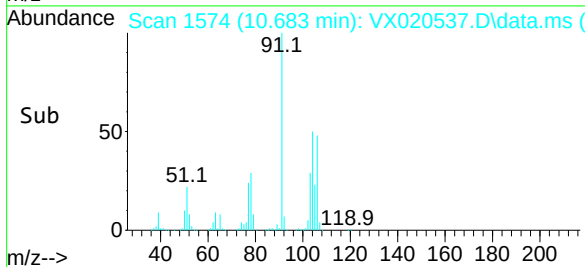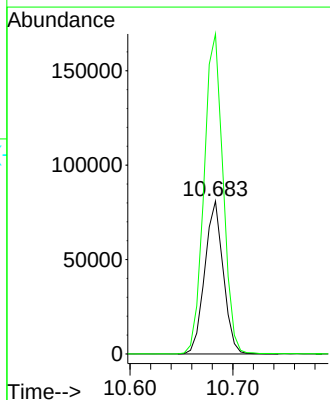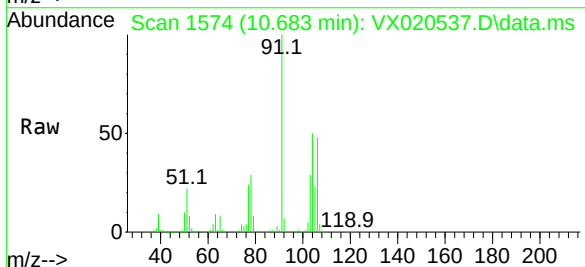



#55

Styrene

Concen: 35.51 ug/L

RT: 10.695 min Scan# 1576

Delta R.T. 0.000 min

Lab File: VX020537.D

Acq: 08 Jan 2021 14:13

Tgt Ion:104 Resp: 289041

Ion Ratio Lower Upper





Ion	Ratio	Lower	Upper
104	100		
78	43.6	30.0	55.6

Instrument :

MSVOA_X

ClientSampled :

X2X33

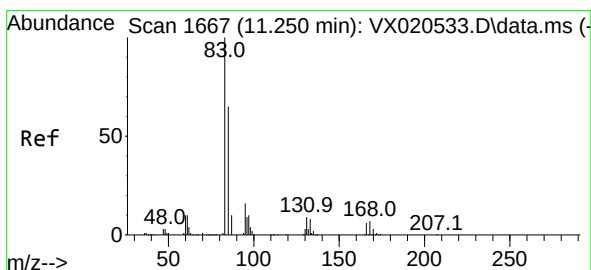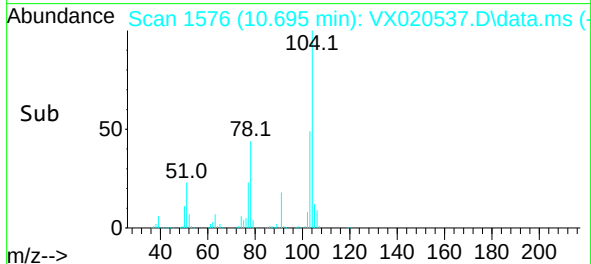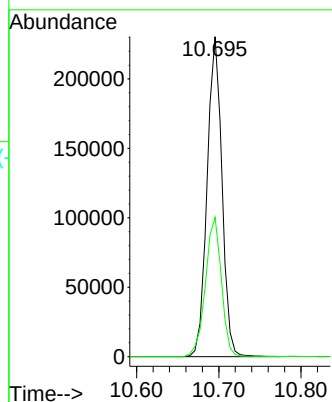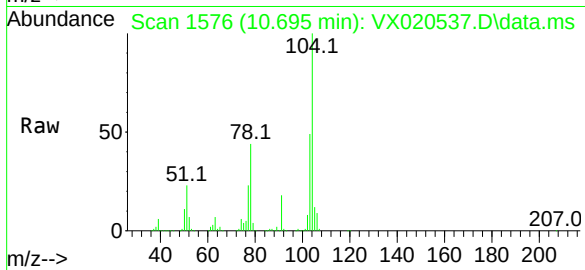

#57

1,1,2,2-Tetrachloroethane

Concen: 67.28 ug/L

RT: 11.250 min Scan# 1667

Delta R.T. 0.000 min




Lab File: VX020537.D


Acq: 08 Jan 2021 14:13

Tgt Ion: 83 Resp: 317289

Ion Ratio Lower Upper


Ion	Ratio	Lower	Upper
83	100		
85	64.5	44.7	82.9
131	9.5	7.8	11.8

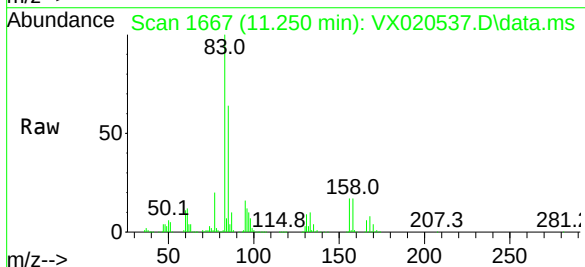






#59
Bromoform
Concen: 18.17 ug/L
RT: 10.842 min Scan# 1600
Delta R.T. 0.006 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13

Instrument :
MSVOA_X
ClientSampleId :
X2X33







Tgt Ion:173 Resp: 40467
Ion Ratio Lower Upper
173 100
175 48.4 39.4 59.2
254 10.5 8.6 13.0

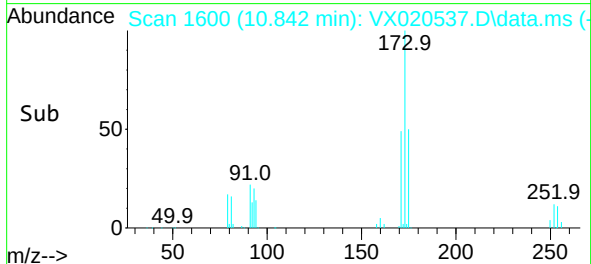

#60
Isopropylbenzene
Concen: 43.38 ug/L
RT: 11.000 min Scan# 1626
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13

Tgt Ion:105 Resp: 545428
Ion Ratio Lower Upper
105 100
120 26.4 21.2 31.8
77 15.7 12.6 18.8


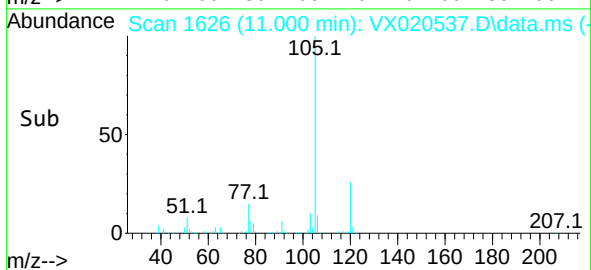

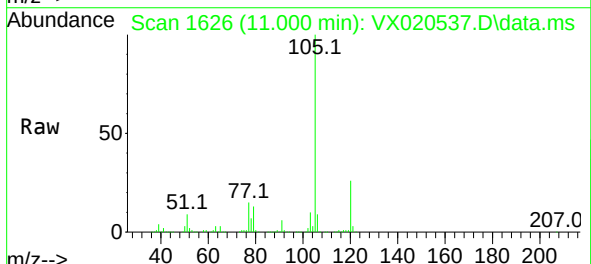


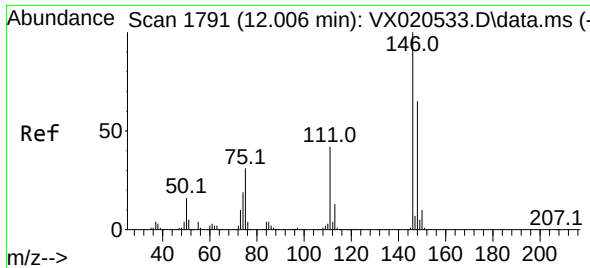

#64
1,3-Dichlorobenzene
Concen: 19.79 ug/L
RT: 12.006 min Scan# 1791
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13




Instrument :
MSVOA_X
ClientSampled :
X2X33


Tgt Ion:146 Resp: 116051
Ion Ratio Lower Upper
146 100
111 40.4 28.9 53.7
148 63.5 47.7 88.7

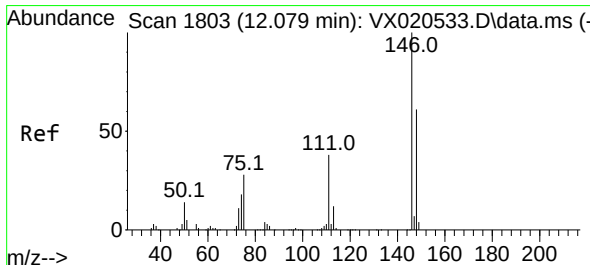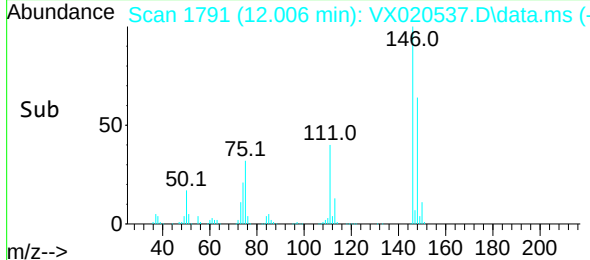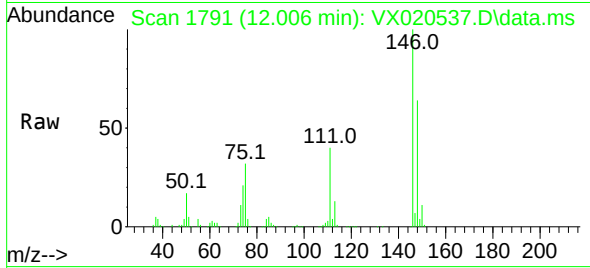

#65
1,4-Dichlorobenzene
Concen: 40.18 ug/L
RT: 12.079 min Scan# 1803
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13

Tgt Ion:146 Resp: 238137
Ion Ratio Lower Upper
146 100
111 40.7 28.7 53.3
148 66.1 45.8 85.2


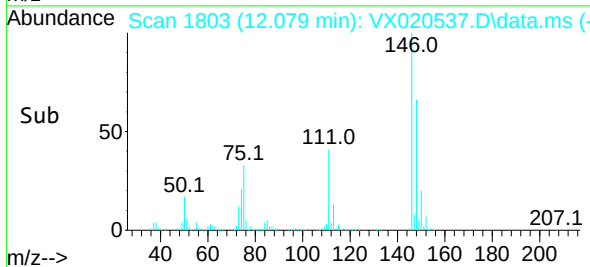

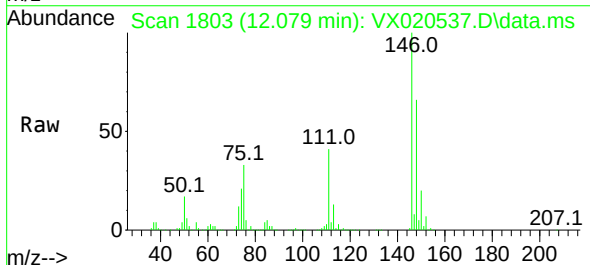




#67
1,2-Dichlorobenzene
Concen: 61.56 ug/L
RT: 12.372 min Scan# 1851
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13




Instrument :
MSVOA_X
ClientSampled :
X2X33


Tgt Ion:146 Resp: 359983
Ion Ratio Lower Upper
146 100
111 43.8 33.8 50.8
148 63.2 51.4 77.2

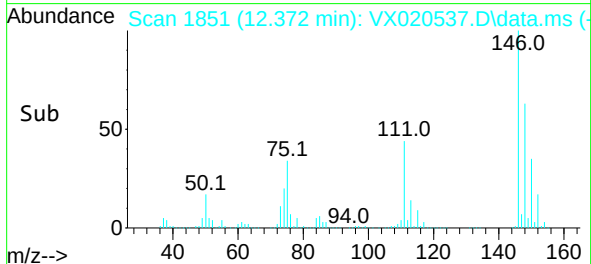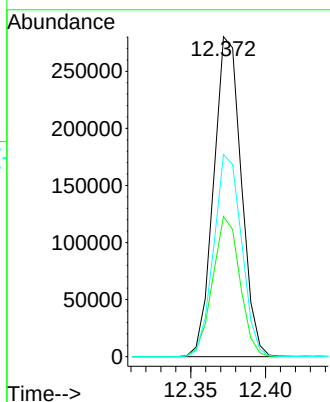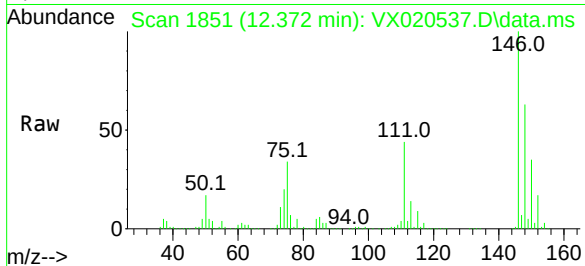

#68
1,2-Dibromo-3-chloropropane
Concen: 71.97 ug/L
RT: 12.982 min Scan# 1951
Delta R.T. 0.000 min
Lab File: VX020537.D
Acq: 08 Jan 2021 14:13

Tgt Ion: 75 Resp: 70806
Ion Ratio Lower Upper
75 100
155 83.6 65.3 97.9
157 100.3 80.5 120.7

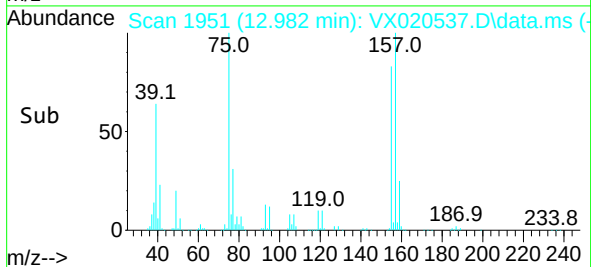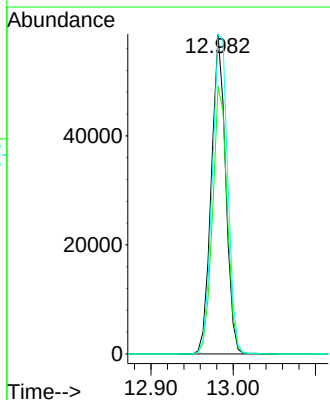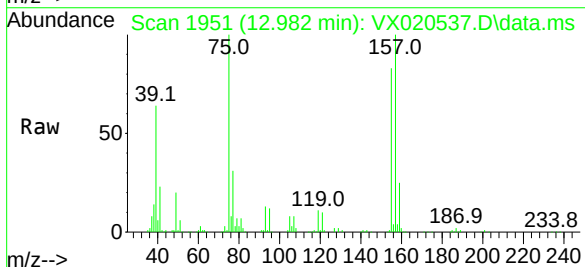



#72

1,2,3-Trichlorobenzene

Concen: 37.76 ug/L

RT: 14.000 min Scan# 2118

Delta R.T. 0.000 min

Lab File: VX020537.D


Acq: 08 Jan 2021 14:13

Instrument :

MSVOA_X

ClientSampleId :

X2X33

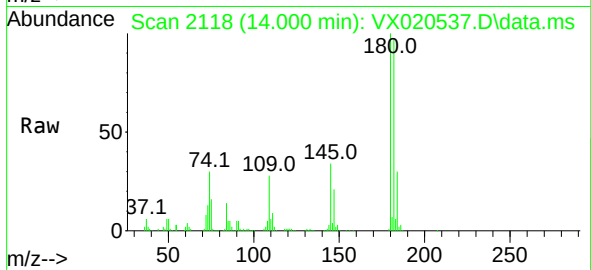

Tgt Ion:180 Resp: 134660

Ion Ratio Lower Upper

180 100

182 96.9 74.6 112.0

145 33.3 25.6 38.4

