

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010821\
 Data File : VX020534.D
 Acq On : 08 Jan 2021 10:28
 Operator : JC/MD
 Sample : VX0108MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK403

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML010721WMA.M

Title : VOC Analysis

Signal : TIC: VX020534.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.386	46	49	58	rVB	209936	214346	13.63%	1.885%
2	1.697	95	100	112	rVB	170694	216802	13.78%	1.907%
3	2.343	199	206	222	rBV	346517	569642	36.22%	5.010%
4	2.550	235	240	244	rBV3	1148	2067	0.13%	0.018%
5	2.642	250	255	259	rBV3	419	890	0.06%	0.008%
6	2.837	281	287	292	rVB5	1377	2531	0.16%	0.022%
7	2.989	306	312	320	rVV	5149	11524	0.73%	0.101%
8	3.050	320	322	326	rVB2	320	382	0.02%	0.003%
9	3.087	326	328	330	rBV2	241	243	0.02%	0.002%
10	3.142	333	337	342	rVB2	596	879	0.06%	0.008%
11	3.428	381	384	387	rBV2	237	341	0.02%	0.003%
12	3.544	401	403	405	rBV2	291	260	0.02%	0.002%
13	3.593	407	411	412	rBV2	248	223	0.01%	0.002%
14	3.788	442	443	447	rVB2	181	221	0.01%	0.002%
15	3.843	450	452	454	rBV	253	249	0.02%	0.002%
16	3.879	454	458	459	rBV2	234	251	0.02%	0.002%
17	3.934	464	467	470	rVB2	181	283	0.02%	0.002%
18	4.288	523	525	528	rVB2	298	224	0.01%	0.002%
19	4.526	554	564	578	rBV	107578	320036	20.35%	2.815%
20	4.812	609	611	614	rVB2	251	245	0.02%	0.002%
21	4.897	624	625	629	rVB2	343	342	0.02%	0.003%
22	4.934	629	631	634	rBV2	257	235	0.01%	0.002%
23	5.135	650	664	681	rBV	209019	627245	39.88%	5.517%
24	5.294	689	690	694	rVB3	389	459	0.03%	0.004%
25	5.458	710	717	725	rVB3	1112	2859	0.18%	0.025%
26	5.562	726	734	737	rBV5	891	2218	0.14%	0.020%
27	5.623	739	744	752	rVB3	1507	3615	0.23%	0.032%
28	5.909	787	791	794	rBV2	178	239	0.02%	0.002%
29	6.037	798	812	829	rBV2	534436	1572832	100.00%	13.834%
30	6.147	829	830	837	rVB6	939	1614	0.10%	0.014%
31	6.531	887	893	894	rBV3	374	567	0.04%	0.005%
32	6.592	901	903	908	rBV2	298	515	0.03%	0.005%
33	6.690	916	919	920	rVB	259	211	0.01%	0.002%
34	6.708	920	922	925	rBV	200	212	0.01%	0.002%
35	6.824	931	941	954	rBV	382349	889674	56.57%	7.825%
36	7.171	990	998	1009	rVB2	9546	22211	1.41%	0.195%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010821\
 Data File : VX020534.D
 Acq On : 08 Jan 2021 10:28
 Operator : JC/MD
 Sample : VX0108MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK403

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML010721WMA.M
 Title : VOC Analysis

37	7.287	1014	1017	1020	rVB2	233	291	0.02%	0.003%
38	7.366	1020	1030	1046	rBV	325852	707334	44.97%	6.222%
39	7.470	1046	1047	1052	rVB4	367	315	0.02%	0.003%
40	7.531	1052	1057	1060	rBV6	783	1276	0.08%	0.011%
41	7.677	1078	1081	1083	rBV2	170	225	0.01%	0.002%
42	7.909	1116	1119	1123	rBV2	170	254	0.02%	0.002%
43	7.970	1125	1129	1135	rVB5	1050	1930	0.12%	0.017%
44	8.366	1187	1194	1208	rBV	205165	343047	21.81%	3.017%
45	8.507	1213	1217	1223	rVB4	844	1766	0.11%	0.016%
46	8.561	1225	1226	1229	rVB3	307	268	0.02%	0.002%
47	8.616	1231	1235	1237	rBV2	289	421	0.03%	0.004%
48	8.689	1240	1247	1262	rBV	781075	1245012	79.16%	10.951%
49	8.854	1273	1274	1279	rVV3	210	249	0.02%	0.002%
50	8.988	1290	1296	1308	rVV	144298	215760	13.72%	1.898%
51	9.134	1318	1320	1322	rBV3	285	258	0.02%	0.002%
52	9.311	1347	1349	1355	rVB4	778	1030	0.07%	0.009%
53	9.360	1355	1357	1361	rBV3	267	336	0.02%	0.003%
54	9.421	1361	1367	1383	rBV	464815	683796	43.48%	6.015%
55	9.622	1397	1400	1401	rBV3	280	297	0.02%	0.003%
56	9.738	1414	1419	1427	rVB4	1883	3114	0.20%	0.027%
57	9.829	1431	1434	1435	rBV	250	236	0.02%	0.002%
58	10.092	1471	1477	1491	rBV	759566	1017096	64.67%	8.946%
59	10.226	1496	1499	1505	rVB4	550	790	0.05%	0.007%
60	10.311	1511	1513	1515	rBV2	290	233	0.01%	0.002%
61	10.342	1515	1518	1522	rVB2	612	845	0.05%	0.007%
62	10.390	1522	1526	1528	rBV2	169	229	0.01%	0.002%
63	10.451	1533	1536	1537	rBV2	204	245	0.02%	0.002%
64	10.518	1544	1547	1550	rBV2	263	249	0.02%	0.002%
65	10.689	1570	1575	1579	rBV4	697	1224	0.08%	0.011%
66	10.750	1584	1585	1588	rBV2	174	213	0.01%	0.002%
67	11.000	1622	1626	1629	rBV	568	653	0.04%	0.006%
68	11.043	1629	1633	1635	rVB2	269	294	0.02%	0.003%
69	11.122	1643	1646	1649	rBV3	757	728	0.05%	0.006%
70	11.232	1658	1664	1671	rBV	572488	743096	47.25%	6.536%
71	11.494	1704	1707	1708	rBV	471	455	0.03%	0.004%
72	11.597	1721	1724	1725	rBV2	240	251	0.02%	0.002%
73	11.658	1731	1734	1736	rBV	265	297	0.02%	0.003%
74	11.750	1744	1749	1751	rBV3	710	1147	0.07%	0.010%
75	11.793	1754	1756	1760	rVB2	596	642	0.04%	0.006%
76	12.006	1786	1791	1794	rBV2	1007	1429	0.09%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010821\
 Data File : VX020534.D
 Acq On : 08 Jan 2021 10:28
 Operator : JC/MD
 Sample : VX0108MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK403

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML010721WMA.M

Title : VOC Analysis

77	12.061	1794	1800	1809	rBV	757480	916911	58.30%	8.065%
78	12.177	1817	1819	1820	rVB2	436	263	0.02%	0.002%
79	12.268	1830	1834	1836	rBV2	357	510	0.03%	0.004%
80	12.359	1843	1849	1857	rBV	799310	992480	63.10%	8.730%
81	12.725	1908	1909	1912	rBV	352	336	0.02%	0.003%
82	12.805	1916	1922	1926	rBV3	542	1187	0.08%	0.010%
83	13.024	1956	1958	1960	rBV	337	338	0.02%	0.003%
84	13.152	1976	1979	1984	rVV2	1591	1933	0.12%	0.017%
85	13.207	1984	1988	1990	rVB3	341	416	0.03%	0.004%
86	13.317	2004	2006	2011	rVB2	210	263	0.02%	0.002%
87	13.378	2014	2016	2018	rBV	348	378	0.02%	0.003%
88	13.463	2029	2030	2032	rBV	444	237	0.02%	0.002%
89	13.487	2032	2034	2035	rVB2	336	210	0.01%	0.002%
90	13.518	2035	2039	2040	rBV	294	415	0.03%	0.004%
91	13.628	2052	2057	2062	rVB4	1778	2498	0.16%	0.022%
92	13.707	2068	2070	2073	rBV3	205	308	0.02%	0.003%
93	13.817	2085	2088	2091	rBV2	1055	1130	0.07%	0.010%
94	13.859	2093	2095	2098	rBV2	307	447	0.03%	0.004%
95	13.999	2115	2118	2123	rVB3	1718	2433	0.15%	0.021%
96	14.158	2142	2144	2145	rBV2	399	251	0.02%	0.002%
97	14.341	2172	2174	2178	rBV3	300	535	0.03%	0.005%
98	14.835	2252	2255	2257	rBV3	403	534	0.03%	0.005%
99	14.938	2270	2272	2273	rBV	409	370	0.02%	0.003%
100	16.176	2473	2475	2478	rBV3	628	620	0.04%	0.005%

Sum of corrected areas: 11369021




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010821\
Data File : VX020534.D
Acq On : 08 Jan 2021 10:28
Operator : JC/MD
Sample : VX0108MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK403

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML010721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L

TIC Integration Parameters: LSCINT.P

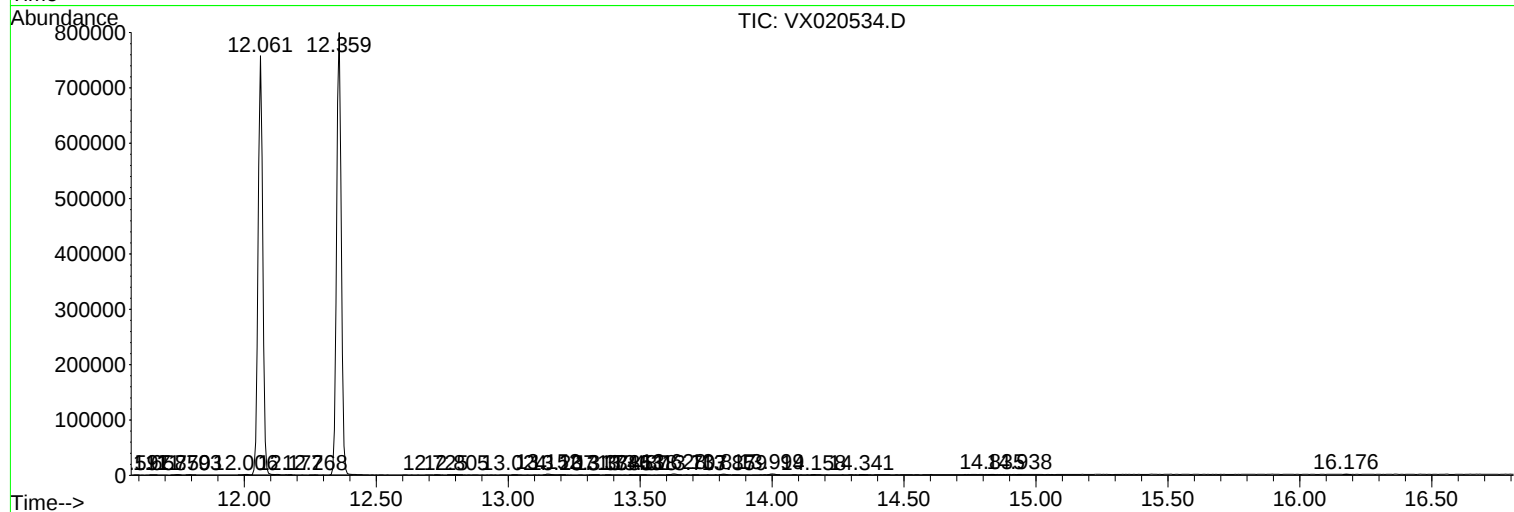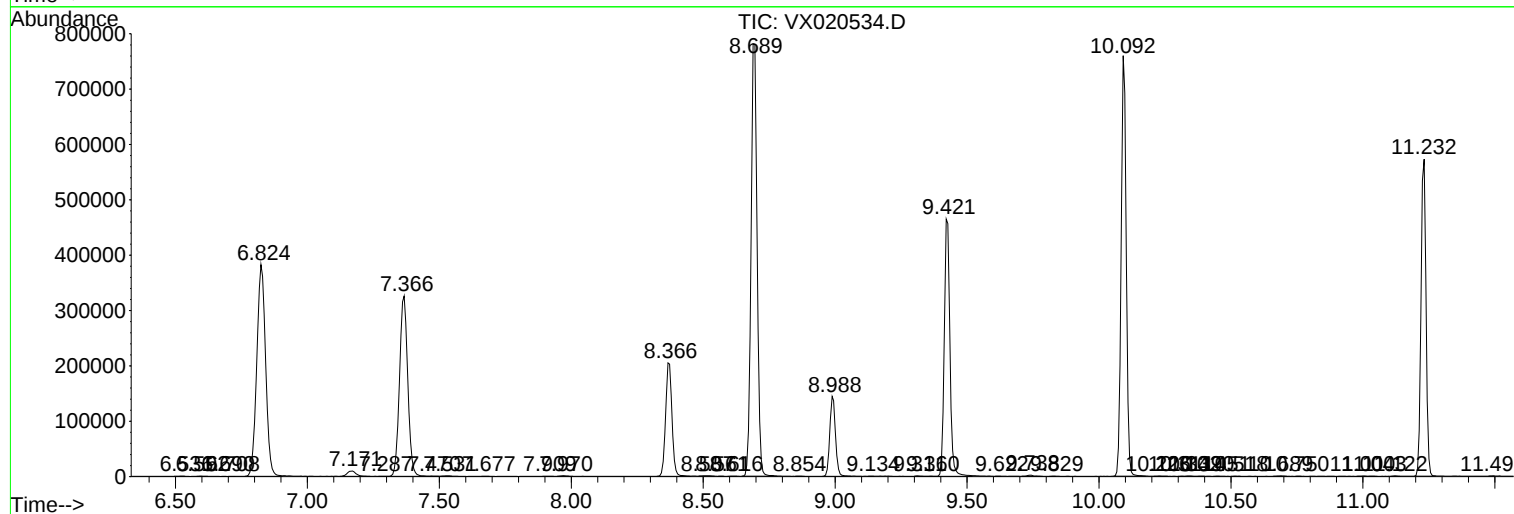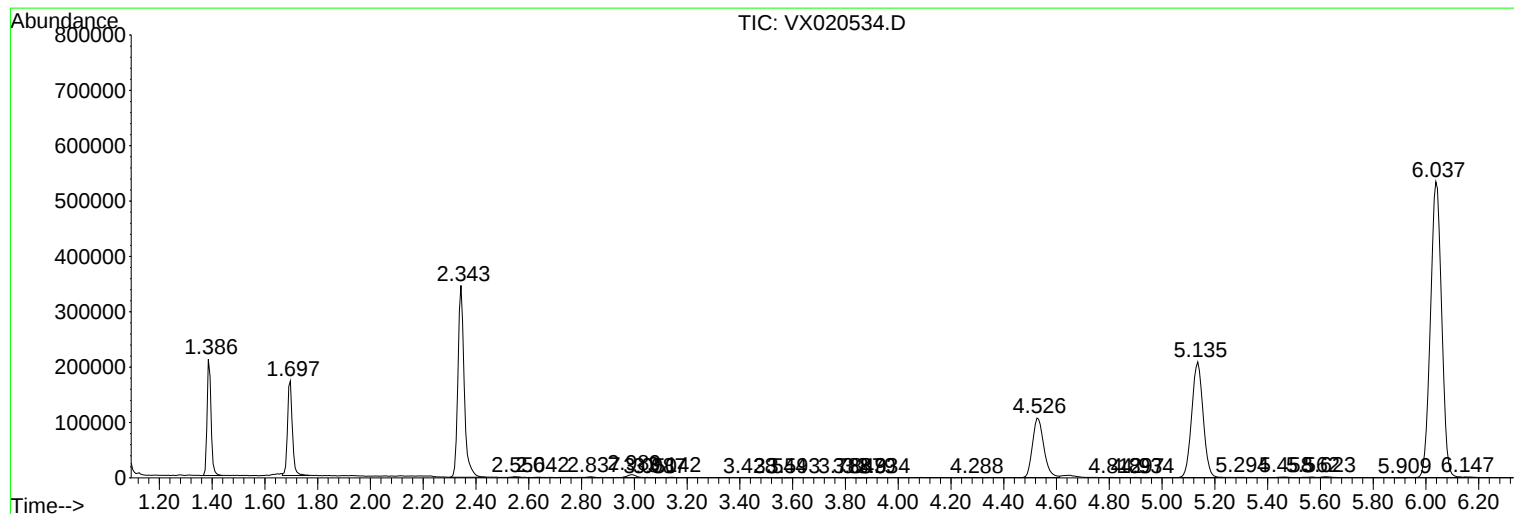

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010821\
Data File : VX020534.D
Acq On : 08 Jan 2021 10:28
Operator : JC/MD
Sample : VX0108MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK403

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML010721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010821\
Data File : VX020534.D
Acq On : 08 Jan 2021 10:28
Operator : JC/MD
Sample : VX0108MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK403

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXML010721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
