
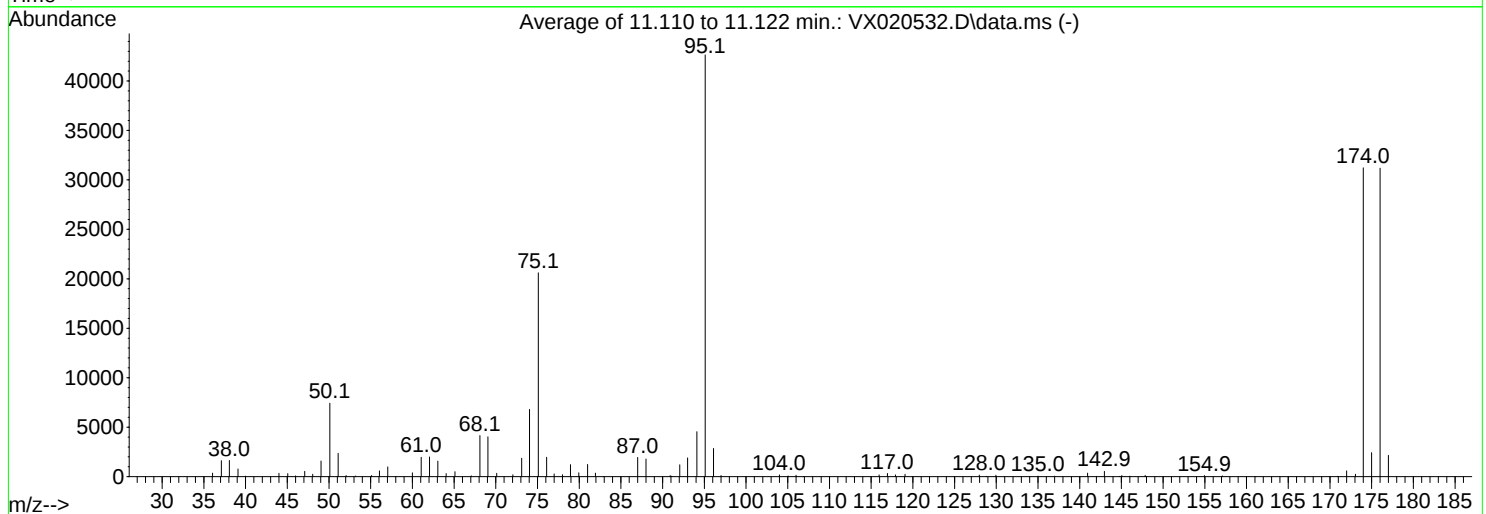


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010821\
Data File : VX020532.D
Acq On : 08 Jan 2021 09:22
Operator : JC/MD
Sample : BFB65
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB651

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM010721WMA.M
Title : VOC Analysis
Last Update : Fri Jan 15 16:52:29 2021

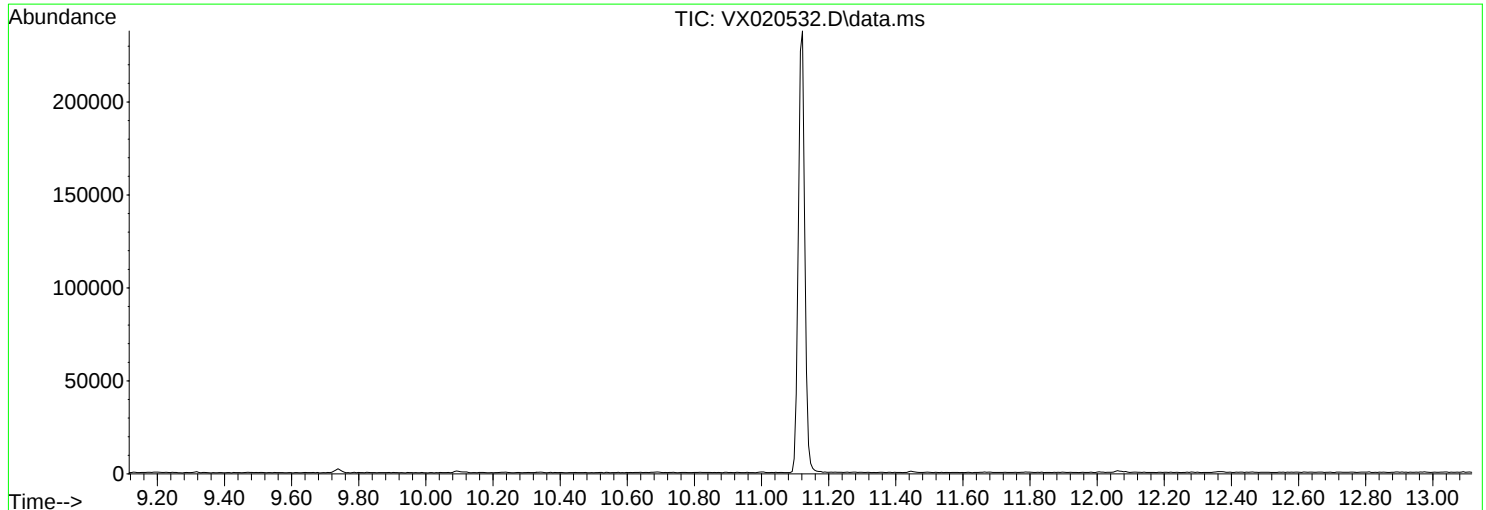

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1639

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.4	7431	PASS
75	95	30	80	48.3	20609	PASS
95	95	100	100	100.0	42643	PASS
96	95	5	9	6.7	2846	PASS
173	174	0.00	2	0.8	240	PASS
174	95	50	120	73.2	31216	PASS
175	174	5	9	7.8	2430	PASS
176	174	95	101	99.9	31187	PASS
177	176	5	9	6.9	2146	PASS

m/z	Abundance
36.00	361.0
37.10	1735.0
38.00	1671.0
39.10	908.0
40.00	244.0
44.00	862.0
45.00	332.0
46.00	65.0
47.10	575.0
48.00	267.0
49.00	1751.0
50.10	7806.0
51.10	2503.0
52.10	109.0
53.20	99.0
55.00	133.0
56.00	654.0
57.10	1182.0
60.00	380.0
61.00	2087.0
62.10	2186.0
63.10	1830.0
64.00	315.0
65.10	646.0
67.10	121.0
68.10	4578.0
69.10	4526.0
70.10	449.0
72.10	231.0
73.10	2202.0
74.10	7684.0
75.10	22704.0
76.10	1916.0
76.90	327.0
77.90	277.0
78.90	1398.0
79.90	420.0
81.00	1379.0
82.00	431.0
87.00	2251.0
88.00	2177.0
90.90	234.0
92.10	1340.0
93.00	2266.0
94.10	5396.0
95.10	48712.0
96.10	3134.0
97.00	118.0
103.90	236.0
105.00	70.0
106.10	172.0
115.90	188.0
117.00	394.0
117.90	197.0
119.10	233.0
128.00	196.0
128.80	99.0
129.90	190.0
135.00	85.0
137.00	82.0
141.00	425.0
142.00	53.0
142.90	681.0
145.10	199.0
146.00	72.0
147.80	135.0
155.00	187.0
157.10	123.0
161.10	55.0
170.90	105.0
172.10	792.0
173.00	364.0
174.00	42552.0
175.00	3106.0
176.00	41344.0
177.00	2848.0

Instrument :
MSVOA_X
ClientSampleId :
BFB651

Scan 1639 (11.079 min): VX020532.D\data.ms
BFB65

m/z	Abundance
40.00	185.0
44.00	421.0
207.20	54.0

Instrument :
MSVOA_X
ClientSampleId :
BFB651

m/z	Abundance
36.10	483.0
37.10	1933.0
38.10	1960.0
39.10	836.0
40.00	241.0
44.00	717.0
45.10	362.0
46.00	55.0
47.10	635.0
48.10	307.0
49.10	1789.0
50.10	8840.0
51.10	2795.0
52.00	145.0
53.20	65.0
55.10	139.0
56.10	707.0
57.00	1069.0
58.00	63.0
60.00	481.0
61.00	2383.0
62.00	2428.0
63.00	1839.0
64.10	356.0
65.10	509.0
67.00	101.0
68.10	4997.0
69.10	4685.0
70.10	339.0
72.00	231.0
73.10	2107.0
74.10	7830.0
75.10	24336.0
76.10	2506.0
77.10	266.0
78.00	196.0
79.00	1364.0
80.00	480.0
81.00	1454.0
82.00	368.0
82.90	63.0
87.00	2243.0
88.00	1970.0
91.10	153.0
92.00	1419.0
93.00	2130.0
94.10	5188.0
95.10	50184.0
96.10	3325.0
97.00	115.0
104.00	221.0
105.00	62.0
106.00	202.0
106.90	53.0
116.00	243.0
116.90	336.0
117.90	170.0
119.00	303.0
127.90	171.0
130.00	152.0
135.00	79.0
141.00	393.0
142.00	62.0
142.90	598.0
145.00	161.0
146.00	62.0
147.90	164.0
154.90	111.0
157.10	101.0
171.90	654.0
173.10	357.0
174.00	33792.0
175.00	2641.0
176.00	34760.0
177.00	2279.0

Instrument :
MSVOA_X
ClientSampleId :
BFB651

m/z	Abundance
36.00	206.0
37.10	1165.0
38.10	1267.0
39.10	590.0
40.00	241.0
44.10	726.0
45.00	227.0
46.00	107.0
47.10	375.0
48.00	165.0
49.00	1194.0
50.10	5647.0
51.10	1784.0
52.00	91.0
53.20	52.0
55.20	67.0
56.10	377.0
57.00	722.0
60.00	330.0
61.10	1398.0
62.10	1376.0
63.10	1033.0
64.10	274.0
65.10	349.0
68.10	2914.0
69.00	2859.0
70.10	253.0
72.00	128.0
73.10	1258.0
74.00	4882.0
75.10	14787.0
76.10	1446.0
77.10	228.0
78.10	109.0
78.90	885.0
80.00	261.0
81.00	875.0
81.90	270.0
87.00	1324.0
88.00	1212.0
90.90	116.0
92.10	823.0
93.00	1308.0
94.10	3034.0
95.10	29032.0
96.10	2080.0
97.00	106.0
104.20	82.0
105.10	67.0
105.90	84.0
115.90	131.0
117.00	237.0
117.90	155.0
119.00	193.0
128.00	103.0
130.00	105.0
137.00	50.0
140.90	274.0
143.00	340.0
144.80	101.0
147.80	97.0
154.80	54.0
172.10	325.0
174.00	17304.0
175.00	1544.0
176.00	17456.0
177.00	1311.0

Instrument :
MSVOA_X
ClientSampleId :
BFB651