



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010824\
Data File : VX039663.D
Acq On : 08 Jan 2024 15:54
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X010824W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue Jan 09 06:15:26 2024

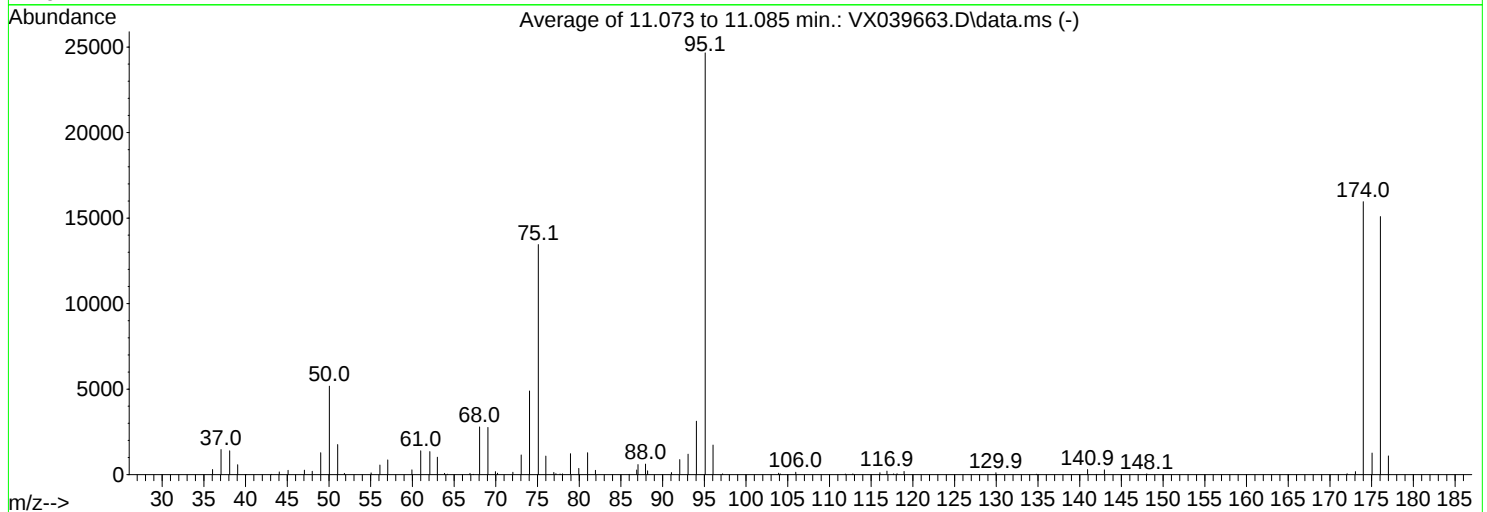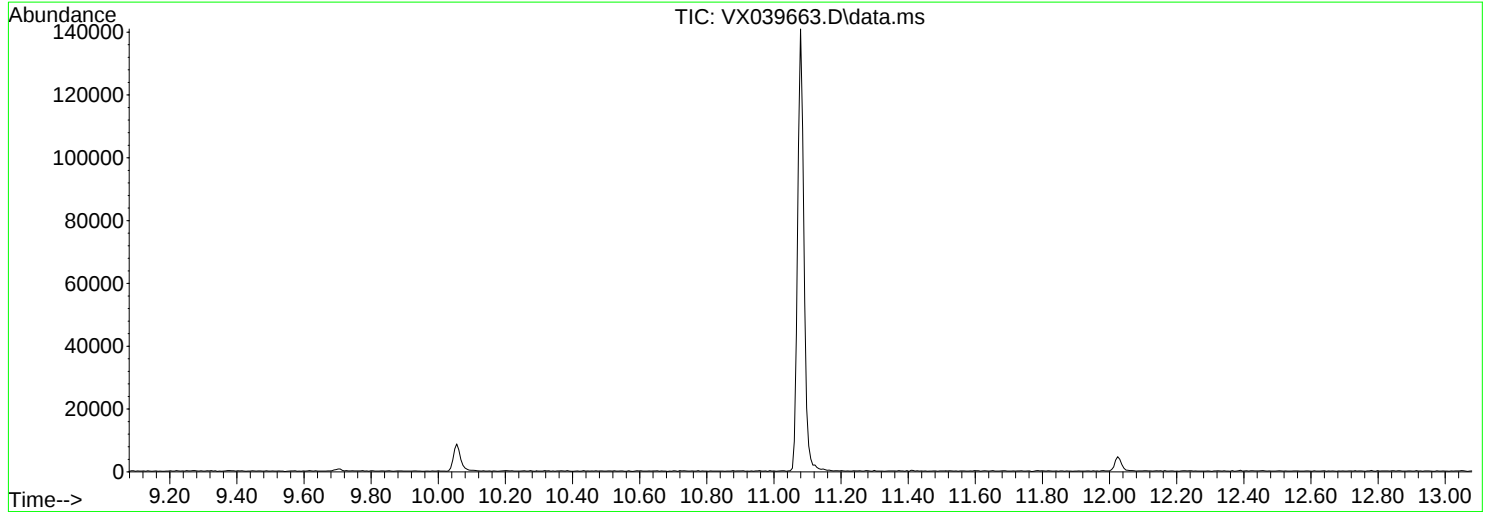

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.0	5177	PASS
75	95	30	60	54.5	13449	PASS
95	95	100	100	100.0	24661	PASS
96	95	5	9	7.0	1732	PASS
173	174	0.00	2	1.1	176	PASS
174	95	50	100	64.7	15964	PASS
175	174	5	9	7.9	1267	PASS
176	174	95	101	94.6	15094	FAIL*
177	176	5	9	7.3	1098	PASS