

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX010920\
 Data File : VX014495.D
 Acq On : 09 Jan 2020 13:39
 Operator : JC/SP
 Sample : L1041-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WGGM-20-WW-TSF-002

Quant Time: Jan 09 15:29:14 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X121219W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Dec 13 01:35:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.01	128	78474	30.00	ug/l	0.01
28) 1,4-Difluorobenzene	6.85	114	436200	30.00	ug/l	0.00
57) Chlorobenzene-d5	10.11	117	394264	30.00	ug/l	0.00

System Monitoring Compounds

27) 1,2-Dichloroethane-d4	6.05	65	168029	29.90	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	99.67%
60) 4-Bromofluorobenzene	11.14	95	179372	28.17	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	93.90%
63) Toluene-d8	8.71	98	526240	29.86	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	99.53%


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX010920\
Data File : VX014495.D
Acq On : 09 Jan 2020 13:39
Operator : JC/SP
Sample : L1041-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WGGM-20-WW-TSF-002

Quant Time: Jan 09 15:29:14 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X121219W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Dec 13 01:35:34 2019
Response via : Initial Calibration

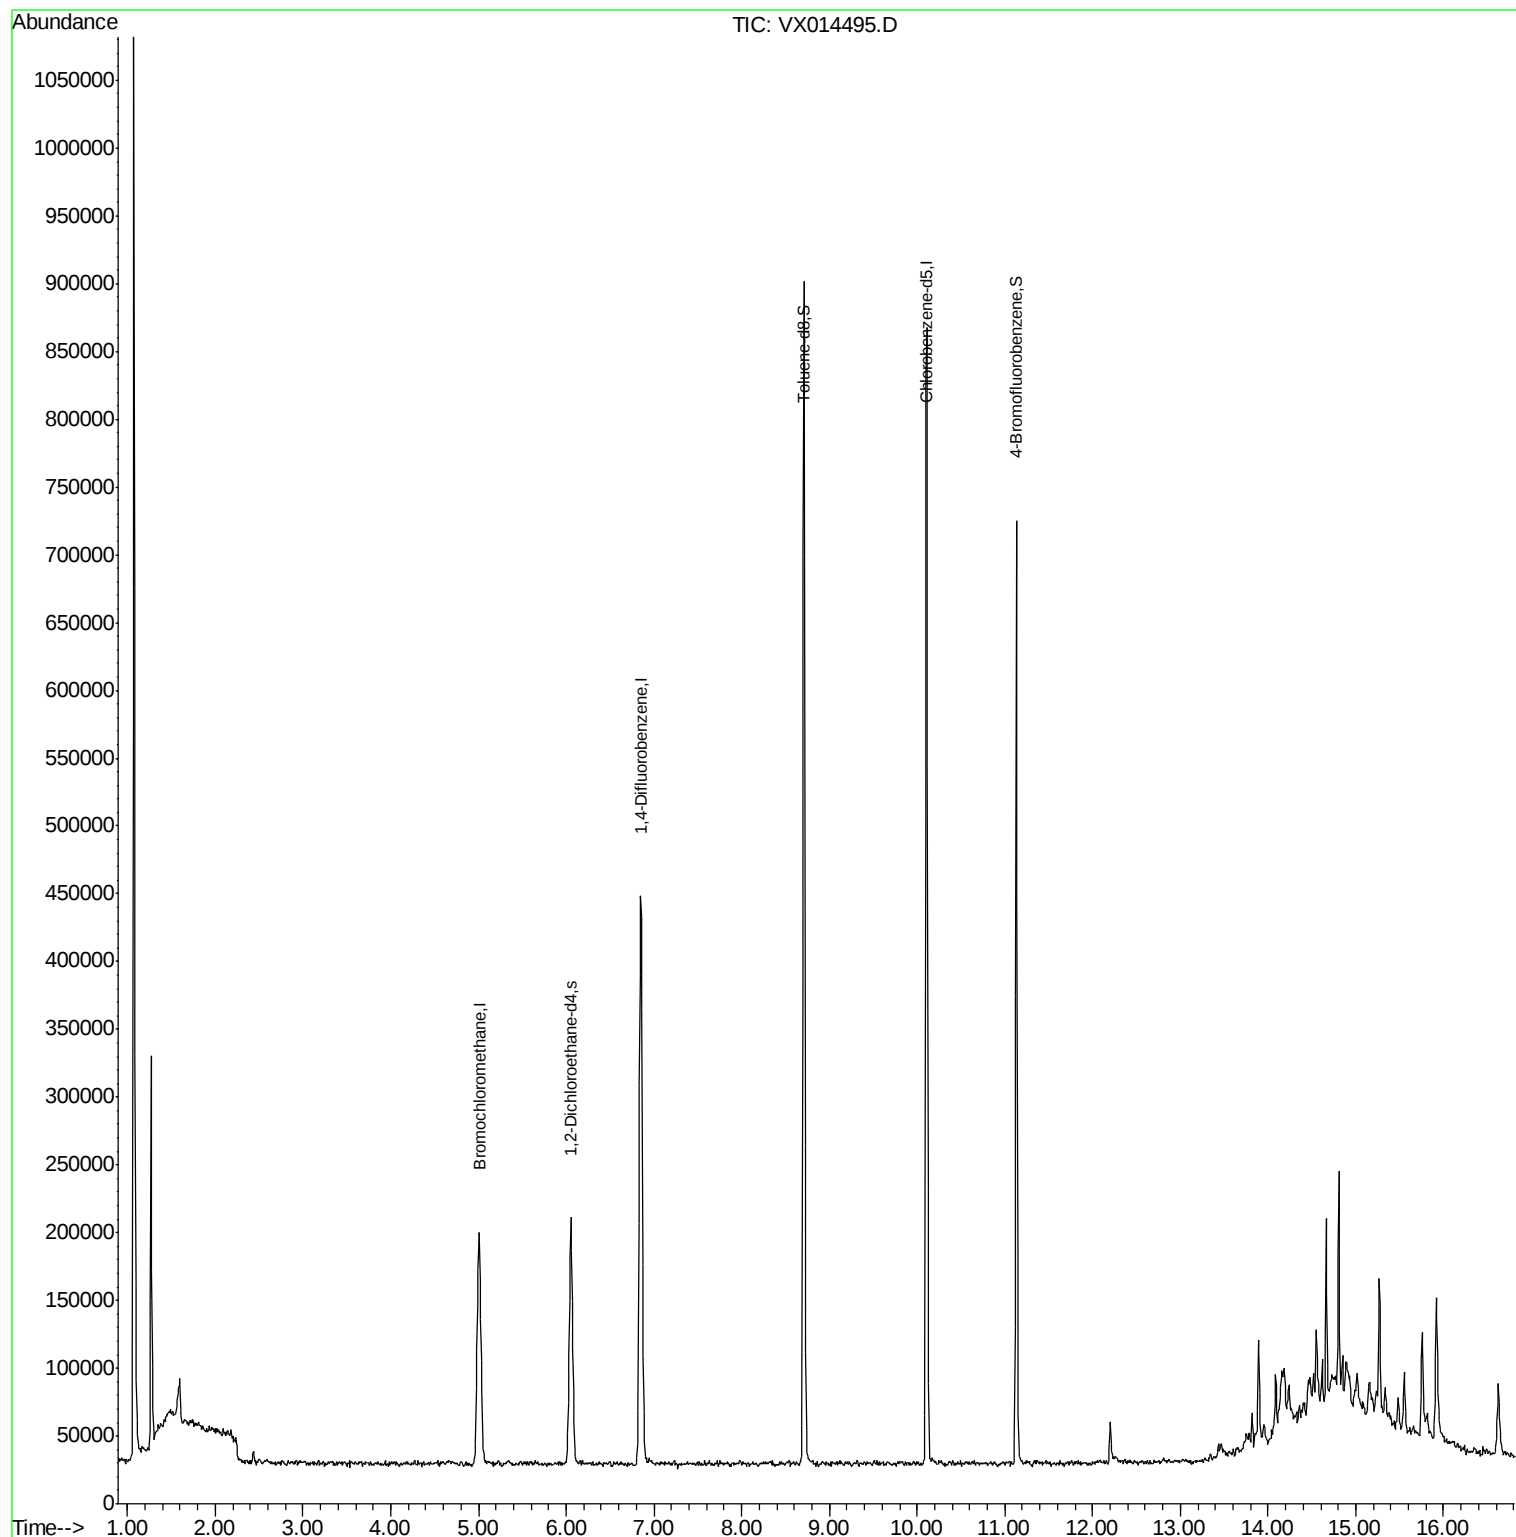

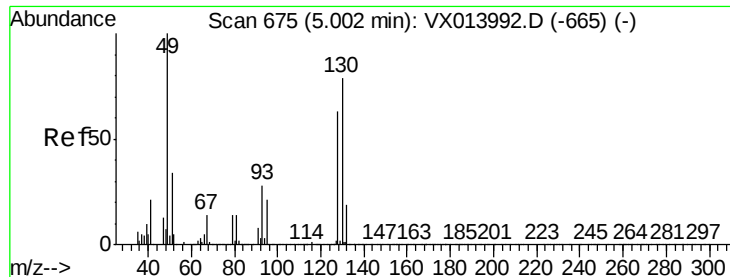

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 5.01 min Scan# 677

Delta R.T. 0.01 min

Lab File: VX014495.D

Acq: 09 Jan 2020 13:39

Instrument :

MSVOA_X

ClientSampleId :

WGGM-20-WW-TSF-002


Tot Ion:128 Resp: 78474

Ion Ratio Lower Upper

128 100

49 158.6 0.0 405.0




130 131.1 0.0 321.5

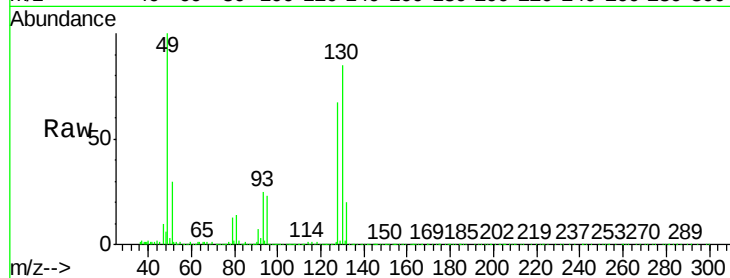

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VX0

Ion 130.00 (129.70 to 130.70): V

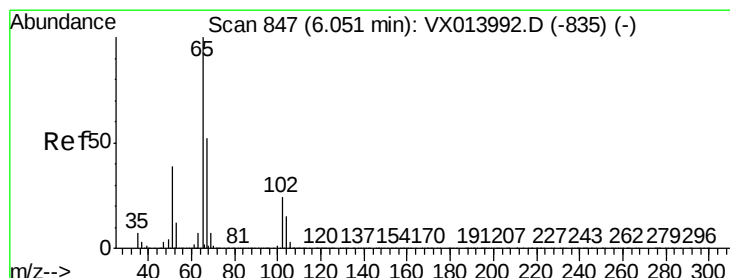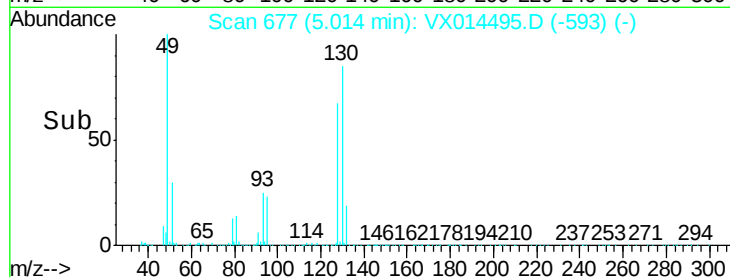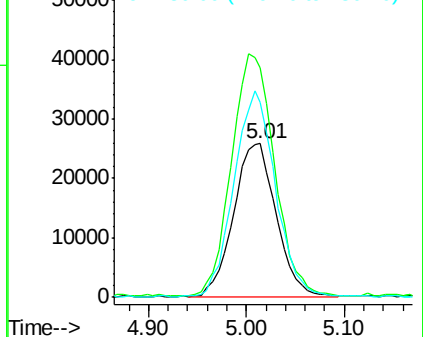

#27

1,2-Dichloroethane-d4

Concen: 29.898 ug/l

RT: 6.05 min Scan# 847

Delta R.T. -0.00 min

Lab File: VX014495.D


Acq: 09 Jan 2020 13:39

Tgt Ion: 65 Resp: 168029

Ion Ratio Lower Upper



65 100


67 52.9 43.1 64.7

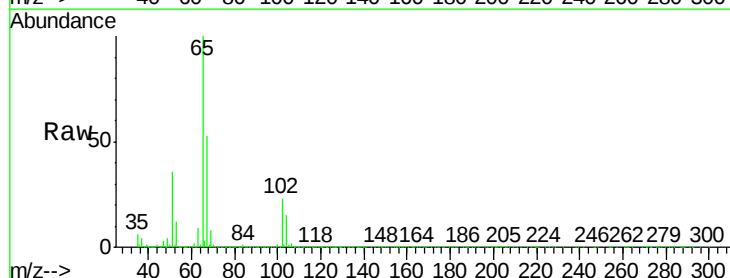

Abundance Ion 65.00 (64.70 to 65.70): VX0

Ion 67.00 (66.70 to 67.70): VX0

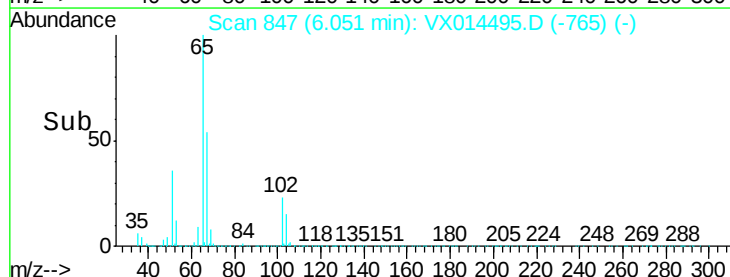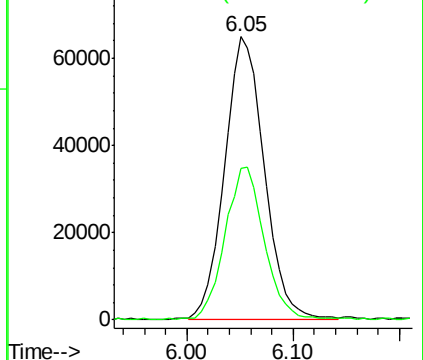

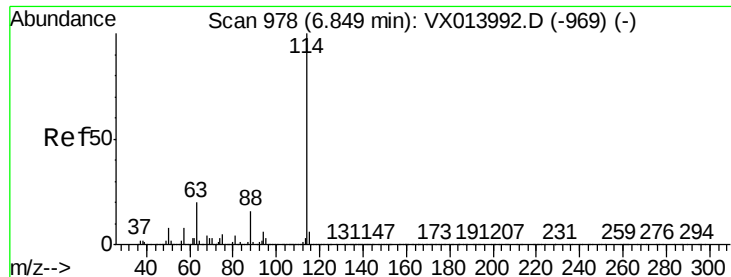

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 6.85 min Scan# 978

Delta R.T. -0.00 min

Lab File: VX014495.D

Acq: 09 Jan 2020 13:39

Instrument :

MSVOA_X

ClientSampleId :

WGGM-20-WW-TSF-002


Tot Ion:114 Resp: 436200

Ion Ratio Lower Upper

114 100

63 20.4 16.1 24.1




88 15.5 12.5 18.7

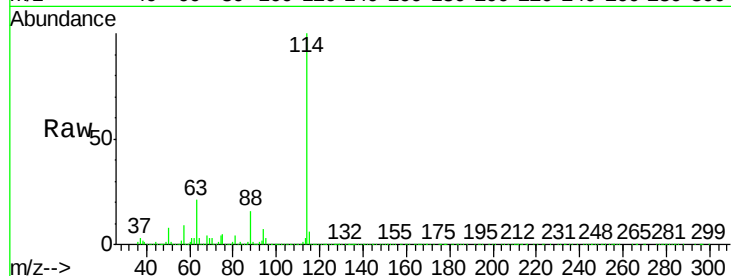

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 88.00 (87.70 to 88.70): VX0

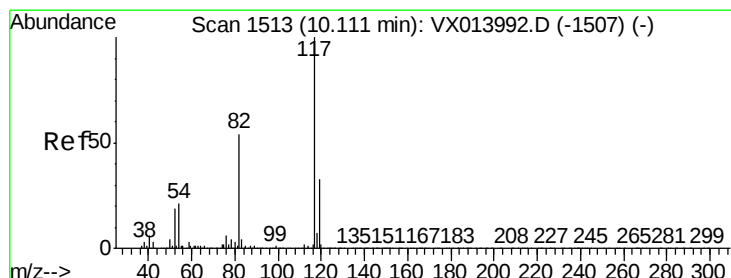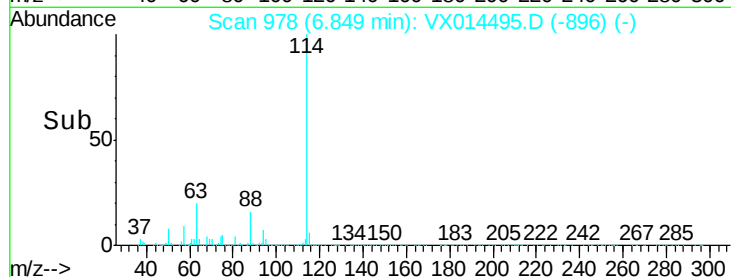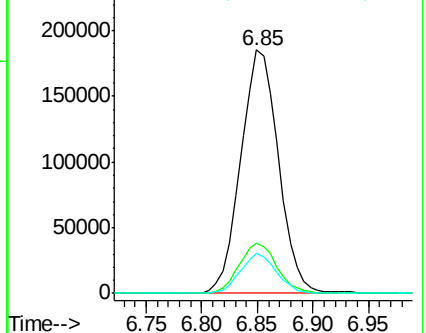

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 10.11 min Scan# 1513

Delta R.T. -0.00 min

Lab File: VX014495.D

Acq: 09 Jan 2020 13:39


Tgt Ion:117 Resp: 394264

Ion Ratio Lower Upper

117 100

82 53.9 43.8 65.6



119 32.1 25.8 38.6

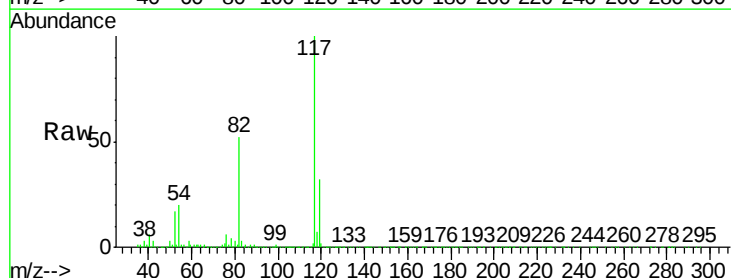


Abundance Ion 117.00 (116.70 to 117.70): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 119.00 (118.70 to 119.70): V



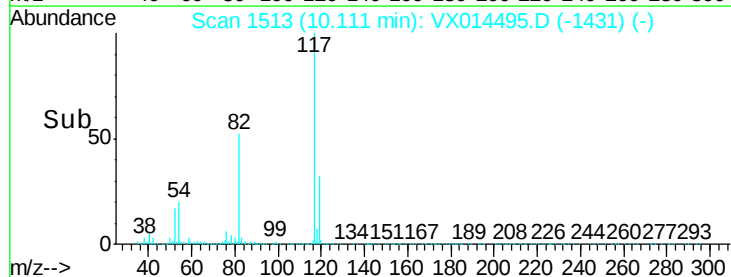
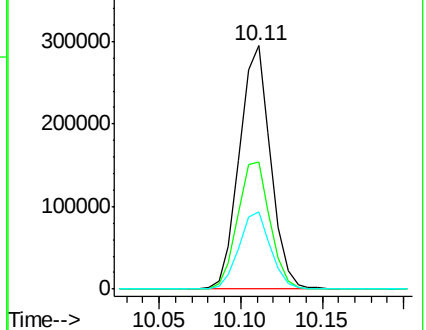


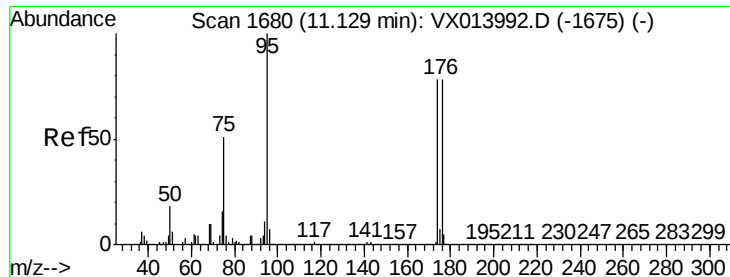

#60
4-Bromofluorobenzene
Concen: 28.174 ug/l
RT: 11.14 min Scan# 1681
Delta R.T. 0.01 min
Lab File: VX014495.D
Acq: 09 Jan 2020 13:39

Instrument :
MSVOA_X
ClientSampleId :
WGM-20-WW-TSF-002

Tot Ion	95	Resp	179372
Ion Ratio	Lower	Upper	
95	100		
174	90.3	70.2	105.2
176	89.3	68.3	102.5

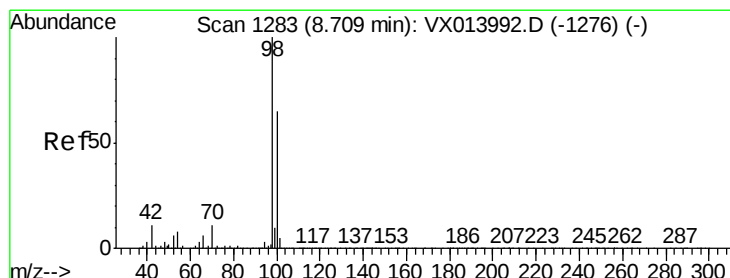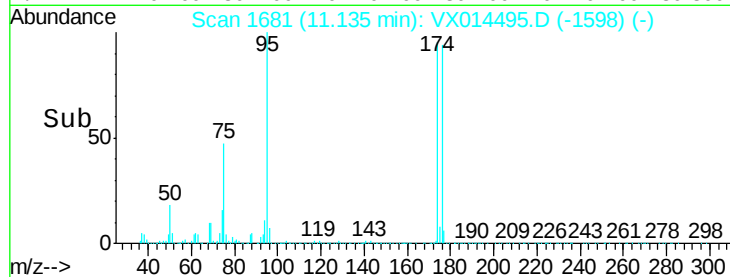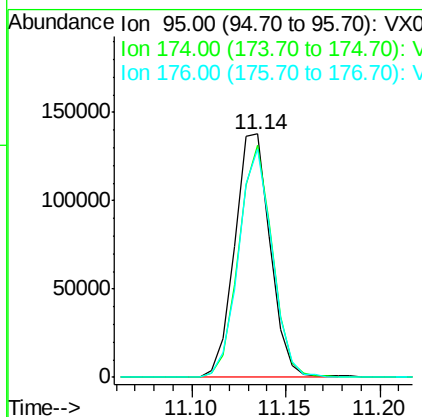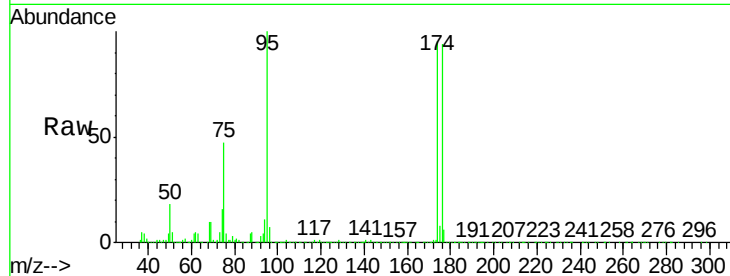

#63
Toluene-d8
Concen: 29.861 ug/l
RT: 8.71 min Scan# 1283
Delta R.T. -0.00 min
Lab File: VX014495.D
Acq: 09 Jan 2020 13:39

Tgt Ion	98	Resp	526240
Ion Ratio	Lower	Upper	
98	100		
100	65.1	52.2	78.2

