


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX010920\
 Data File : VX014486.D
 Acq On : 09 Jan 2020 09:23
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X121219W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Dec 13 01:35:34 2019

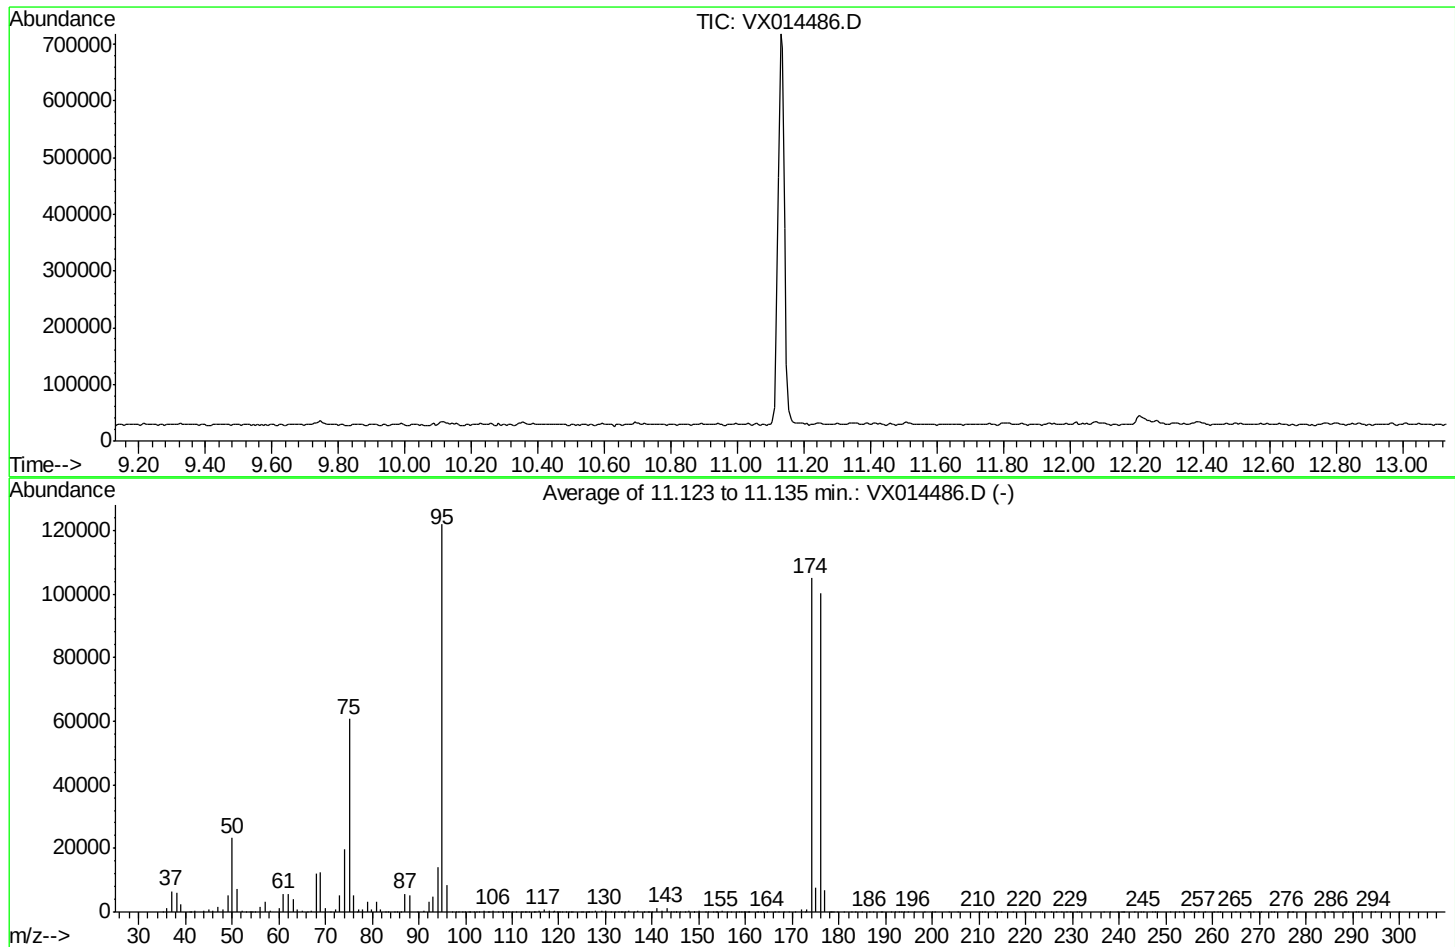

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1674

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	23202	PASS
75	95	30	60	49.8	60762	PASS
95	95	100	100	100.0	121901	PASS
96	95	5	9	6.8	8268	PASS
173	174	0.00	2	1.0	1007	PASS
174	95	50	100	86.1	104944	PASS
175	174	5	9	7.4	7766	PASS
176	174	95	101	95.5	100221	PASS
177	176	5	9	6.7	6736	PASS