


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010924\
Data File : VX039672.D
Acq On : 09 Jan 2024 10:03
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X010824W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue Jan 09 06:15:26 2024

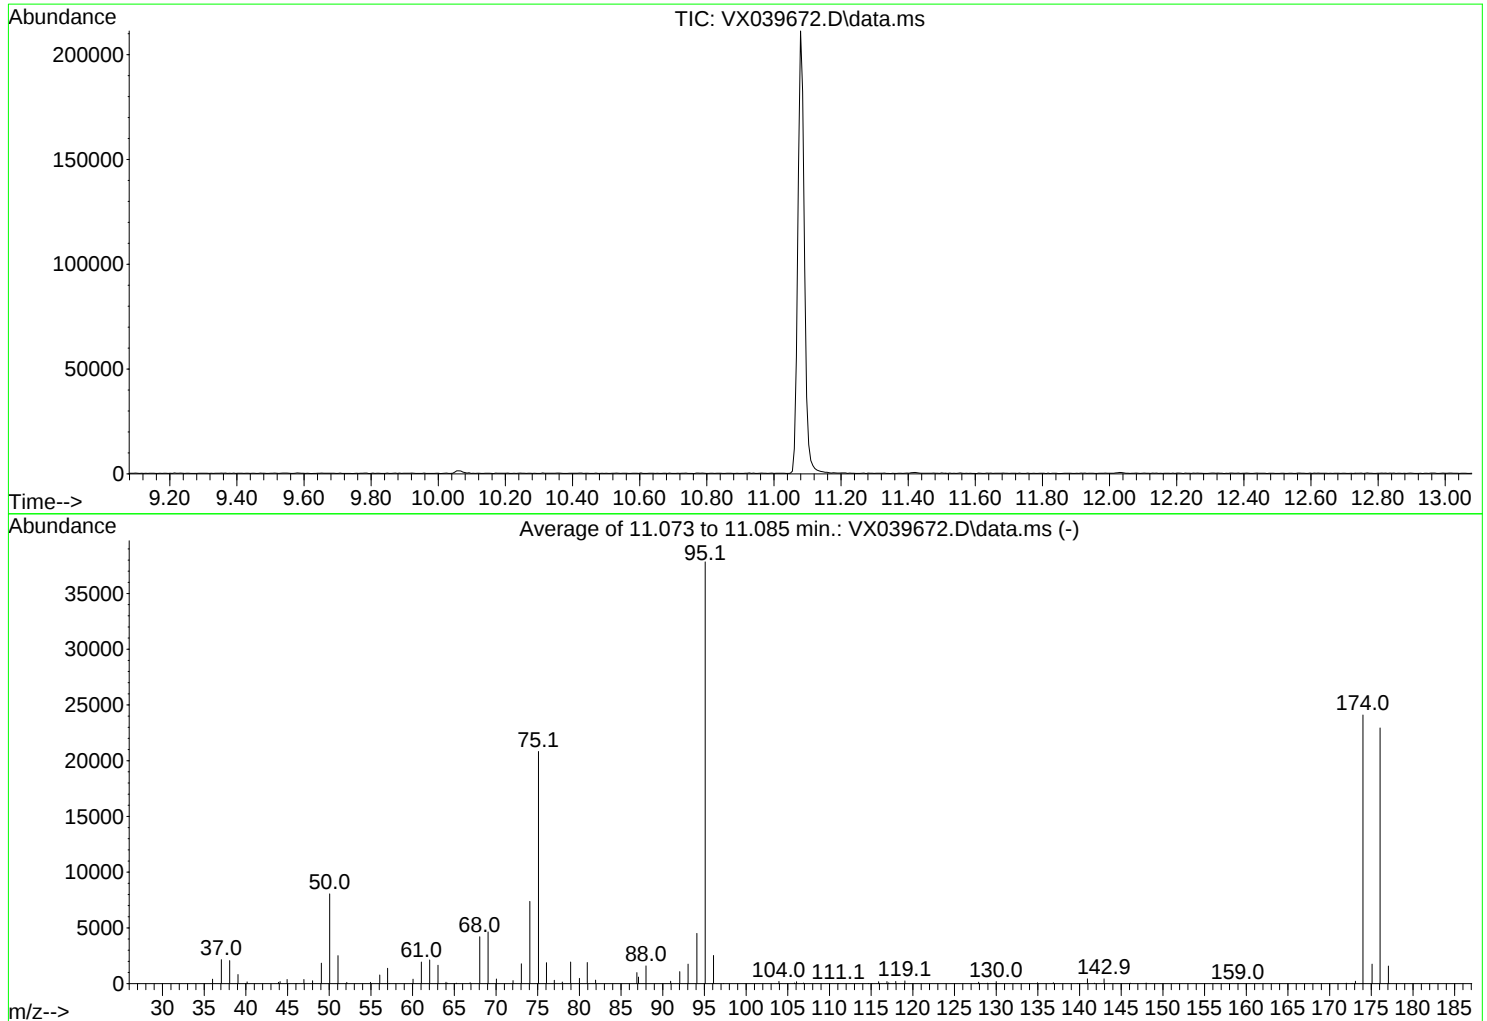

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	8049	PASS
75	95	30	60	55.0	20827	PASS
95	95	100	100	100.0	37843	PASS
96	95	5	9	6.7	2533	PASS
173	174	0.00	2	0.9	214	PASS
174	95	50	100	63.7	24107	PASS
175	174	5	9	7.3	1757	PASS
176	174	95	101	95.2	22941	PASS
177	176	5	9	6.9	1579	PASS