



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX010924\
Data File : VX039679.D
Acq On : 09 Jan 2024 14:54
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010924W.M
Title : SW846 8260
Last Update : Wed Jan 10 07:39:55 2024

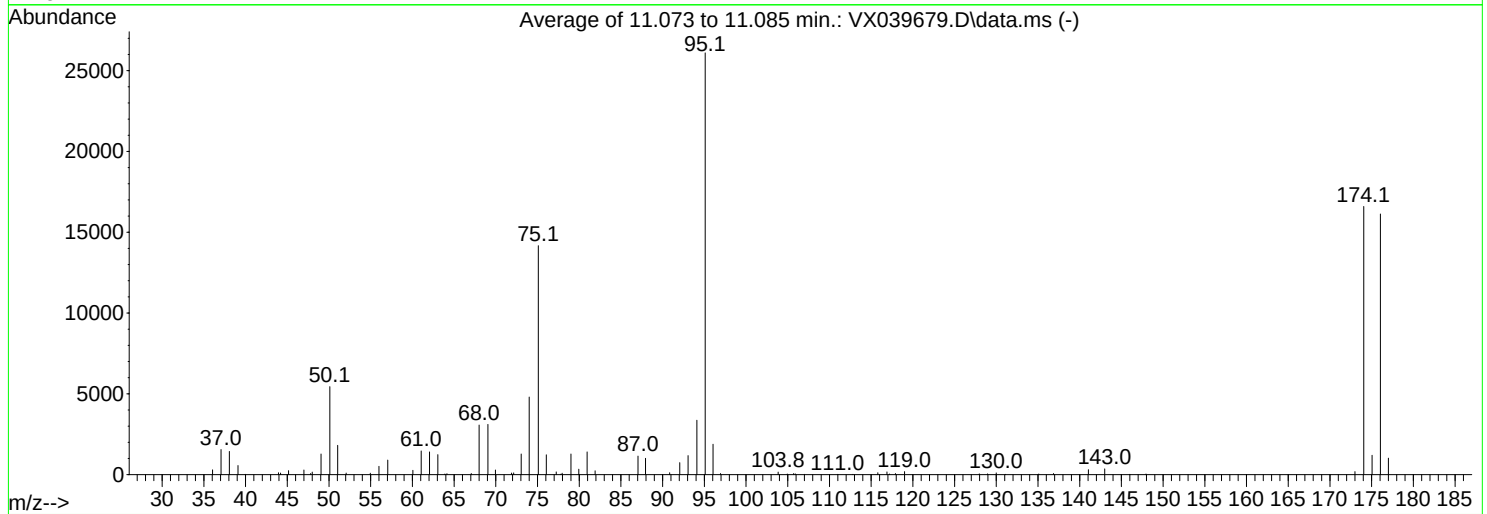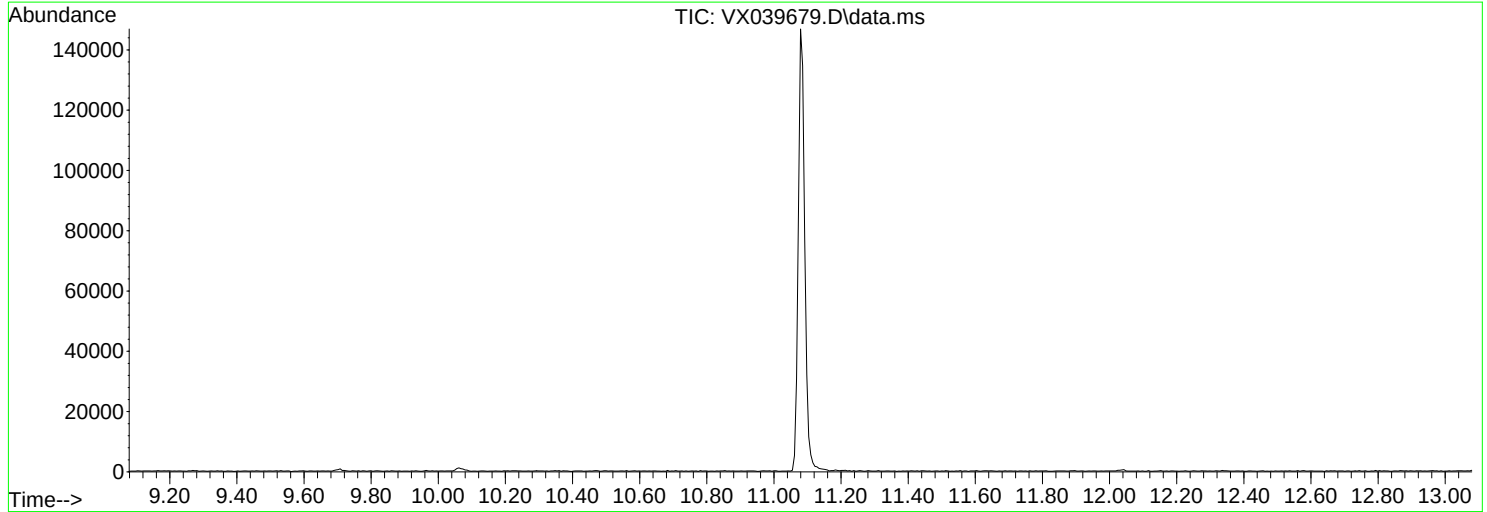

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	5444	PASS
75	95	30	60	54.3	14173	PASS
95	95	100	100	100.0	26101	PASS
96	95	5	9	7.2	1882	PASS
173	174	0.00	2	1.1	186	PASS
174	95	50	100	63.6	16591	PASS
175	174	5	9	7.2	1200	PASS
176	174	95	101	97.2	16133	PASS
177	176	5	9	6.3	1018	PASS