

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX011019\
 Data File : VX006995.D
 Acq On : 10 Jan 2019 17:34
 Operator : JC/MD
 Sample : K1099-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-18

Quant Time: Jan 11 07:14:35 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 08 14:06:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	612300	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	947218	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	900049	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	433171	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	323136	50.50	ug/l	0.00
Spiked Amount			Recovery	=	101.00%	
35) Dibromofluoromethane	5.51	113	284667	46.93	ug/l	0.00
Spiked Amount			Recovery	=	93.86%	
50) Toluene-d8	8.71	98	1145303	51.58	ug/l	0.00
Spiked Amount			Recovery	=	103.16%	
62) 4-Bromofluorobenzene	11.13	95	409961	52.96	ug/l	0.00
Spiked Amount			Recovery	=	105.92%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	3.07	59	2798	1.854	ug/l	95
13) Acrolein	2.28	56	335	3.592	ug/l #	81
14) Allyl chloride	2.86	41	81624	8.463	ug/l #	26
16) Acetone	2.45	43	25631	8.102	ug/l	99
18) Methyl Acetate	2.78	43	21602	2.358	ug/l	95
20) Methylene Chloride	2.86	84	2357064	395.648	ug/l	95
25) 2-Butanone	4.70	43	11766	2.599	ug/l #	82
29) Tetrahydrofuran	5.17	42	2804	0.953	ug/l	96
36) 1,1-Dichloropropene	5.67	75	39504	4.797	ug/l #	50
38) Carbon Tetrachloride	5.67	117	55519	6.701	ug/l #	15
43) Isopropyl Acetate	6.46	43	29701	2.133	ug/l	100
48) Methyl methacrylate	7.68	41	18824	2.632	ug/l #	12
49) 1,4-Dioxane	7.76	88	327	Below Cal	#	27
51) 4-Methyl-2-Pentanone	8.62	43	147527	16.483	ug/l #	49
54) cis-1,3-Dichloropropene	8.62	75	75845	8.196	ug/l #	62
57) 1,3-Dichloropropane	9.54	76	14882	1.405	ug/l #	43
59) 2-Hexanone	9.54	43	200253	29.361	ug/l #	52
65) Chlorobenzene	10.13	112	5033	0.256	ug/l	92
68) m/p-Xylenes	10.36	106	5617	0.440	ug/l	99
69) o-Xylene	10.69	106	3233	0.260	ug/l	81
71) Bromoform	11.01	173	136	4.748	ug/l #	28
76) 1,2,3-Trichloropropane	11.13	75	192113	21.886	ug/l #	40
81) trans-1,4-Dichloro-2-buten	11.13	75	192113	64.834	ug/l #	10
84) 1,2,4-Trimethylbenzene	11.80	105	11296	0.440	ug/l	93
88) 1,4-Dichlorobenzene	12.08	146	884	0.206	ug/l #	1
90) Hexachloroethane	12.58	117	566	3.031	ug/l #	6
95) Naphthalene	13.83	128	218578	7.004	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX011019\
Data File : VX006995.D
Acq On : 10 Jan 2019 17:34
Operator : JC/MD
Sample : K1099-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-18

Quant Time: Jan 11 07:14:35 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 08 14:06:59 2019
Response via : Initial Calibration

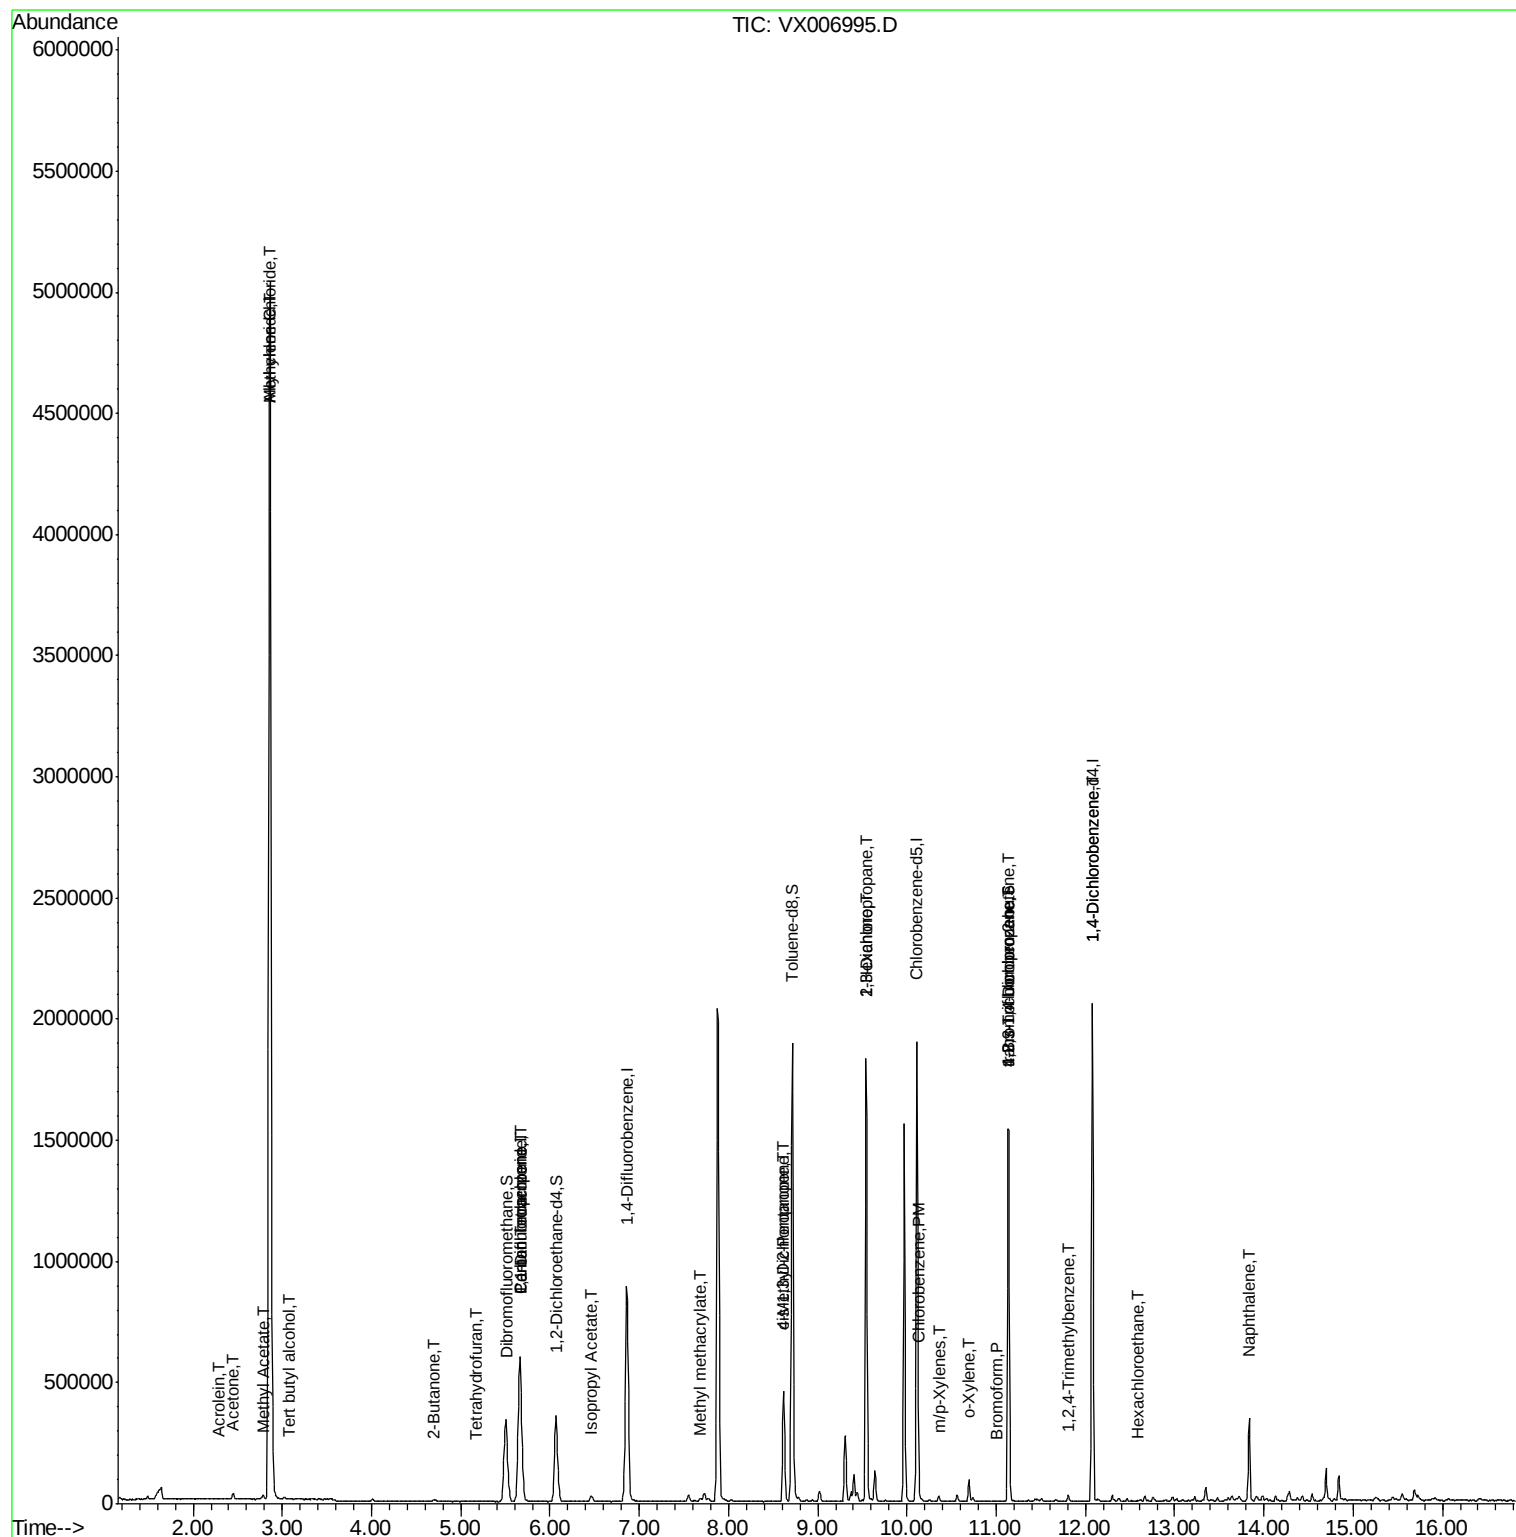

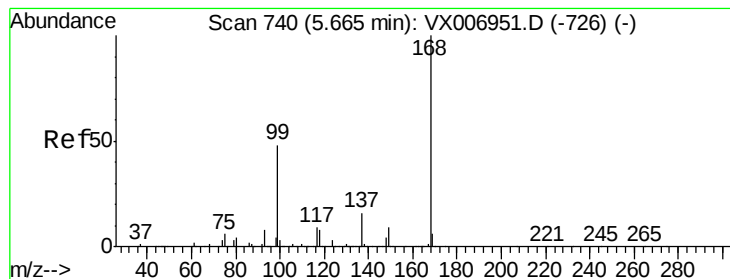

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.00 min

Lab File: VX006995.D

Acq: 10 Jan 2019 17:34

Instrument :

MSVOA_X

ClientSampleId :


TP-18

Tgt Ion:168 Resp: 612300

Ion Ratio Lower Upper

168 100

99 50.3 41.8 62.8



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

200000



150000

100000

50000

0

Time-->

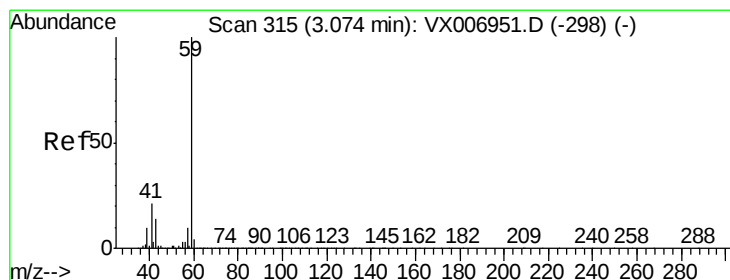

#11

Tert butyl alcohol

Concen: 1.854 ug/l

RT: 3.07 min Scan# 315

Delta R.T. -0.00 min

Lab File: VX006995.D


Acq: 10 Jan 2019 17:34

Tgt Ion: 59 Resp: 2798

Ion Ratio Lower Upper

59 100

57 12.3 8.5 12.7



Abundance Ion 59.00 (58.70 to 59.70): VX0

Ion 57.00 (56.70 to 57.70): VX0

3.07


1500


1000

500

0

Time-->



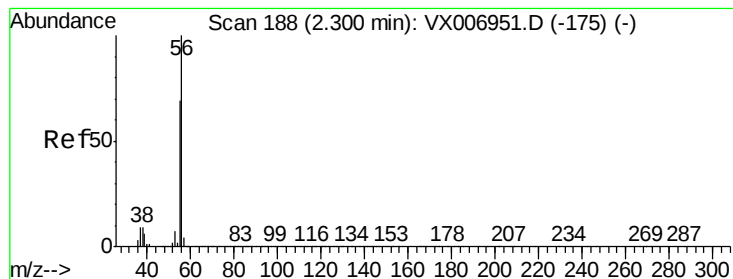

#13

Acrolein

Concen: 3.592 ug/l

RT: 2.28 min Scan# 185

Delta R.T. -0.02 min

Lab File: VX006995.D

Acq: 10 Jan 2019 17:34

Instrument :

MSVOA_X

ClientSampleId :





TP-18

Tgt Ion: 56 Resp: 335

Ion Ratio Lower Upper

56 100

55 57.0 58.2 87.4#

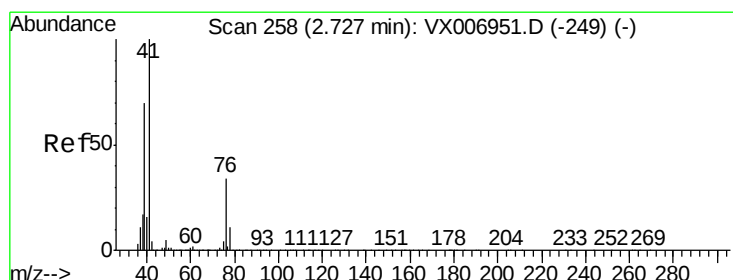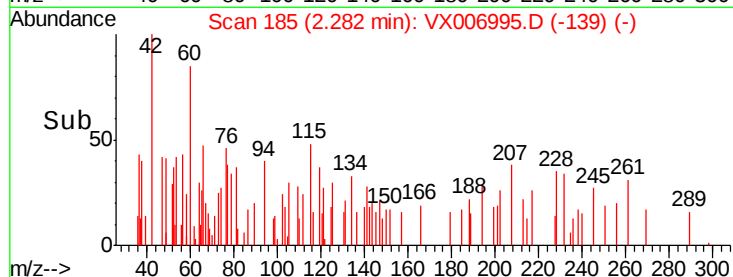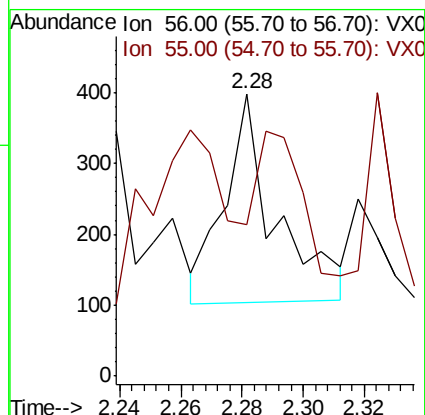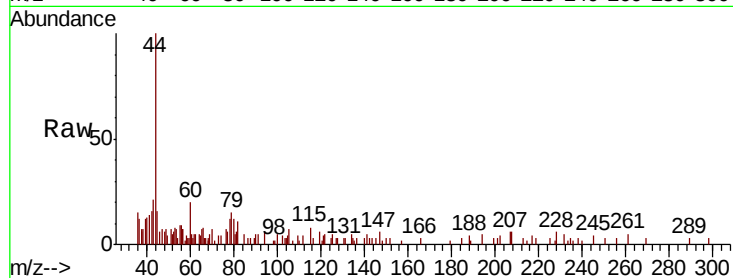

#14

Allyl chloride

Concen: 8.463 ug/l

RT: 2.86 min Scan# 280

Delta R.T. 0.13 min

Lab File: VX006995.D

Acq: 10 Jan 2019 17:34




Tgt Ion: 41 Resp: 81624


Ion Ratio Lower Upper

41 100

39 1.9 53.6 80.4#

76 0.0 27.4 41.2#


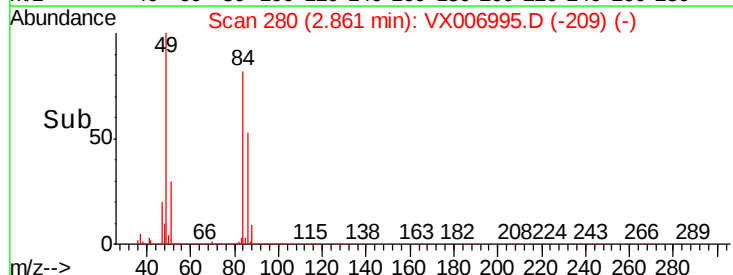
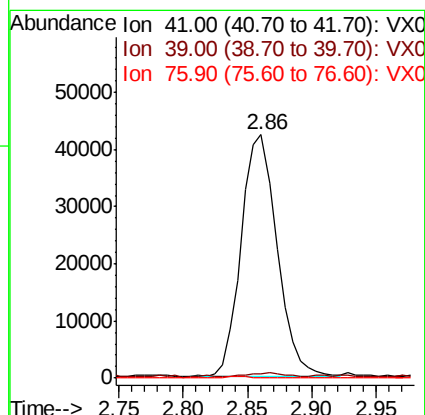
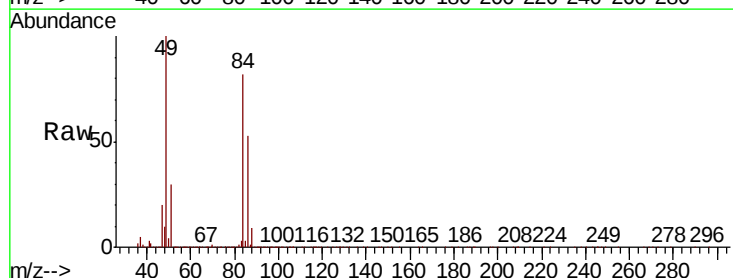


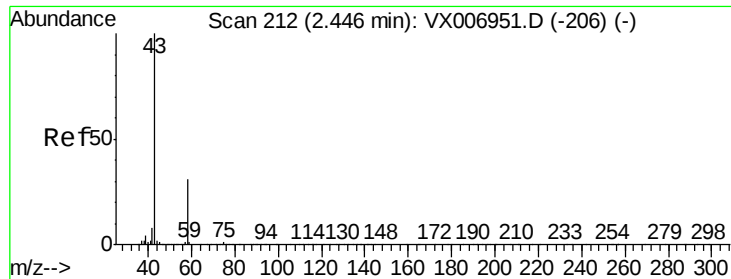

#16
Acetone
Concen: 8.102 ug/l
RT: 2.45 min Scan# 212
Delta R.T. -0.00 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34




Instrument :
MSVOA_X
ClientSampleId :
TP-18


Tgt Ion: 43 Resp: 25631
Ion Ratio Lower Upper
43 100
58 31.6 25.0 37.6

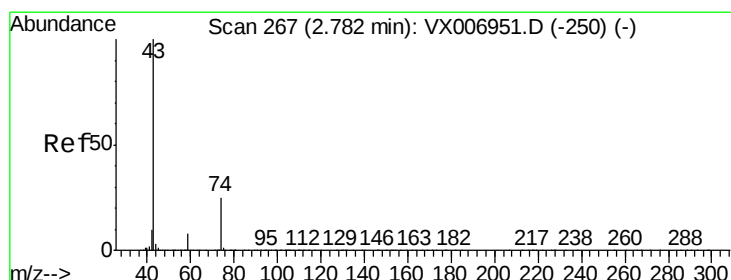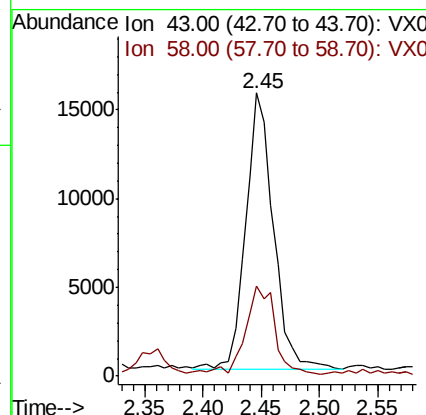

#18
Methyl Acetate
Concen: 2.358 ug/l
RT: 2.78 min Scan# 266
Delta R.T. -0.01 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34

Tgt Ion: 43 Resp: 21602
Ion Ratio Lower Upper
43 100
74 25.5 18.6 28.0

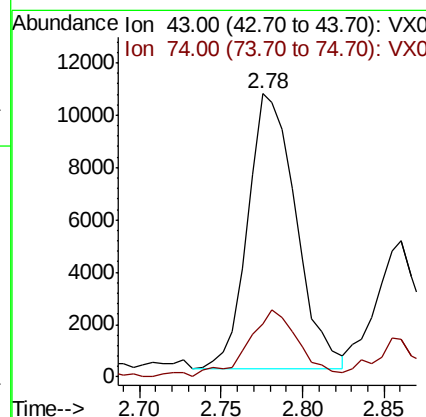







#20
Methylene Chloride
Concen: 395.648 ug/l
RT: 2.86 min Scan# 280
Delta R.T. 0.00 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34

Instrument :
MSVOA_X
ClientSampleId :
TP-18

Tgt Ion: 84 Resp: 2357064




Ion	Ratio	Lower	Upper
84	100		
49	121.8	91.8	137.6
51	37.1	28.5	42.7
86	65.1	50.2	75.2

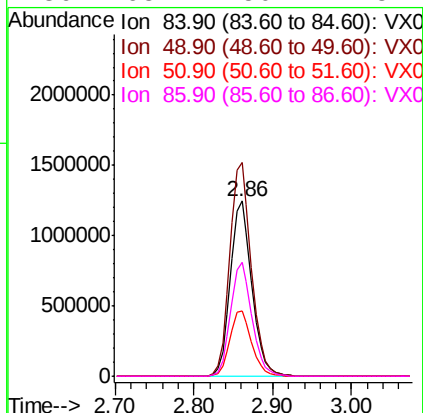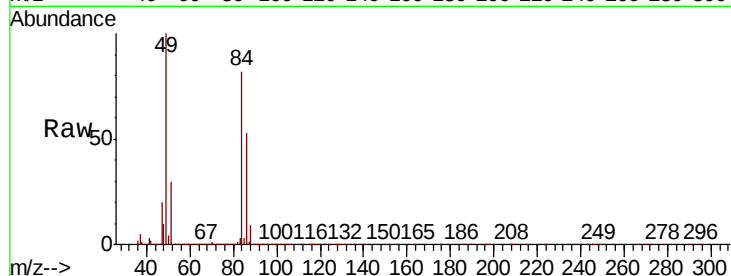


#25
2-Butanone
Concen: 2.599 ug/l
RT: 4.70 min Scan# 581
Delta R.T. -0.01 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34

Tgt Ion: 43 Resp: 11766

Ion	Ratio	Lower	Upper
43	100		
72	18.3	22.4	33.6#


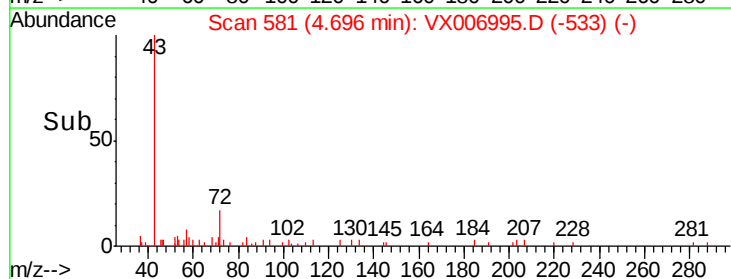
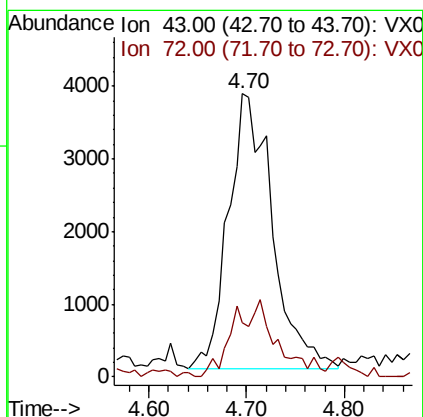



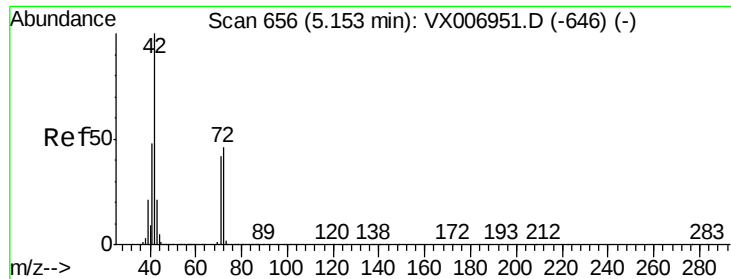

#29
Tetrahydrofuran
Concen: 0.953 ug/l
RT: 5.17 min Scan# 658
Delta R.T. 0.01 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34




Instrument :
MSVOA_X
ClientSampleId :
TP-18


Tgt Ion: 42 Resp: 2804
Ion Ratio Lower Upper
42 100
72 46.4 38.9 58.3
71 48.3 36.2 54.4

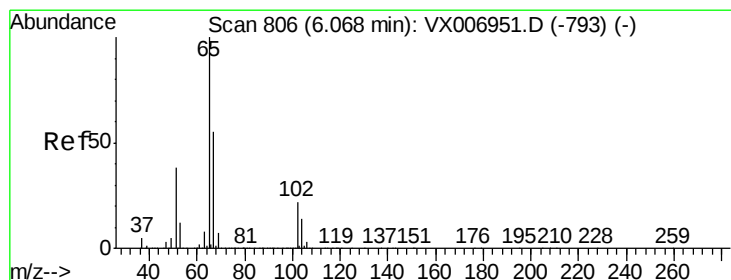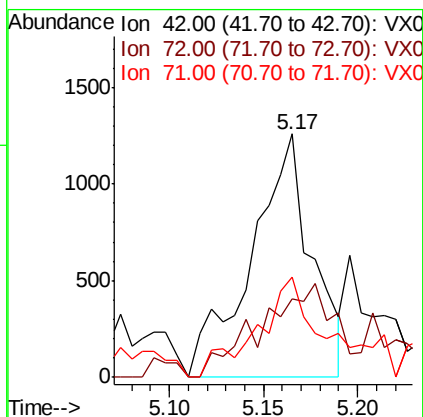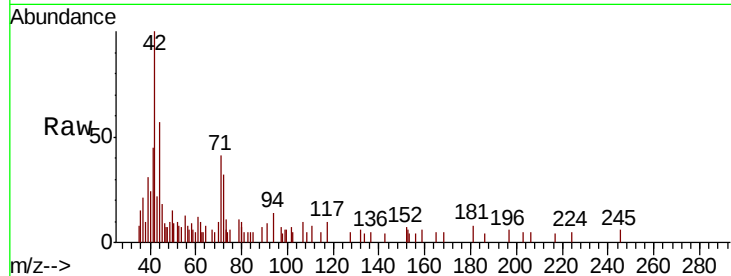

#33
1,2-Dichloroethane-d4
Concen: 50.497 ug/l
RT: 6.07 min Scan# 806
Delta R.T. -0.00 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34

Tgt Ion: 65 Resp: 323136
Ion Ratio Lower Upper
65 100
67 54.6 0.0 105.0

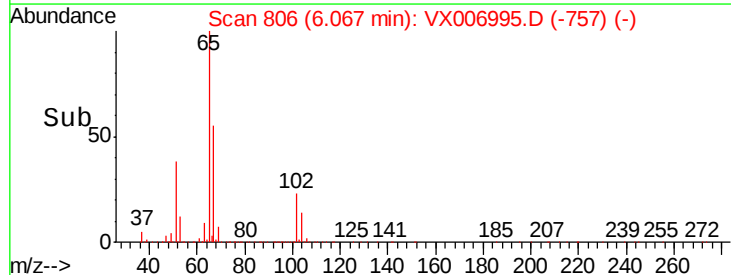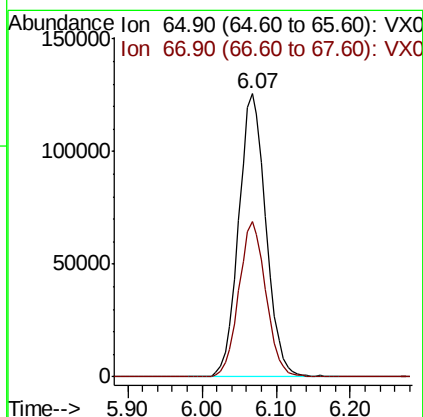



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX006995.D

Acq: 10 Jan 2019 17:34

Instrument :

MSVOA_X

ClientSampleId :

TP-18


Tgt Ion:114 Resp: 947218

Ion Ratio Lower Upper

114 100

63 18.7 0.0 34.8




88 14.2 0.0 28.8

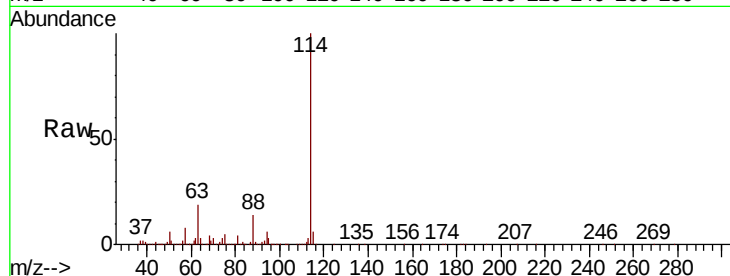

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

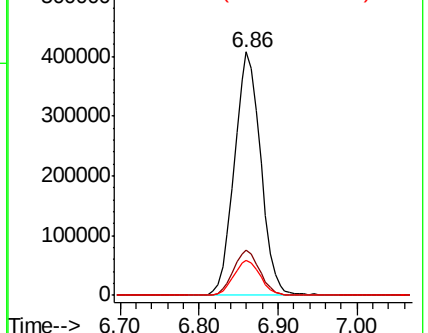

#35

Dibromofluoromethane

Concen: 46.929 ug/l

RT: 5.51 min Scan# 714

Delta R.T. 0.01 min

Lab File: VX006995.D

Acq: 10 Jan 2019 17:34


Tgt Ion:113 Resp: 284667

Ion Ratio Lower Upper

113 100

111 103.0 81.6 122.4



192 22.5 16.7 25.1




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

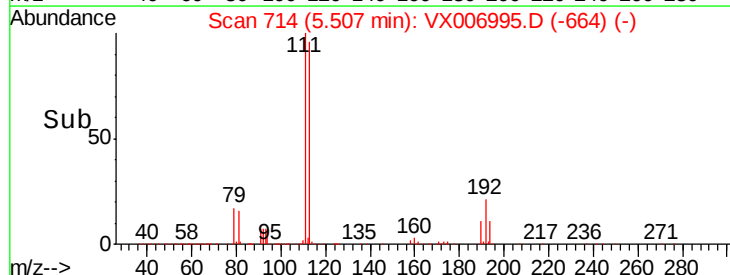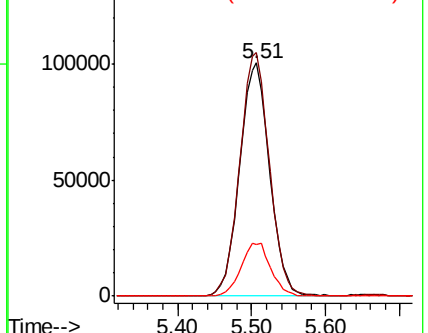

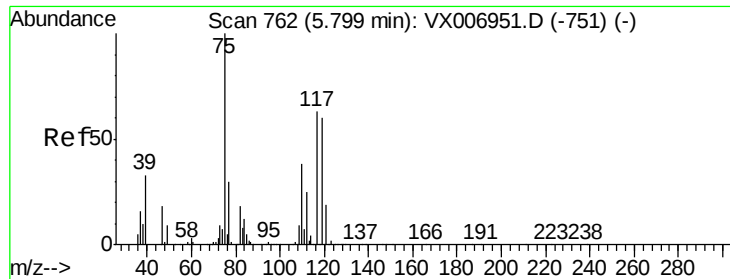

#36

1,1-Dichloropropene

Concen: 4.797 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.13 min

Lab File: VX006995.D

Acq: 10 Jan 2019 17:34

Instrument :

MSVOA_X

ClientSampleId :

TP-18


Tgt Ion: 75 Resp: 39504

Ion Ratio Lower Upper

75 100

110 12.2 20.2 60.5#




77 0.3 24.8 37.2#

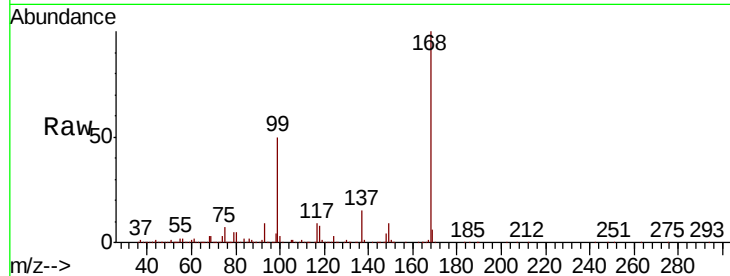

Abundance Ion 74.90 (74.60 to 75.60): VX006995.D (-713) (-)

Ion 109.90 (109.60 to 110.60): VX006995.D (-713) (-)

Ion 76.90 (76.60 to 77.60): VX006995.D (-713) (-)

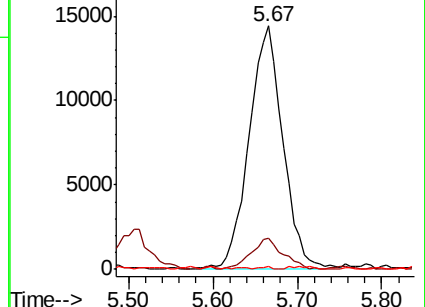

#38

Carbon Tetrachloride

Concen: 6.701 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.12 min

Lab File: VX006995.D

Acq: 10 Jan 2019 17:34


Tgt Ion: 117 Resp: 55519

Ion Ratio Lower Upper

117 100

119 5.6 79.4 119.2#



121 0.0 24.0 36.0#




Abundance Ion 116.80 (116.50 to 117.50): VX006995.D (-710) (-)

Ion 118.80 (118.50 to 119.50): VX006995.D (-710) (-)

Ion 120.80 (120.50 to 121.50): VX006995.D (-710) (-)

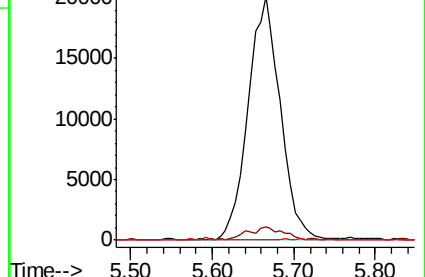



#43

Isopropyl Acetate

Concen: 2.133 ug/l

RT: 6.46 min Scan# 870

Delta R.T. -0.00 min

Lab File: VX006995.D

Acq: 10 Jan 2019 17:34

Instrument :

MSVOA_X

ClientSampleId :

TP-18


Tgt Ion: 43 Resp: 29701

Ion Ratio Lower Upper

43 100

61 21.1 16.8 25.2




87 15.7 12.4 18.6



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

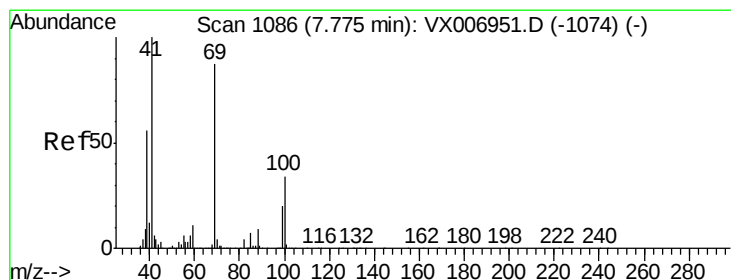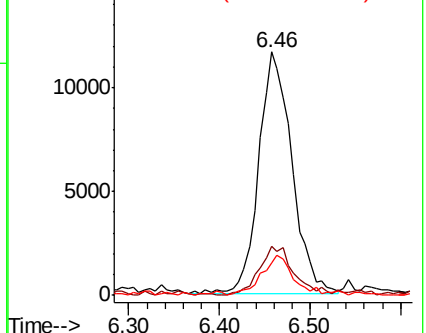

#48

Methyl methacrylate

Concen: 2.632 ug/l

RT: 7.68 min Scan# 1071

Delta R.T. -0.09 min

Lab File: VX006995.D

Acq: 10 Jan 2019 17:34


Tgt Ion: 41 Resp: 18824

Ion Ratio Lower Upper

41 100

69 1.6 72.4 108.6#



39 0.0 45.8 68.8#




Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0




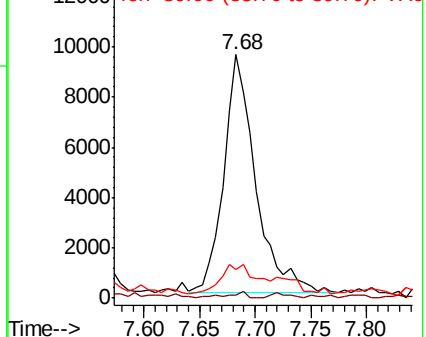


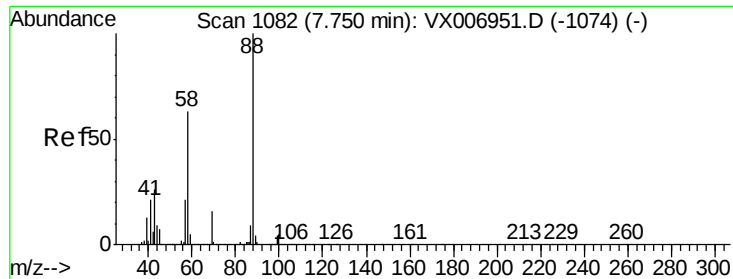

#49
1,4-Dioxane
Concen: Below Cal
RT: 7.76 min Scan# 1084
Delta R.T. 0.01 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34




Instrument :
MSVOA_X
ClientSampleId :
TP-18


Tgt Ion: 88 Resp: 327
Ion Ratio Lower Upper
88 100
43 0.0 22.2 33.4#
58 0.0 51.0 76.4#

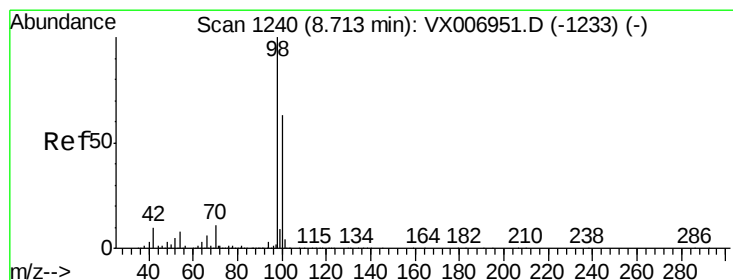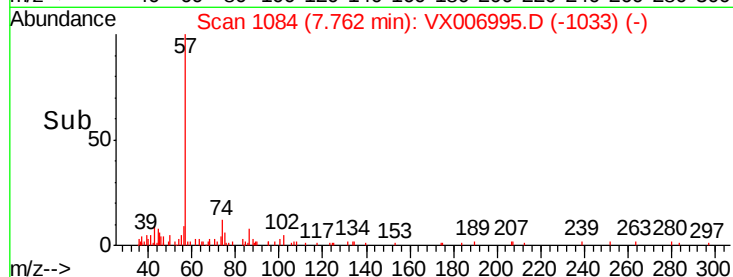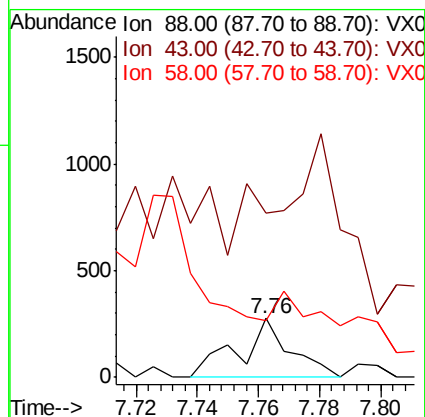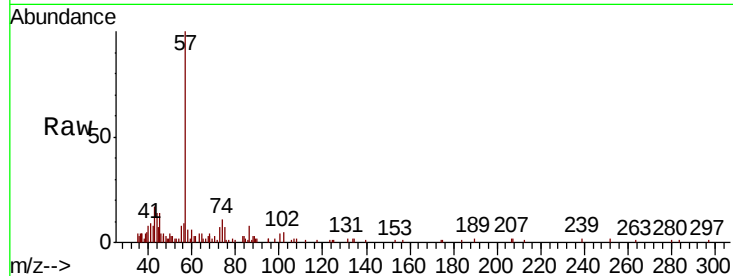

#50
Toluene-d8
Concen: 51.583 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. -0.00 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34

Tgt Ion: 98 Resp: 1145303
Ion Ratio Lower Upper
98 100
100 64.3 52.0 78.0


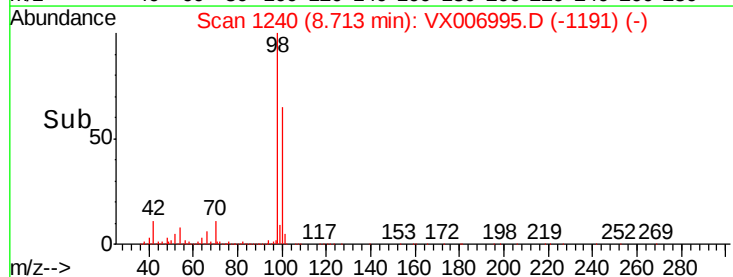
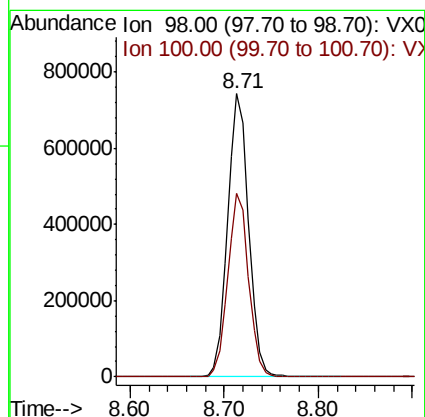
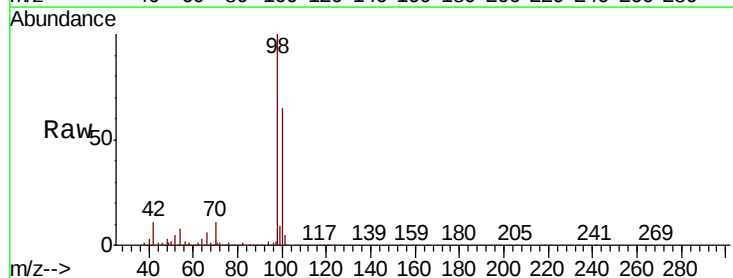




#51
 4-Methyl-2-Pentanone
 Concen: 16.483 ug/l
 RT: 8.62 min Scan# 1224
 Delta R.T. -0.03 min
 Lab File: VX006995.D
 Acq: 10 Jan 2019 17:34




Instrument :
 MSVOA_X
 ClientSampled :
 TP-18


Tgt Ion: 43 Resp: 147527
 Ion Ratio Lower Upper
 43 100
 58 8.1 31.8 47.6#

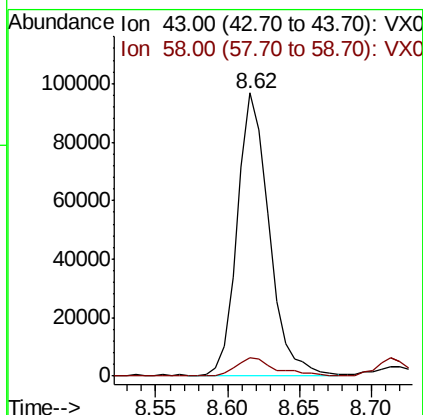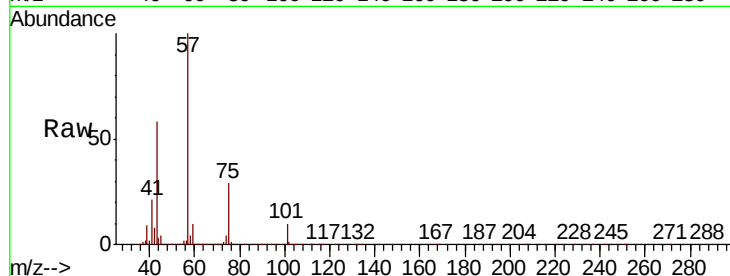

#54
 cis-1,3-Dichloropropene
 Concen: 8.196 ug/l
 RT: 8.62 min Scan# 1224
 Delta R.T. 0.18 min
 Lab File: VX006995.D
 Acq: 10 Jan 2019 17:34

Tgt Ion: 75 Resp: 75845
 Ion Ratio Lower Upper
 75 100
 77 0.4 26.2 39.2#
 39 30.1 36.7 55.1#

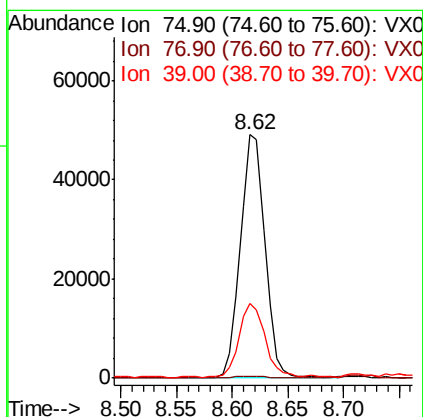

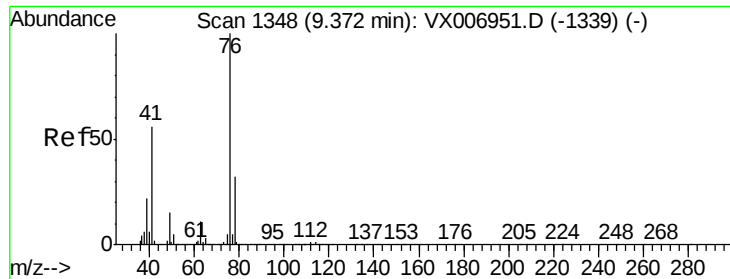

#57

1,3-Dichloropropane

Concen: 1.405 ug/l

RT: 9.54 min Scan# 1376

Delta R.T. 0.17 min

Lab File: VX006995.D

Acq: 10 Jan 2019 17:34

Instrument :

MSVOA_X

ClientSampled :


TP-18

Tgt Ion: 76 Resp: 14882

Ion Ratio Lower Upper

76 100

78 0.7 26.0 39.0#

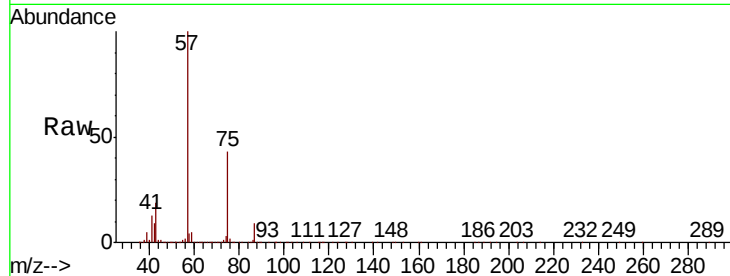

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0



9.54

10000

5000

0

Time-->

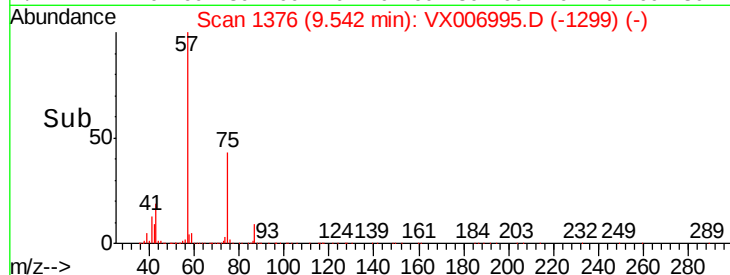

#59

2-Hexanone

Concen: 29.361 ug/l

RT: 9.54 min Scan# 1376

Delta R.T. 0.05 min

Lab File: VX006995.D


Acq: 10 Jan 2019 17:34

Tgt Ion: 43 Resp: 200253

Ion Ratio Lower Upper

43 100

58 20.4 27.7 83.1#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

9.54


150000


100000

50000

0

Time-->









#62
4-Bromofluorobenzene
Concen: 52.963 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34




Instrument :
MSVOA_X
ClientSampleId :
TP-18


Tgt Ion	Ratio	Lower	Upper
95	100		
174	91.2	0.0	182.2
176	89.4	0.0	178.8

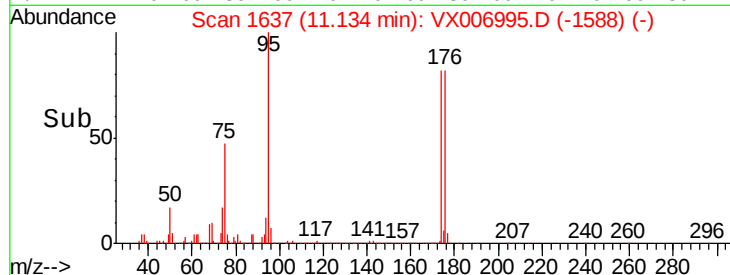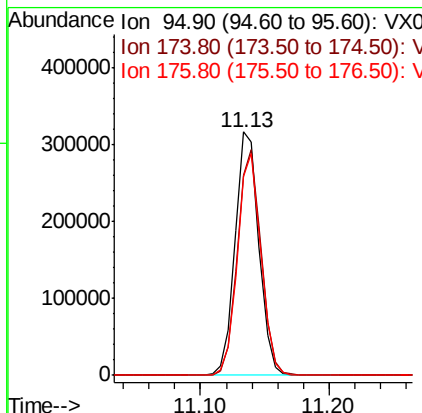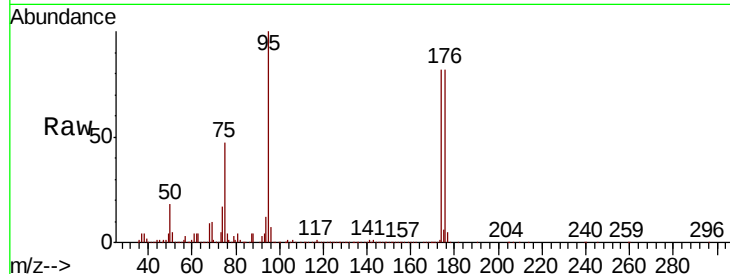

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.01 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34

Tgt Ion	Ratio	Lower	Upper
117	100		
82	52.6	41.0	61.6
119	31.3	25.4	38.0



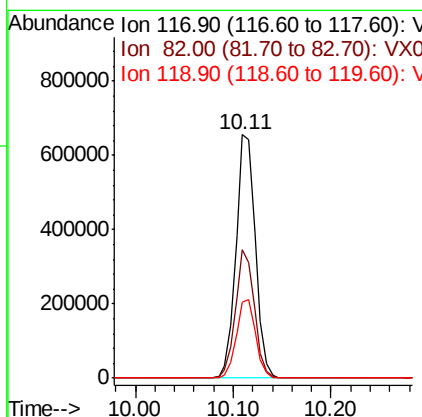
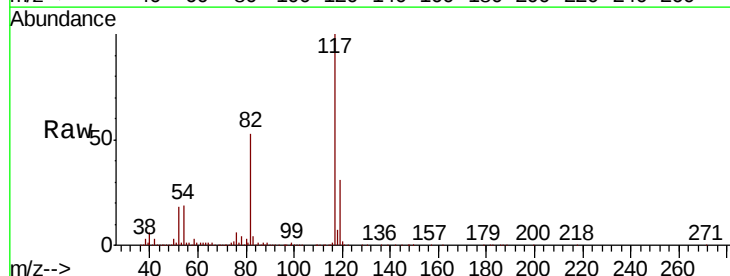




#65
Chlorobenzene
Concen: 0.256 ug/l
RT: 10.13 min Scan# 1473
Delta R.T. -0.01 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34




Instrument :
MSVOA_X
ClientSampled :
TP-18


Tgt Ion:112 Resp: 5033
Ion Ratio Lower Upper
112 100
114 27.8 25.7 38.5

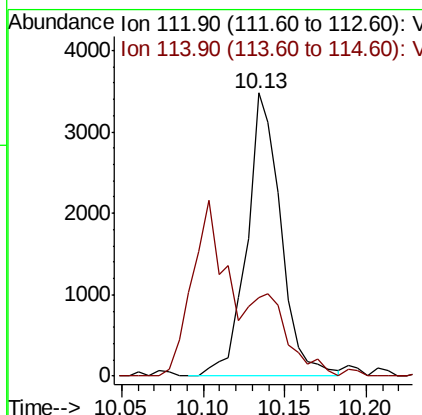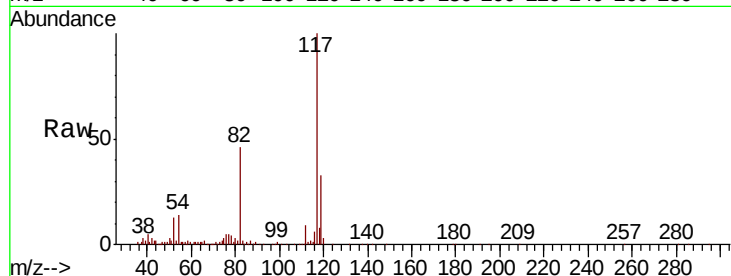

#68
m/p-Xylenes
Concen: 0.440 ug/l
RT: 10.36 min Scan# 1510
Delta R.T. -0.00 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34

Tgt Ion:106 Resp: 5617
Ion Ratio Lower Upper
106 100
91 195.5 155.8 233.6



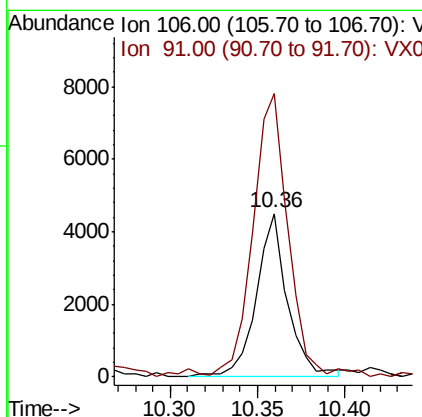



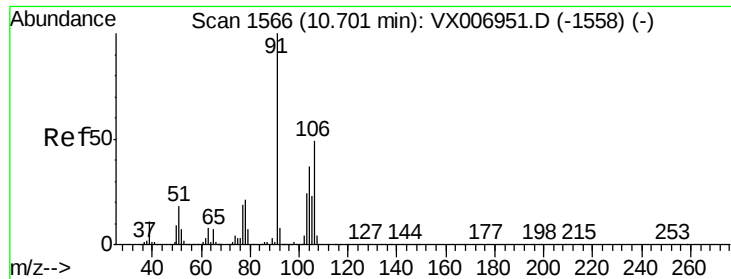

#69
o-Xylene
Concen: 0.260 ug/l
RT: 10.69 min Scan# 1565
Delta R.T. -0.01 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34




Instrument :
MSVOA_X
ClientSampled :
TP-18


Tgt Ion:106 Resp: 3233
Ion Ratio Lower Upper
106 100
91 174.2 101.3 303.7

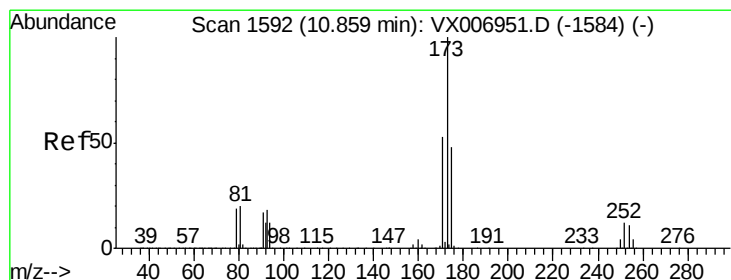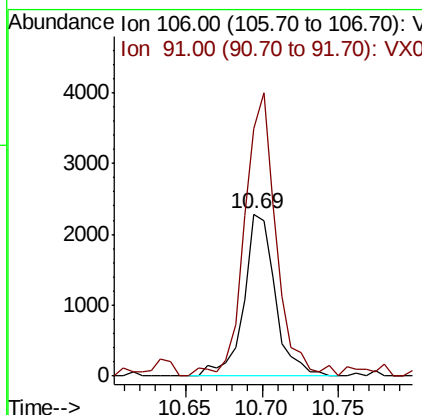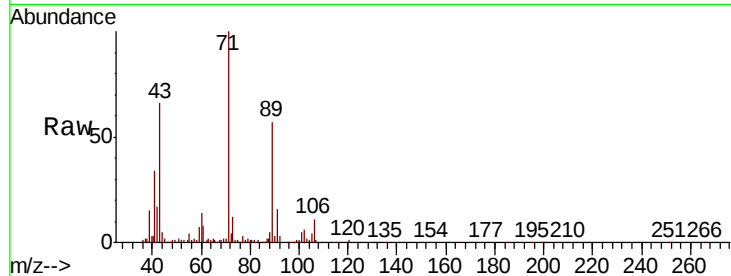

#71
Bromoform
Concen: 4.748 ug/l
RT: 11.01 min Scan# 1616
Delta R.T. 0.15 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34

Tgt Ion:173 Resp: 136
Ion Ratio Lower Upper
173 100
175 0.0 24.7 74.1#
254 0.0 0.2 0.2#

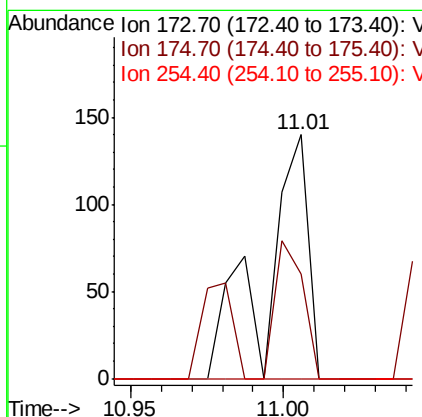




#72




1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34

Instrument :
MSVOA_X
ClientSampleId :
TP-18

Tgt Ion	Ratio	Lower	Upper
152	100		
115	55.2	39.1	117.2
150	157.0	0.0	344.8

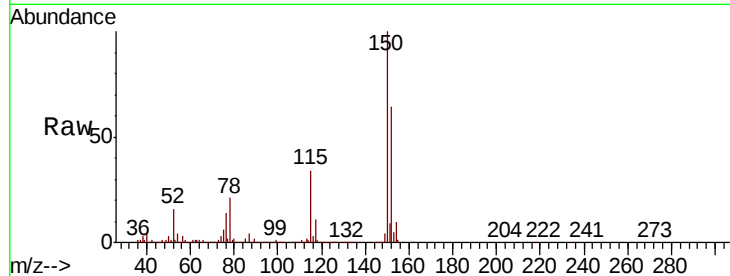


Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

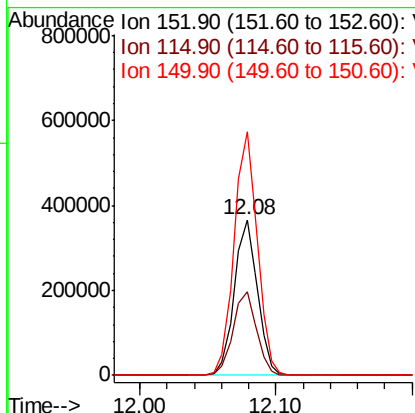



#76


1,2,3-Trichloropropane
Concen: 21.886 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.16 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34

Tgt Ion	Ratio	Lower	Upper
75	100		
77	1.4	18.5	55.5#



Abundance Ion 74.90 (74.60 to 75.60): VX0
Ion 77.00 (76.70 to 77.70): VX0



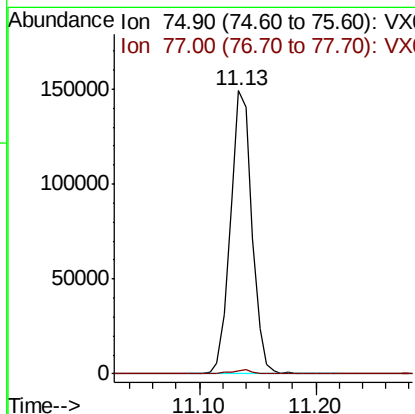





#81
 trans-1,4-Dichloro-2-butene
 Concen: 64.834 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. 0.06 min
 Lab File: VX006995.D
 Acq: 10 Jan 2019 17:34




Instrument :
 MSVOA_X
 ClientSampleId :
 TP-18


Tgt Ion: 75 Resp: 192113
 Ion Ratio Lower Upper
 75 100
 53 0.0 79.7 119.5#
 89 0.1 38.0 57.0#

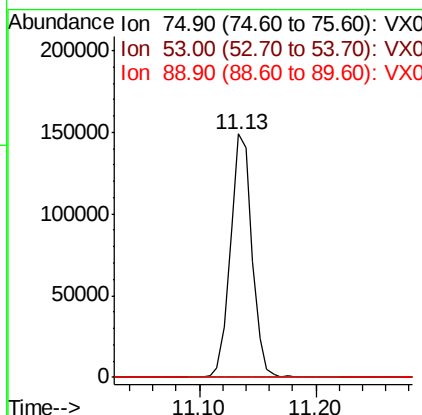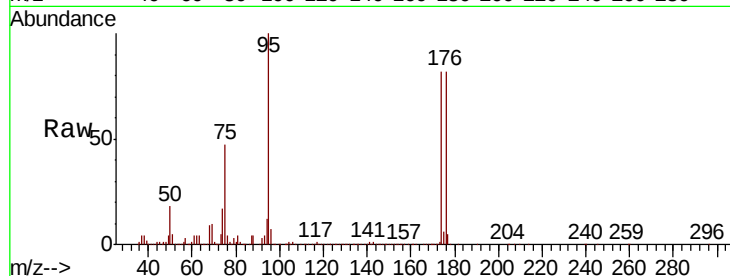

#84
 1,2,4-Trimethylbenzene
 Concen: 0.440 ug/l
 RT: 11.80 min Scan# 1747
 Delta R.T. -0.00 min
 Lab File: VX006995.D
 Acq: 10 Jan 2019 17:34

Tgt Ion: 105 Resp: 11296
 Ion Ratio Lower Upper
 105 100
 120 50.8 23.2 69.6



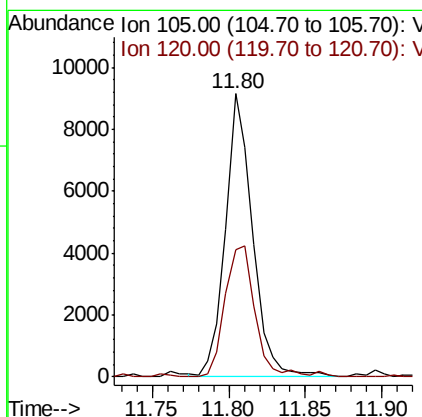



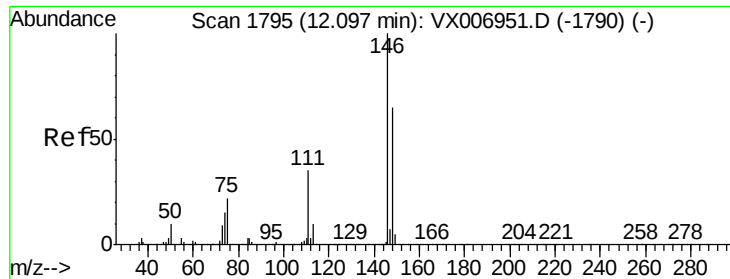

#88
 1,4-Dichlorobenzene
 Concen: 0.206 ug/l
 RT: 12.08 min Scan# 1793
 Delta R.T. -0.01 min
 Lab File: VX006995.D
 Acq: 10 Jan 2019 17:34




Instrument :
 MSVOA_X
 ClientSampleId :
 TP-18


Tgt Ion:146 Resp: 884
 Ion Ratio Lower Upper
 146 100
 111 644.9 18.1 54.1#
 148 299.0 31.9 95.9#

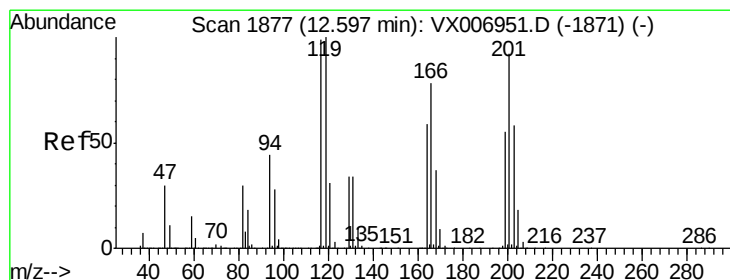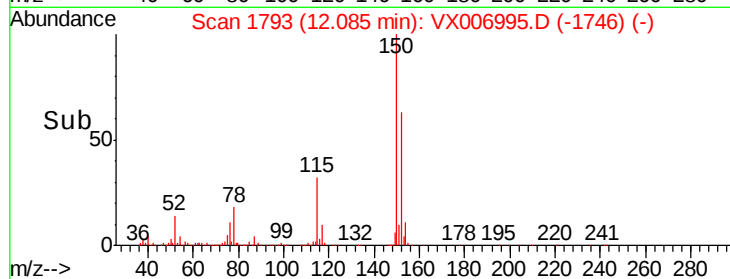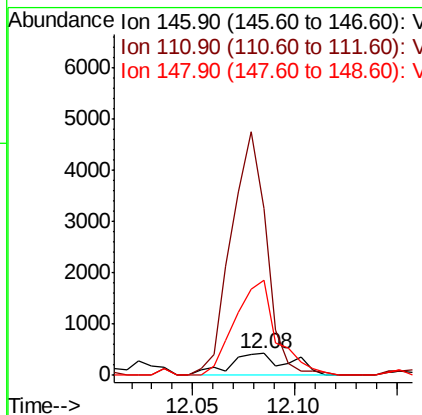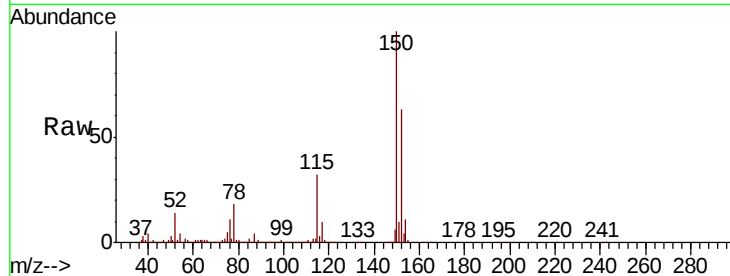

#90
 Hexachloroethane
 Concen: 3.031 ug/l
 RT: 12.58 min Scan# 1875
 Delta R.T. -0.01 min
 Lab File: VX006995.D
 Acq: 10 Jan 2019 17:34

Tgt Ion:117 Resp: 566
 Ion Ratio Lower Upper
 117 100
 201 0.0 42.9 128.7#

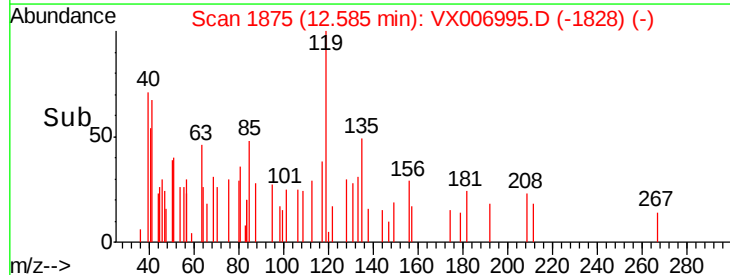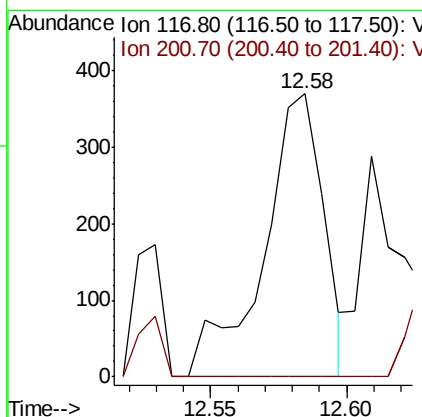



#95
Naphthalene
Concen: 7.004 ug/l
RT: 13.83 min Scan# 2080
Delta R.T. -0.00 min
Lab File: VX006995.D
Acq: 10 Jan 2019 17:34

Instrument :
MSVOA_X
ClientSampleId :
TP-18

Tgt Ion	Ratio	Lower	Upper
128	100		
127	13.0	10.1	15.1
129	10.9	8.6	13.0

