

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX011019\
 Data File : VX006982.D
 Acq On : 10 Jan 2019 11:40
 Operator : JC/MD
 Sample : VX0110WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0110WBL01

Quant Time: Jan 11 07:31:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 08 14:06:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	621800	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	952394	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	878703	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	428055	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.06	65	332159	51.11	ug/l	0.00
Spiked Amount						
			Recovery	=	102.22%	
35) Dibromofluoromethane	5.50	113	297800	48.83	ug/l	0.00
Spiked Amount						
			Recovery	=	97.66%	
50) Toluene-d8	8.71	98	1130607	50.64	ug/l	0.00
Spiked Amount						
			Recovery	=	101.28%	
62) 4-Bromofluorobenzene	11.13	95	400267	51.43	ug/l	0.00
Spiked Amount						
			Recovery	=	102.86%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX011019\
Data File : VX006982.D
Acq On : 10 Jan 2019 11:40
Operator : JC/MD
Sample : VX0110WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0110WBL01

Quant Time: Jan 11 07:31:37 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 08 14:06:59 2019
Response via : Initial Calibration

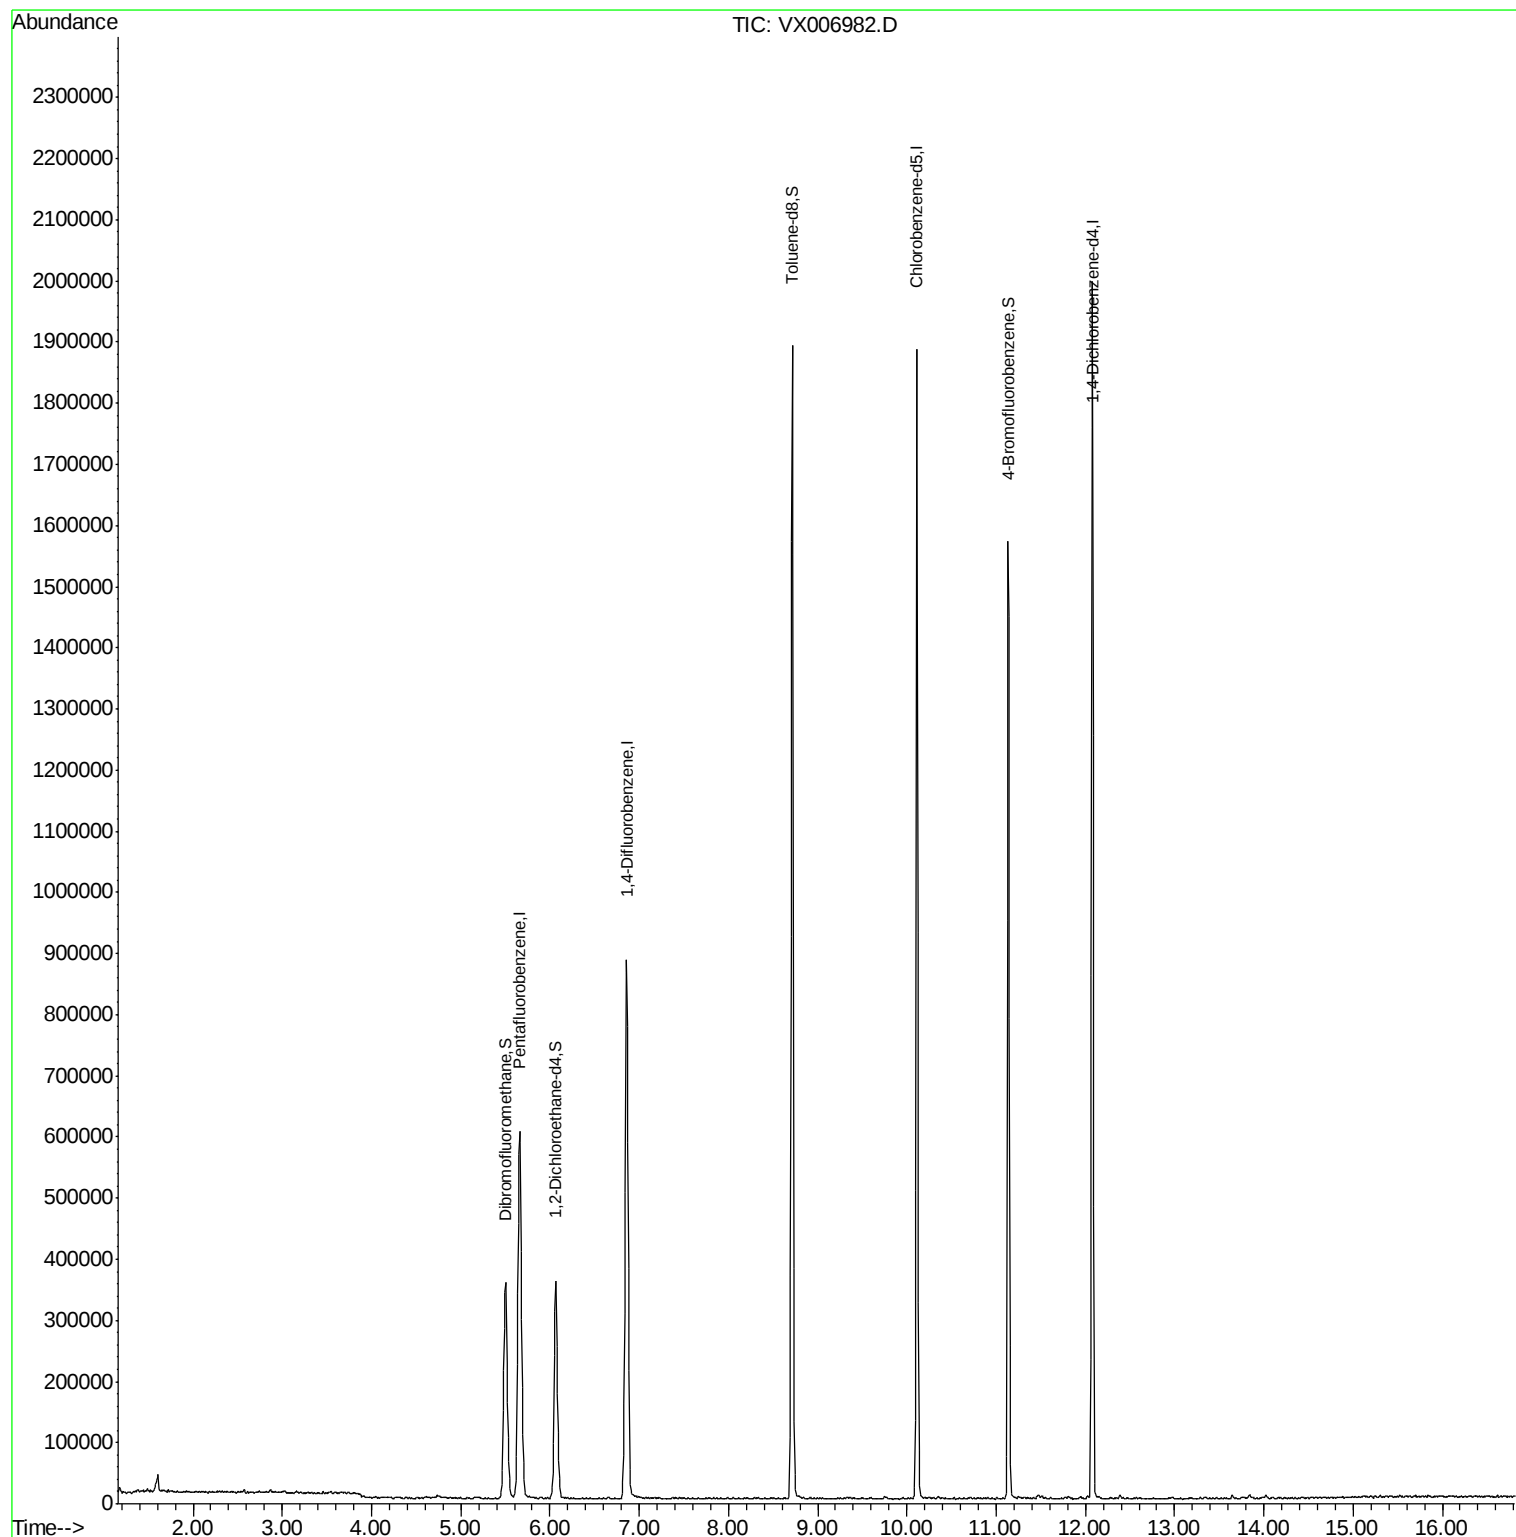

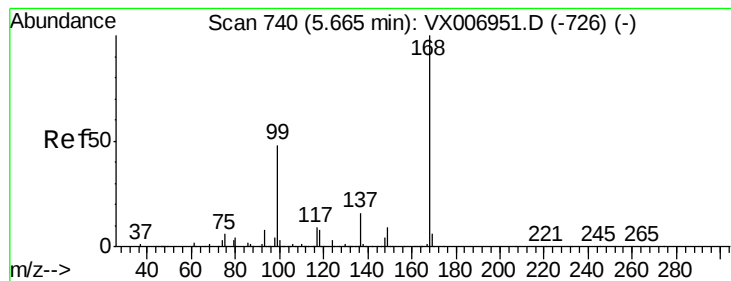

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.01 min

Lab File: VX006982.D

Acq: 10 Jan 2019 11:40

Instrument :

MSVOA_X

ClientSampleId :


VX0110WBL01

Tot Ion:168 Resp: 621800

Ion Ratio Lower Upper

168 100




99 48.7 41.8 62.8

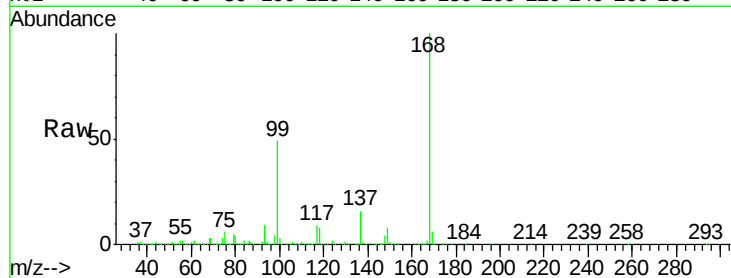

Abundance Ion 167.90 (167.60 to 168.60): VX0

Ion 98.90 (98.60 to 99.60): VX0

5.66

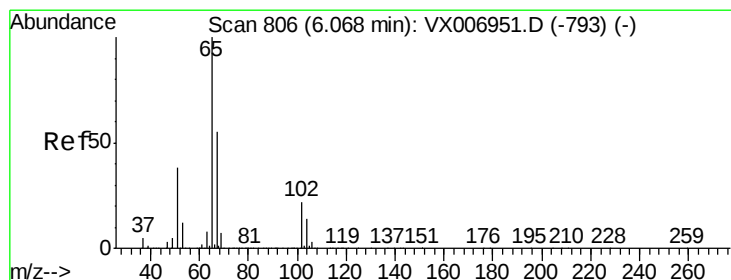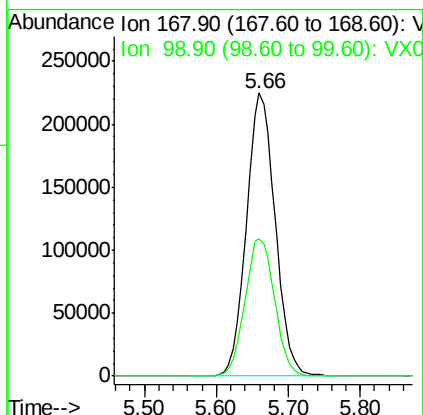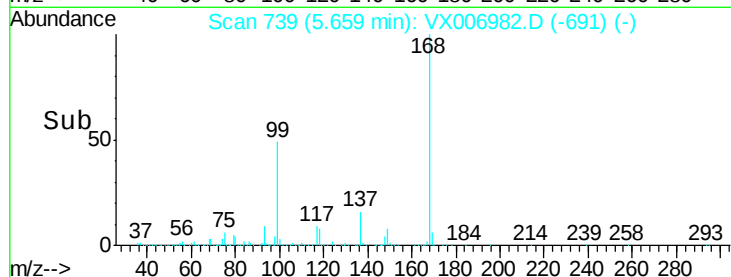

#33

1,2-Dichloroethane-d4

Concen: 51.114 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.01 min

Lab File: VX006982.D


Acq: 10 Jan 2019 11:40

Tgt Ion: 65 Resp: 332159

Ion Ratio Lower Upper

65 100



67 53.3 0.0 105.0

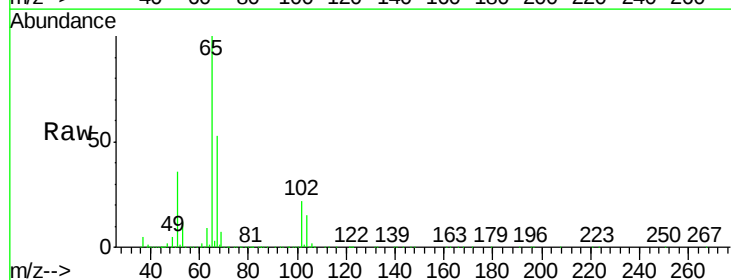


Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.06

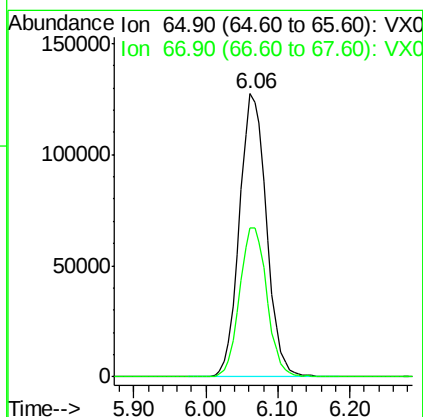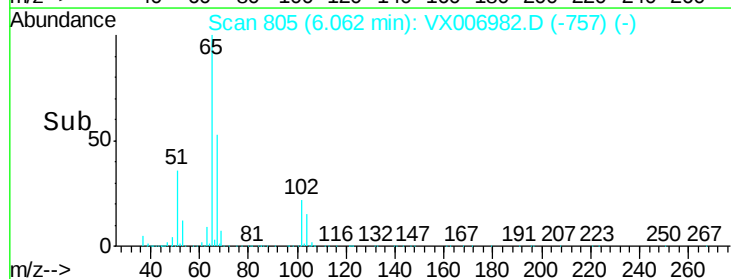

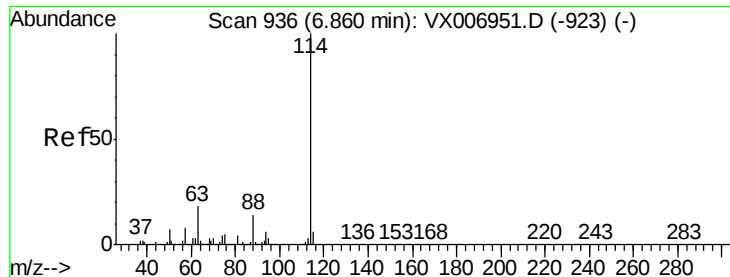

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX006982.D

Acq: 10 Jan 2019 11:40

Instrument :

MSVOA_X

ClientSampleId :

VX0110WBL01


Tot Ion:114 Resp: 952394

Ion Ratio Lower Upper

114 100

63 17.6 0.0 34.8




88 14.9 0.0 28.8

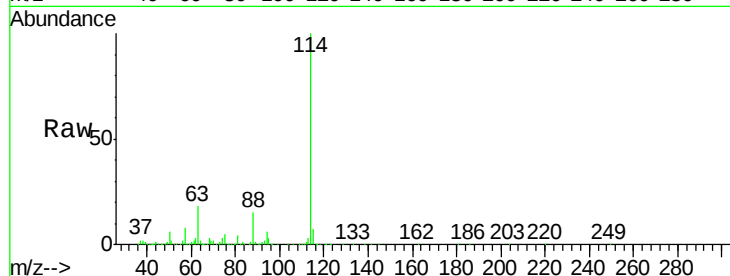

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

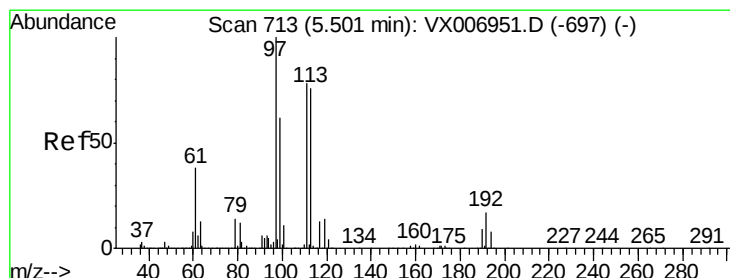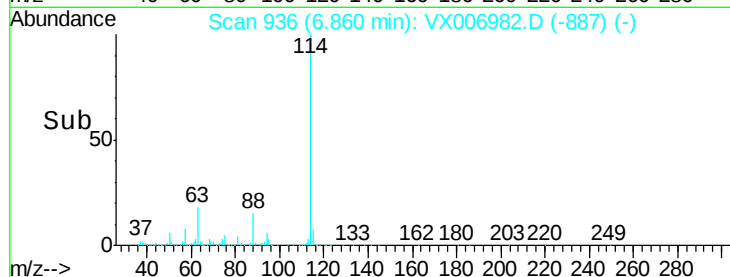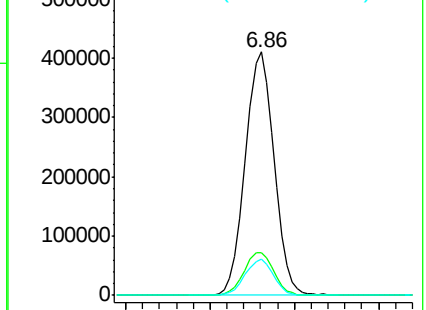

#35

Dibromofluoromethane

Concen: 48.827 ug/l

RT: 5.50 min Scan# 713

Delta R.T. 0.00 min

Lab File: VX006982.D

Acq: 10 Jan 2019 11:40


Tgt Ion:113 Resp: 297800

Ion Ratio Lower Upper

113 100

111 102.5 81.6 122.4



192 22.3 16.7 25.1

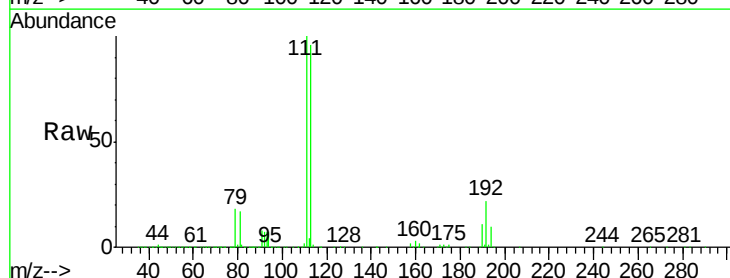


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

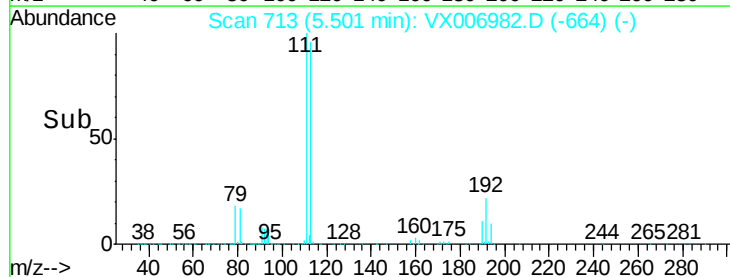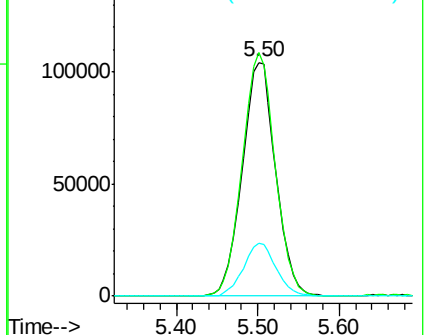

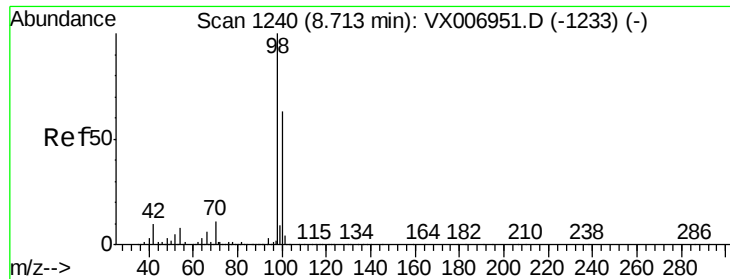

#50

Toluene-d8

Concen: 50.644 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX006982.D

Acq: 10 Jan 2019 11:40

Instrument :

MSVOA_X

ClientSampleId :


VX0110WBL01

Tot Ion: 98 Resp: 1130607

Ion Ratio Lower Upper




98 100

100 63.8 52.0 78.0

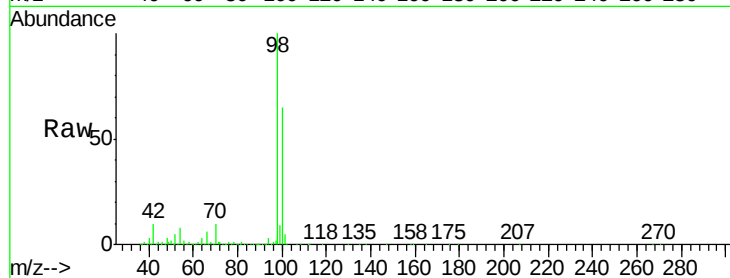

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

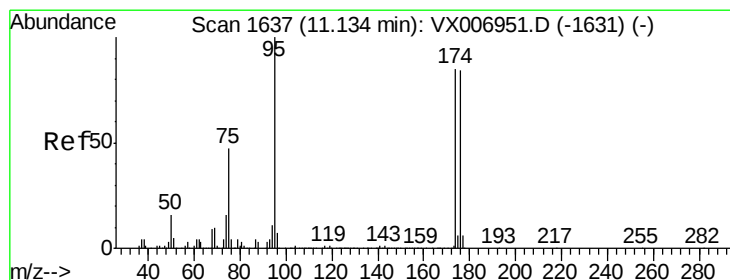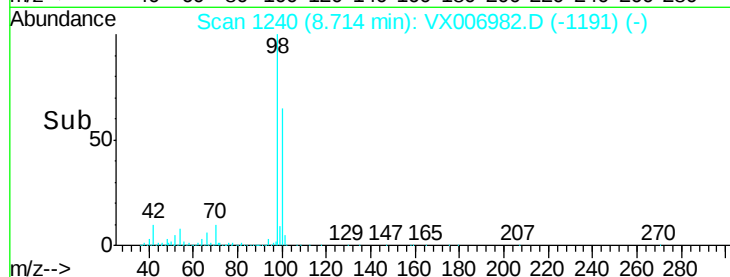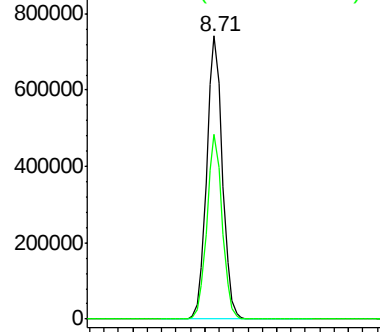

#62

4-Bromofluorobenzene

Concen: 51.429 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX006982.D

Acq: 10 Jan 2019 11:40


Tgt Ion: 95 Resp: 400267

Ion Ratio Lower Upper

95 100

174 91.4 0.0 182.2



176 90.4 0.0 178.8

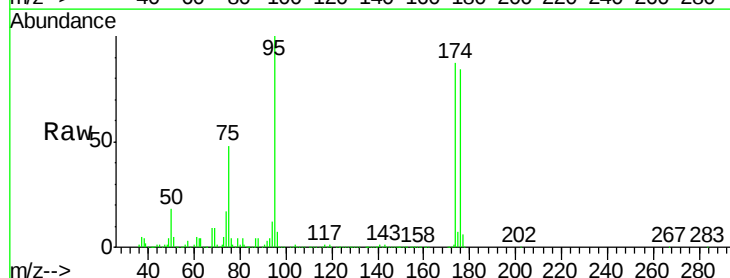


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V



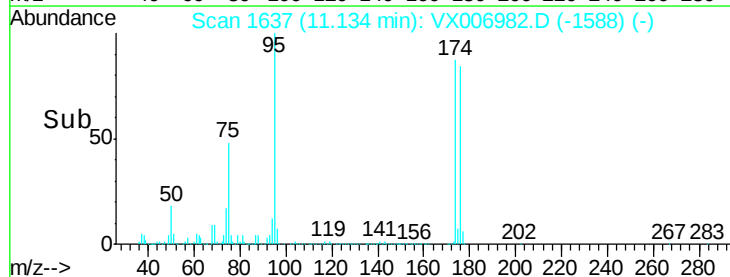
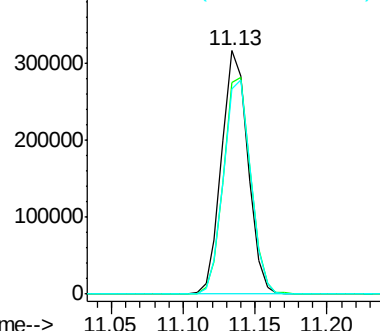


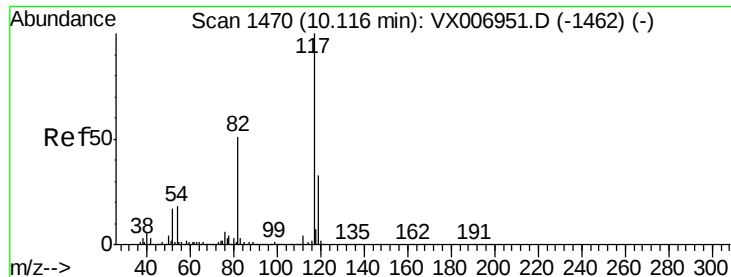

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.01 min
Lab File: VX006982.D
Acq: 10 Jan 2019 11:40

Instrument :
MSVOA_X
ClientSampleId :
VX0110WBL01

Tot Ion:117 Resp: 878703
Ion Ratio Lower Upper
117 100
82 52.7 41.0 61.6
119 31.8 25.4 38.0

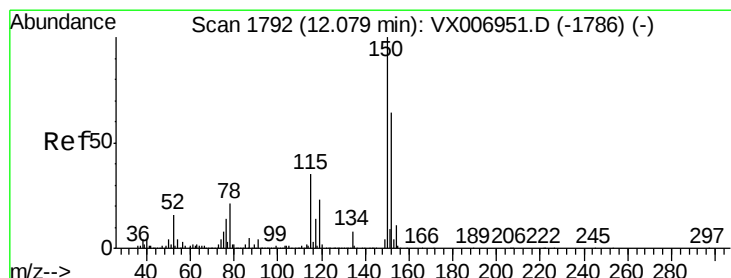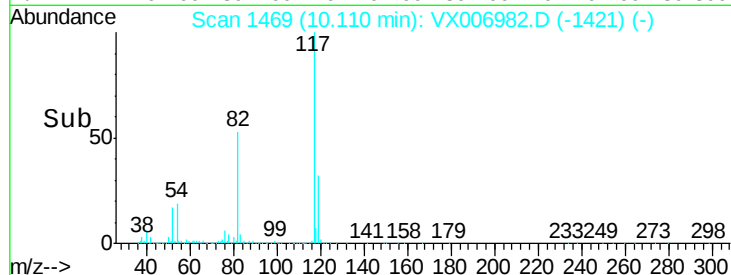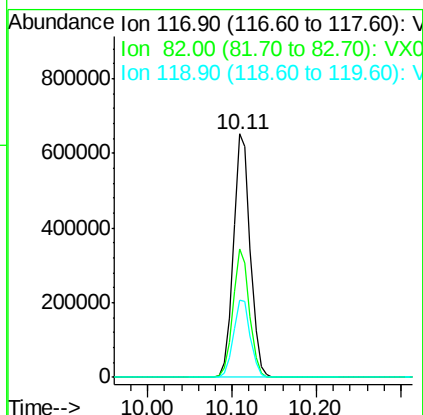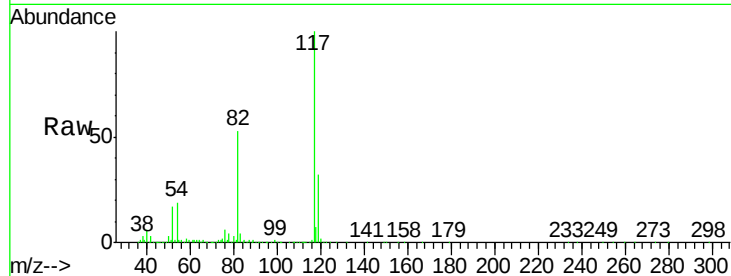

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. 0.00 min
Lab File: VX006982.D
Acq: 10 Jan 2019 11:40

Tgt Ion:152 Resp: 428055
Ion Ratio Lower Upper
152 100
115 54.2 39.1 117.2
150 156.4 0.0 344.8

