


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX011019\  
 Data File : VX006980.D  
 Acq On : 10 Jan 2019 09:53  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M  
 Title : SW846 8260  
 Last Update : Tue Jan 08 14:06:59 2019

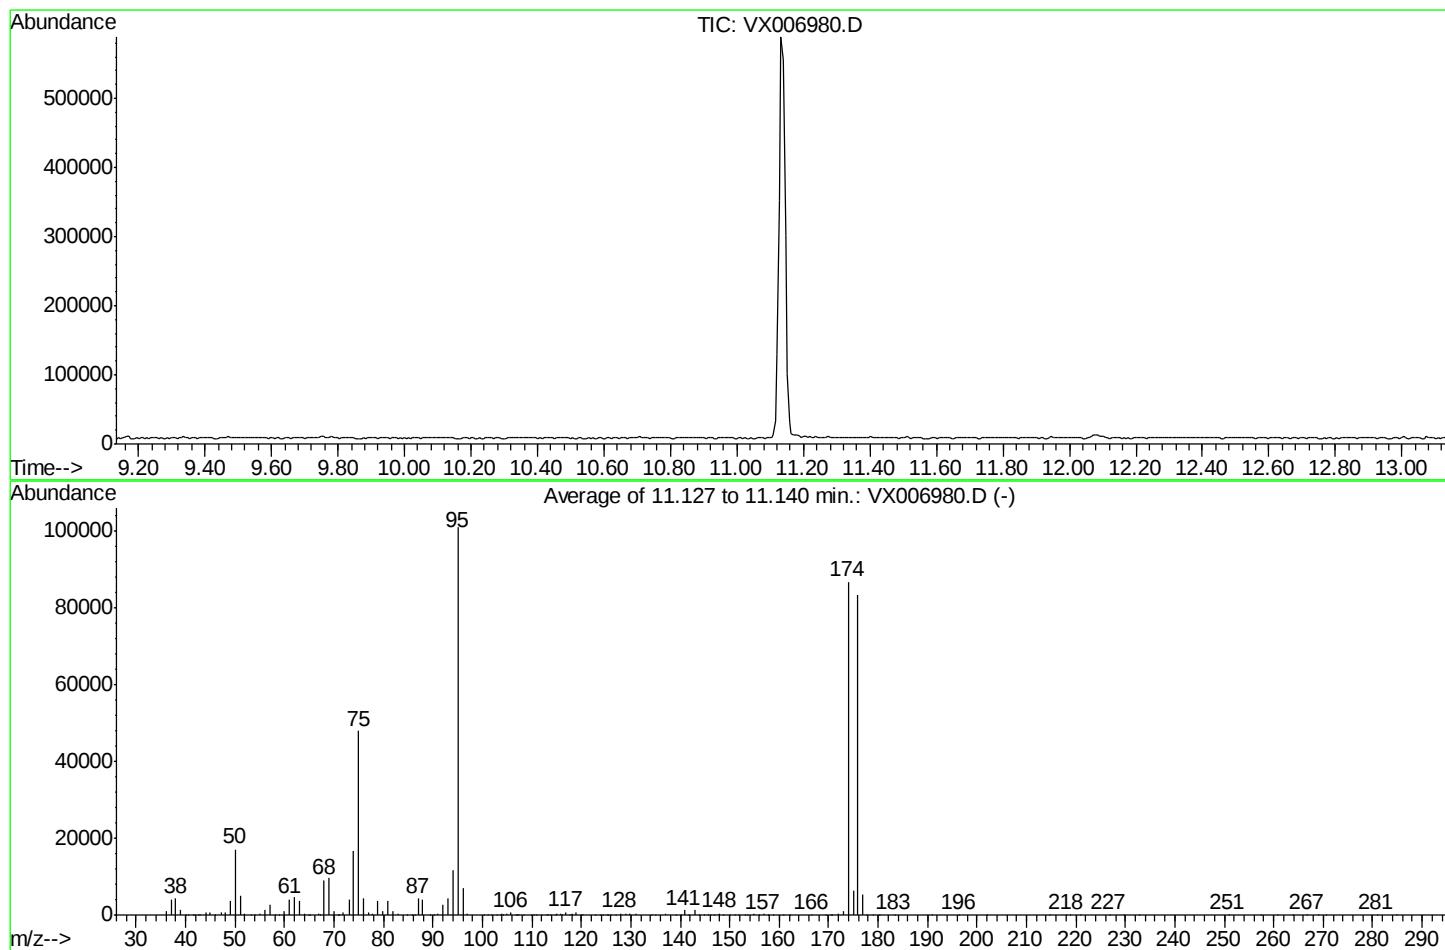

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 16.9      | 17029   | PASS             |
| 75          | 95           | 30           | 60           | 47.5      | 47900   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 100909  | PASS             |
| 96          | 95           | 5            | 9            | 6.8       | 6896    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.2       | 1080    | PASS             |
| 174         | 95           | 50           | 100          | 86.0      | 86805   | PASS             |
| 175         | 174          | 5            | 9            | 7.4       | 6435    | PASS             |
| 176         | 174          | 95           | 101          | 96.0      | 83304   | PASS             |
| 177         | 176          | 5            | 9            | 6.3       | 5256    | PASS             |