

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX011020\
 Data File : VX014542.D
 Acq On : 10 Jan 2020 17:08
 Operator : JC/SP
 Sample : L1080-08
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-5

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	45	rBV	1545948	1809775	79.32%	13.157%
2	1.271	59	63	68	rBV	29188	39294	1.72%	0.286%
3	1.594	108	116	119	rBV7	25001	48240	2.11%	0.351%
4	5.490	743	755	765	rBV2	258539	748349	32.80%	5.440%
5	5.654	771	782	799	rBV	470349	1290426	56.56%	9.381%
6	6.057	838	848	860	rBV	286864	747111	32.75%	5.431%
7	6.849	969	978	991	rBV	701680	1642209	71.98%	11.938%
8	8.709	1277	1283	1293	rBV	1484740	2281532	100.00%	16.586%
9	10.105	1506	1512	1520	rBV	1408278	1916446	84.00%	13.932%
10	11.135	1675	1681	1690	rBV	1103574	1443985	63.29%	10.497%
11	12.074	1830	1835	1843	rBV	1443256	1725595	75.63%	12.545%
12	12.202	1852	1856	1862	rBV	21199	33373	1.46%	0.243%
13	12.263	1863	1866	1876	rVB	17584	29258	1.28%	0.213%


Sum of corrected areas: 13755593

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX011020\
Data File : VX014542.D
Acq On : 10 Jan 2020 17:08
Operator : JC/SP
Sample : L1080-08
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

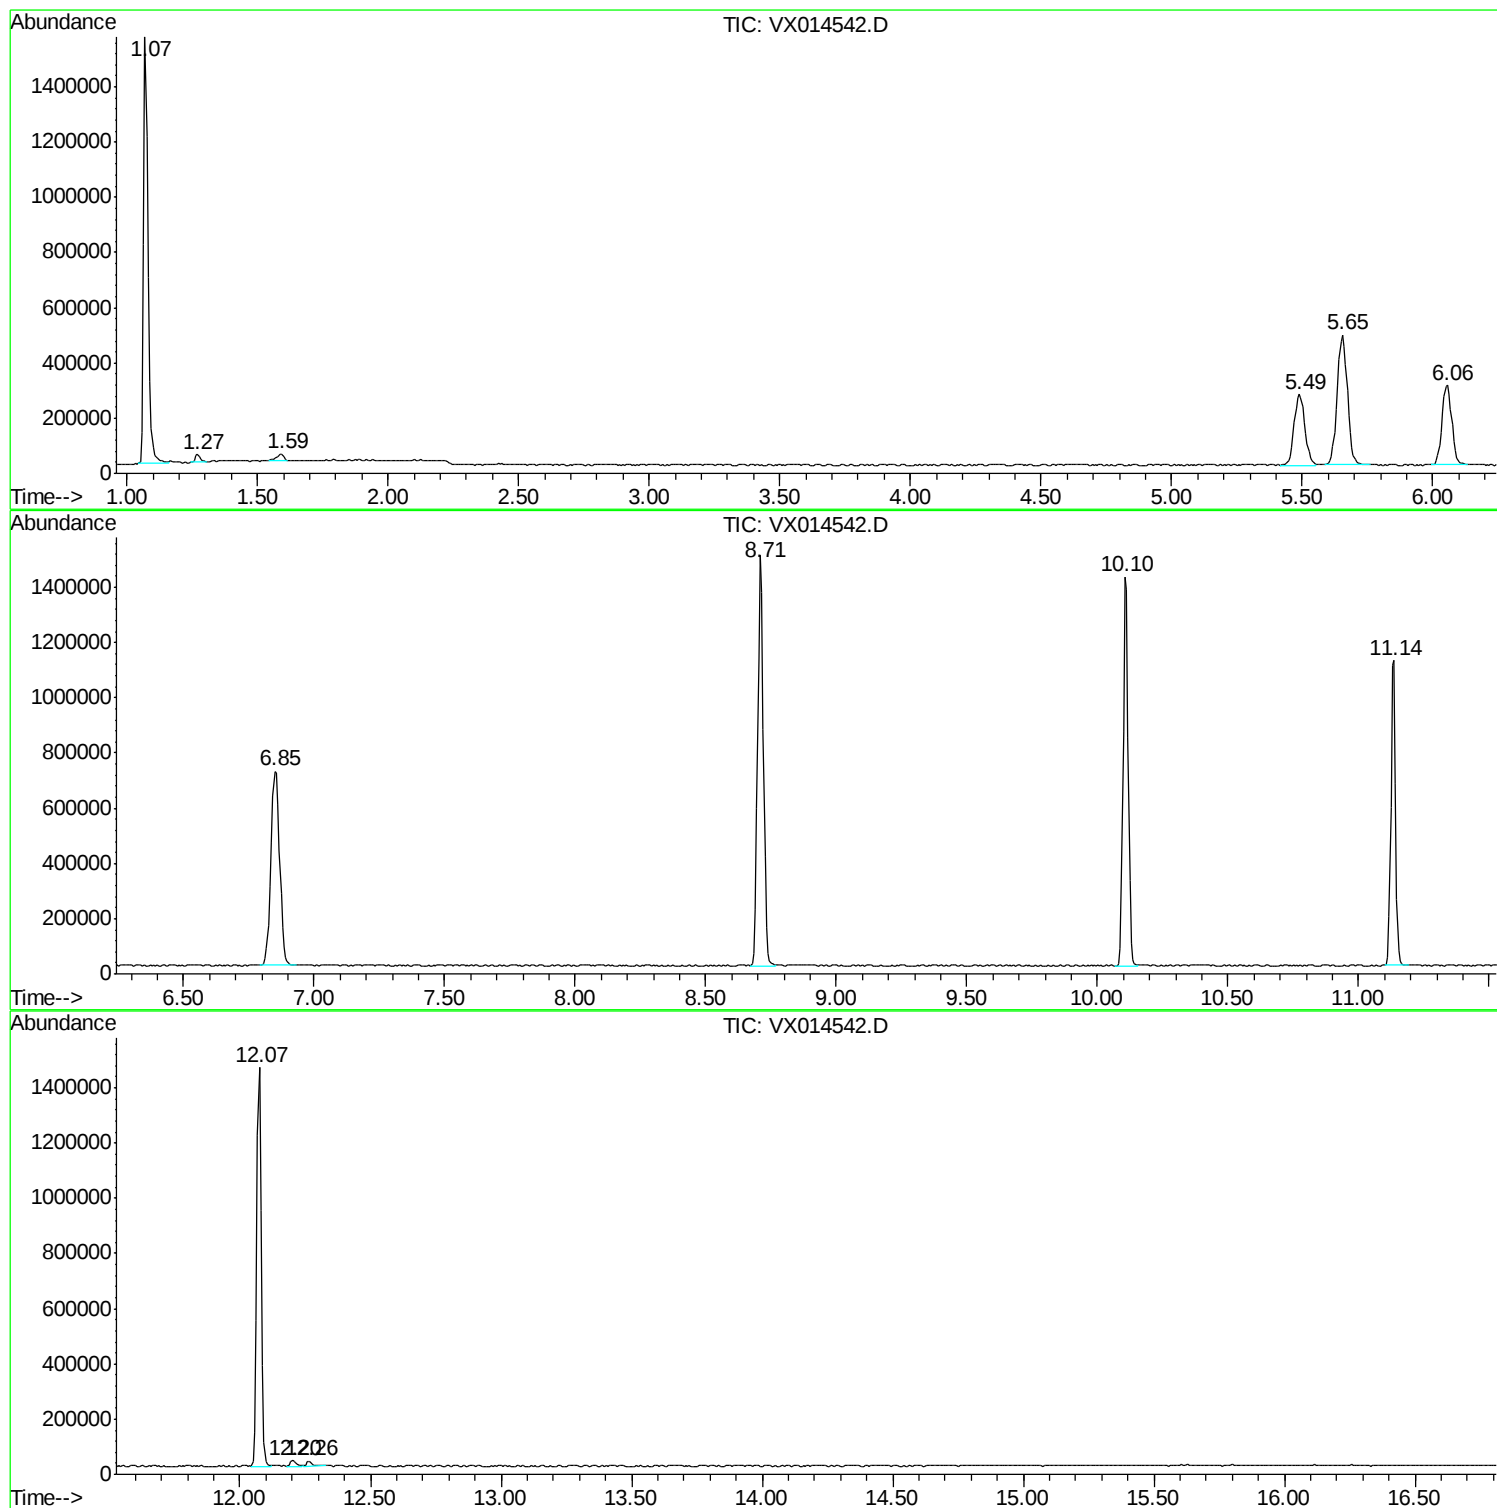

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX011020\
Data File : VX014542.D
Acq On : 10 Jan 2020 17:08
Operator : JC/SP
Sample : L1080-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX011020\
Data File : VX014542.D
Acq On : 10 Jan 2020 17:08
Operator : JC/SP
Sample : L1080-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc