

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX011020\
 Data File : VX014544.D
 Acq On : 10 Jan 2020 17:55
 Operator : JC/SP
 Sample : L1080-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	45	rBV	2334813	2713106	100.00%	18.162%
2	1.271	59	63	67	rBV2	29473	41073	1.51%	0.275%
3	1.588	111	115	120	rVB8	26942	45263	1.67%	0.303%
4	3.179	370	376	384	rVB2	27382	62047	2.29%	0.415%
5	5.490	743	755	766	rBV	267363	751842	27.71%	5.033%
6	5.655	769	782	798	rVB	471465	1303913	48.06%	8.729%
7	6.051	837	847	858	rBV	291301	760645	28.04%	5.092%
8	6.849	969	978	989	rBV	709382	1660502	61.20%	11.116%
9	8.709	1275	1283	1295	rBV	1490318	2293970	84.55%	15.356%
10	10.111	1507	1513	1521	rBV	1437313	1968820	72.57%	13.180%
11	11.135	1672	1681	1690	rBV	1130672	1508812	55.61%	10.100%
12	12.074	1829	1835	1844	rBV	1429941	1793731	66.11%	12.008%
13	12.196	1852	1855	1862	rBV2	18004	34400	1.27%	0.230%


Sum of corrected areas: 14938124

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX011020\
Data File : VX014544.D
Acq On : 10 Jan 2020 17:55
Operator : JC/SP
Sample : L1080-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

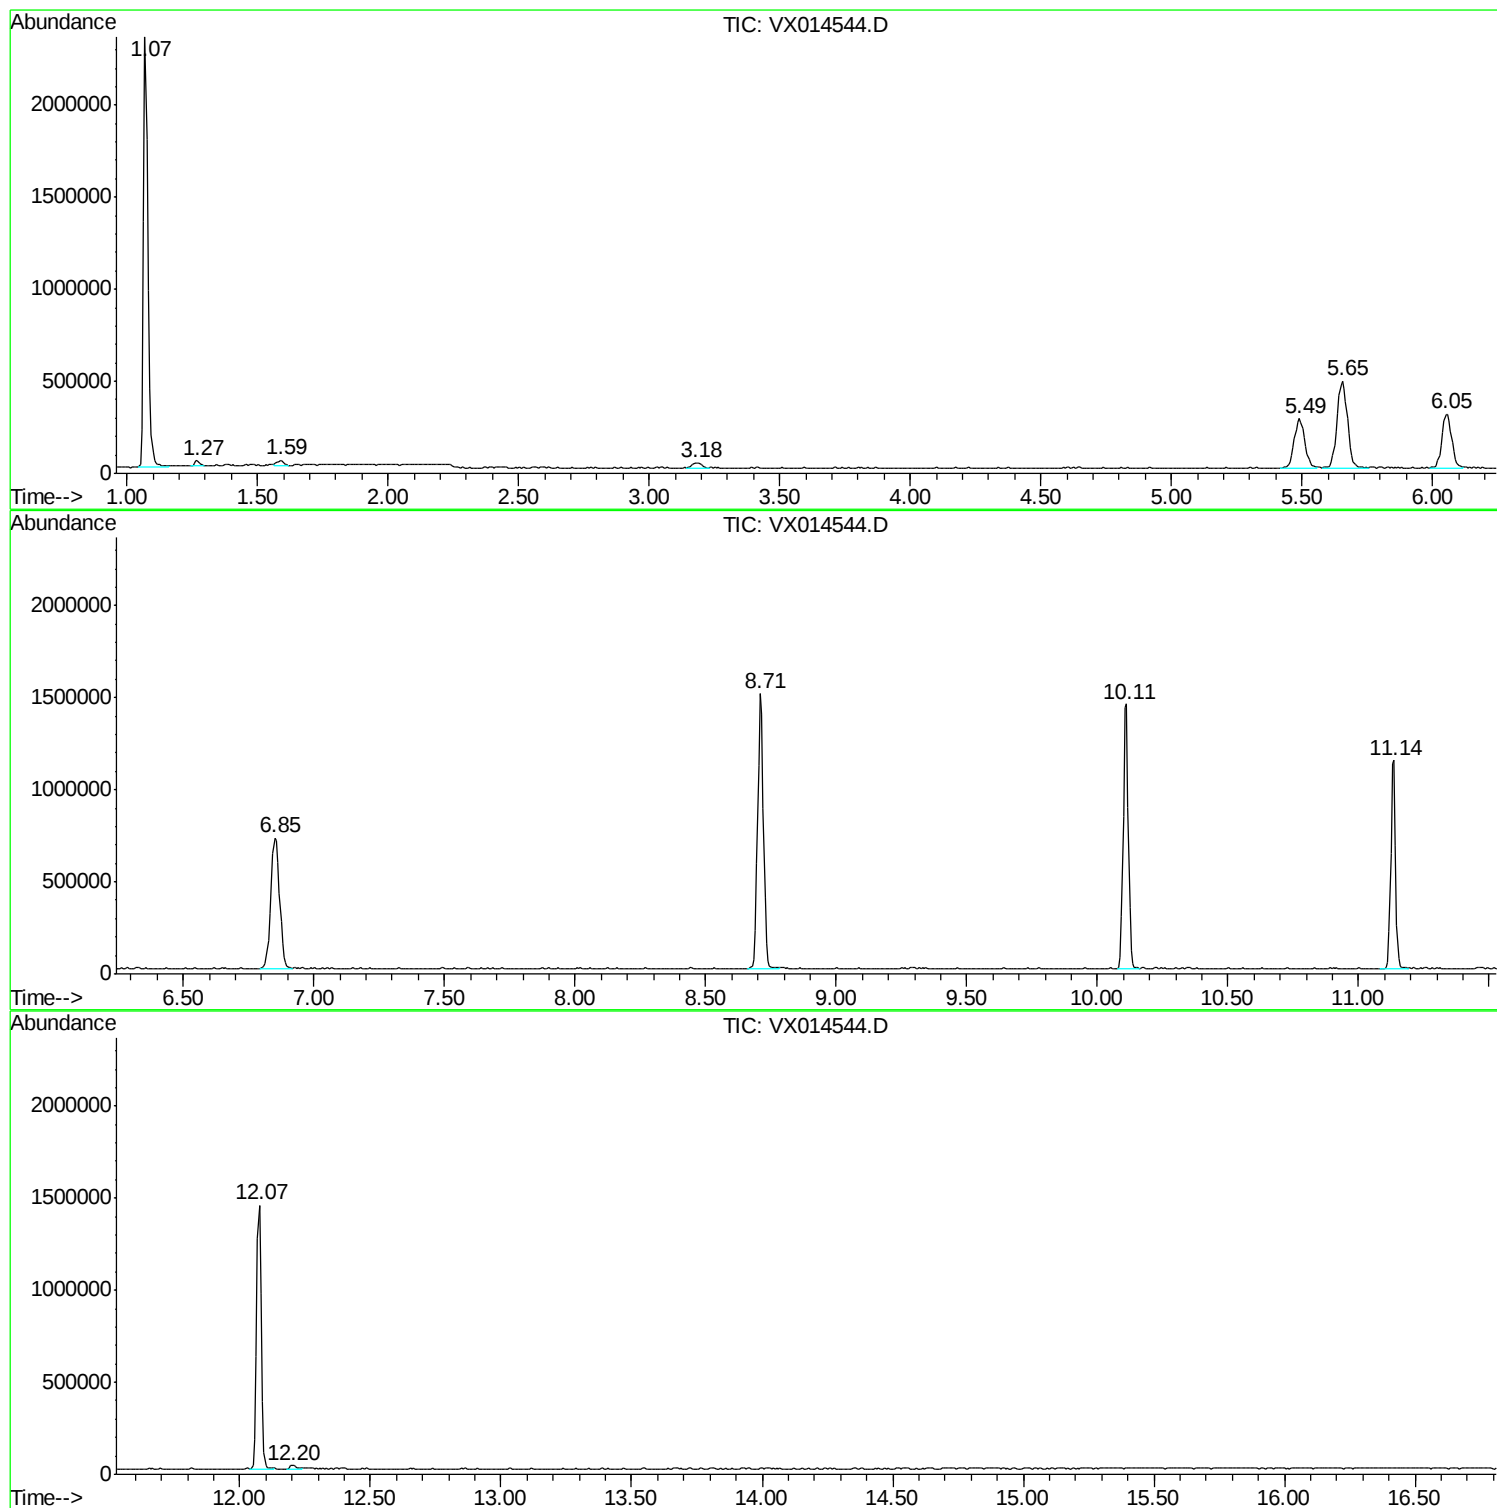

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX011020\
Data File : VX014544.D
Acq On : 10 Jan 2020 17:55
Operator : JC/SP
Sample : L1080-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX011020\
Data File : VX014544.D
Acq On : 10 Jan 2020 17:55
Operator : JC/SP
Sample : L1080-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc