


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX011020\
 Data File : VX014521.D
 Acq On : 10 Jan 2020 08:16
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M
 Title : SW846 8260
 Last Update : Tue Jan 07 15:54:41 2020

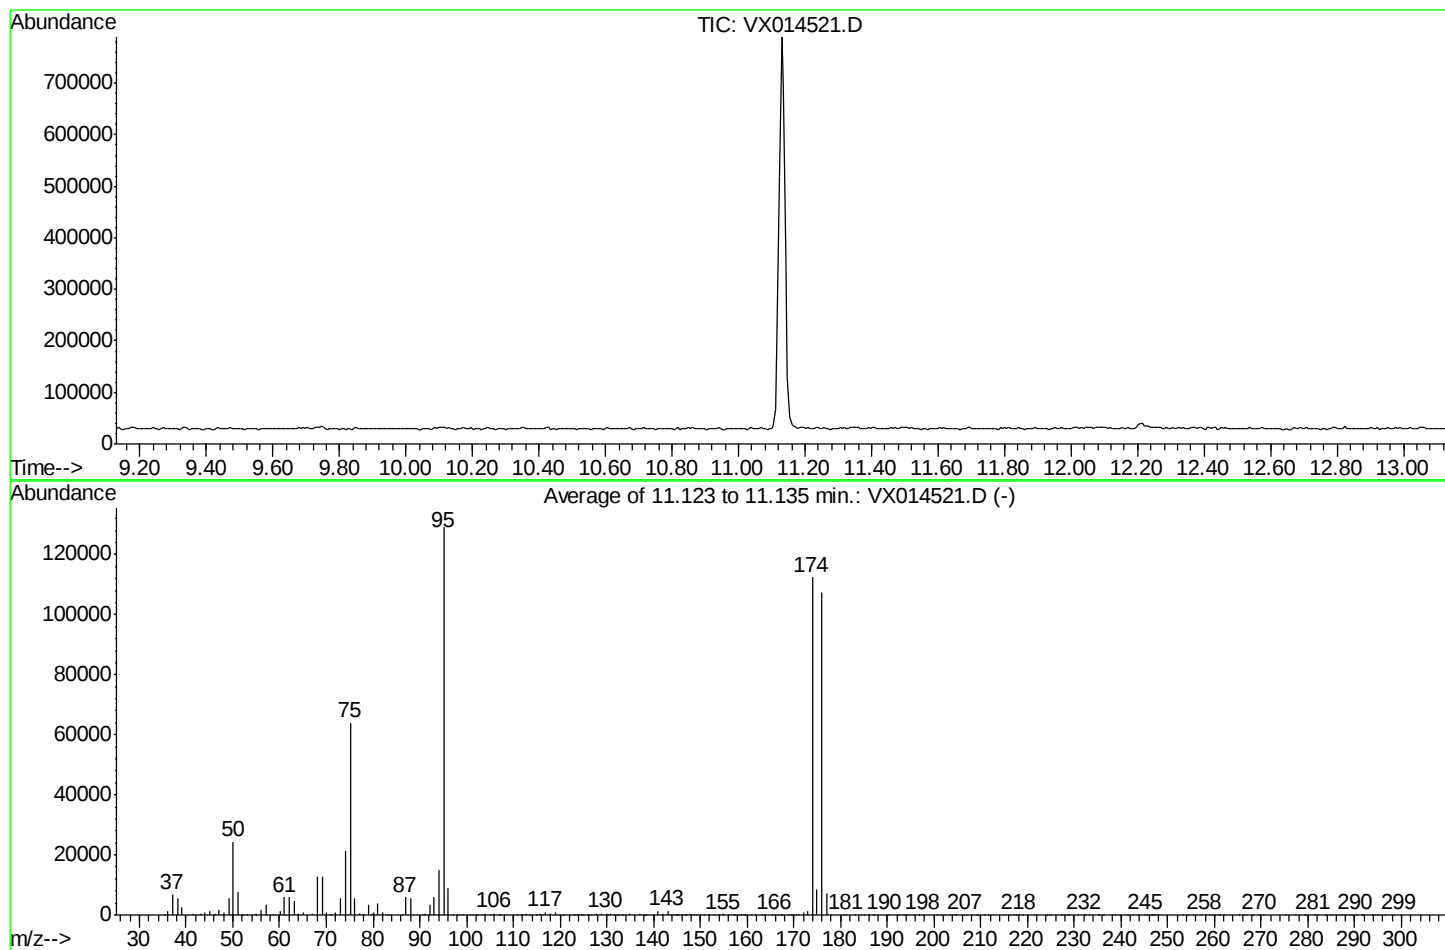

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	24301	PASS
75	95	30	60	49.7	64139	PASS
95	95	100	100	100.0	129056	PASS
96	95	5	9	7.0	9089	PASS
173	174	0.00	2	1.2	1340	PASS
174	95	50	100	87.0	112320	PASS
175	174	5	9	7.7	8649	PASS
176	174	95	101	95.5	107266	PASS
177	176	5	9	6.7	7170	PASS