



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011023\
Data File : VX033675.D
Acq On : 10 Jan 2023 08:24
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X010423W.M
Title : SW846 8260
Last Update : Thu Jan 05 04:43:25 2023

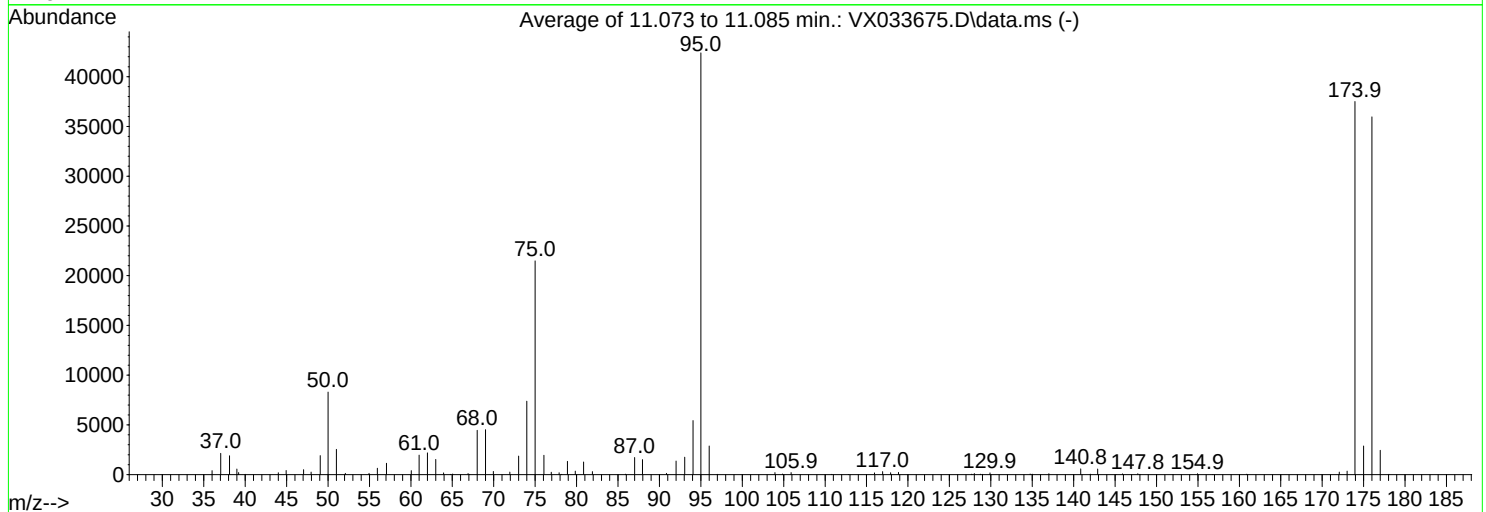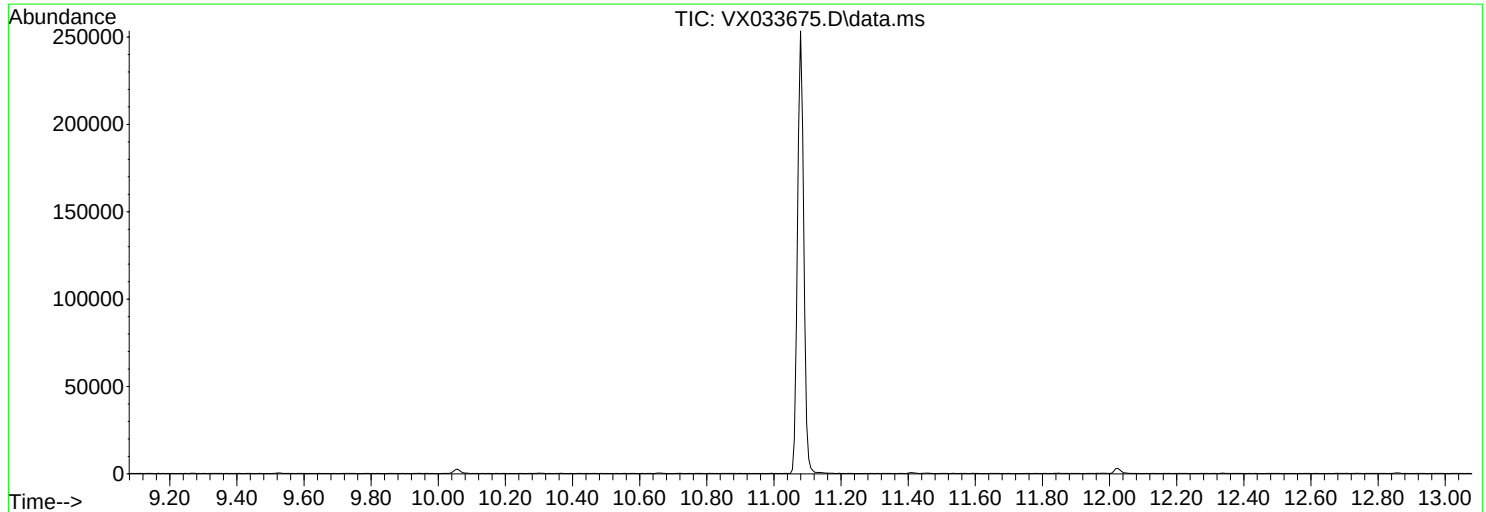

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	8306	PASS
75	95	30	60	50.7	21480	PASS
95	95	100	100	100.0	42397	PASS
96	95	5	9	6.8	2878	PASS
173	174	0.00	2	0.9	350	PASS
174	95	50	100	88.5	37512	PASS
175	174	5	9	7.7	2873	PASS
176	174	95	101	95.9	35957	PASS
177	176	5	9	6.8	2449	PASS