

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011024\
 Data File : VX039706.D
 Acq On : 10 Jan 2024 16:08
 Operator : JC/MD
 Sample : P1098-03 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 AUD-1311

Quant Time: Jan 11 04:00:37 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 11 03:51:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	83776	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	166569	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	172308	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	83069	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	67329	47.977	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	95.960%
35) Dibromofluoromethane	5.385	113	54533	48.607	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.220%
50) Toluene-d8	8.647	98	208371	49.244	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.480%
62) 4-Bromofluorobenzene	11.079	95	89742	54.236	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	108.480%


Target Compounds				Qvalue		
5) Bromomethane	1.612	94	134	0.201	ug/l #	54
11) Tert butyl alcohol	2.941	59	746	2.042	ug/l #	78
13) Acrolein	2.160	56	20	Below Cal	#	14
15) Acrylonitrile	3.069	53	170	0.225	ug/l #	74
16) Acetone	2.380	43	1226	1.553	ug/l #	88
17) Carbon Disulfide	2.514	76	1138	0.393	ug/l #	92
20) Methylene Chloride	2.794	84	665	0.557	ug/l #	88
21) trans-1,2-Dichloroethene	3.093	96	748	0.705	ug/l #	94
31) Cyclohexane	5.550	56	2461	1.329	ug/l #	24
36) 1,1-Dichloropropene	5.550	75	7796	4.464	ug/l #	47
38) Carbon Tetrachloride	5.550	117	9271	5.796	ug/l #	15
44) Trichloroethene	7.141	130	439	0.362	ug/l	58
46) Dibromomethane	7.592	93	268	0.293	ug/l #	49
52) Toluene	8.720	92	811	0.275	ug/l #	72
59) 2-Hexanone	9.445	43	425	0.228	ug/l #	61
65) Chlorobenzene	10.079	112	1649	0.459	ug/l	93
67) Ethyl Benzene	10.195	91	1649	0.247	ug/l	95
68) m/p-Xylenes	10.299	106	912	0.372	ug/l	97
69) o-Xylene	10.646	106	722	0.298	ug/l	87
70) Styrene	10.659	104	1177	0.297	ug/l	91
76) 1,2,3-Trichloropropane	11.079	75	48899	22.705	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	48899	65.661	ug/l #	5
84) 1,2,4-Trimethylbenzene	11.756	105	1216	0.217	ug/l	93
87) 1,3-Dichlorobenzene	11.969	146	690	0.244	ug/l #	82
88) 1,4-Dichlorobenzene	12.043	146	2015	0.691	ug/l #	42
89) n-Butylbenzene	12.335	91	1549	0.288	ug/l	93
91) 1,2-Dichlorobenzene	12.335	146	1212	0.434	ug/l	97
92) 1,2-Dibromo-3-Chloropr...	12.945	75	220	0.356	ug/l	83
93) 1,2,4-Trichlorobenzene	13.585	180	2014	1.181	ug/l	97
94) Hexachlorobutadiene	13.725	225	1345	1.897	ug/l	94
95) Naphthalene	13.780	128	7015	1.117	ug/l	99
96) 1,2,3-Trichlorobenzene	13.957	180	580	0.337	ug/l	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011024\
Data File : VX039706.D
Acq On : 10 Jan 2024 16:08
Operator : JC/MD
Sample : P1098-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1311

Quant Time: Jan 11 04:00:37 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 11 03:51:26 2024
Response via : Initial Calibration




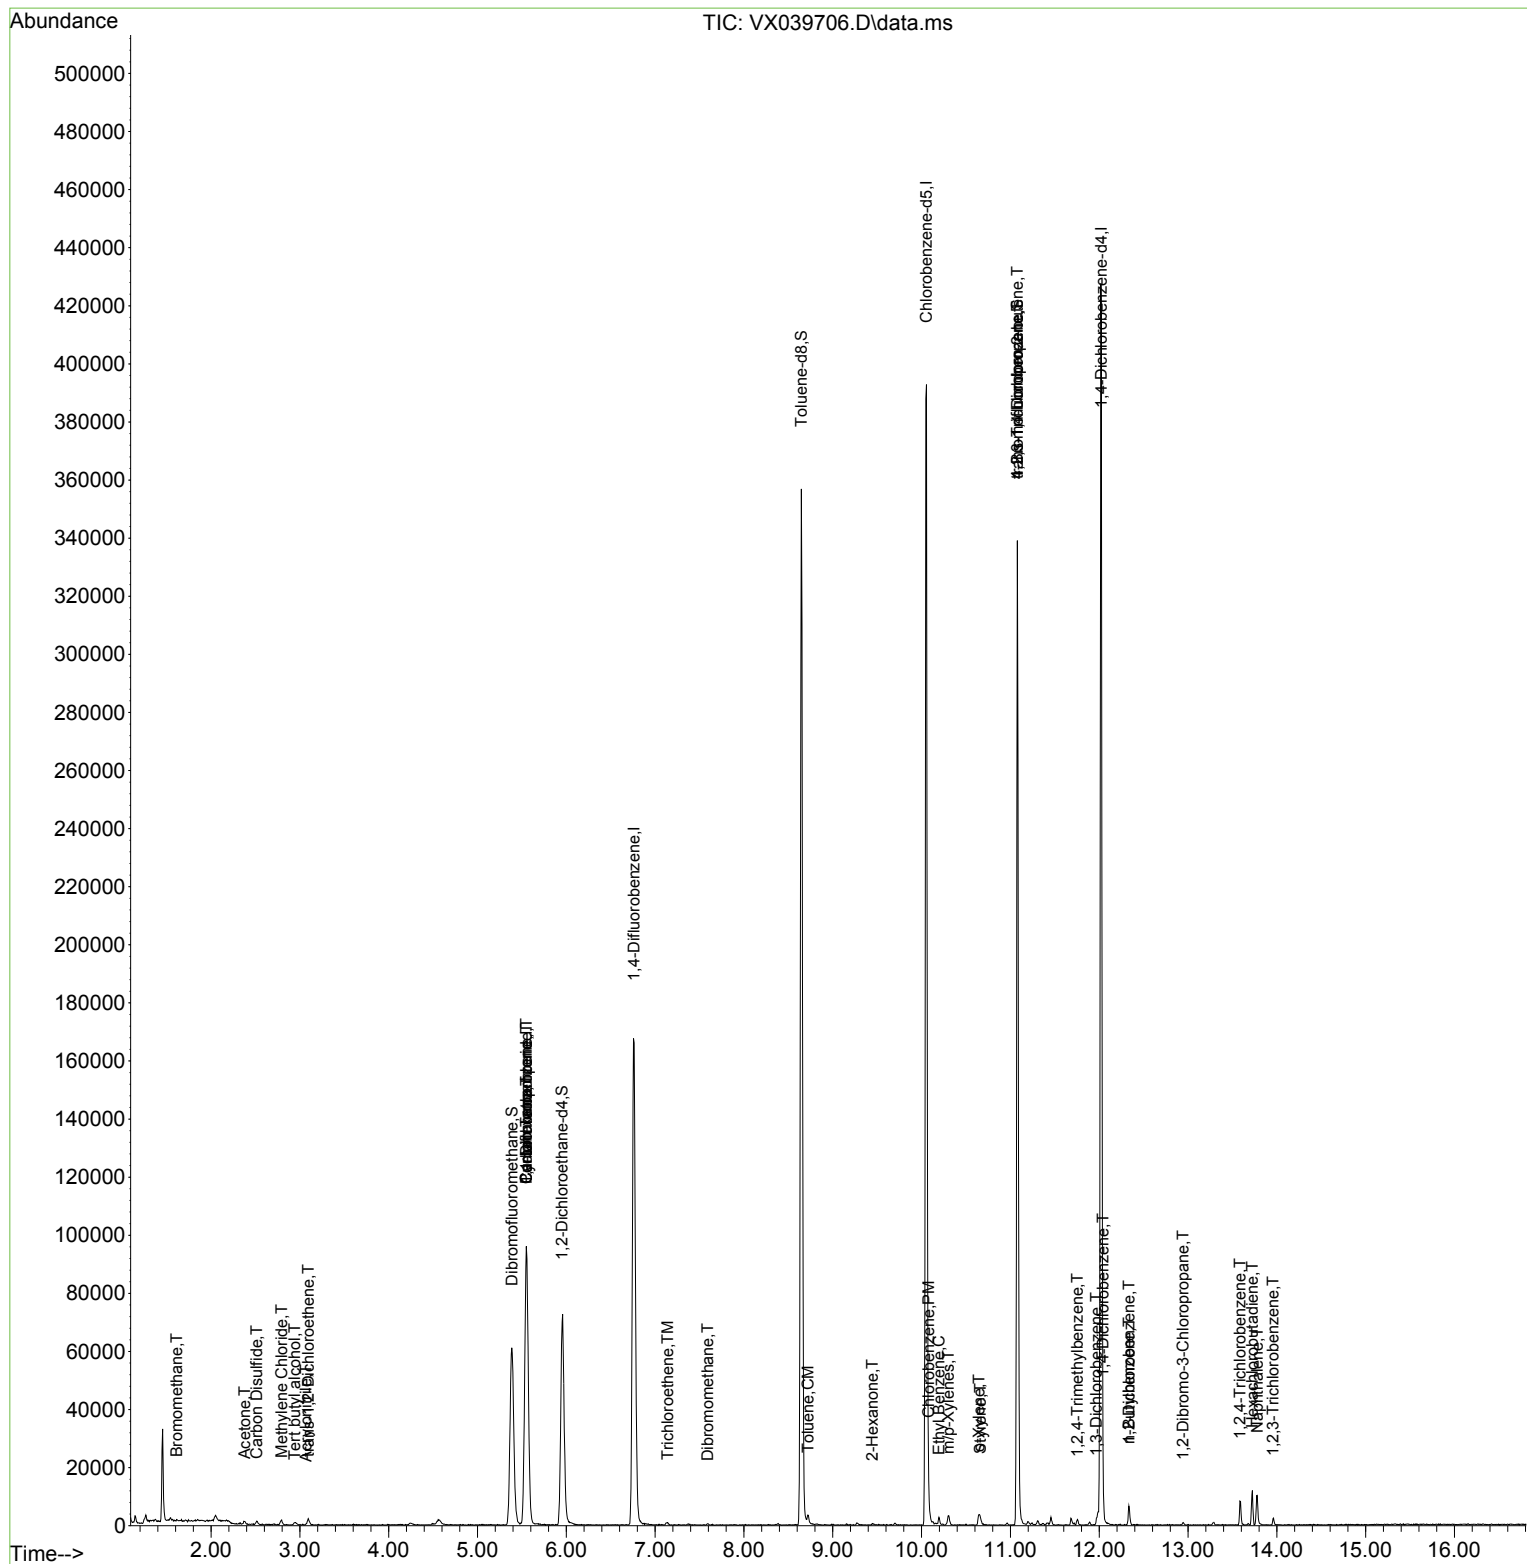




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08




Instrument :
MSVOA_X
ClientSampleId :
AUD-1311


Tgt Ion:168 Resp: 83776
Ion Ratio Lower Upper
168 100
99 63.1 56.6 85.0

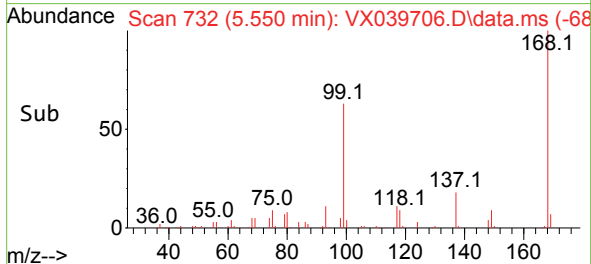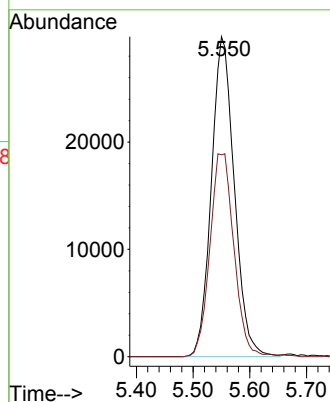

#5
Bromomethane
Concen: 0.201 ug/l
RT: 1.612 min Scan# 86
Delta R.T. 0.012 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08

Tgt Ion: 94 Resp: 134
Ion Ratio Lower Upper
94 100
96 49.3 74.6 111.8#


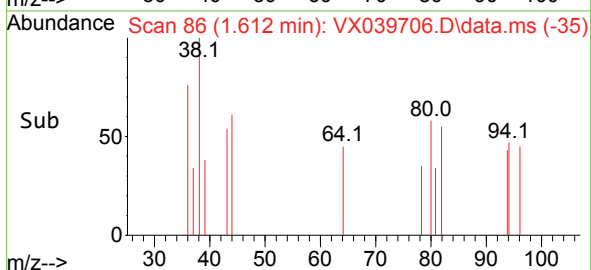




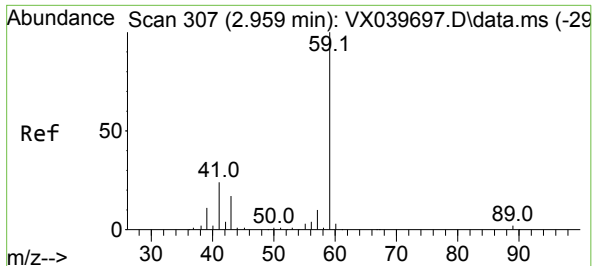

#11
Tert butyl alcohol
Concen: 2.042 ug/l
RT: 2.941 min Scan# 30
Delta R.T. -0.018 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08




Instrument :
MSVOA_X
ClientSampleId :
AUD-1311


Tgt Ion: 59 Resp: 746
Ion Ratio Lower Upper
59 100
57 0.0 6.0 9.0#

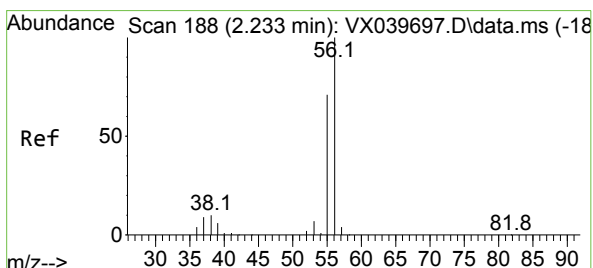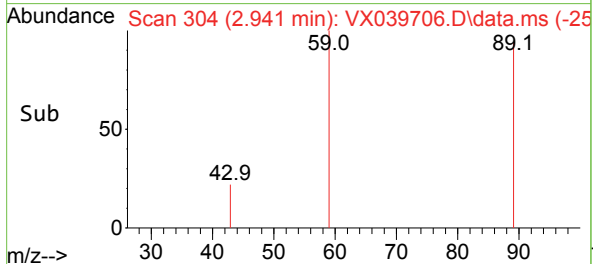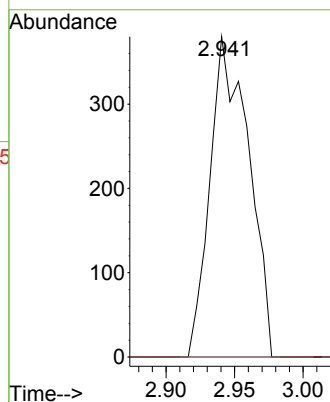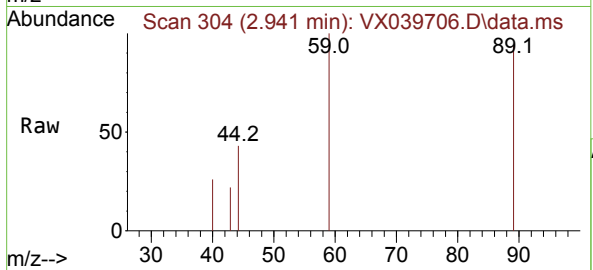

#13
Acrolein
Concen: Below Cal
RT: 2.160 min Scan# 176
Delta R.T. -0.073 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08

Tgt Ion: 56 Resp: 20
Ion Ratio Lower Upper
56 100
55 0.0 57.1 85.7#


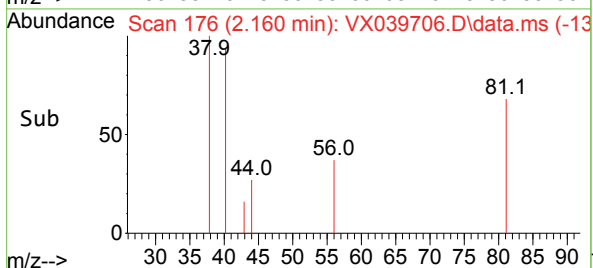

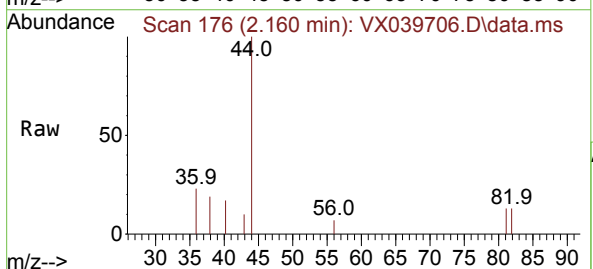




#15
Acrylonitrile
Concen: 0.225 ug/l
RT: 3.069 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08




Instrument :
MSVOA_X
ClientSampleId :
AUD-1311


Tgt Ion: 53 Resp: 170
Ion Ratio Lower Upper
53 100
52 73.5 66.0 99.0
51 0.0 29.8 44.6#

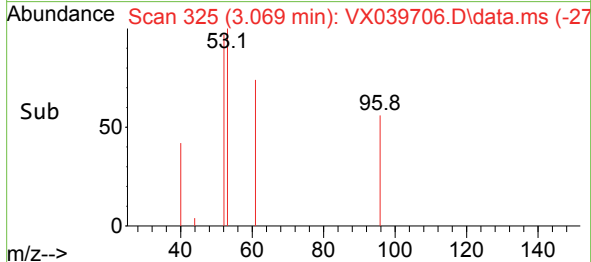

#16
Acetone
Concen: 1.553 ug/l
RT: 2.380 min Scan# 212
Delta R.T. 0.000 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08

Tgt Ion: 43 Resp: 1226
Ion Ratio Lower Upper
43 100
58 33.7 21.9 32.9#

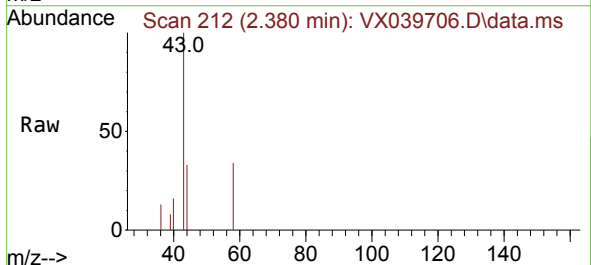



#17

Carbon Disulfide

Concen: 0.393 ug/l

RT: 2.514 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX039706.D

Acq: 10 Jan 2024 16:08

Instrument :

MSVOA_X

ClientSampleId :





AUD-1311

Tgt Ion: 76 Resp: 1138

Ion Ratio Lower Upper

76 100

78 11.8 7.0 10.6#

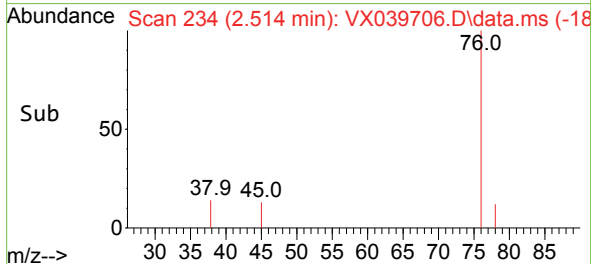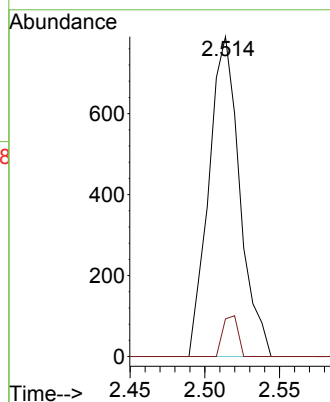

#20

Methylene Chloride

Concen: 0.557 ug/l

RT: 2.794 min Scan# 280

Delta R.T. 0.006 min

Lab File: VX039706.D

Acq: 10 Jan 2024 16:08

Tgt Ion: 84 Resp: 665




Ion Ratio Lower Upper


84 100

49 146.1 103.6 155.4

51 31.5 33.8 50.6#

86 59.1 49.4 74.0


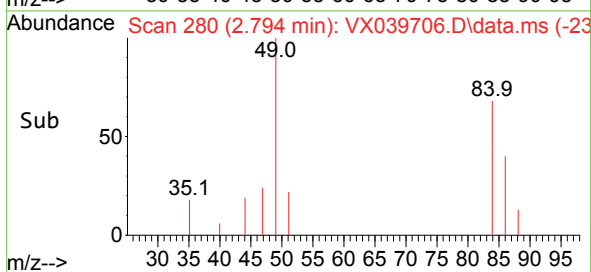






#21
trans-1,2-Dichloroethene
Concen: 0.705 ug/l
RT: 3.093 min Scan# 31
Delta R.T. 0.000 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08




Instrument :
MSVOA_X
ClientSampleId :
AUD-1311


Tgt Ion: 96 Resp: 748
Ion Ratio Lower Upper
96 100
61 149.2 119.2 178.8
98 77.2 48.7 73.1#

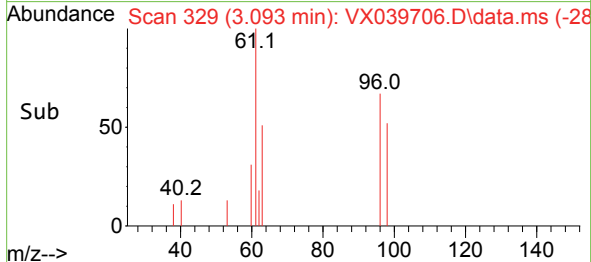

#31
Cyclohexane
Concen: 1.329 ug/l
RT: 5.550 min Scan# 732
Delta R.T. 0.079 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08

Tgt Ion: 56 Resp: 2461
Ion Ratio Lower Upper
56 100
69 157.1 23.4 35.2#
84 99.0 65.9 98.9#

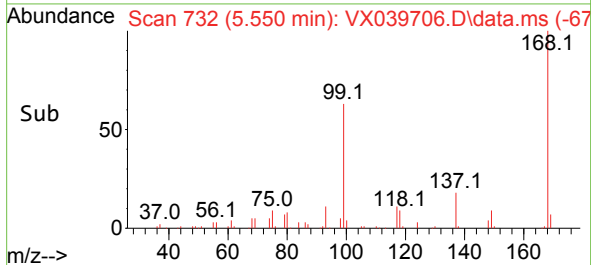



#33

1,2-Dichloroethane-d4

Concen: 47.977 ug/l

RT: 5.952 min Scan# 798

Delta R.T. 0.000 min

Lab File: VX039706.D

Acq: 10 Jan 2024 16:08

Instrument :

MSVOA_X

ClientSampleId :





AUD-1311

Tgt Ion: 65 Resp: 67329

Ion Ratio Lower Upper

65 100

67 53.5 0.0 100.2

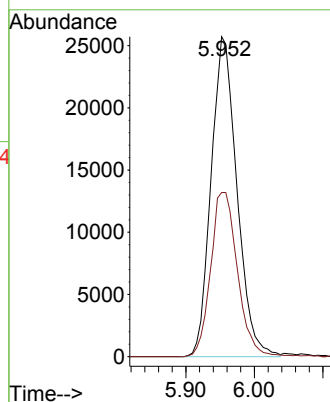

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.006 min

Lab File: VX039706.D

Acq: 10 Jan 2024 16:08




Tgt Ion: 114 Resp: 166569


Ion Ratio Lower Upper

114 100

63 22.0 0.0 45.0

88 17.0 0.0 36.6


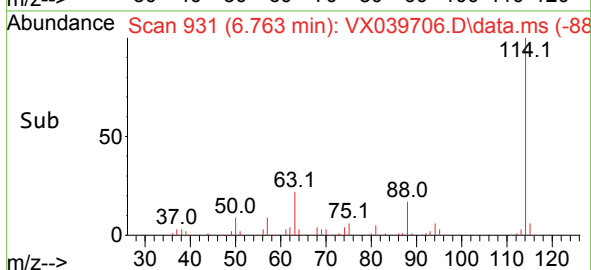






#35
Dibromofluoromethane
Concen: 48.607 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08




Instrument :
MSVOA_X
ClientSampleId :
AUD-1311


Tgt Ion:113 Resp: 54533
Ion Ratio Lower Upper
113 100
111 103.1 82.9 124.3
192 16.2 13.3 19.9

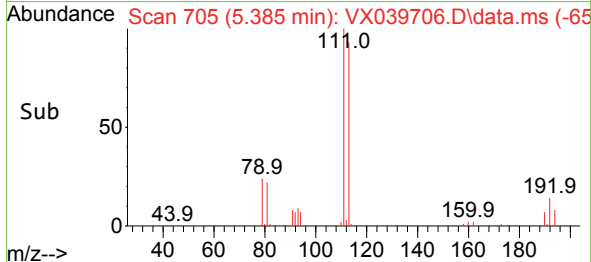

#36
1,1-Dichloropropene
Concen: 4.464 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.140 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08


Tgt Ion: 75 Resp: 7796
Ion Ratio Lower Upper
75 100
110 5.0 17.0 50.9#
77 0.0 24.7 37.1#

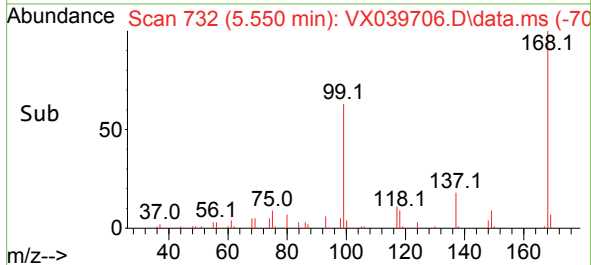






#38
Carbon Tetrachloride
Concen: 5.796 ug/l
RT: 5.550 min Scan# 711
Delta R.T. -0.128 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08

Instrument :
MSVOA_X
ClientSampleId :
AUD-1311







Tgt Ion:117 Resp: 9271
Ion Ratio Lower Upper
117 100
119 4.8 78.2 117.2#
121 0.0 24.4 36.6#

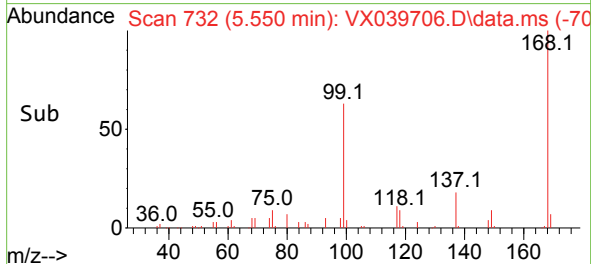

#44
Trichloroethene
Concen: 0.362 ug/l
RT: 7.141 min Scan# 993
Delta R.T. 0.018 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08

Tgt Ion:130 Resp: 439
Ion Ratio Lower Upper
130 100
95 60.2 0.0 204.4









#46
Dibromomethane
Concen: 0.293 ug/l
RT: 7.592 min Scan# 1065
Delta R.T. 0.012 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08




Instrument :
MSVOA_X
ClientSampleId :
AUD-1311


Tgt Ion: 93 Resp: 268
Ion Ratio Lower Upper
93 100
95 59.0 66.6 100.0#
174 18.7 69.4 104.0#

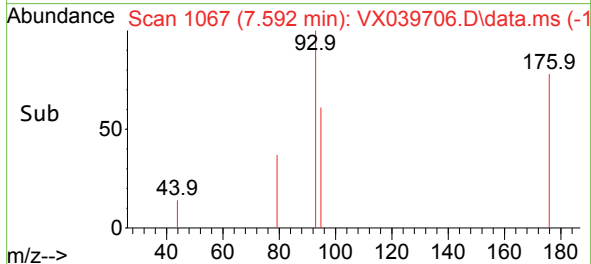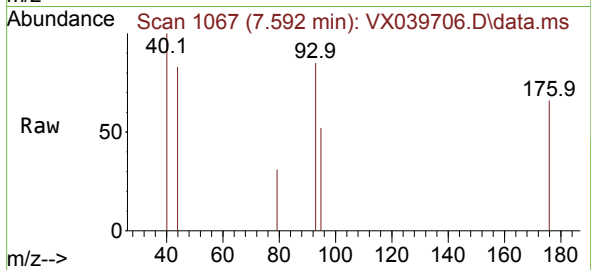

#50
Toluene-d8
Concen: 49.244 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08

Tgt Ion: 98 Resp: 208371
Ion Ratio Lower Upper
98 100
100 63.5 53.1 79.7





#52

Toluene

Concen: 0.275 ug/l

RT: 8.720 min Scan# 1371

Delta R.T. 0.006 min

Lab File: VX039706.D

Acq: 10 Jan 2024 16:08

Instrument :

MSVOA_X

ClientSampleId :





AUD-1311

Tgt Ion: 92 Resp: 811

Ion Ratio Lower Upper

92 100

91 206.3 134.2 201.2#

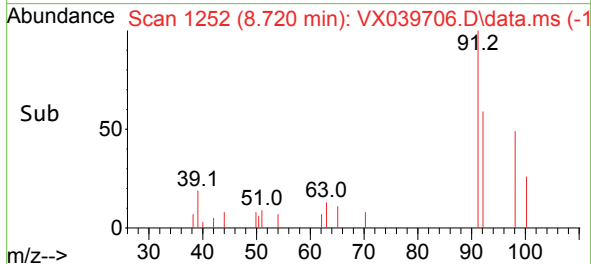

#59

2-Hexanone

Concen: 0.228 ug/l

RT: 9.445 min Scan# 1371

Delta R.T. 0.018 min

Lab File: VX039706.D




Acq: 10 Jan 2024 16:08


Tgt Ion: 43 Resp: 425

Ion Ratio Lower Upper

43 100

58 24.9 26.2 78.5#


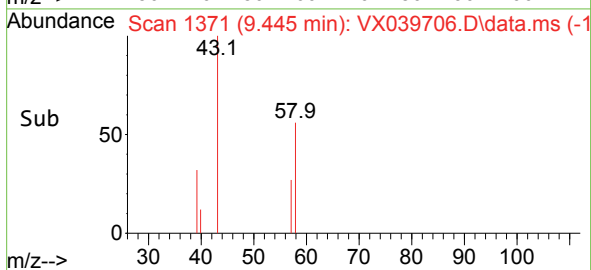






#62
4-Bromofluorobenzene
Concen: 54.236 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08




Instrument :
MSVOA_X
ClientSampleId :
AUD-1311


Tgt Ion: 95 Resp: 89742
Ion Ratio Lower Upper
95 100
174 67.8 0.0 135.6
176 65.3 0.0 131.0

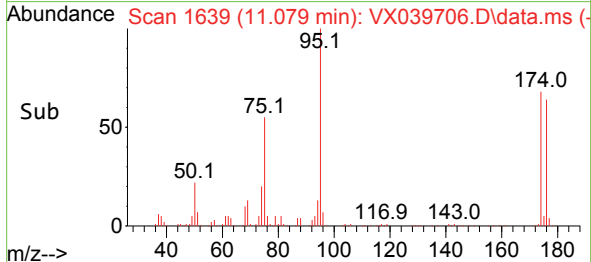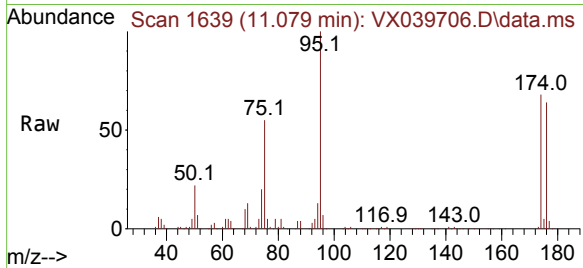

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08

Tgt Ion: 117 Resp: 172308
Ion Ratio Lower Upper
117 100
82 57.8 46.2 69.4
119 32.0 25.5 38.3




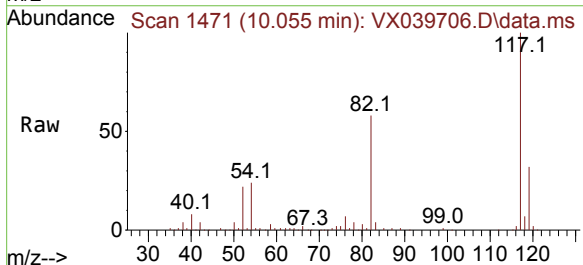




#65
Chlorobenzene
Concen: 0.459 ug/l
RT: 10.079 min Scan# 1475
Delta R.T. 0.000 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08




Instrument :
MSVOA_X
ClientSampleId :
AUD-1311


Tgt Ion:112 Resp: 1649
Ion Ratio Lower Upper
112 100
114 28.1 25.7 38.5

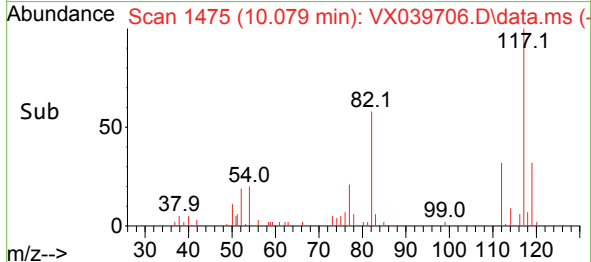

#67
Ethyl Benzene
Concen: 0.247 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08

Tgt Ion: 91 Resp: 1649
Ion Ratio Lower Upper
91 100
106 28.6 24.9 37.3




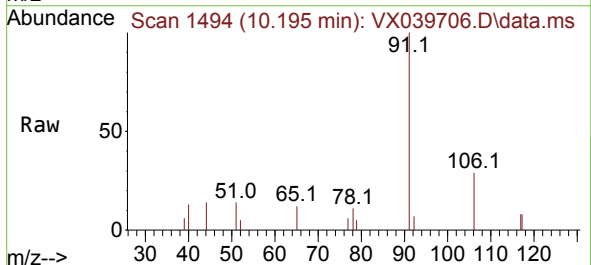




#68
m/p-Xylenes
Concen: 0.372 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08




Instrument :
MSVOA_X
ClientSampleId :
AUD-1311


Tgt Ion:106 Resp: 912
Ion Ratio Lower Upper
106 100
91 202.7 165.5 248.3

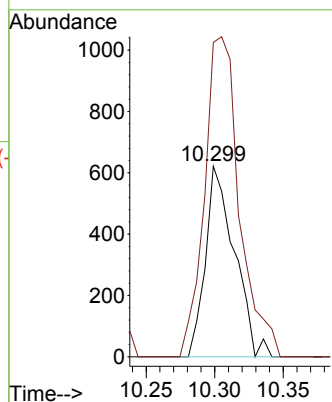

#69
o-Xylene
Concen: 0.298 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.006 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08

Tgt Ion:106 Resp: 722
Ion Ratio Lower Upper
106 100
91 239.2 108.9 326.8

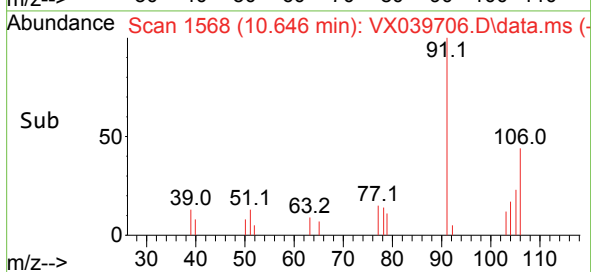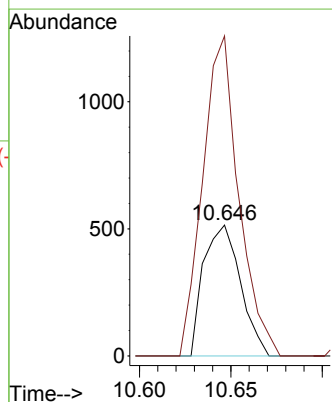

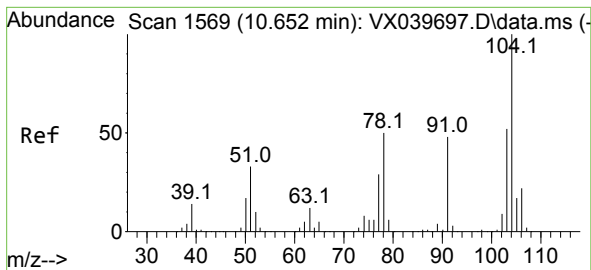

#70

Styrene

Concen: 0.297 ug/l

RT: 10.659 min Scan# 1177

Delta R.T. 0.006 min

Lab File: VX039706.D

Acq: 10 Jan 2024 16:08

Instrument :

MSVOA_X

ClientSampleId :

AUD-1311





Tgt Ion:104 Resp: 1177

Ion Ratio Lower Upper

104 100

78 60.0 43.6 65.4

103 61.7 43.6 65.4

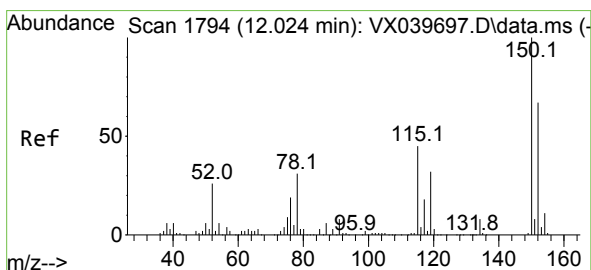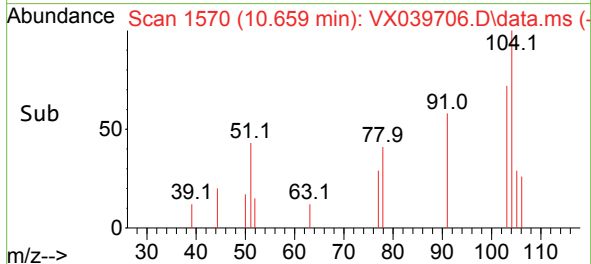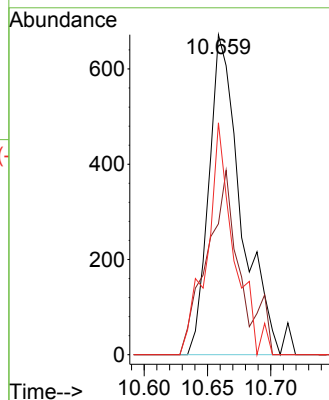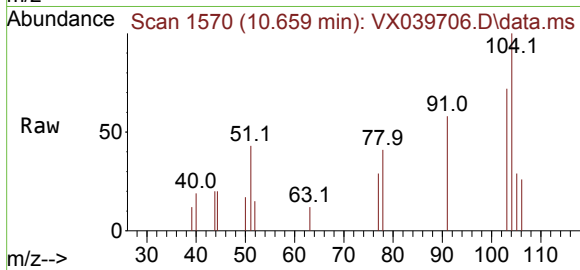

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX039706.D

Acq: 10 Jan 2024 16:08




Tgt Ion:152 Resp: 83069


Ion Ratio Lower Upper

152 100

115 65.2 43.3 129.9

150 158.3 0.0 345.0


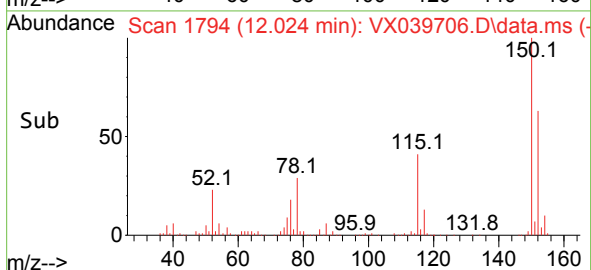
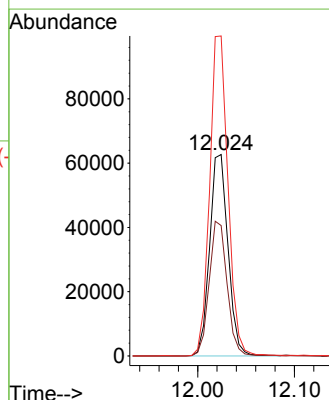
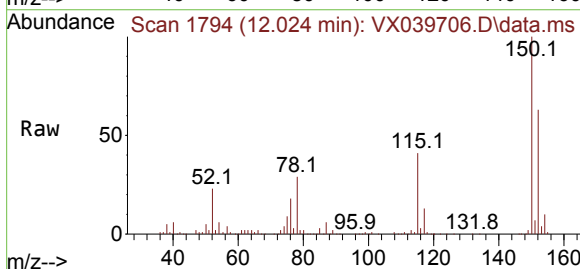




#76
1,2,3-Trichloropropane
Concen: 22.705 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08




Instrument :
MSVOA_X
ClientSampleId :
AUD-1311


Tgt Ion: 75 Resp: 48899
Ion Ratio Lower Upper
75 100
77 0.9 19.1 57.5#

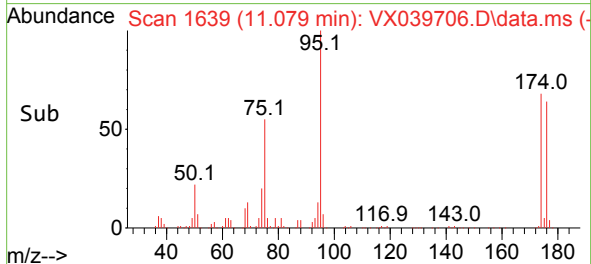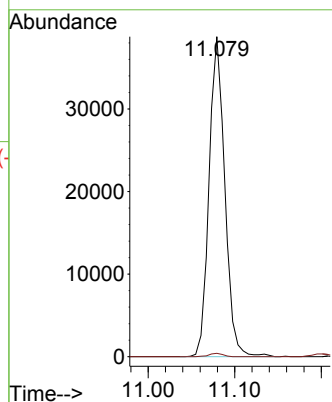

#81
trans-1,4-Dichloro-2-butene
Concen: 65.661 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08

Tgt Ion: 75 Resp: 48899
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#





#84

1,2,4-Trimethylbenzene

Concen: 0.217 ug/l

RT: 11.756 min Scan# 1750

Delta R.T. 0.006 min

Lab File: VX039706.D

Acq: 10 Jan 2024 16:08

Instrument :

MSVOA_X

ClientSampleId :





AUD-1311

Tgt Ion:105 Resp: 1216

Ion Ratio Lower Upper

105 100

120 38.1 21.2 63.6

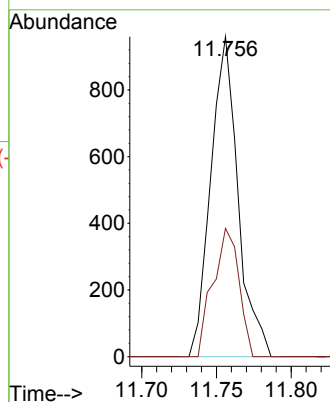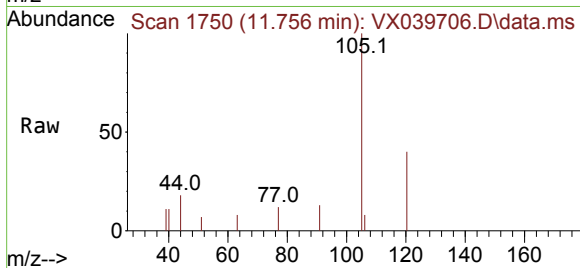

#87

1,3-Dichlorobenzene

Concen: 0.244 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. 0.000 min

Lab File: VX039706.D

Acq: 10 Jan 2024 16:08




Tgt Ion:146 Resp: 690


Ion Ratio Lower Upper

146 100

111 70.6 22.1 66.1#

148 65.2 31.8 95.3


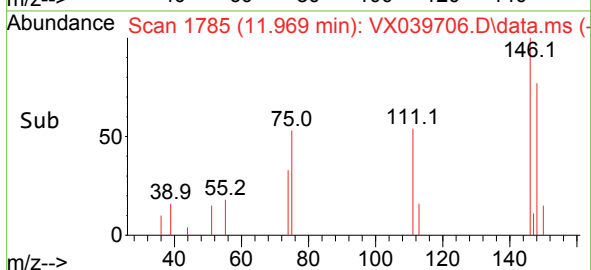

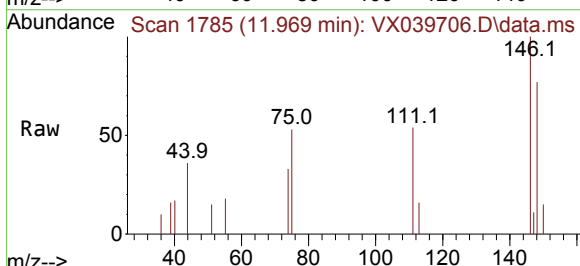




#88
1,4-Dichlorobenzene
Concen: 0.691 ug/l
RT: 12.043 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08




Instrument :
MSVOA_X
ClientSampleId :
AUD-1311


Tgt Ion:146 Resp: 2015
Ion Ratio Lower Upper
146 100
111 115.5 21.3 63.7#
148 79.4 31.8 95.4

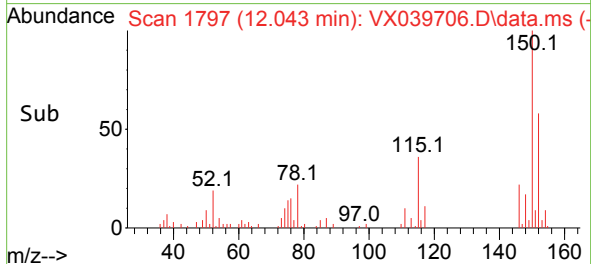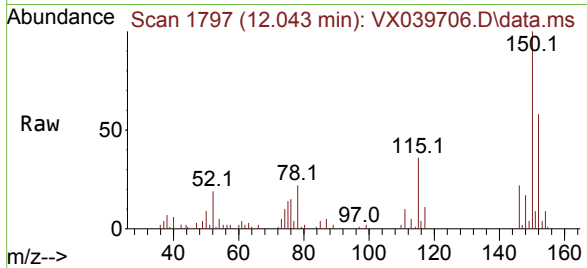

#89
n-Butylbenzene
Concen: 0.288 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.006 min
Lab File: VX039706.D
Acq: 10 Jan 2024 16:08

Tgt Ion: 91 Resp: 1549
Ion Ratio Lower Upper
91 100
92 48.5 27.4 82.0
134 23.6 12.6 37.8

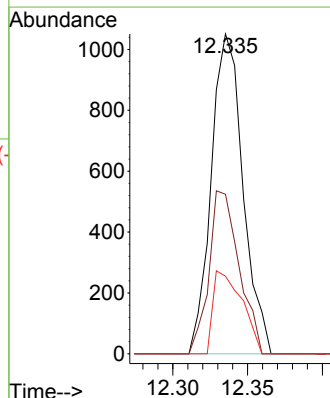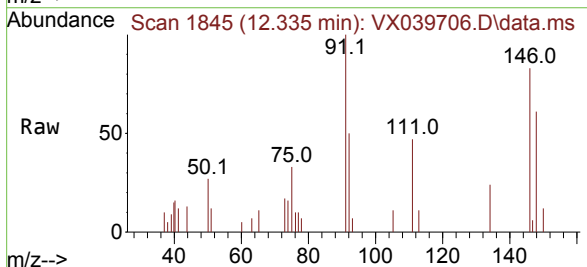

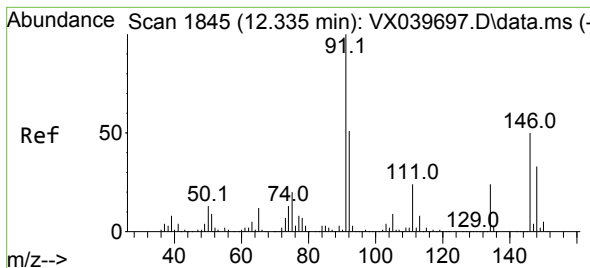

#91

1,2-Dichlorobenzene

Concen: 0.434 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.000 min

Lab File: VX039706.D

Acq: 10 Jan 2024 16:08

Instrument :

MSVOA_X

ClientSampleId :

AUD-1311





Tgt Ion:146 Resp: 1212

Ion Ratio Lower Upper

146 100

111 48.1 22.4 67.0

148 62.0 31.6 95.0

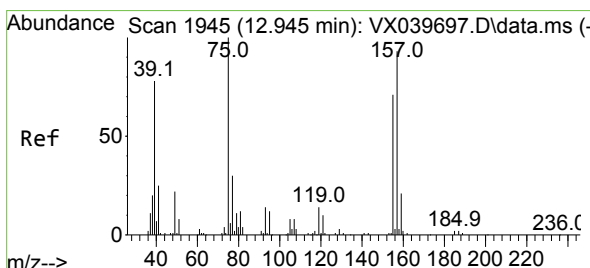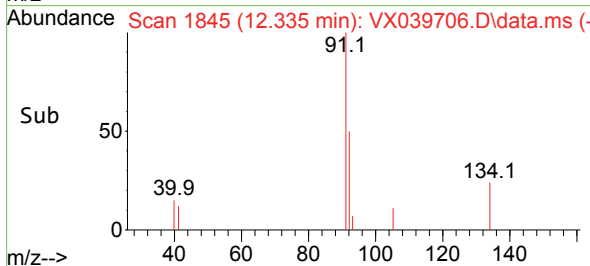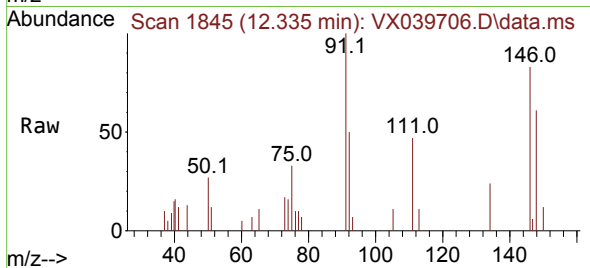

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.356 ug/l

RT: 12.945 min Scan# 1945

Delta R.T. 0.000 min

Lab File: VX039706.D

Acq: 10 Jan 2024 16:08




Tgt Ion: 75 Resp: 220


Ion Ratio Lower Upper

75 100

155 51.4 36.1 108.5

157 80.0 44.9 134.7

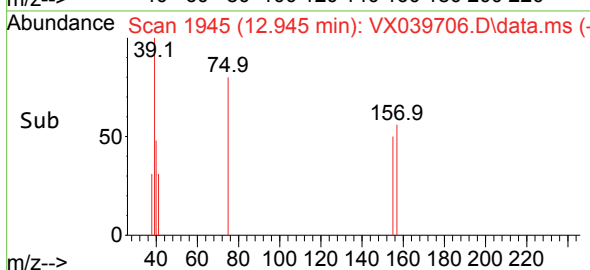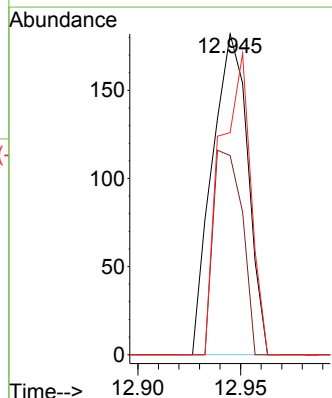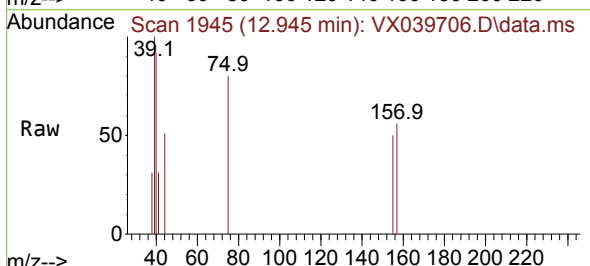



#93

1,2,4-Trichlorobenzene

Concen: 1.181 ug/l

RT: 13.585 min Scan# 2050

Delta R.T. 0.000 min

Lab File: VX039706.D

Acq: 10 Jan 2024 16:08

Instrument :

MSVOA_X

ClientSampleId :

AUD-1311





Tgt Ion:180 Resp: 2014

Ion Ratio Lower Upper

180 100

182 96.4 48.3 144.8

145 29.8 18.0 54.0

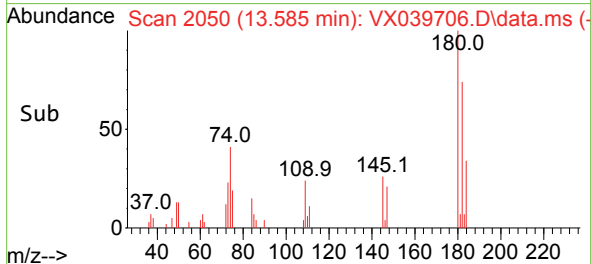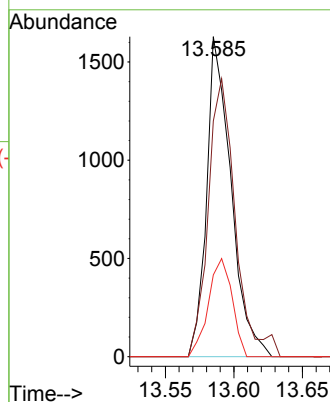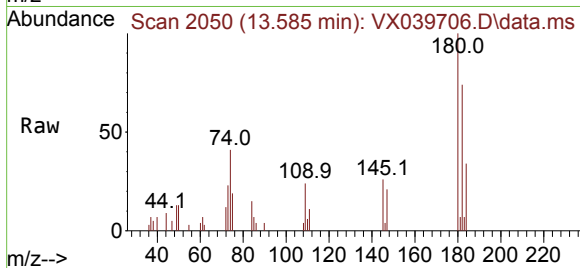

#94

Hexachlorobutadiene

Concen: 1.897 ug/l

RT: 13.725 min Scan# 2073

Delta R.T. 0.000 min

Lab File: VX039706.D

Acq: 10 Jan 2024 16:08




Tgt Ion:225 Resp: 1345


Ion Ratio Lower Upper

225 100

223 65.1 31.1 93.2

227 71.1 32.5 97.5

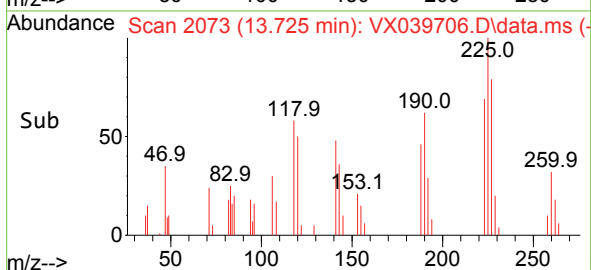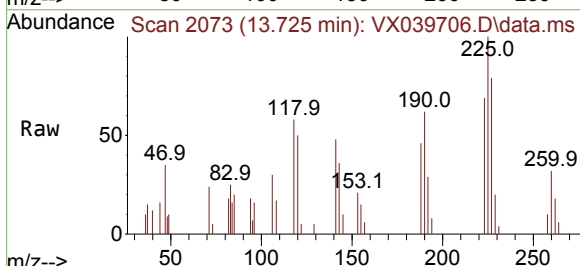



#95

Naphthalene

Concen: 1.117 ug/l

RT: 13.780 min Scan# 2081

Delta R.T. 0.006 min

Lab File: VX039706.D

Acq: 10 Jan 2024 16:08

Instrument :

MSVOA_X

ClientSampleId :

AUD-1311





Tgt Ion:128 Resp: 7015

Ion Ratio Lower Upper

128 100

127 12.9 10.3 15.5

129 10.3 8.8 13.2

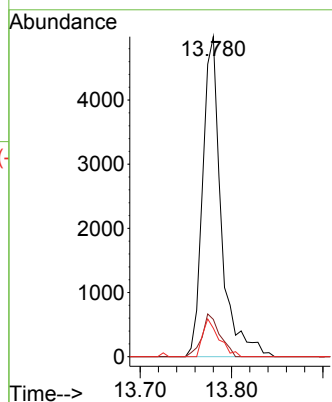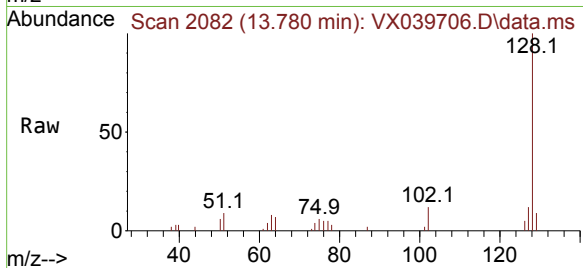

#96

1,2,3-Trichlorobenzene

Concen: 0.337 ug/l

RT: 13.957 min Scan# 2111

Delta R.T. -0.006 min

Lab File: VX039706.D

Acq: 10 Jan 2024 16:08

Tgt Ion:180 Resp: 580

Ion Ratio Lower Upper

180 100

182 112.4 46.9 140.6

145 25.9 17.8 53.5

