



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011024\
Data File : VX039693.D
Acq On : 10 Jan 2024 09:59
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
Title : SW846 8260
Last Update : Thu Jan 11 03:51:26 2024

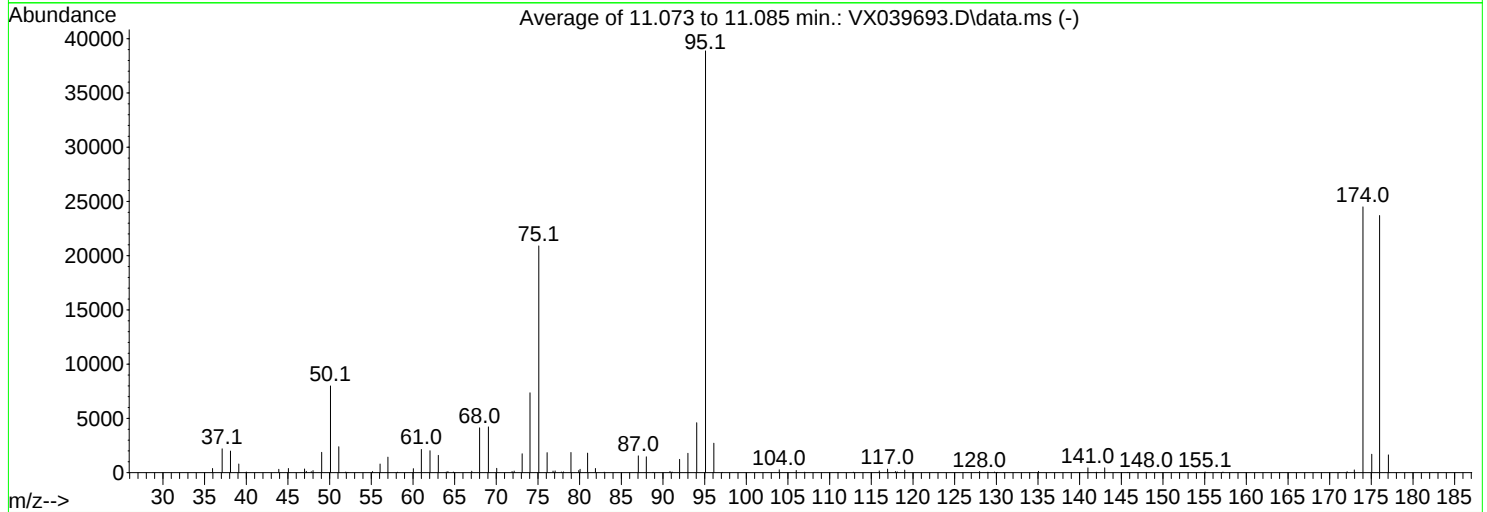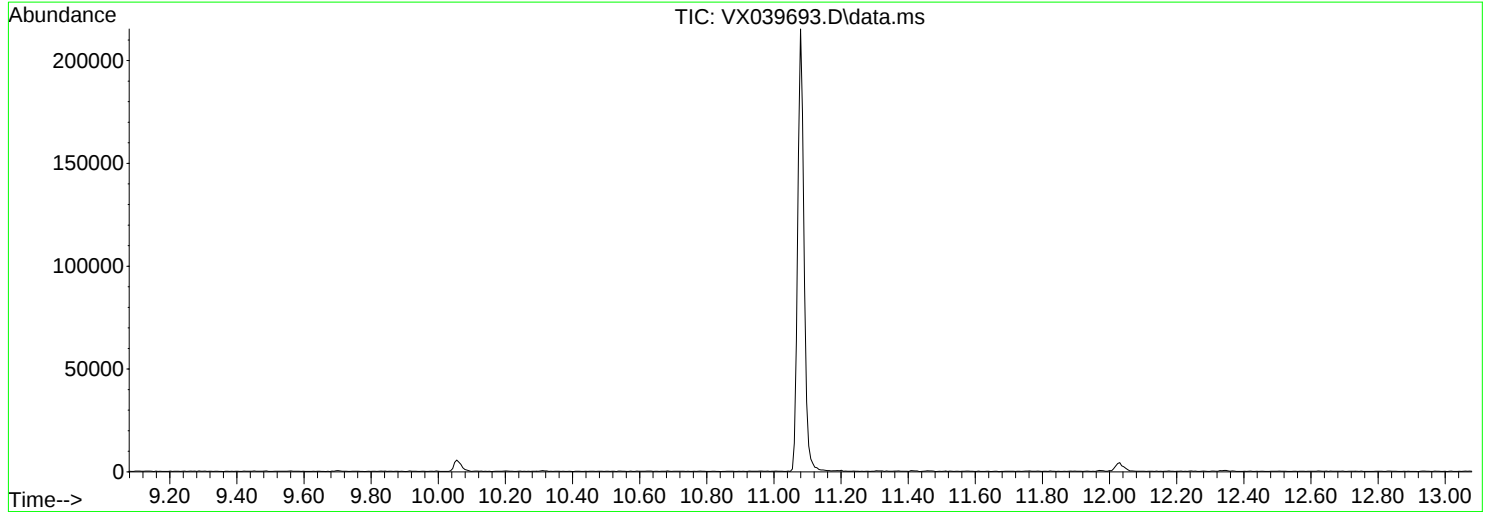

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.6	7997	PASS
75	95	30	60	53.7	20899	PASS
95	95	100	100	100.0	38883	PASS
96	95	5	9	7.0	2719	PASS
173	174	0.00	2	1.0	250	PASS
174	95	50	100	63.0	24493	PASS
175	174	5	9	6.9	1697	PASS
176	174	95	101	96.8	23709	PASS
177	176	5	9	6.9	1636	PASS