


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX011119\
Data File : VX007003.D
Acq On : 11 Jan 2019 10:23
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Title : SW846 8260
Last Update : Tue Jan 08 14:06:59 2019

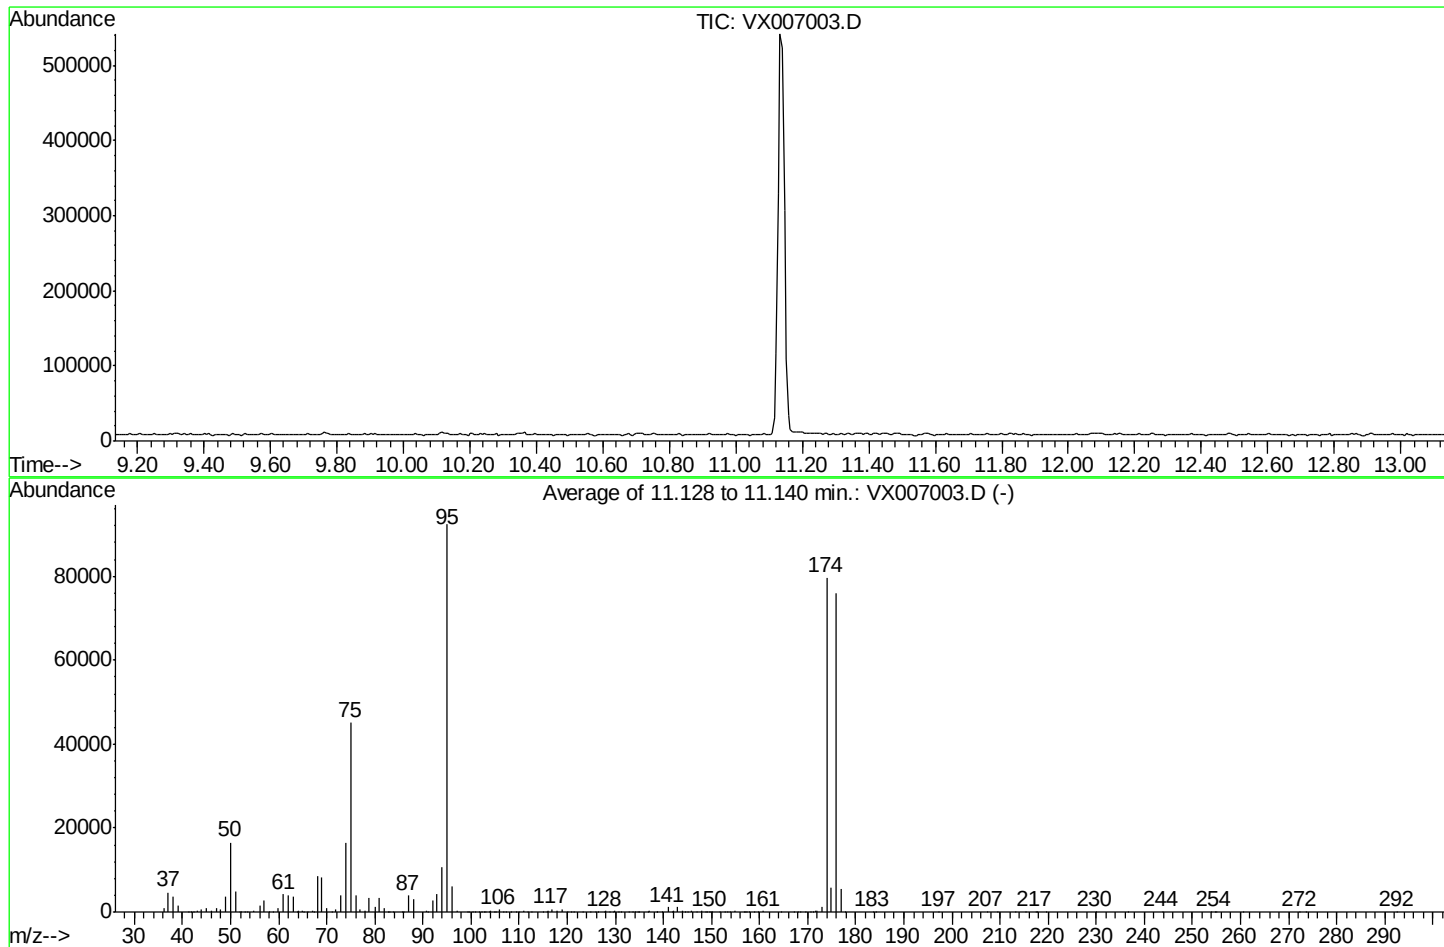

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	16512	PASS
75	95	30	60	48.9	45125	PASS
95	95	100	100	100.0	92354	PASS
96	95	5	9	6.7	6166	PASS
173	174	0.00	2	1.5	1161	PASS
174	95	50	100	86.3	79690	PASS
175	174	5	9	7.4	5859	PASS
176	174	95	101	95.4	76018	PASS
177	176	5	9	7.1	5381	PASS