


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011121\
 Data File : VX020544.D
 Acq On : 11 Jan 2021 09:25
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011121W.M
 Title : SW846 8260
 Last Update : Mon Jan 11 15:05:37 2021

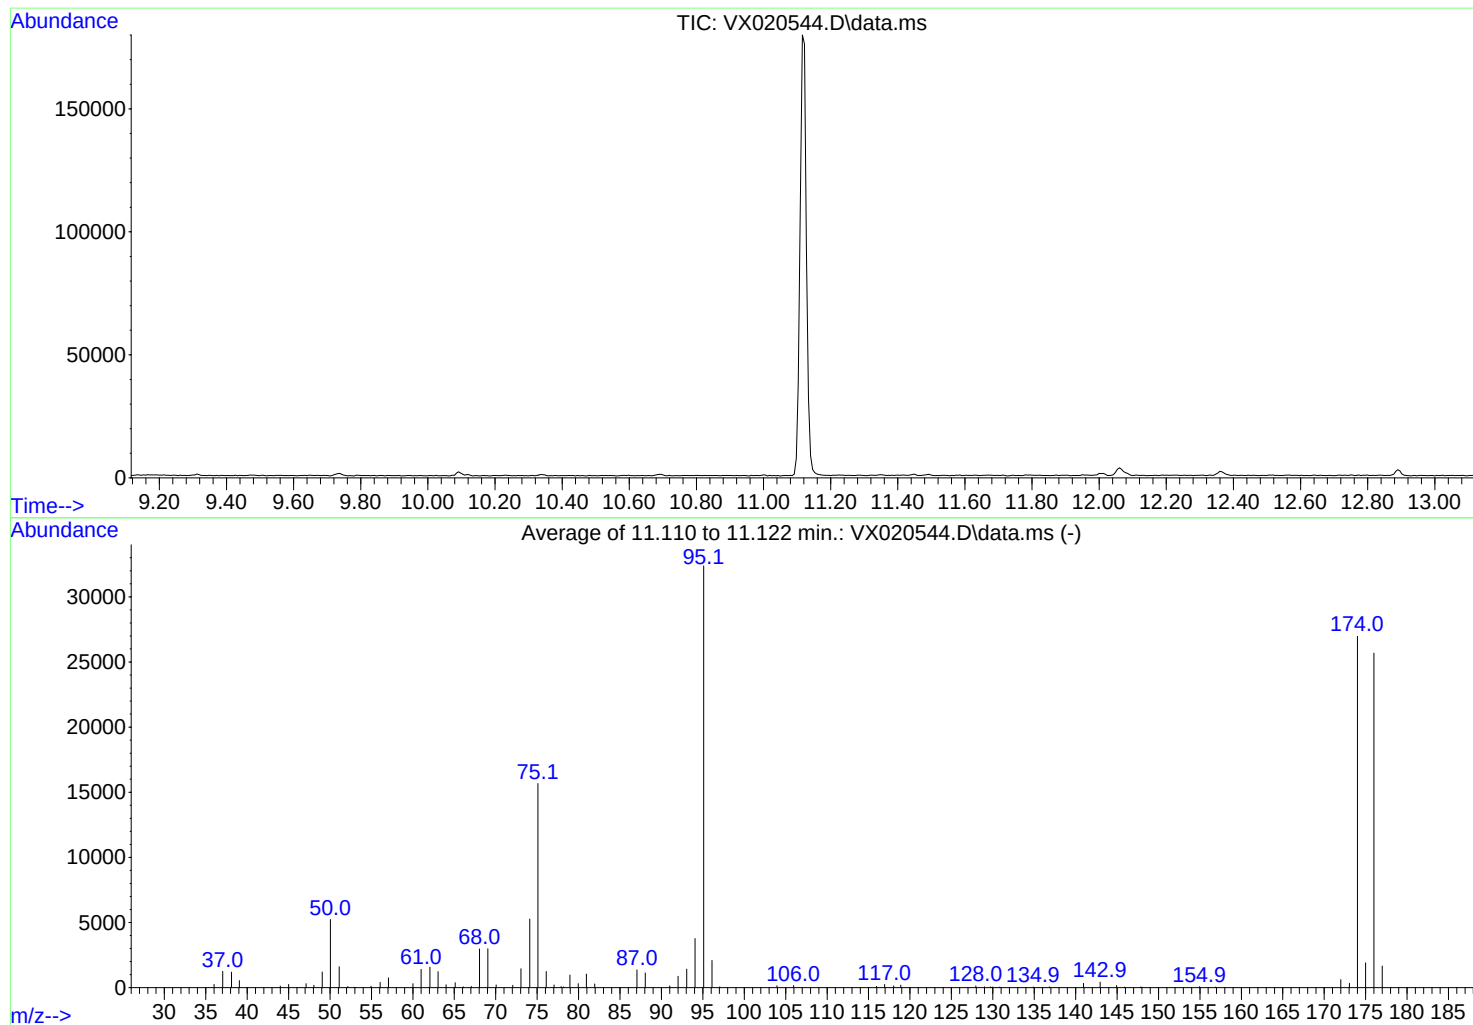

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	5231	PASS
75	95	30	60	48.4	15674	PASS
95	95	100	100	100.0	32381	PASS
96	95	5	9	6.5	2089	PASS
173	174	0.00	2	1.2	329	PASS
174	95	50	100	83.3	26974	PASS
175	174	5	9	7.1	1911	PASS
176	174	95	101	95.2	25683	PASS
177	176	5	9	6.5	1659	PASS