



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011124\
Data File : VX039709.D
Acq On : 11 Jan 2024 08:32
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
Title : SW846 8260
Last Update : Thu Jan 11 03:51:26 2024

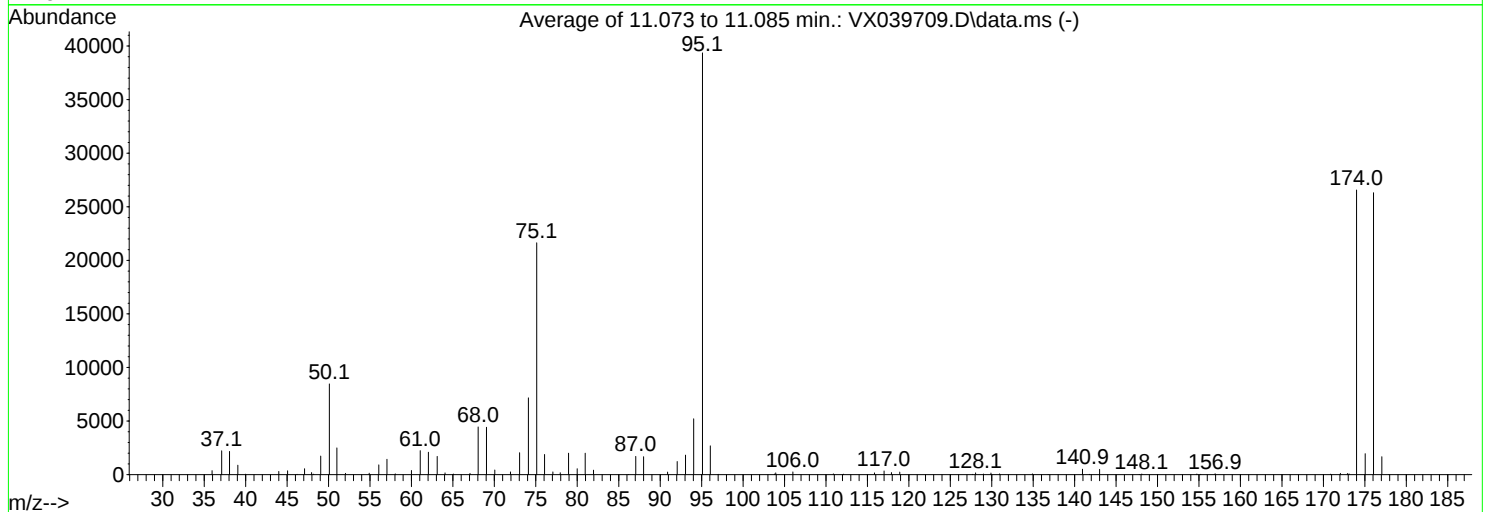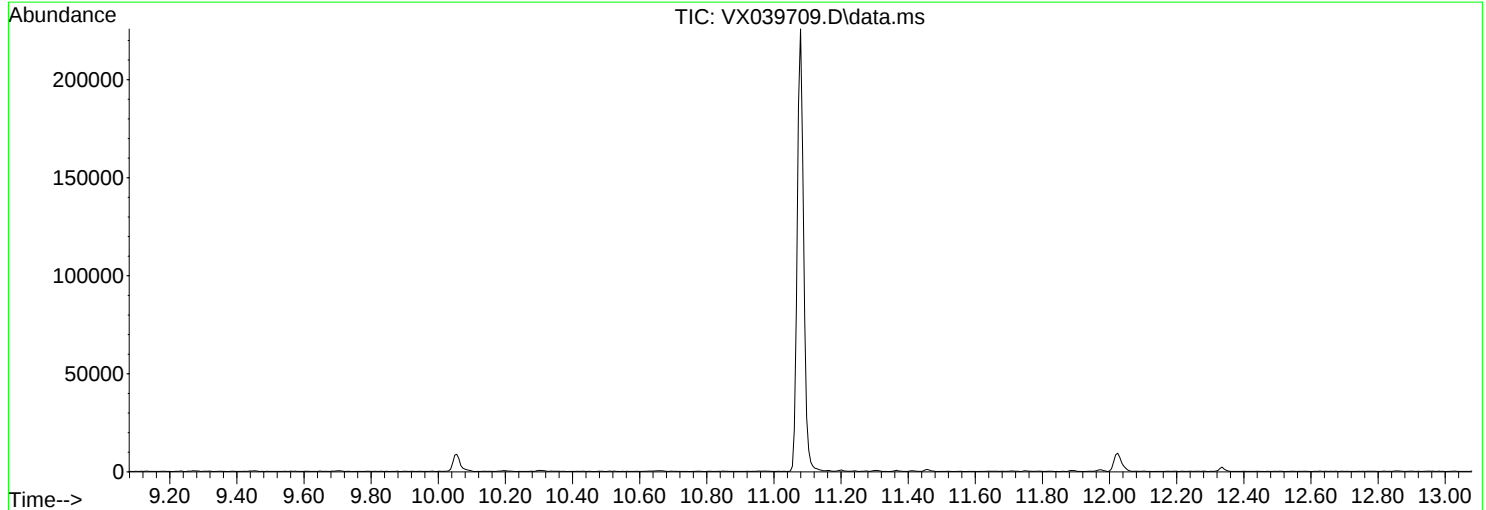

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.5	8468	PASS
75	95	30	60	55.0	21643	PASS
95	95	100	100	100.0	39365	PASS
96	95	5	9	6.8	2685	PASS
173	174	0.00	2	0.4	102	PASS
174	95	50	100	67.5	26571	PASS
175	174	5	9	7.4	1957	PASS
176	174	95	101	99.0	26317	PASS
177	176	5	9	6.4	1677	PASS