


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011221\
 Data File : VX020569.D
 Acq On : 12 Jan 2021 09:58
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011121W.M
 Title : SW846 8260
 Last Update : Mon Jan 11 15:05:37 2021

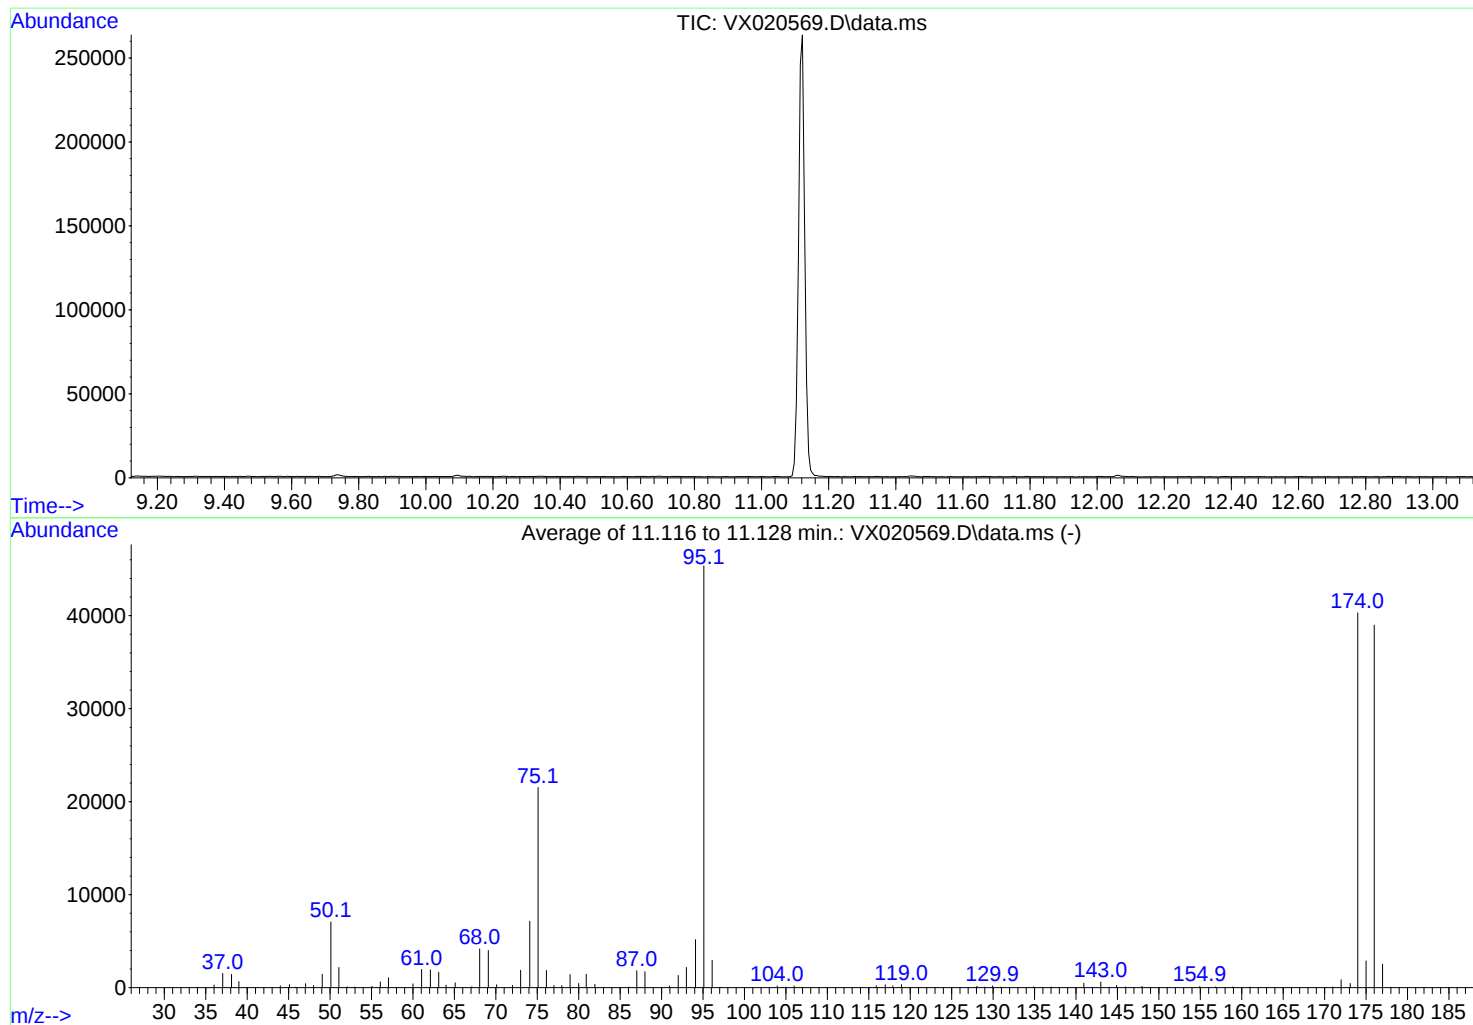

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	7079	PASS
75	95	30	60	47.5	21525	PASS
95	95	100	100	100.0	45357	PASS
96	95	5	9	6.5	2941	PASS
173	174	0.00	2	1.1	448	PASS
174	95	50	100	88.9	40317	PASS
175	174	5	9	7.1	2867	PASS
176	174	95	101	96.7	38997	PASS
177	176	5	9	6.5	2523	PASS