

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011222\
 Data File : VX026436.D
 Acq On : 12 Jan 2022 11:44
 Operator : JC/MD
 Sample : VX0112WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0112WBL01

Quant Time: Jan 13 05:52:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 11 14:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	155488	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	258196	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	224529	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	93682	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	107295	49.398	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	98.800%
35) Dibromofluoromethane	5.391	113	81200	48.700	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.400%
50) Toluene-d8	8.647	98	302624	50.367	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.740%
62) 4-Bromofluorobenzene	11.079	95	107963	50.582	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	101.160%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011222\
Data File : VX026436.D
Acq On : 12 Jan 2022 11:44
Operator : JC/MD
Sample : VX0112WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0112WBL01

Quant Time: Jan 13 05:52:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 11 14:45:13 2022
Response via : Initial Calibration




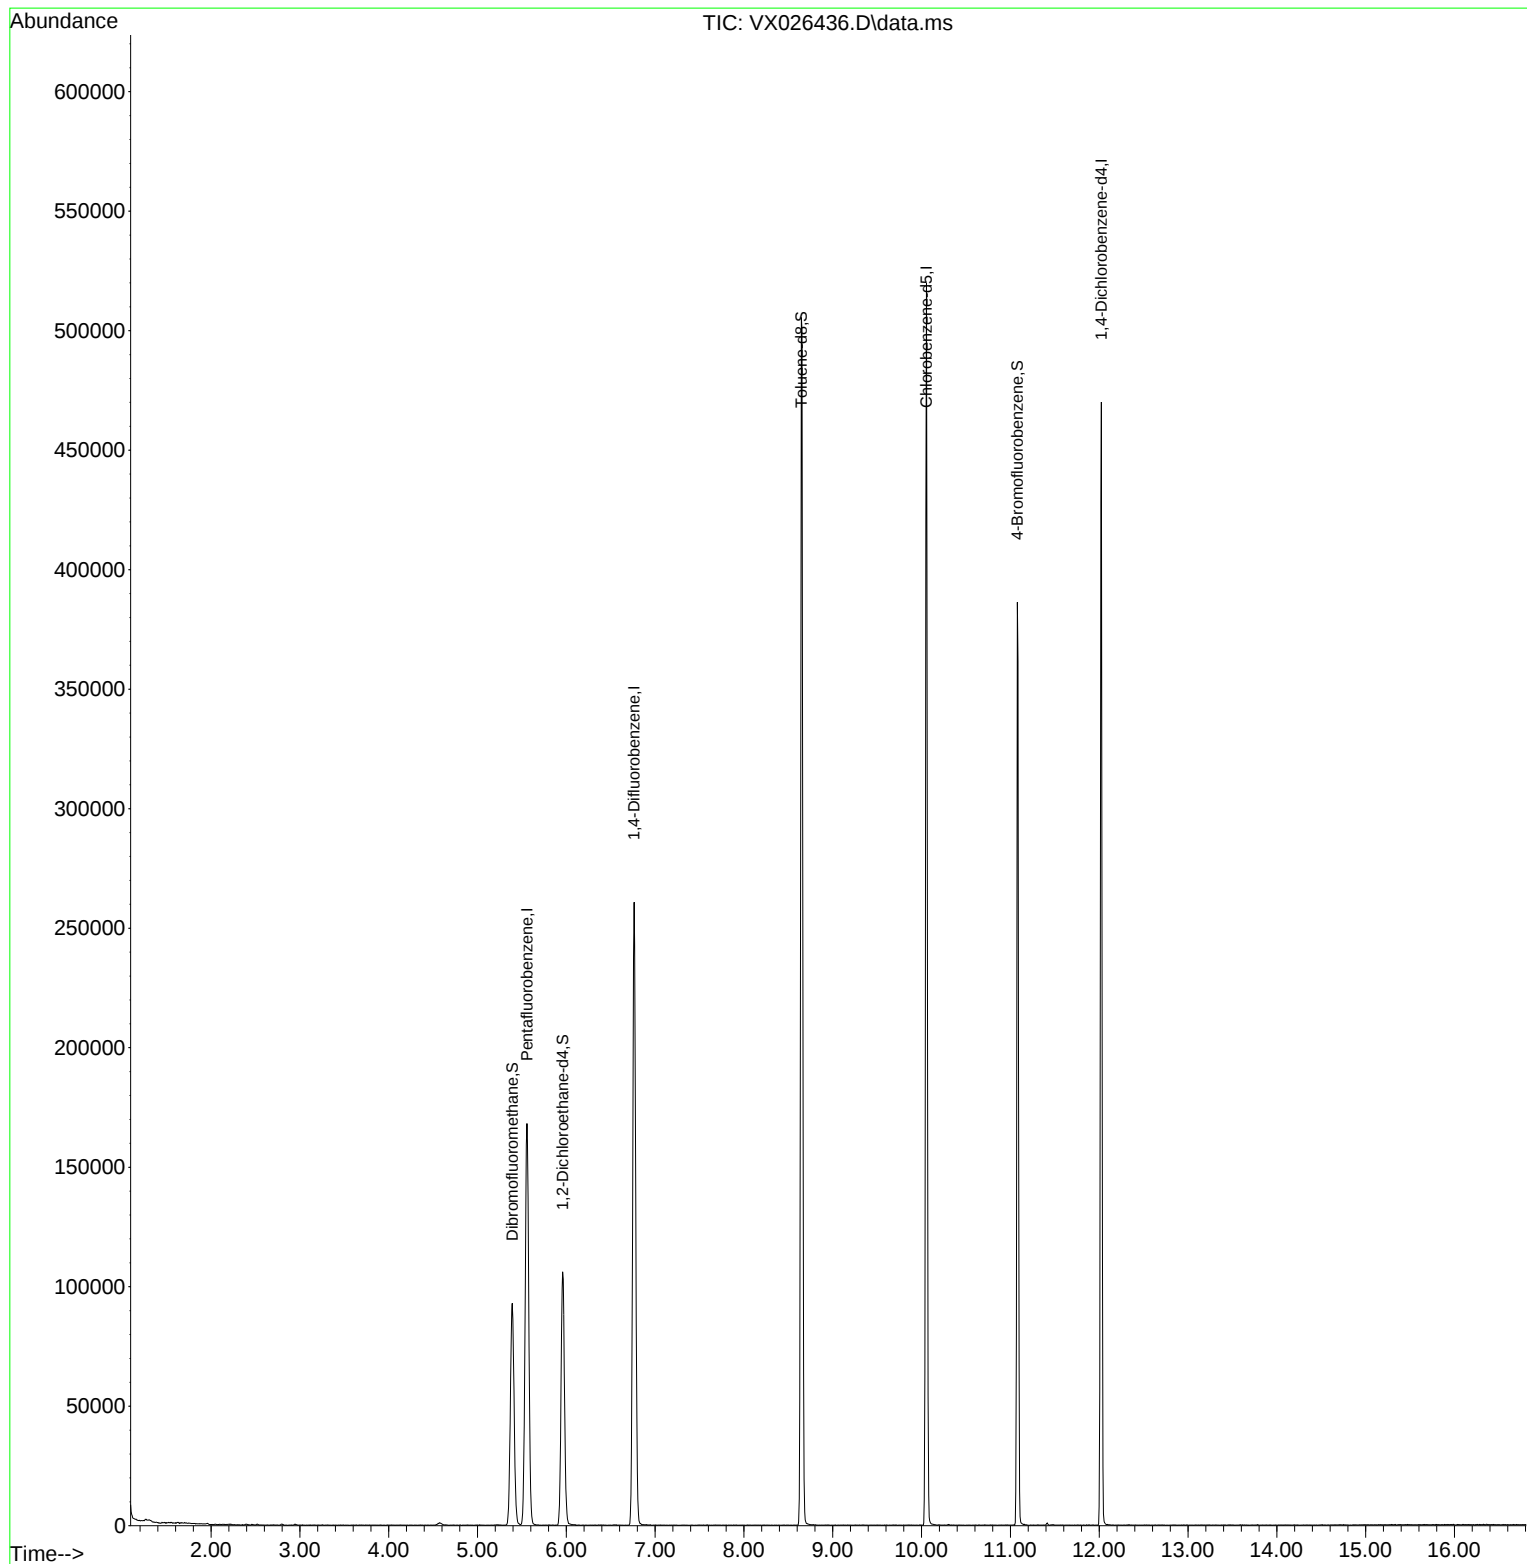


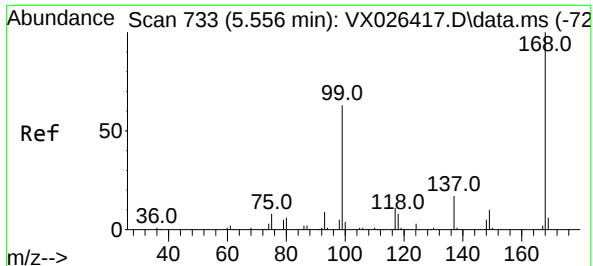

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.000 min
Lab File: VX026436.D
Acq: 12 Jan 2022 11:44




Instrument :
MSVOA_X
ClientSampleId :
VX0112WBL01


Tgt Ion:168 Resp: 155488
Ion Ratio Lower Upper
168 100
99 61.4 50.3 75.5

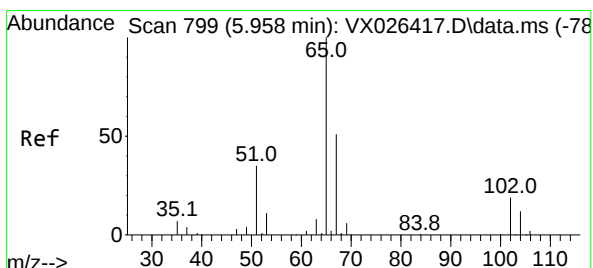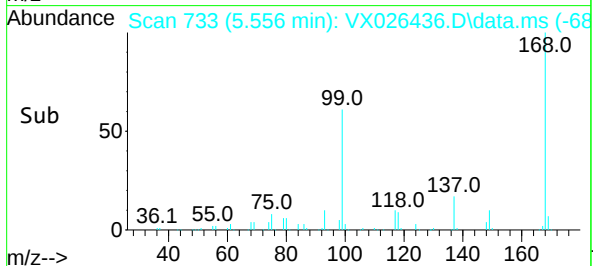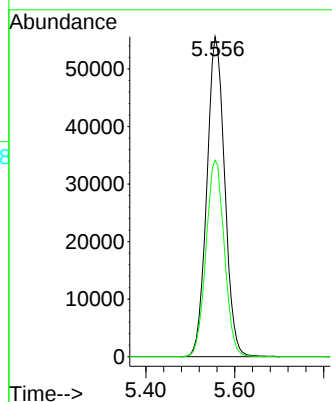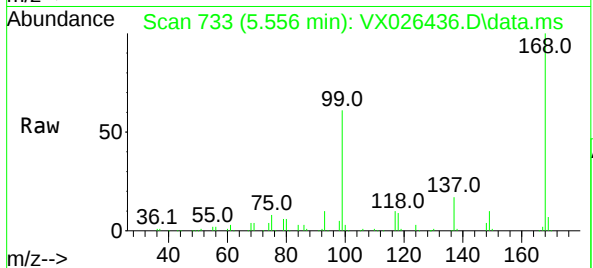

#33
1,2-Dichloroethane-d4
Concen: 49.398 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX026436.D
Acq: 12 Jan 2022 11:44

Tgt Ion: 65 Resp: 107295
Ion Ratio Lower Upper
65 100
67 49.7 0.0 100.8


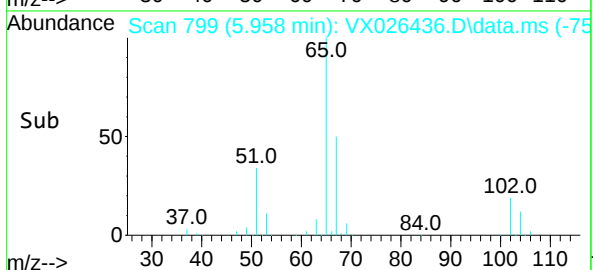
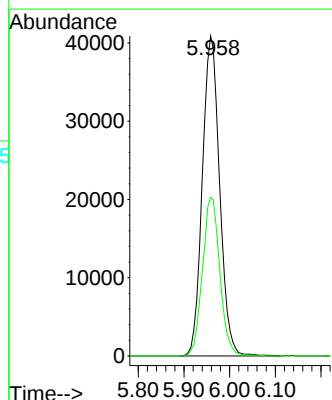
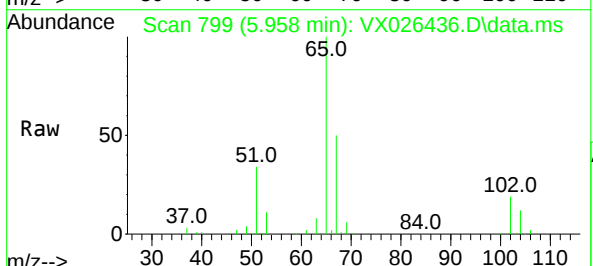


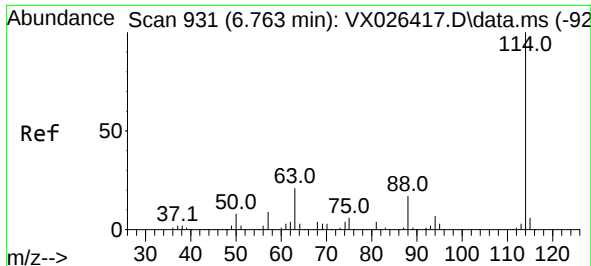

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX026436.D
Acq: 12 Jan 2022 11:44




Instrument :
MSVOA_X
ClientSampleId :
VX0112WBL01


Tgt Ion:114 Resp: 258196
Ion Ratio Lower Upper
114 100
63 22.0 0.0 42.8
88 16.6 0.0 33.0

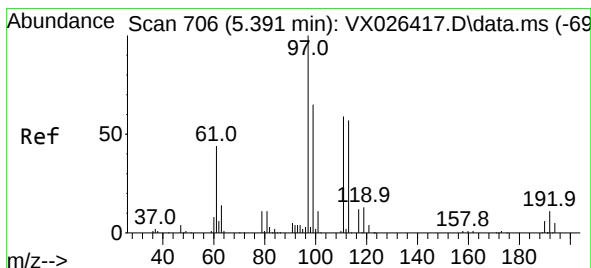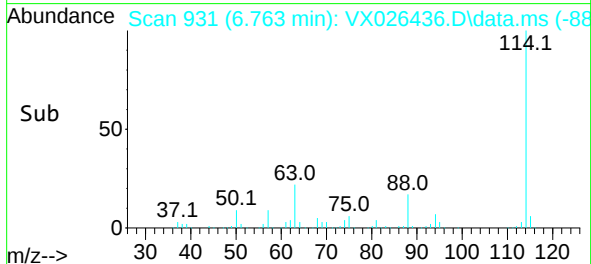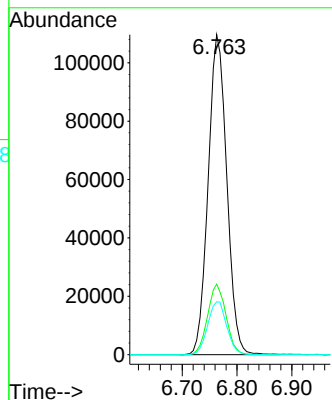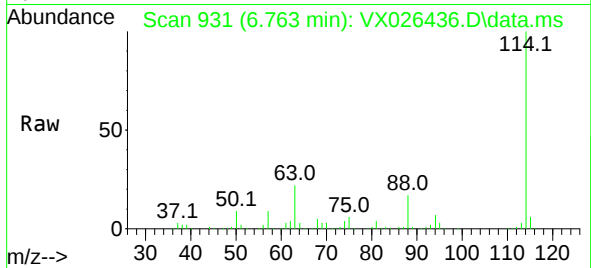

#35
Dibromofluoromethane
Concen: 48.700 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.000 min
Lab File: VX026436.D
Acq: 12 Jan 2022 11:44

Tgt Ion:113 Resp: 81200
Ion Ratio Lower Upper
113 100
111 103.4 81.2 121.8
192 19.2 15.0 22.4


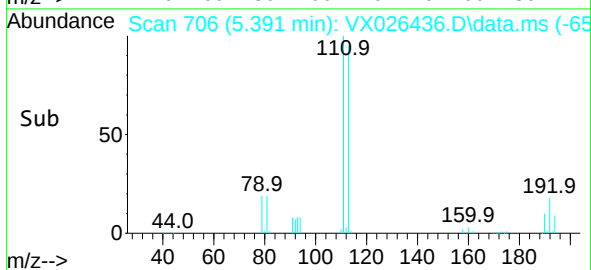
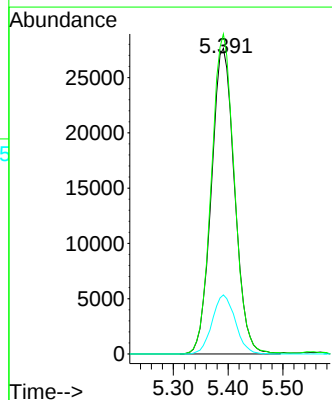
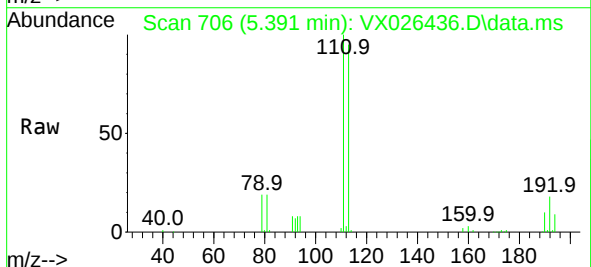


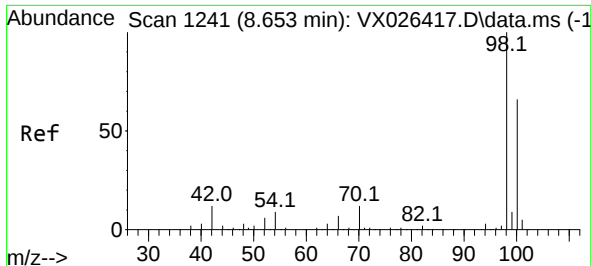

#50
Toluene-d8
Concen: 50.367 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX026436.D
Acq: 12 Jan 2022 11:44




Instrument :
MSVOA_X
ClientSampleId :
VX0112WBL01


Tgt Ion: 98 Resp: 302624
Ion Ratio Lower Upper
98 100
100 66.0 53.2 79.8

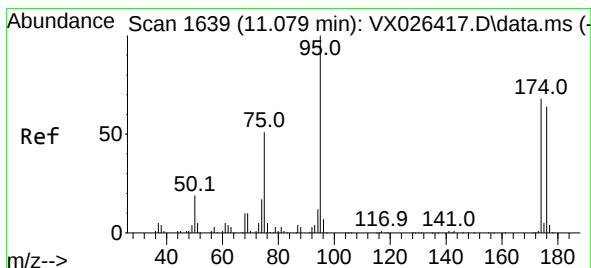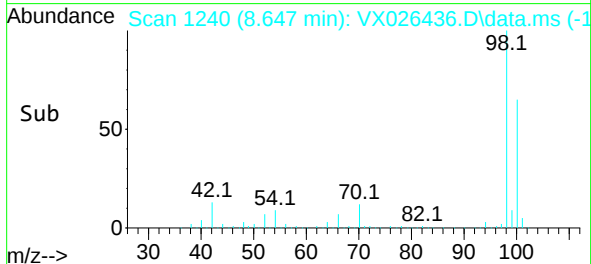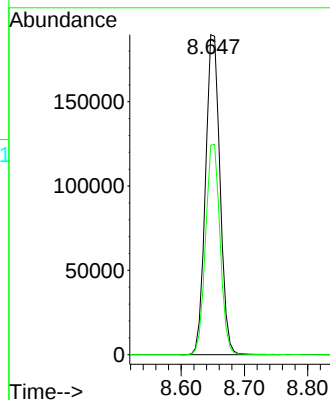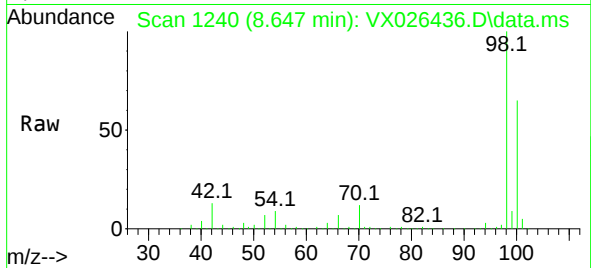

#62
4-Bromofluorobenzene
Concen: 50.582 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX026436.D
Acq: 12 Jan 2022 11:44

Tgt Ion: 95 Resp: 107963
Ion Ratio Lower Upper
95 100
174 71.6 0.0 148.6
176 69.2 0.0 141.4


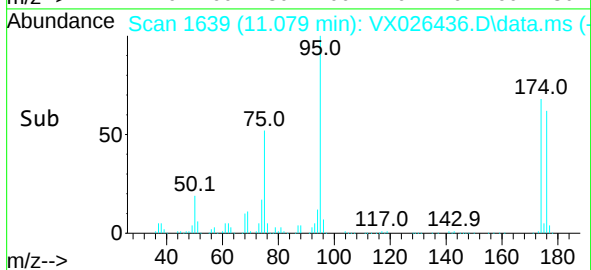
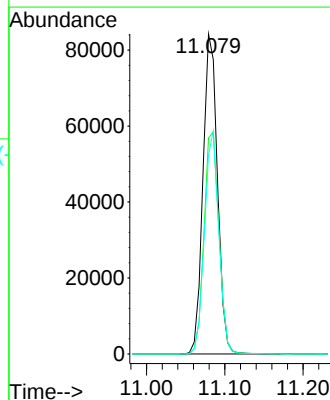
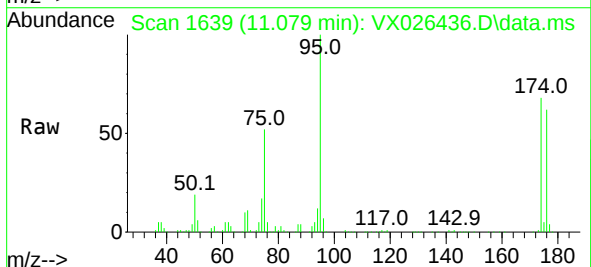


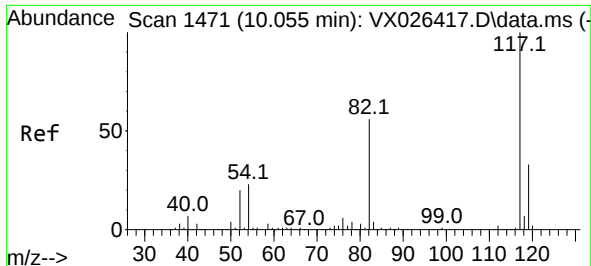

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX026436.D
Acq: 12 Jan 2022 11:44

Instrument :
MSVOA_X
ClientSampleId :
VX0112WBL01

Tgt Ion:117 Resp: 224529
Ion Ratio Lower Upper
117 100
82 57.6 45.2 67.8
119 31.7 26.2 39.2

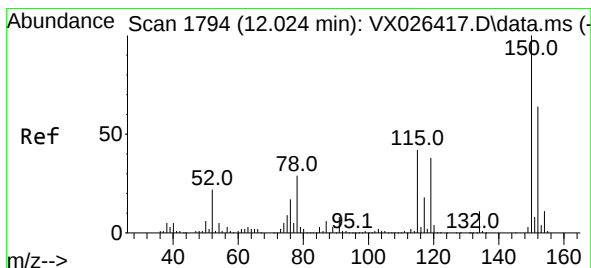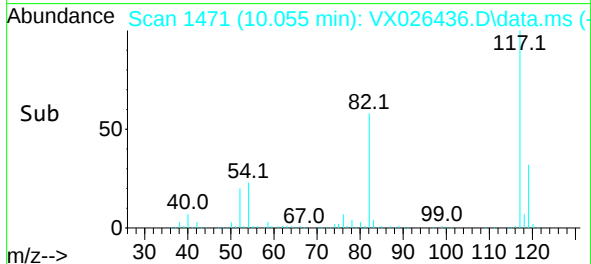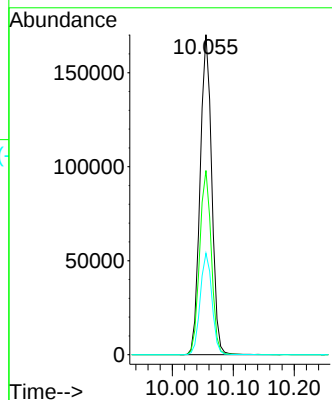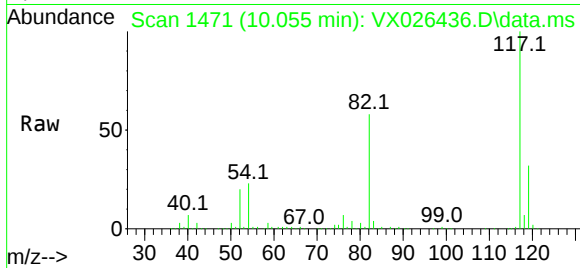

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX026436.D
Acq: 12 Jan 2022 11:44

Tgt Ion:152 Resp: 93682
Ion Ratio Lower Upper
152 100
115 62.7 44.2 132.6
150 158.4 0.0 348.2

