
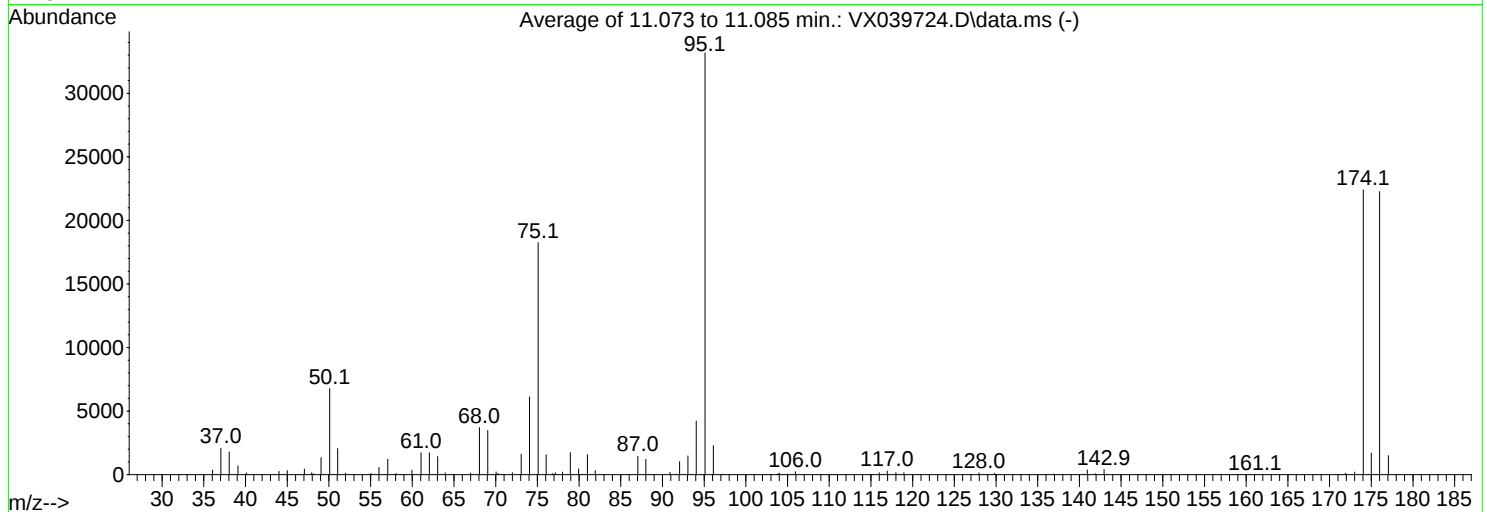


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011224\
Data File : VX039724.D
Acq On : 12 Jan 2024 08:33
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
Title : SW846 8260
Last Update : Thu Jan 11 03:51:26 2024

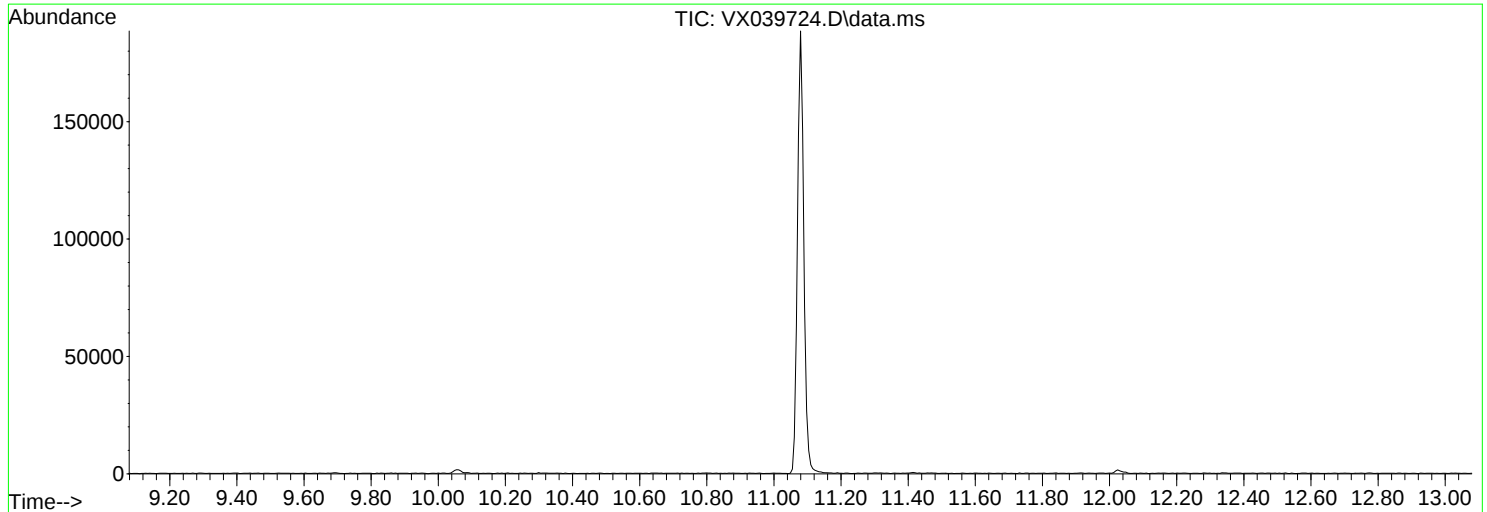

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.4	6774	PASS
75	95	30	60	55.0	18259	PASS
95	95	100	100	100.0	33184	PASS
96	95	5	9	6.9	2286	PASS
173	174	0.00	2	0.9	207	PASS
174	95	50	100	67.5	22405	PASS
175	174	5	9	7.6	1704	PASS
176	174	95	101	99.4	22272	PASS
177	176	5	9	6.7	1497	PASS