
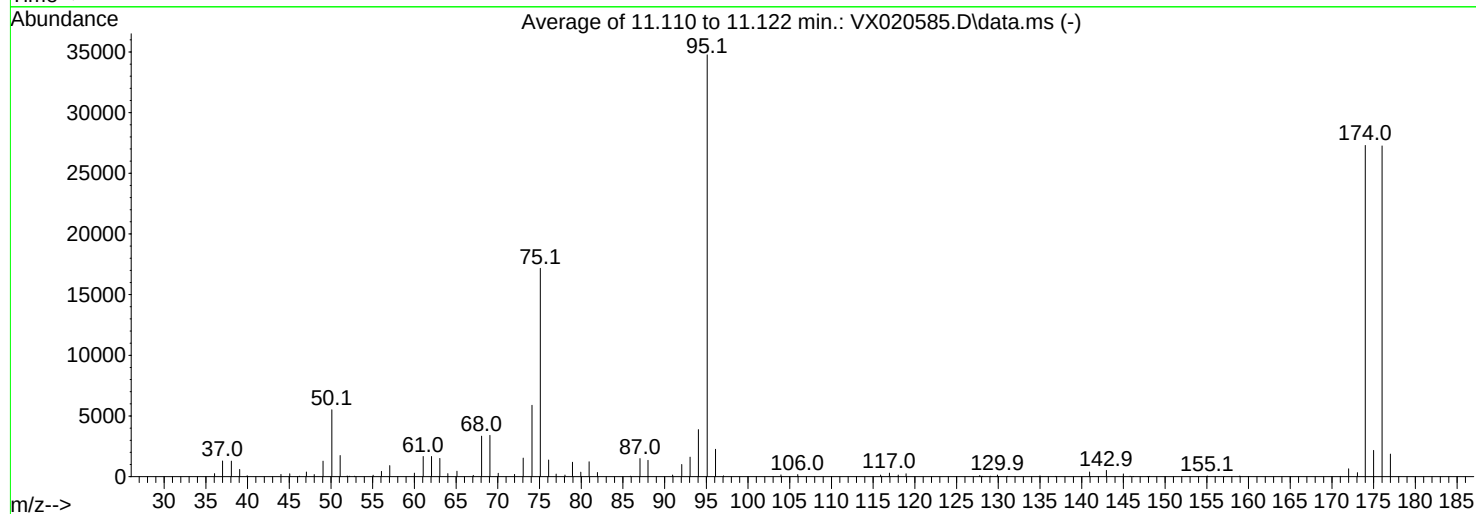


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011321\
Data File : VX020585.D
Acq On : 13 Jan 2021 10:33
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011121W.M
Title : SW846 8260
Last Update : Mon Jan 11 15:05:37 2021

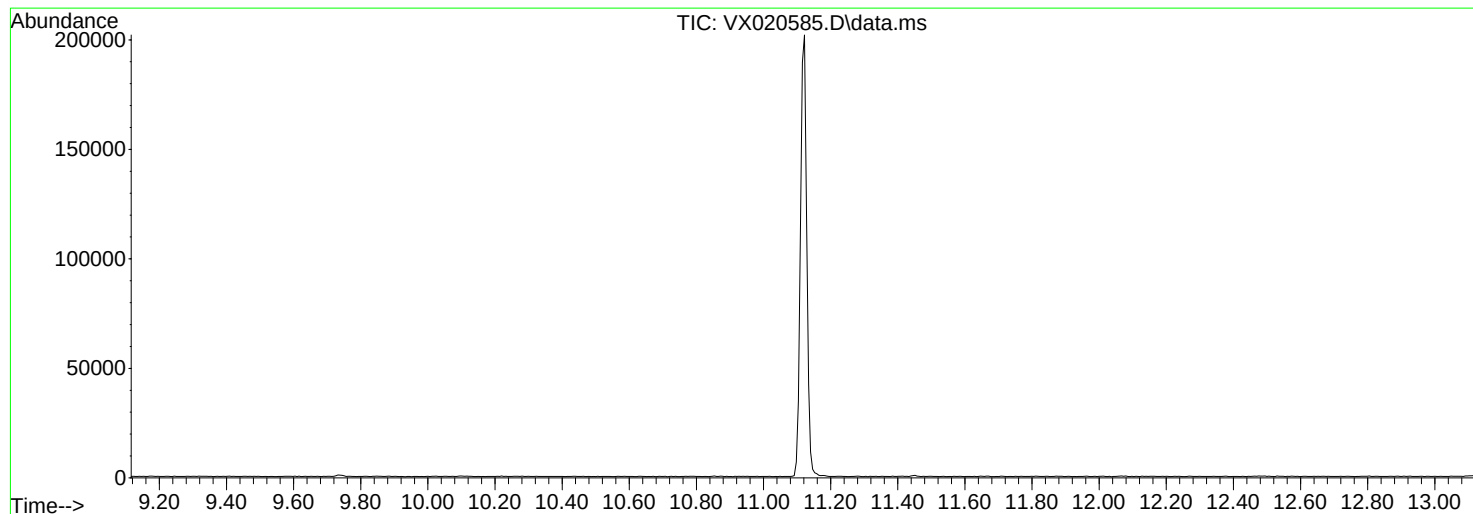

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	5518	PASS
75	95	30	60	49.4	17169	PASS
95	95	100	100	100.0	34763	PASS
96	95	5	9	6.5	2261	PASS
173	174	0.00	2	1.2	335	PASS
174	95	50	100	78.5	27302	PASS
175	174	5	9	7.9	2158	PASS
176	174	95	101	99.8	27261	PASS
177	176	5	9	6.8	1855	PASS