

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX011419\
 Data File : VX007044.D
 Acq On : 14 Jan 2019 17:22
 Operator : JC/SP
 Sample : K1126-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 15 00:30:12 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 08 14:06:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	588197	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	910804	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	872962	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	434699	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	310805	50.56	ug/l	0.00
Spiked Amount			Recovery	=	101.12%	
35) Dibromofluoromethane	5.51	113	279742	47.96	ug/l	0.00
Spiked Amount			Recovery	=	95.92%	
50) Toluene-d8	8.71	98	1111742	52.07	ug/l	0.00
Spiked Amount			Recovery	=	104.14%	
62) 4-Bromofluorobenzene	11.13	95	397272	53.38	ug/l	0.00
Spiked Amount			Recovery	=	106.76%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.32	50	1412	0.251	ug/l #	73
5) Bromomethane	1.64	94	1590	0.246	ug/l	84
8) Diethyl Ether	2.20	74	1085	0.279	ug/l	87
11) Tert butyl alcohol	3.02	59	2902	2.001	ug/l #	79
13) Acrolein	2.30	56	371	3.670	ug/l #	55
14) Allyl chloride	2.85	41	19167	2.069	ug/l #	28
16) Acetone	2.45	43	23689	7.795	ug/l	93
18) Methyl Acetate	2.78	43	7119	0.809	ug/l #	84
20) Methylene Chloride	2.86	84	538772	93.706	ug/l	97
25) 2-Butanone	4.70	43	1820	0.419	ug/l	93
29) Tetrahydrofuran	5.17	42	1325	0.469	ug/l #	72
30) Chloroform	5.23	83	2868	0.281	ug/l #	78
36) 1,1-Dichloropropene	5.66	75	38565	4.870	ug/l #	49
37) Ethyl Acetate	4.70	43	1820	0.214	ug/l	97
38) Carbon Tetrachloride	5.67	117	54256	6.810	ug/l #	13
43) Isopropyl Acetate	6.46	43	22125	1.652	ug/l	93
48) Methyl methacrylate	7.68	41	12544	1.824	ug/l #	19
49) 1,4-Dioxane	7.74	88	87	Below Cal	#	27
51) 4-Methyl-2-Pentanone	8.62	43	129328	15.028	ug/l #	48
54) cis-1,3-Dichloropropene	8.62	75	64304	7.226	ug/l #	62
59) 2-Hexanone	9.54	43	139989	21.346	ug/l #	52
71) Bromoform	10.76	173	125	4.747	ug/l #	28
76) 1,2,3-Trichloropropane	11.13	75	189334	21.493	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.51	105	5341	0.209	ug/l	99
81) trans-1,4-Dichloro-2-buten	11.13	75	189334	63.739	ug/l #	10
90) Hexachloroethane	12.59	117	96	2.929	ug/l #	6
95) Naphthalene	13.83	128	30378	0.970	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX011419\
Data File : VX007044.D
Acq On : 14 Jan 2019 17:22
Operator : JC/SP
Sample : K1126-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jan 15 00:30:12 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 08 14:06:59 2019
Response via : Initial Calibration

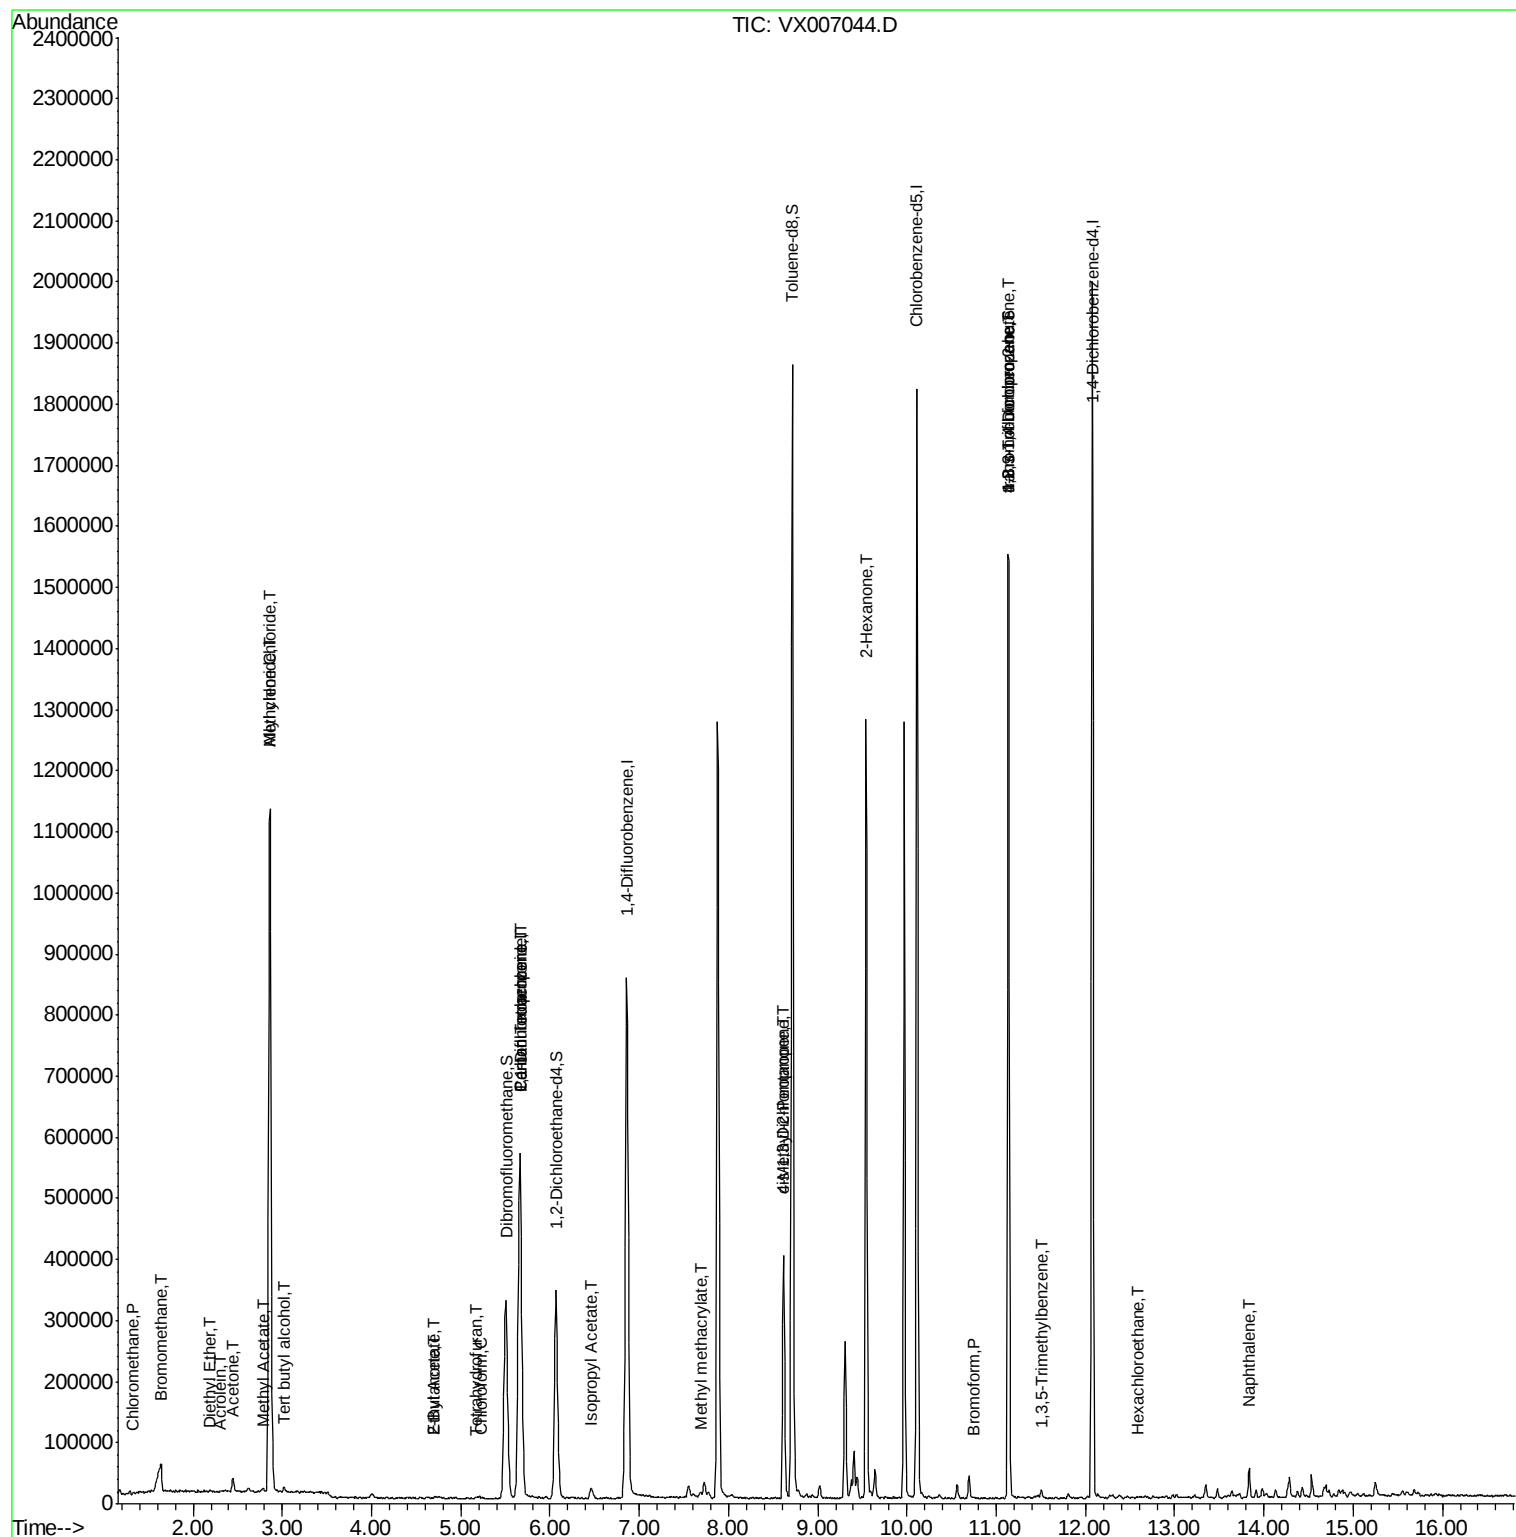

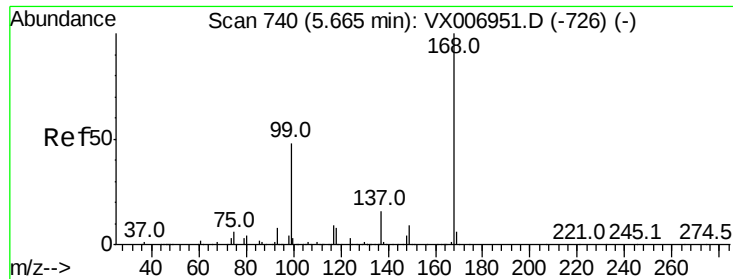

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX007044.D

Acq: 14 Jan 2019 17:22


Instrument :
MSVOA_X
ClientSampleId :

Tot Ion:168 Resp: 588197

Ion Ratio Lower Upper

168 100

99 50.8 41.8 62.8

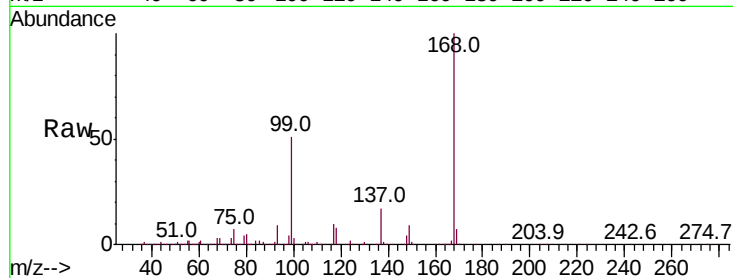

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

200000



150000

100000

50000

0

Time-->

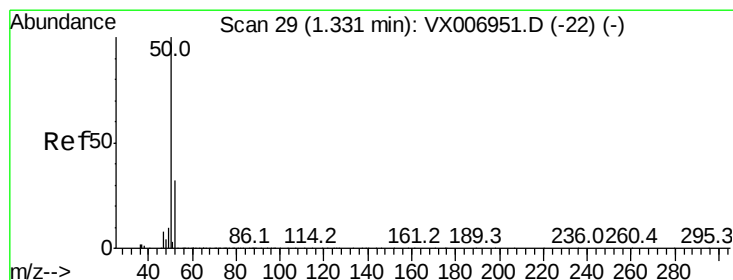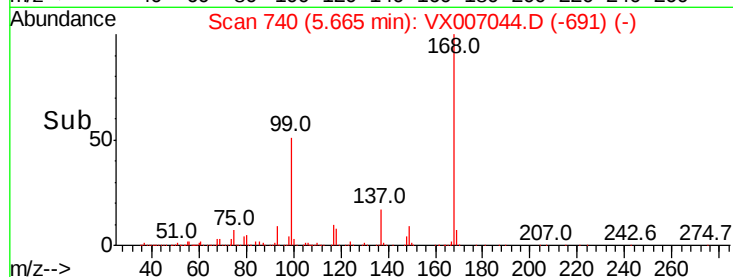

#3

Chloromethane

Concen: 0.251 ug/l

RT: 1.32 min Scan# 28

Delta R.T. -0.01 min

Lab File: VX007044.D


Acq: 14 Jan 2019 17:22

Tgt Ion: 50 Resp: 1412

Ion Ratio Lower Upper

50 100

52 16.5 25.4 38.2#

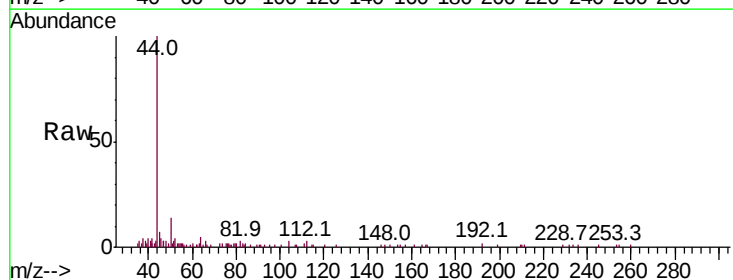

Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.32

1000

800


600


400

200

0

Time-->

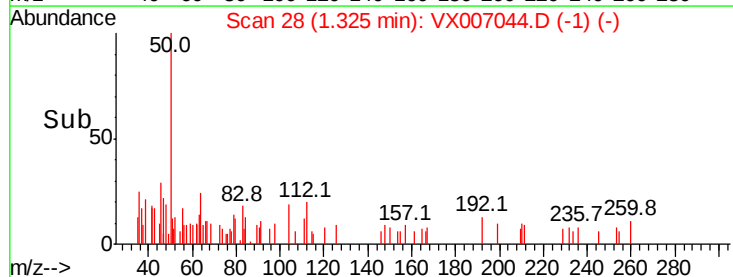



#5

Bromomethane

Concen: 0.246 ug/l

RT: 1.64 min Scan# 80

Delta R.T. 0.00 min

Lab File: VX007044.D

Acq: 14 Jan 2019 17:22

Instrument :

MSVOA_X





ClientSampled :

Tot Ion: 94 Resp: 1590

Ion Ratio Lower Upper

94 100

96 76.5 73.4 110.2

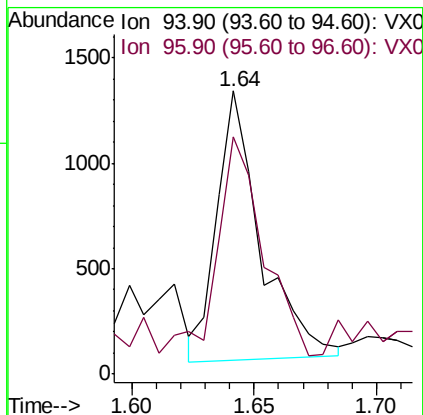

#8

Diethyl Ether

Concen: 0.279 ug/l

RT: 2.20 min Scan# 171

Delta R.T. 0.01 min

Lab File: VX007044.D




Acq: 14 Jan 2019 17:22


Tgt Ion: 74 Resp: 1085

Ion Ratio Lower Upper

74 100

45 104.8 46.3 138.9

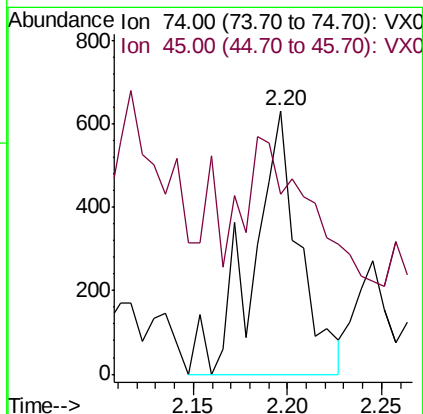




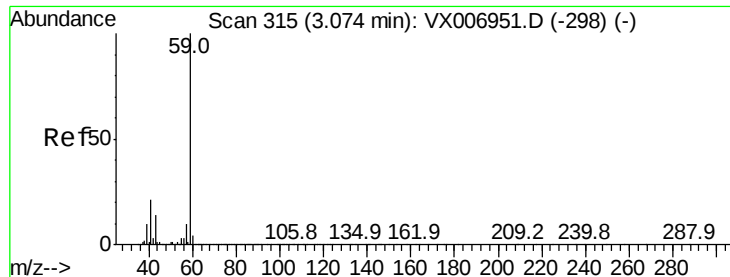


#11

Tert butyl alcohol
Concen: 2.001 ug/l
RT: 3.02 min Scan# 306
Delta R.T. -0.05 min
Lab File: VX007044.D
Acq: 14 Jan 2019 17:22

Instrument :
MSVOA_X
ClientSampleId :




Tot Ion: 59 Resp: 2902
Ion Ratio Lower Upper
59 100
57 2.9 8.5 12.7#

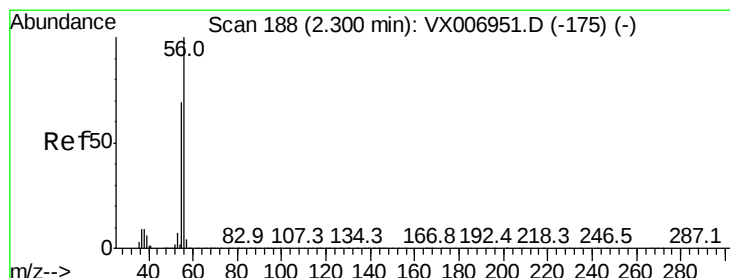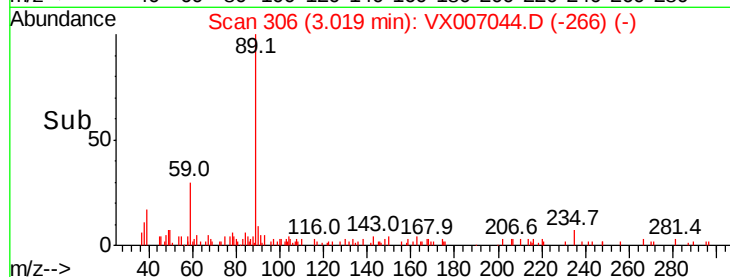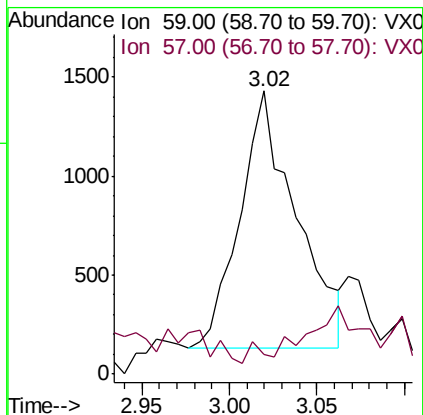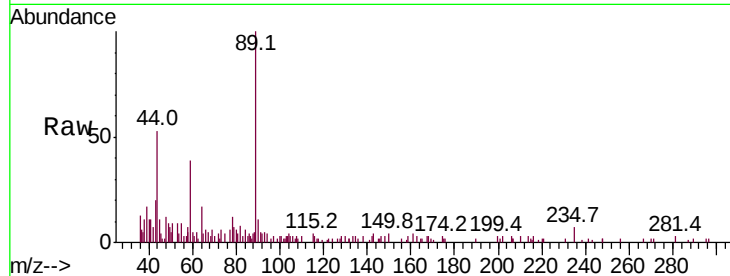


#13

Acrolein
Concen: 3.670 ug/l
RT: 2.30 min Scan# 188
Delta R.T. 0.00 min
Lab File: VX007044.D
Acq: 14 Jan 2019 17:22

Tgt Ion: 56 Resp: 371
Ion Ratio Lower Upper
56 100
55 35.3 58.2 87.4#


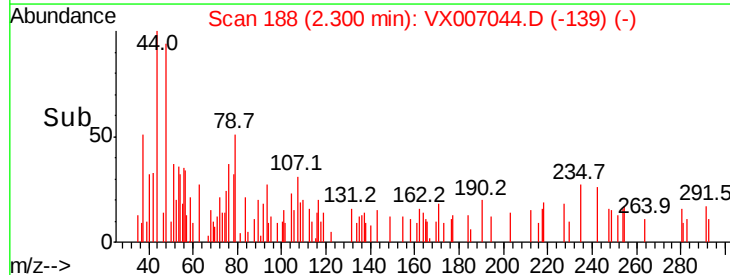
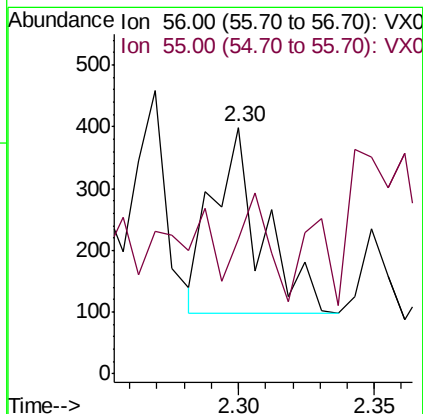
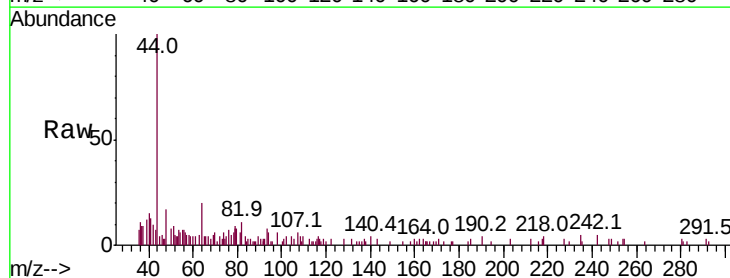




#14
Allvl chloride
Concen: 2.069 ug/l
RT: 2.85 min Scan# 279
Delta R.T. 0.13 min
Lab File: VX007044.D
Acq: 14 Jan 2019 17:22




Instrument :
MSVOA_X
ClientSampled :


Tot Ion: 41 Resp: 19167
Ion Ratio Lower Upper
41 100
39 3.4 53.6 80.4#
76 0.5 27.4 41.2#

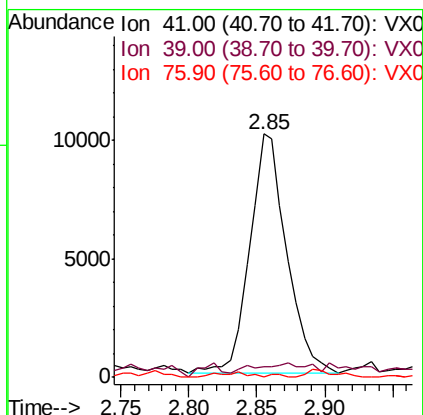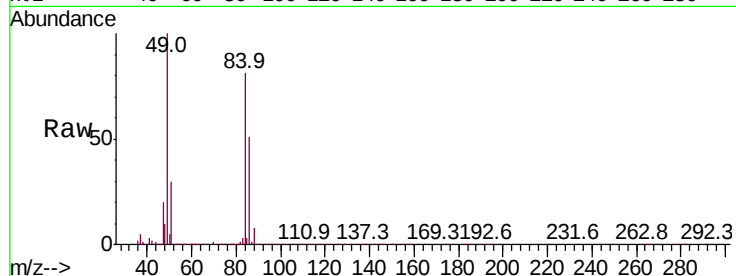

#16
Acetone
Concen: 7.795 ug/l
RT: 2.45 min Scan# 212
Delta R.T. 0.00 min
Lab File: VX007044.D
Acq: 14 Jan 2019 17:22

Tgt Ion: 43 Resp: 23689
Ion Ratio Lower Upper
43 100
58 27.5 25.0 37.6



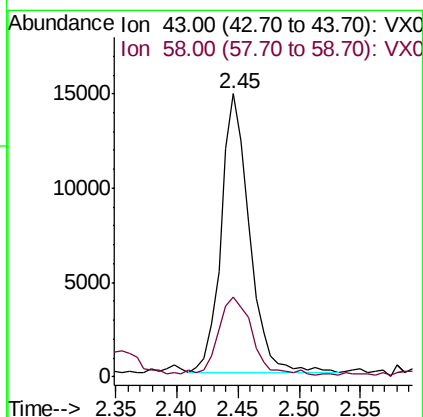



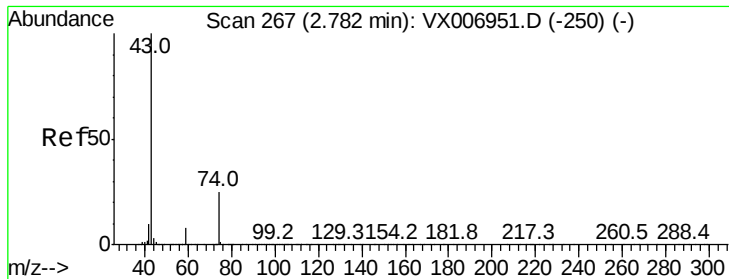

#18
Methyl Acetate
Concen: 0.809 ug/l
RT: 2.78 min Scan# 267
Delta R.T. 0.00 min
Lab File: VX007044.D
Acq: 14 Jan 2019 17:22




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 43 Resp: 7119
Ion Ratio Lower Upper
43 100
74 31.0 18.6 28.0#

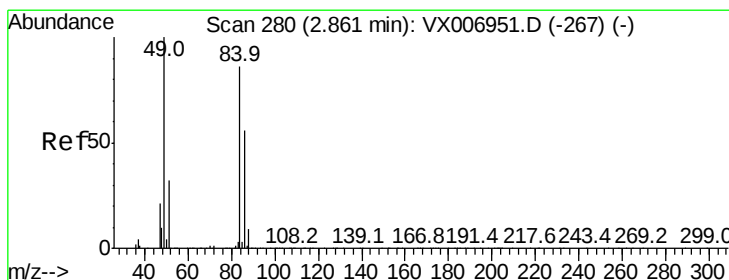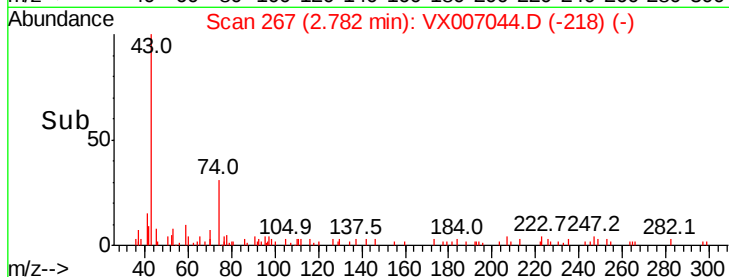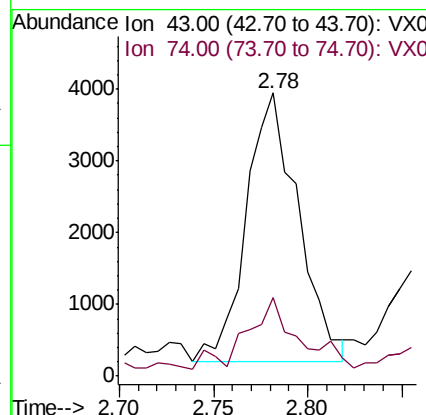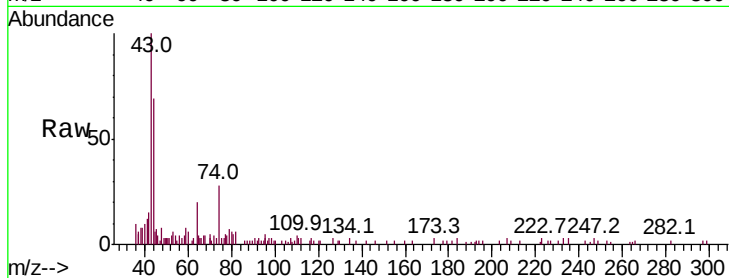

#20
Methylene Chloride
Concen: 93.706 ug/l
RT: 2.86 min Scan# 280
Delta R.T. 0.00 min
Lab File: VX007044.D
Acq: 14 Jan 2019 17:22

Tgt Ion: 84 Resp: 538772
Ion Ratio Lower Upper
84 100
49 119.5 91.8 137.6
51 35.3 28.5 42.7
86 63.2 50.2 75.2


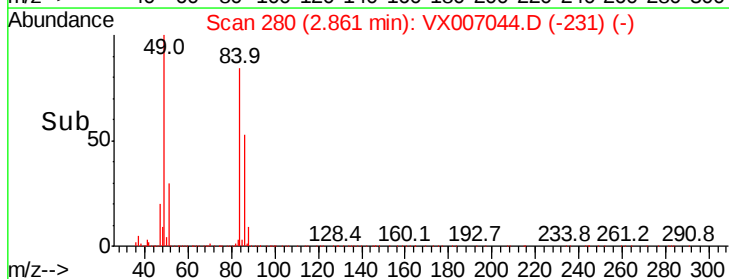
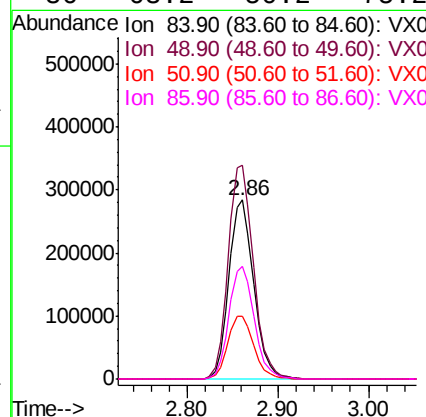
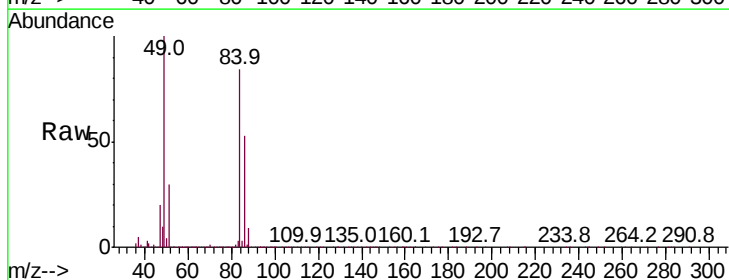


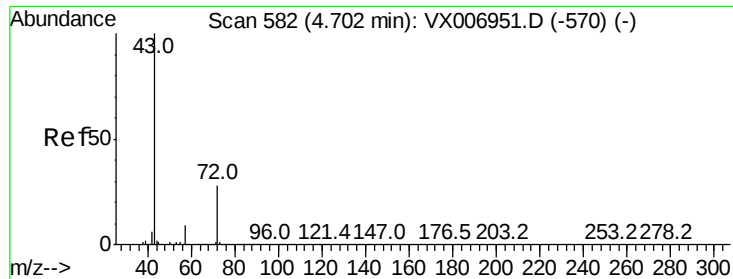

#25
2-Butanone
Concen: 0.419 ug/l
RT: 4.70 min Scan# 581
Delta R.T. -0.01 min
Lab File: VX007044.D
Acq: 14 Jan 2019 17:22




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 43 Resp: 1820
Ion Ratio Lower Upper
43 100
72 31.9 22.4 33.6

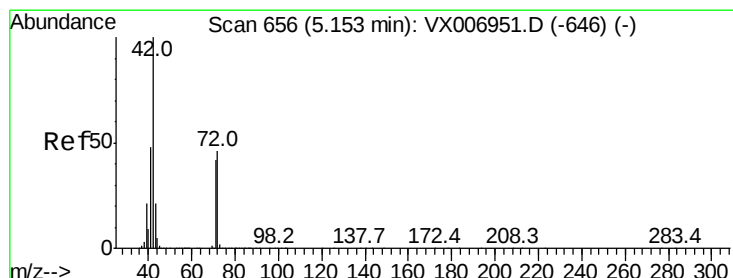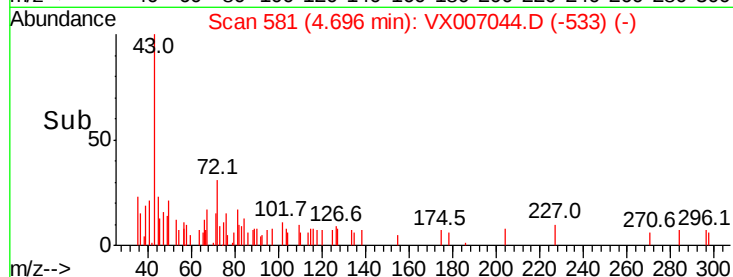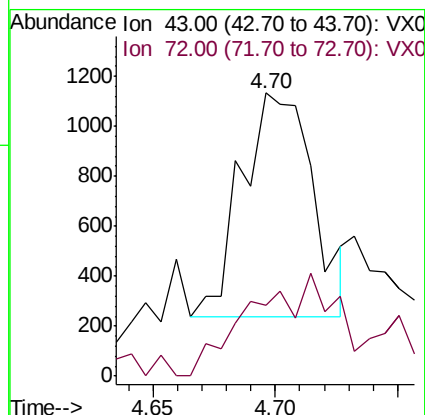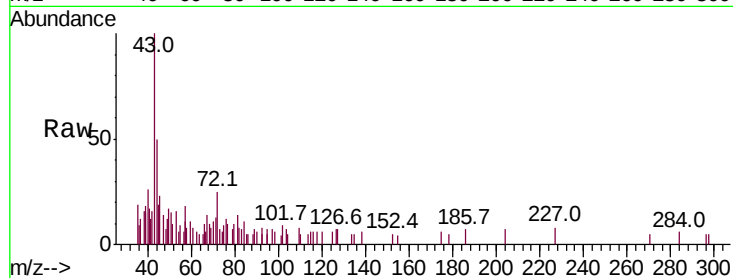

#29
Tetrahydrofuran
Concen: 0.469 ug/l
RT: 5.17 min Scan# 658
Delta R.T. 0.01 min
Lab File: VX007044.D
Acq: 14 Jan 2019 17:22

Tgt Ion: 42 Resp: 1325
Ion Ratio Lower Upper
42 100
72 77.4 38.9 58.3#
71 53.2 36.2 54.4


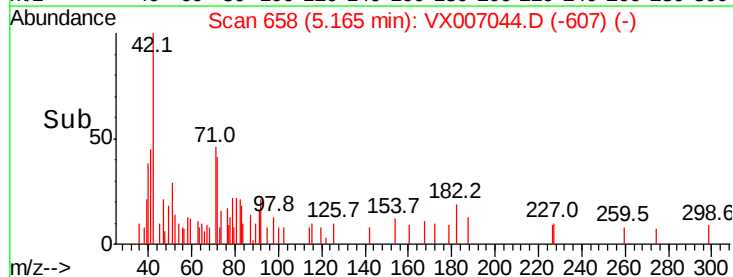
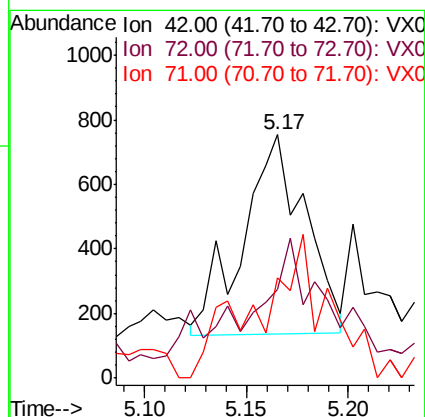
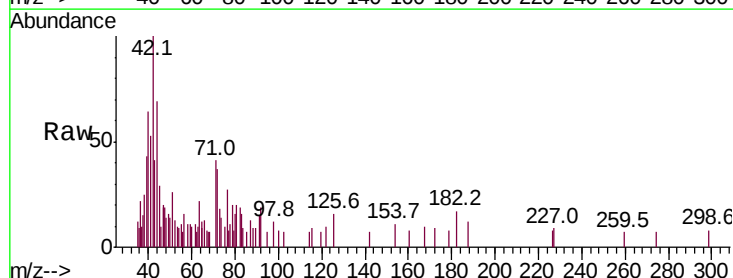


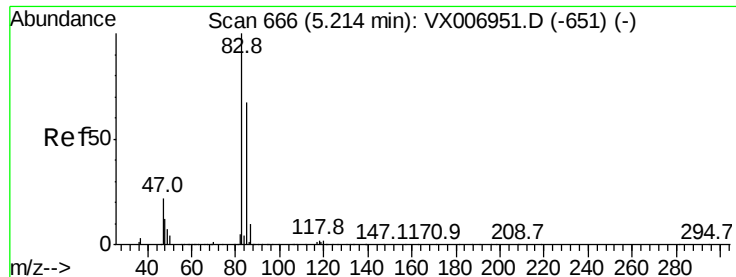

#30
Chloroform
Concen: 0.281 ug/l
RT: 5.23 min Scan# 669
Delta R.T. 0.02 min
Lab File: VX007044.D
Acq: 14 Jan 2019 17:22




Instrument :
MSVOA_X
ClientSampled :


Tot Ion: 83 Resp: 2868
Ion Ratio Lower Upper
83 100
85 46.4 51.2 76.8#

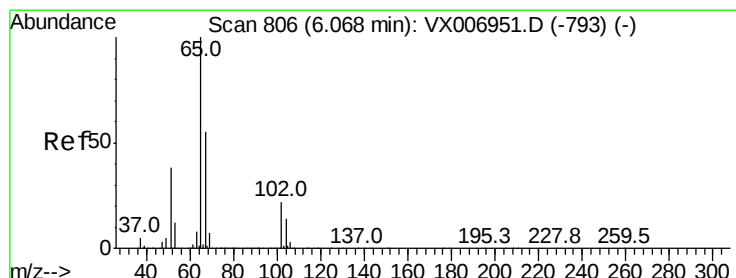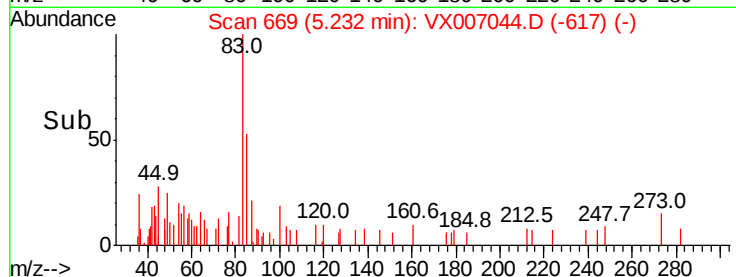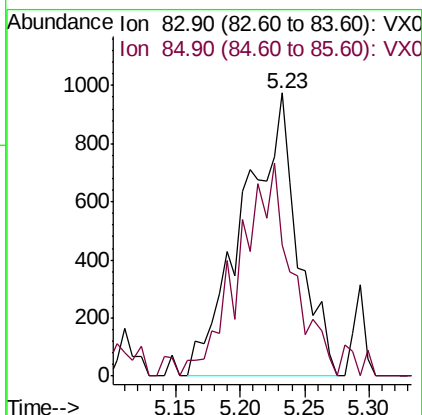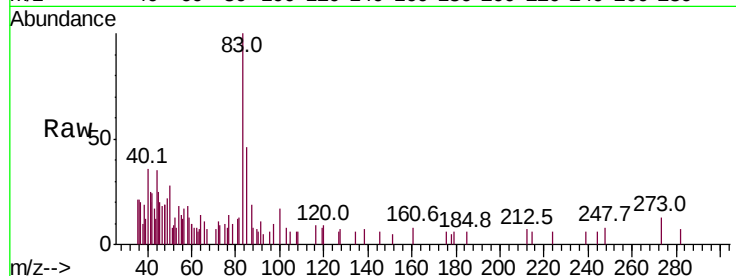

#33
1,2-Dichloroethane-d4
Concen: 50.561 ug/l
RT: 6.07 min Scan# 806
Delta R.T. 0.00 min
Lab File: VX007044.D
Acq: 14 Jan 2019 17:22

Tgt Ion: 65 Resp: 310805
Ion Ratio Lower Upper
65 100
67 53.6 0.0 105.0

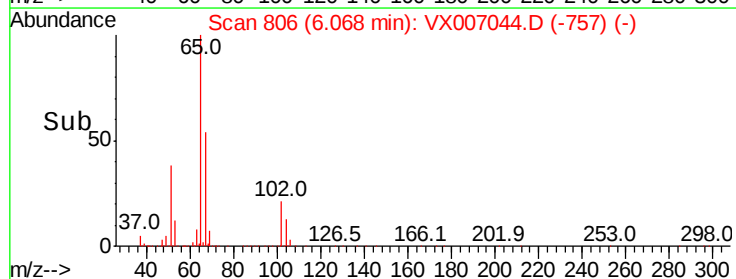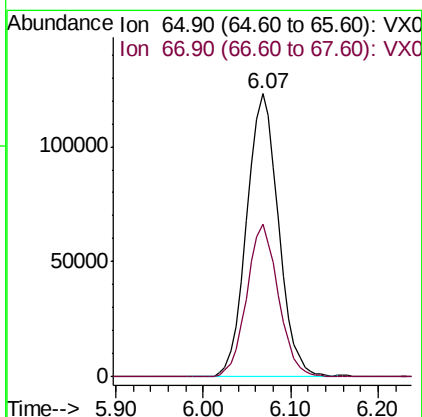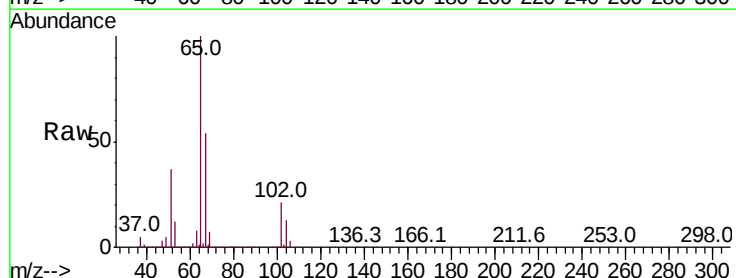



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX007044.D

Acq: 14 Jan 2019 17:22

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:114 Resp: 910804

Ion Ratio Lower Upper

114 100

63 18.2 0.0 34.8




88 14.2 0.0 28.8

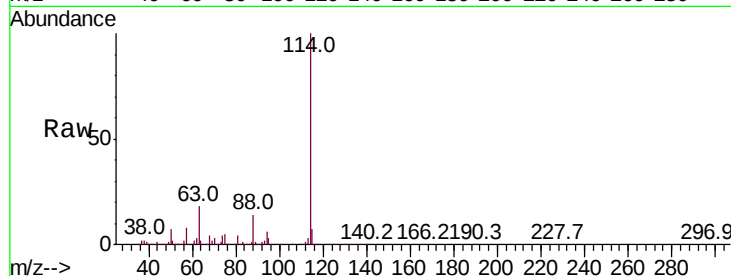

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

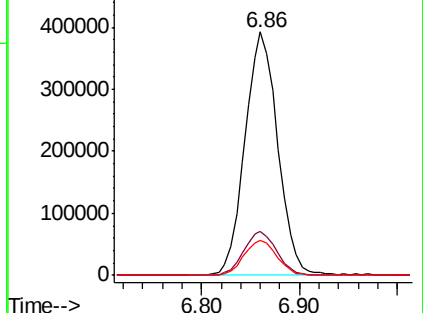

#35

Dibromofluoromethane

Concen: 47.961 ug/l

RT: 5.51 min Scan# 714

Delta R.T. 0.01 min

Lab File: VX007044.D

Acq: 14 Jan 2019 17:22


Tgt Ion:113 Resp: 279742

Ion Ratio Lower Upper

113 100

111 100.9 81.6 122.4



192 22.0 16.7 25.1




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

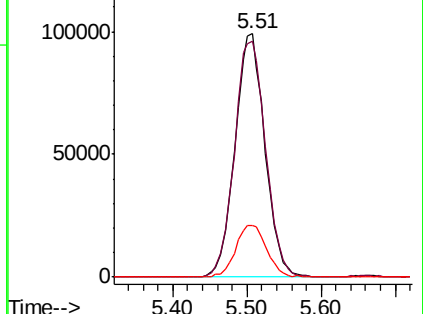



#36

1,1-Dichloropropene

Concen: 4.870 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.14 min

Lab File: VX007044.D

Acq: 14 Jan 2019 17:22

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion: 75 Resp: 38565

Ion Ratio Lower Upper

75 100

110 10.4 20.2 60.5#




77 0.4 24.8 37.2#

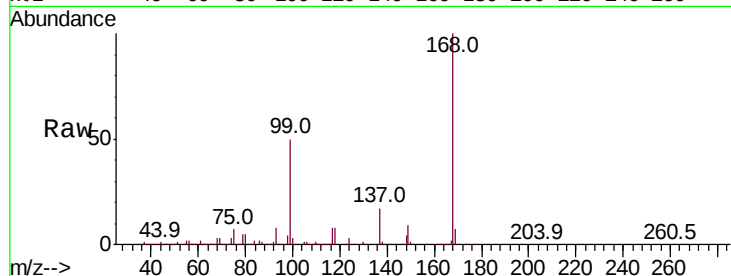

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

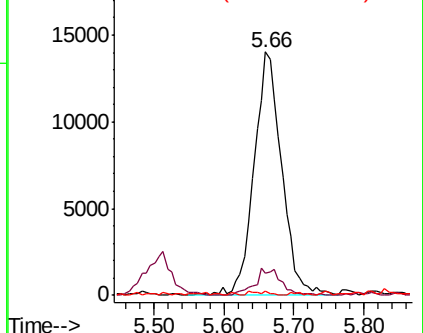

#37

Ethyl Acetate

Concen: 0.214 ug/l

RT: 4.70 min Scan# 581

Delta R.T. -0.16 min

Lab File: VX007044.D

Acq: 14 Jan 2019 17:22


Tgt Ion: 43 Resp: 1820

Ion Ratio Lower Upper

43 100

61 15.0 11.9 17.9



70 9.7 9.7 14.5




Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 70.00 (69.70 to 70.70): VX0

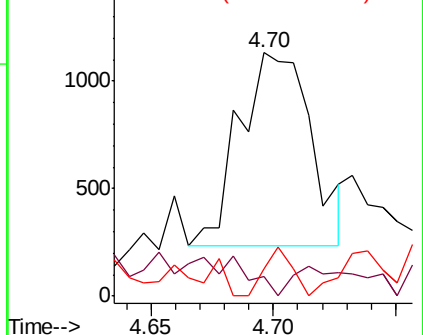

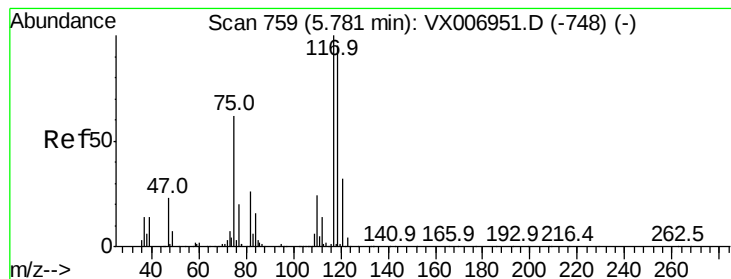

#38

Carbon Tetrachloride

Concen: 6.810 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.12 min

Lab File: VX007044.D

Acq: 14 Jan 2019 17:22

Instrument :

MSVOA_X

ClientSampled :


Tot Ion:117 Resp: 54256

Ion Ratio Lower Upper

117 100

119 3.6 79.4 119.2#




121 0.0 24.0 36.0#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

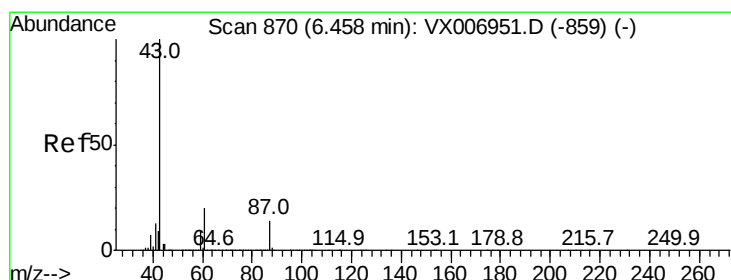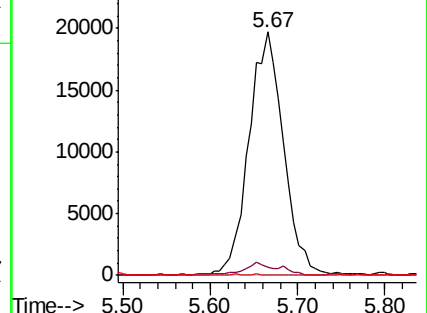

#43

Isopropyl Acetate

Concen: 1.652 ug/l

RT: 6.46 min Scan# 870

Delta R.T. 0.00 min

Lab File: VX007044.D

Acq: 14 Jan 2019 17:22


Tgt Ion: 43 Resp: 22125

Ion Ratio Lower Upper

43 100

61 24.6 16.8 25.2



87 18.1 12.4 18.6




Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

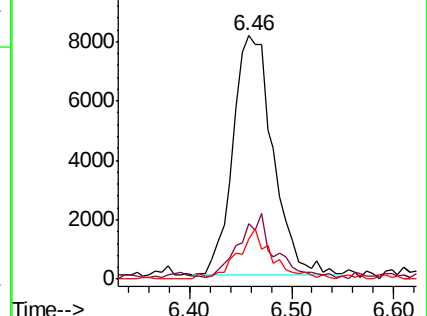



#48

Methvl methacrylate

Concen: 1.824 ug/l

RT: 7.68 min Scan# 1071





Delta R.T. -0.09 min

Lab File: VX007044.D

Acq: 14 Jan 2019 17:22

Instrument :
MSVOA_X
ClientSampleId :

Tot Ion:	41	Resp:	12544
Ion	Ratio	Lower	Upper
41	100		
69	0.9	72.4	108.6#
39	14.4	45.8	68.8#

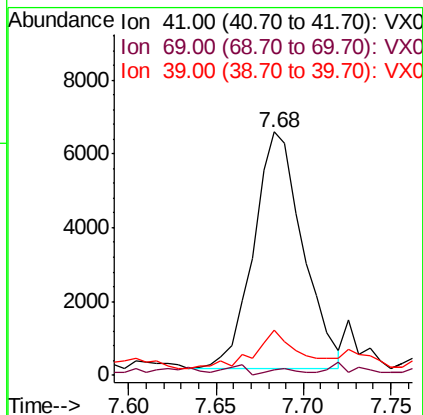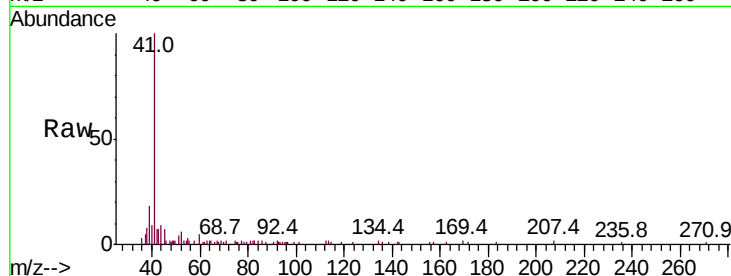

#49

1,4-Dioxane

Concen: Below Cal




RT: 7.74 min Scan# 1080


Delta R.T. -0.01 min

Lab File: VX007044.D

Acq: 14 Jan 2019 17:22

Tgt Ion:	88	Resp:	87
Ion	Ratio	Lower	Upper
88	100		
43	0.0	22.2	33.4#
58	0.0	51.0	76.4#

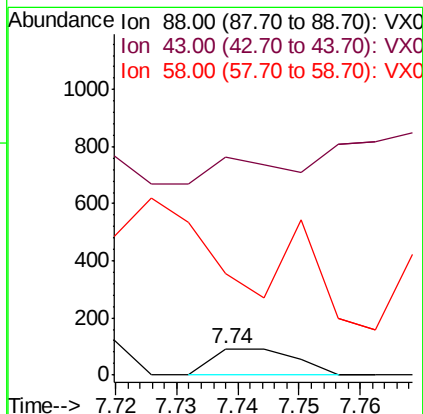

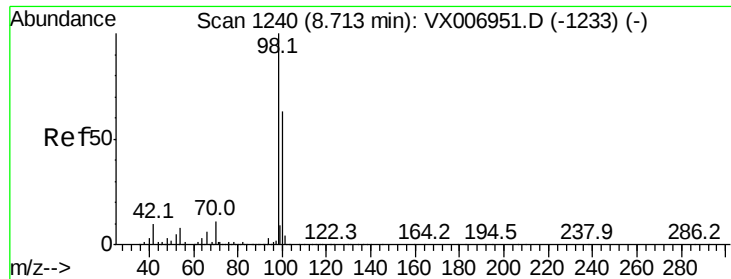

#50

Toluene-d8

Concen: 52.073 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX007044.D

Acq: 14 Jan 2019 17:22





Instrument :
MSVOA_X
ClientSampleId :

Tot Ion: 98 Resp: 1111742

Ion Ratio Lower Upper

98 100

100 63.5 52.0 78.0

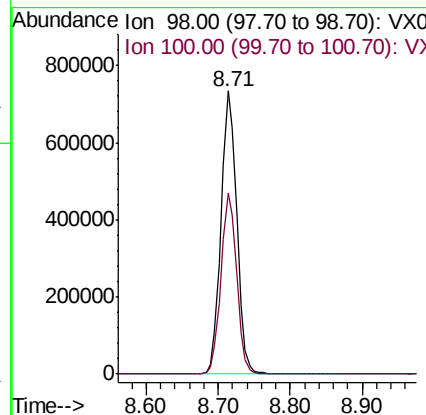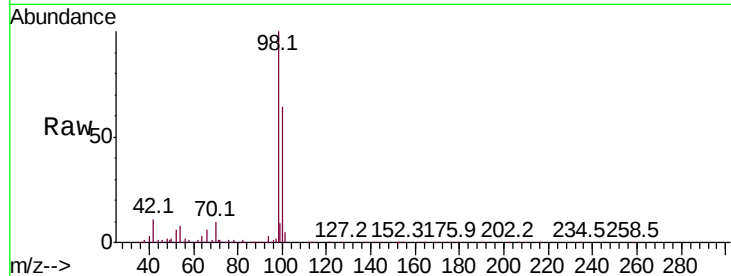

#51

4-Methyl-2-Pentanone

Concen: 15.028 ug/l

RT: 8.62 min Scan# 1224

Delta R.T. -0.03 min

Lab File: VX007044.D




Acq: 14 Jan 2019 17:22


Tgt Ion: 43 Resp: 129328

Ion Ratio Lower Upper

43 100

58 7.7 31.8 47.6#

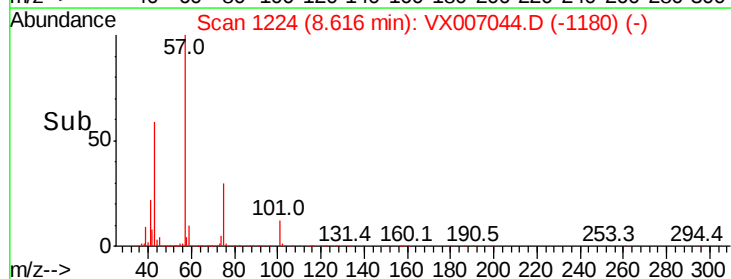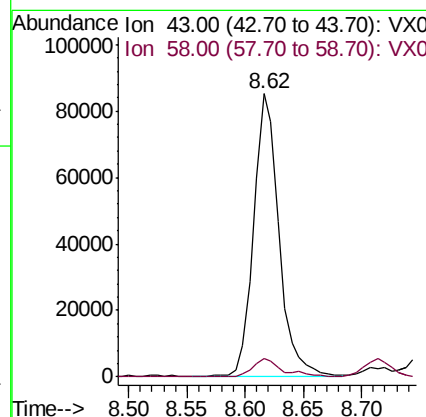

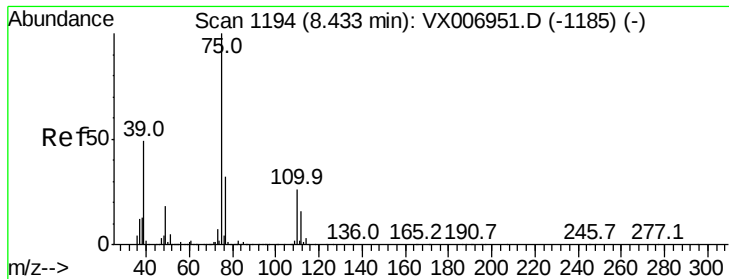

#54

cis-1,3-Dichloropropene

Concen: 7.226 ug/l

RT: 8.62 min Scan# 1224

Delta R.T. 0.18 min

Lab File: VX007044.D

Acq: 14 Jan 2019 17:22

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion: 75 Resp: 64304

Ion Ratio Lower Upper

75 100

77 0.3 26.2 39.2#




39 30.2 36.7 55.1#

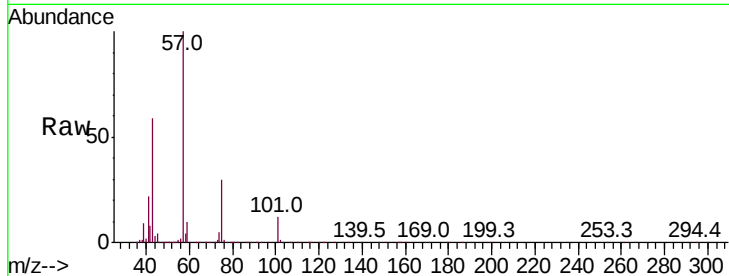

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 76.90 (76.60 to 77.60): VX0

Ion 39.00 (38.70 to 39.70): VX0

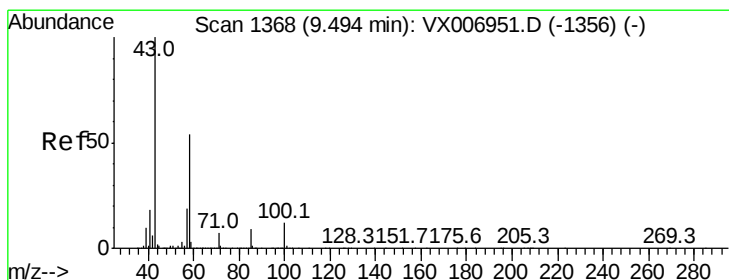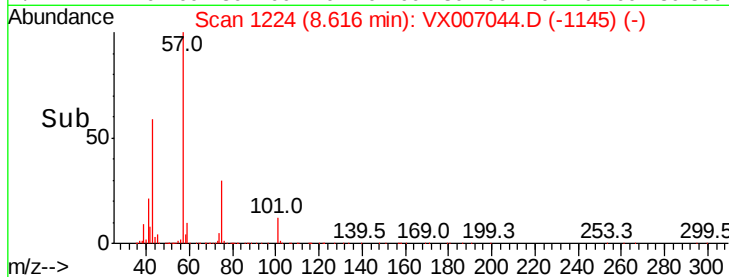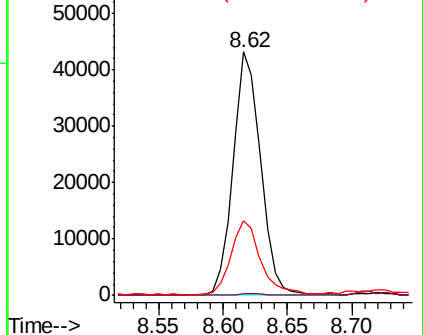

#59

2-Hexanone

Concen: 21.346 ug/l

RT: 9.54 min Scan# 1376

Delta R.T. 0.05 min

Lab File: VX007044.D


Acq: 14 Jan 2019 17:22

Tgt Ion: 43 Resp: 139989

Ion Ratio Lower Upper



43 100


58 20.3 27.7 83.1#

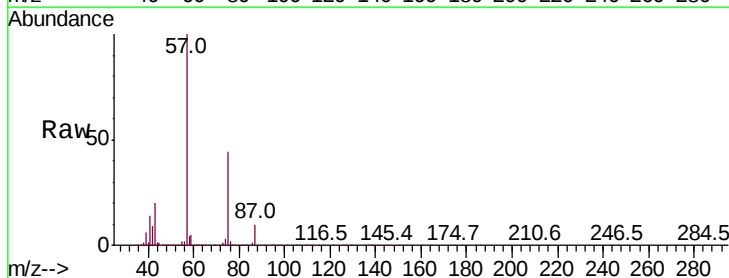

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0



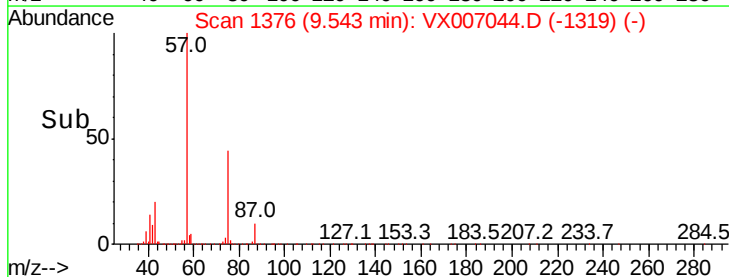
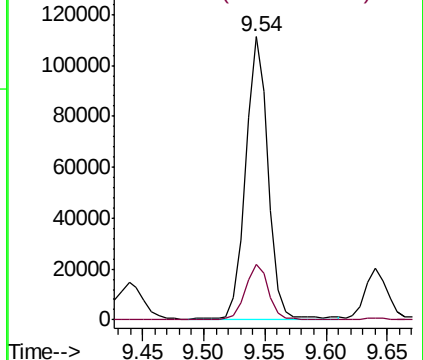


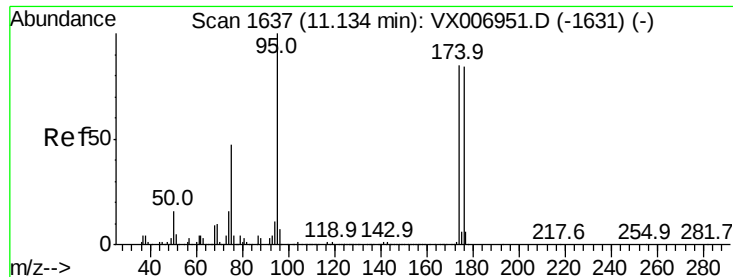

#62
4-Bromofluorobenzene
Concen: 53.375 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. 0.00 min
Lab File: VX007044.D
Acq: 14 Jan 2019 17:22




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 95 Resp: 397272
Ion Ratio Lower Upper
95 100
174 93.2 0.0 182.2
176 90.3 0.0 178.8

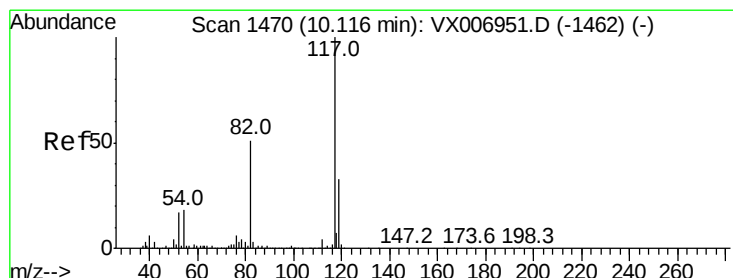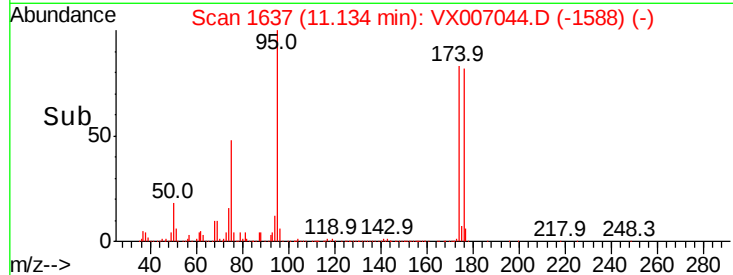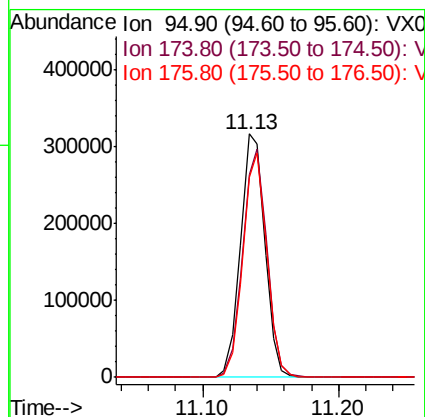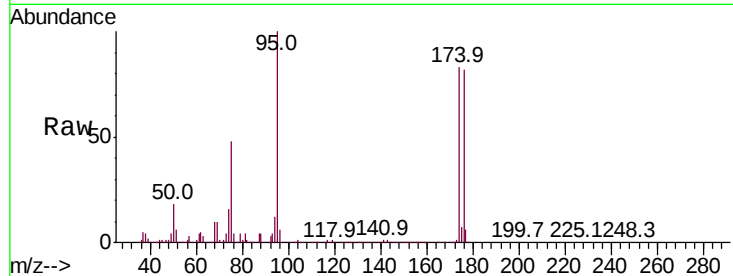

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.01 min
Lab File: VX007044.D
Acq: 14 Jan 2019 17:22

Tgt Ion: 117 Resp: 872962
Ion Ratio Lower Upper
117 100
82 52.8 41.0 61.6
119 32.1 25.4 38.0

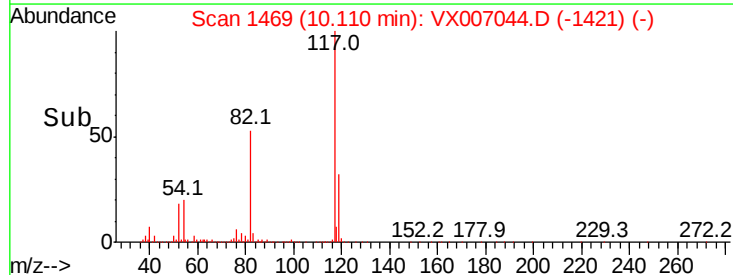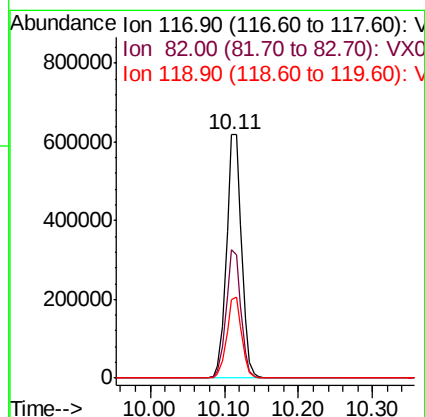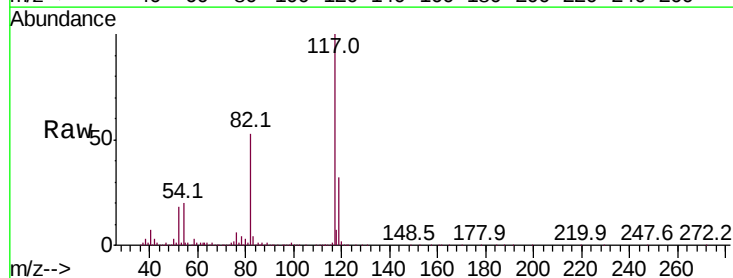

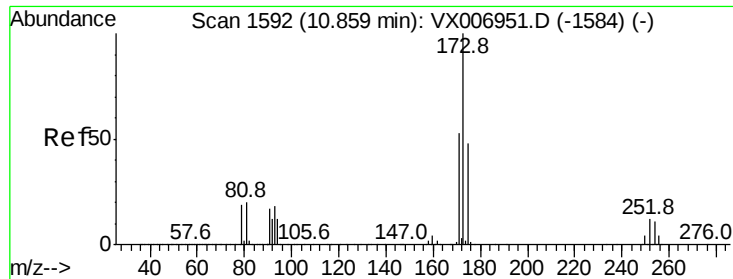

#71

Bromoform

Concen: 4.747 ug/l

RT: 10.76 min Scan# 1576

Delta R.T. -0.10 min

Lab File: VX007044.D

Acq: 14 Jan 2019 17:22

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:173 Resp: 125

Ion Ratio Lower Upper

173 100

175 0.0 24.7 74.1#




254 17.6 0.2 0.2#

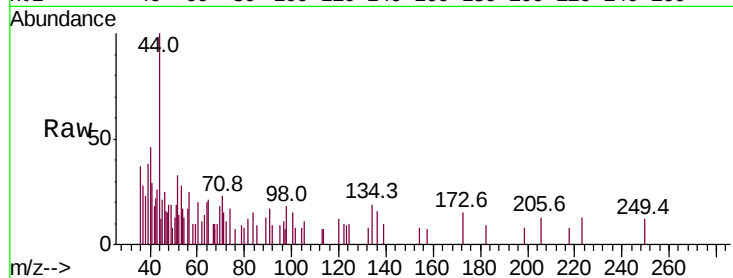

Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

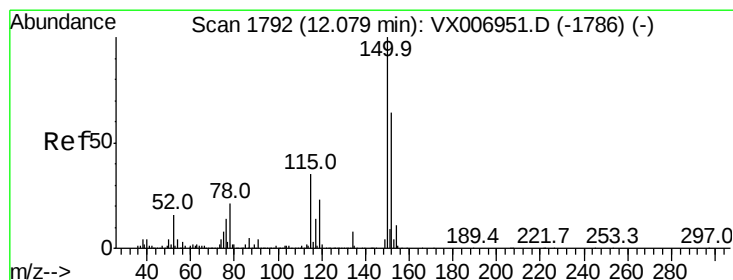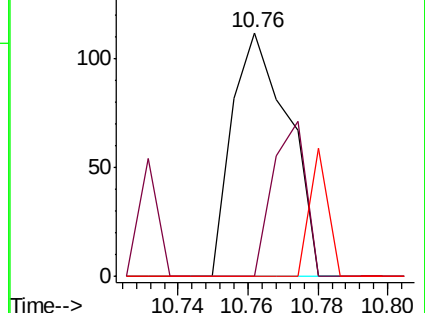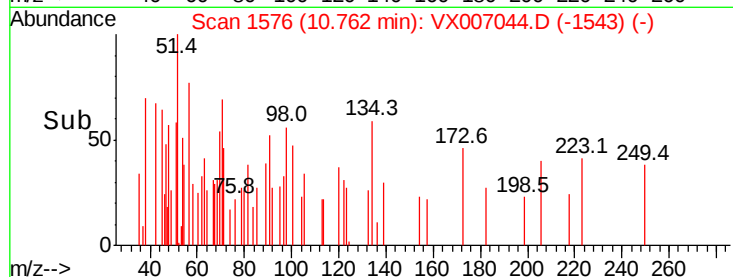

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. 0.00 min

Lab File: VX007044.D

Acq: 14 Jan 2019 17:22


Tgt Ion:152 Resp: 434699

Ion Ratio Lower Upper

152 100

115 52.9 39.1 117.2



150 153.8 0.0 344.8

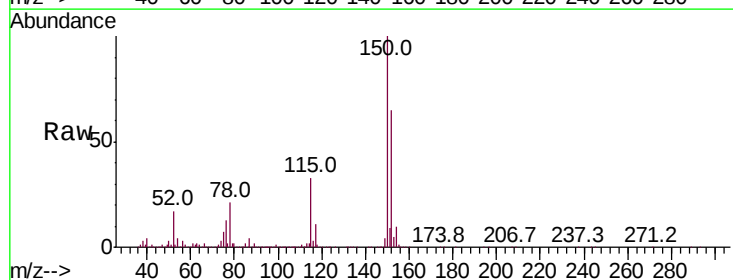


Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

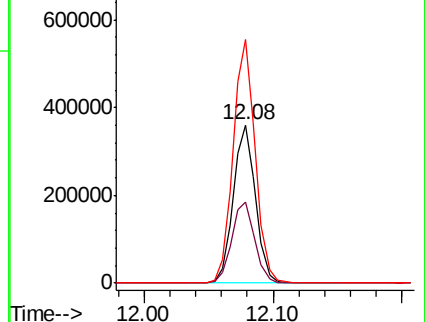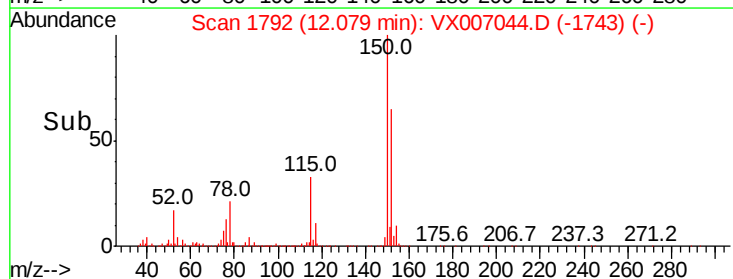

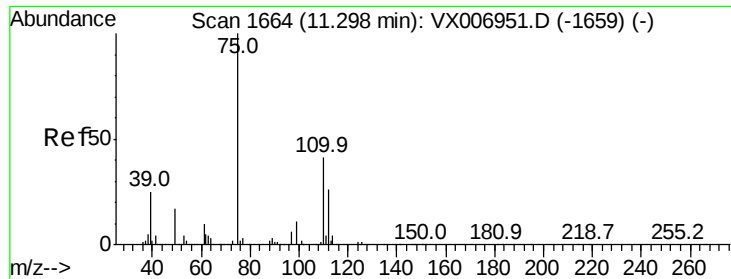

#76

1,2,3-Trichloropropane

Concen: 21.493 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.16 min

Lab File: VX007044.D

Acq: 14 Jan 2019 17:22

Instrument :

MSVOA_X





ClientSampleId :

Tot Ion: 75 Resp: 189334

Ion Ratio Lower Upper

75 100

77 1.4 18.5 55.5#

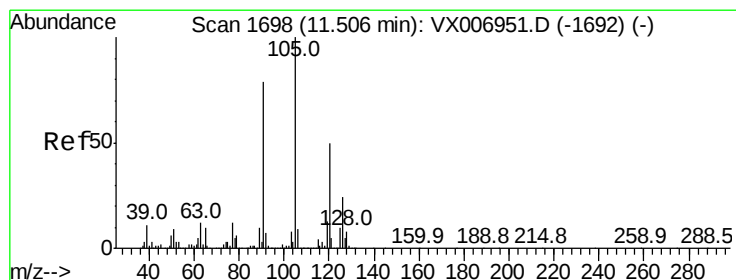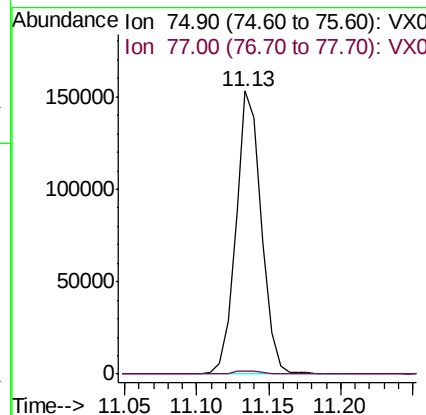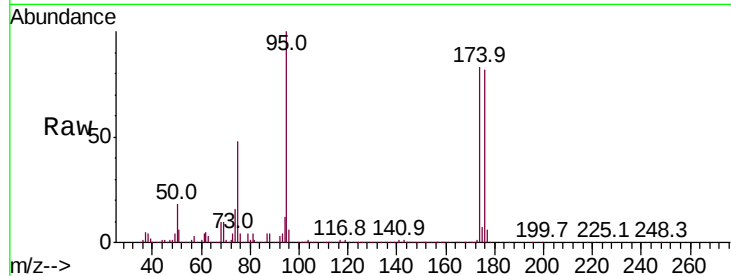

#80

1,3,5-Trimethylbenzene

Concen: 0.209 ug/l

RT: 11.51 min Scan# 1698

Delta R.T. 0.00 min

Lab File: VX007044.D




Acq: 14 Jan 2019 17:22


Tgt Ion:105 Resp: 5341

Ion Ratio Lower Upper

105 100

120 49.2 25.1 75.3

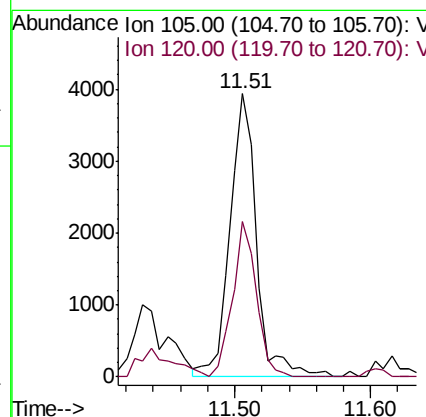

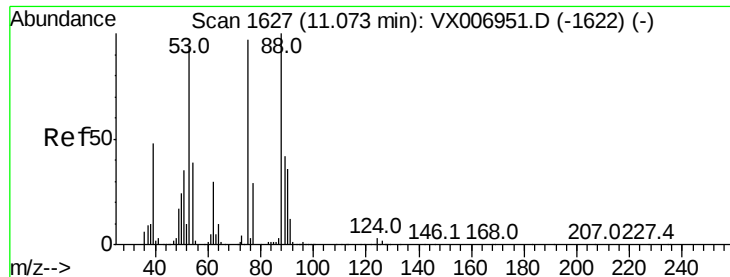

#81

trans-1,4-Dichloro-2-butene

Concen: 63.739 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.06 min

Lab File: VX007044.D

Acq: 14 Jan 2019 17:22

Instrument :

MSVOA_X

ClientSampleId :





Tot Ion: 75 Resp: 189334

Ion Ratio Lower Upper

75 100

53 0.0 79.7 119.5#

89 0.2 38.0 57.0#

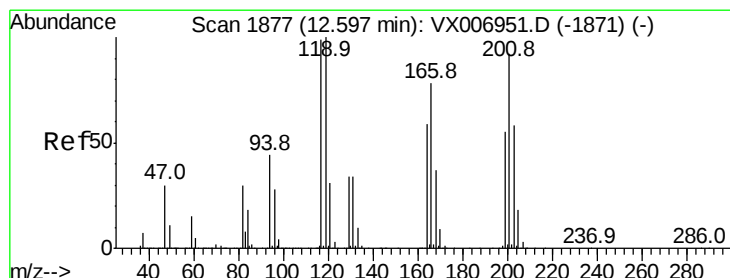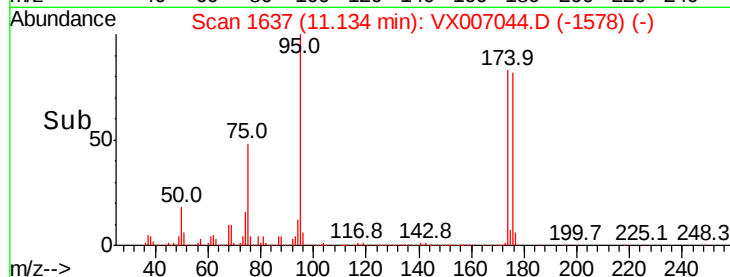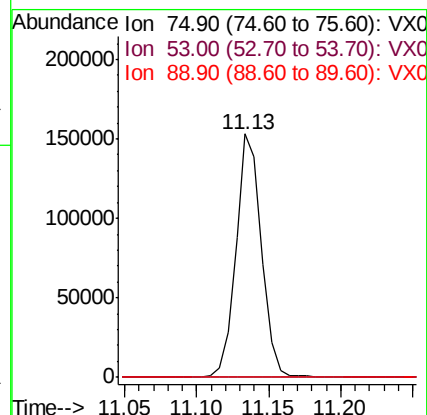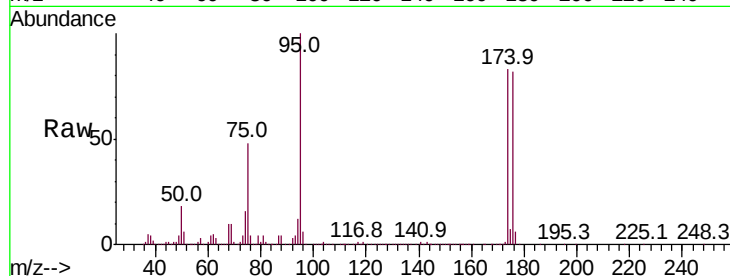

#90

Hexachloroethane

Concen: 2.929 ug/l

RT: 12.59 min Scan# 1876

Delta R.T. -0.01 min

Lab File: VX007044.D




Acq: 14 Jan 2019 17:22


Tgt Ion: 117 Resp: 96

Ion Ratio Lower Upper

117 100

201 0.0 42.9 128.7#

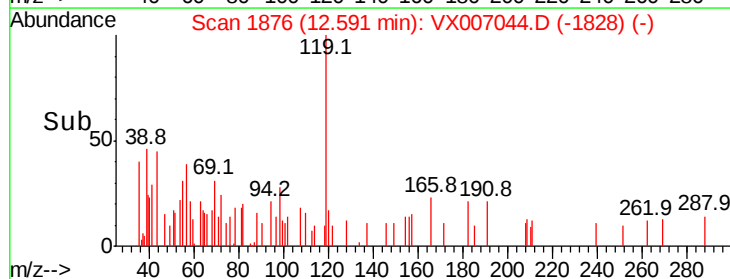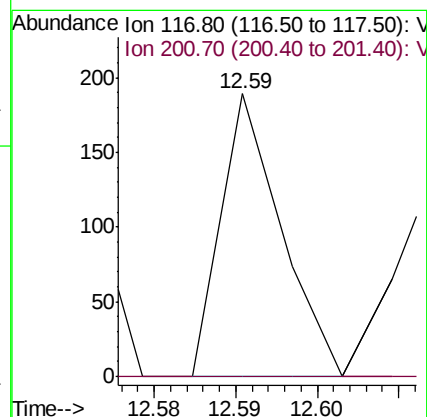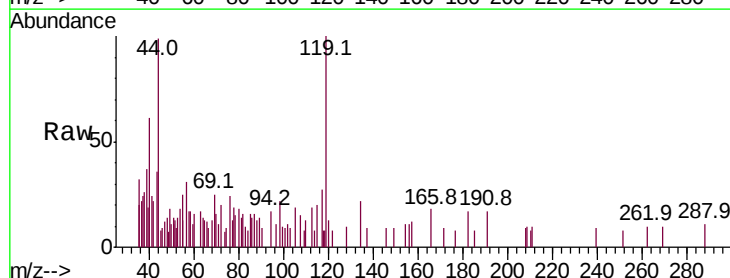

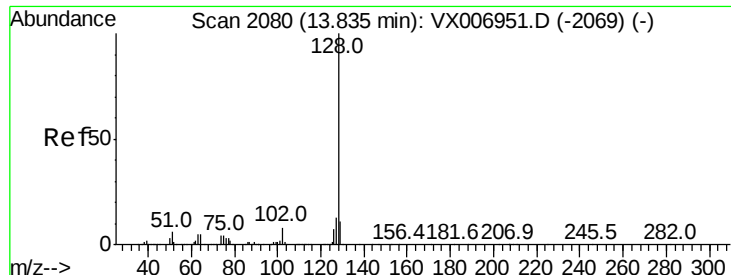

#95
Naphthalene
Concen: 0.970 ug/l
RT: 13.83 min Scan# 2080
Delta R.T. 0.00 min
Lab File: VX007044.D
Acq: 14 Jan 2019 17:22

Instrument :
MSVOA_X
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
128	100		
127	14.3	10.1	15.1
129	12.2	8.6	13.0

