

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX011419\
 Data File : VX007046.D
 Acq On : 14 Jan 2019 18:16
 Operator : JC/SP
 Sample : K1128-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 15 00:30:44 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 08 14:06:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	603101	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	923361	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	880947	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	431943	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	322826	51.22	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.44%	
35) Dibromofluoromethane	5.51	113	286592	48.47	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.94%	
50) Toluene-d8	8.71	98	1129006	52.16	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.32%	
62) 4-Bromofluorobenzene	11.13	95	403619	53.49	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.98%	


Target Compounds					Qvalue	
3) Chloromethane	1.33	50	1922	0.333	ug/l	93
5) Bromomethane	1.64	94	1441	0.217	ug/l	98
11) Tert butyl alcohol	3.02	59	4583	3.082	ug/l #	86
13) Acrolein	2.29	56	80	3.207	ug/l #	13
14) Allyl chloride	2.86	41	69664	7.333	ug/l #	25
16) Acetone	2.45	43	22504	7.222	ug/l	97
18) Methyl Acetate	2.78	43	20088	2.226	ug/l	94
20) Methylene Chloride	2.86	84	1960391	333.994	ug/l	96
25) 2-Butanone	4.71	43	3492	0.783	ug/l #	80
29) Tetrahydrofuran	5.17	42	1292	0.446	ug/l #	47
30) Chloroform	5.22	83	2630	0.252	ug/l	91
36) 1,1-Dichloropropene	5.66	75	39023	4.861	ug/l #	49
38) Carbon Tetrachloride	5.67	117	53094	6.573	ug/l #	14
43) Isopropyl Acetate	6.46	43	24197	1.782	ug/l	96
48) Methyl methacrylate	7.69	41	13546	1.943	ug/l #	12
49) 1,4-Dioxane	7.80	88	130	Below Cal	#	1
51) 4-Methyl-2-Pentanone	8.62	43	131121	15.029	ug/l #	46
54) cis-1,3-Dichloropropene	8.62	75	65665	7.279	ug/l #	61
57) 1,3-Dichloropropane	9.54	76	13659	1.323	ug/l #	44
59) 2-Hexanone	9.54	43	175088	26.334	ug/l #	51
68) m/p-Xylenes	10.36	106	4853	0.388	ug/l	98
69) o-Xylene	10.70	106	2472	0.203	ug/l	96
76) 1,2,3-Trichloropropane	11.13	75	189404	21.638	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.51	105	9304	0.366	ug/l	97
81) trans-1,4-Dichloro-2-buten	11.13	75	189404	64.144	ug/l #	10
84) 1,2,4-Trimethylbenzene	11.80	105	23099	0.903	ug/l	98
88) 1,4-Dichlorobenzene	12.10	146	1308	0.236	ug/l #	1
90) Hexachloroethane	12.60	117	393	2.994	ug/l #	6
95) Naphthalene	13.83	128	97894	3.146	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX011419\
Data File : VX007046.D
Acq On : 14 Jan 2019 18:16
Operator : JC/SP
Sample : K1128-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jan 15 00:30:44 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 08 14:06:59 2019
Response via : Initial Calibration

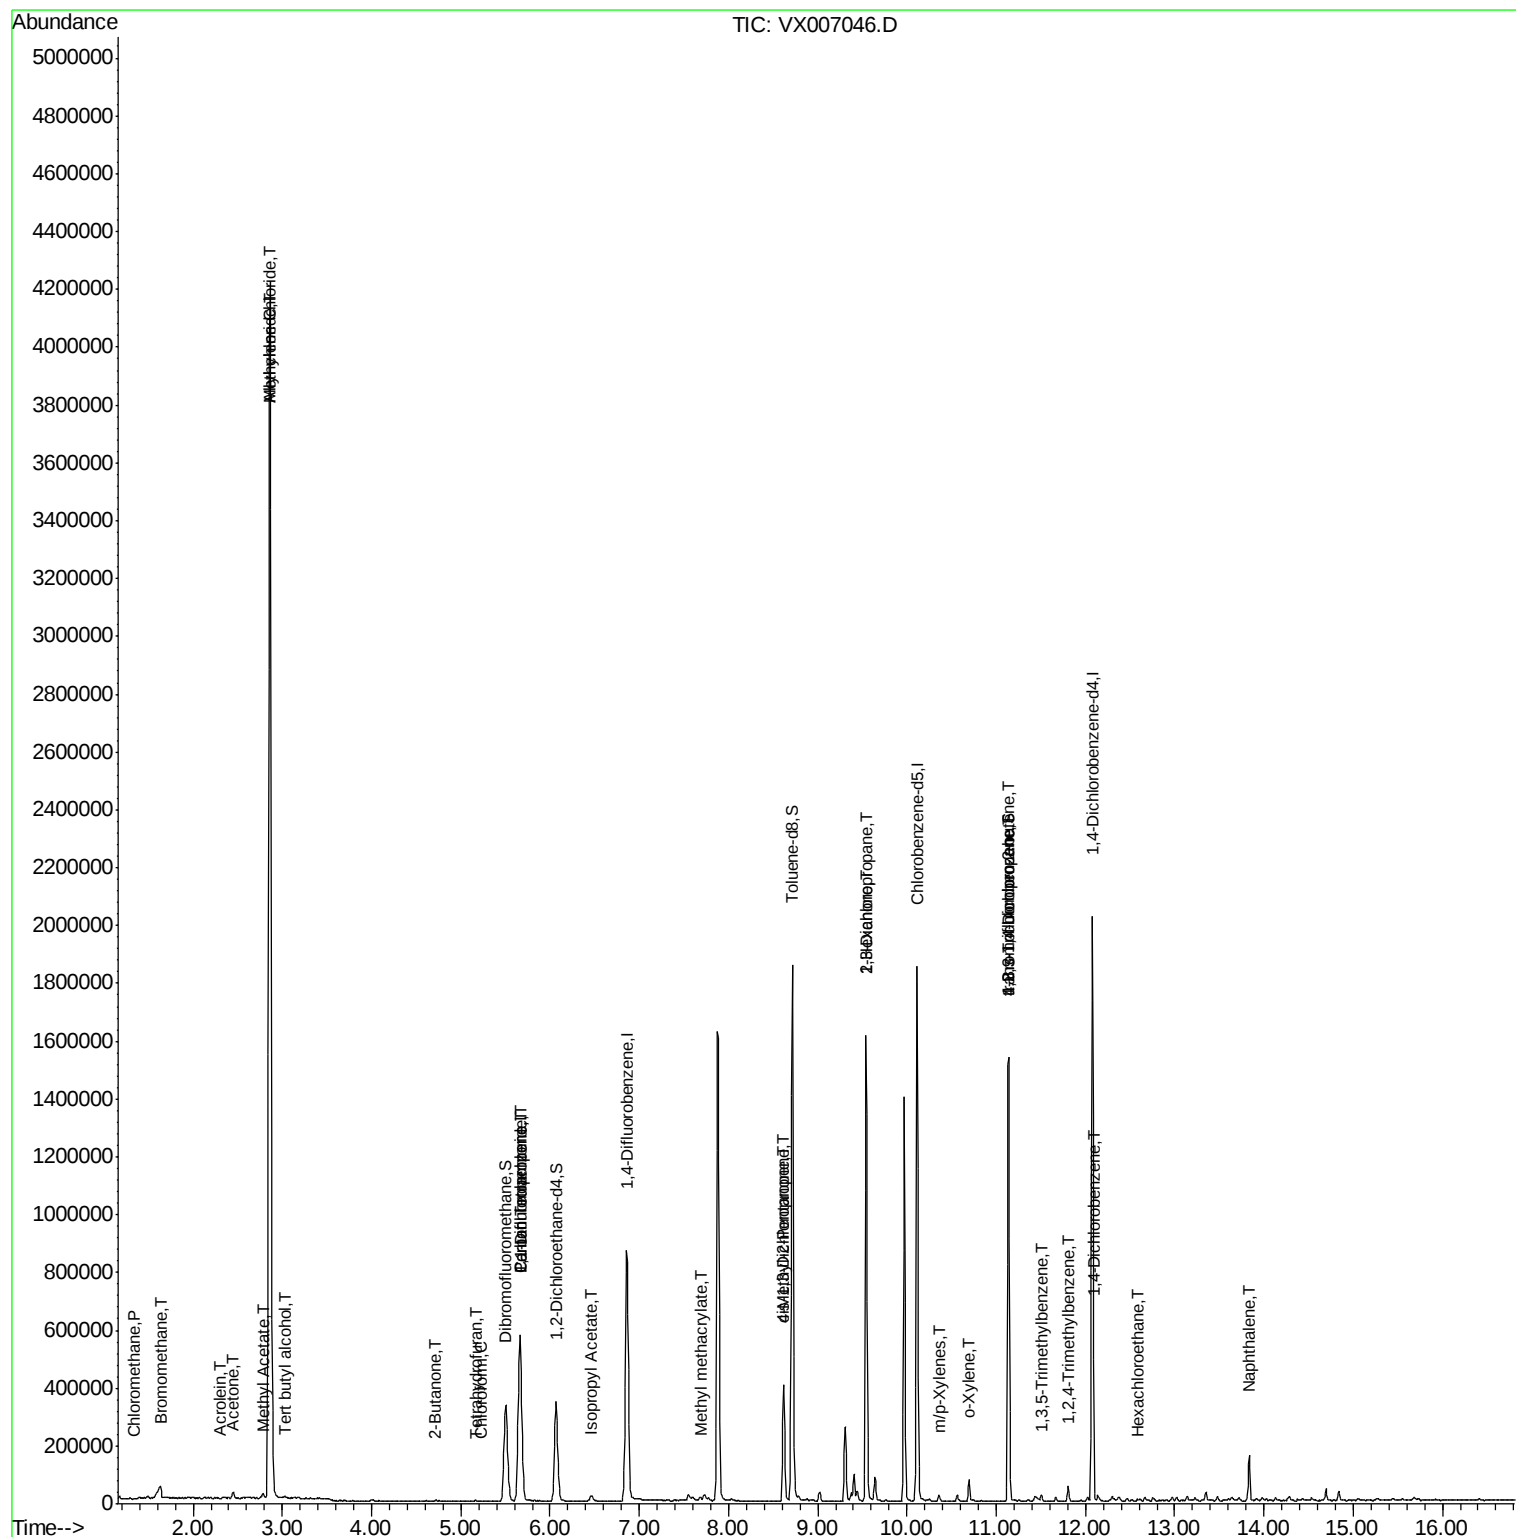

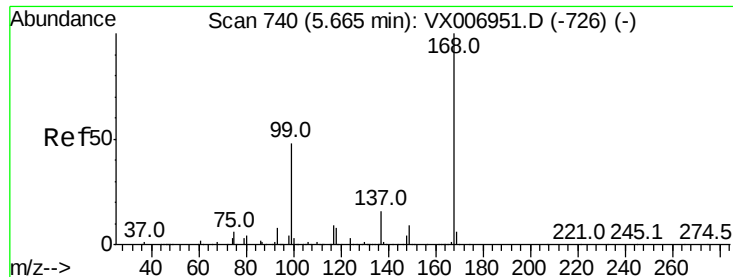

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.00 min

Lab File: VX007046.D

Acq: 14 Jan 2019 18:16


Instrument :
MSVOA_X
ClientSampleId :

Tot Ion:168 Resp: 603101

Ion Ratio Lower Upper

168 100

99 50.8 41.8 62.8

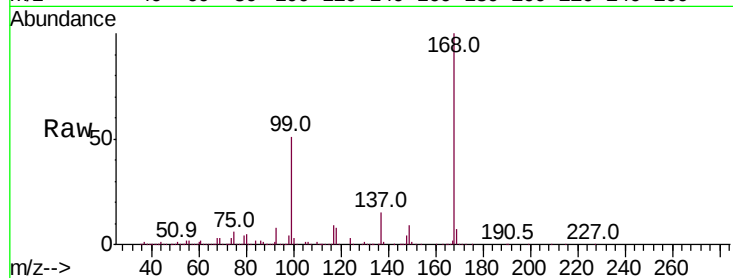

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

200000



150000

100000

50000

0

Time-->

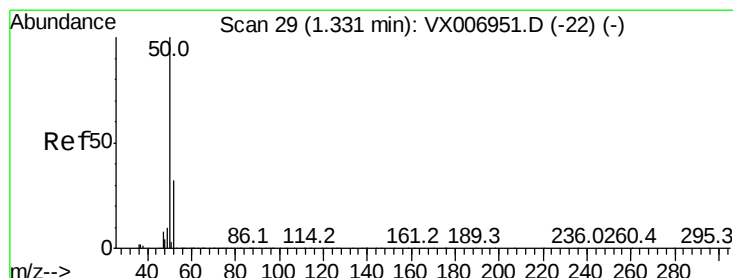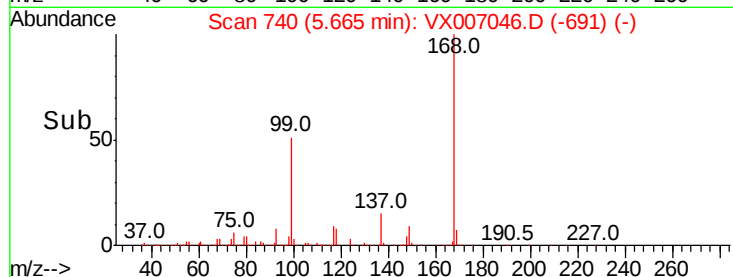

#3

Chloromethane

Concen: 0.333 ug/l

RT: 1.33 min Scan# 29

Delta R.T. -0.00 min

Lab File: VX007046.D


Acq: 14 Jan 2019 18:16

Tgt Ion: 50 Resp: 1922

Ion Ratio Lower Upper

50 100

52 35.6 25.4 38.2

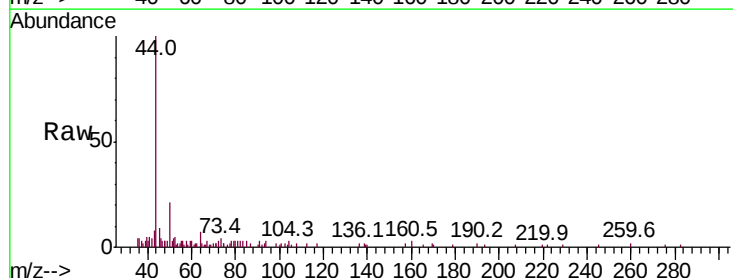

Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.33

1200

1000

800


600


400

200

0

Time-->

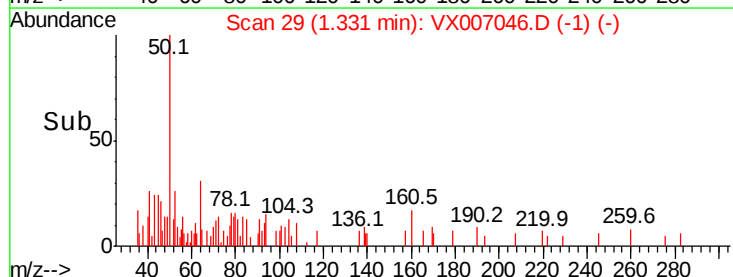

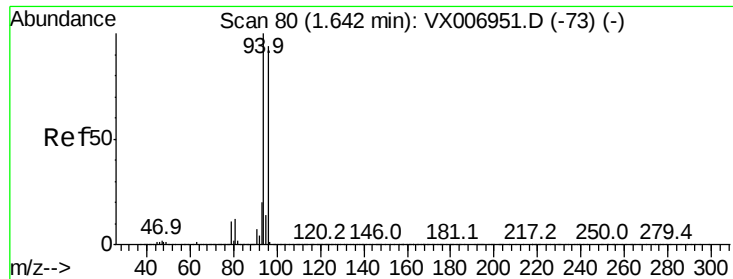

#5

Bromomethane

Concen: 0.217 ug/l

RT: 1.64 min Scan# 80

Delta R.T. -0.00 min

Lab File: VX007046.D

Acq: 14 Jan 2019 18:16

Instrument :

MSVOA_X





ClientSampleId :

Tot Ion: 94 Resp: 1441

Ion Ratio Lower Upper

94 100

96 93.8 73.4 110.2

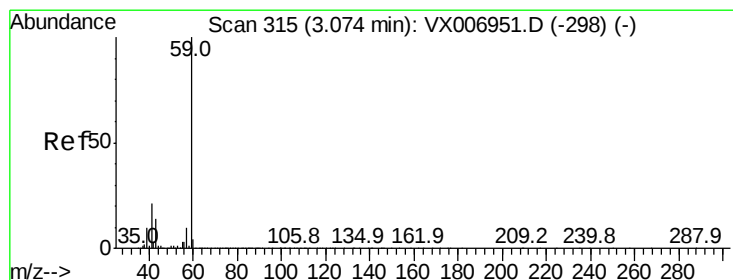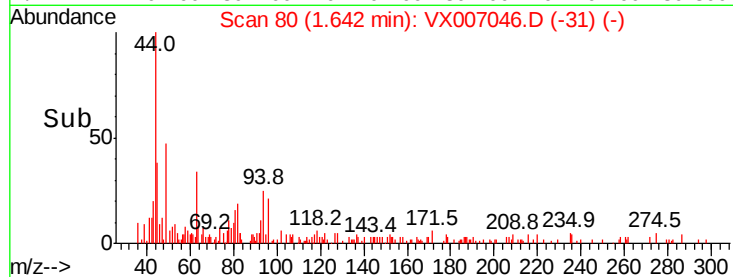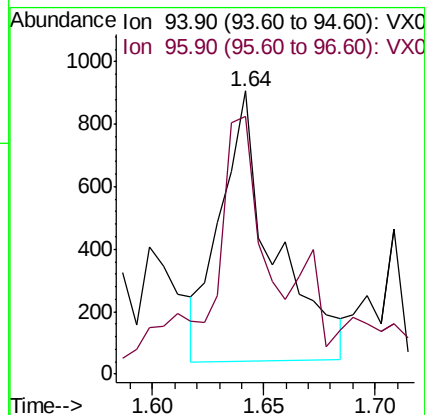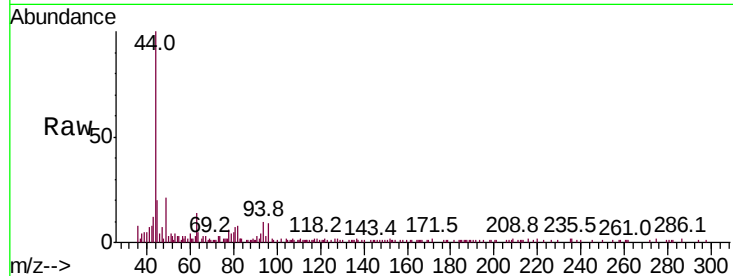

#11

Tert butyl alcohol

Concen: 3.082 ug/l

RT: 3.02 min Scan# 306

Delta R.T. -0.05 min

Lab File: VX007046.D




Acq: 14 Jan 2019 18:16


Tgt Ion: 59 Resp: 4583

Ion Ratio Lower Upper

59 100

57 5.3 8.5 12.7#

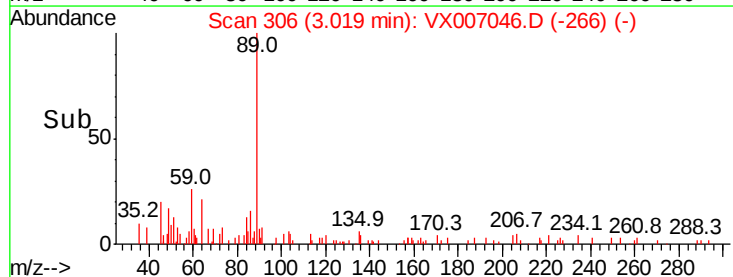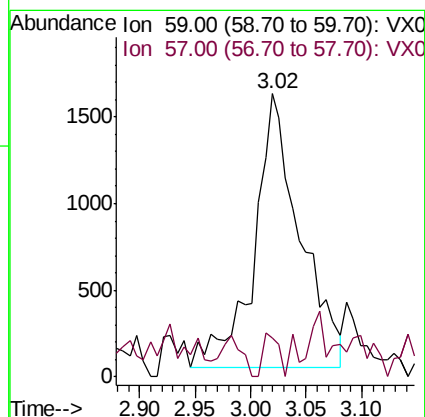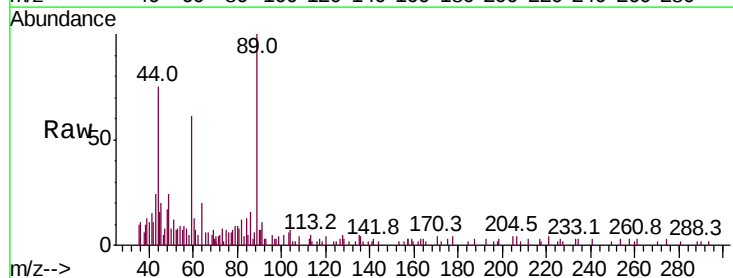

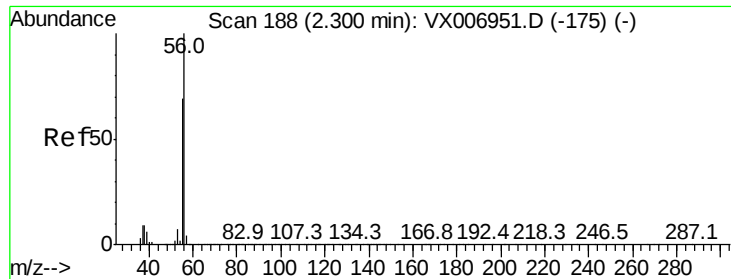

#13

Acrolein

Concen: 3.207 ug/l

RT: 2.29 min Scan# 187

Delta R.T. -0.01 min

Lab File: VX007046.D

Acq: 14 Jan 2019 18:16





Instrument :
MSVOA_X
ClientSampleId :

Tot Ion: 56 Resp: 80

Ion Ratio Lower Upper

56 100

55 0.0 58.2 87.4#

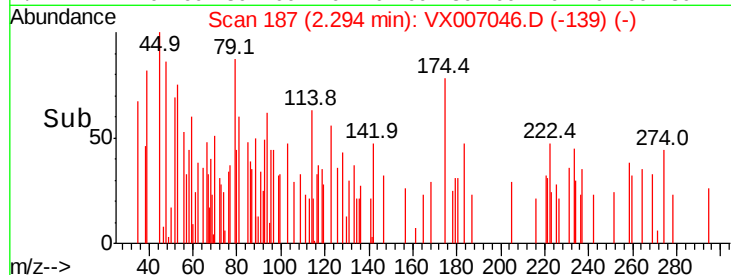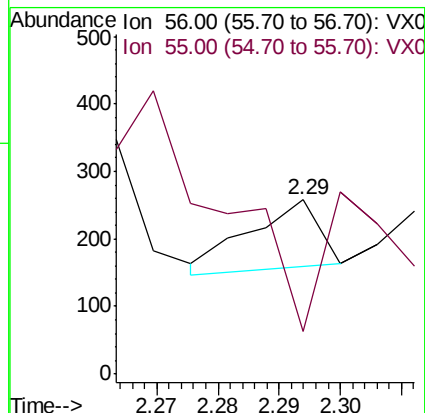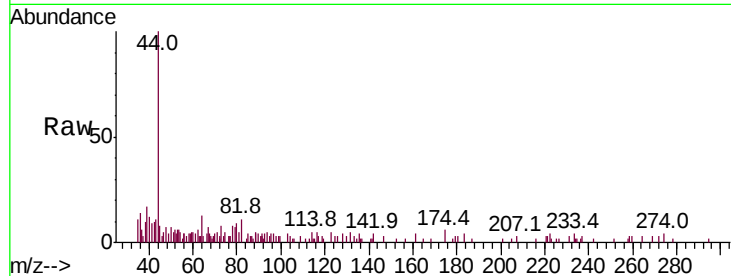

#14

Allyl chloride

Concen: 7.333 ug/l

RT: 2.86 min Scan# 280

Delta R.T. 0.13 min

Lab File: VX007046.D

Acq: 14 Jan 2019 18:16




Tgt Ion: 41 Resp: 69664


Ion Ratio Lower Upper

41 100

39 0.0 53.6 80.4#

76 0.0 27.4 41.2#


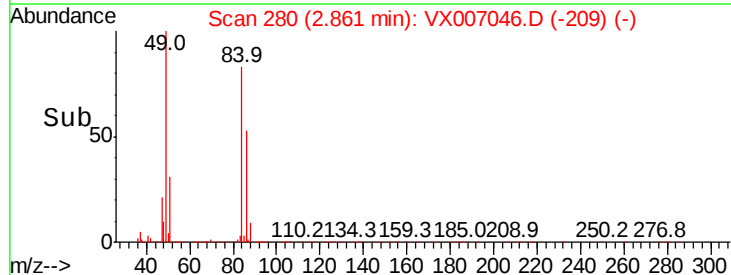
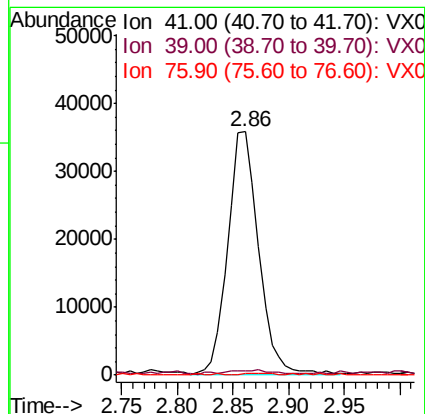



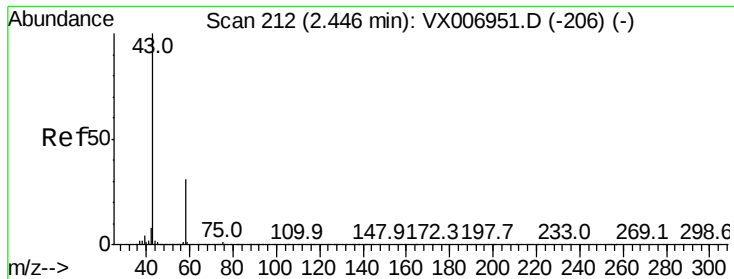

#16
Acetone
Concen: 7.222 ug/l
RT: 2.45 min Scan# 212
Delta R.T. -0.00 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 43 Resp: 22504
Ion Ratio Lower Upper
43 100
58 29.8 25.0 37.6

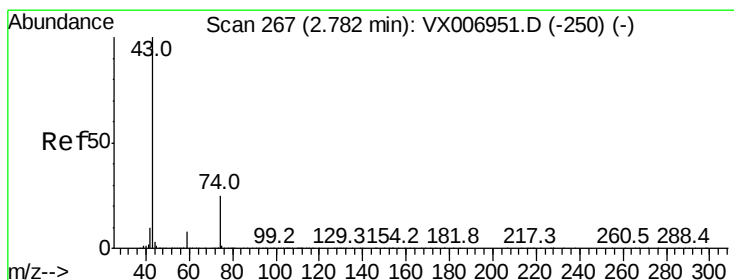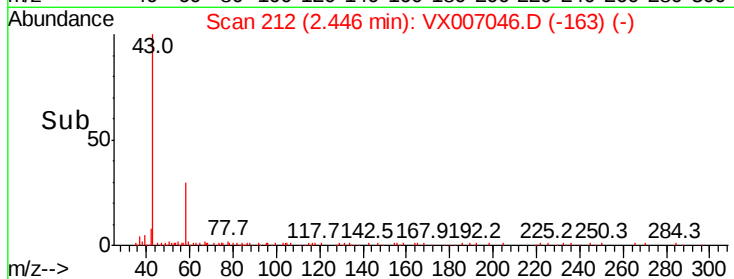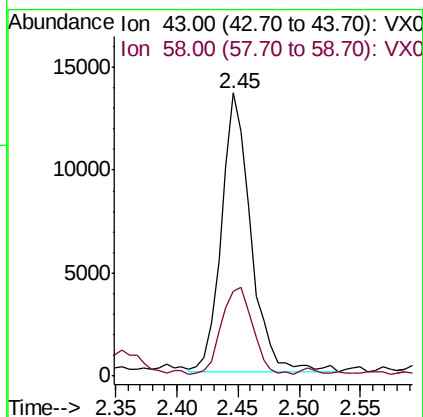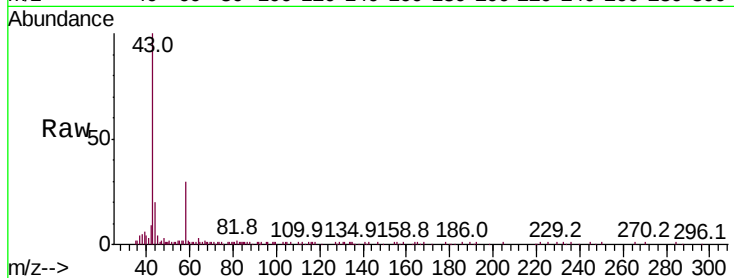

#18
Methyl Acetate
Concen: 2.226 ug/l
RT: 2.78 min Scan# 267
Delta R.T. -0.00 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16

Tgt Ion: 43 Resp: 20088
Ion Ratio Lower Upper
43 100
74 26.1 18.6 28.0


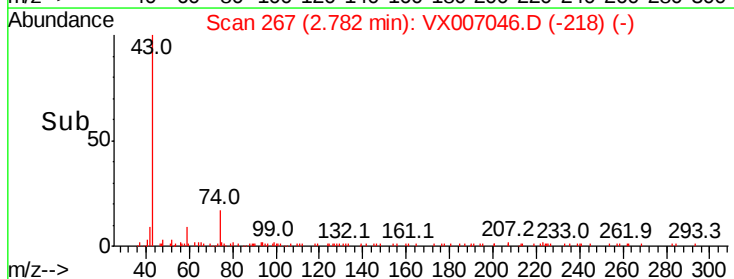
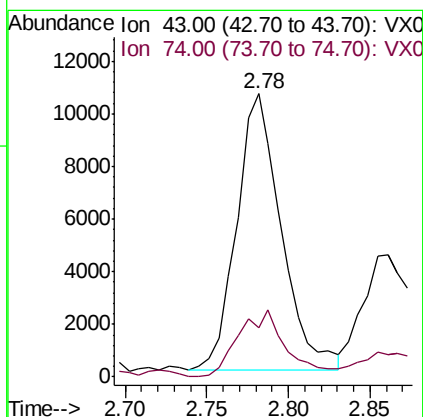
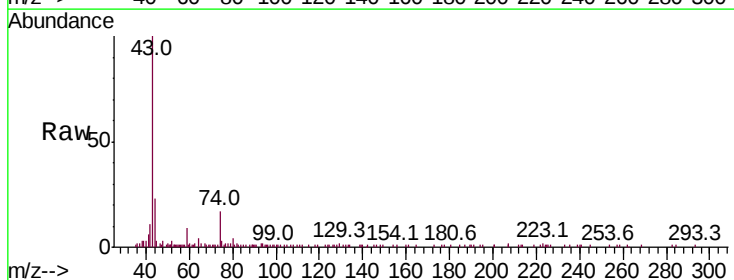


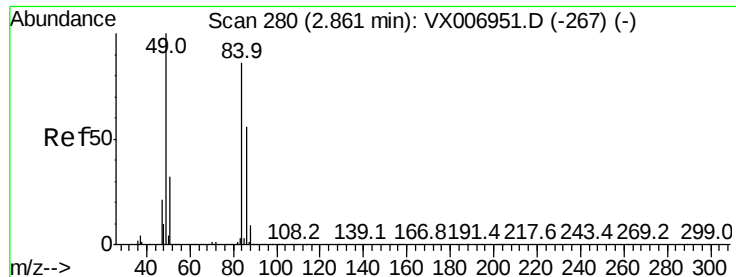

#20
Methvlene Chloride
Concen: 333.994 ug/l
RT: 2.86 min Scan# 280
Delta R.T. 0.00 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion:	84	Resp:	1960391
Ion	Ratio	Lower	Upper
84	100		
49	121.0	91.8	137.6
51	37.6	28.5	42.7
86	64.5	50.2	75.2

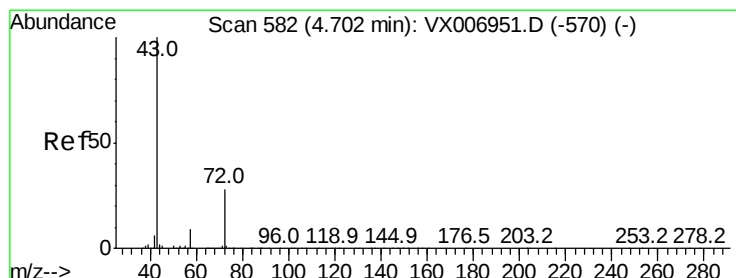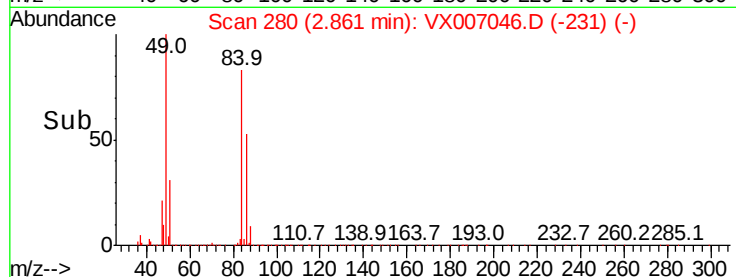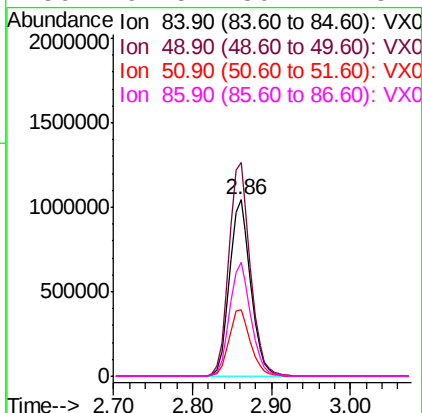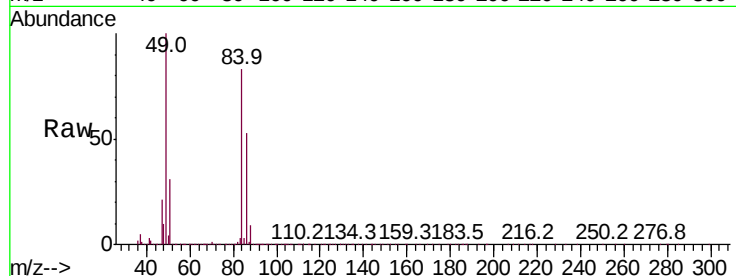

#25
2-Butanone
Concen: 0.783 ug/l
RT: 4.71 min Scan# 584
Delta R.T. 0.01 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16

Tgt Ion:	43	Resp:	3492
Ion	Ratio	Lower	Upper
43	100		
72	17.5	22.4	33.6#


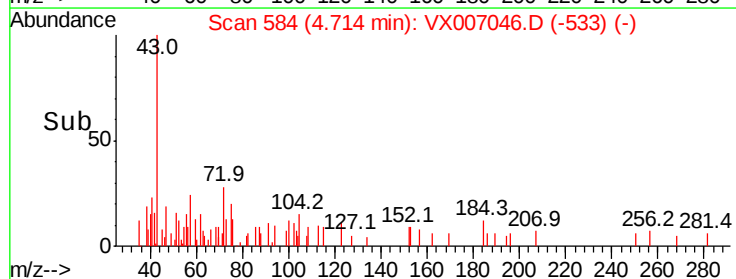
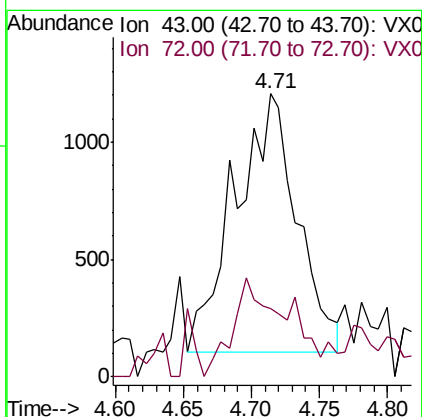
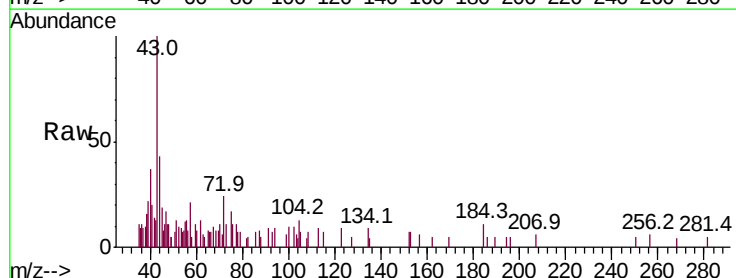


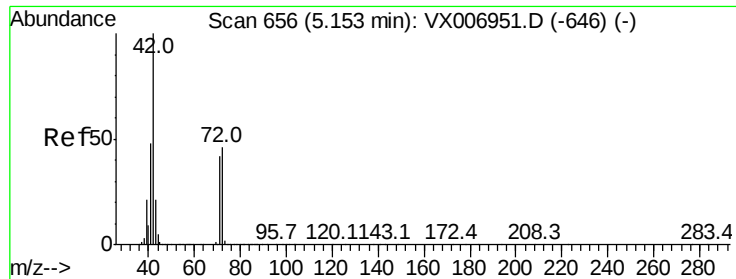

#29
Tetrahydrofuran
Concen: 0.446 ug/l
RT: 5.17 min Scan# 659
Delta R.T. 0.02 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16




Instrument :
MSVOA_X
ClientSampled :


Tot Ion: 42 Resp: 1292
Ion Ratio Lower Upper
42 100
72 19.3 38.9 58.3#
71 87.0 36.2 54.4#

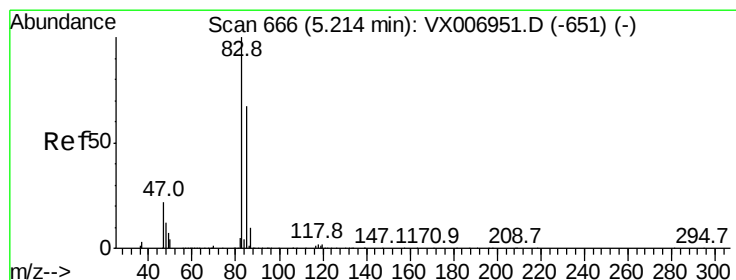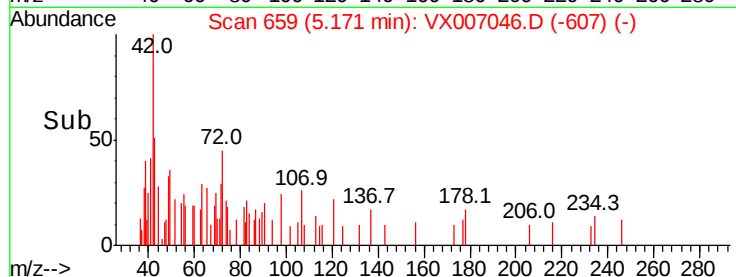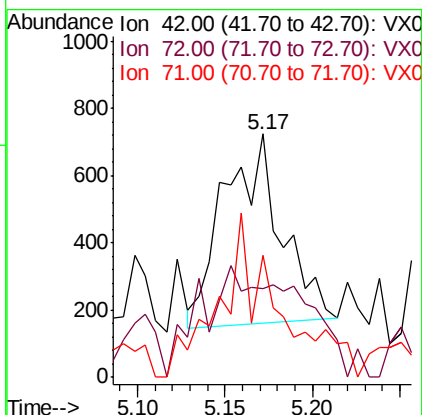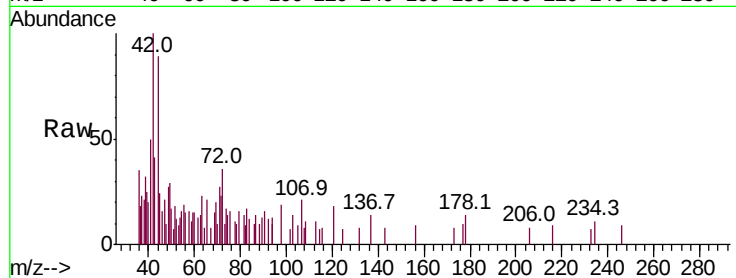

#30
Chloroform
Concen: 0.252 ug/l
RT: 5.22 min Scan# 667
Delta R.T. 0.01 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16

Tgt Ion: 83 Resp: 2630
Ion Ratio Lower Upper
83 100
85 70.8 51.2 76.8

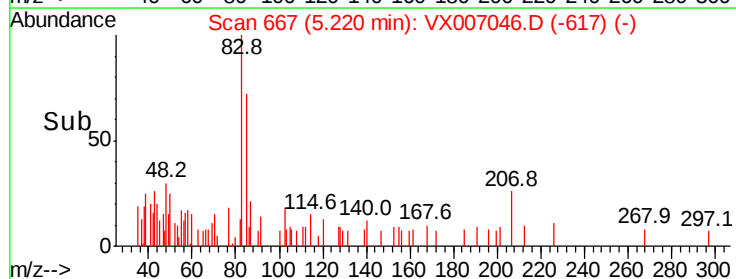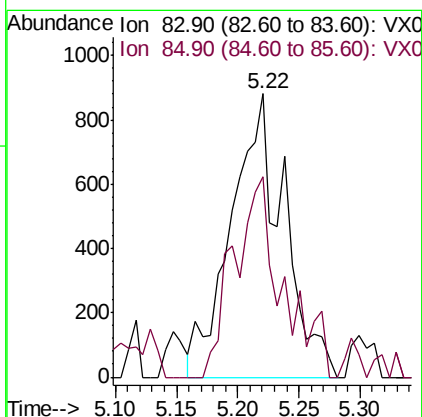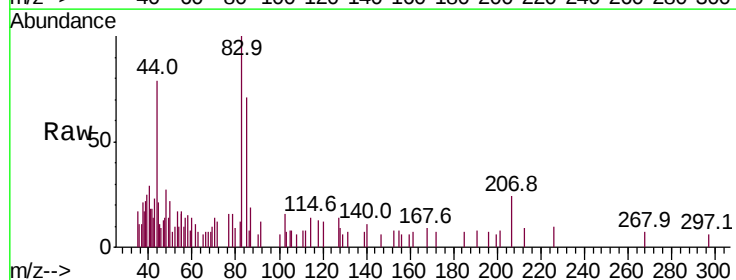



#33

1,2-Dichloroethane-d4

Concen: 51.218 ug/l

RT: 6.07 min Scan# 806

Delta R.T. -0.00 min

Lab File: VX007046.D

Acq: 14 Jan 2019 18:16

Instrument :

MSVOA_X


ClientSampled :

Tot Ion: 65 Resp: 322826

Ion Ratio Lower Upper




65 100

67 53.7 0.0 105.0

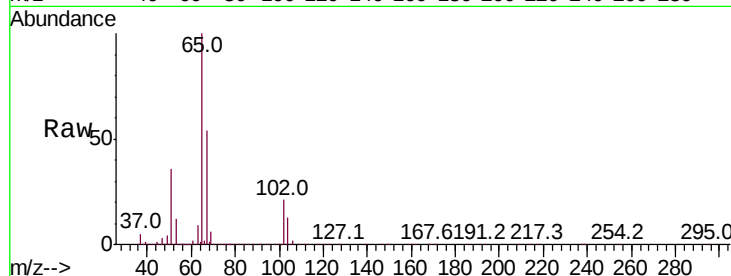

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

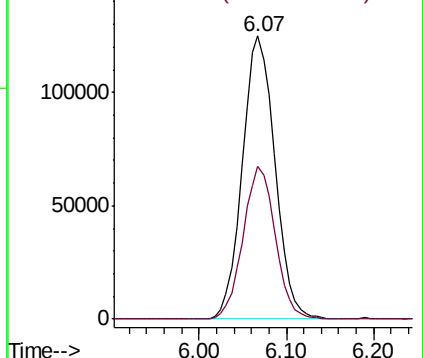

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX007046.D

Acq: 14 Jan 2019 18:16


Tgt Ion: 114 Resp: 923361

Ion Ratio Lower Upper

114 100

63 17.9 0.0 34.8



88 14.3 0.0 28.8




Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0




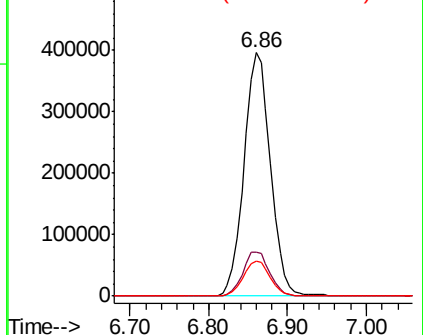


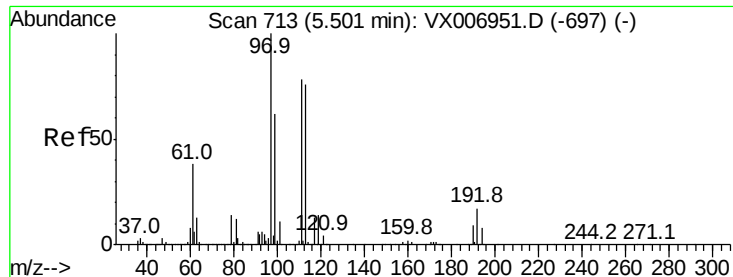

#35
Dibromofluoromethane
Concen: 48.467 ug/l
RT: 5.51 min Scan# 714
Delta R.T. 0.01 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion:113 Resp: 286592
Ion Ratio Lower Upper
113 100
111 101.4 81.6 122.4
192 21.5 16.7 25.1

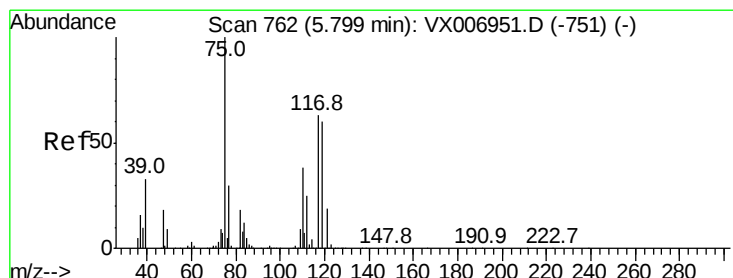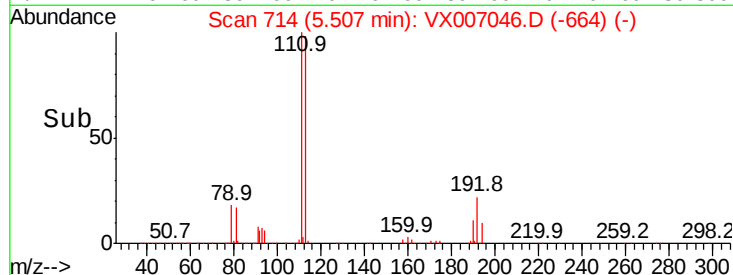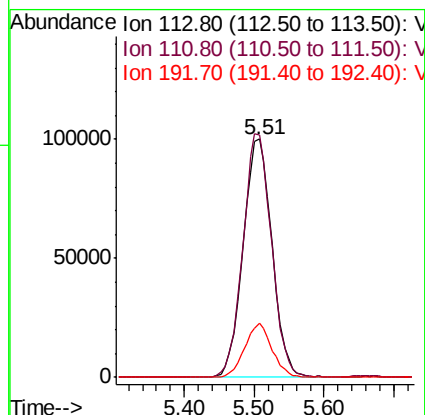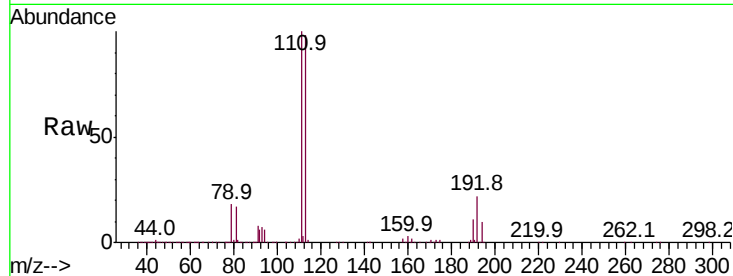

#36
1,1-Dichloropropene
Concen: 4.861 ug/l
RT: 5.66 min Scan# 739
Delta R.T. -0.14 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16

Tgt Ion: 75 Resp: 39023
Ion Ratio Lower Upper
75 100
110 10.7 20.2 60.5#
77 0.5 24.8 37.2#

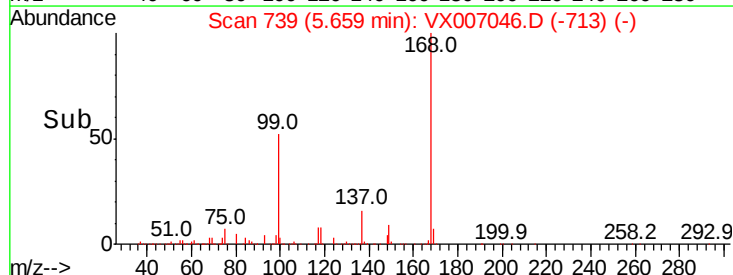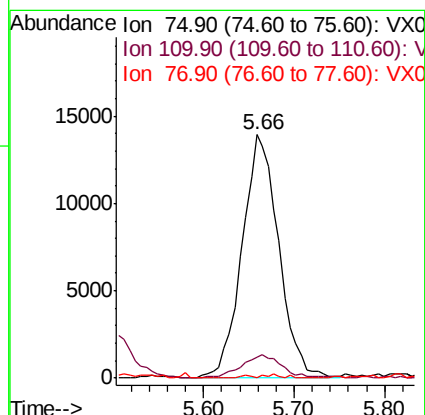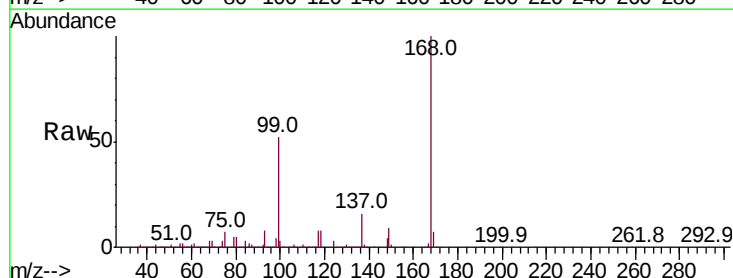



#38

Carbon Tetrachloride

Concen: 6.573 ug/l

RT: 5.67 min Scan# 740





Delta R.T. -0.12 min

Lab File: VX007046.D

Acq: 14 Jan 2019 18:16

Instrument :
MSVOA_X
ClientSampled :

Tot Ion:	117	Resp:	53094
Ion	Ratio	Lower	Upper
117	100		
119	4.3	79.4	119.2#
121	0.0	24.0	36.0#

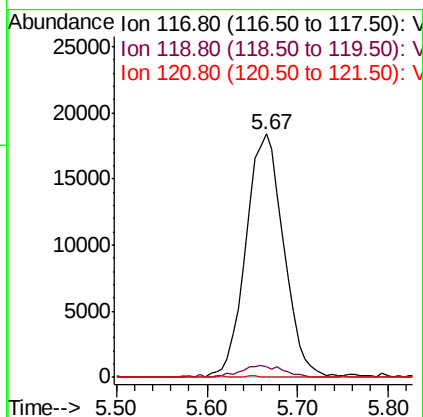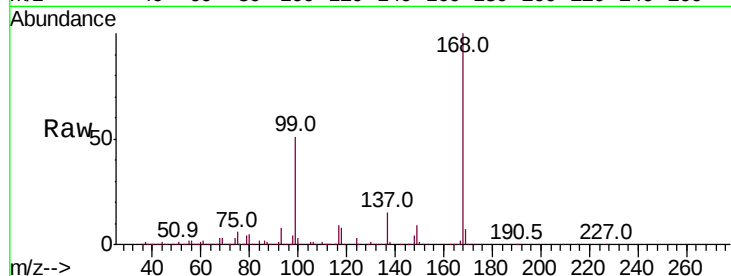

#43

Isopropyl Acetate

Concen: 1.782 ug/l




RT: 6.46 min Scan# 870


Delta R.T. -0.00 min

Lab File: VX007046.D

Acq: 14 Jan 2019 18:16

Tgt Ion:	43	Resp:	24197
Ion	Ratio	Lower	Upper
43	100		
61	23.3	16.8	25.2
87	17.1	12.4	18.6



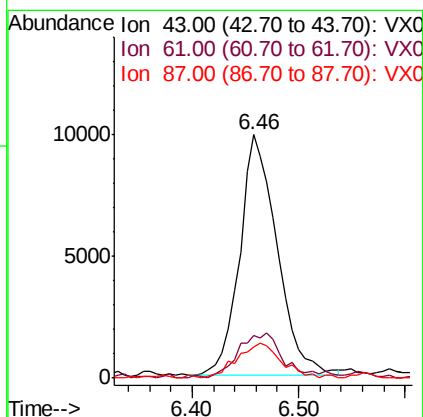



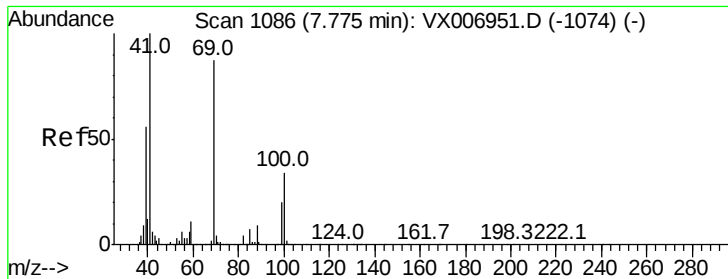

#48
Methvl methacrylate
Concen: 1.943 ug/l
RT: 7.69 min Scan# 1072
Delta R.T. -0.09 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 41 Resp: 13546
Ion Ratio Lower Upper
41 100
69 1.3 72.4 108.6#
39 0.0 45.8 68.8#

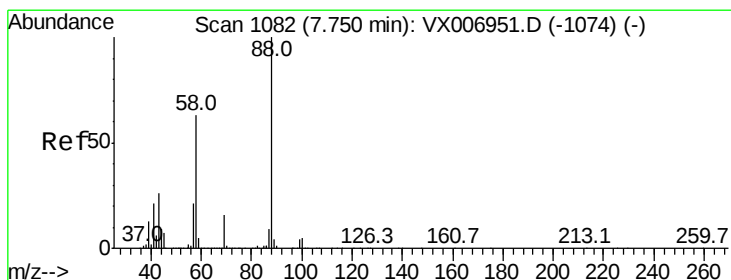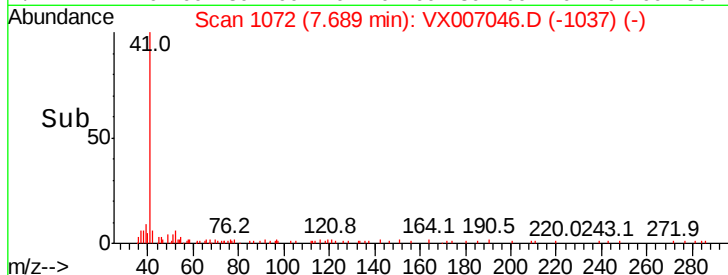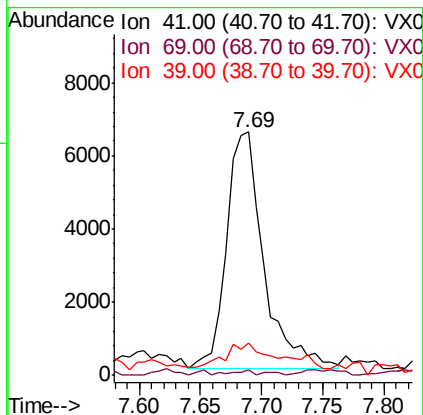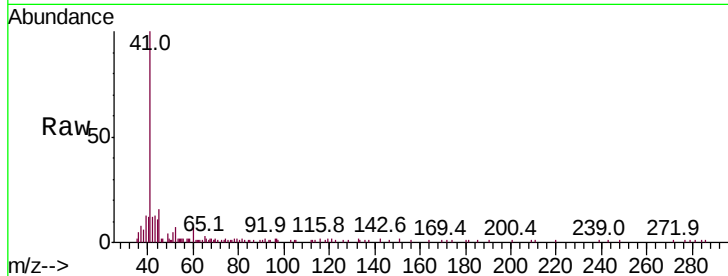

#49
1,4-Dioxane
Concen: Below Cal
RT: 7.80 min Scan# 1090
Delta R.T. 0.05 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16

Tgt Ion: 88 Resp: 130
Ion Ratio Lower Upper
88 100
43 0.0 22.2 33.4#
58 400.0 51.0 76.4#

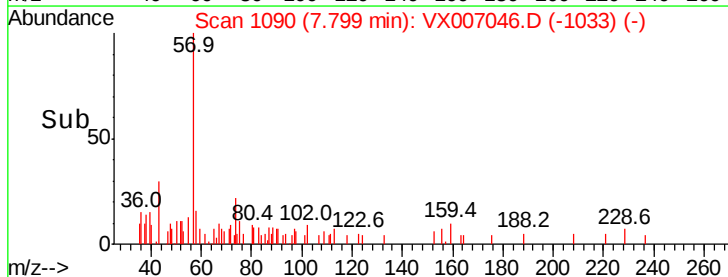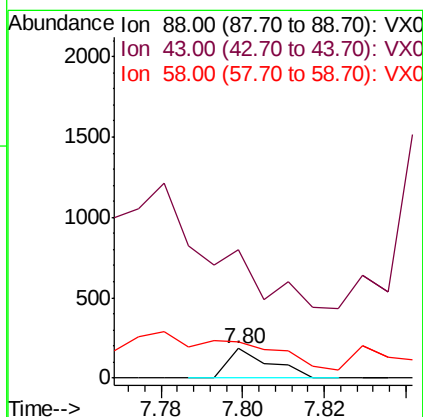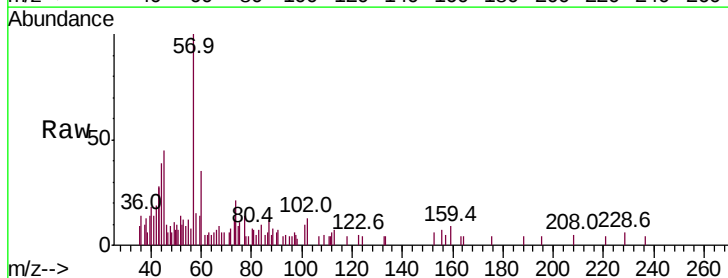

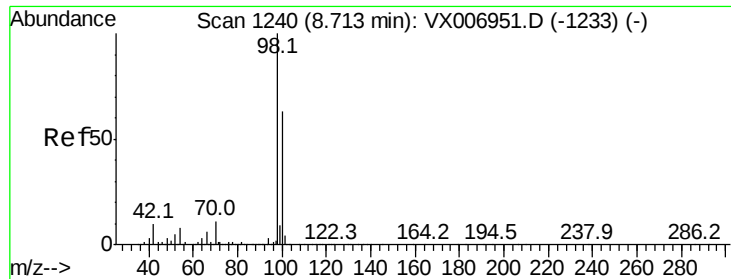

#50

Toluene-d8

Concen: 52.163 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX007046.D

Acq: 14 Jan 2019 18:16





Instrument :
MSVOA_X
ClientSampleId :

Tot Ion: 98 Resp: 1129006

Ion Ratio Lower Upper

98 100

100 64.5 52.0 78.0

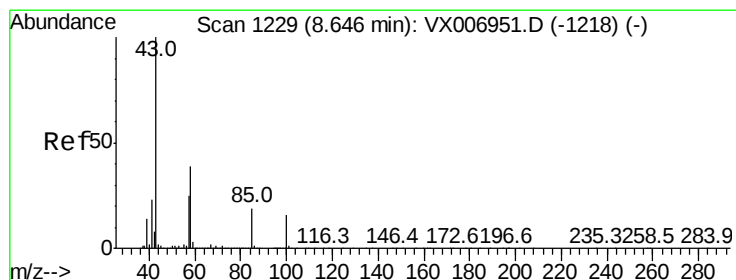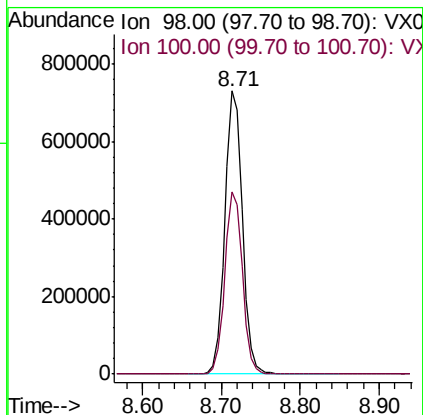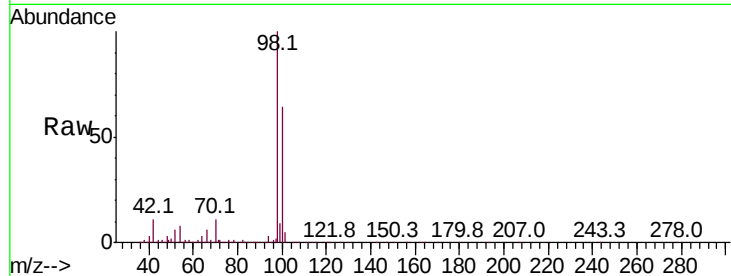

#51

4-Methyl-2-Pentanone

Concen: 15.029 ug/l

RT: 8.62 min Scan# 1224

Delta R.T. -0.03 min

Lab File: VX007046.D




Acq: 14 Jan 2019 18:16


Tgt Ion: 43 Resp: 131121

Ion Ratio Lower Upper

43 100

58 6.5 31.8 47.6#

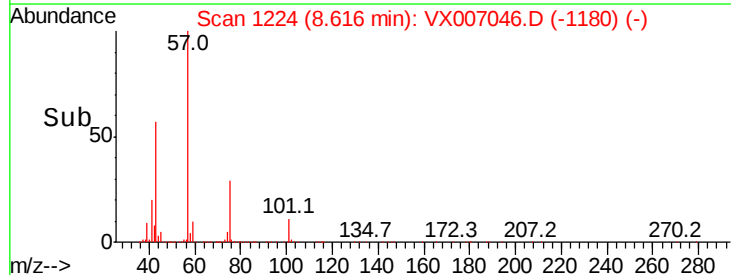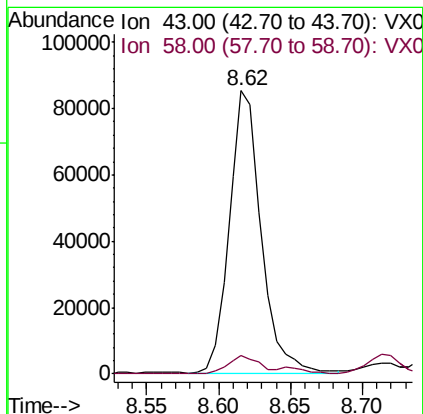

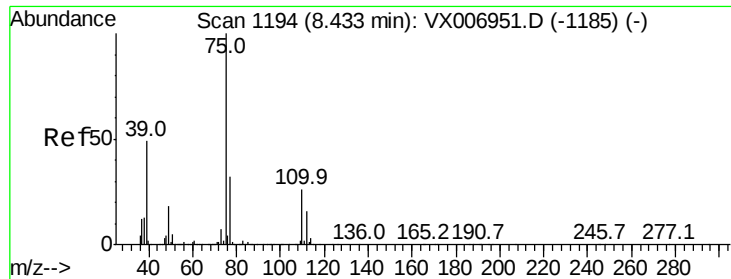

#54

cis-1,3-Dichloropropene

Concen: 7.279 ug/l

RT: 8.62 min Scan# 1225

Delta R.T. 0.19 min

Lab File: VX007046.D

Acq: 14 Jan 2019 18:16

Instrument :
MSVOA_X
ClientSampled :


Tot Ion: 75 Resp: 65665

Ion Ratio Lower Upper




75 100

77 0.5 26.2 39.2#

39 28.2 36.7 55.1#



Abundance Ion 74.90 (74.60 to 75.60): VX0
Ion 76.90 (76.60 to 77.60): VX0
Ion 39.00 (38.70 to 39.70): VX0

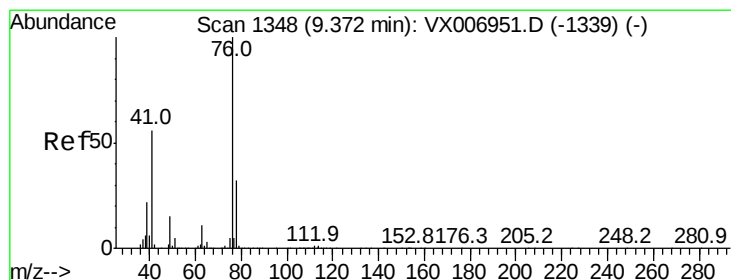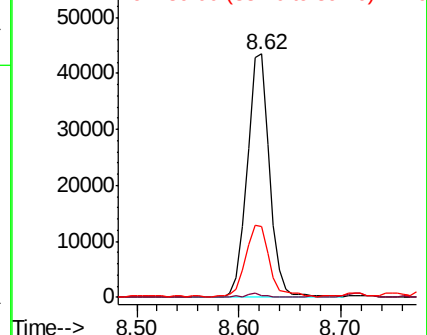

#57

1,3-Dichloropropane

Concen: 1.323 ug/l

RT: 9.54 min Scan# 1376

Delta R.T. 0.17 min

Lab File: VX007046.D


Acq: 14 Jan 2019 18:16

Tgt Ion: 76 Resp: 13659



Ion Ratio Lower Upper


76 100

78 1.1 26.0 39.0#



Abundance Ion 75.90 (75.60 to 76.60): VX0
Ion 77.90 (77.60 to 78.60): VX0



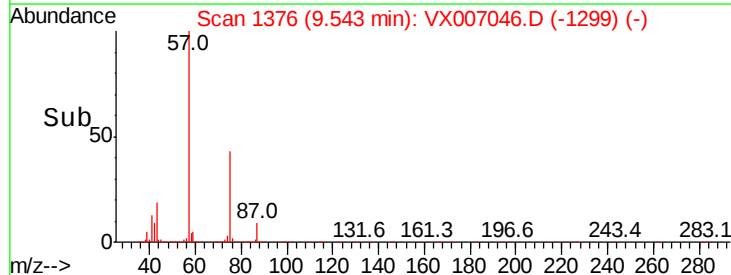
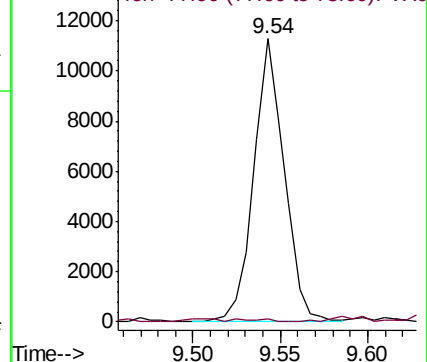


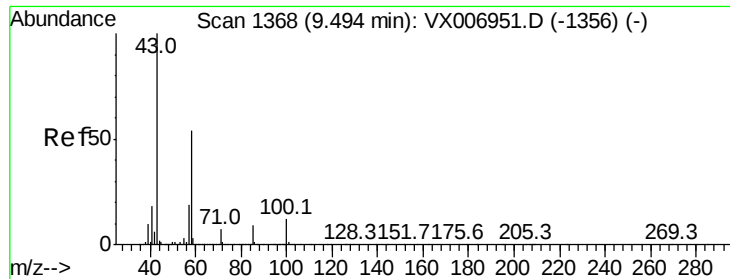

#59
2-Hexanone
Concen: 26.334 ug/l
RT: 9.54 min Scan# 1376
Delta R.T. 0.05 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 43 Resp: 175088
Ion Ratio Lower Upper
43 100
58 20.2 27.7 83.1#

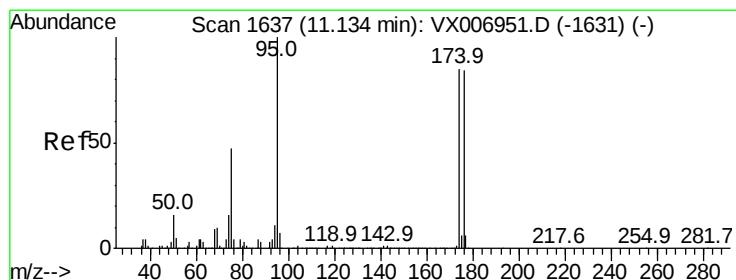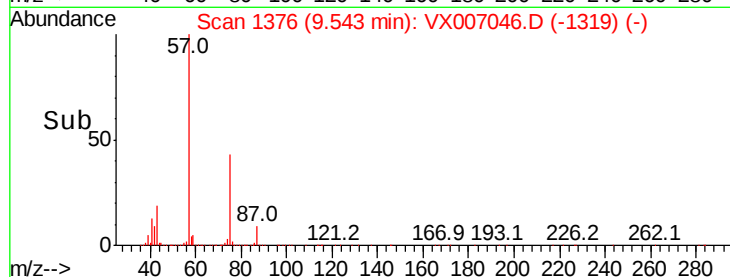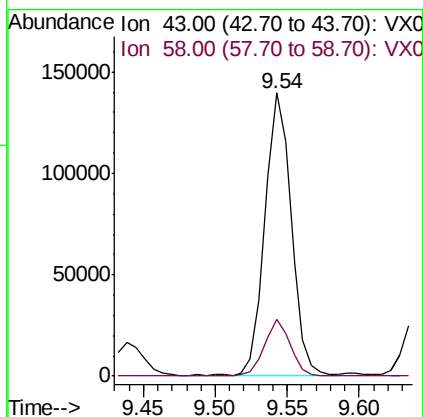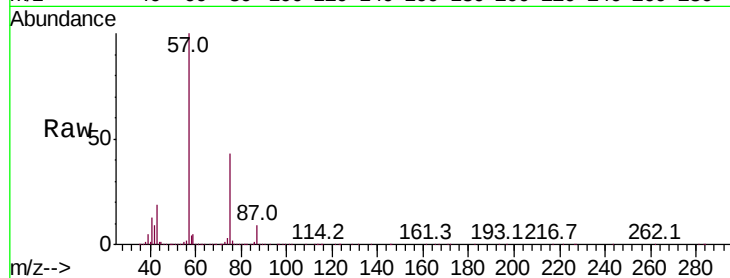

#62
4-Bromofluorobenzene
Concen: 53.491 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16

Tgt Ion: 95 Resp: 403619
Ion Ratio Lower Upper
95 100
174 92.0 0.0 182.2
176 88.8 0.0 178.8


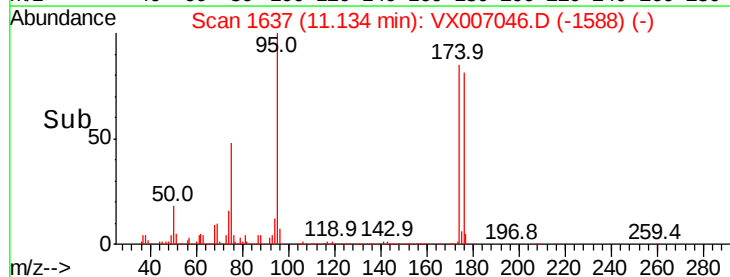
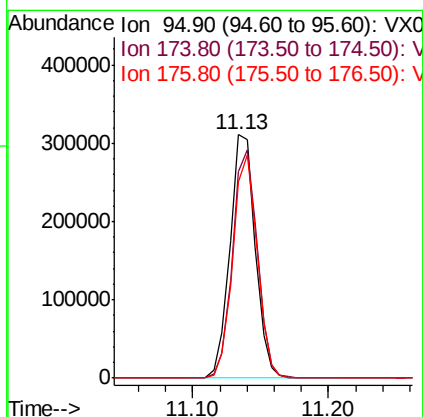
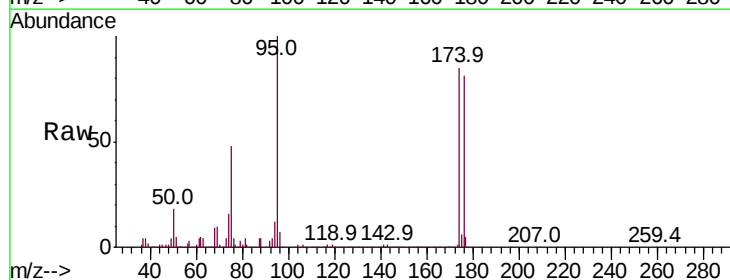




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. -0.00 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16




Instrument :
MSVOA_X
ClientSampled :


Tot Ion:117 Resp: 880947
Ion Ratio Lower Upper
117 100
82 50.3 41.0 61.6
119 32.7 25.4 38.0

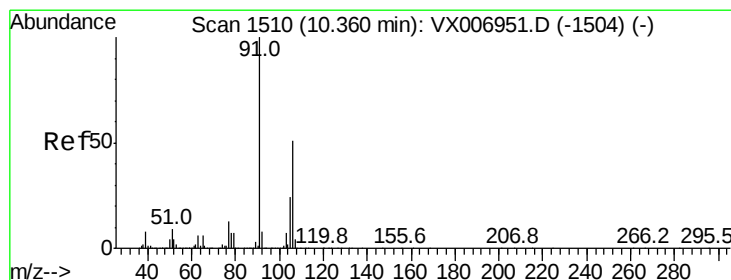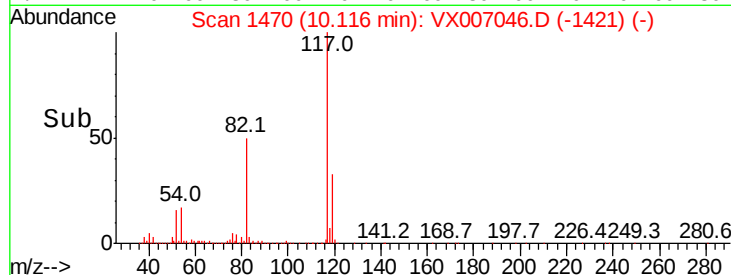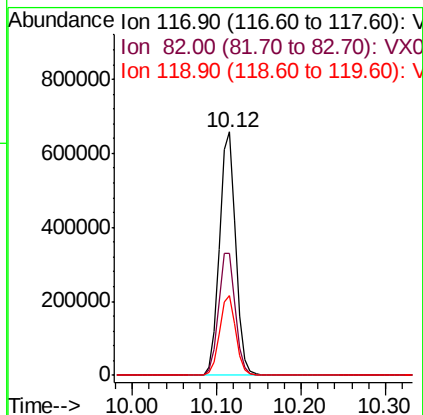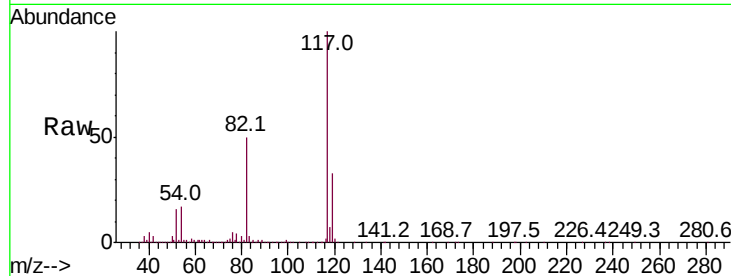

#68
m/p-Xylenes
Concen: 0.388 ug/l
RT: 10.36 min Scan# 1510
Delta R.T. -0.00 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16

Tgt Ion:106 Resp: 4853
Ion Ratio Lower Upper
106 100
91 191.4 155.8 233.6


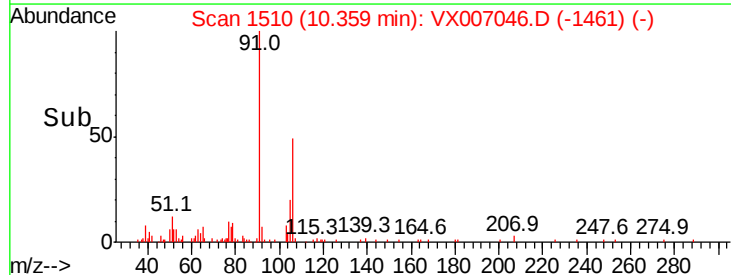
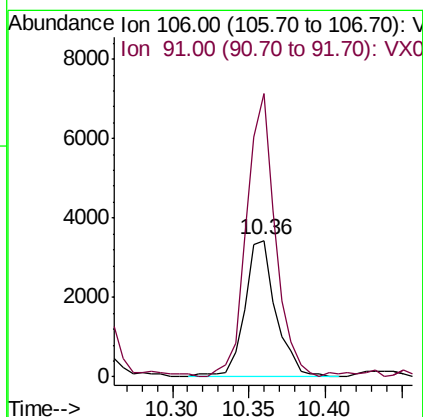



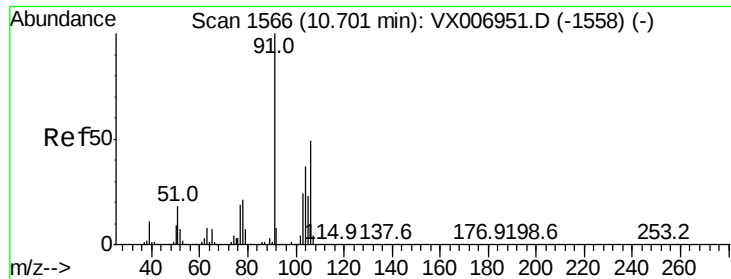

#69
o-Xylene
Concen: 0.203 ug/l
RT: 10.70 min Scan# 1566
Delta R.T. -0.00 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16




Instrument :
MSVOA_X
ClientSampled :


Tot Ion:106 Resp: 2472
Ion Ratio Lower Upper
106 100
91 208.4 101.3 303.7

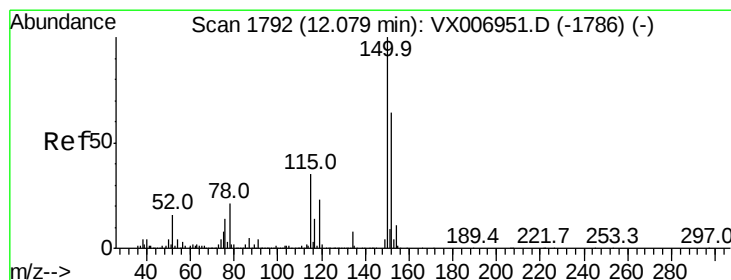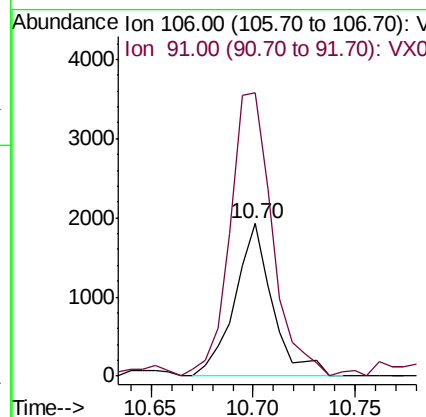

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16

Tgt Ion:152 Resp: 431943
Ion Ratio Lower Upper
152 100
115 53.8 39.1 117.2
150 155.4 0.0 344.8

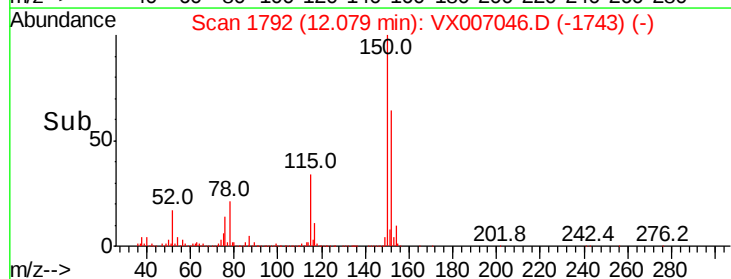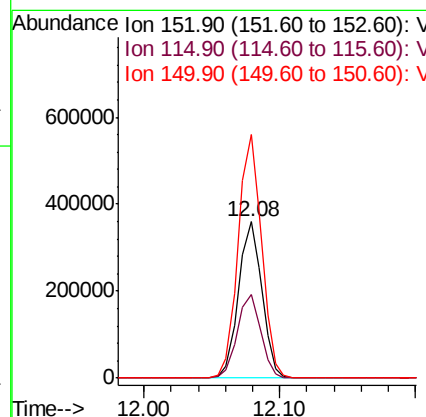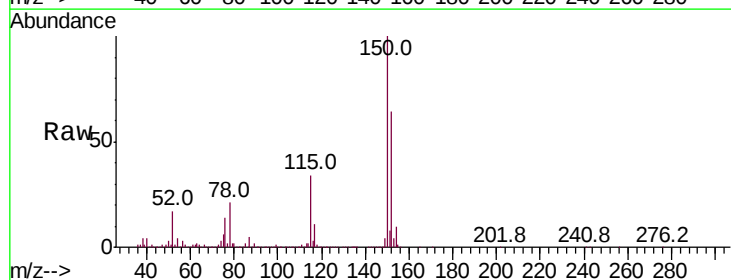

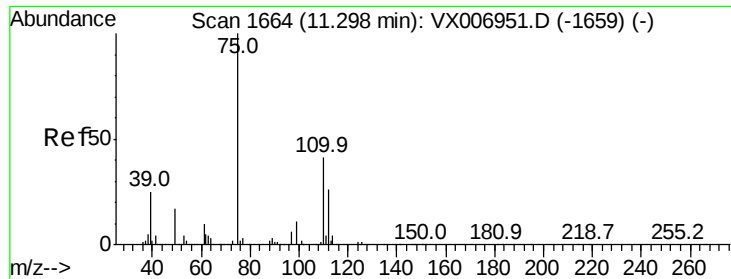

#76

1,2,3-Trichloropropane

Concen: 21.638 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.16 min

Lab File: VX007046.D

Acq: 14 Jan 2019 18:16

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 75 Resp: 189404

Ion Ratio Lower Upper

75 100

77 1.5 18.5 55.5#

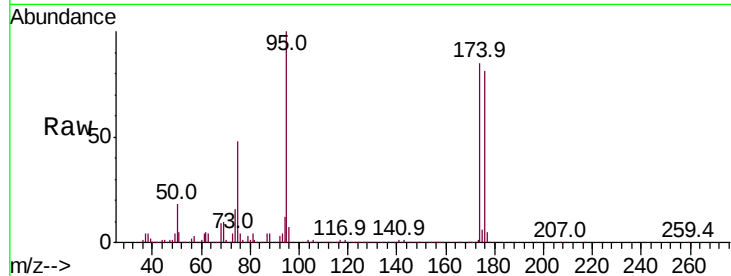

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

11.13



150000

100000

50000

0

Time--> 11.05 11.10 11.15 11.20

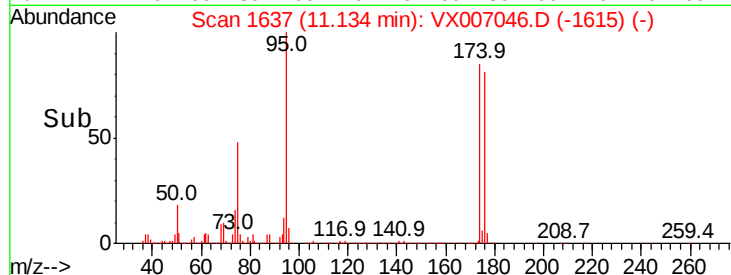

#80

1,3,5-Trimethylbenzene

Concen: 0.366 ug/l

RT: 11.51 min Scan# 1698

Delta R.T. -0.00 min

Lab File: VX007046.D


Acq: 14 Jan 2019 18:16

Tgt Ion:105 Resp: 9304

Ion Ratio Lower Upper

105 100

120 52.1 25.1 75.3



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

11.51

8000


6000


4000

2000

0

Time--> 11.50 11.55




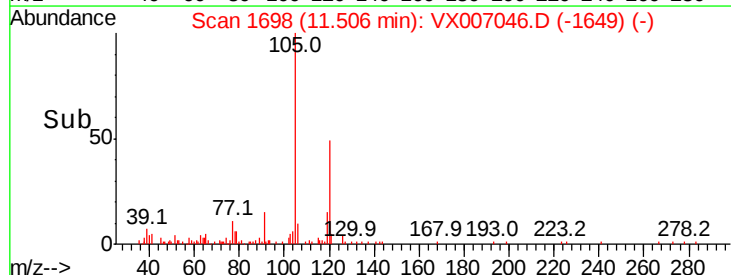




#81
trans-1,4-Dichloro-2-butene
Concen: 64.144 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. 0.06 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 75 Resp: 189404
Ion Ratio Lower Upper
75 100
53 0.1 79.7 119.5#
89 0.1 38.0 57.0#

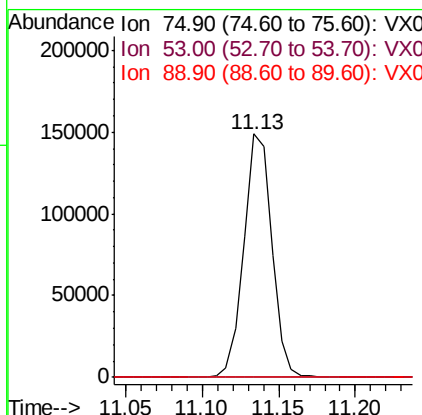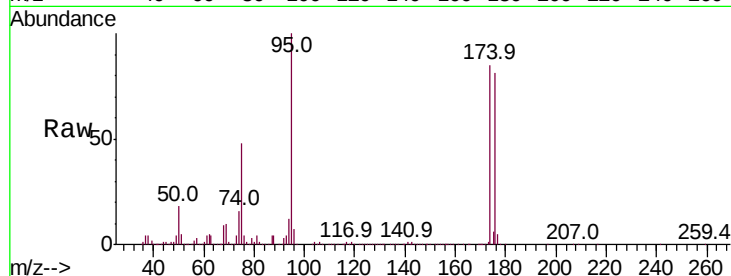

#84
1,2,4-Trimethylbenzene
Concen: 0.903 ug/l
RT: 11.80 min Scan# 1747
Delta R.T. -0.00 min
Lab File: VX007046.D
Acq: 14 Jan 2019 18:16

Tgt Ion:105 Resp: 23099
Ion Ratio Lower Upper
105 100
120 47.5 23.2 69.6



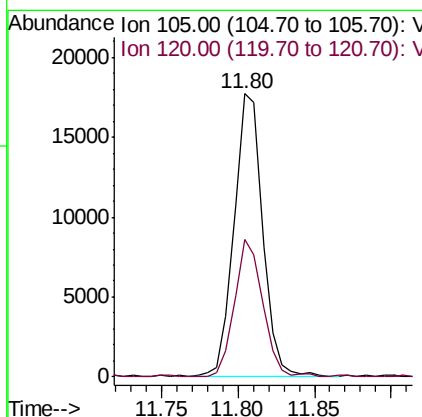



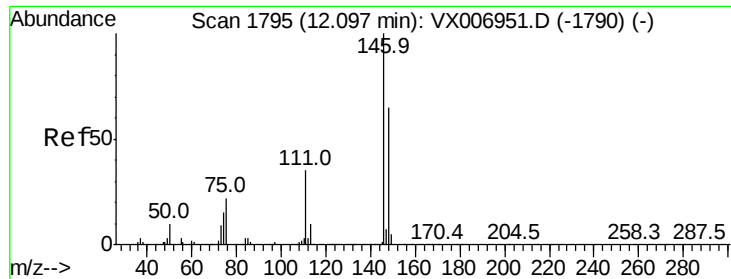

#88
 1,4-Dichlorobenzene
 Concen: 0.236 ug/l
 RT: 12.10 min Scan# 1795
 Delta R.T. -0.00 min
 Lab File: VX007046.D
 Acq: 14 Jan 2019 18:16




Instrument :
 MSVOA_X
 ClientSampled :


Tot Ion:146 Resp: 1308
 Ion Ratio Lower Upper
 146 100
 111 419.9 18.1 54.1#
 148 205.3 31.9 95.9#

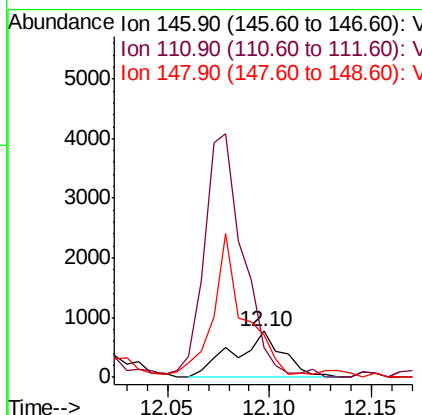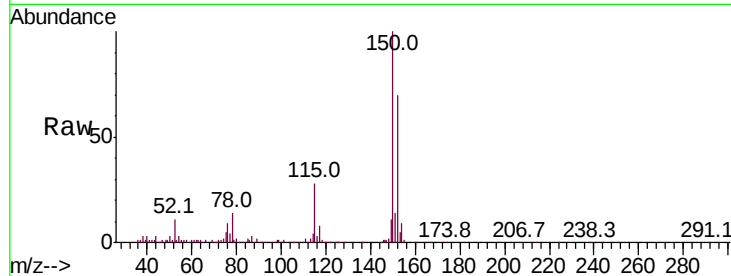

#90
 Hexachloroethane
 Concen: 2.994 ug/l
 RT: 12.60 min Scan# 1877
 Delta R.T. 0.00 min
 Lab File: VX007046.D
 Acq: 14 Jan 2019 18:16

Tgt Ion:117 Resp: 393
 Ion Ratio Lower Upper
 117 100
 201 0.0 42.9 128.7#

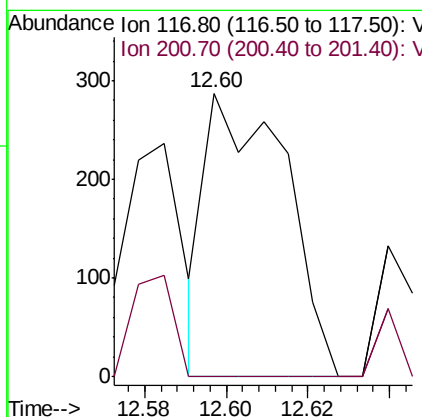

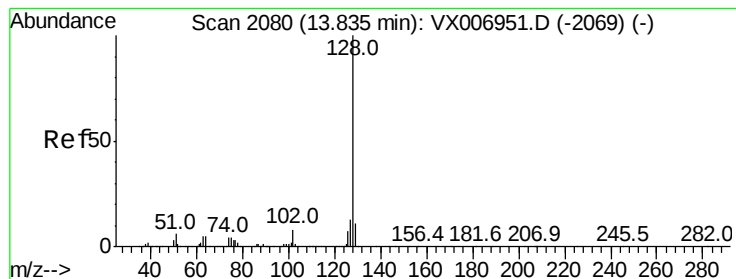

#95

Naphthalene

Concen: 3.146 ug/l

RT: 13.83 min Scan# 2080

Delta R.T. -0.00 min

Lab File: VX007046.D

Acq: 14 Jan 2019 18:16

Instrument :

MSVOA_X

ClientSampleId :

Tot Ion:128 Resp: 97894

Ion Ratio Lower Upper

128 100

127 13.2 10.1 15.1

129 11.7 8.6 13.0

