

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX011420\
 Data File : VX014603.D
 Acq On : 14 Jan 2020 13:19
 Operator : JC/SP
 Sample : FOUNTAIN1
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FOUNTAIN1

Quant Time: Jan 15 00:56:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 07 15:54:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	459630	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	715924	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	646074	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	294442	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.05	65	259978	50.67	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.34%	
35) Dibromofluoromethane	5.49	113	218555	50.43	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.86%	
50) Toluene-d8	8.71	98	850135	50.55	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.10%	
62) 4-Bromofluorobenzene	11.13	95	286592	46.42	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.84%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX011420\
Data File : VX014603.D
Acq On : 14 Jan 2020 13:19
Operator : JC/SP
Sample : FOUNTAIN1
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FOUNTAIN1

Quant Time: Jan 15 00:56:49 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 07 15:54:41 2020
Response via : Initial Calibration

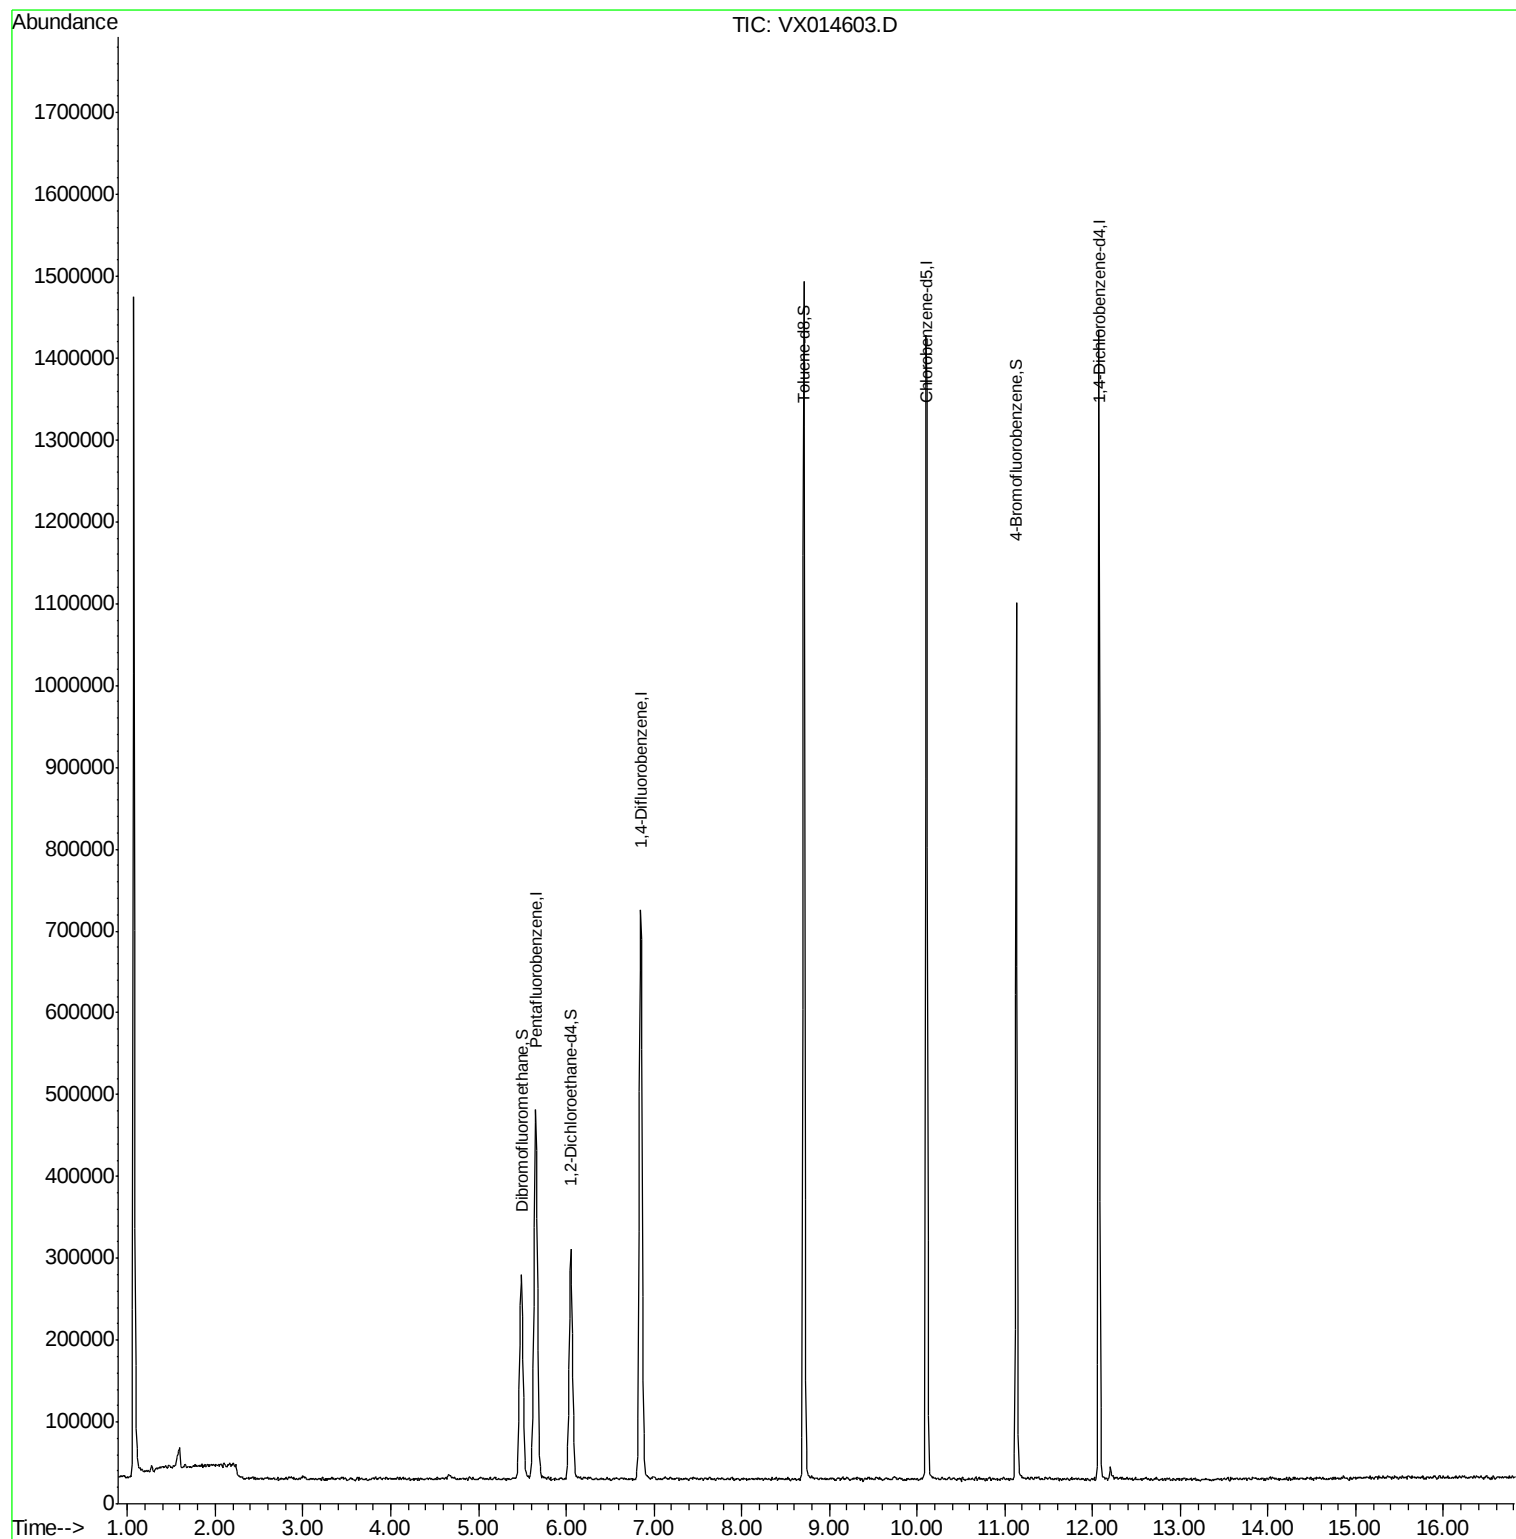

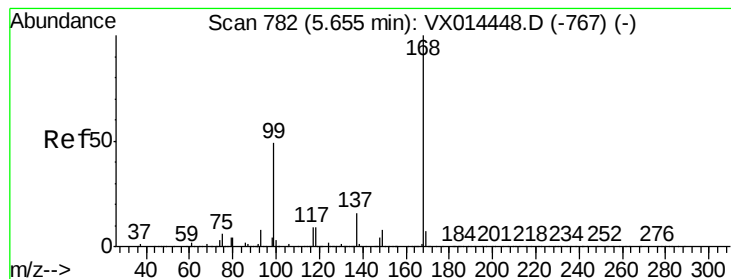

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 782

Delta R.T. -0.00 min

Lab File: VX014603.D

Acq: 14 Jan 2020 13:19

Instrument :

MSVOA_X

ClientSampleId :


FOUNTAIN1

Tot Ion:168 Resp: 459630

Ion Ratio Lower Upper

168 100

99 49.0 39.2 58.8

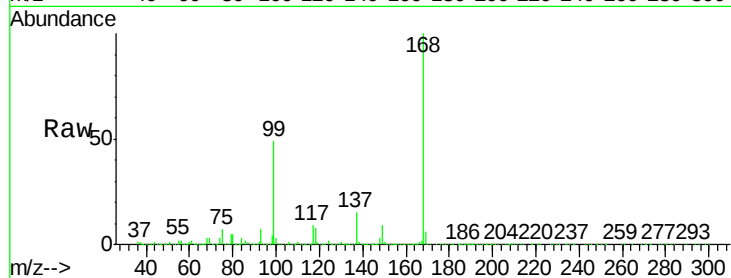

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65



150000

100000

50000

0

Time-->

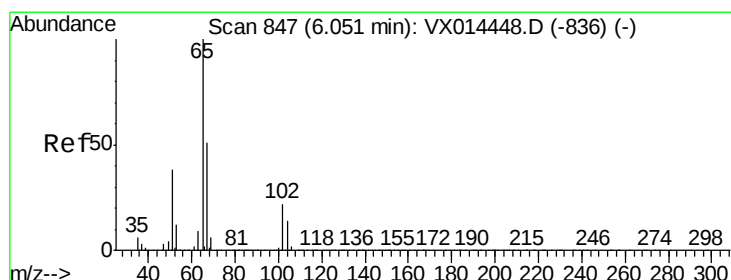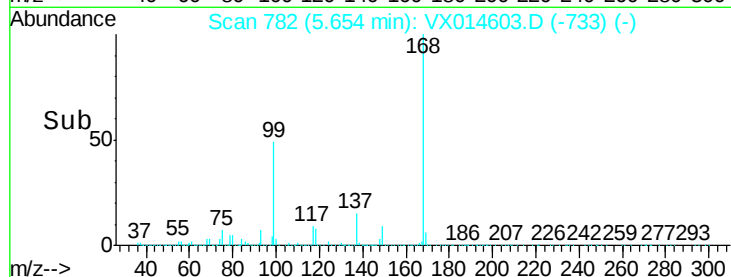

#33

1,2-Dichloroethane-d4

Concen: 50.668 ug/l

RT: 6.05 min Scan# 847

Delta R.T. -0.00 min

Lab File: VX014603.D


Acq: 14 Jan 2020 13:19

Tgt Ion: 65 Resp: 259978

Ion Ratio Lower Upper

65 100

67 52.9 0.0 106.2

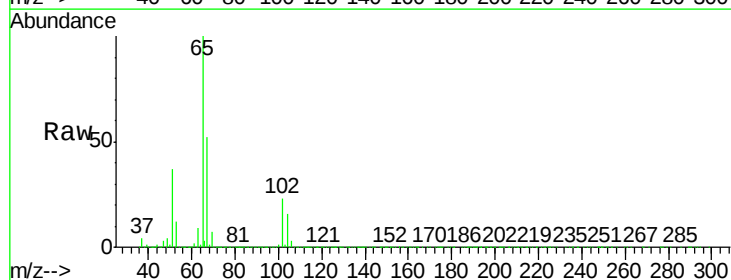

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.05

120000

100000

80000


60000


40000

20000

0

Time-->

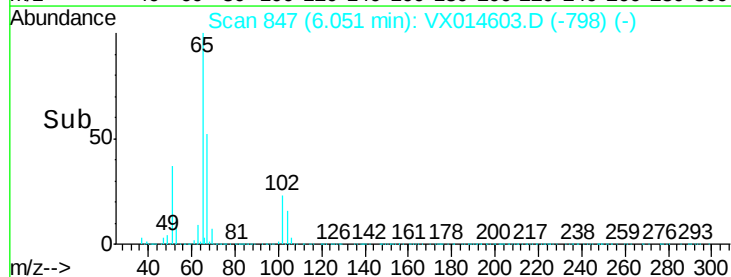

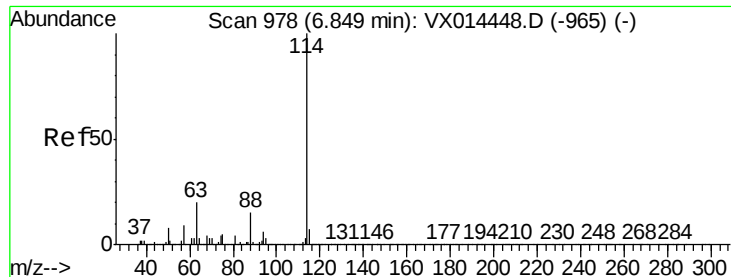

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 978

Delta R.T. -0.00 min

Lab File: VX014603.D

Acq: 14 Jan 2020 13:19

Instrument :

MSVOA_X

ClientSampleId :

FOUNTAIN1


Tot Ion:114 Resp: 715924

Ion Ratio Lower Upper

114 100

63 20.0 0.0 39.6




88 15.8 0.0 30.8

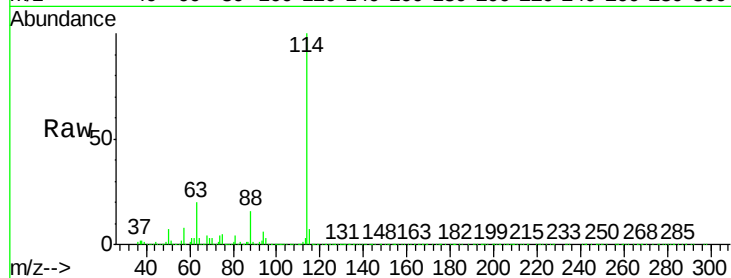

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

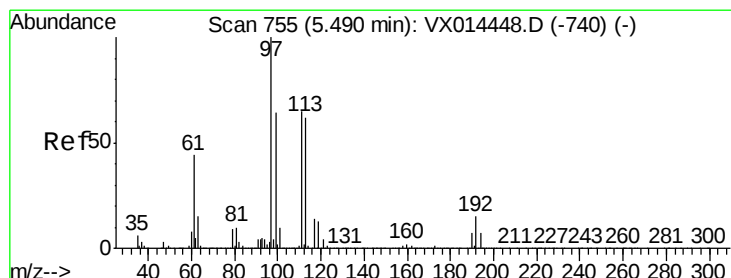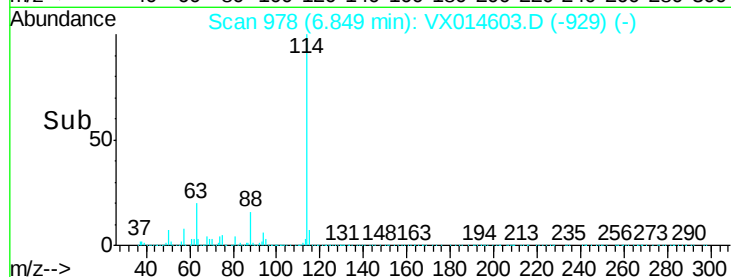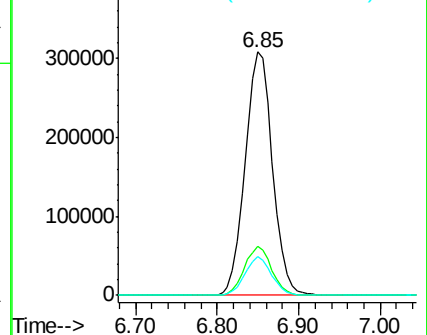

#35

Dibromofluoromethane

Concen: 50.430 ug/l

RT: 5.49 min Scan# 755

Delta R.T. -0.00 min

Lab File: VX014603.D

Acq: 14 Jan 2020 13:19


Tgt Ion:113 Resp: 218555

Ion Ratio Lower Upper

113 100

111 101.1 81.5 122.3



192 22.6 19.2 28.8

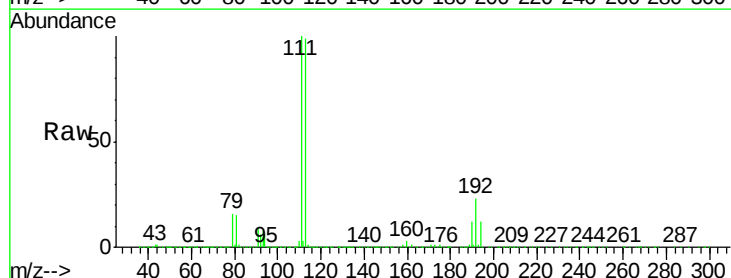


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

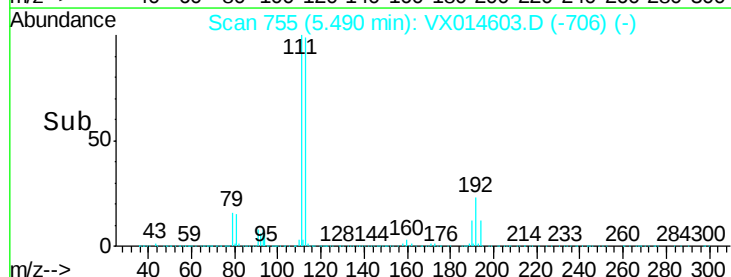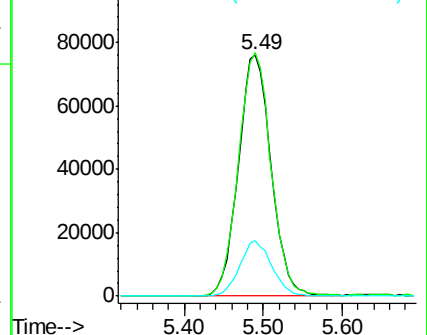

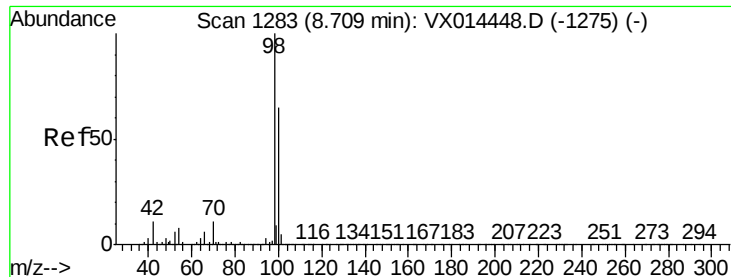

#50

Toluene-d8

Concen: 50.549 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. -0.00 min

Lab File: VX014603.D

Acq: 14 Jan 2020 13:19

Instrument :

MSVOA_X

ClientSampleId :





FOUNTAIN1

Tot Ion: 98 Resp: 850135

Ion Ratio Lower Upper

98 100

100 66.1 53.2 79.8

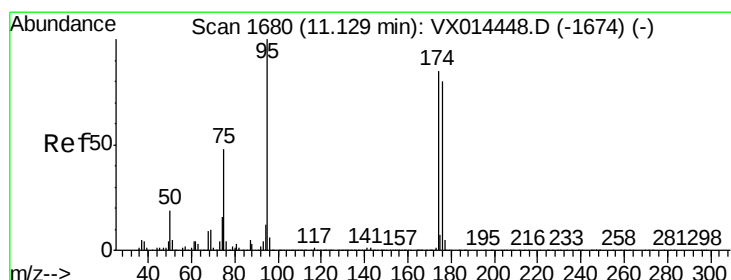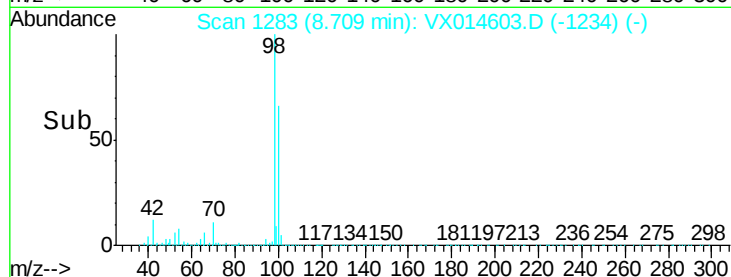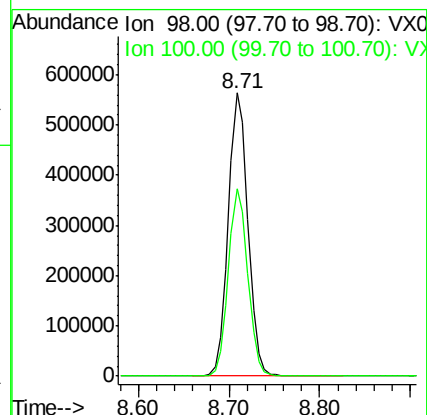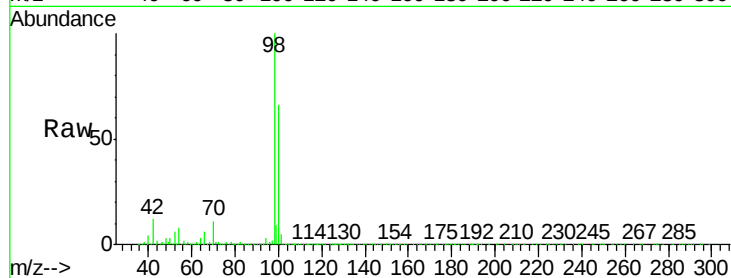

#62

4-Bromofluorobenzene

Concen: 46.419 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.00 min

Lab File: VX014603.D

Acq: 14 Jan 2020 13:19




Tgt Ion: 95 Resp: 286592


Ion Ratio Lower Upper

95 100

174 89.7 0.0 180.8

176 86.8 0.0 172.8


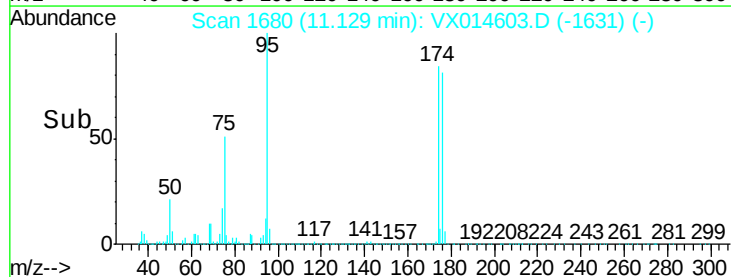
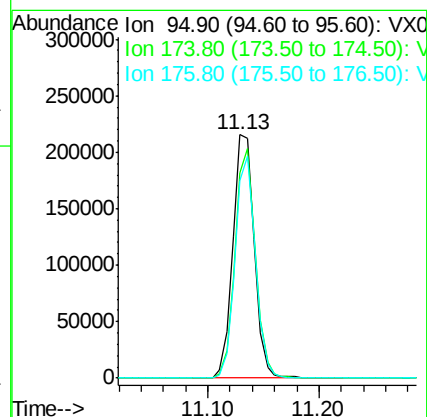
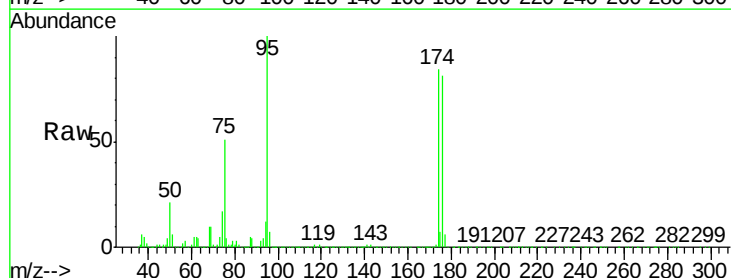


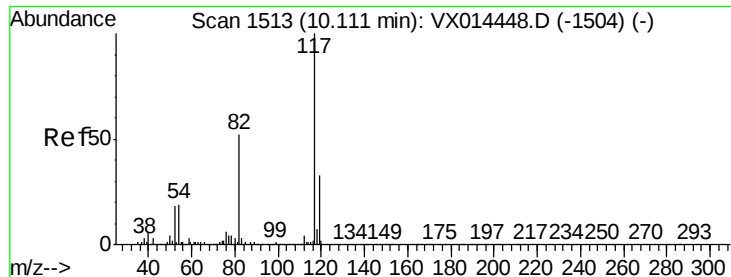

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1512
Delta R.T. -0.01 min
Lab File: VX014603.D
Acq: 14 Jan 2020 13:19

Instrument :
MSVOA_X
ClientSampled :
FOUNTAIN1

Tot Ion:117 Resp: 646074
Ion Ratio Lower Upper
117 100
82 54.9 41.8 62.6
119 31.6 26.2 39.4

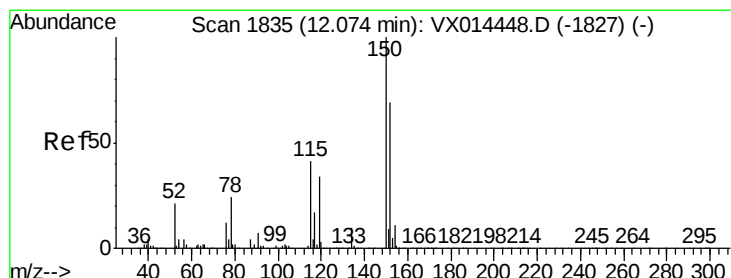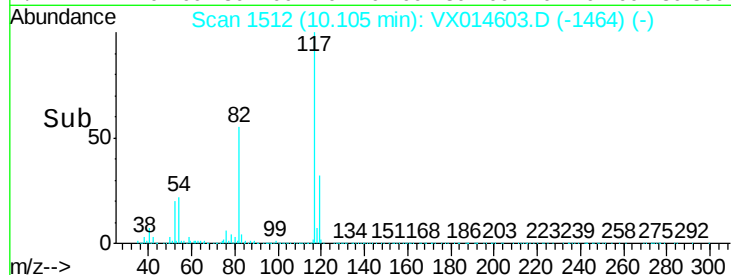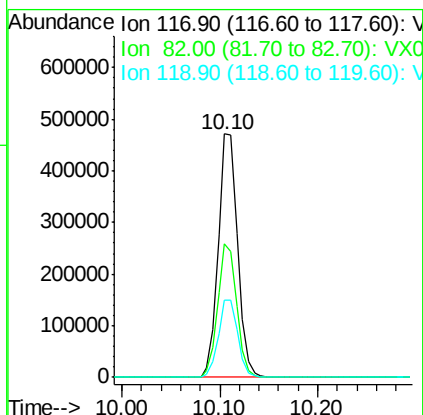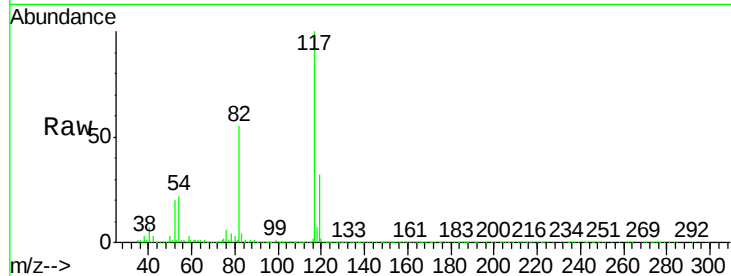

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. -0.00 min
Lab File: VX014603.D
Acq: 14 Jan 2020 13:19

Tgt Ion:152 Resp: 294442
Ion Ratio Lower Upper
152 100
115 56.7 39.5 118.3
150 157.3 0.0 350.2

