
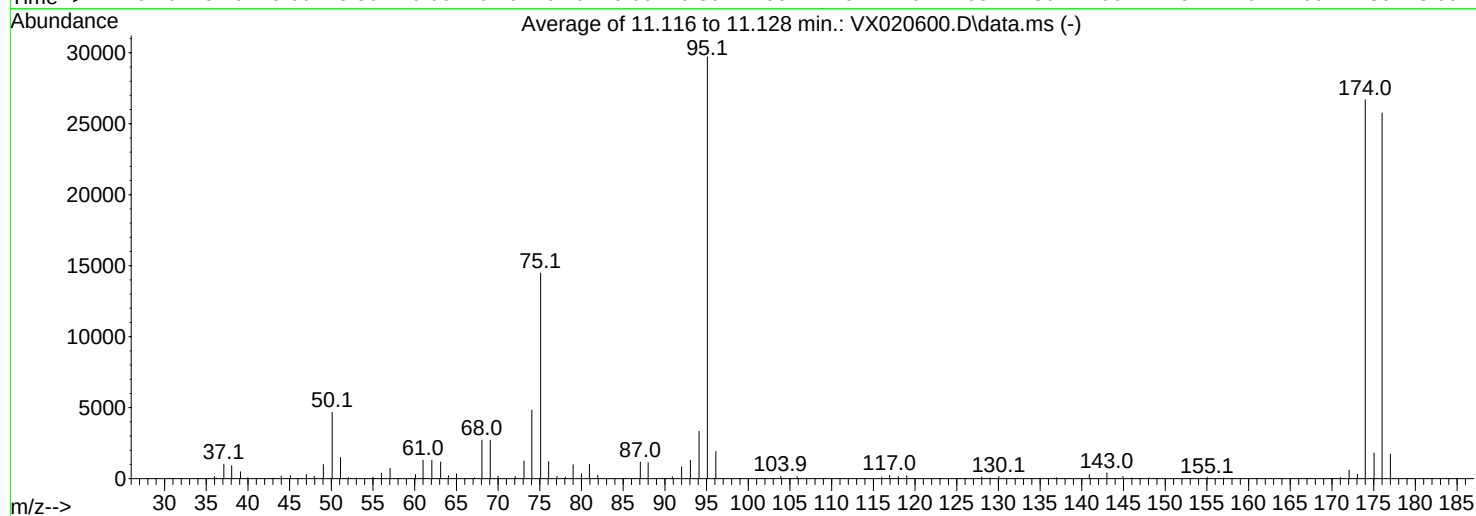


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011421\
Data File : VX020600.D
Acq On : 14 Jan 2021 09:19
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011121W.M
Title : SW846 8260
Last Update : Mon Jan 11 15:05:37 2021

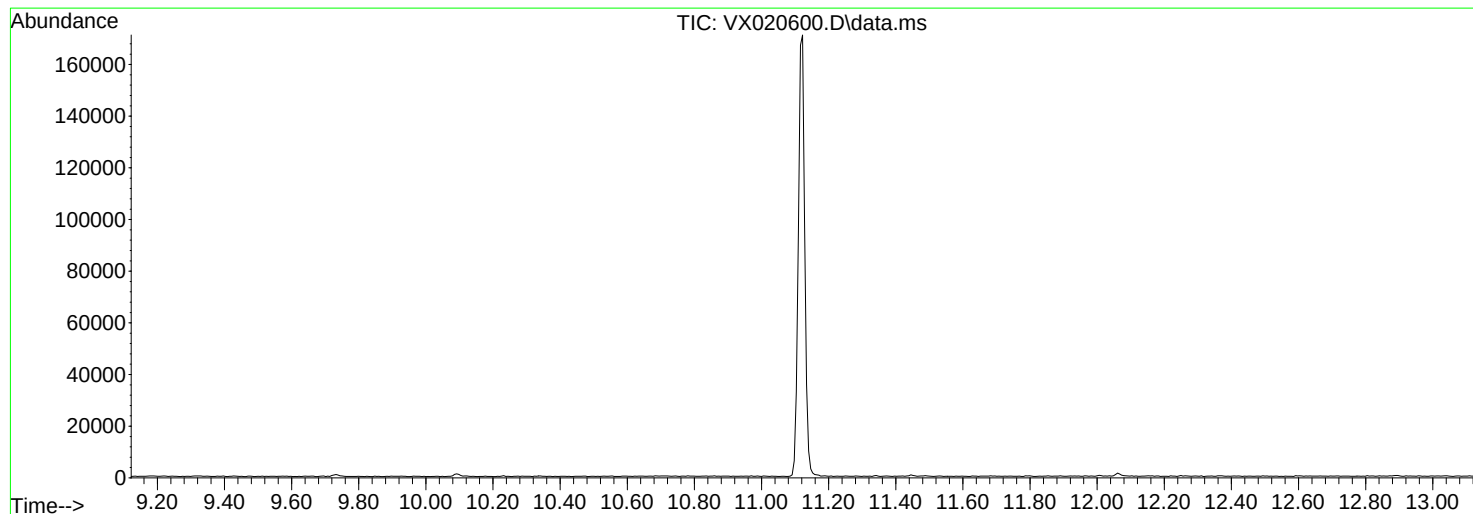

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.7	4672	PASS
75	95	30	60	48.8	14489	PASS
95	95	100	100	100.0	29712	PASS
96	95	5	9	6.4	1916	PASS
173	174	0.00	2	1.1	303	PASS
174	95	50	100	89.8	26688	PASS
175	174	5	9	6.8	1818	PASS
176	174	95	101	96.5	25757	PASS
177	176	5	9	6.7	1730	PASS