
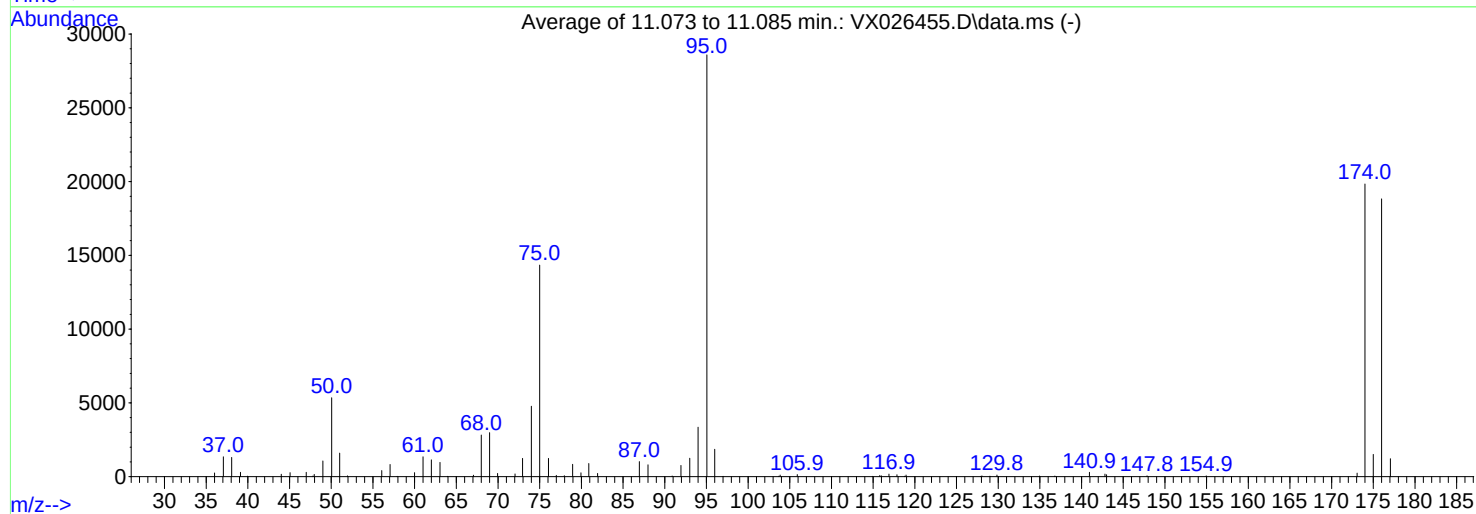


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011422\
 Data File : VX026455.D
 Acq On : 14 Jan 2022 15:03
 Operator : JC/MD
 Sample : VSTDCCC020
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 LabSampleId :
 VSTDCCC020

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X011022W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Mon Jan 10 12:50:55 2022

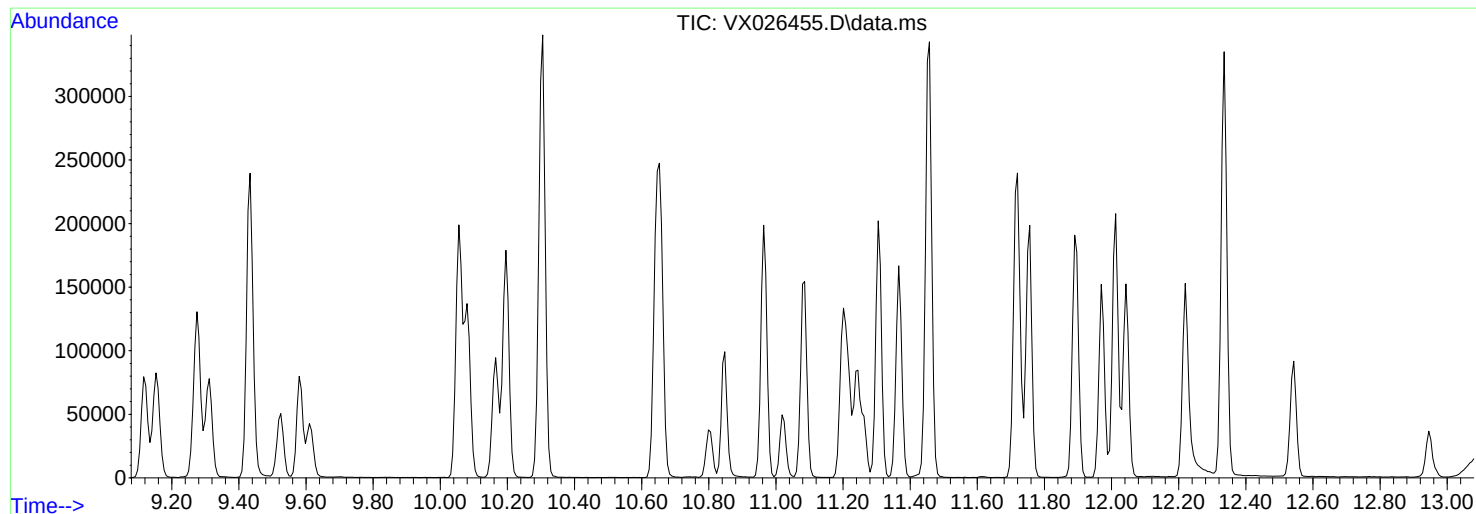

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	5348	PASS
75	95	30	60	50.2	14340	PASS
95	95	100	100	100.0	28589	PASS
96	95	5	9	6.5	1857	PASS
173	174	0.00	2	1.2	242	PASS
174	95	50	100	69.4	19830	PASS
175	174	5	9	7.6	1503	PASS
176	174	95	101	95.0	18830	PASS
177	176	5	9	6.5	1219	PASS