

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX011423\  
 Data File : VX033733.D  
 Acq On : 13 Jan 2023 19:24  
 Operator : JC/MD  
 Sample : PB150223ZHE#05  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :

Quant Time: Jan 16 05:39:02 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X011123W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Jan 11 14:48:42 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc      | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|-----------|--------|----------|
| Internal Standards            |        |       |          |           |        |          |
| 1) Pentafluorobenzene         | 5.550  | 168   | 116603   | 50.000    | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 6.763  | 114   | 178786   | 50.000    | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 10.055 | 117   | 175436   | 50.000    | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 12.024 | 152   | 81650    | 50.000    | ug/l   | 0.00     |
| System Monitoring Compounds   |        |       |          |           |        |          |
| 33) 1,2-Dichloroethane-d4     | 5.958  | 65    | 71508    | 58.244    | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 78 - 117 | Recovery  | =      | 116.480% |
| 35) Dibromofluoromethane      | 5.385  | 113   | 54877    | 49.431    | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 75 - 124 | Recovery  | =      | 98.860%  |
| 50) Toluene-d8                | 8.647  | 98    | 217156   | 53.686    | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 92 - 112 | Recovery  | =      | 107.380% |
| 62) 4-Bromofluorobenzene      | 11.079 | 95    | 79360    | 52.843    | ug/l   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 83 - 123 | Recovery  | =      | 105.680% |
| Target Compounds              |        |       |          |           |        | Qvalue   |
| 3) Chloromethane              | 1.307  | 50    | 725      | 0.708     | ug/l # | 43       |
| 11) Tert butyl alcohol        | 2.995  | 59    | 347      | 1.627     | ug/l # | 86       |
| 16) Acetone                   | 2.392  | 43    | 21717    | 38.177    | ug/l   | 92       |
| 17) Carbon Disulfide          | 2.514  | 76    | 69       | 1.850     | ug/l # | 76       |
| 18) Methyl Acetate            | 2.709  | 43    | 1676     | 0.978     | ug/l   | 91       |
| 20) Methylene Chloride        | 2.794  | 84    | 3388     | 0.704     | ug/l   | 92       |
| 25) 2-Butanone                | 4.580  | 43    | 6435     | 8.022     | ug/l   | 93       |
| 29) Tetrahydrofuran           | 5.026  | 42    | 255      | 0.504     | ug/l # | 39       |
| 31) Cyclohexane               | 5.544  | 56    | 2415     | 1.337     | ug/l # | 32       |
| 36) 1,1-Dichloropropene       | 5.544  | 75    | 8420     | 5.197     | ug/l # | 48       |
| 37) Ethyl Acetate             | 4.721  | 43    | 18436    | 9.617     | ug/l   | 98       |
| 38) Carbon Tetrachloride      | 5.550  | 117   | 10971    | 6.538     | ug/l # | 13       |
| 43) Isopropyl Acetate         | 6.342  | 43    | 81452    | 31.844    | ug/l   | 97       |
| 48) Methyl methacrylate       | 7.799  | 41    | 85482    | 66.343    | ug/l # | 46       |
| 49) 1,4-Dioxane               | 7.793  | 88    | 89       | 3.123     | ug/l # | 1        |
| 51) 4-Methyl-2-Pentanone      | 8.549  | 43    | 70051    | 44.593    | ug/l # | 49       |
| 53) t-1,3-Dichloropropene     | 8.952  | 75    | 516      | 0.324     | ug/l # | 43       |
| 54) cis-1,3-Dichloropropene   | 8.549  | 75    | 27874    | 15.620    | ug/l # | 72       |
| 56) Ethyl methacrylate        | 9.244  | 69    | 533      | 0.314     | ug/l # | 1        |
| 57) 1,3-Dichloropropane       | 9.482  | 76    | 3994     | 2.040     | ug/l # | 43       |
| 59) 2-Hexanone                | 9.482  | 43    | 60411    | 55.252    | ug/l # | 47       |
| 73) Isopropylbenzene          | 11.079 | 105   | 101      | Below Cal | #      | 48       |
| 74) N-amyl acetate            | 10.640 | 43    | 21215    | 9.895     | ug/l # | 51       |
| 76) 1,2,3-Trichloropropane    | 11.079 | 75    | 42658    | 28.435    | ug/l # | 34       |
| 81) trans-1,4-Dichloro-2-b... | 11.079 | 75    | 42658    | 88.373    | ug/l # | 8        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX011423\  
Data File : VX033733.D  
Acq On : 13 Jan 2023 19:24  
Operator : JC/MD  
Sample : PB150223ZHE#05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :


Quant Time: Jan 16 05:39:02 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X011123W.M  
Quant Title : SW846 8260  
QLast Update : Wed Jan 11 14:48:42 2023  
Response via : Initial Calibration

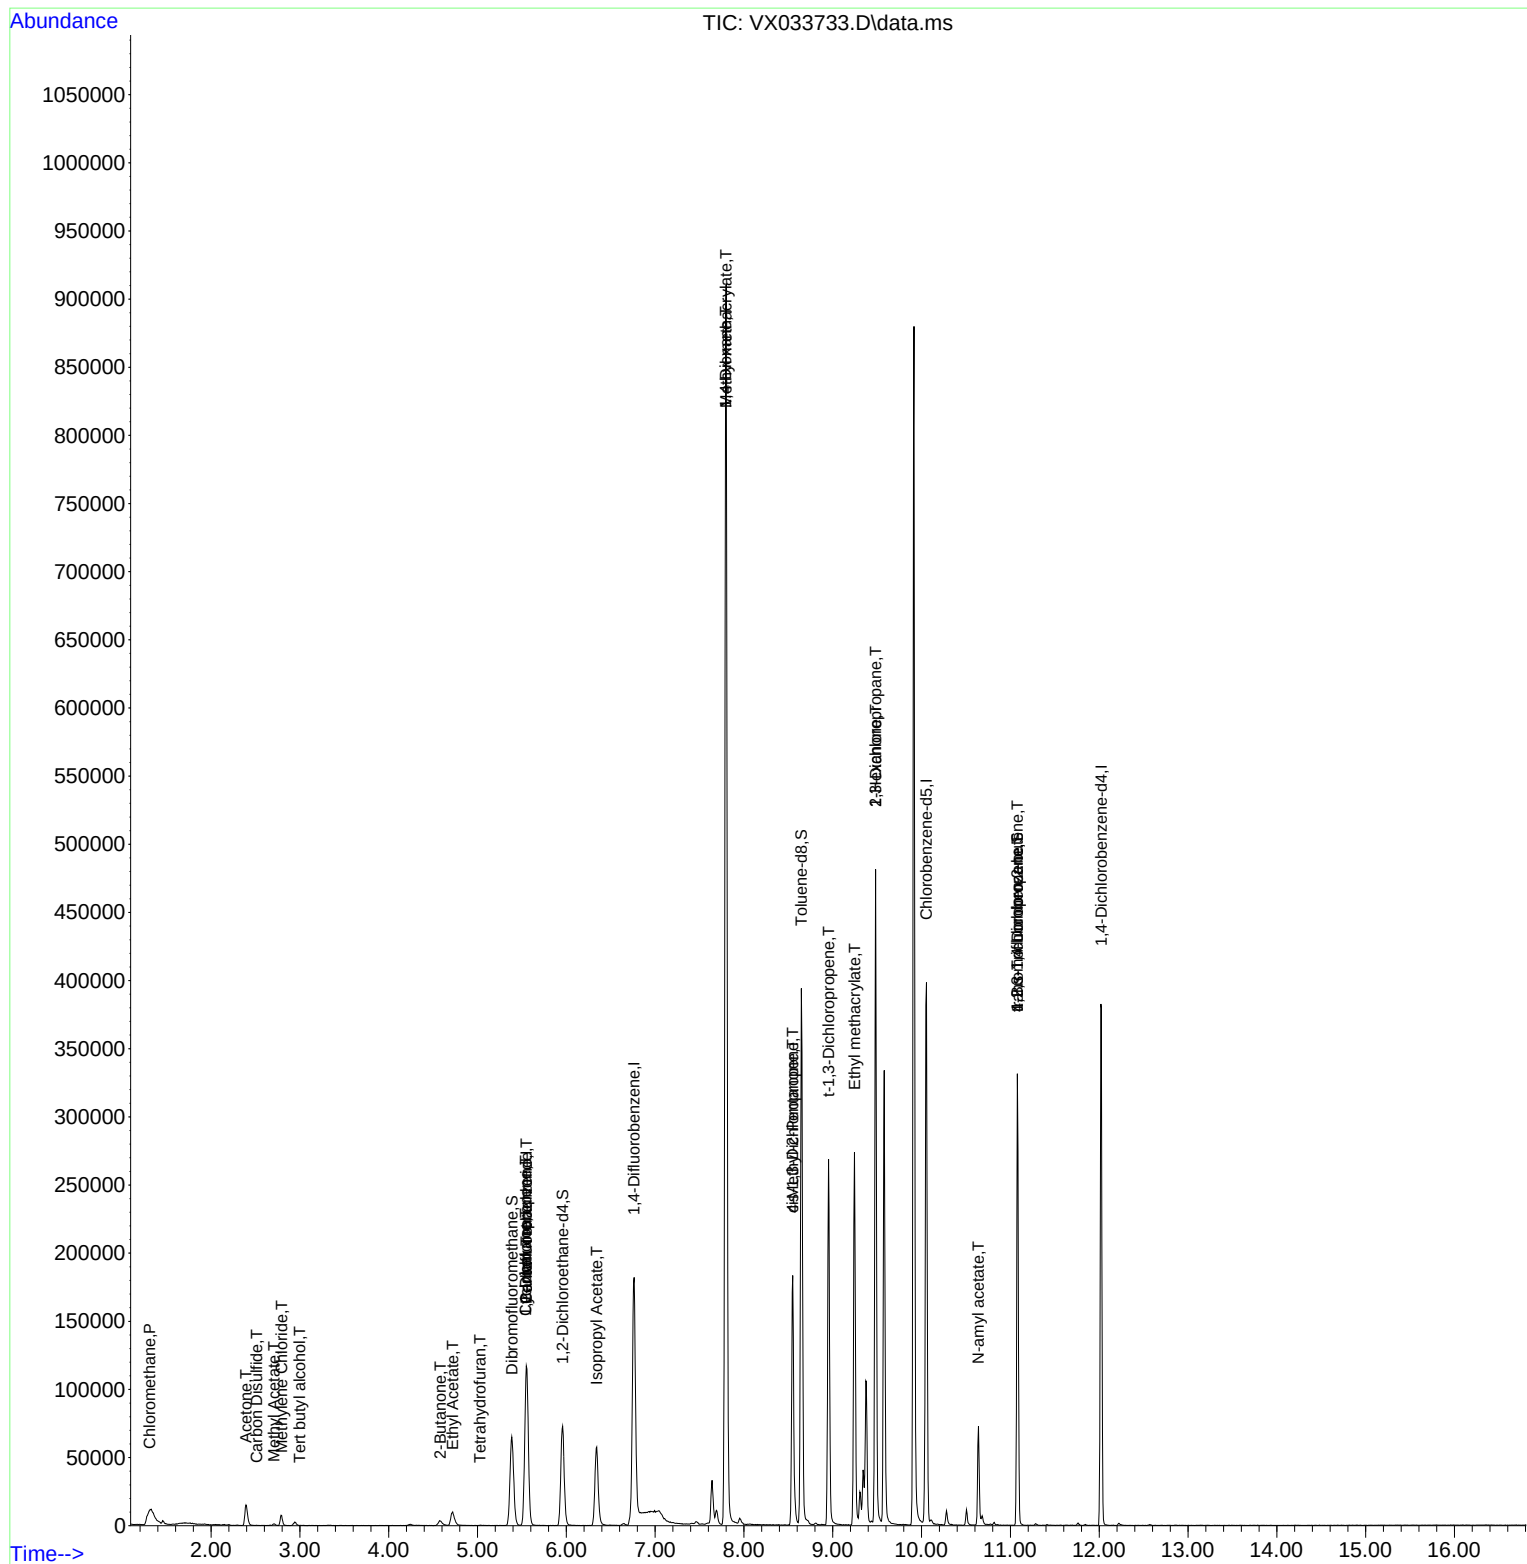



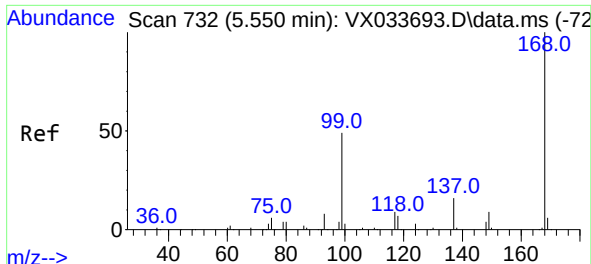


#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 71  
Delta R.T. -0.000 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24

Instrument :  
MSVOA\_X  
ClientSampleId :



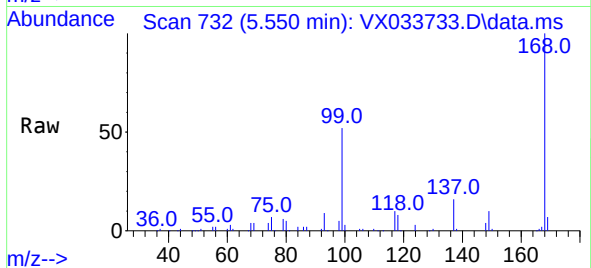



Tgt Ion:168 Resp: 116603  
Ion Ratio Lower Upper  
168 100  
99 52.5 39.6 59.4

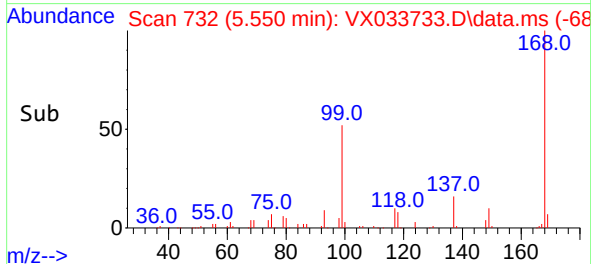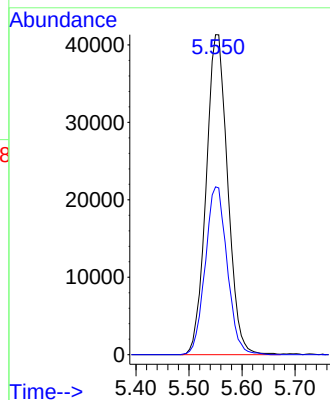

#3  
Chloromethane  
Concen: 0.708 ug/l  
RT: 1.307 min Scan# 36  
Delta R.T. 0.012 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24

Tgt Ion: 50 Resp: 725  
Ion Ratio Lower Upper  
50 100  
52 0.0 25.2 37.8#

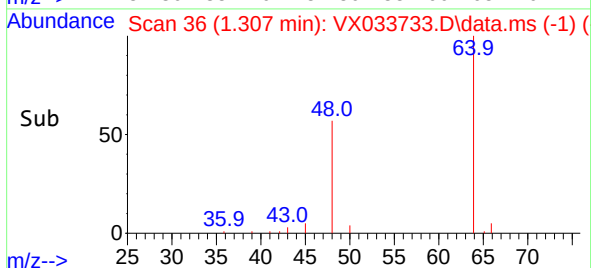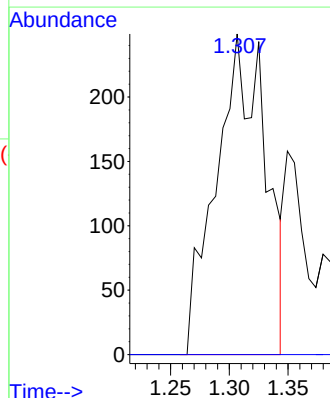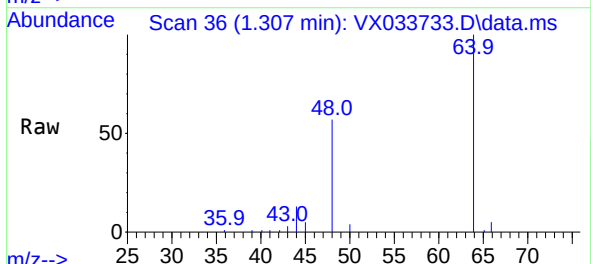



#11

Tert butyl alcohol

Concen: 1.627 ug/l

RT: 2.995 min Scan# 31

Delta R.T. -0.024 min

Lab File: VX033733.D

Acq: 13 Jan 2023 19:24

Instrument :

MSVOA\_X





ClientSampleId :

Tgt Ion: 59 Resp: 347

Ion Ratio Lower Upper

59 100

57 0.0 3.7 5.5#

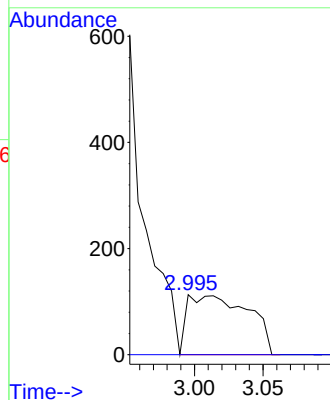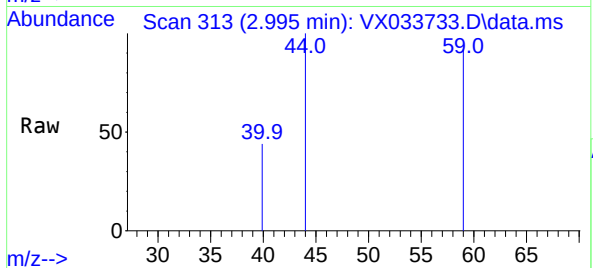

#16

Acetone

Concen: 38.177 ug/l

RT: 2.392 min Scan# 214

Delta R.T. -0.006 min

Lab File: VX033733.D




Acq: 13 Jan 2023 19:24


Tgt Ion: 43 Resp: 21717

Ion Ratio Lower Upper

43 100


58 23.9 22.6 33.8

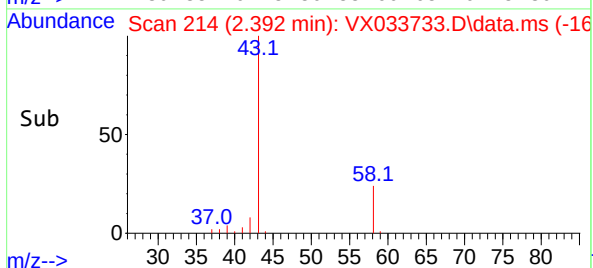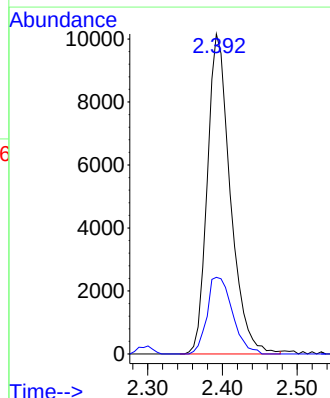






#17  
Carbon Disulfide  
Concen: 1.850 ug/l  
RT: 2.514 min Scan# 21  
Delta R.T. -0.000 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24

Instrument :  
MSVOA\_X  
ClientSampleId :



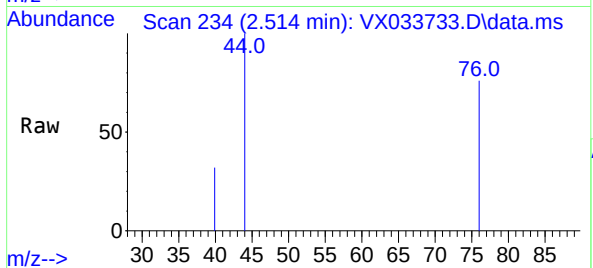



Tgt Ion: 76 Resp: 69  
Ion Ratio Lower Upper  
76 100  
78 0.0 7.0 10.6#

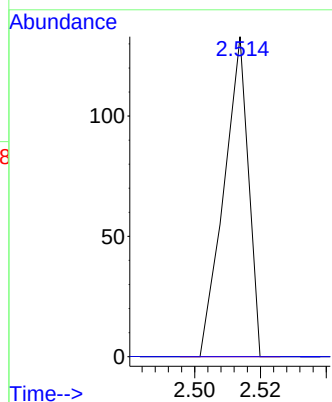

#18  
Methyl Acetate  
Concen: 0.978 ug/l  
RT: 2.709 min Scan# 266  
Delta R.T. -0.000 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24


Tgt Ion: 43 Resp: 1676  
Ion Ratio Lower Upper  
43 100  
74 18.7 18.2 27.4

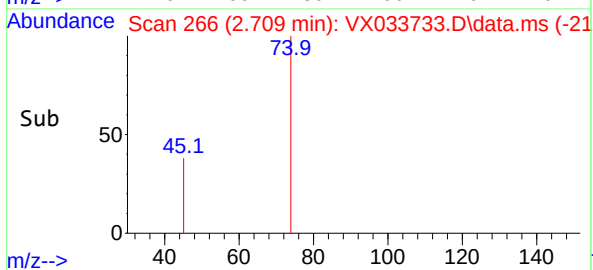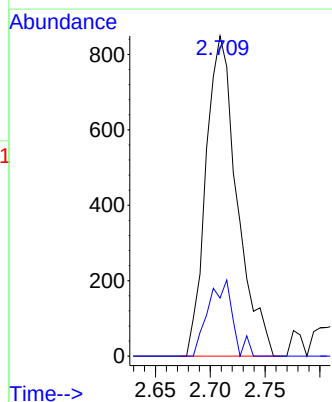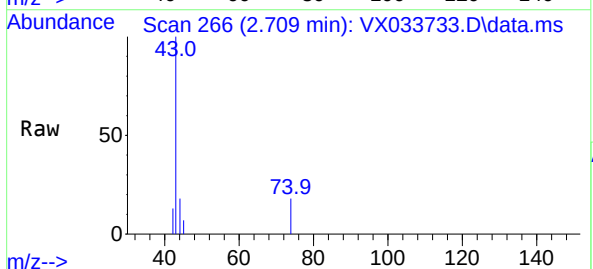

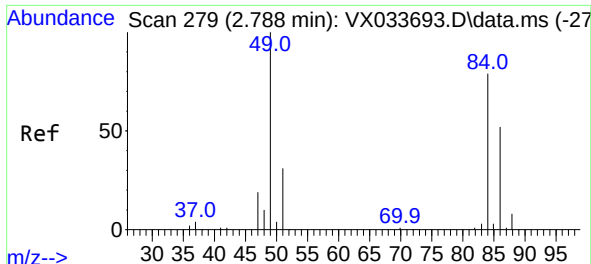




#20  
Methylene Chloride  
Concen: 0.704 ug/l  
RT: 2.794 min Scan# 21  
Delta R.T. 0.006 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24

Instrument :  
MSVOA\_X  
ClientSampleId :



Tgt Ion: 84 Resp: 3388




| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 84  | 100   |       |       |
| 49  | 114.2 | 101.1 | 151.7 |
| 51  | 40.9  | 31.0  | 46.6  |
| 86  | 62.3  | 52.6  | 79.0  |

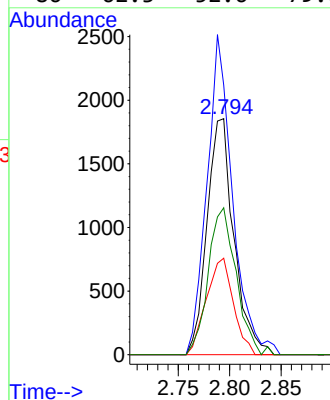


#25  
2-Butanone  
Concen: 8.022 ug/l  
RT: 4.580 min Scan# 573  
Delta R.T. 0.012 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24

Tgt Ion: 43 Resp: 6435

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 43  | 100   |       |       |
| 72  | 20.8  | 19.4  | 29.2  |

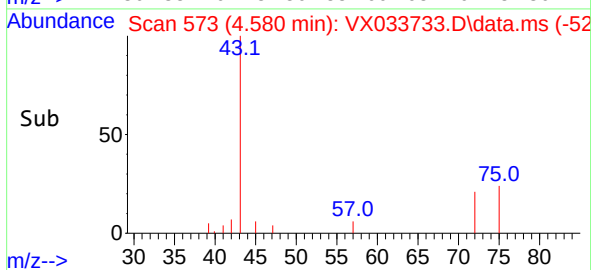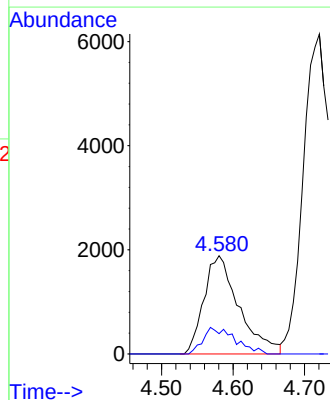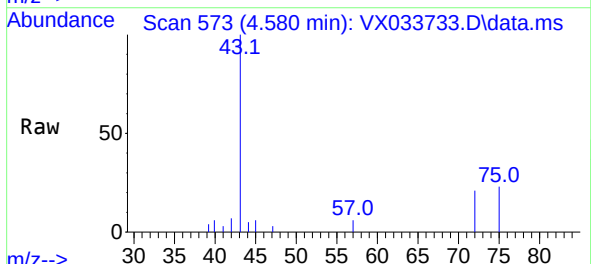



#29

Tetrahydrofuran

Concen: 0.504 ug/l

RT: 5.026 min Scan# 644

Delta R.T. 0.012 min

Lab File: VX033733.D





Acq: 13 Jan 2023 19:24

Instrument :

MSVOA\_X

ClientSampleId :

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 42    | Resp: | 255   |
| Ion      | Ratio | Lower | Upper |
| 42       | 100   |       |       |
| 72       | 0.0   | 34.8  | 52.2# |
| 71       | 7.5   | 32.2  | 48.2# |

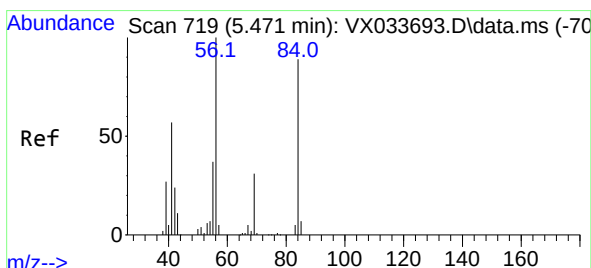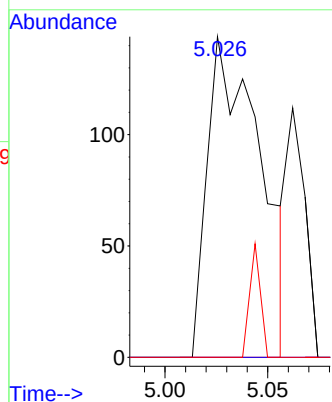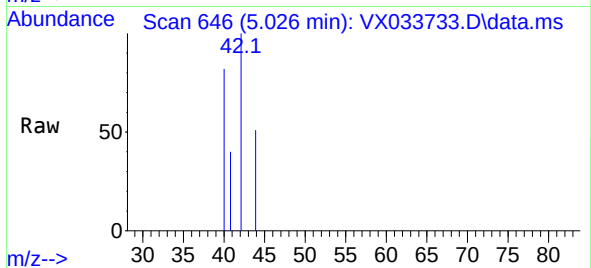

#31

Cyclohexane

Concen: 1.337 ug/l




RT: 5.544 min Scan# 731


Delta R.T. 0.073 min

Lab File: VX033733.D

Acq: 13 Jan 2023 19:24


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 56    | Resp: | 2415  |
| Ion      | Ratio | Lower | Upper |
| 56       | 100   |       |       |
| 69       | 145.6 | 24.6  | 37.0# |
| 84       | 106.5 | 71.0  | 106.6 |

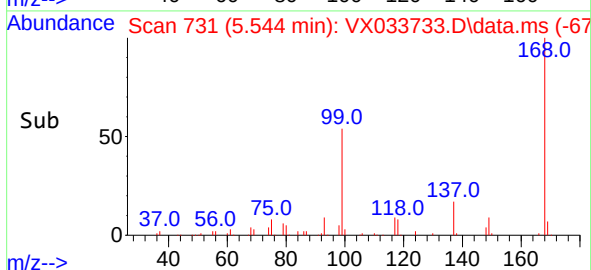






#33  
1,2-Dichloroethane-d4  
Concen: 58.244 ug/l  
RT: 5.958 min Scan# 799  
Delta R.T. -0.000 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24

Instrument :  
MSVOA\_X  
ClientSampleId :






Tgt Ion: 65 Resp: 71508  
Ion Ratio Lower Upper  
65 100  
67 50.5 0.0 104.8

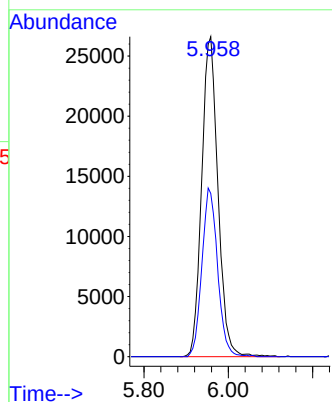


#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.763 min Scan# 931  
Delta R.T. 0.000 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24

Tgt Ion: 114 Resp: 178786  
Ion Ratio Lower Upper  
114 100  
63 21.0 0.0 37.4  
88 15.2 0.0 30.6

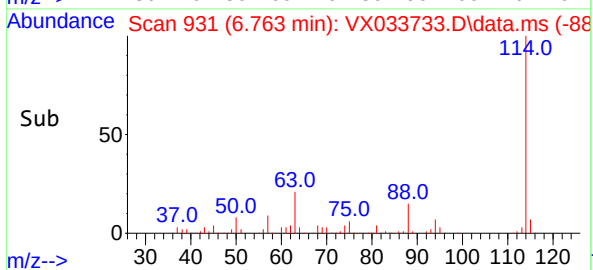






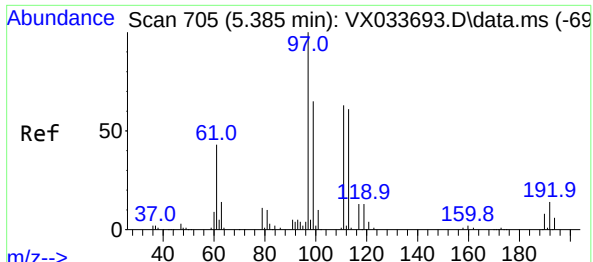


#35  
Dibromofluoromethane  
Concen: 49.431 ug/l  
RT: 5.385 min Scan# 705  
Delta R.T. -0.000 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24

Instrument :  
MSVOA\_X  
ClientSampleId :



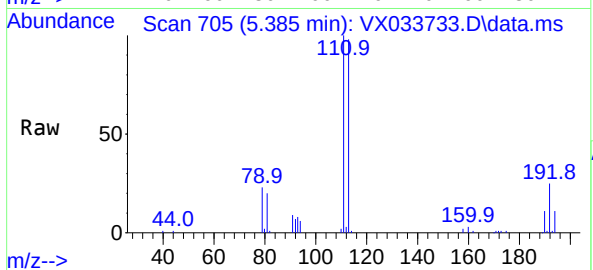



Tgt Ion:113 Resp: 54877  
Ion Ratio Lower Upper  
113 100  
111 101.9 83.0 124.6  
192 23.0 19.0 28.4



#36  
1,1-Dichloropropene  
Concen: 5.197 ug/l  
RT: 5.544 min Scan# 731  
Delta R.T. -0.146 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24

Tgt Ion: 75 Resp: 8420  
Ion Ratio Lower Upper  
75 100  
110 8.8 18.8 56.4#  
77 0.0 25.1 37.7#

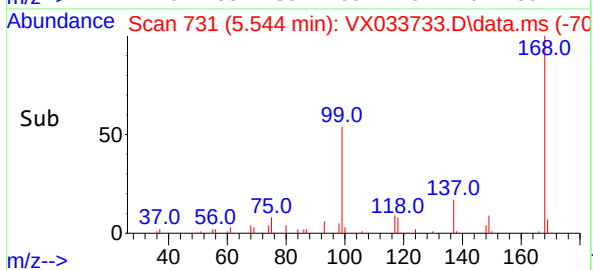



#37

Ethyl Acetate

Concen: 9.617 ug/l

RT: 4.721 min Scan# 595

Delta R.T. 0.006 min


Lab File: VX033733.D

Acq: 13 Jan 2023 19:24

Instrument :

MSVOA\_X

ClientSampleId :

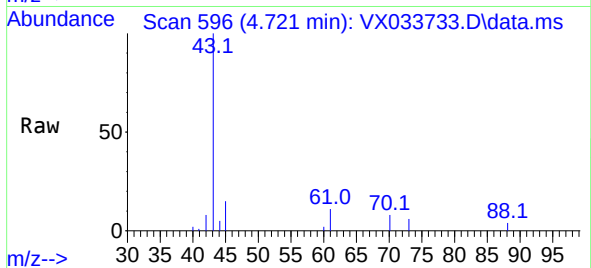




Tgt Ion: 43 Resp: 18436

Ion Ratio Lower Upper

43 100

61 12.8 11.1 16.7

70 10.2 8.5 12.7

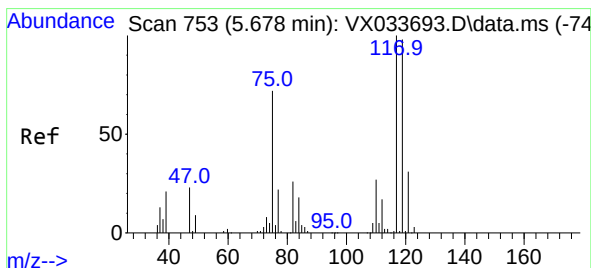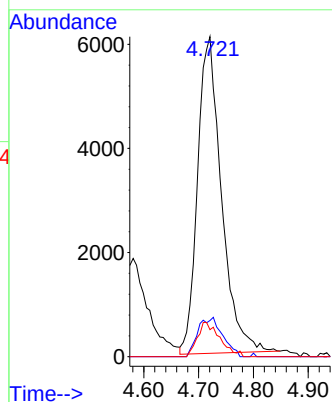

#38

Carbon Tetrachloride

Concen: 6.538 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.128 min

Lab File: VX033733.D

Acq: 13 Jan 2023 19:24




Tgt Ion: 117 Resp: 10971


Ion Ratio Lower Upper

117 100

119 2.4 78.0 117.0#


121 0.0 24.4 36.6#

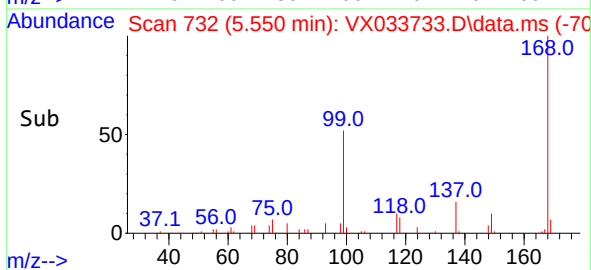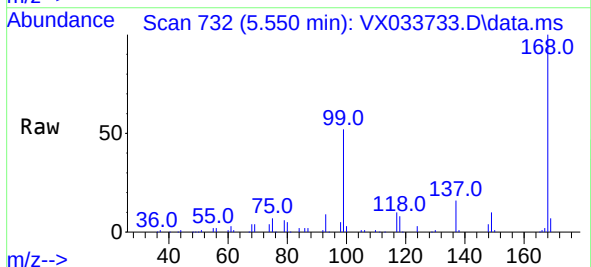






#43  
Isopropyl Acetate  
Concen: 31.844 ug/l  
RT: 6.342 min Scan# 81  
Delta R.T. 0.006 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24

Instrument :  
MSVOA\_X  
ClientSampleId :







Tgt Ion: 43 Resp: 81452  
Ion Ratio Lower Upper  
43 100  
61 17.9 15.7 23.5  
87 12.0 10.6 15.8



#48  
Methyl methacrylate  
Concen: 66.343 ug/l  
RT: 7.799 min Scan# 1101  
Delta R.T. 0.110 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24

Tgt Ion: 41 Resp: 85482  
Ion Ratio Lower Upper  
41 100  
69 0.2 63.1 94.7#  
39 54.7 43.2 64.8

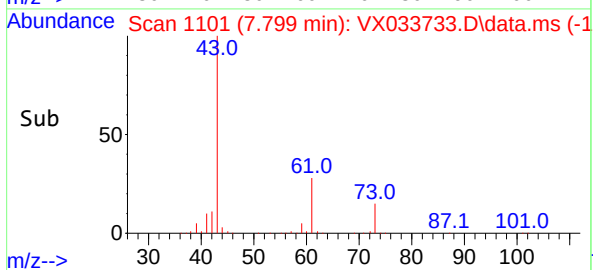



#49

1,4-Dioxane

Concen: 3.123 ug/l

RT: 7.793 min Scan# 1100

Delta R.T. 0.055 min

Lab File: VX033733.D

Acq: 13 Jan 2023 19:24

Instrument :

MSVOA\_X

ClientSampleId :





Tgt Ion: 88 Resp: 89

Ion Ratio Lower Upper

88 100

43 970601.1 0.0 0.0#

58 3684.3 56.5 84.7#

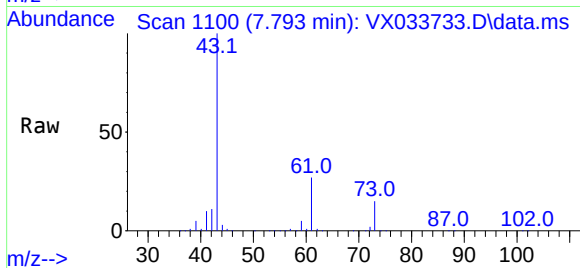

#50

Toluene-d8

Concen: 53.686 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.000 min

Lab File: VX033733.D




Acq: 13 Jan 2023 19:24


Tgt Ion: 98 Resp: 217156

Ion Ratio Lower Upper

98 100

100 66.8 53.6 80.4


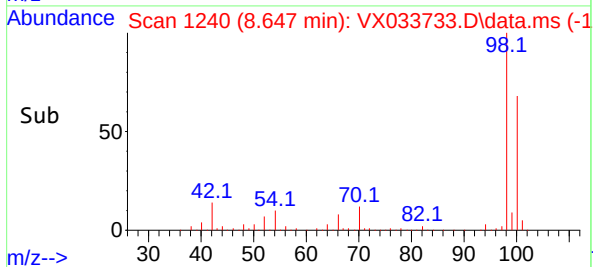

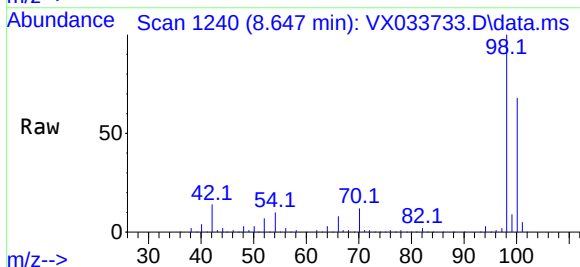




#51  
4-Methyl-2-Pentanone  
Concen: 44.593 ug/l  
RT: 8.549 min Scan# 11  
Delta R.T. -0.024 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 43 Resp: 70051  
Ion Ratio Lower Upper  
43 100  
58 8.1 31.2 46.8#

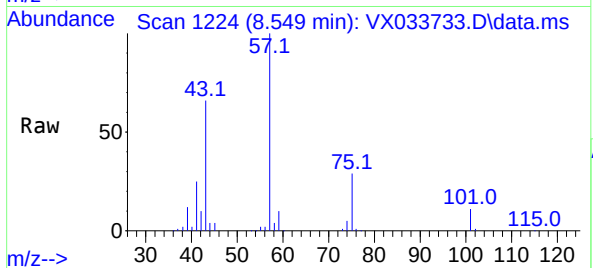

#53  
t-1,3-Dichloropropene  
Concen: 0.324 ug/l  
RT: 8.952 min Scan# 1290  
Delta R.T. -0.024 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24

Tgt Ion: 75 Resp: 516  
Ion Ratio Lower Upper  
75 100  
77 0.0 25.5 38.3#

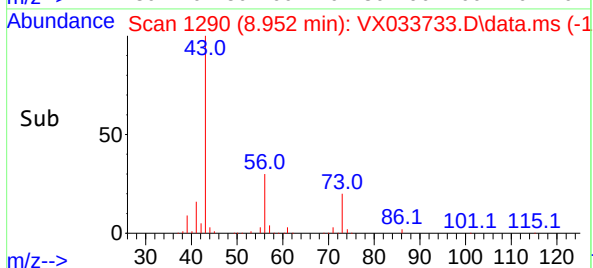



#54

cis-1,3-Dichloropropene

Concen: 15.620 ug/l

RT: 8.549 min Scan# 11

Delta R.T. 0.183 min

Lab File: VX033733.D

Acq: 13 Jan 2023 19:24

Instrument :

MSVOA\_X

ClientSampleId :





Tgt Ion: 75 Resp: 27874

Ion Ratio Lower Upper

75 100

77 0.6 25.0 37.6#

39 41.7 38.6 58.0

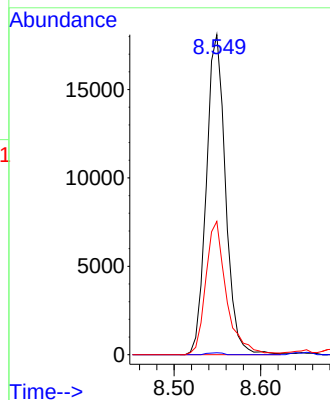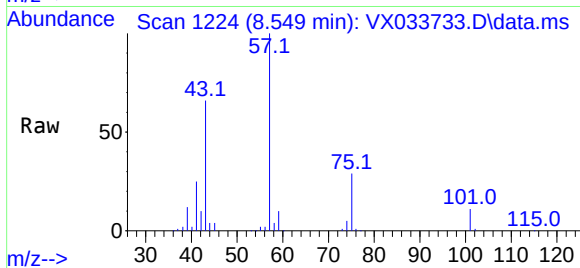

#56

Ethyl methacrylate

Concen: 0.314 ug/l

RT: 9.244 min Scan# 1338

Delta R.T. 0.128 min

Lab File: VX033733.D

Acq: 13 Jan 2023 19:24




Tgt Ion: 69 Resp: 533


Ion Ratio Lower Upper

69 100

41 8746.5 55.1 82.7#

39 3732.5 28.5 42.7#


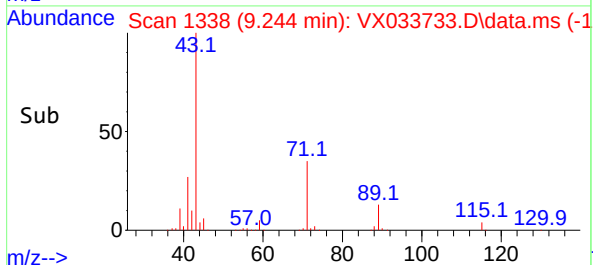
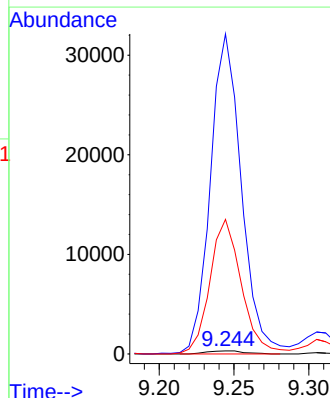
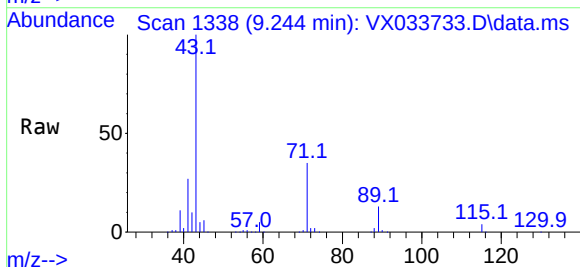




#57  
1,3-Dichloropropane  
Concen: 2.040 ug/l  
RT: 9.482 min Scan# 1377  
Delta R.T. 0.177 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 76 Resp: 3994  
Ion Ratio Lower Upper  
76 100  
78 0.0 25.6 38.4#

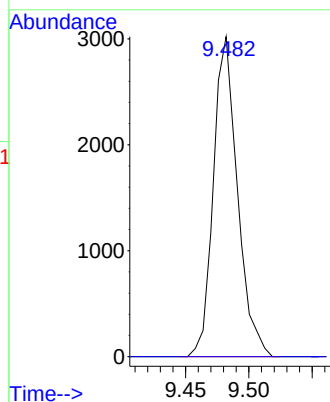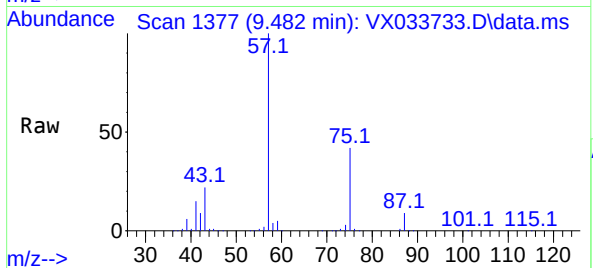

#59  
2-Hexanone  
Concen: 55.252 ug/l  
RT: 9.482 min Scan# 1377  
Delta R.T. 0.049 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24


Tgt Ion: 43 Resp: 60411  
Ion Ratio Lower Upper  
43 100  
58 16.8 27.4 82.0#

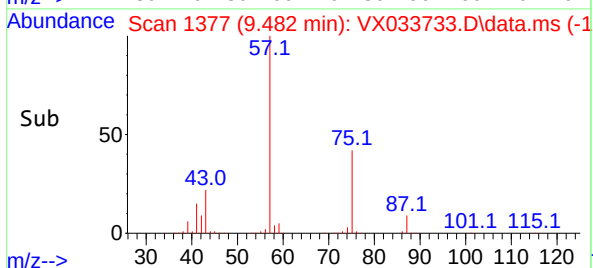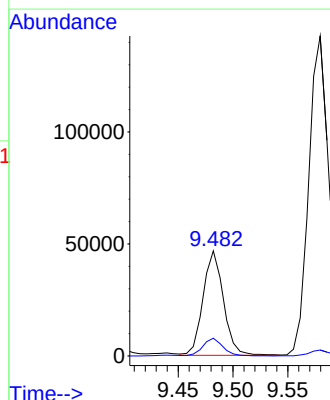






#62  
4-Bromofluorobenzene  
Concen: 52.843 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.000 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24

Instrument :  
MSVOA\_X  
ClientSampleId :



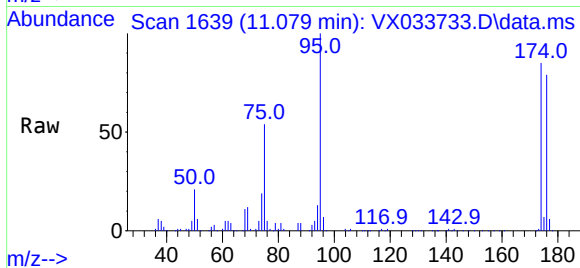


Tgt Ion: 95 Resp: 79360  
Ion Ratio Lower Upper  
95 100  
174 88.1 0.0 184.4  
176 85.1 0.0 178.8

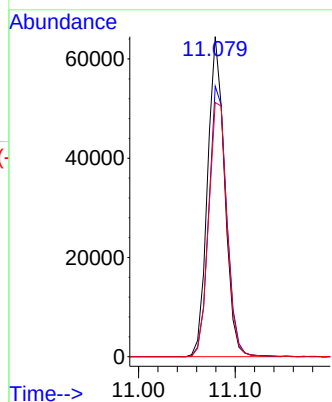


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. 0.000 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24

Tgt Ion: 117 Resp: 175436  
Ion Ratio Lower Upper  
117 100  
82 53.3 40.6 60.8  
119 32.7 25.6 38.4

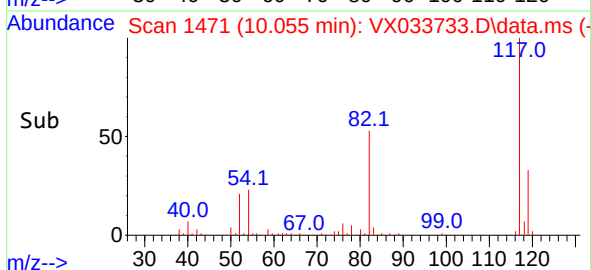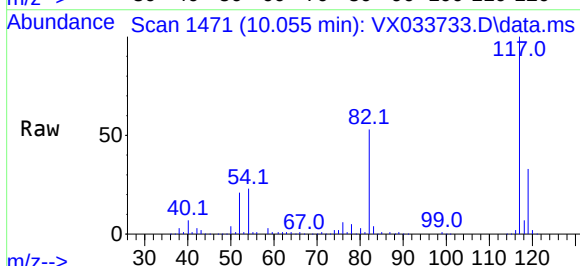









#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.024 min Scan# 11  
Delta R.T. -0.000 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24


Instrument :  
MSVOA\_X  
ClientSampleId :

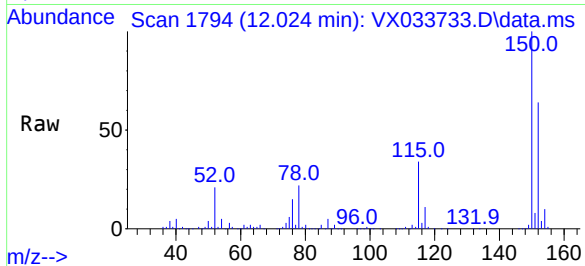



Tgt Ion:152 Resp: 81650  
Ion Ratio Lower Upper  
152 100  
115 55.8 38.7 116.1  
150 156.7 0.0 348.2

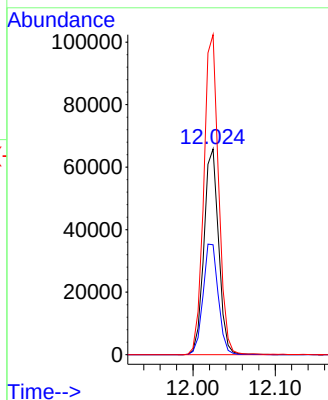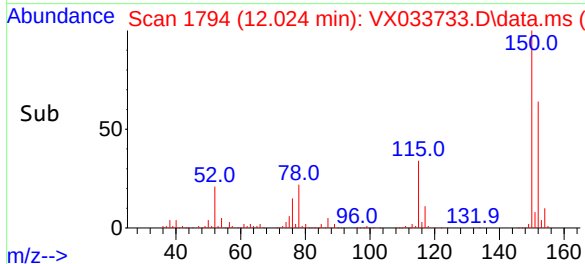


#73  
Isopropylbenzene  
Concen: Below Cal  
RT: 11.079 min Scan# 1639  
Delta R.T. 0.115 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24

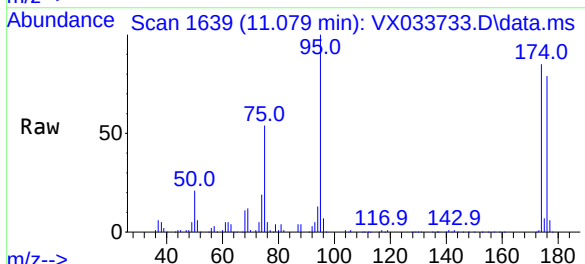


Tgt Ion:105 Resp: 101  
Ion Ratio Lower Upper  
105 100  
120 0.0 13.6 40.8#

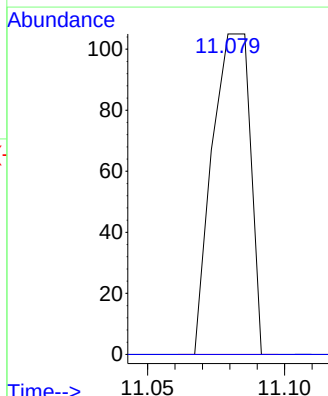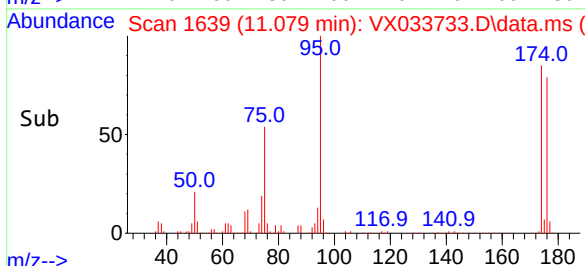



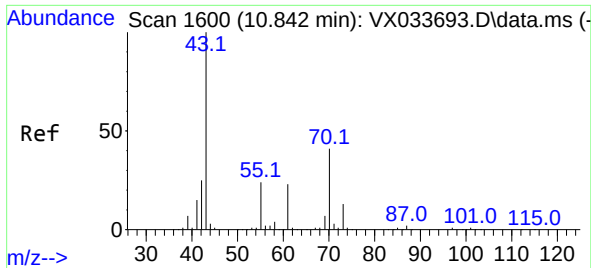


#74  
N-amy1 acetate  
Concen: 9.895 ug/l  
RT: 10.640 min Scan# 1639  
Delta R.T. -0.201 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24

Instrument :  
MSVOA\_X  
ClientSampleId :



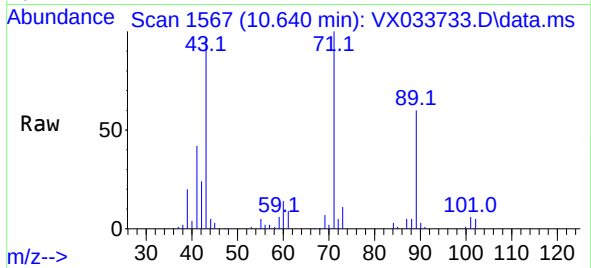



|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 43    | Resp: | 21215 |
| Ion      | Ratio | Lower | Upper |
| 43       | 100   |       |       |
| 70       | 1.8   | 34.8  | 52.2# |
| 55       | 4.8   | 19.4  | 29.0# |
| 61       | 8.9   | 19.4  | 29.2# |

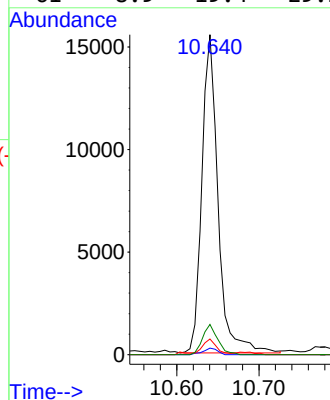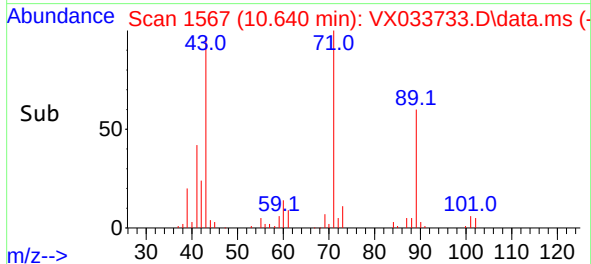

#76  
1,2,3-Trichloropropane  
Concen: 28.435 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.159 min  
Lab File: VX033733.D  
Acq: 13 Jan 2023 19:24


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 75    | Resp: | 42658 |
| Ion      | Ratio | Lower | Upper |
| 75       | 100   |       |       |
| 77       | 1.1   | 21.8  | 65.4# |

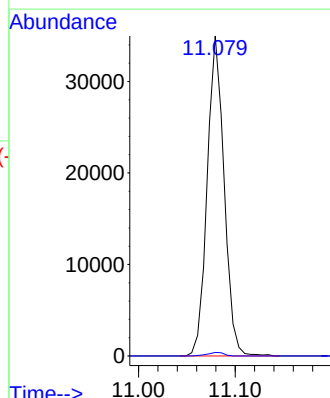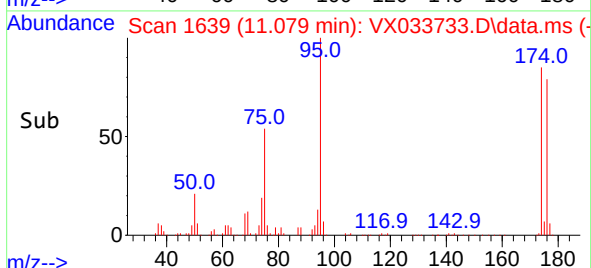



#81  
 trans-1,4-Dichloro-2-butene  
 Concen: 88.373 ug/l  
 RT: 11.079 min Scan# 1  
 Delta R.T. 0.061 min  
 Lab File: VX033733.D  
 Acq: 13 Jan 2023 19:24

Instrument :  
 MSVOA\_X  
 ClientSampleId :



Tgt Ion: 75 Resp: 42658  

| Ion | Ratio | Lower | Upper  |
|-----|-------|-------|--------|
| 75  | 100   |       |        |
| 53  | 0.0   | 83.0  | 124.6# |
| 89  | 0.0   | 37.7  | 56.5#  |

