


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX011519\
Data File : VX007048.D
Acq On : 15 Jan 2019 09:41
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Title : SW846 8260
Last Update : Tue Jan 08 14:06:59 2019

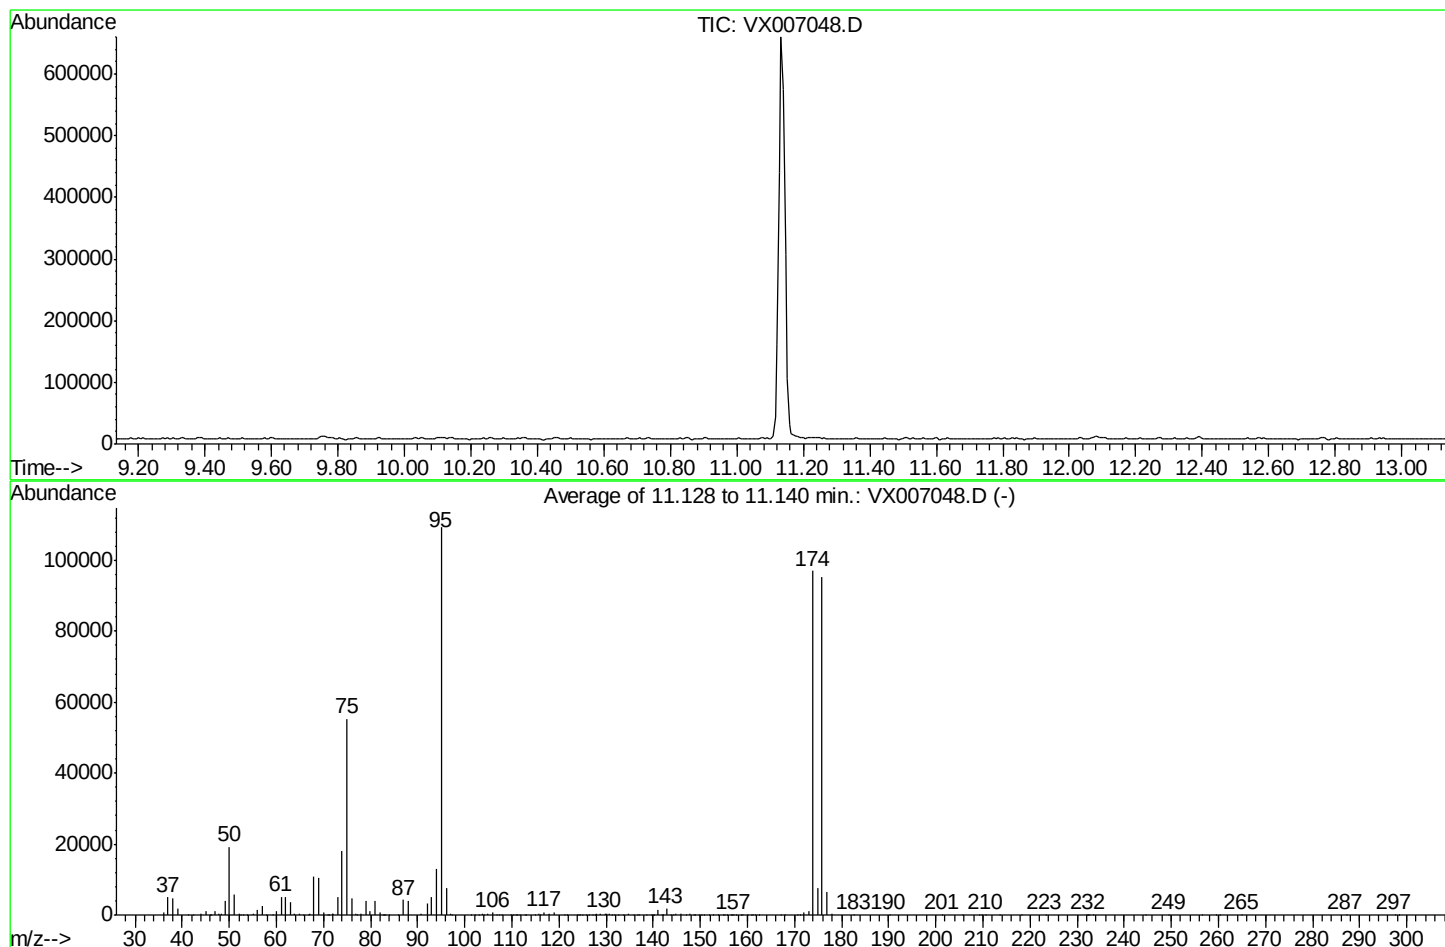

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	19151	PASS
75	95	30	60	50.6	55229	PASS
95	95	100	100	100.0	109256	PASS
96	95	5	9	7.0	7606	PASS
173	174	0.00	2	1.3	1224	PASS
174	95	50	100	88.7	96893	PASS
175	174	5	9	8.0	7757	PASS
176	174	95	101	98.4	95301	PASS
177	176	5	9	6.7	6397	PASS