

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011521\
 Data File : VX020636.D
 Acq On : 15 Jan 2021 17:23
 Operator : JC/MD
 Sample : M1158-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6

Quant Time: Jan 16 00:56:41 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011121W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jan 11 15:05:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	197582	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.830	114	345598	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.098	117	321610	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.061	152	138290	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.031	65	137975	58.14	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	116.28%
35) Dibromofluoromethane	5.464	113	117421	49.04	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	98.08%
50) Toluene-d8	8.695	98	413953	48.31	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	96.62%
62) 4-Bromofluorobenzene	11.122	95	148195	48.98	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	97.96%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011521\
Data File : VX020636.D
Acq On : 15 Jan 2021 17:23
Operator : JC/MD
Sample : M1158-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Quant Time: Jan 16 00:56:41 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011121W.M
Quant Title : SW846 8260
QLast Update : Mon Jan 11 15:05:37 2021
Response via : Initial Calibration




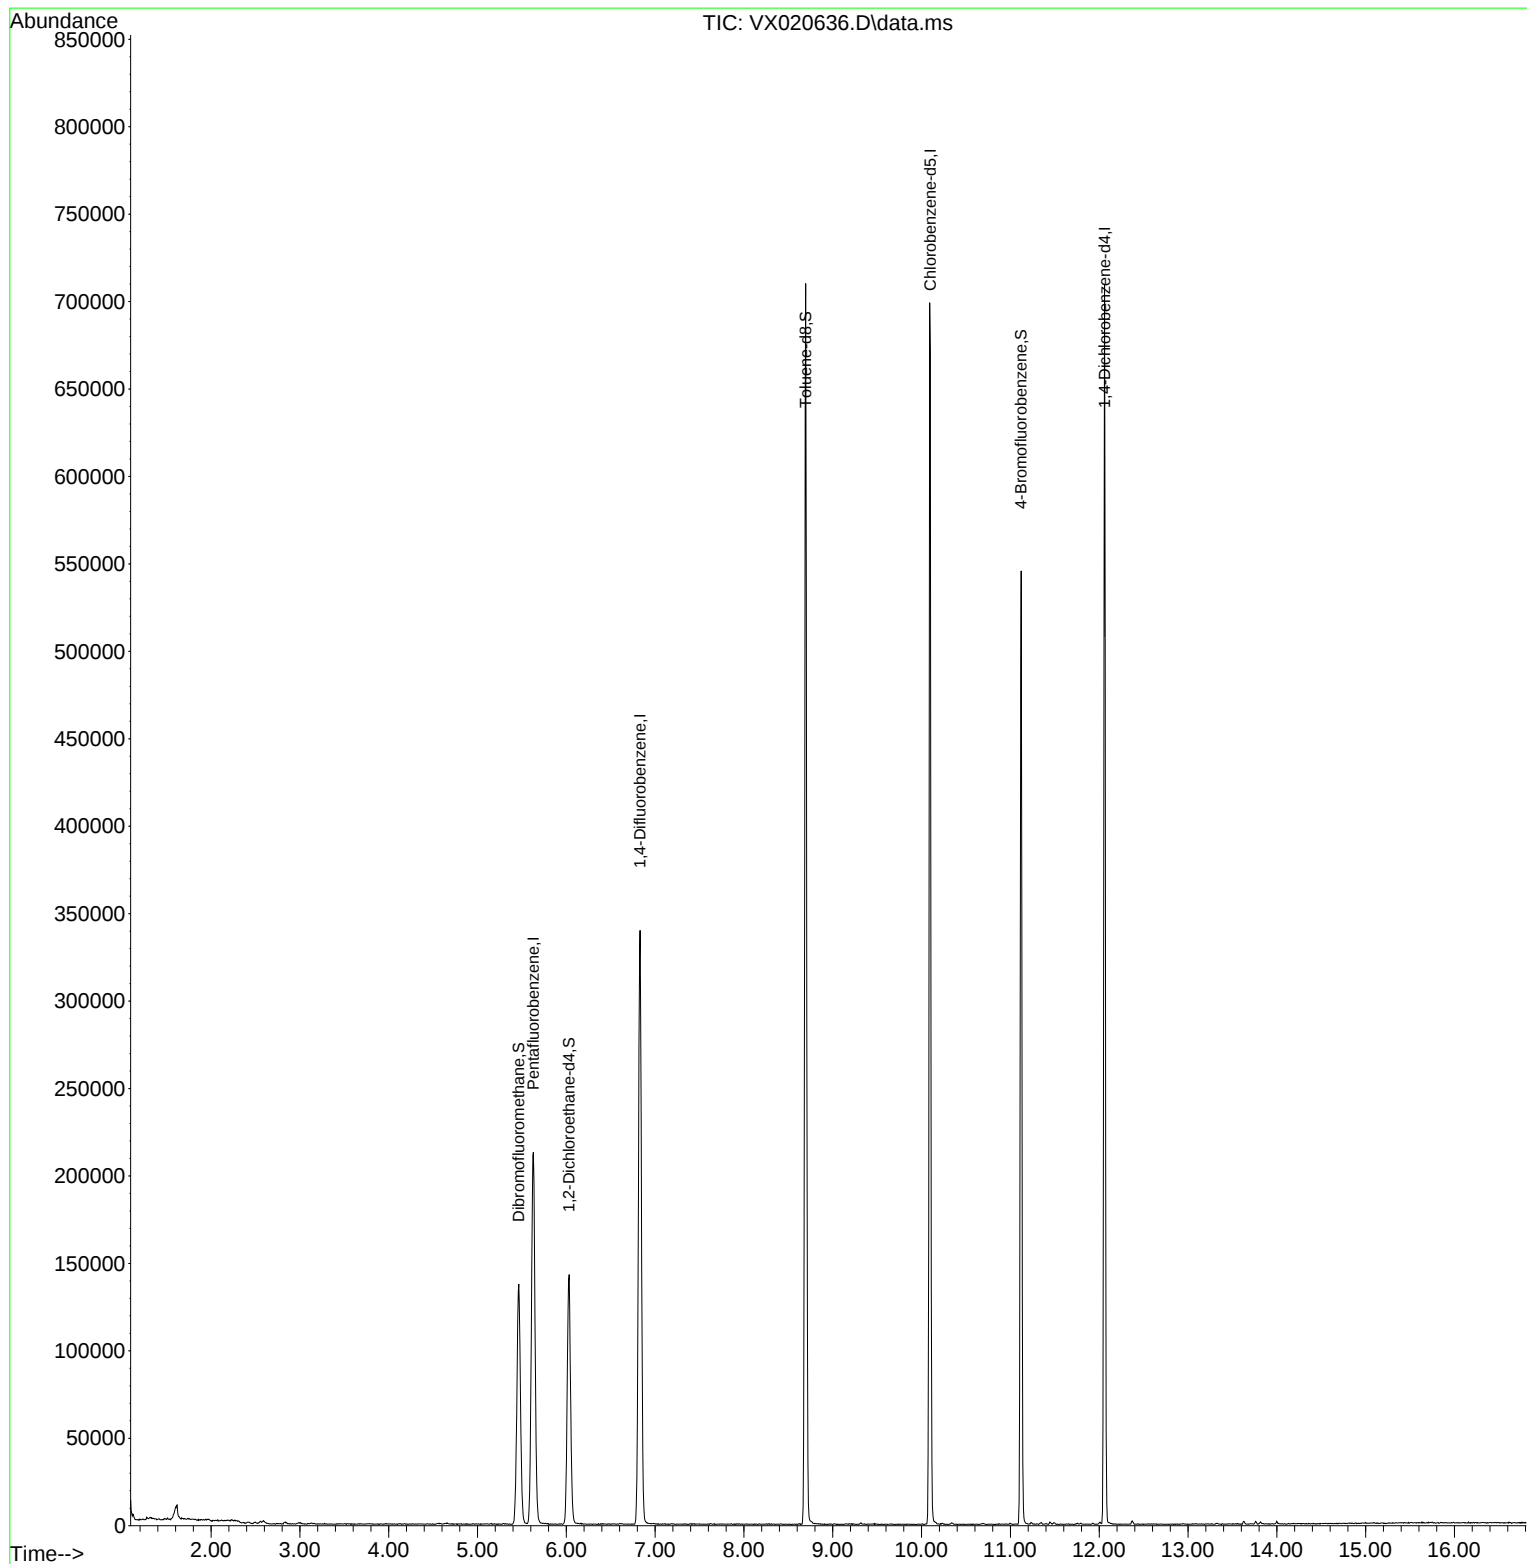


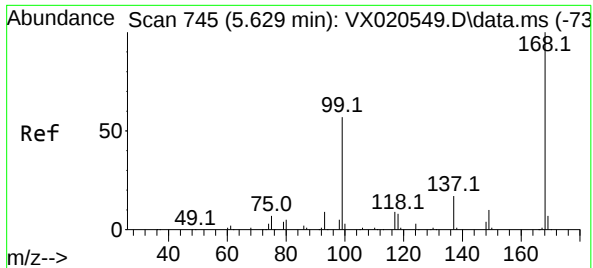

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 745
Delta R.T. -0.000 min
Lab File: VX020636.D
Acq: 15 Jan 2021 17:23




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:168 Resp: 197582
Ion Ratio Lower Upper
168 100
99 62.1 45.8 68.6

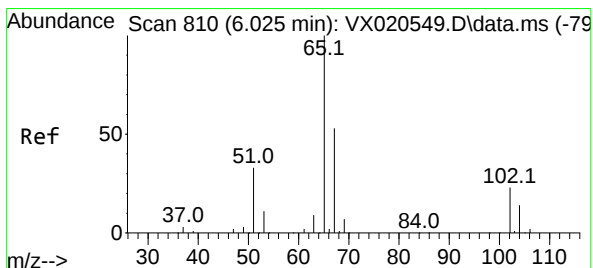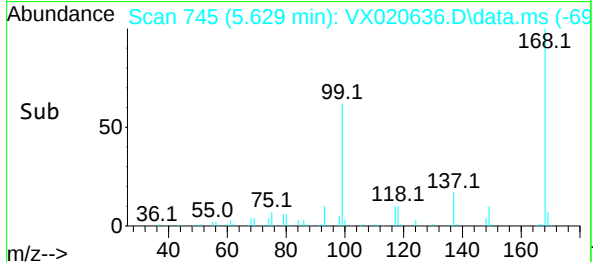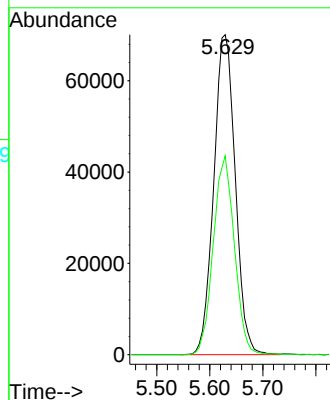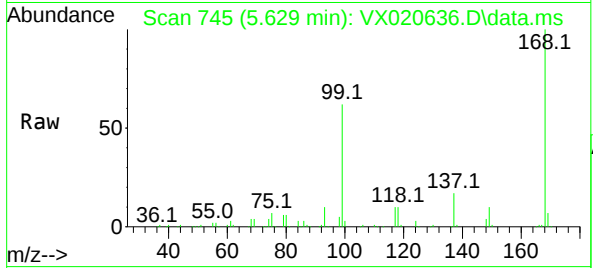

#33
1,2-Dichloroethane-d4
Concen: 58.14 ug/l
RT: 6.031 min Scan# 811
Delta R.T. 0.006 min
Lab File: VX020636.D
Acq: 15 Jan 2021 17:23

Tgt Ion: 65 Resp: 137975
Ion Ratio Lower Upper
65 100
67 51.4 0.0 105.4


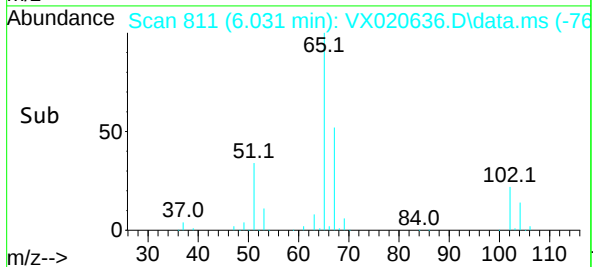
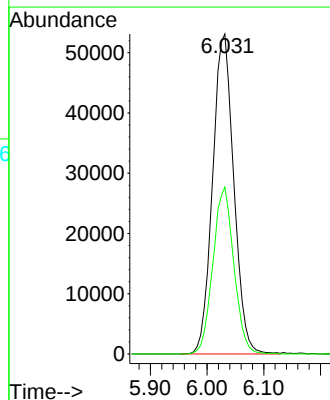
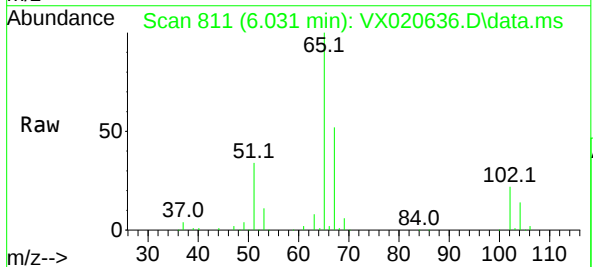


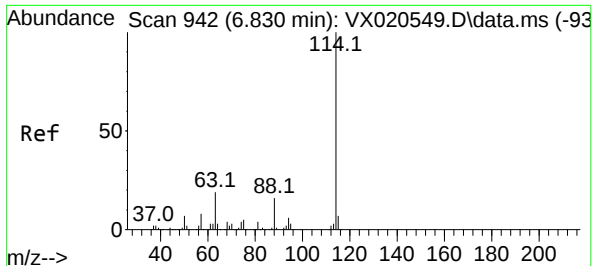

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.830 min Scan# 942
Delta R.T. -0.000 min
Lab File: VX020636.D
Acq: 15 Jan 2021 17:23




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:114 Resp: 345598
Ion Ratio Lower Upper
114 100
63 19.5 0.0 40.8
88 15.9 0.0 32.8

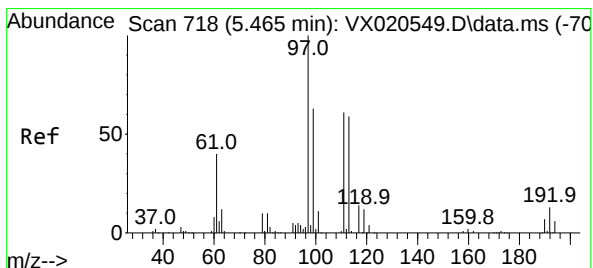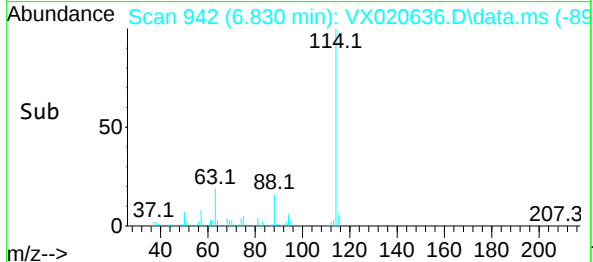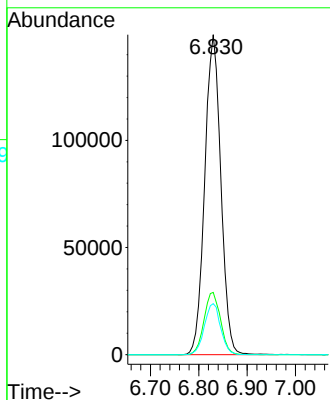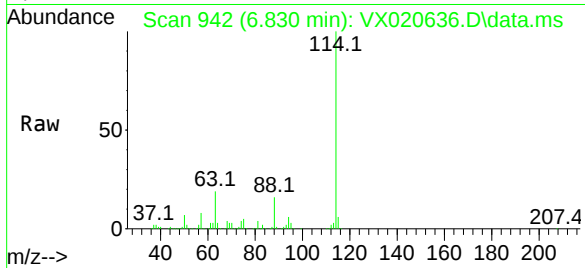

#35
Dibromofluoromethane
Concen: 49.04 ug/l
RT: 5.464 min Scan# 718
Delta R.T. -0.001 min
Lab File: VX020636.D
Acq: 15 Jan 2021 17:23

Tgt Ion:113 Resp: 117421
Ion Ratio Lower Upper
113 100
111 101.6 81.9 122.9
192 18.9 16.7 25.1


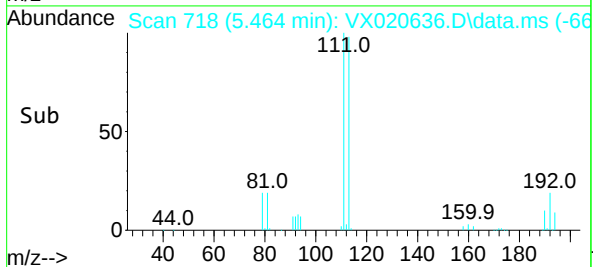
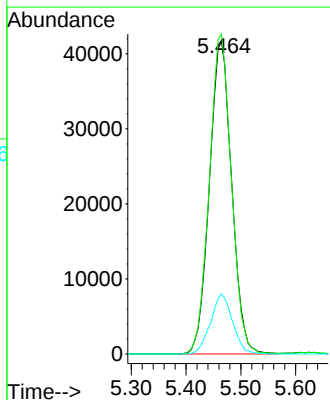
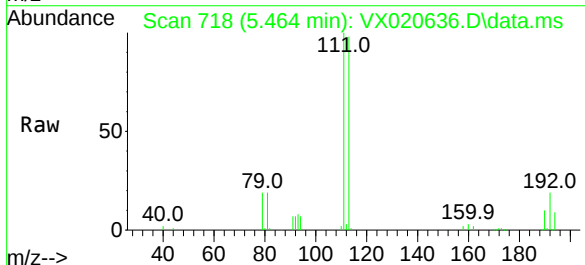


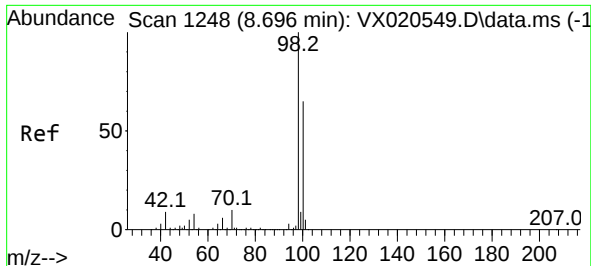

#50
Toluene-d8
Concen: 48.31 ug/l
RT: 8.695 min Scan# 1248
Delta R.T. -0.001 min
Lab File: VX020636.D
Acq: 15 Jan 2021 17:23




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion: 98 Resp: 413953
Ion Ratio Lower Upper
98 100
100 65.8 51.9 77.9

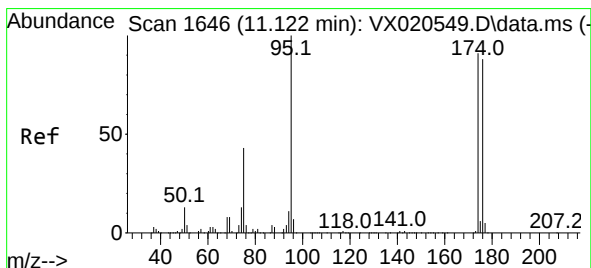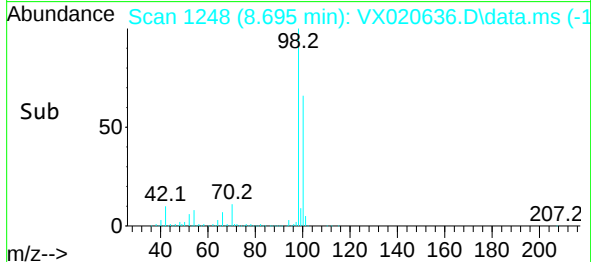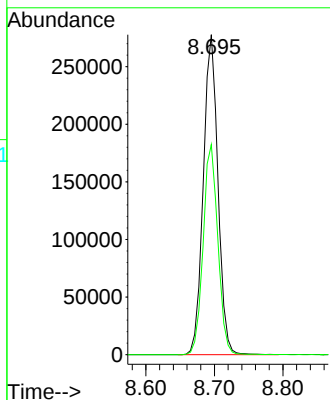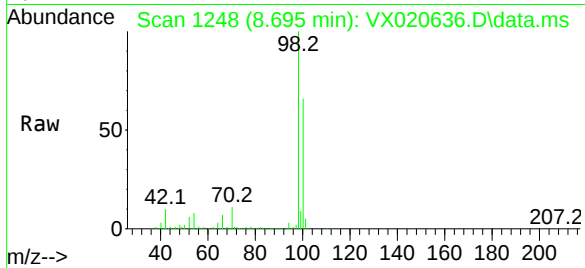

#62
4-Bromofluorobenzene
Concen: 48.98 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. -0.000 min
Lab File: VX020636.D
Acq: 15 Jan 2021 17:23

Tgt Ion: 95 Resp: 148195
Ion Ratio Lower Upper
95 100
174 74.3 0.0 154.6
176 71.3 0.0 155.8


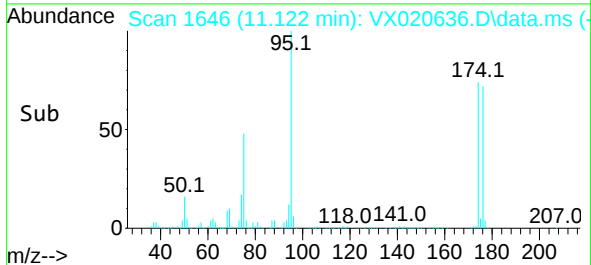
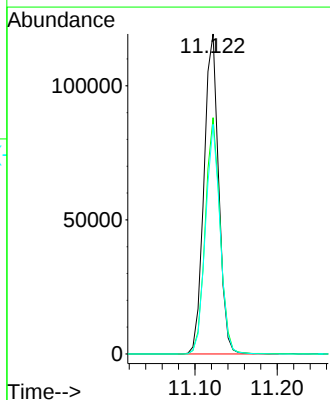
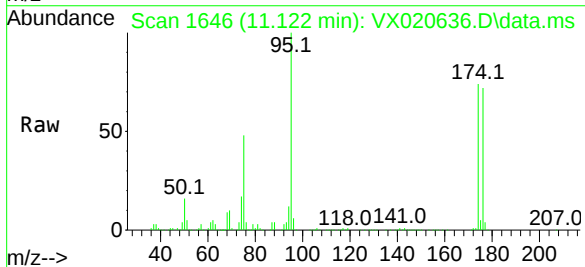


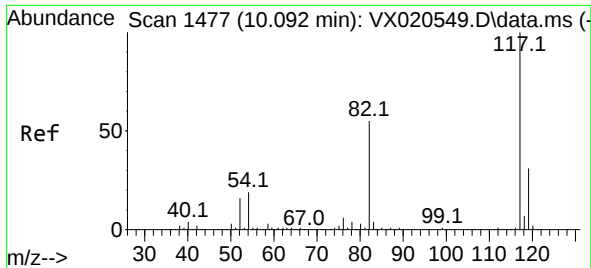

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.098 min Scan# 1478
Delta R.T. 0.006 min
Lab File: VX020636.D
Acq: 15 Jan 2021 17:23

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tgt Ion:117 Resp: 321610
Ion Ratio Lower Upper
117 100
82 52.1 47.4 71.2
119 32.2 26.6 39.8

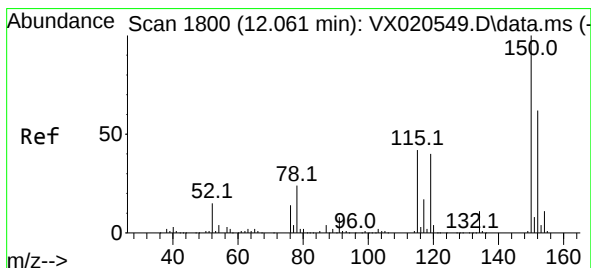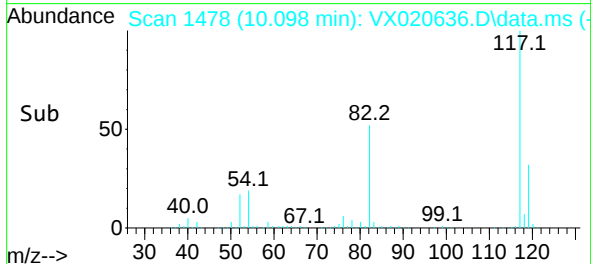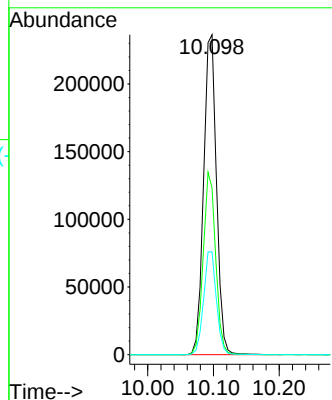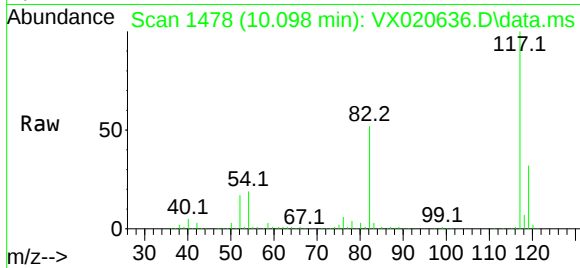

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.061 min Scan# 1800
Delta R.T. -0.000 min
Lab File: VX020636.D
Acq: 15 Jan 2021 17:23

Tgt Ion:152 Resp: 138290
Ion Ratio Lower Upper
152 100
115 62.7 41.1 123.3
150 159.5 0.0 349.0

