
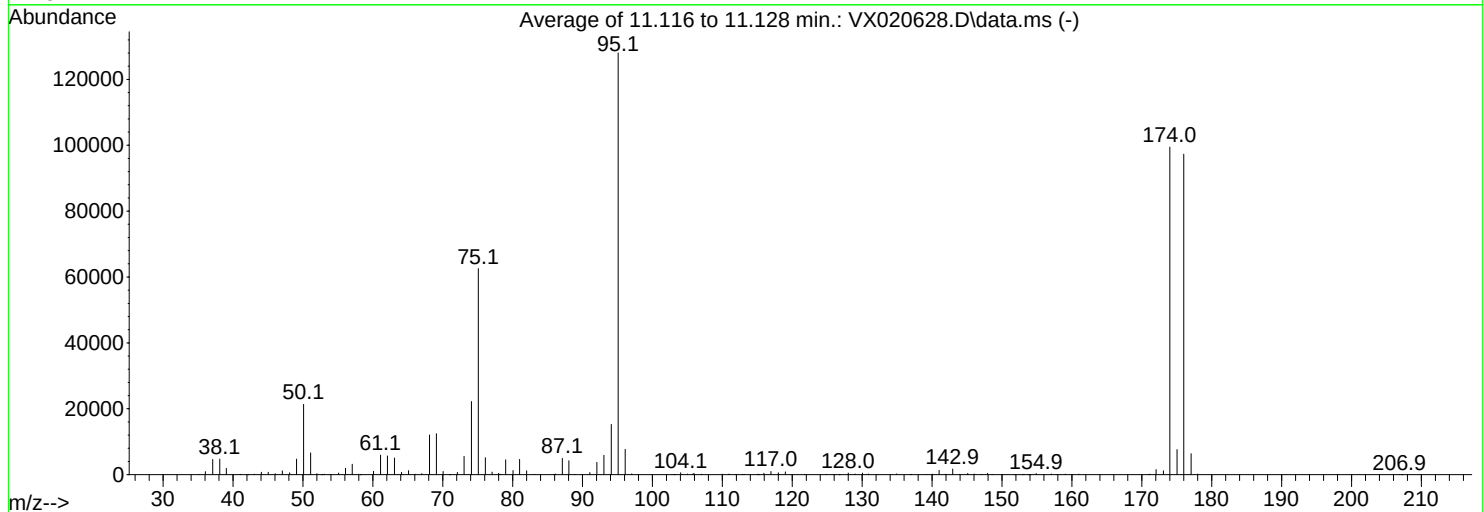


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011521\
 Data File : VX020628.D
 Acq On : 15 Jan 2021 12:08
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X011121W.M
 Title : SW846 8260
 Last Update : Mon Jan 11 15:05:37 2021

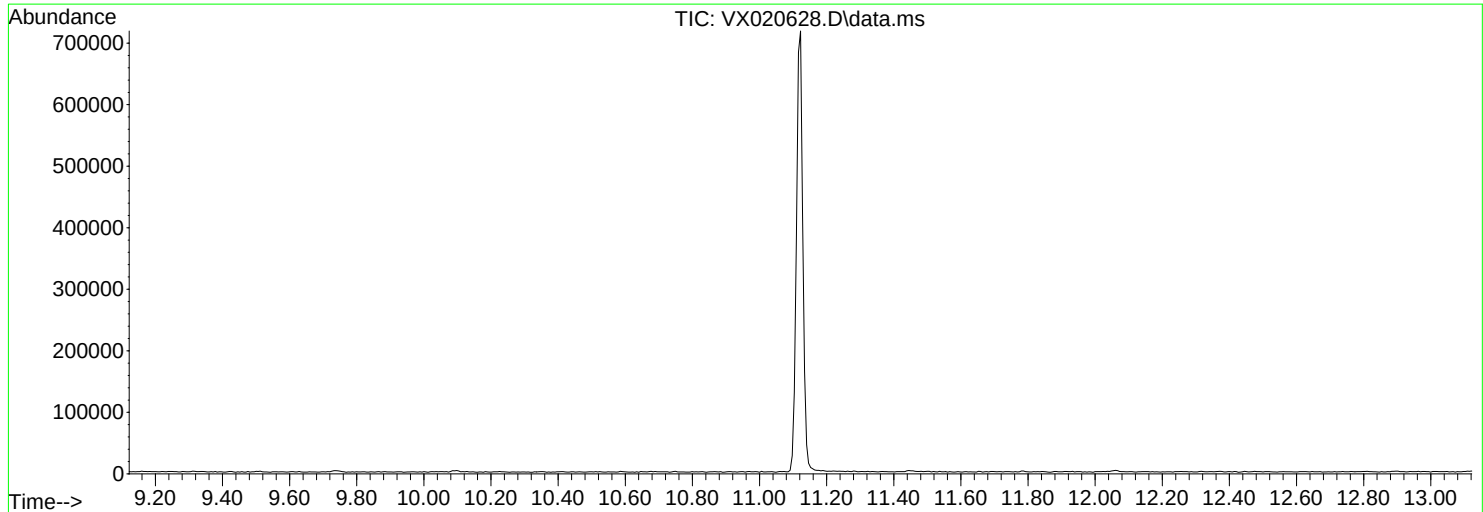

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	21346	PASS
75	95	30	60	48.9	62581	PASS
95	95	100	100	100.0	128056	PASS
96	95	5	9	6.0	7659	PASS
173	174	0.00	2	1.2	1159	PASS
174	95	50	100	77.7	99445	PASS
175	174	5	9	7.7	7638	PASS
176	174	95	101	97.8	97293	PASS
177	176	5	9	6.6	6373	PASS