

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011522\
 Data File : VX026471.D
 Acq On : 14 Jan 2022 22:32
 Operator : JC/MD
 Sample : N1124-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 17 00:42:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 11 14:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	135640	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	228034	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	195750	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	86603	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	94736	49.998	ug/l	0.00
Spiked Amount 50.000	Range 78	- 117	Recovery	= 100.000%		
35) Dibromofluoromethane	5.391	113	71982	48.882	ug/l	0.00
Spiked Amount 50.000	Range 75	- 124	Recovery	= 97.760%		
50) Toluene-d8	8.653	98	260565	49.103	ug/l	0.00
Spiked Amount 50.000	Range 92	- 112	Recovery	= 98.200%		
62) 4-Bromofluorobenzene	11.079	95	95223	50.514	ug/l	0.00
Spiked Amount 50.000	Range 83	- 123	Recovery	= 101.020%		
Target Compounds						Qvalue
11) Tert butyl alcohol	2.959	59	194	0.736	ug/l #	75
13) Acrolein	2.252	56	72	0.257	ug/l	99
14) Allyl chloride	2.794	41	724	0.278	ug/l #	25
16) Acetone	2.386	43	233577	241.731	ug/l	98
18) Methyl Acetate	2.709	43	1041	0.542	ug/l #	81
20) Methylene Chloride	2.794	84	18458	11.562	ug/l	99
25) 2-Butanone	4.568	43	3773	3.003	ug/l	94
27) cis-1,2-Dichloroethene	4.495	96	1025	0.586	ug/l	96
29) Tetrahydrofuran	5.032	42	305	0.409	ug/l #	39
31) Cyclohexane	5.556	56	2837	1.015	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	10822	4.655	ug/l #	50
38) Carbon Tetrachloride	5.556	117	14440	6.039	ug/l #	16
39) Methylcyclohexane	7.385	83	1113	0.397	ug/l #	81
43) Isopropyl Acetate	6.349	43	12127	3.192	ug/l	98
48) Methyl methacrylate	7.799	41	63823	33.903	ug/l #	45
49) 1,4-Dioxane	7.806	88	29	0.939	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	42324	18.785	ug/l #	50
52) Toluene	8.720	92	3758	0.954	ug/l	99
54) cis-1,3-Dichloropropene	8.549	75	18836	7.677	ug/l #	60
55) 1,1,2-Trichloroethane	9.110	97	520	0.338	ug/l #	15
57) 1,3-Dichloropropane	9.482	76	10887	4.084	ug/l #	43
59) 2-Hexanone	9.482	43	162035	93.963	ug/l #	50
67) Ethyl Benzene	10.195	91	44628	5.958	ug/l	96
68) m/p-Xylenes	10.299	106	73217	26.118	ug/l	98
69) o-Xylene	10.640	106	58138	21.492	ug/l	98
70) Styrene	10.640	104	2890	0.655	ug/l #	1
73) Isopropylbenzene	10.964	105	52821	7.441	ug/l	99
74) N-amyl acetate	10.860	43	1467	0.535	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	11.220	83	1579	0.829	ug/l #	29
76) 1,2,3-Trichloropropane	11.378	75	6089	3.193	ug/l #	1
78) n-propylbenzene	11.305	91	130540	16.126	ug/l	99
79) 2-Chlorotoluene	11.378	91	86931	17.709	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	485448	82.949	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.079	75	49437	78.622	ug/l #	3
82) 4-Chlorotoluene	11.451	91	53649	9.509	ug/l #	46
83) tert-Butylbenzene	11.713	119	19239	3.521	ug/l	91

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011522\
 Data File : VX026471.D
 Acq On : 14 Jan 2022 22:32
 Operator : JC/MD
 Sample : N1124-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 17 00:42:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 11 14:45:13 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
84) 1,2,4-Trimethylbenzene	11.756	105	1335395	228.134	ug/l	97
85) sec-Butylbenzene	11.890	105	65255	9.234	ug/l	98
86) p-Isopropyltoluene	12.012	119	78812	13.293	ug/l	100
89) n-Butylbenzene	12.323	91	84826	16.672	ug/l #	20
90) Hexachloroethane	12.530	117	15642	17.299	ug/l #	14
92) 1,2-Dibromo-3-Chloropr...	12.963	75	1166	2.532	ug/l #	3
95) Naphthalene	13.780	128	227348	36.905	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011522\
Data File : VX026471.D
Acq On : 14 Jan 2022 22:32
Operator : JC/MD
Sample : N1124-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jan 17 00:42:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 11 14:45:13 2022
Response via : Initial Calibration

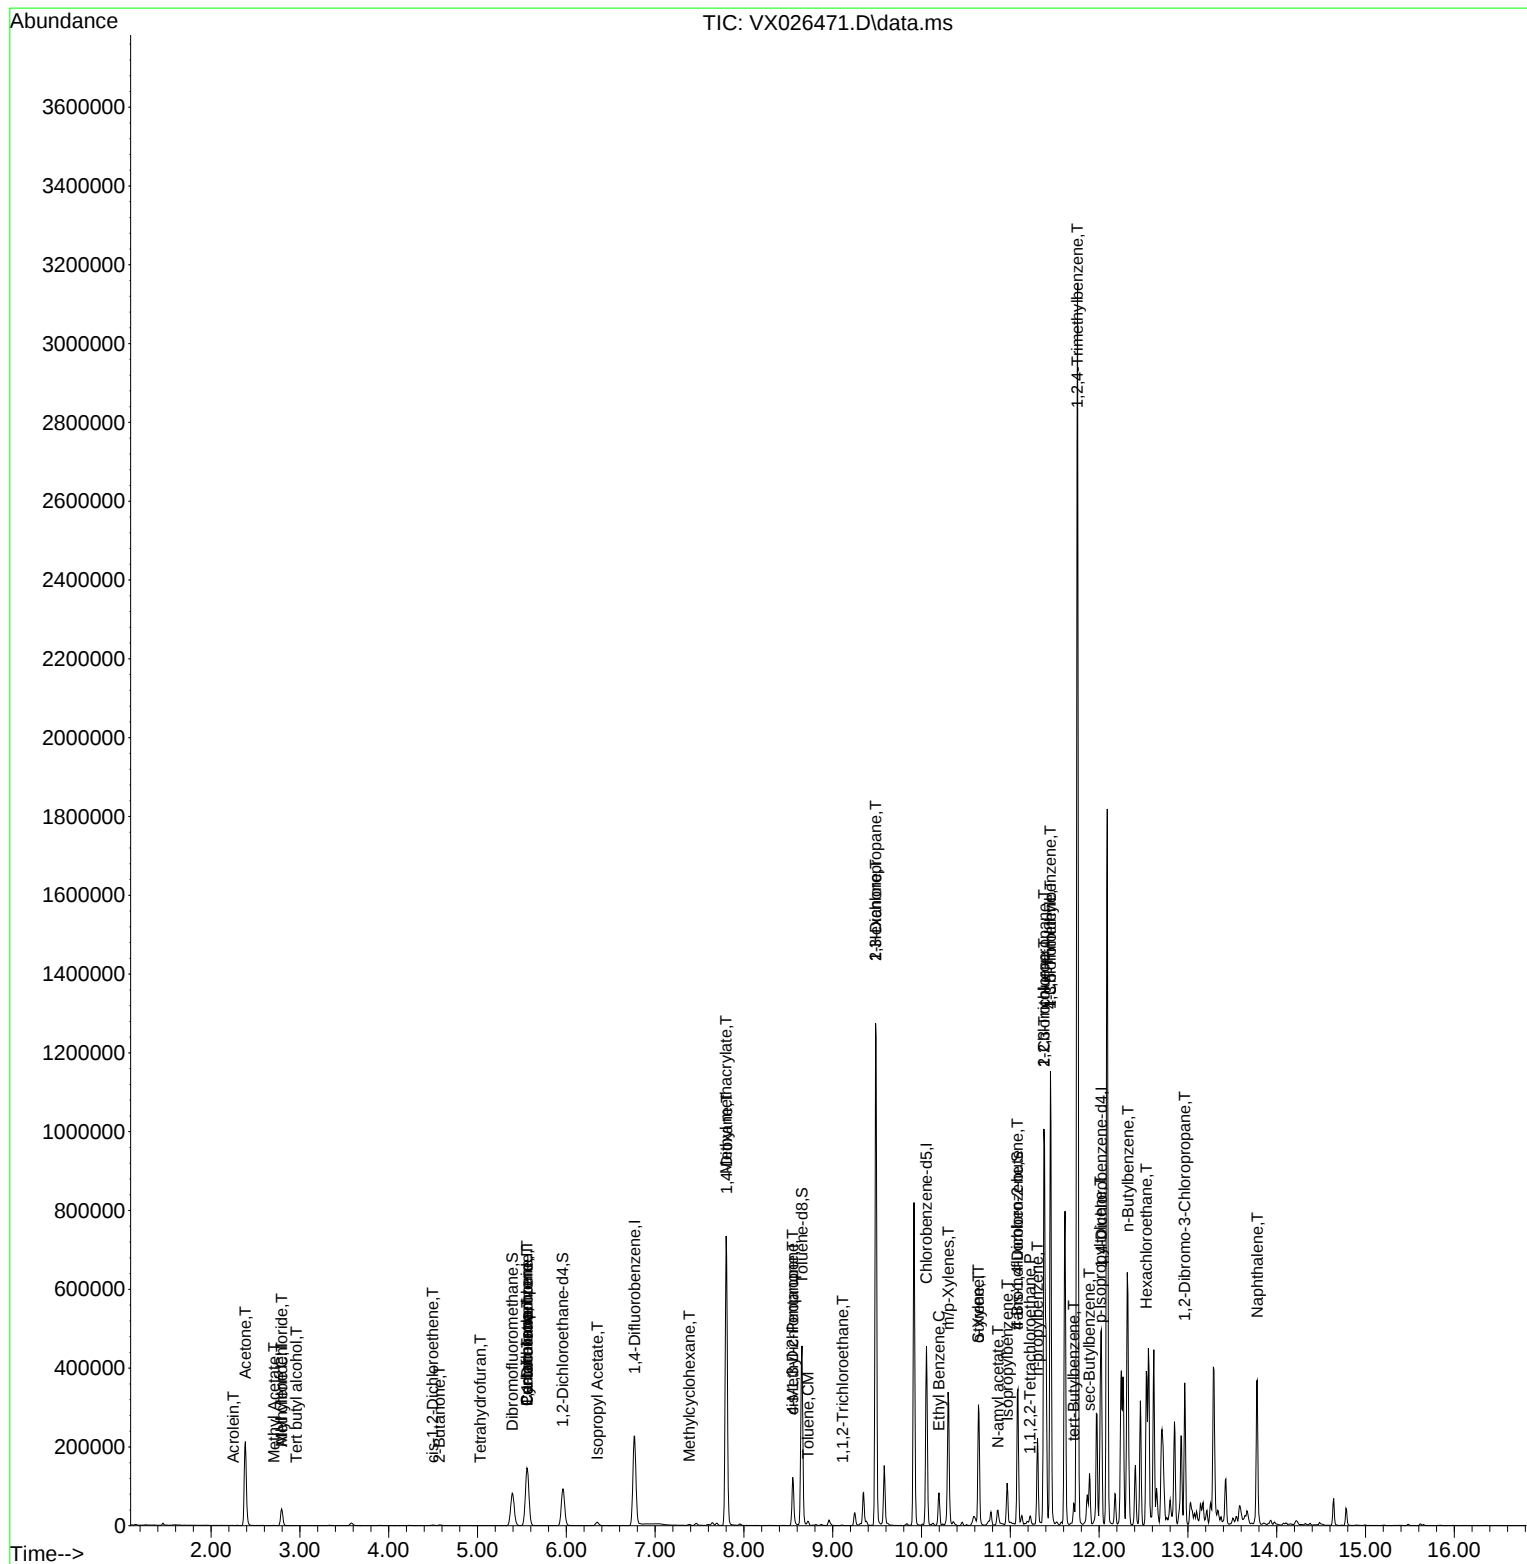



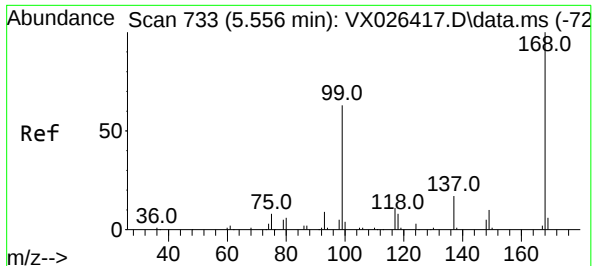


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:168 Resp: 135640
Ion Ratio Lower Upper
168 100
99 61.6 50.3 75.5

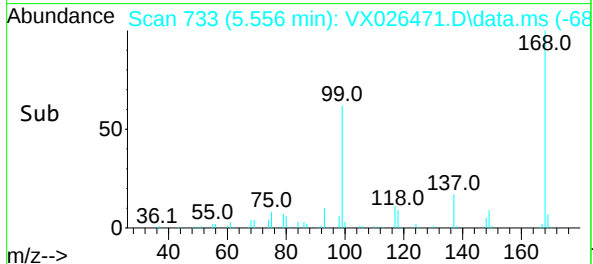

#11
Tert butyl alcohol
Concen: 0.736 ug/l
RT: 2.959 min Scan# 307
Delta R.T. -0.048 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32

Tgt Ion: 59 Resp: 194
Ion Ratio Lower Upper
59 100
57 0.0 7.2 10.8#

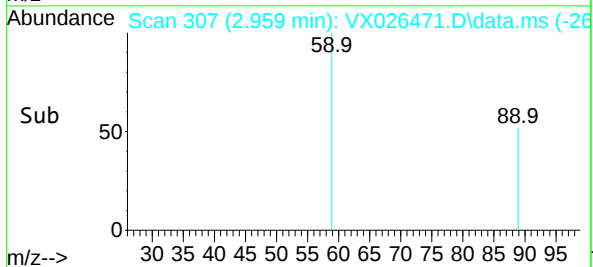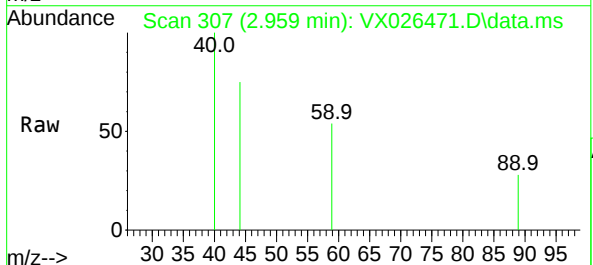

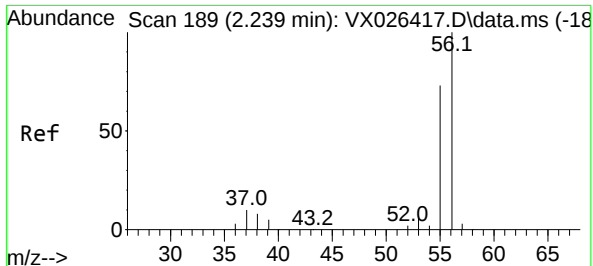

#13

Acrolein

Concen: 0.257 ug/l

RT: 2.252 min Scan# 191

Delta R.T. 0.012 min

Lab File: VX026471.D

Acq: 14 Jan 2022 22:32

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 56 Resp: 72

Ion Ratio Lower Upper

56 100

55 72.2 56.9 85.3

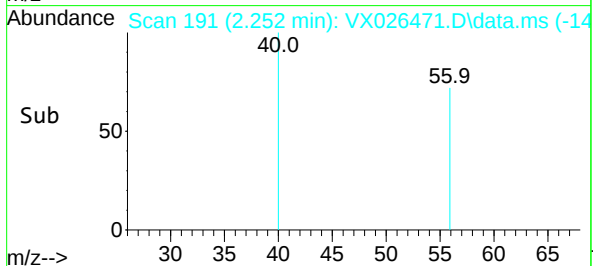

#14

Allyl chloride

Concen: 0.278 ug/l

RT: 2.794 min Scan# 280

Delta R.T. 0.122 min

Lab File: VX026471.D

Acq: 14 Jan 2022 22:32




Tgt Ion: 41 Resp: 724


Ion Ratio Lower Upper

41 100

39 0.0 54.2 81.4#

76 0.0 25.2 37.8#


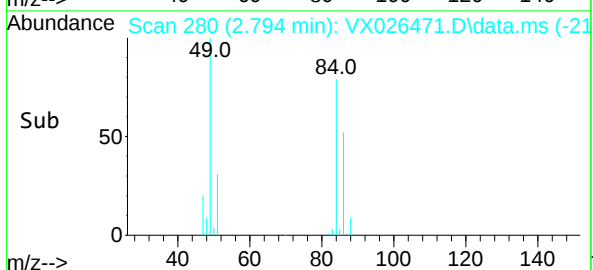

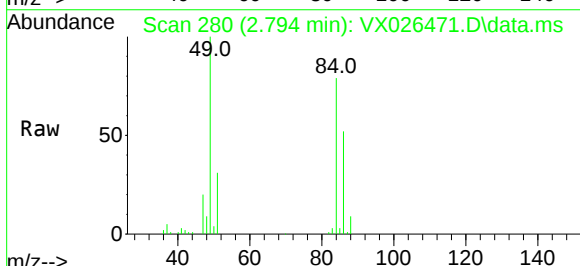




#16
Acetone
Concen: 241.731 ug/l
RT: 2.386 min Scan# 214
Delta R.T. -0.006 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 233577
Ion Ratio Lower Upper
43 100
58 29.6 23.0 34.6



#18
Methyl Acetate
Concen: 0.542 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.000 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32

Tgt Ion: 43 Resp: 1041
Ion Ratio Lower Upper
43 100
74 13.7 18.3 27.5#

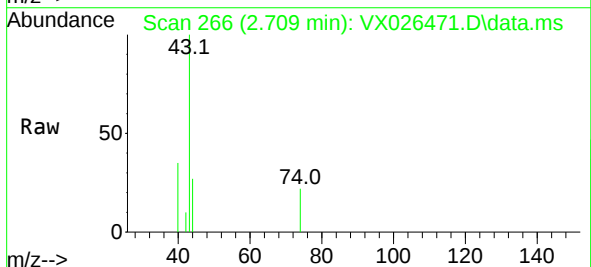



#20

Methylene Chloride

Concen: 11.562 ug/l

RT: 2.794 min Scan# 21

Delta R.T. 0.000 min


Lab File: VX026471.D

Acq: 14 Jan 2022 22:32

Instrument :

MSVOA_X

ClientSampleId :



Tgt Ion: 84 Resp: 18458




Ion Ratio Lower Upper

84 100

49 126.0 101.5 152.3

51 39.3 31.2 46.8

86 64.9 51.3 76.9



#25

2-Butanone

Concen: 3.003 ug/l

RT: 4.568 min Scan# 571

Delta R.T. 0.006 min

Lab File: VX026471.D




Acq: 14 Jan 2022 22:32


Tgt Ion: 43 Resp: 3773

Ion Ratio Lower Upper

43 100

72 22.2 20.4 30.6

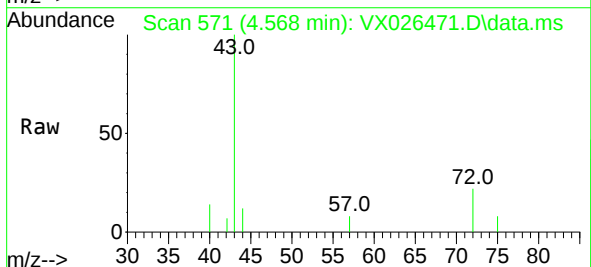



#27

cis-1,2-Dichloroethene

Concen: 0.586 ug/l

RT: 4.495 min Scan# 51

Delta R.T. 0.000 min


Lab File: VX026471.D

Acq: 14 Jan 2022 22:32

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion: 96 Resp: 1025

Ion Ratio Lower Upper

96 100

61 143.9 0.0 296.6

98 67.9 0.0 128.8



#29

Tetrahydrofuran

Concen: 0.409 ug/l

RT: 5.032 min Scan# 647

Delta R.T. 0.018 min

Lab File: VX026471.D

Acq: 14 Jan 2022 22:32




Tgt Ion: 42 Resp: 305


Ion Ratio Lower Upper

42 100

72 6.2 34.6 52.0#


71 0.0 31.8 47.8#

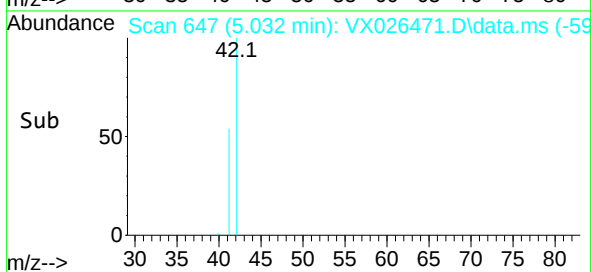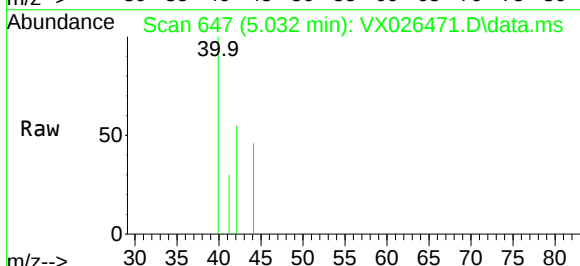



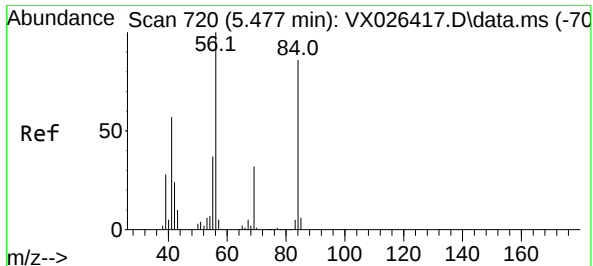


#31
Cyclohexane
Concen: 1.015 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.079 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 2837
Ion Ratio Lower Upper
56 100
69 199.1 25.8 38.6#
84 158.5 68.9 103.3#

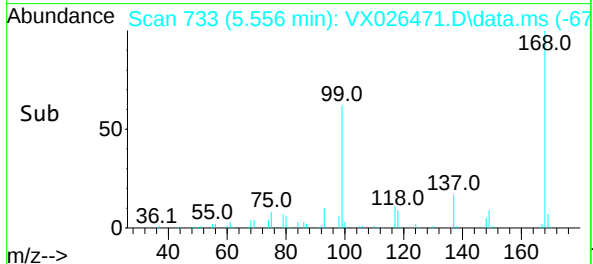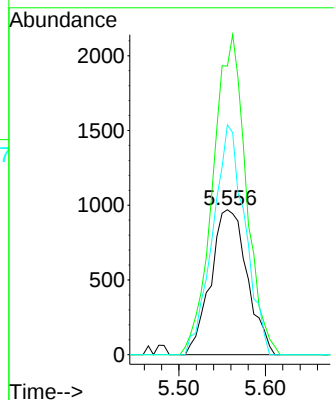

#33
1,2-Dichloroethane-d4
Concen: 49.998 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32

Tgt Ion: 65 Resp: 94736
Ion Ratio Lower Upper
65 100
67 50.3 0.0 100.8


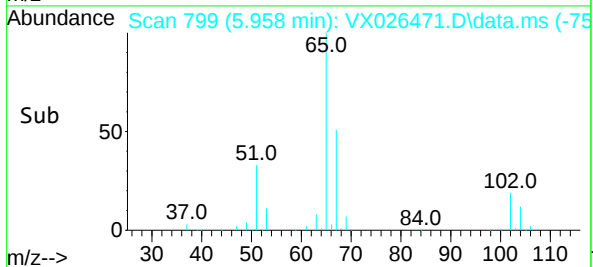
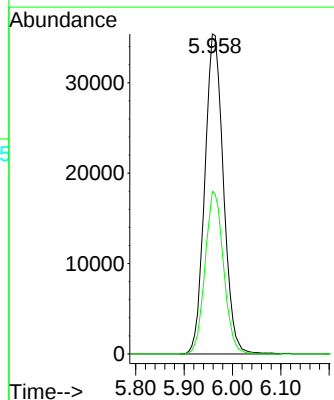
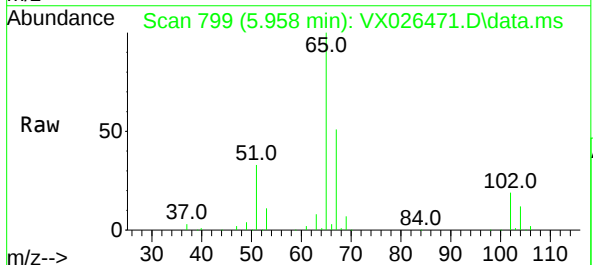




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 228034
Ion Ratio Lower Upper
114 100
63 20.9 0.0 42.8
88 16.0 0.0 33.0



#35
Dibromofluoromethane
Concen: 48.882 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32

Tgt Ion:113 Resp: 71982
Ion Ratio Lower Upper
113 100
111 102.5 81.2 121.8
192 19.1 15.0 22.4

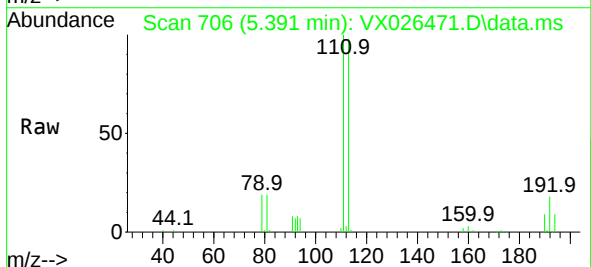



#36

1,1-Dichloropropene

Concen: 4.655 ug/l

RT: 5.556 min Scan# 71

Delta R.T. -0.140 min


Lab File: VX026471.D

Acq: 14 Jan 2022 22:32

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion: 75 Resp: 10822

Ion Ratio Lower Upper

75 100

110 9.2 17.2 51.6#

77 0.0 24.6 36.8#



#38

Carbon Tetrachloride

Concen: 6.039 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.128 min

Lab File: VX026471.D

Acq: 14 Jan 2022 22:32




Tgt Ion: 117 Resp: 14440


Ion Ratio Lower Upper

117 100

119 4.1 74.7 112.1#

121 0.0 25.4 38.0#

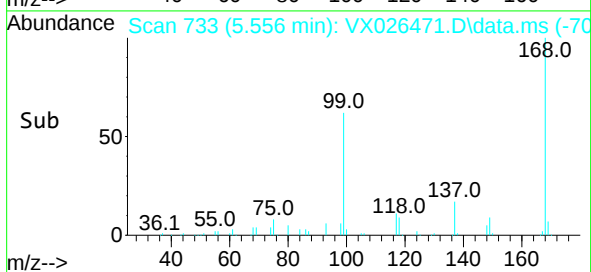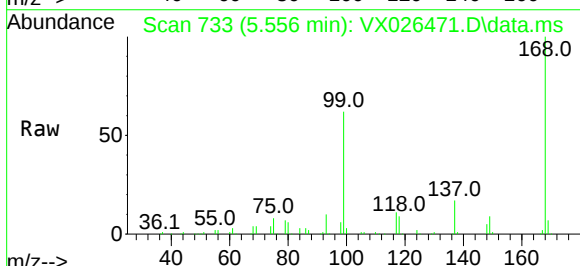

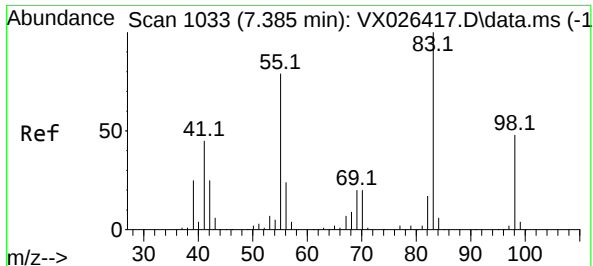

#39

Methylcyclohexane

Concen: 0.397 ug/l

RT: 7.385 min Scan# 1

Delta R.T. 0.000 min


Lab File: VX026471.D

Acq: 14 Jan 2022 22:32



Instrument :

MSVOA_X

ClientSampleId :



Tgt Ion: 83	Resp: 1113
Ion Ratio	Lower Upper
83	100
55	103.0 63.6 95.4#
98	51.6 38.4 57.6

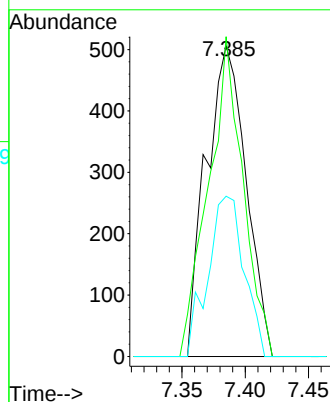

#43

Isopropyl Acetate

Concen: 3.192 ug/l




RT: 6.349 min Scan# 863


Delta R.T. 0.006 min

Lab File: VX026471.D

Acq: 14 Jan 2022 22:32

Tgt Ion: 43	Resp: 12127
Ion Ratio	Lower Upper
43	100
61	18.6 15.4 23.0
87	11.7 10.2 15.2

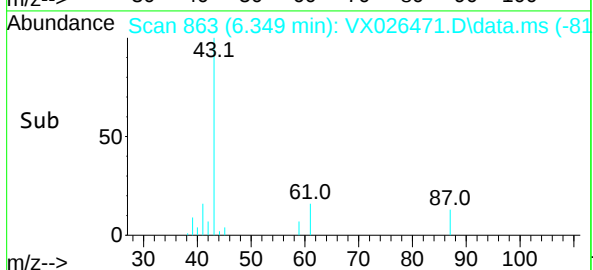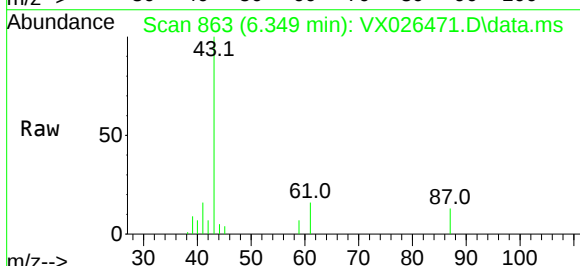

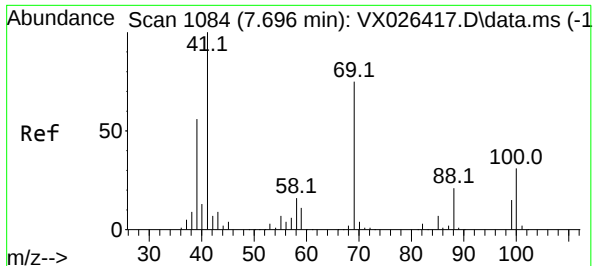

#48

Methyl methacrylate

Concen: 33.903 ug/l

RT: 7.799 min Scan# 1101

Delta R.T. 0.104 min

Lab File: VX026471.D

Acq: 14 Jan 2022 22:32

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 41 Resp: 63823

Ion Ratio Lower Upper

41 100

69 0.0 62.2 93.4#

39 51.5 45.4 68.0

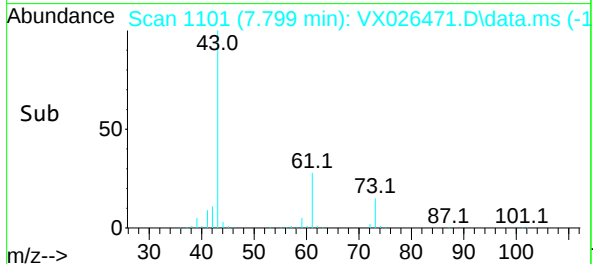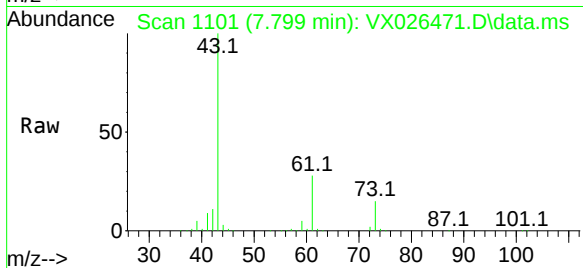

#49

1,4-Dioxane

Concen: 0.939 ug/l

RT: 7.806 min Scan# 1102

Delta R.T. 0.110 min

Lab File: VX026471.D

Acq: 14 Jan 2022 22:32




Tgt Ion: 88 Resp: 29


Ion Ratio Lower Upper

88 100

43 2346072.4 29.9 44.9#

58 9175.9 57.8 86.6#


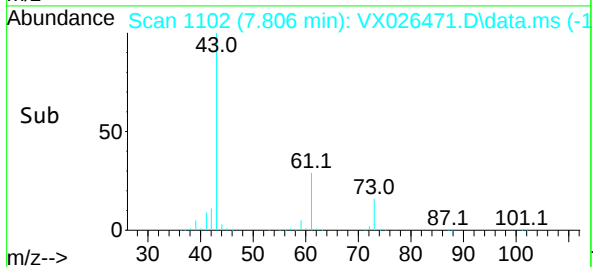

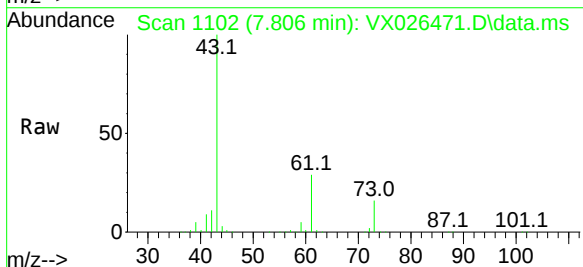




#50
Toluene-d8
Concen: 49.103 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 260565
Ion Ratio Lower Upper
98 100
100 66.4 53.2 79.8



#51
4-Methyl-2-Pentanone
Concen: 18.785 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.024 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32

Tgt Ion: 43 Resp: 42324
Ion Ratio Lower Upper
43 100
58 7.6 30.5 45.7#




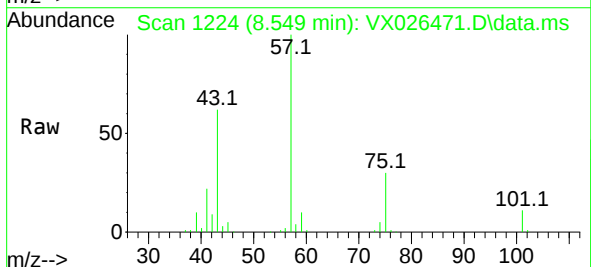


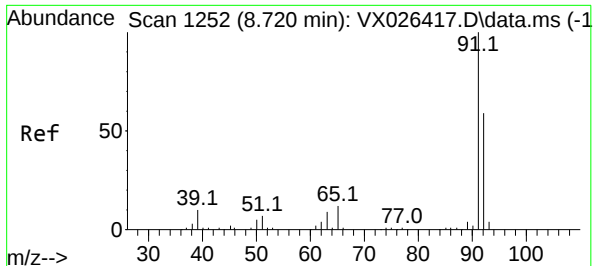

#52
Toluene
Concen: 0.954 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 92 Resp: 3758
Ion Ratio Lower Upper
92 100
91 171.4 135.7 203.5

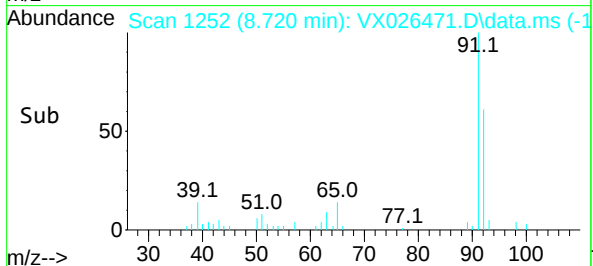

#54
cis-1,3-Dichloropropene
Concen: 7.677 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. 0.183 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32


Tgt Ion: 75 Resp: 18836
Ion Ratio Lower Upper
75 100
77 0.6 26.2 39.2#
39 33.3 43.5 65.3#

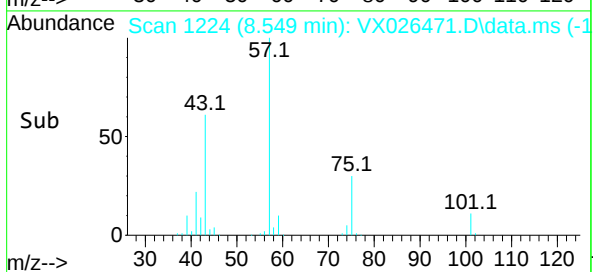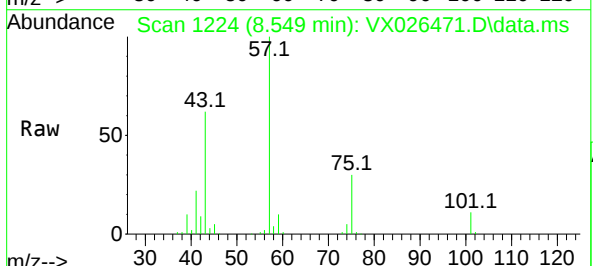






#55
 1,1,2-Trichloroethane
 Concen: 0.338 ug/l
 RT: 9.110 min Scan# 11
 Delta R.T. -0.043 min
 Lab File: VX026471.D
 Acq: 14 Jan 2022 22:32

Instrument :
 MSVOA_X
 ClientSampleId :



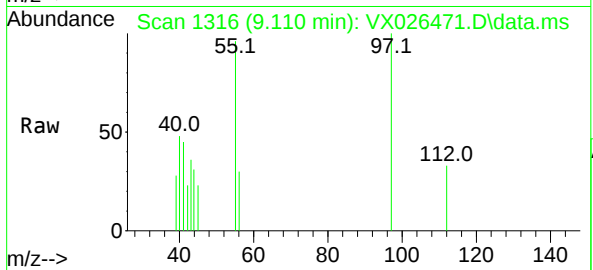



Tgt Ion: 97	Resp: 520
Ion Ratio	Lower Upper
97 100	
83 0.0	68.4 102.6#
85 0.0	44.0 66.0#
99 0.0	49.8 74.6#

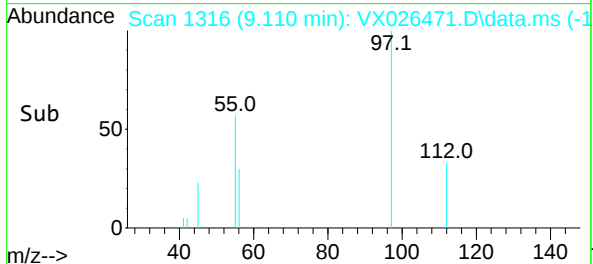

#57
 1,3-Dichloropropane
 Concen: 4.084 ug/l
 RT: 9.482 min Scan# 1377
 Delta R.T. 0.171 min
 Lab File: VX026471.D
 Acq: 14 Jan 2022 22:32

Tgt Ion: 76	Resp: 10887
Ion Ratio	Lower Upper
76 100	
78 0.0	25.7 38.5#


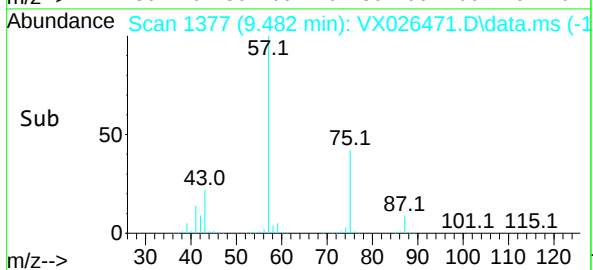

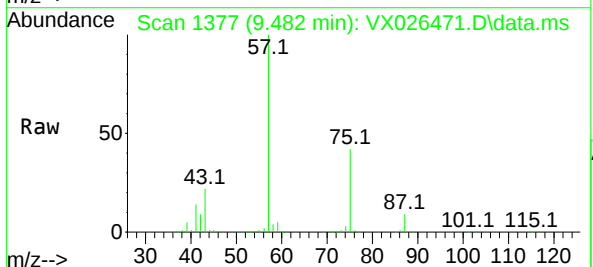




#59
2-Hexanone
Concen: 93.963 ug/l
RT: 9.482 min Scan# 11
Delta R.T. 0.049 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 162035
Ion Ratio Lower Upper
43 100
58 17.6 26.4 79.2#

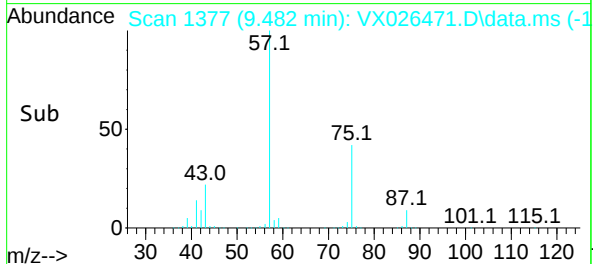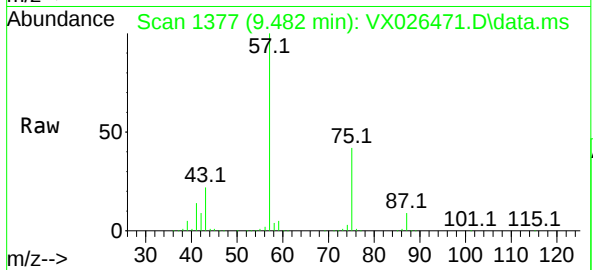

#62
4-Bromofluorobenzene
Concen: 50.514 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32

Tgt Ion: 95 Resp: 95223
Ion Ratio Lower Upper
95 100
174 73.0 0.0 148.6
176 70.7 0.0 141.4


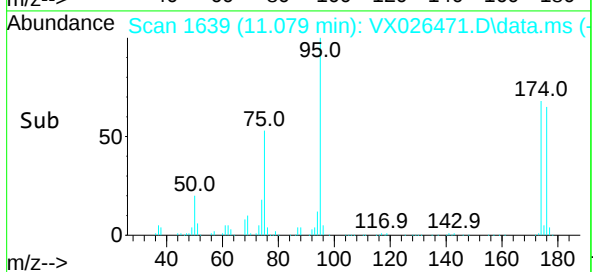

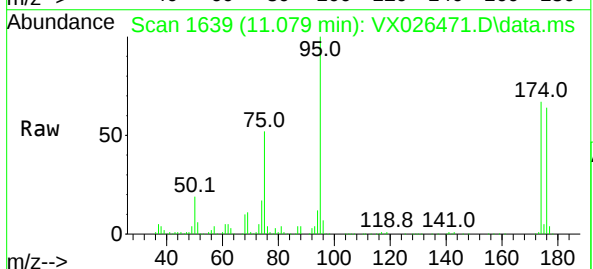




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 195750
Ion Ratio Lower Upper
117 100
82 58.3 45.2 67.8
119 32.1 26.2 39.2

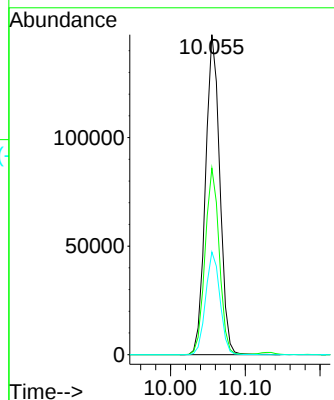

#67
Ethyl Benzene
Concen: 5.958 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32

Tgt Ion: 91 Resp: 44628
Ion Ratio Lower Upper
91 100
106 28.7 24.7 37.1


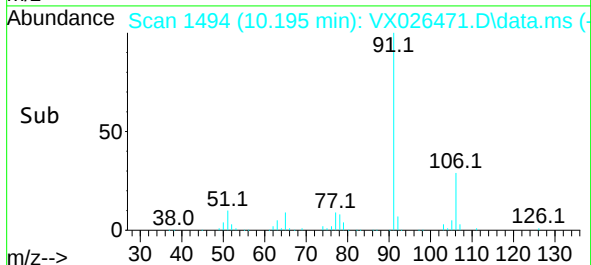
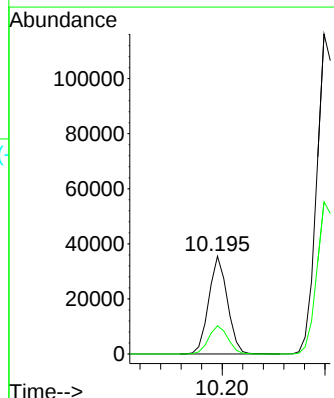
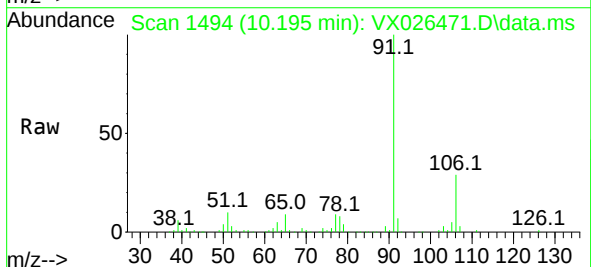




#68
m/p-Xylenes
Concen: 26.118 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.006 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 73217
Ion Ratio Lower Upper
106 100
91 209.5 165.3 247.9

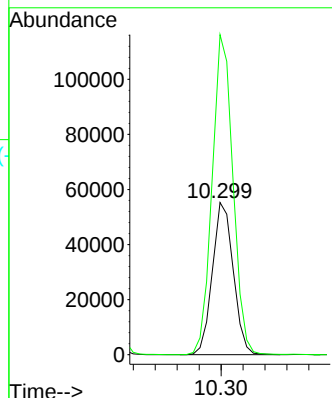

#69
o-Xylene
Concen: 21.492 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32

Tgt Ion:106 Resp: 58138
Ion Ratio Lower Upper
106 100
91 222.6 109.7 329.0



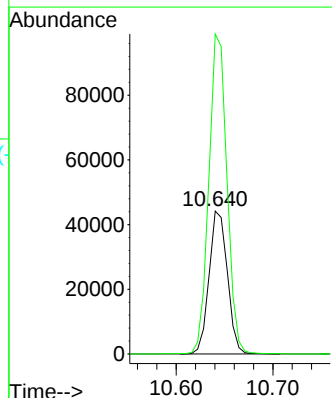
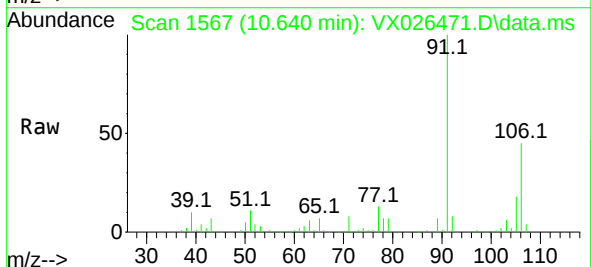




#70
Styrene
Concen: 0.655 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.018 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:104 Resp: 2890
Ion Ratio Lower Upper
104 100
78 321.0 42.5 63.7#
103 279.9 43.3 64.9#

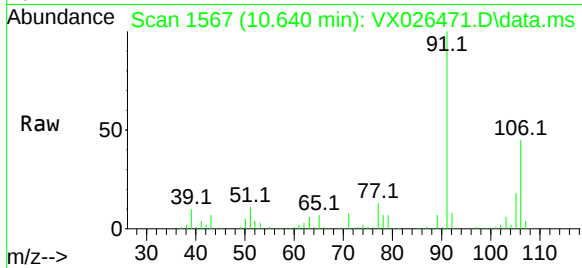

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32

Tgt Ion:152 Resp: 86603
Ion Ratio Lower Upper
152 100
115 69.0 44.2 132.6
150 156.9 0.0 348.2




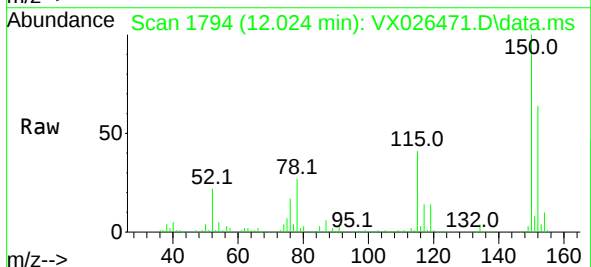




#73
Isopropylbenzene
Concen: 7.441 ug/l
RT: 10.964 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 52821
Ion Ratio Lower Upper
105 100
120 25.8 13.1 39.1



#74
N-ethyl acetate
Concen: 0.535 ug/l
RT: 10.860 min Scan# 1603
Delta R.T. 0.018 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32

Tgt Ion: 43 Resp: 1467
Ion Ratio Lower Upper
43 100
70 117.9 32.9 49.3#
55 621.5 18.3 27.5#
61 0.0 18.9 28.3#


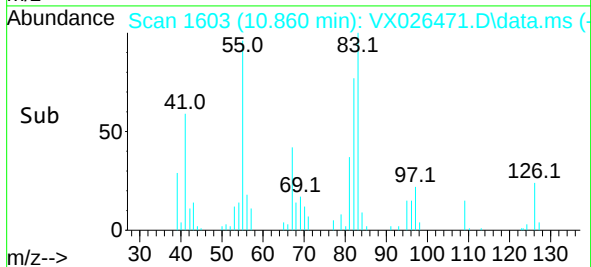

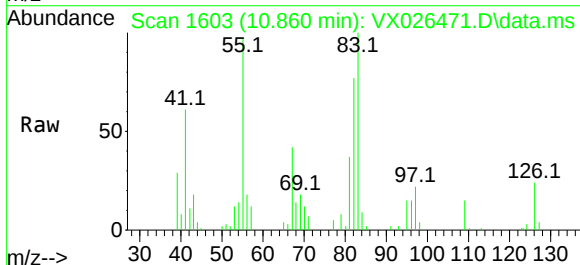




#75
 1,1,2,2-Tetrachloroethane
 Concen: 0.829 ug/l
 RT: 11.220 min Scan# 1687
 Delta R.T. 0.006 min
 Lab File: VX026471.D
 Acq: 14 Jan 2022 22:32




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 83 Resp: 1579
 Ion Ratio Lower Upper
 83 100
 131 0.0 5.3 15.9#
 85 2.7 32.0 96.2#



#76
 1,2,3-Trichloropropane
 Concen: 3.193 ug/l
 RT: 11.378 min Scan# 1688
 Delta R.T. 0.134 min
 Lab File: VX026471.D
 Acq: 14 Jan 2022 22:32

Tgt Ion: 75 Resp: 6089
 Ion Ratio Lower Upper
 75 100
 77 1378.5 18.3 54.8#

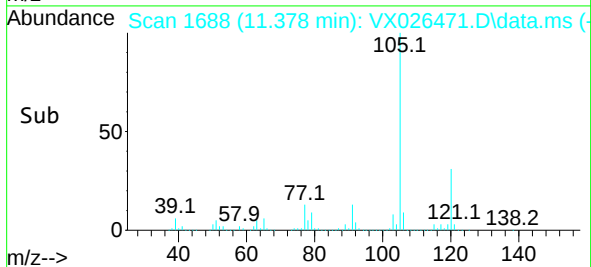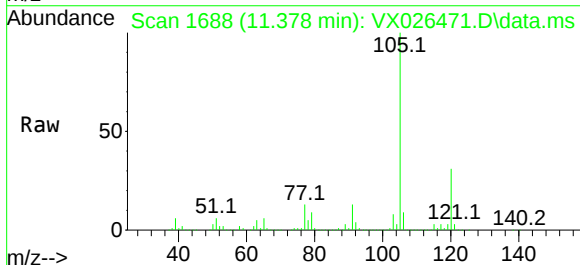



#78

n-propylbenzene

Concen: 16.126 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX026471.D

Acq: 14 Jan 2022 22:32

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 130540

Ion Ratio Lower Upper

91 100

120 22.4 11.6 34.7



#79

2-Chlorotoluene

Concen: 17.709 ug/l

RT: 11.378 min Scan# 1688

Delta R.T. 0.012 min

Lab File: VX026471.D




Acq: 14 Jan 2022 22:32


Tgt Ion: 91 Resp: 86931

Ion Ratio Lower Upper

91 100


126 0.0 16.4 49.2#

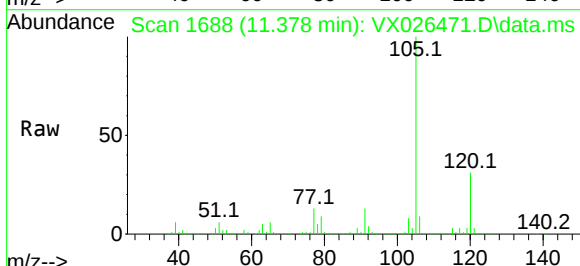






#80
1,3,5-Trimethylbenzene
Concen: 82.949 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:105 Resp: 485448
Ion Ratio Lower Upper
105 100
120 48.2 24.0 72.0



#81
trans-1,4-Dichloro-2-butene
Concen: 78.622 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32

Tgt Ion: 75 Resp: 49437
Ion Ratio Lower Upper
75 100
53 0.0 94.0 141.0#
89 0.0 37.0 55.4#




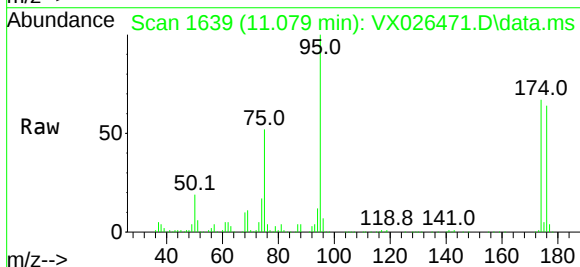




#82
4-Chlorotoluene
Concen: 9.509 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 53649
Ion Ratio Lower Upper
91 100
126 0.0 14.1 42.4#



#83
tert-Butylbenzene
Concen: 3.521 ug/l
RT: 11.713 min Scan# 1743
Delta R.T. 0.000 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32

Tgt Ion: 119 Resp: 19239
Ion Ratio Lower Upper
119 100
91 71.5 31.4 94.0
134 24.0 11.8 35.3


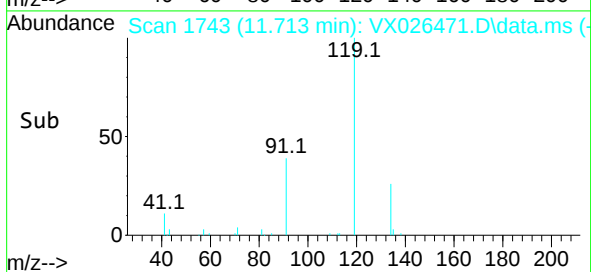

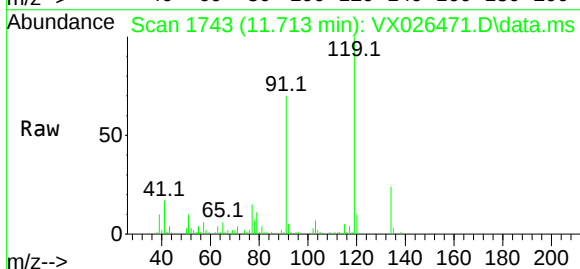




#84
 1,2,4-Trimethylbenzene
 Concen: 228.134 ug/l
 RT: 11.756 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: VX026471.D
 Acq: 14 Jan 2022 22:32




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion:105 Resp: 1335395
 Ion Ratio Lower Upper
 105 100
 120 45.6 21.9 65.5

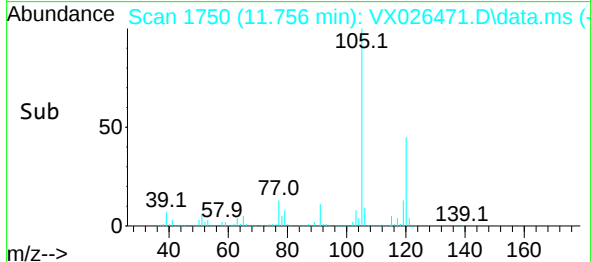

#85
 sec-Butylbenzene
 Concen: 9.234 ug/l
 RT: 11.890 min Scan# 1772
 Delta R.T. 0.000 min
 Lab File: VX026471.D
 Acq: 14 Jan 2022 22:32

Tgt Ion:105 Resp: 65255
 Ion Ratio Lower Upper
 105 100
 134 19.3 10.1 30.1


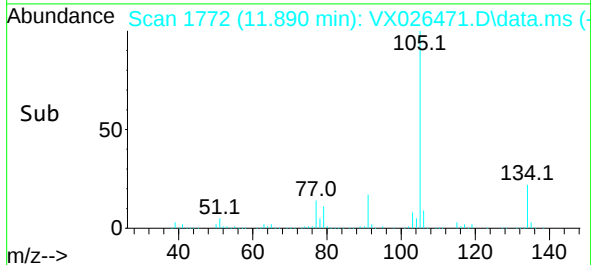

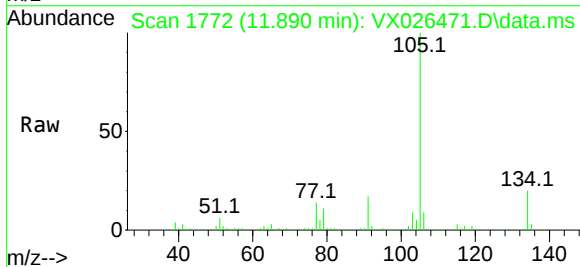


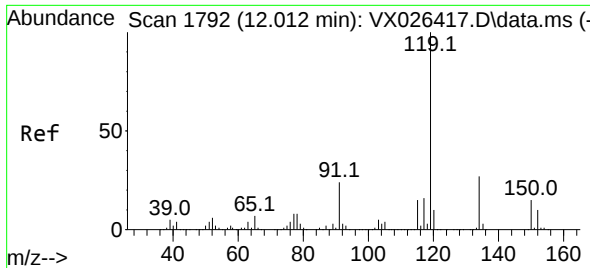

#86
 p-Isopropyltoluene
 Concen: 13.293 ug/l
 RT: 12.012 min Scan# 119
 Delta R.T. 0.000 min
 Lab File: VX026471.D
 Acq: 14 Jan 2022 22:32




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion:119 Resp: 78812
 Ion Ratio Lower Upper
 119 100
 134 26.1 13.0 39.0
 91 25.5 12.6 37.6

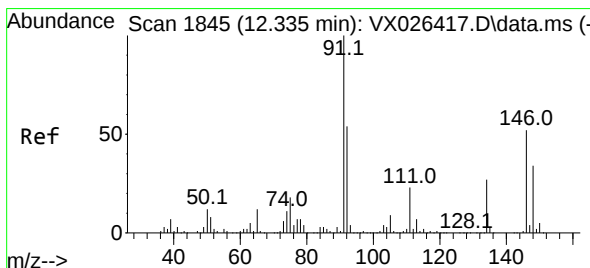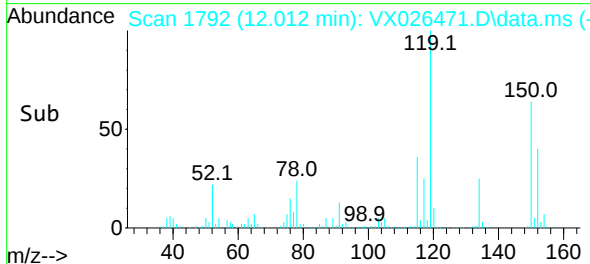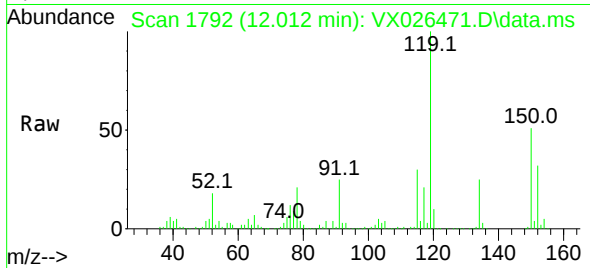

#89
 n-Butylbenzene
 Concen: 16.672 ug/l
 RT: 12.323 min Scan# 1843
 Delta R.T. -0.012 min
 Lab File: VX026471.D
 Acq: 14 Jan 2022 22:32

Tgt Ion: 91 Resp: 84826
 Ion Ratio Lower Upper
 91 100
 92 29.3 27.2 81.6
 134 115.2 13.1 39.1#


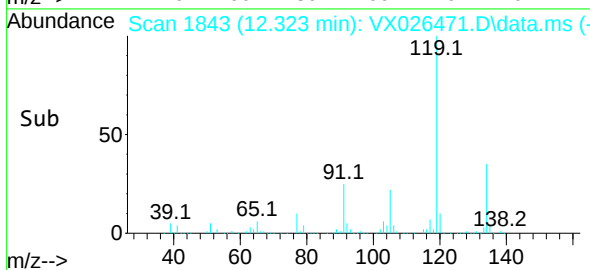

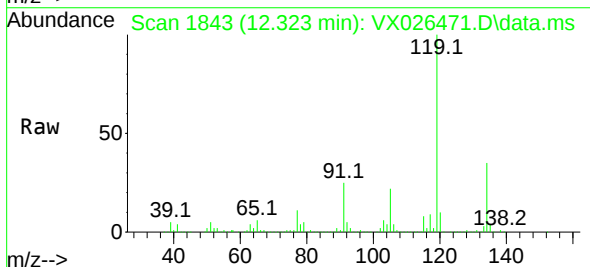




#90
Hexachloroethane
Concen: 17.299 ug/l
RT: 12.530 min Scan# 117
Delta R.T. -0.012 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 15642
Ion Ratio Lower Upper
117 100
201 0.0 35.6 106.8#



#92
1,2-Dibromo-3-Chloropropane
Concen: 2.532 ug/l
RT: 12.963 min Scan# 1948
Delta R.T. 0.018 min
Lab File: VX026471.D
Acq: 14 Jan 2022 22:32

Tgt Ion: 75 Resp: 1166
Ion Ratio Lower Upper
75 100
155 0.0 40.0 119.9#
157 0.0 51.6 154.8#

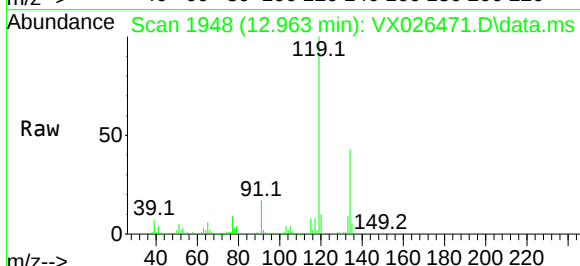



#95

Naphthalene

Concen: 36.905 ug/l

RT: 13.780 min Scan# 2082

Delta R.T. 0.006 min


Lab File: VX026471.D

Acq: 14 Jan 2022 22:32

Instrument :

MSVOA_X

ClientSampleId :



Tgt Ion:128 Resp: 227348

Ion Ratio Lower Upper

128 100

127 12.9 10.3 15.5

129 11.5 8.7 13.1

