


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX011522\  
 Data File : VX026456.D  
 Acq On : 14 Jan 2022 16:19  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X011122W.M  
 Title : SW846 8260  
 Last Update : Tue Jan 11 14:45:13 2022

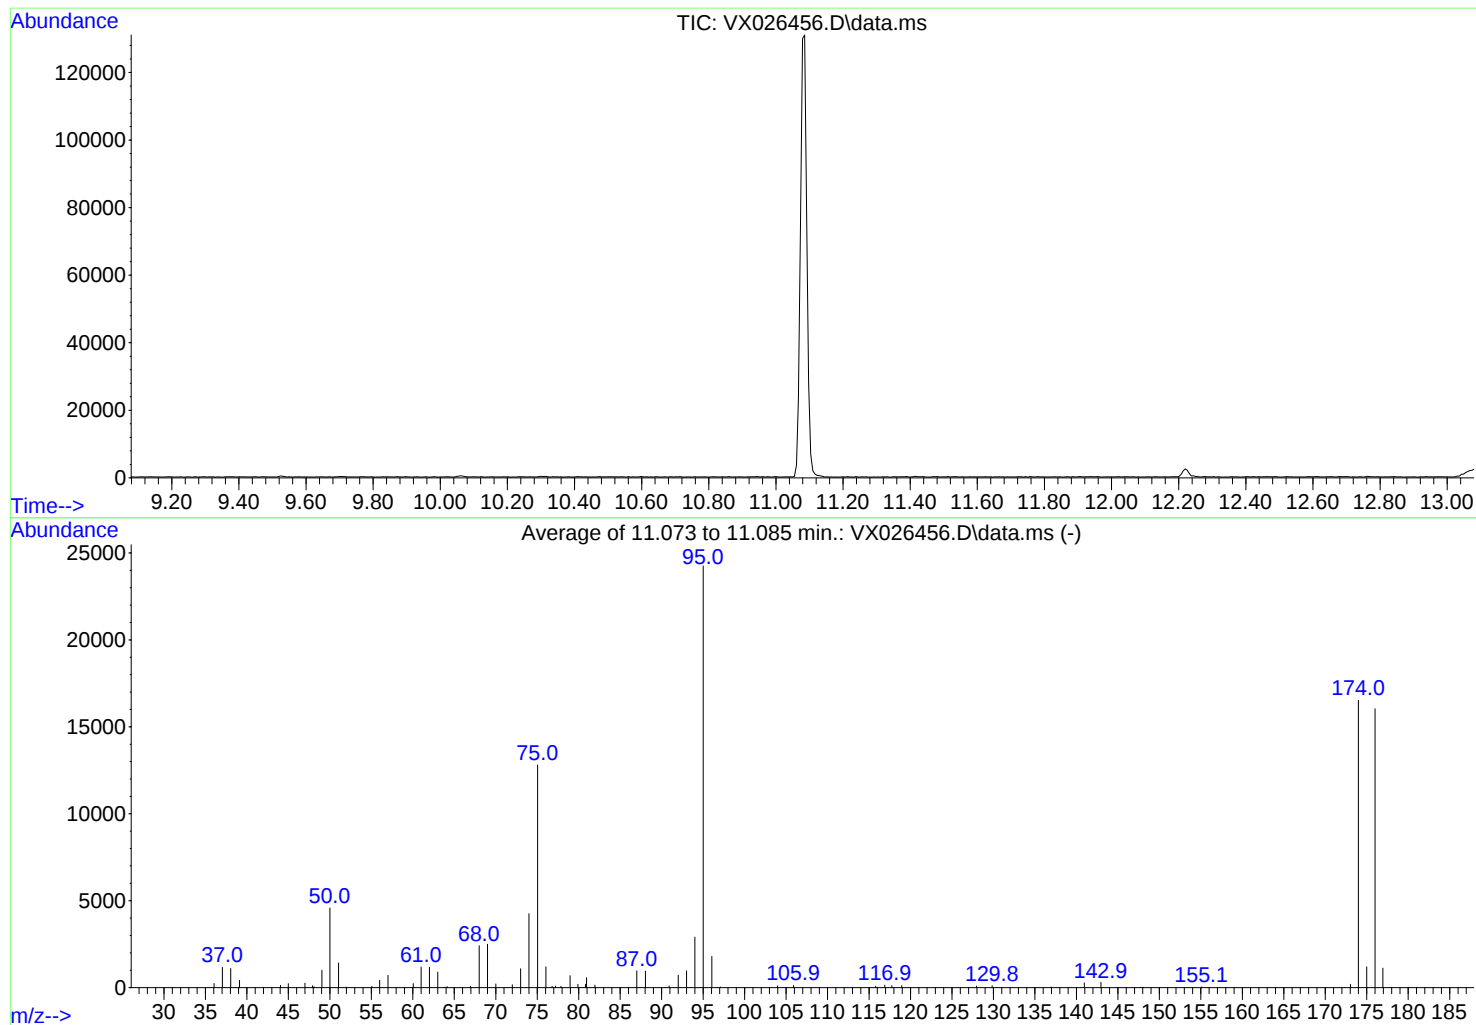

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 18.9         | 4585       | PASS                |
| 75             | 95              | 30              | 60              | 52.8         | 12800      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 24259      | PASS                |
| 96             | 95              | 5               | 9               | 7.4          | 1792       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.2          | 198        | PASS                |
| 174            | 95              | 50              | 100             | 68.1         | 16527      | PASS                |
| 175            | 174             | 5               | 9               | 7.2          | 1194       | PASS                |
| 176            | 174             | 95              | 101             | 97.1         | 16044      | PASS                |
| 177            | 176             | 5               | 9               | 7.0          | 1121       | PASS                |