

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011524\
 Data File : VX039750.D
 Acq On : 15 Jan 2024 12:51
 Operator : JC/MD
 Sample : VX0115WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0115WBL01

Quant Time: Jan 16 01:38:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 11 03:51:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	114114	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	212117	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	209156	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	98701	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	87134	45.582	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	91.160%
35) Dibromofluoromethane	5.385	113	68233	47.759	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.520%
50) Toluene-d8	8.647	98	262875	48.785	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.580%
62) 4-Bromofluorobenzene	11.079	95	107588	51.059	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	102.120%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011524\
Data File : VX039750.D
Acq On : 15 Jan 2024 12:51
Operator : JC/MD
Sample : VX0115WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0115WBL01

Quant Time: Jan 16 01:38:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 11 03:51:26 2024
Response via : Initial Calibration




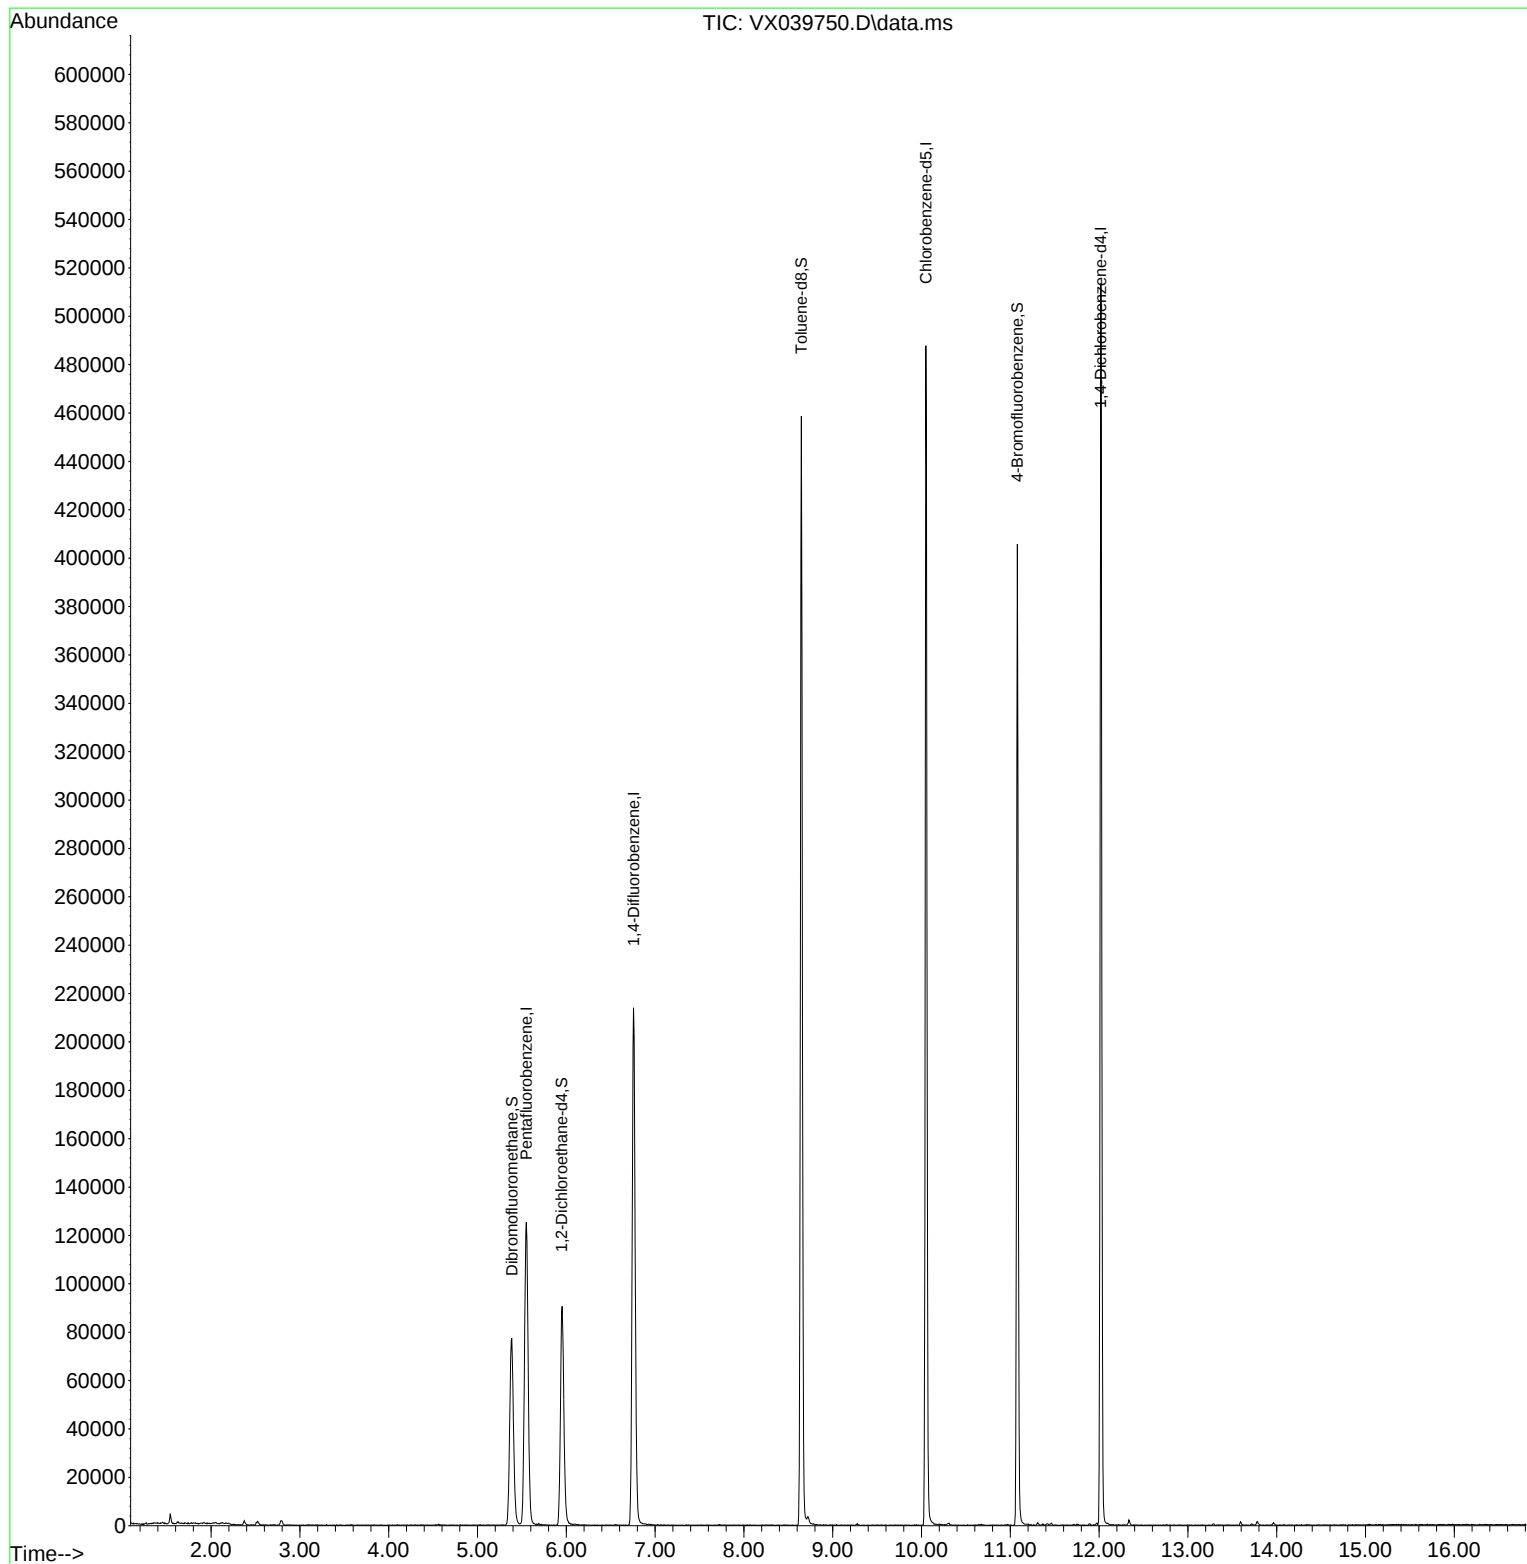


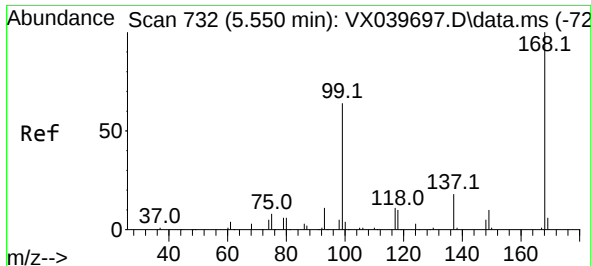

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 711
Delta R.T. -0.000 min
Lab File: VX039750.D
Acq: 15 Jan 2024 12:51




Instrument :
MSVOA_X
ClientSampleId :
VX0115WBL01


Tgt Ion:168 Resp: 114114
Ion Ratio Lower Upper
168 100
99 62.8 56.6 85.0

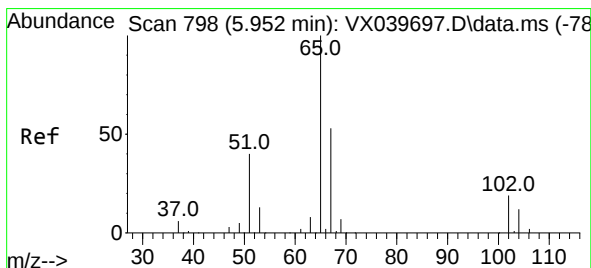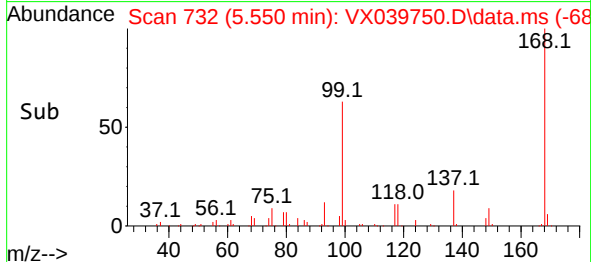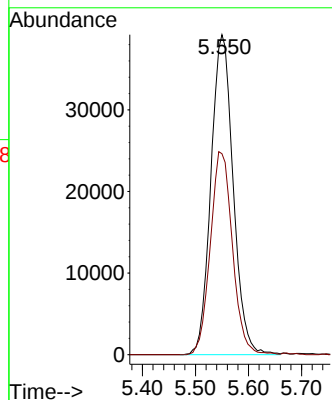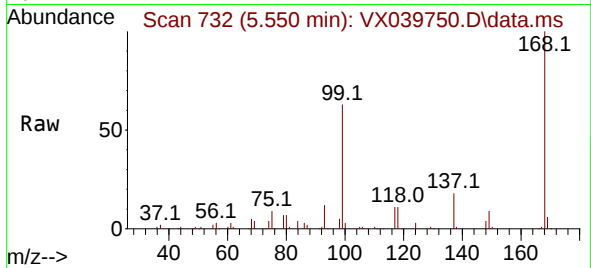

#33
1,2-Dichloroethane-d4
Concen: 45.582 ug/l
RT: 5.946 min Scan# 797
Delta R.T. -0.006 min
Lab File: VX039750.D
Acq: 15 Jan 2024 12:51

Tgt Ion: 65 Resp: 87134
Ion Ratio Lower Upper
65 100
67 52.3 0.0 100.2


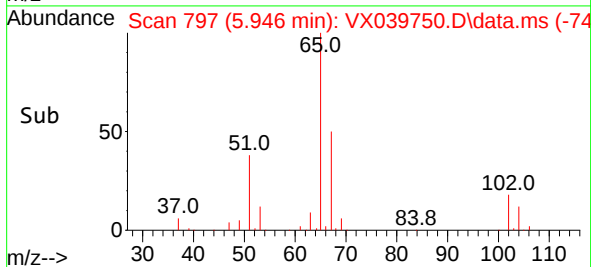
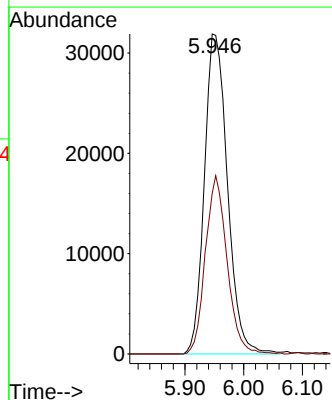
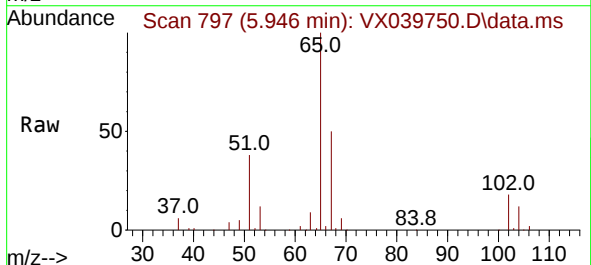


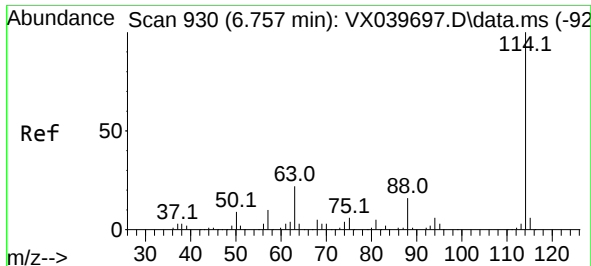

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX039750.D
Acq: 15 Jan 2024 12:51




Instrument :
MSVOA_X
ClientSampleId :
VX0115WBL01


Tgt Ion:114 Resp: 212117
Ion Ratio Lower Upper
114 100
63 23.5 0.0 45.0
88 17.3 0.0 36.6

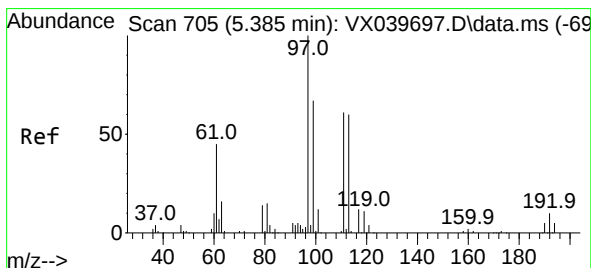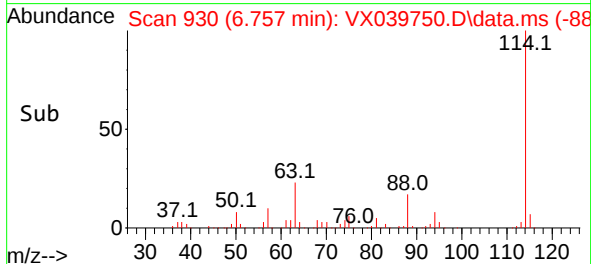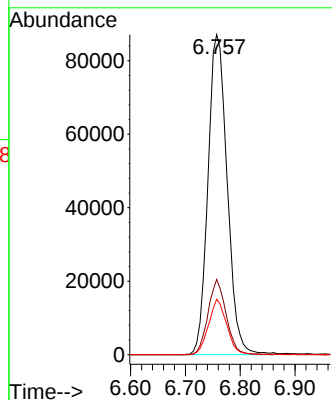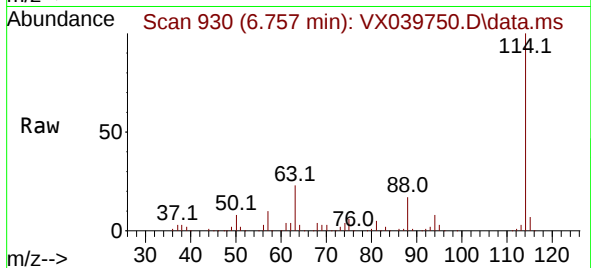

#35
Dibromofluoromethane
Concen: 47.759 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX039750.D
Acq: 15 Jan 2024 12:51

Tgt Ion:113 Resp: 68233
Ion Ratio Lower Upper
113 100
111 103.5 82.9 124.3
192 16.4 13.3 19.9


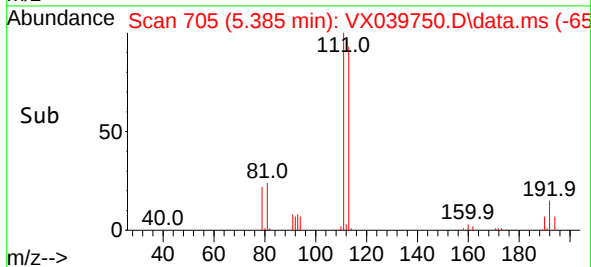
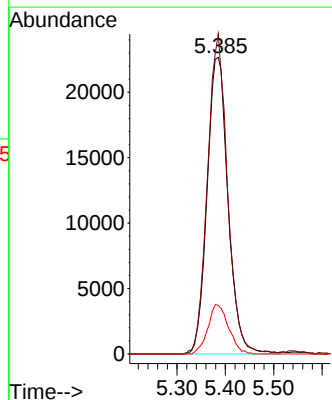
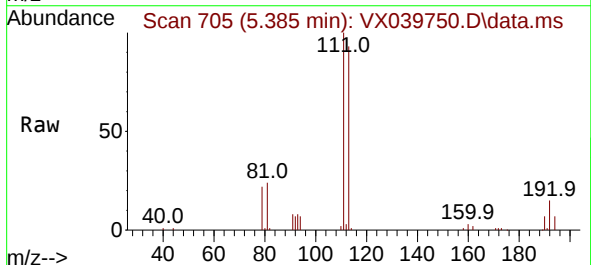


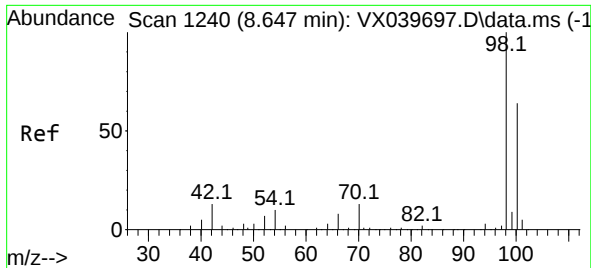

#50
Toluene-d8
Concen: 48.785 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX039750.D
Acq: 15 Jan 2024 12:51




Instrument :
MSVOA_X
ClientSampleId :
VX0115WBL01


Tgt Ion: 98 Resp: 262875
Ion Ratio Lower Upper
98 100
100 63.3 53.1 79.7

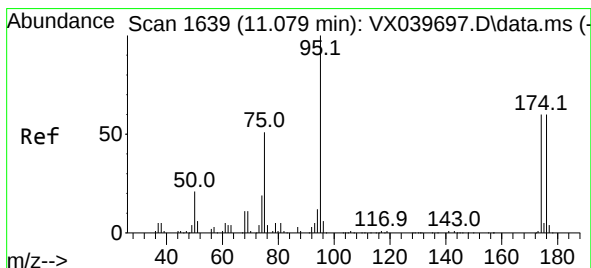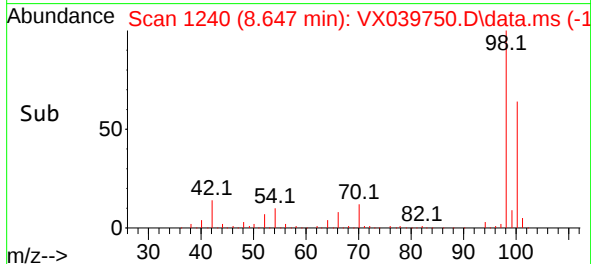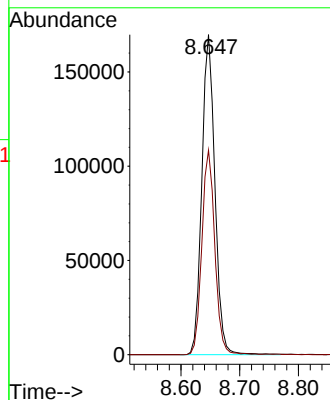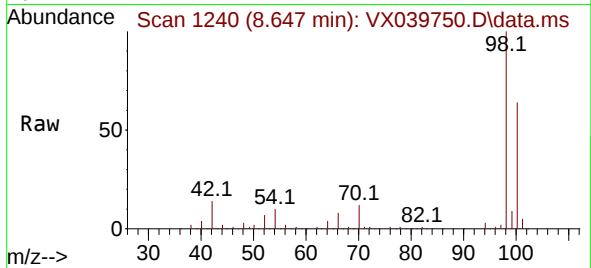

#62
4-Bromofluorobenzene
Concen: 51.059 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX039750.D
Acq: 15 Jan 2024 12:51

Tgt Ion: 95 Resp: 107588
Ion Ratio Lower Upper
95 100
174 68.5 0.0 135.6
176 66.1 0.0 131.0


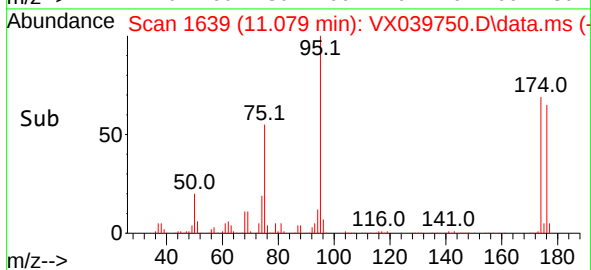
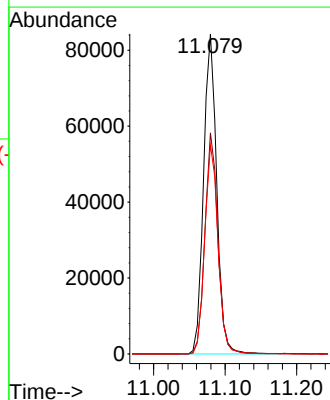
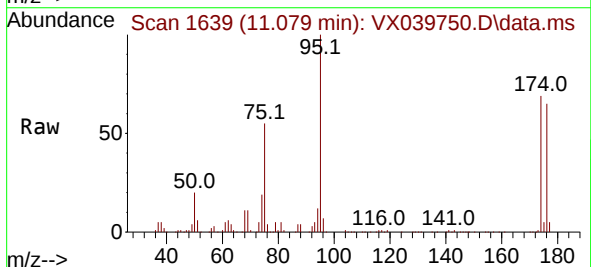


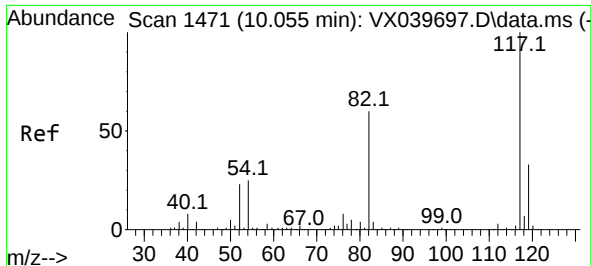

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX039750.D
Acq: 15 Jan 2024 12:51

Instrument :
MSVOA_X
ClientSampleId :
VX0115WBL01

Tgt Ion:117 Resp: 209156
Ion Ratio Lower Upper
117 100
82 60.9 46.2 69.4
119 32.2 25.5 38.3

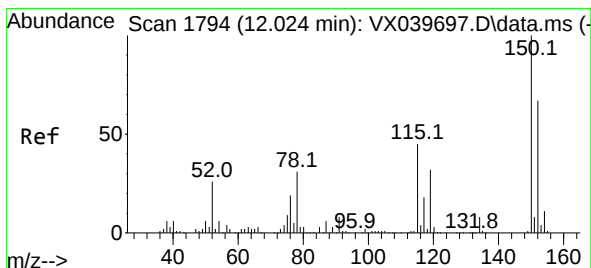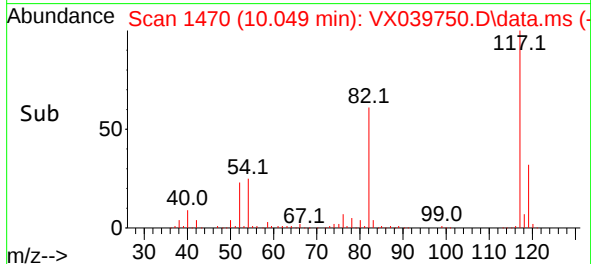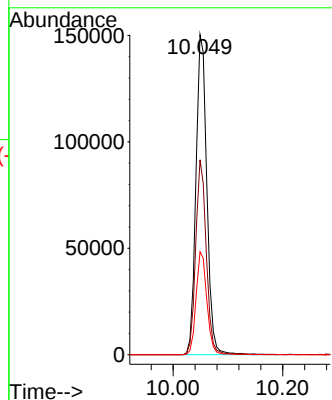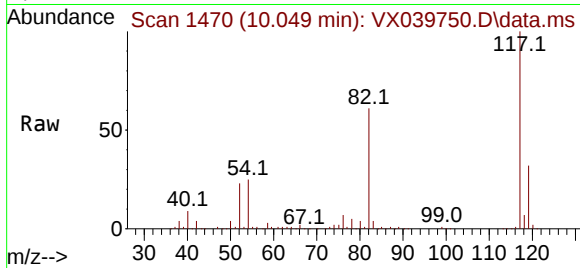

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.006 min
Lab File: VX039750.D
Acq: 15 Jan 2024 12:51

Tgt Ion:152 Resp: 98701
Ion Ratio Lower Upper
152 100
115 64.2 43.3 129.9
150 157.4 0.0 345.0

