



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011525\
Data File : VX044647.D
Acq On : 15 Jan 2025 09:30
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011525W.M
Title : SW846 8260
Last Update : Thu Jan 16 01:16:09 2025

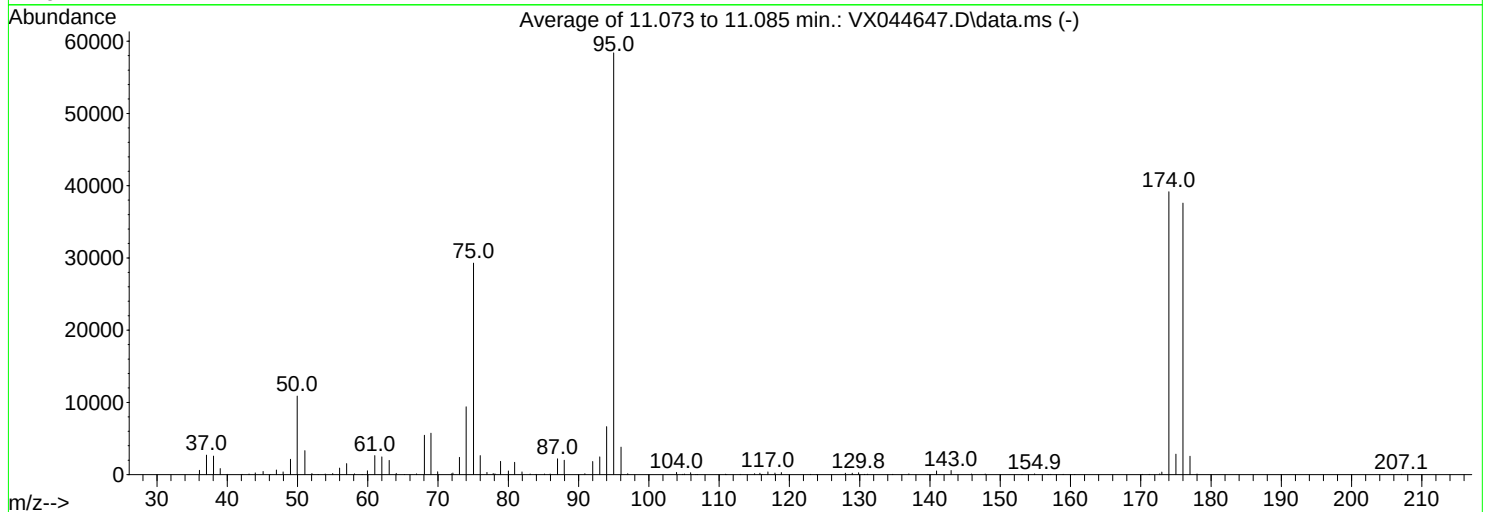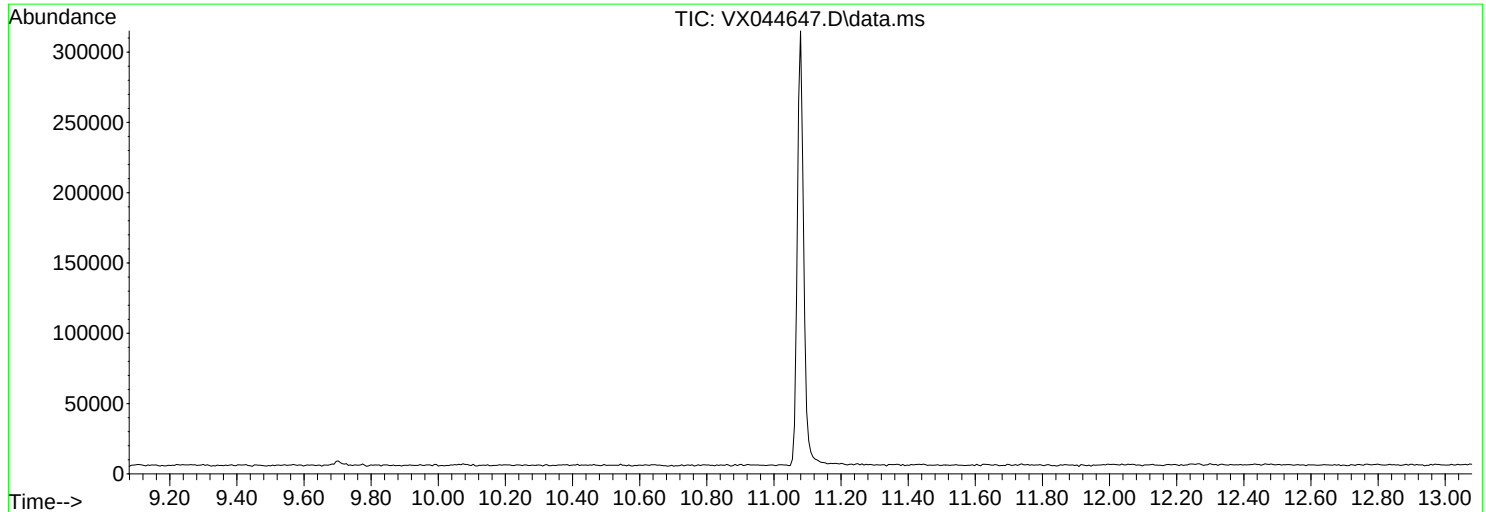

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	10879	PASS
75	95	30	60	50.2	29285	PASS
95	95	100	100	100.0	58391	PASS
96	95	5	9	6.5	3805	PASS
173	174	0.00	2	0.9	350	PASS
174	95	50	100	67.1	39163	PASS
175	174	5	9	7.3	2842	PASS
176	174	95	101	96.0	37587	PASS
177	176	5	9	6.8	2538	PASS