


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX011619\
Data File : VX007066.D
Acq On : 16 Jan 2019 09:09
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Title : SW846 8260
Last Update : Tue Jan 08 14:06:59 2019

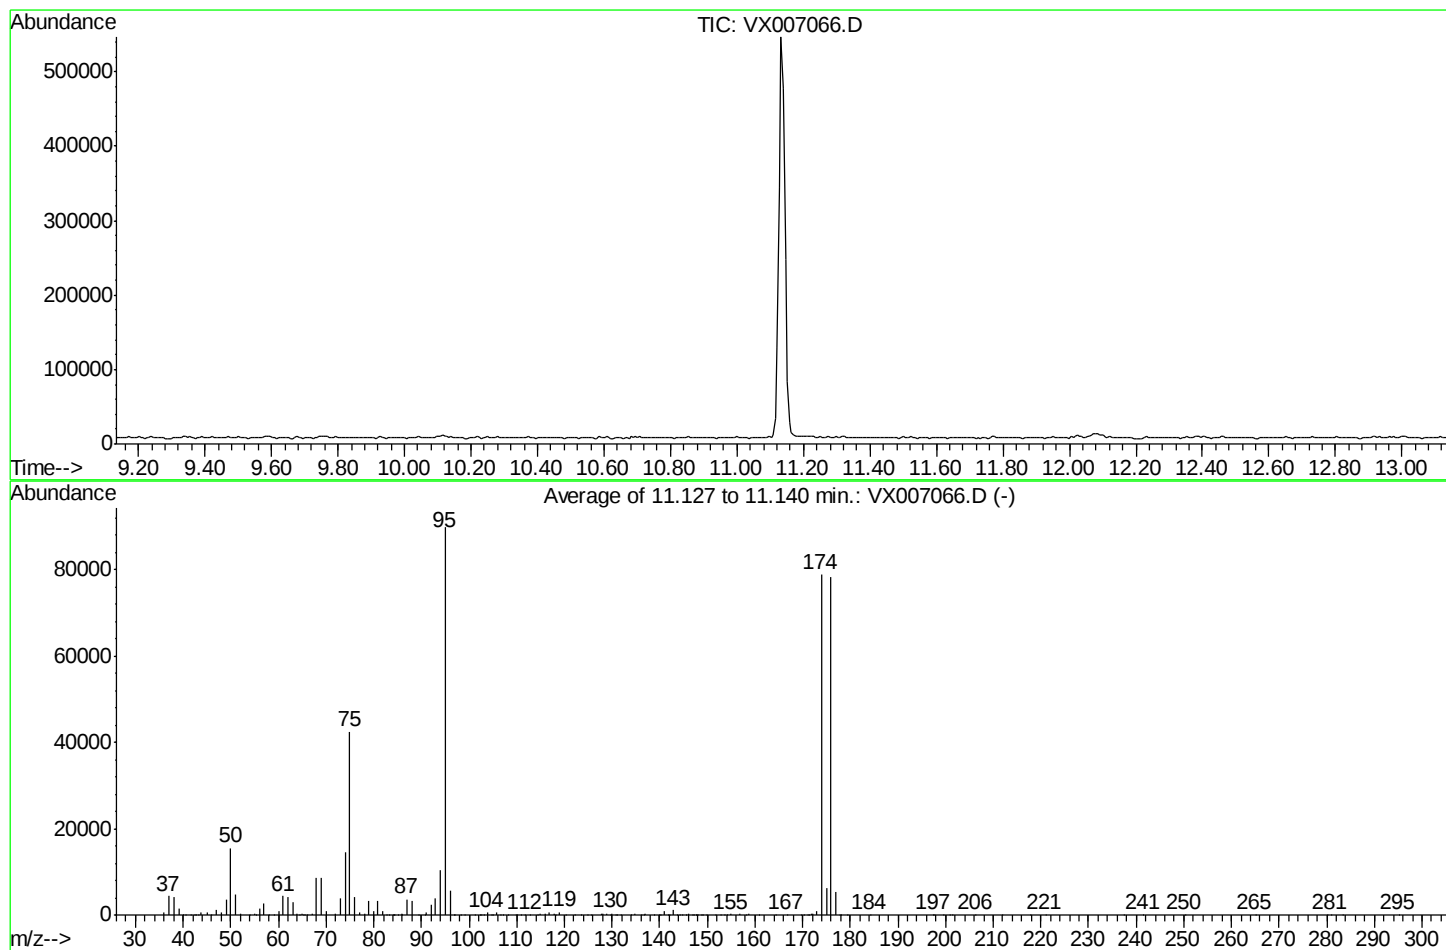

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	15463	PASS
75	95	30	60	47.4	42570	PASS
95	95	100	100	100.0	89864	PASS
96	95	5	9	6.3	5623	PASS
173	174	0.00	2	1.3	1046	PASS
174	95	50	100	87.8	78901	PASS
175	174	5	9	7.9	6265	PASS
176	174	95	101	99.3	78370	PASS
177	176	5	9	6.8	5355	PASS