

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX011620\
 Data File : VX014634.D
 Acq On : 16 Jan 2020 13:37
 Operator : JC/SP
 Sample : L1135-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TE-MW-A-1

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X011520W.M

Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.594	107	116	122	rVB	25517	52812	4.47%	1.065%
2	2.588	273	279	286	rVB	47369	86618	7.33%	1.747%
3	5.008	665	676	690	rVB3	153298	460986	39.01%	9.299%
4	6.051	838	847	858	rBV	169897	430586	36.44%	8.685%
5	6.849	969	978	989	rBV	366537	855701	72.41%	17.261%
6	7.203	1032	1036	1044	rVB9	16356	38437	3.25%	0.775%
7	8.709	1276	1283	1292	rBV	761911	1181731	100.00%	23.837%
8	9.331	1379	1385	1391	rVB2	74377	108141	9.15%	2.181%
9	10.105	1507	1512	1524	rVB	718151	988441	83.64%	19.938%
10	11.135	1675	1681	1689	rVB	548656	727092	61.53%	14.666%
11	12.080	1830	1836	1841	rVB10	5857	13471	1.14%	0.272%
12	12.208	1852	1857	1861	rBV2	8562	13513	1.14%	0.273%


Sum of corrected areas: 4957529

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX011620\
Data File : VX014634.D
Acq On : 16 Jan 2020 13:37
Operator : JC/SP
Sample : L1135-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TE-MW-A-1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X011520W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

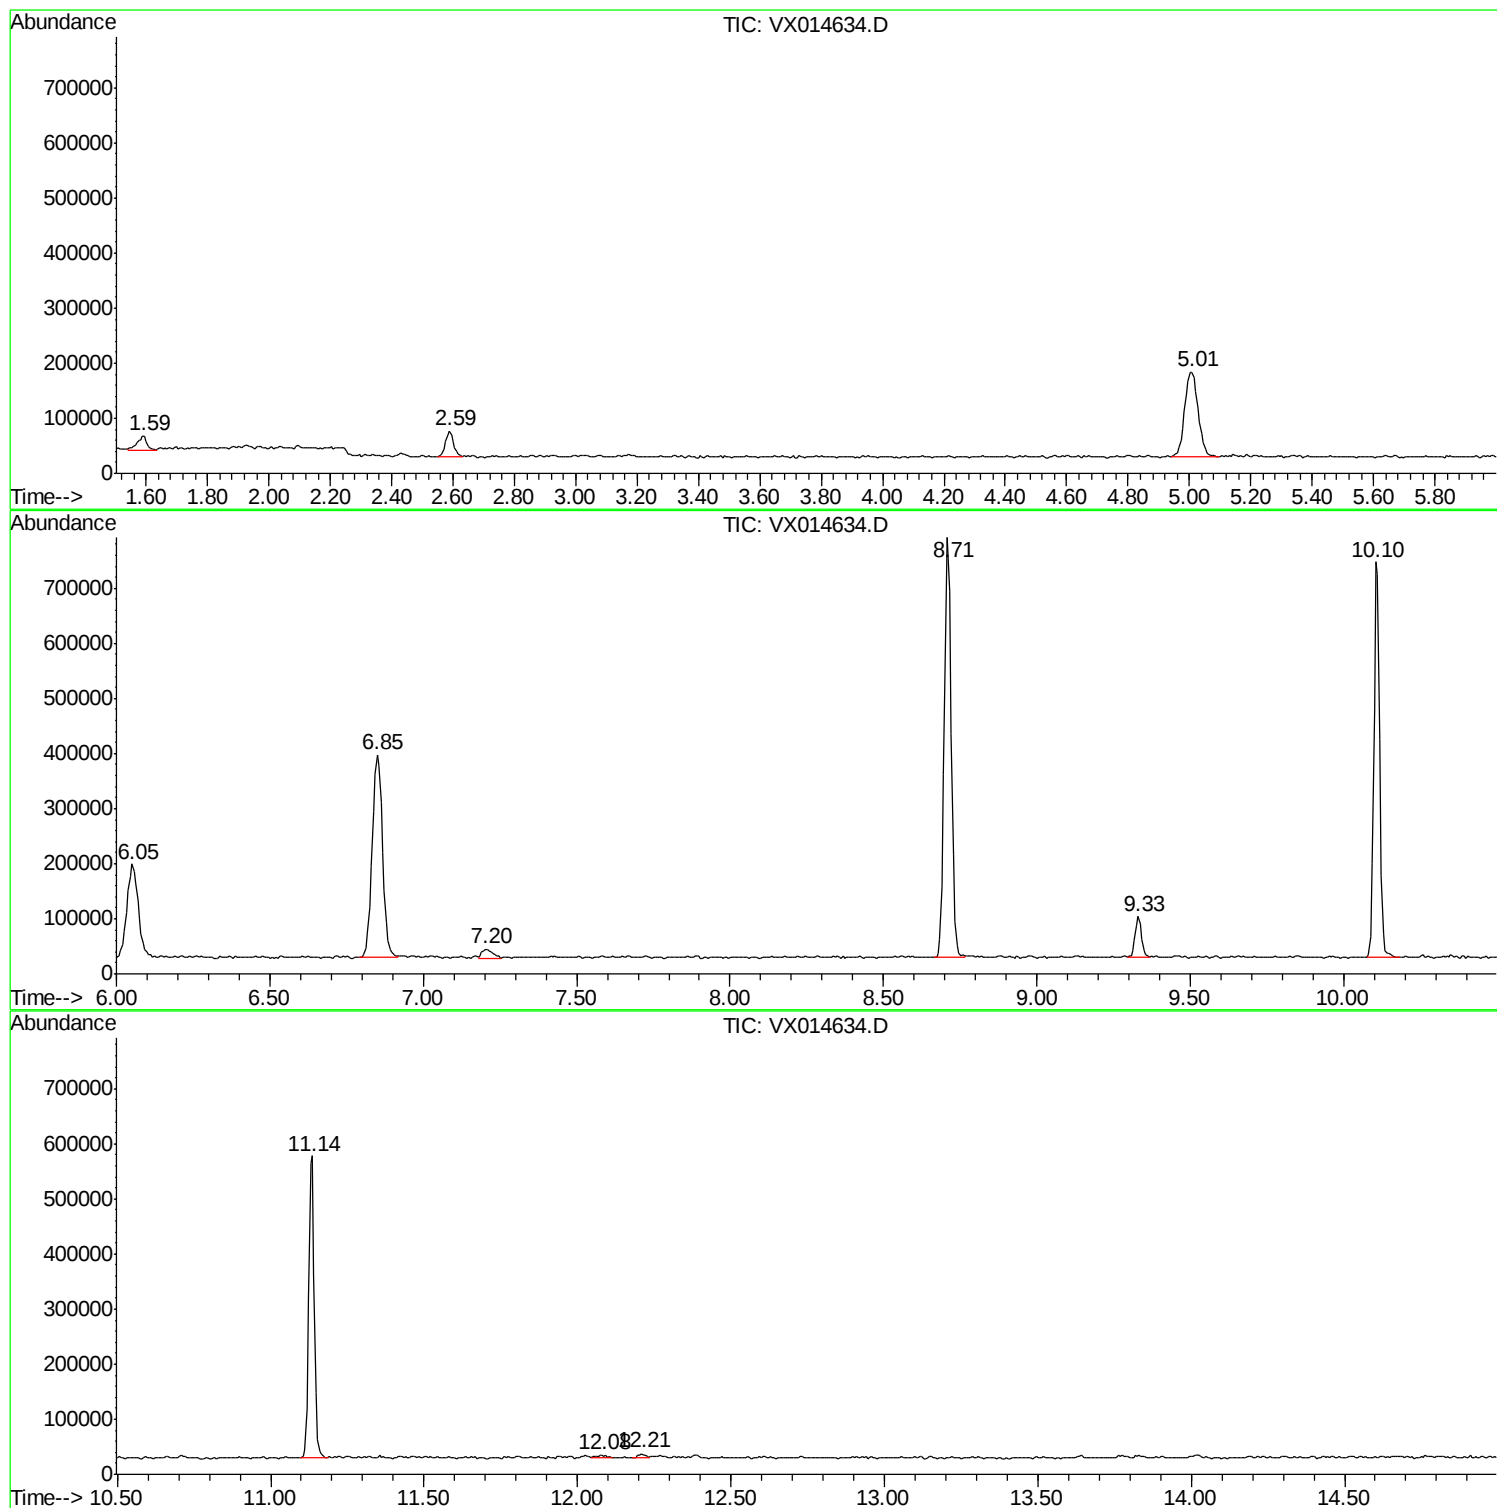

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX011620\
Data File : VX014634.D
Acq On : 16 Jan 2020 13:37
Operator : JC/SP
Sample : L1135-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TE-MW-A-1










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X011520W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.59 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.59	3.44 ug/l	52812	Bromochloromethane	5.01

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3,4-Dichlorobutane nitrile	137	C4H5Cl2N	034362-21-5	25
2		Nitrofurazone	198	C6H6N4O4	000059-87-0	12
3		Methylene Chloride	84	CH2Cl2	000075-09-2	10
4		Chloromethylphosphonic dichloride	166	CH2Cl3OP	001983-26-2	10
5		Mitozolomide	242	C7H7ClN6O2	085622-95-3	9

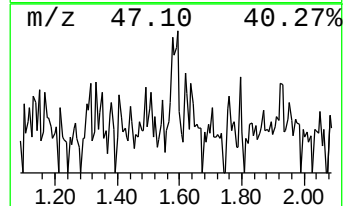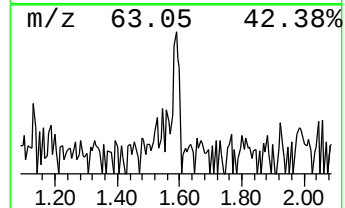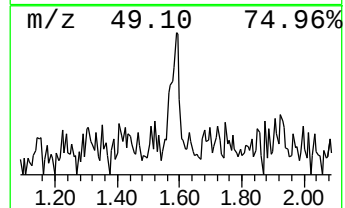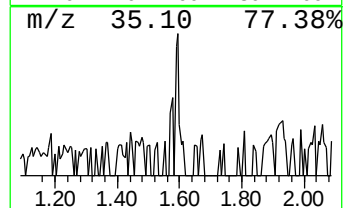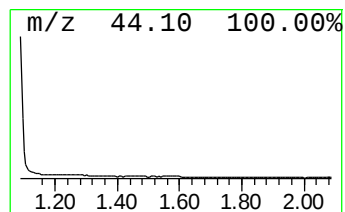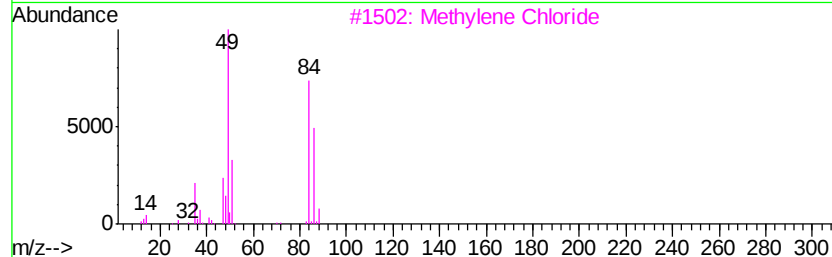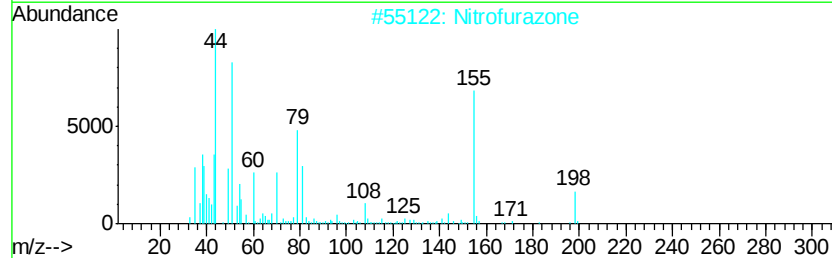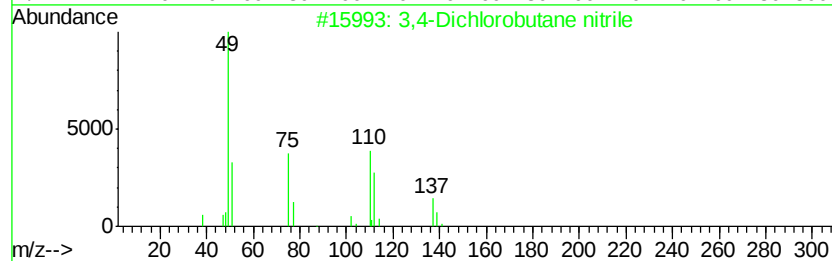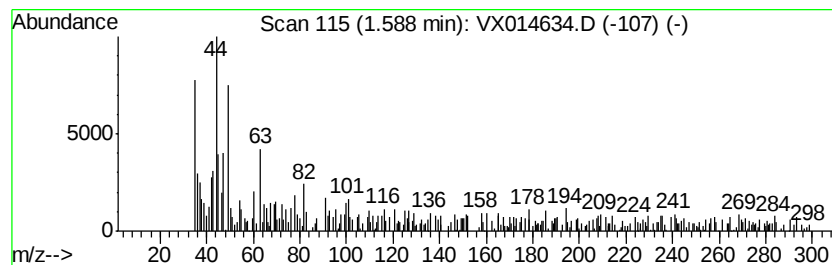

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX011620\
Data File : VX014634.D
Acq On : 16 Jan 2020 13:37
Operator : JC/SP
Sample : L1135-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TE-MW-A-1










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X011520W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	5.64 ug/l	86618	Bromochloromethane	5.01

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	72
2		Isopropyl Alcohol	60	C3H8O	000067-63-0	64
3		Isopropyl Alcohol	60	C3H8O	000067-63-0	64
4		Pentane, 1-methoxy-	102	C6H14O	000628-80-8	56
5		Methoxyacetyl chloride	108	C3H5ClO2	038870-89-2	50

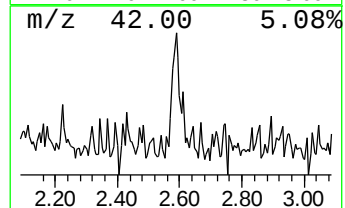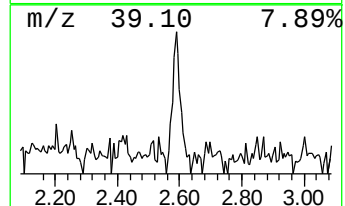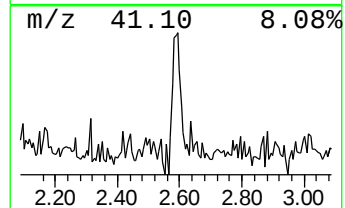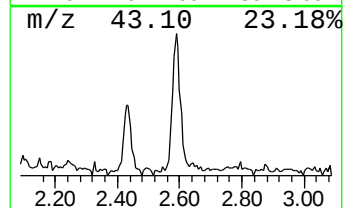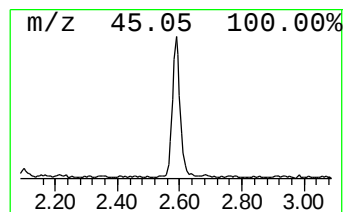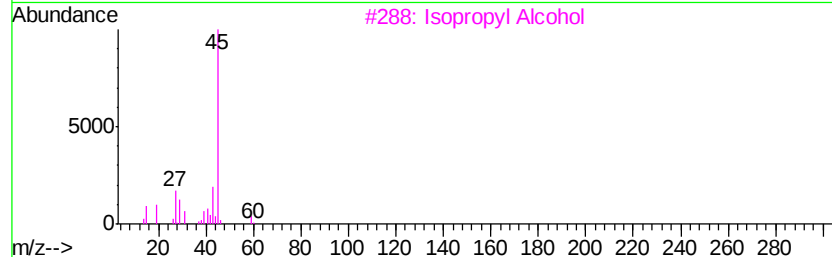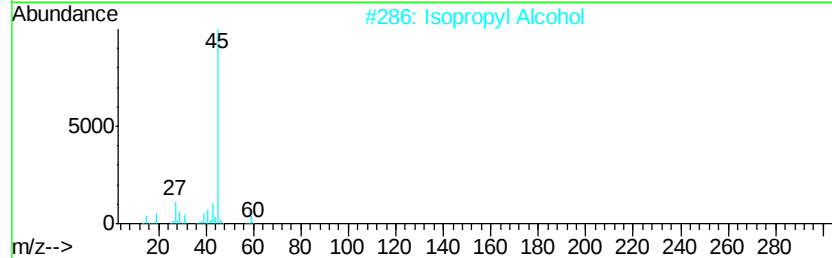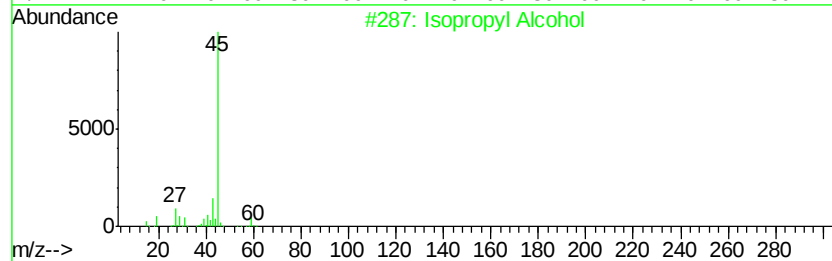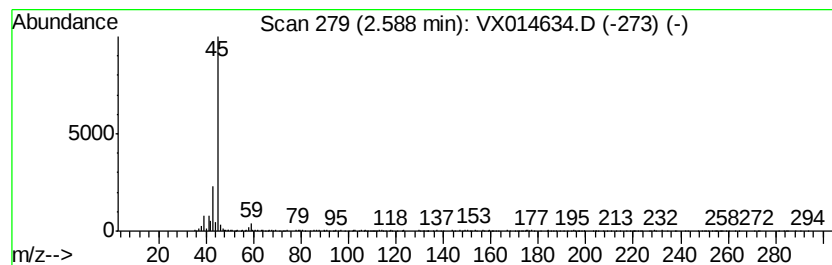

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX011620\
Data File : VX014634.D
Acq On : 16 Jan 2020 13:37
Operator : JC/SP
Sample : L1135-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TE-MW-A-1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X011520W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.59	1.59	3.4	ug/l	52812	1	5.01	460986	30.0
Isopropyl Alcohol	2.59	5.6	ug/l	86618	1	5.01	460986	30.0