

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011624\
 Data File : VX039780.D
 Acq On : 16 Jan 2024 17:25
 Operator : JC/MD
 Sample : P1149-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-191-GW-148-150

Quant Time: Jan 17 01:52:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 11 03:51:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	91400	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	175503	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	170741	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	83399	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	72157	47.128	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	94.260%
35) Dibromofluoromethane	5.385	113	55932	47.316	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.640%
50) Toluene-d8	8.647	98	214480	48.108	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	96.220%
62) 4-Bromofluorobenzene	11.079	95	87985	50.467	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	100.940%
Target Compounds						
16) Acetone	2.379	43	2721	3.160	ug/l	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011624\
Data File : VX039780.D
Acq On : 16 Jan 2024 17:25
Operator : JC/MD
Sample : P1149-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-191-GW-148-150


Quant Time: Jan 17 01:52:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 11 03:51:26 2024
Response via : Initial Calibration

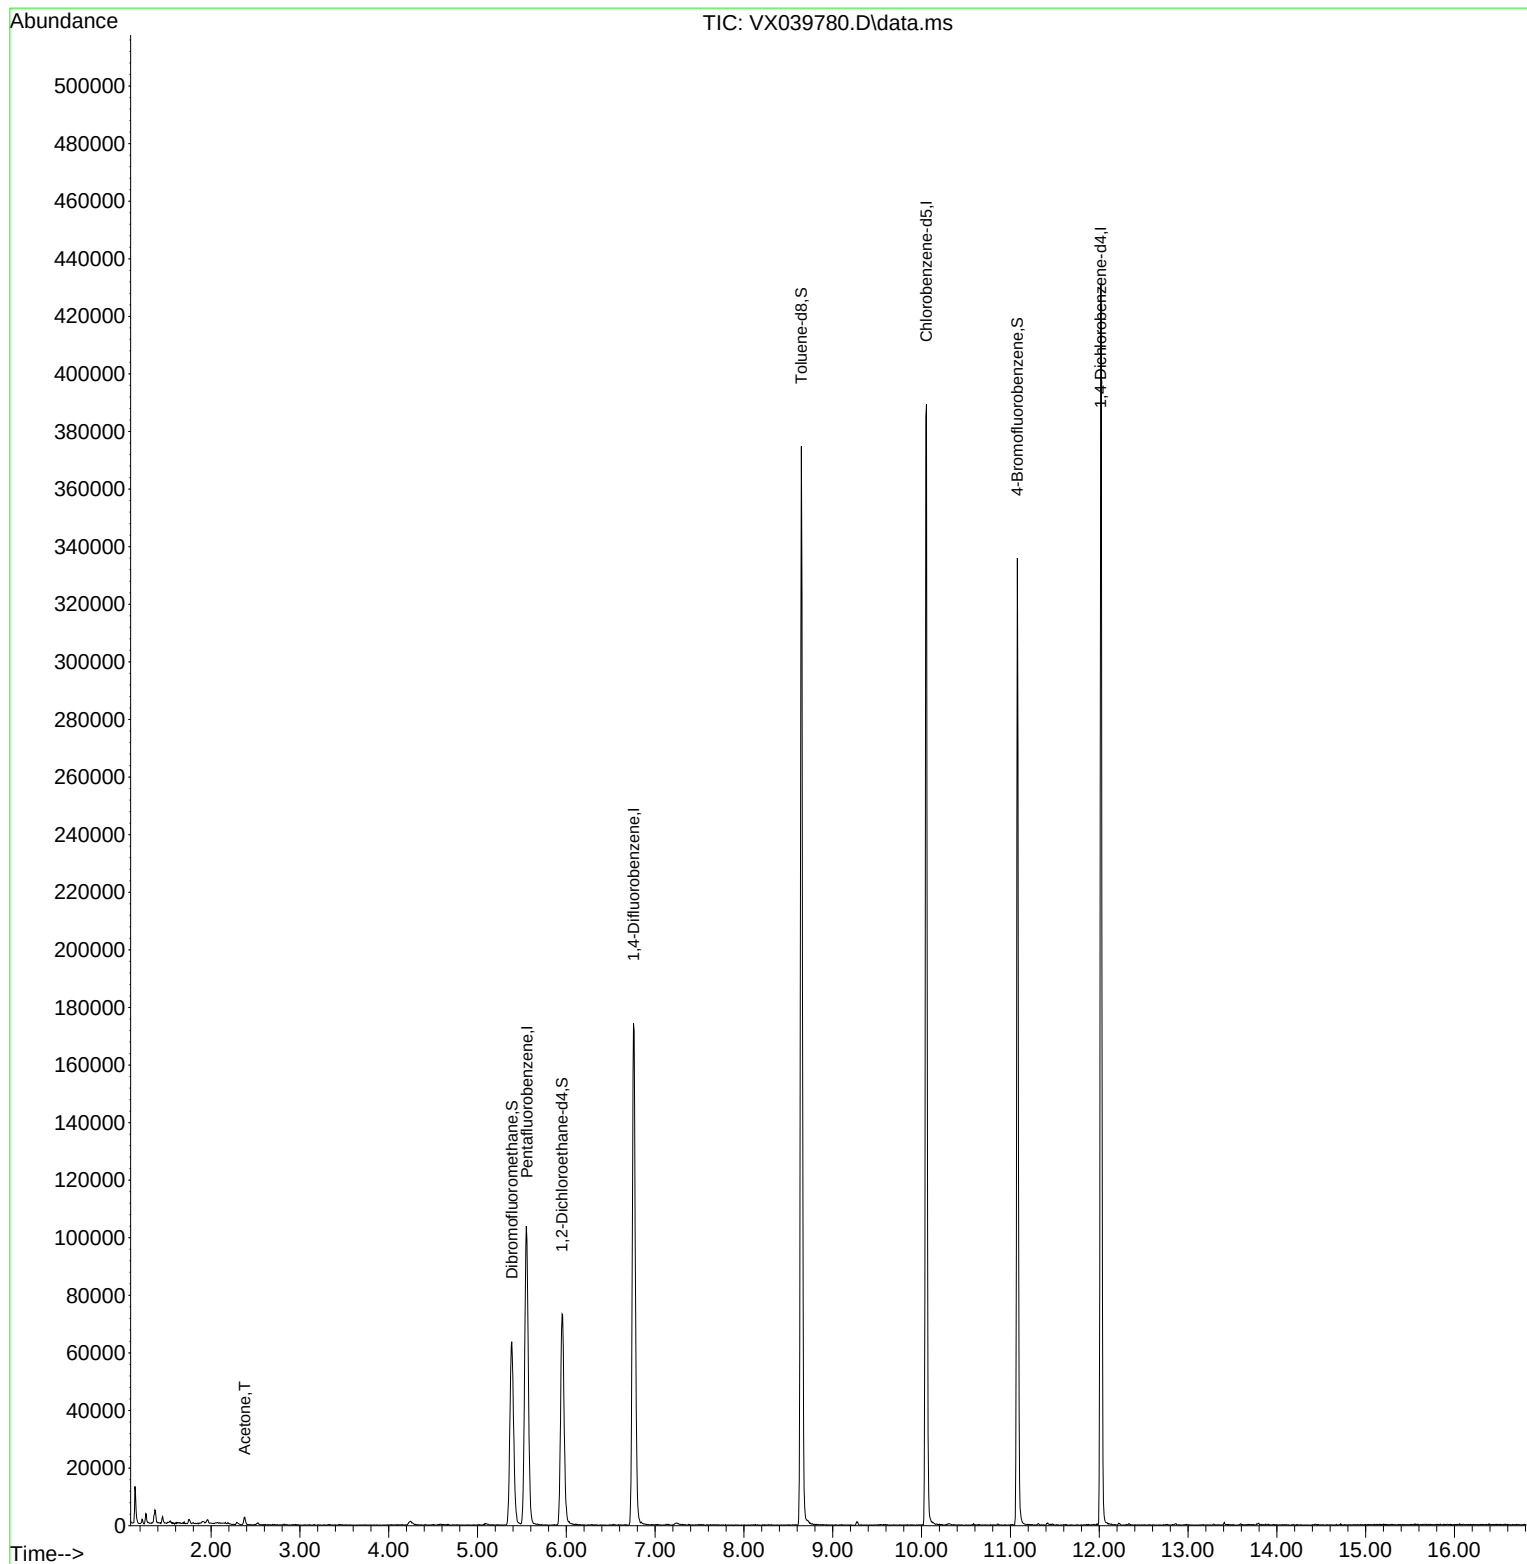



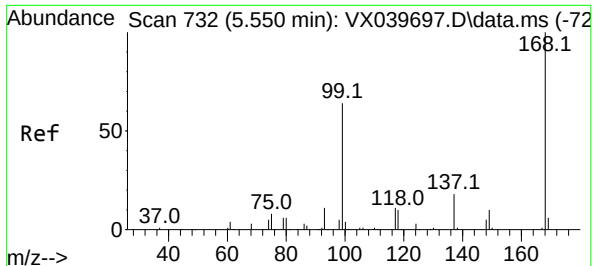


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX039780.D
Acq: 16 Jan 2024 17:25

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-191-GW-148-150



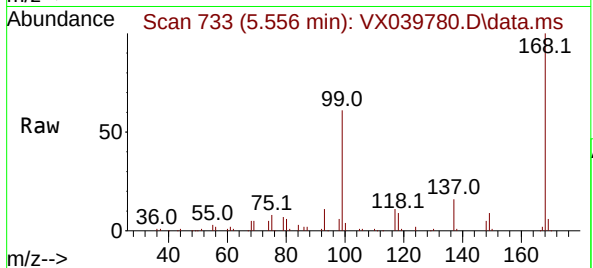



Tgt Ion:168 Resp: 91400
Ion Ratio Lower Upper
168 100
99 60.7 56.6 85.0

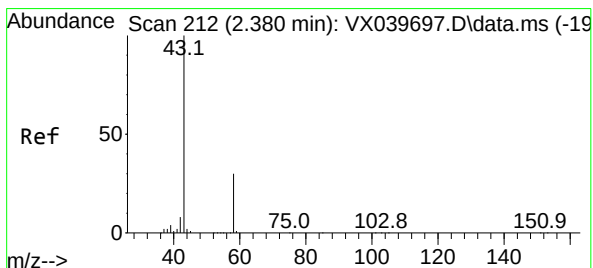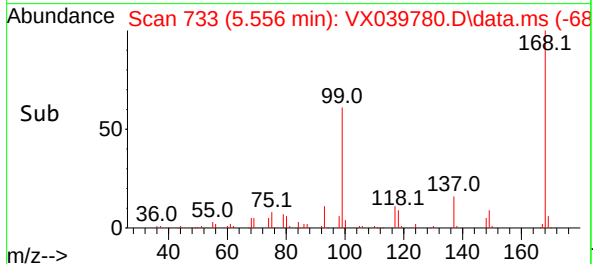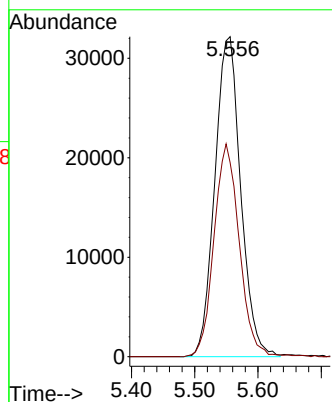

#16
Acetone
Concen: 3.160 ug/l
RT: 2.379 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX039780.D
Acq: 16 Jan 2024 17:25

Tgt Ion: 43 Resp: 2721
Ion Ratio Lower Upper
43 100
58 24.8 21.9 32.9

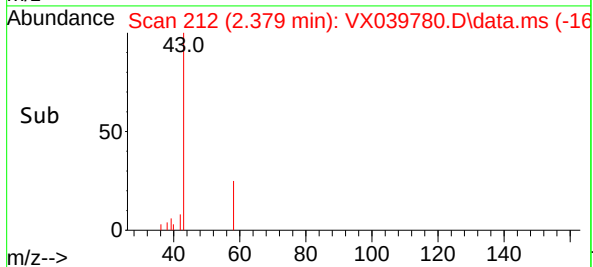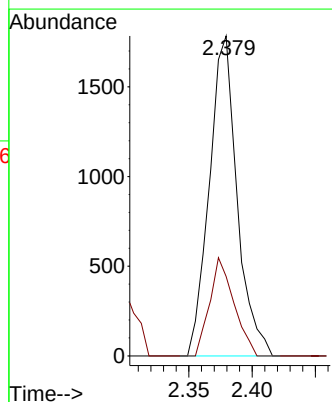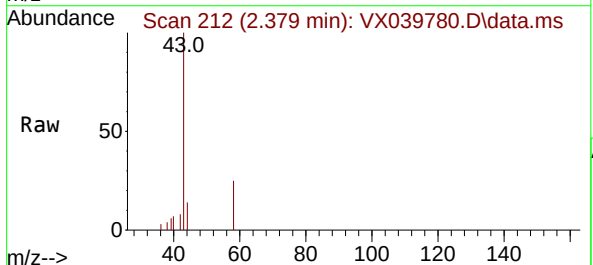

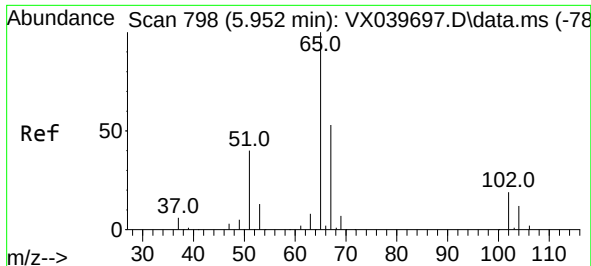

#33

1,2-Dichloroethane-d4

Concen: 47.128 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.000 min

Lab File: VX039780.D

Acq: 16 Jan 2024 17:25

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB-191-GW-148-150

Tgt Ion: 65 Resp: 72157

Ion Ratio Lower Upper

65 100

67 52.1 0.0 100.2

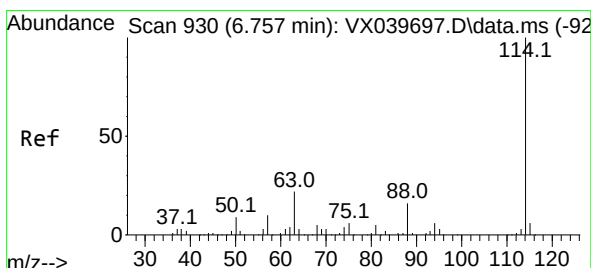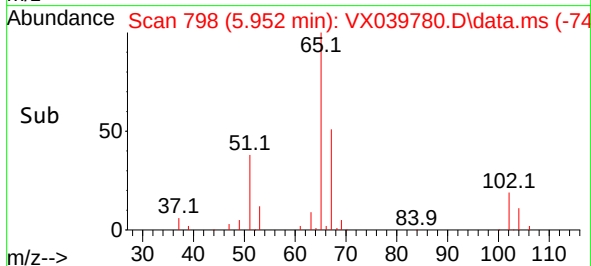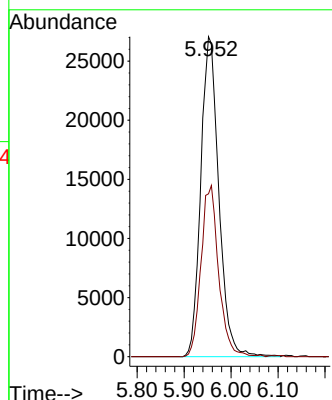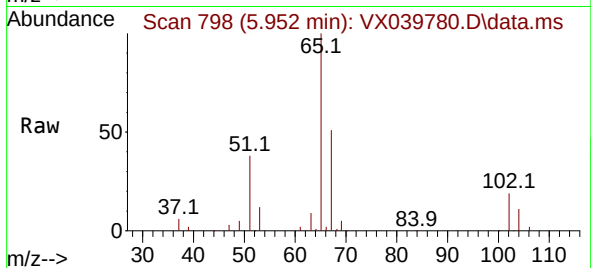

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.000 min

Lab File: VX039780.D

Acq: 16 Jan 2024 17:25




Tgt Ion: 114 Resp: 175503


Ion Ratio Lower Upper

114 100

63 21.3 0.0 45.0

88 16.1 0.0 36.6


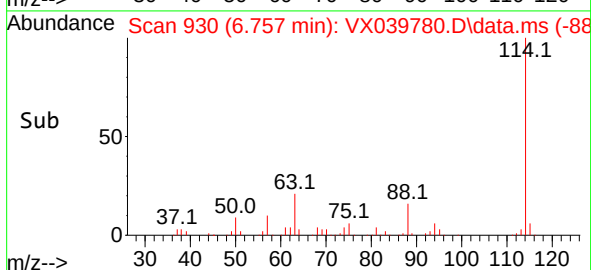
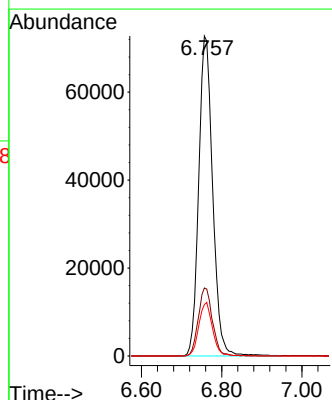
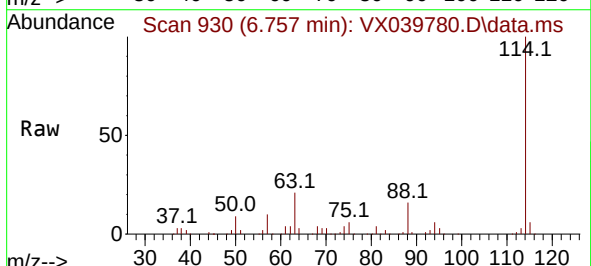


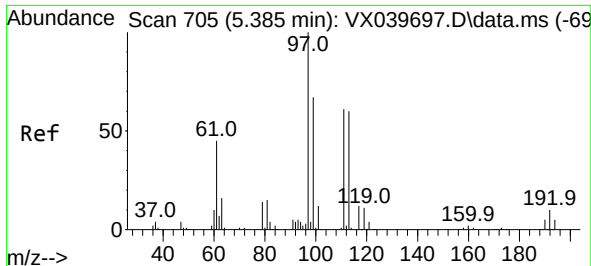

#35
Dibromofluoromethane
Concen: 47.316 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX039780.D
Acq: 16 Jan 2024 17:25




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-191-GW-148-150


Tgt Ion:113 Resp: 55932
Ion Ratio Lower Upper
113 100
111 102.5 82.9 124.3
192 16.8 13.3 19.9

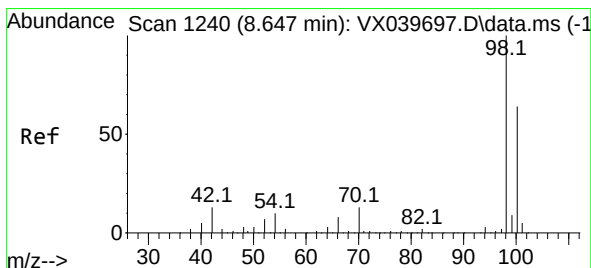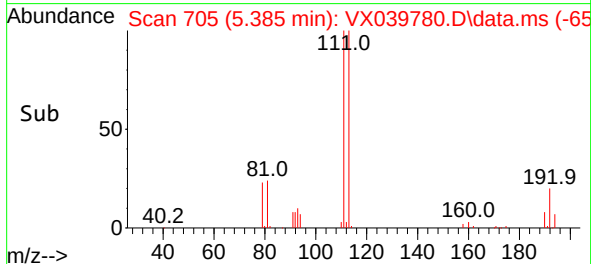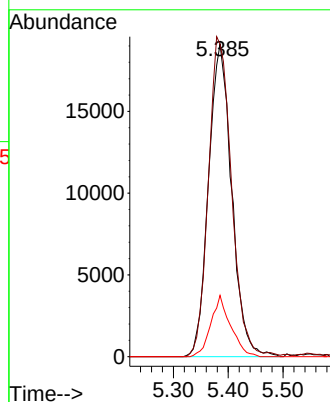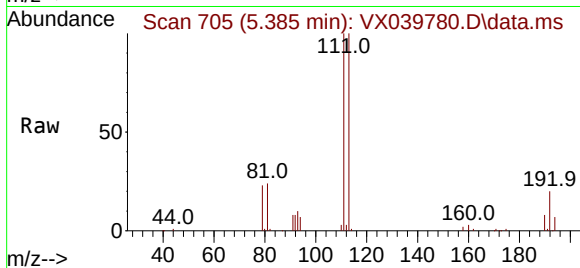

#50
Toluene-d8
Concen: 48.108 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX039780.D
Acq: 16 Jan 2024 17:25

Tgt Ion: 98 Resp: 214480
Ion Ratio Lower Upper
98 100
100 64.6 53.1 79.7


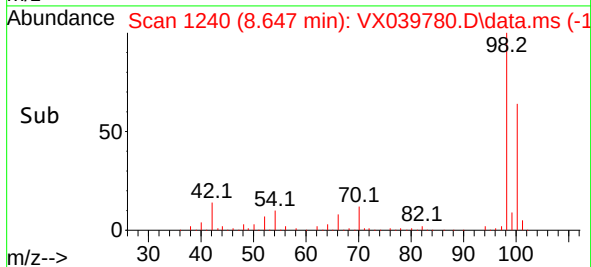
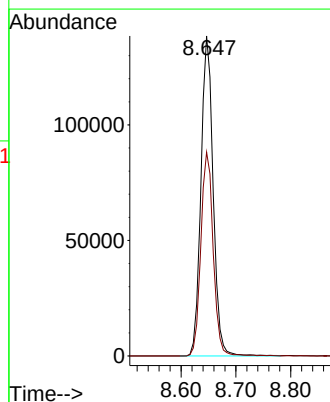
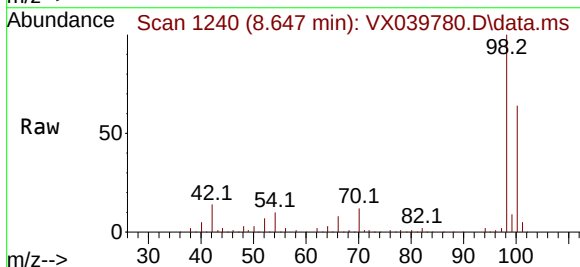


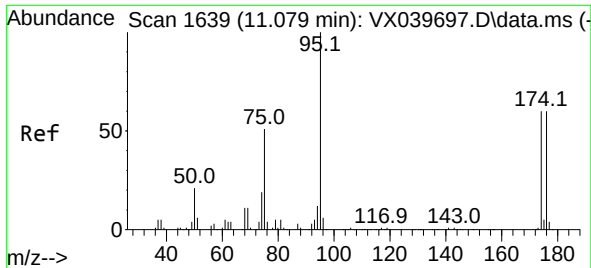

#62
4-Bromofluorobenzene
Concen: 50.467 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX039780.D
Acq: 16 Jan 2024 17:25




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-191-GW-148-150


Tgt Ion: 95 Resp: 87985
Ion Ratio Lower Upper
95 100
174 69.1 0.0 135.6
176 66.6 0.0 131.0

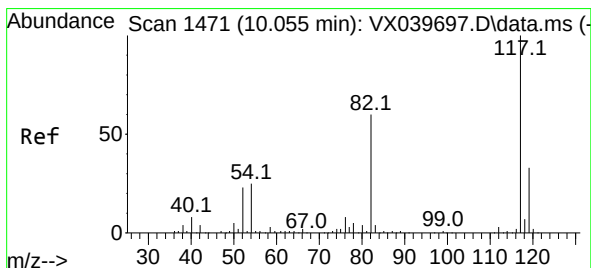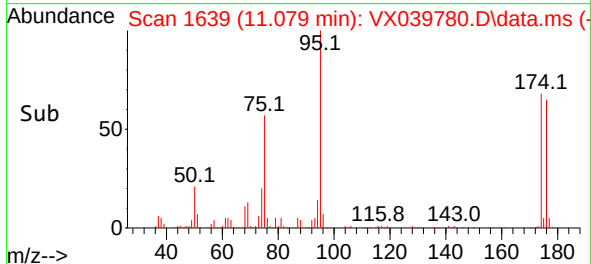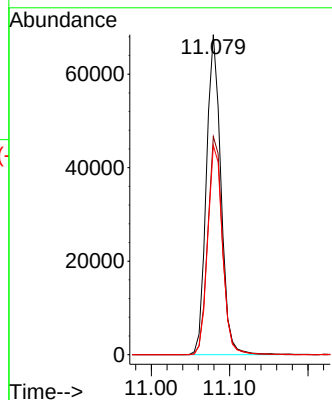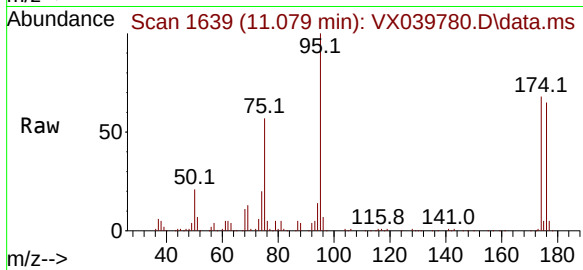

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX039780.D
Acq: 16 Jan 2024 17:25

Tgt Ion: 117 Resp: 170741
Ion Ratio Lower Upper
117 100
82 57.2 46.2 69.4
119 33.2 25.5 38.3

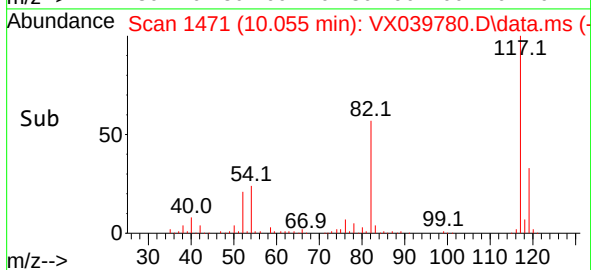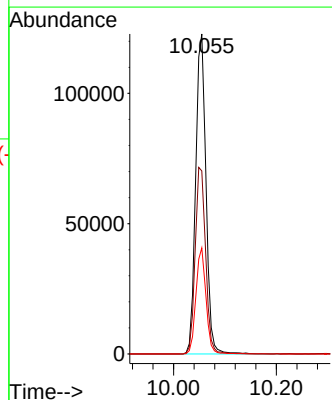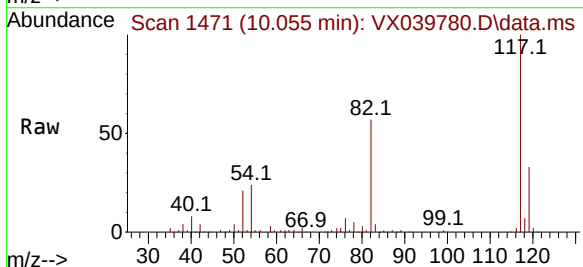

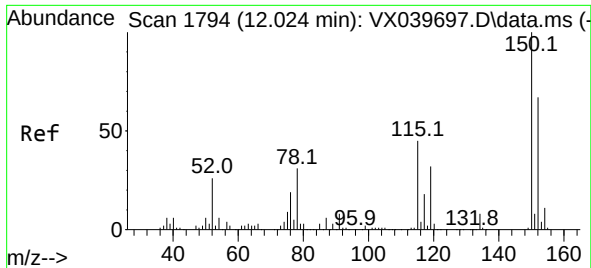

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX039780.D


Acq: 16 Jan 2024 17:25

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB-191-GW-148-150

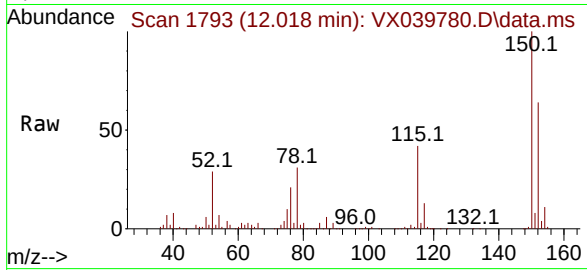

Tgt Ion:152 Resp: 83399

Ion Ratio Lower Upper

152 100

115 64.6 43.3 129.9

150 157.7 0.0 345.0

