

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX011719\  
 Data File : VX007080.D  
 Acq On : 17 Jan 2019 11:23  
 Operator : JC/SP  
 Sample : VX0117MBL01  
 Misc : 5.00µ/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0117MBL01

Quant Time: Jan 18 05:41:25 2019  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Jan 08 14:06:59 2019  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) Pentafluorobenzene      | 5.66  | 168  | 562213   | 50.00 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 6.86  | 114  | 873527   | 50.00 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 10.12 | 117  | 826571   | 50.00 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 12.08 | 152  | 405627   | 50.00 | ug/l  | 0.00     |

| System Monitoring Compounds | R.T.  | QIon | Response | Conc  | Units   | Dev(Min) |
|-----------------------------|-------|------|----------|-------|---------|----------|
| 33) 1,2-Dichloroethane-d4   | 6.07  | 65   | 306279   | 52.13 | ug/l    | 0.00     |
| Spiked Amount 50.000        |       |      | Recovery | =     | 104.26% |          |
| 35) Dibromofluoromethane    | 5.51  | 113  | 268847   | 48.06 | ug/l    | 0.00     |
| Spiked Amount 50.000        |       |      | Recovery | =     | 96.12%  |          |
| 50) Toluene-d8              | 8.71  | 98   | 1053596  | 51.46 | ug/l    | 0.00     |
| Spiked Amount 50.000        |       |      | Recovery | =     | 102.92% |          |
| 62) 4-Bromofluorobenzene    | 11.13 | 95   | 377034   | 52.82 | ug/l    | 0.00     |
| Spiked Amount 50.000        |       |      | Recovery | =     | 105.64% |          |


| Target Compounds | Qvalue |
|------------------|--------|
|------------------|--------|


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX011719\  
Data File : VX007080.D  
Acq On : 17 Jan 2019 11:23  
Operator : JC/SP  
Sample : VX0117MBL01  
Misc : 5.0g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0117MBL01

Quant Time: Jan 18 05:41:25 2019  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M  
Quant Title : SW846 8260  
QLast Update : Tue Jan 08 14:06:59 2019  
Response via : Initial Calibration

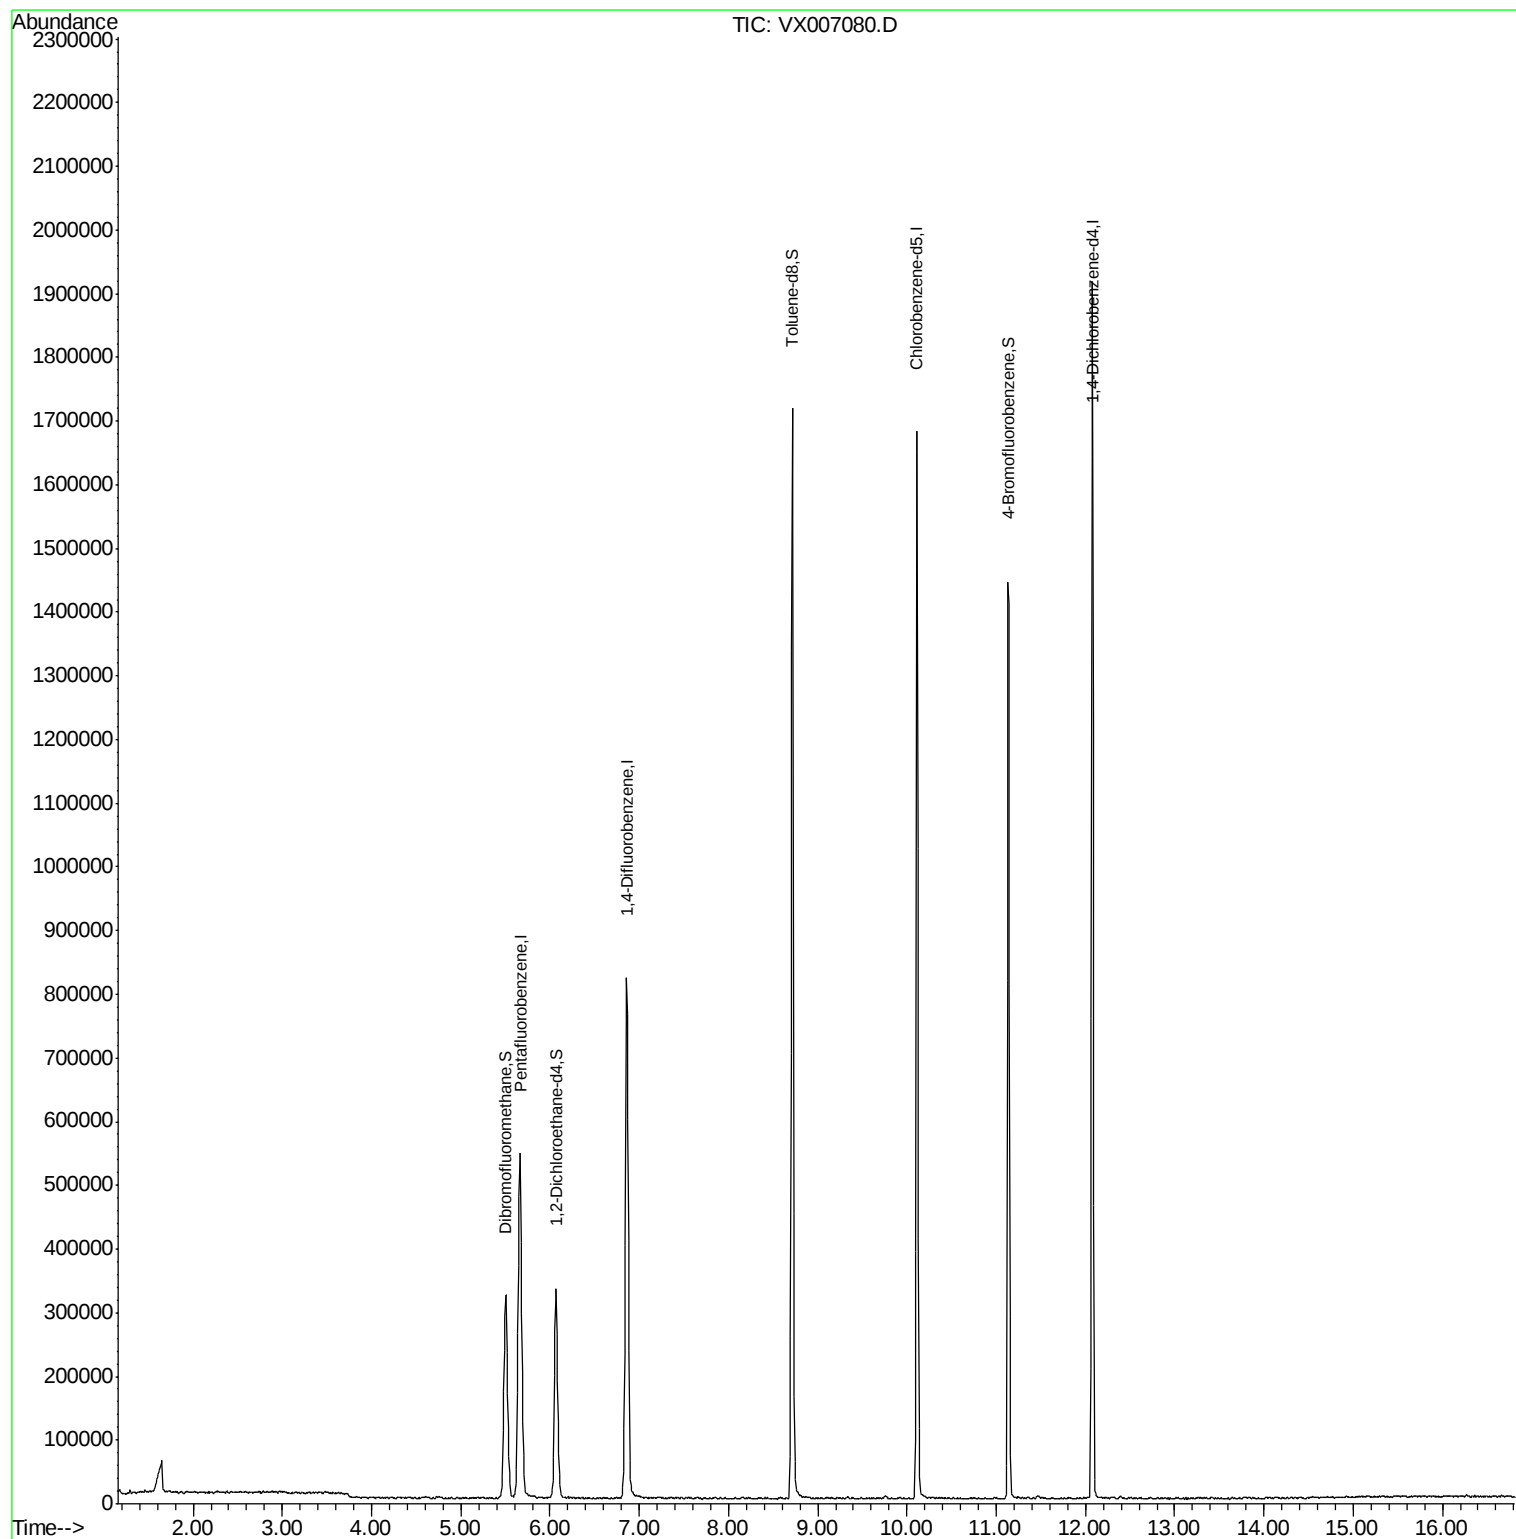

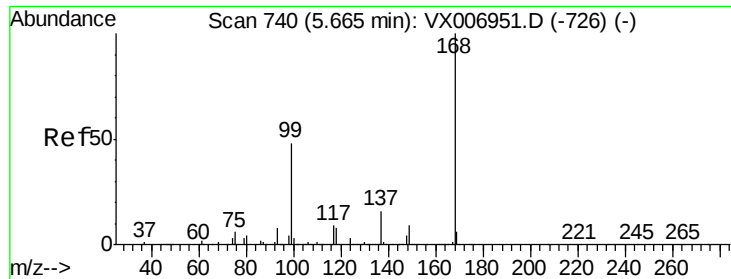

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 740

Delta R.T. -0.00 min

Lab File: VX007080.D

Acq: 17 Jan 2019 11:23

Instrument :

MSVOA\_X

ClientSampleId :


VX0117MBL01

Tot Ion:168 Resp: 562213

Ion Ratio Lower Upper

168 100

99 49.4 41.8 62.8

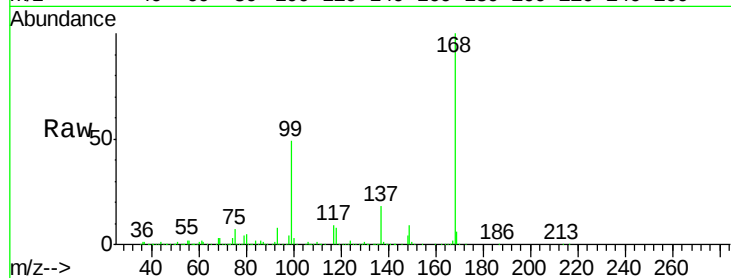

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66

200000

150000



100000

50000

0

Time-->

5.60 5.70 5.80

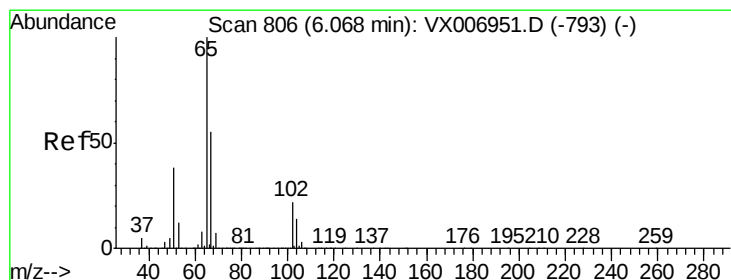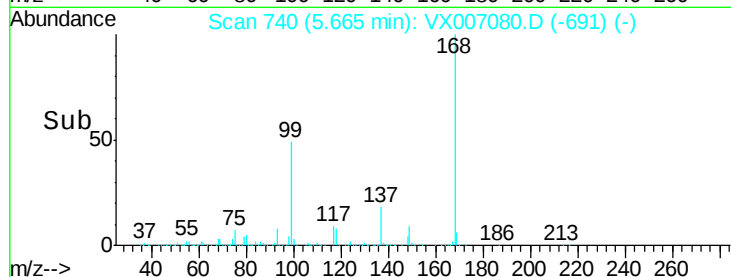

#33

1,2-Dichloroethane-d4

Concen: 52.127 ug/l

RT: 6.07 min Scan# 806

Delta R.T. -0.00 min

Lab File: VX007080.D


Acq: 17 Jan 2019 11:23

Tgt Ion: 65 Resp: 306279

Ion Ratio Lower Upper

65 100

67 53.3 0.0 105.0

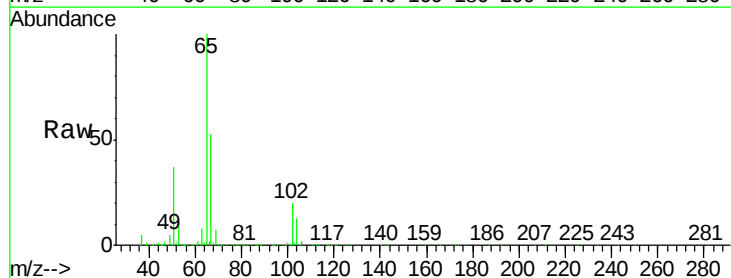

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07


100000


50000

0

Time-->

5.90 6.00 6.10 6.20

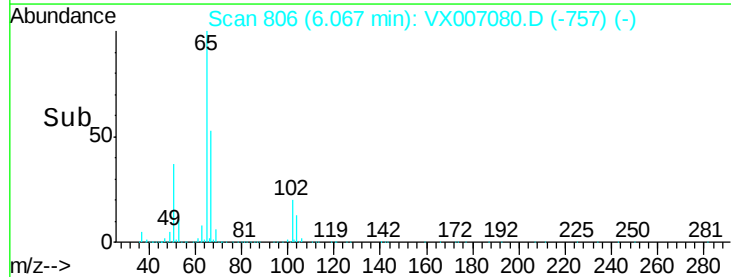

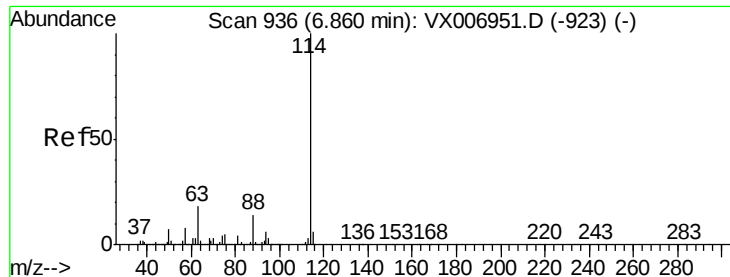

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX007080.D

Acq: 17 Jan 2019 11:23

Instrument :

MSVOA\_X

ClientSampleId :

VX0117MBL01


Tot Ion:114 Resp: 873527

Ion Ratio Lower Upper

114 100

63 18.6 0.0 34.8




88 14.9 0.0 28.8

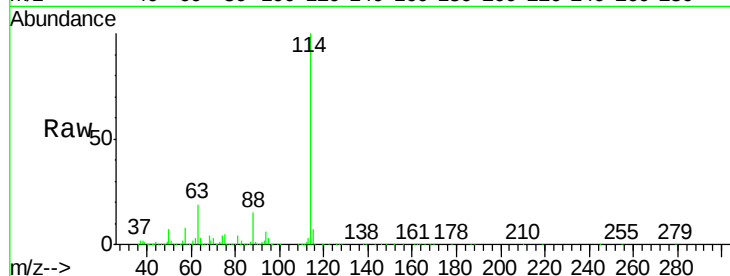

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

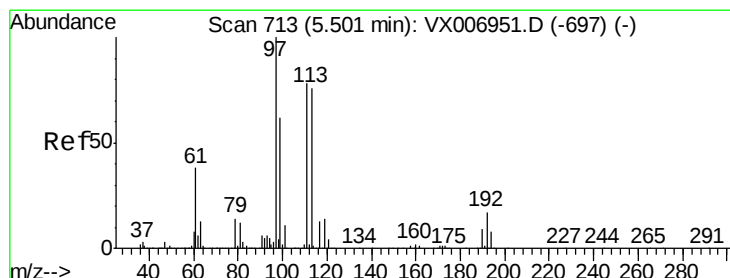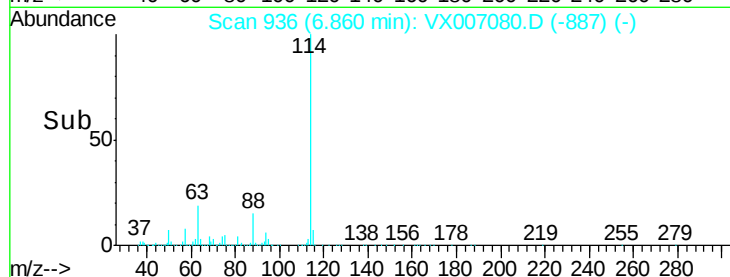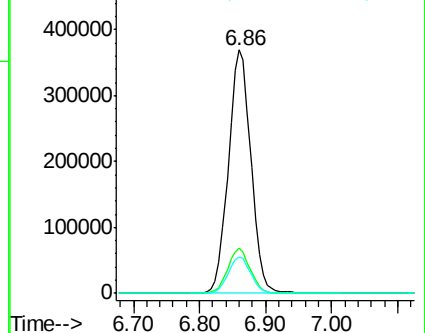

#35

Dibromofluoromethane

Concen: 48.060 ug/l

RT: 5.51 min Scan# 714

Delta R.T. 0.01 min

Lab File: VX007080.D

Acq: 17 Jan 2019 11:23


Tgt Ion:113 Resp: 268847

Ion Ratio Lower Upper

113 100

111 103.1 81.6 122.4



192 23.1 16.7 25.1

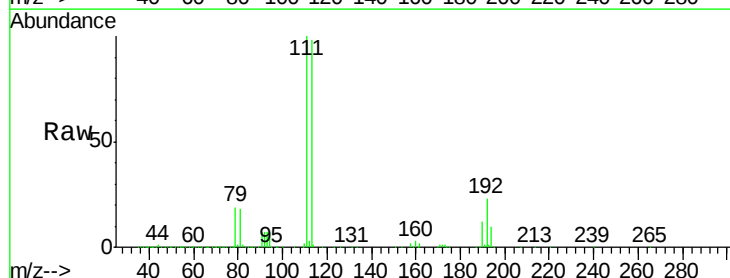


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

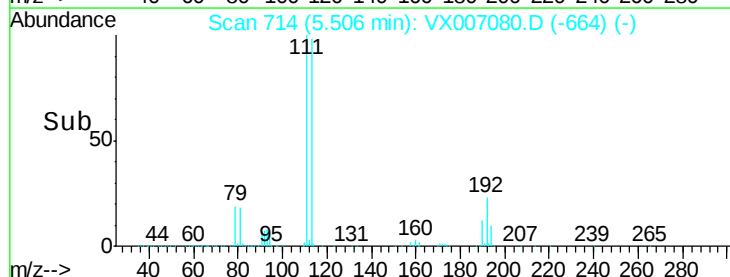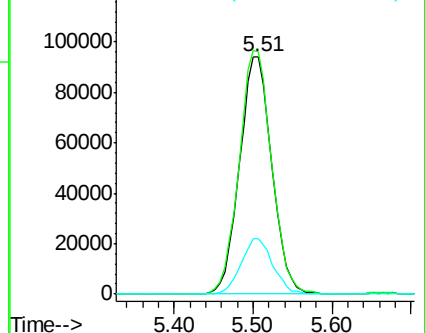

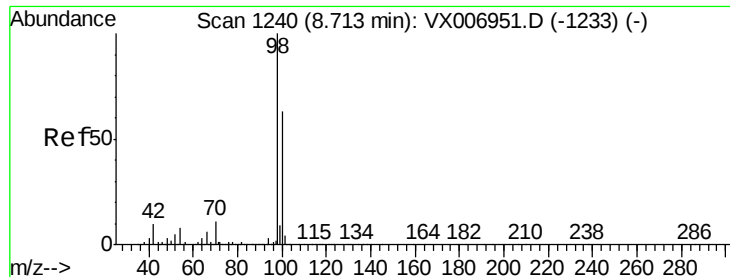

#50

Toluene-d8

Concen: 51.456 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX007080.D

Acq: 17 Jan 2019 11:23

Instrument :

MSVOA\_X

ClientSampleId :


VX0117MBL01

Tot Ion: 98 Resp: 1053596

Ion Ratio Lower Upper

98 100

100 63.6 52.0 78.0

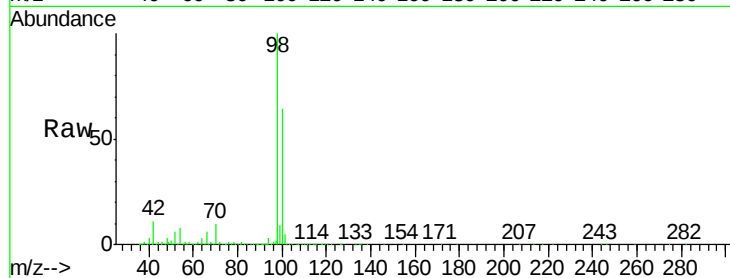

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

8.71

600000



400000

200000

0

Time-->

8.60 8.70 8.80 8.90

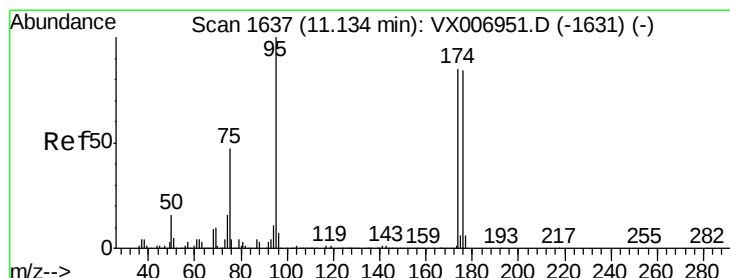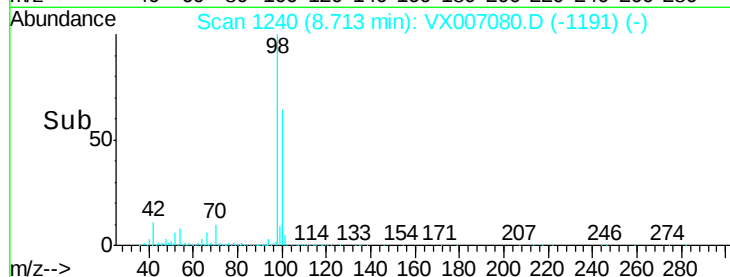

#62

4-Bromofluorobenzene

Concen: 52.818 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX007080.D

Acq: 17 Jan 2019 11:23


Tgt Ion: 95 Resp: 377034

Ion Ratio Lower Upper

95 100

174 92.5 0.0 182.2

176 88.7 0.0 178.8

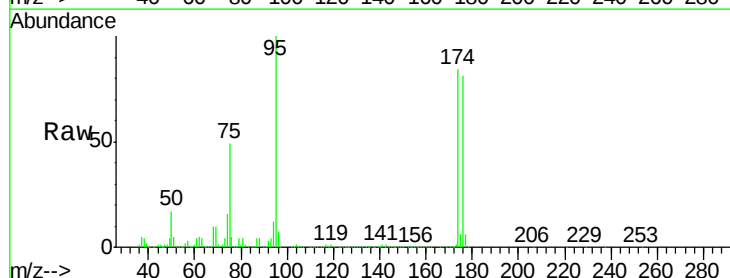

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

400000

300000


200000


100000

0

Time-->

11.10 11.20




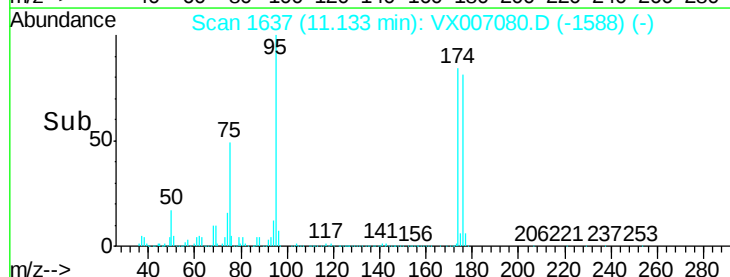


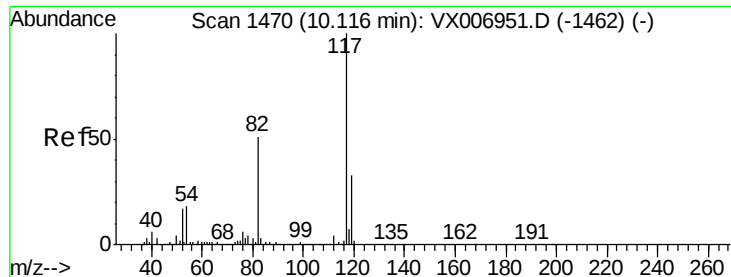

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.12 min Scan# 1470  
Delta R.T. -0.00 min  
Lab File: VX007080.D  
Acq: 17 Jan 2019 11:23

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0117MBL01

Tot Ion:117 Resp: 826571  
Ion Ratio Lower Upper  
117 100  
82 49.5 41.0 61.6  
119 32.5 25.4 38.0

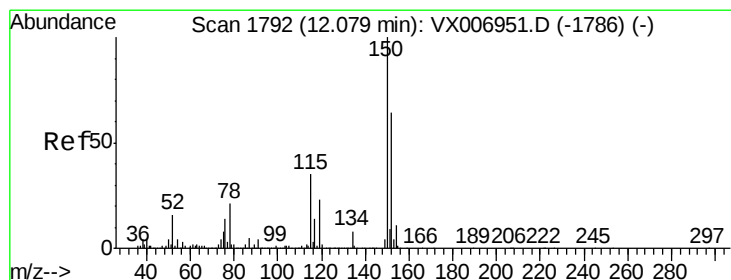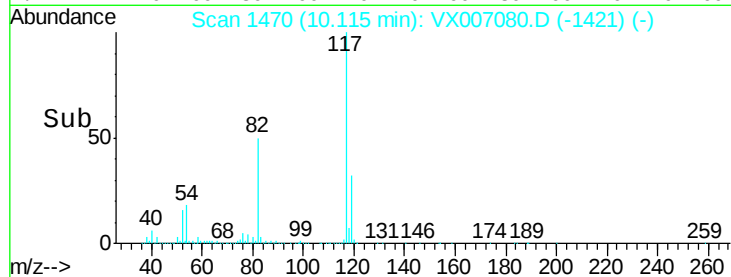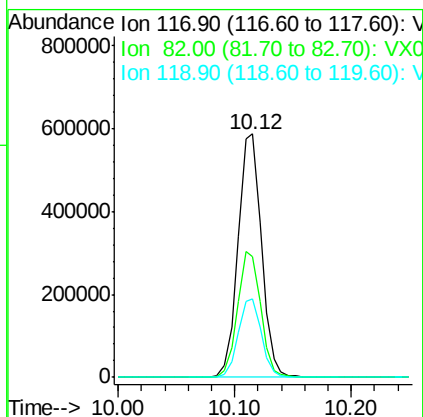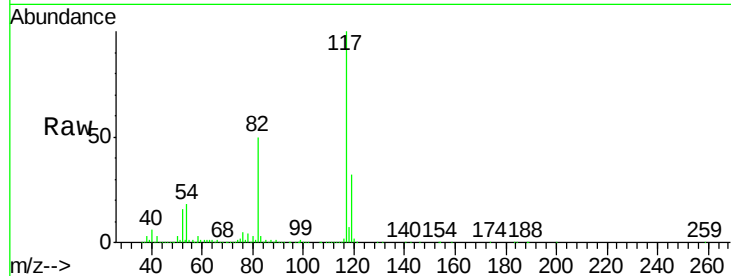

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.08 min Scan# 1792  
Delta R.T. -0.00 min  
Lab File: VX007080.D  
Acq: 17 Jan 2019 11:23

Tgt Ion:152 Resp: 405627  
Ion Ratio Lower Upper  
152 100  
115 54.6 39.1 117.2  
150 154.8 0.0 344.8

