


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX011720\
Data File : VX014642.D
Acq On : 17 Jan 2020 08:41
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010720W.M
Title : SW846 8260
Last Update : Tue Jan 07 15:54:41 2020

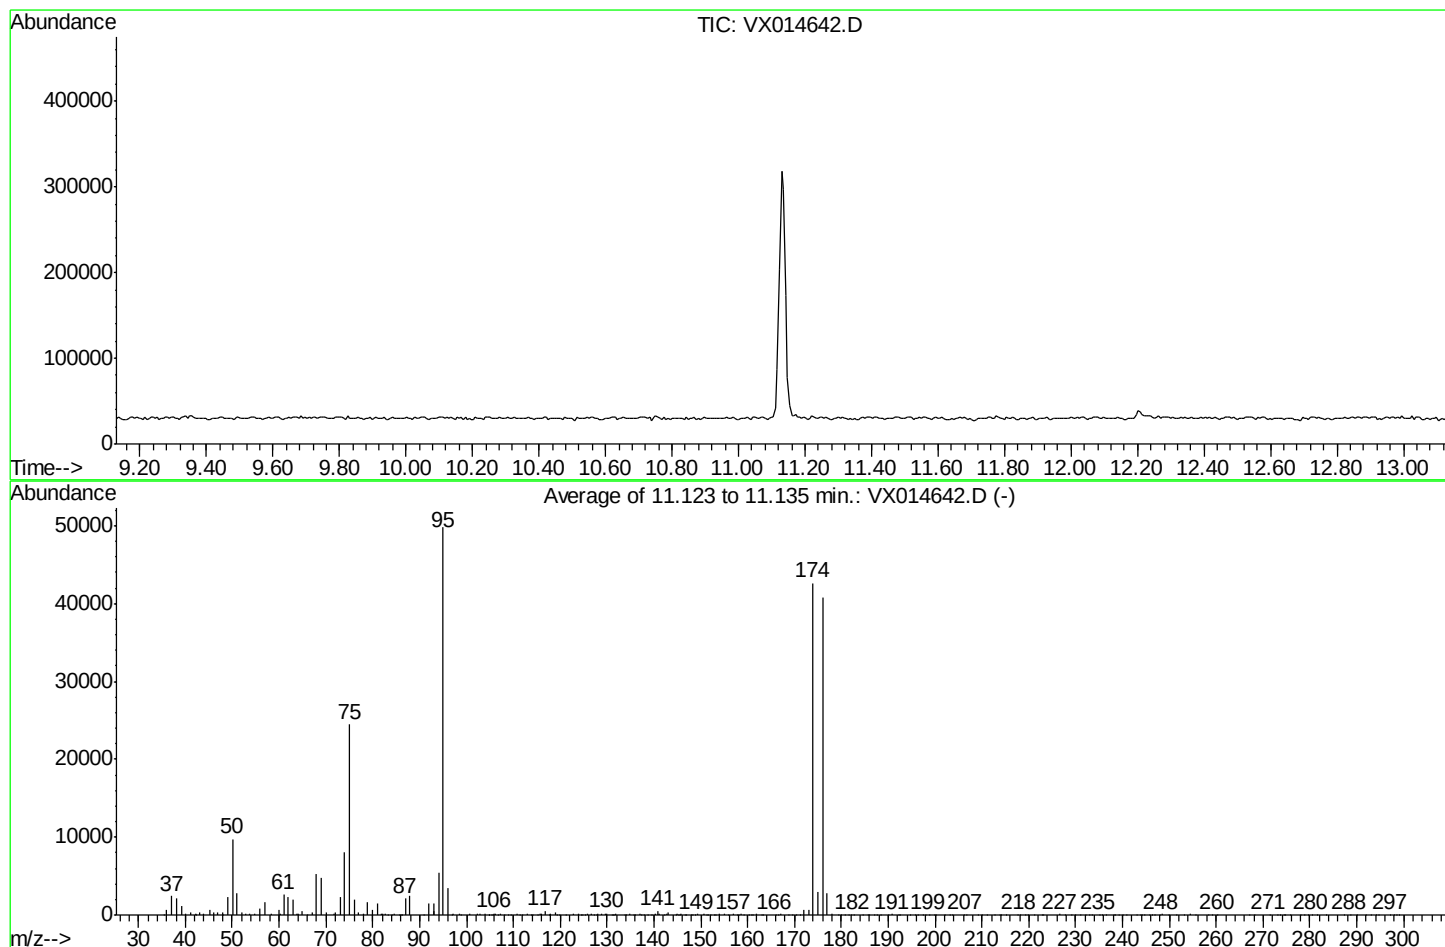

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	9751	PASS
75	95	30	60	49.2	24475	PASS
95	95	100	100	100.0	49792	PASS
96	95	5	9	6.9	3451	PASS
173	174	0.00	2	1.5	624	PASS
174	95	50	100	85.7	42663	PASS
175	174	5	9	7.1	3028	PASS
176	174	95	101	95.7	40816	PASS
177	176	5	9	6.8	2761	PASS