
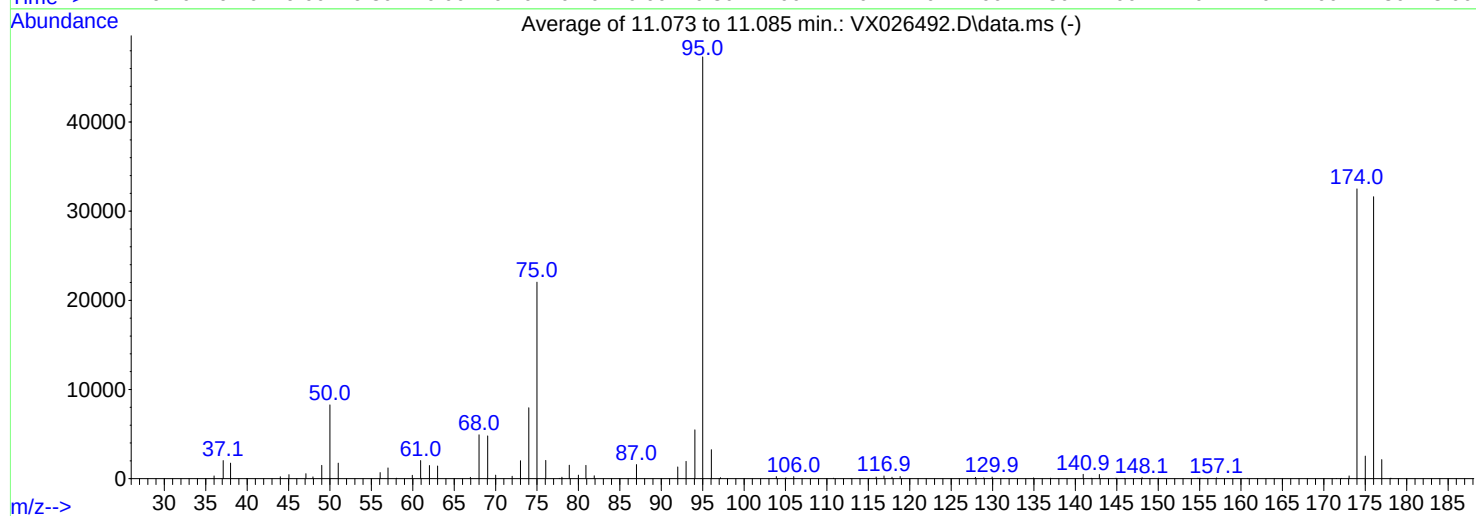


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011722\
 Data File : VX026492.D
 Acq On : 17 Jan 2022 16:48
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 LabSampleId :
 VSTDCCC050

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Title : SW846 8260
 Last Update : Tue Jan 11 14:45:13 2022

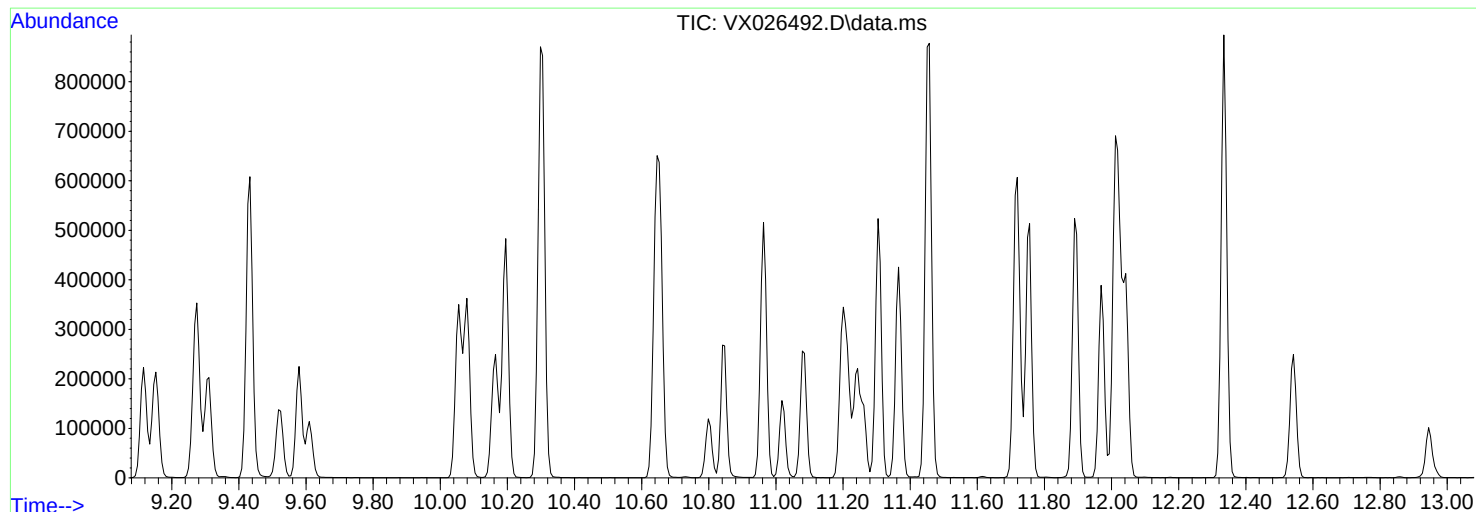

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	8278	PASS
75	95	30	60	46.6	22035	PASS
95	95	100	100	100.0	47312	PASS
96	95	5	9	6.9	3248	PASS
173	174	0.00	2	0.9	302	PASS
174	95	50	100	68.7	32509	PASS
175	174	5	9	7.8	2534	PASS
176	174	95	101	97.3	31632	PASS
177	176	5	9	6.7	2133	PASS