



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011723\
Data File : VX033752.D
Acq On : 17 Jan 2023 09:47
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Title : SW846 8260
Last Update : Wed Jan 11 14:48:42 2023

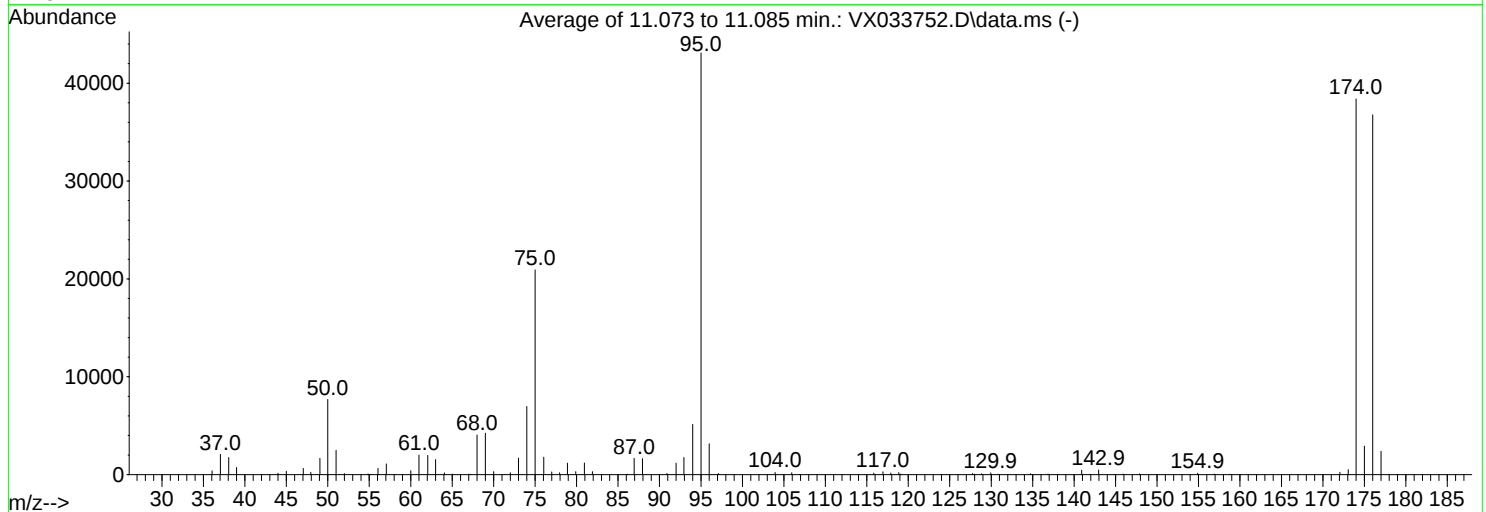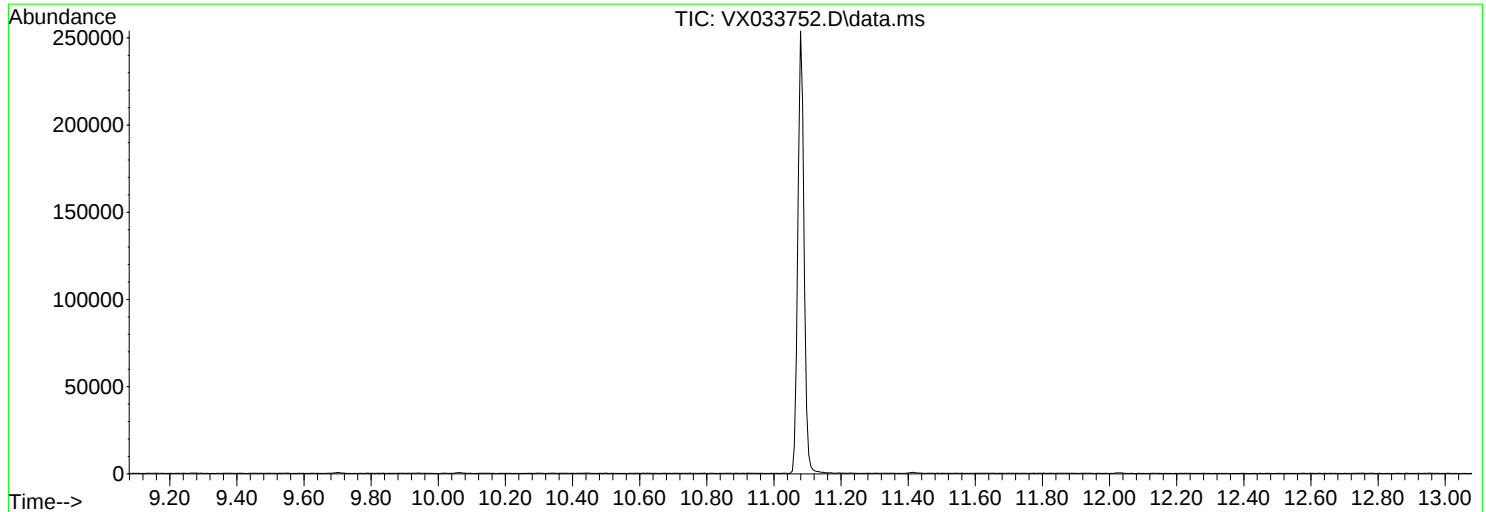

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	7679	PASS
75	95	30	60	48.6	20936	PASS
95	95	100	100	100.0	43101	PASS
96	95	5	9	7.3	3159	PASS
173	174	0.00	2	1.3	512	PASS
174	95	50	100	89.1	38384	PASS
175	174	5	9	7.6	2904	PASS
176	174	95	101	95.8	36773	PASS
177	176	5	9	6.5	2388	PASS