

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011724\
 Data File : VX039792.D
 Acq On : 17 Jan 2024 11:22
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Jan 18 02:39:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 11 03:51:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	90584	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	167010	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	162190	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	78463	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	69350	45.703	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	91.400%
35) Dibromofluoromethane	5.385	113	54924	48.826	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.660%
50) Toluene-d8	8.647	98	208502	49.145	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.300%
62) 4-Bromofluorobenzene	11.079	95	82107	49.490	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	98.980%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011724\
Data File : VX039792.D
Acq On : 17 Jan 2024 11:22
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Jan 18 02:39:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 11 03:51:26 2024
Response via : Initial Calibration

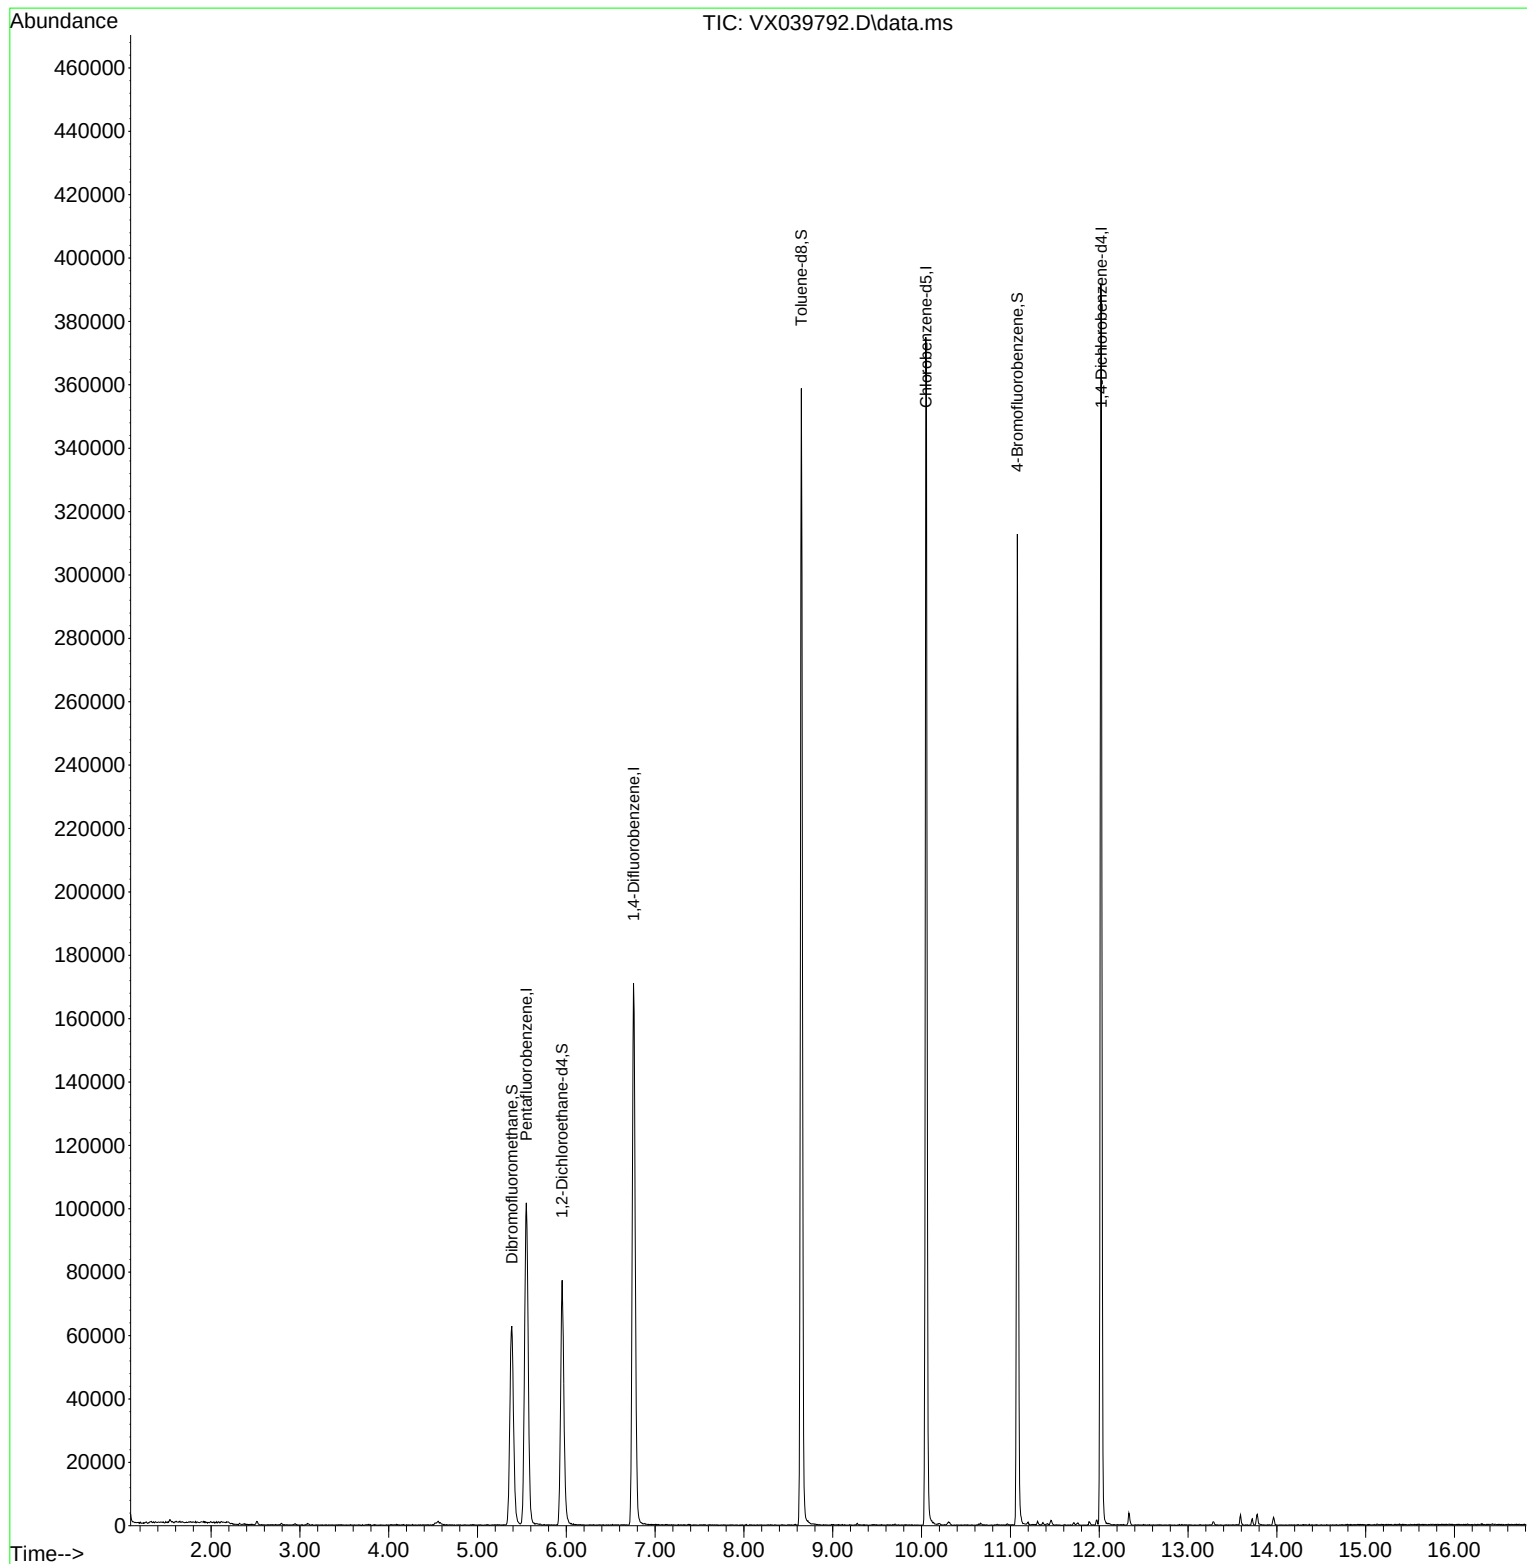

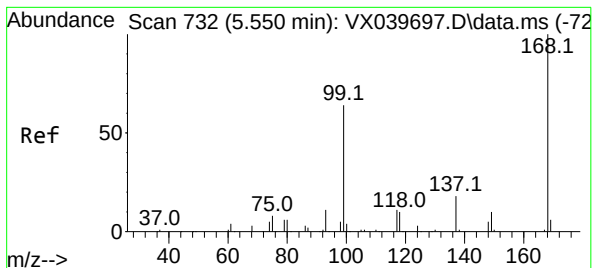

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 71

Delta R.T. -0.000 min

Lab File: VX039792.D

Acq: 17 Jan 2024 11:22

Instrument :

MSVOA_X

ClientSampleId :





IBLK

Tgt Ion:168 Resp: 90584

Ion Ratio Lower Upper

168 100

99 67.2 56.6 85.0

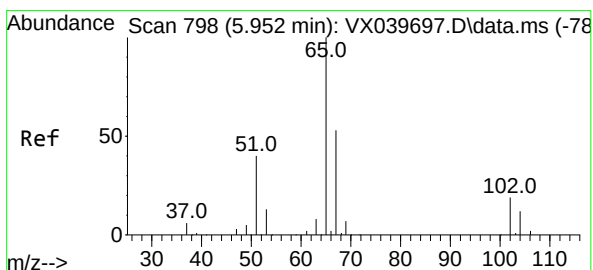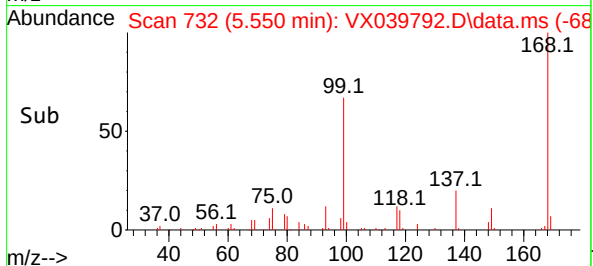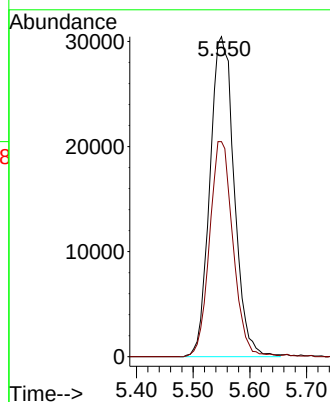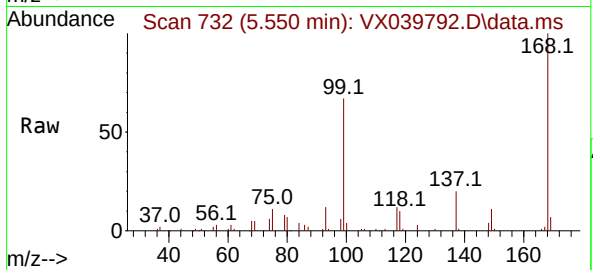

#33

1,2-Dichloroethane-d4

Concen: 45.703 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.000 min

Lab File: VX039792.D




Acq: 17 Jan 2024 11:22


Tgt Ion: 65 Resp: 69350

Ion Ratio Lower Upper

65 100

67 53.2 0.0 100.2


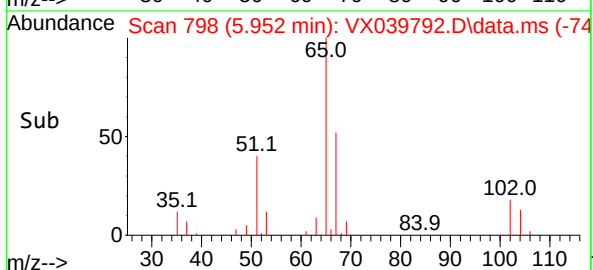
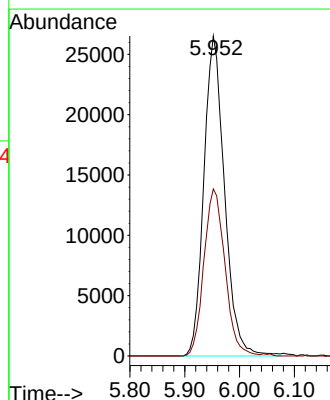
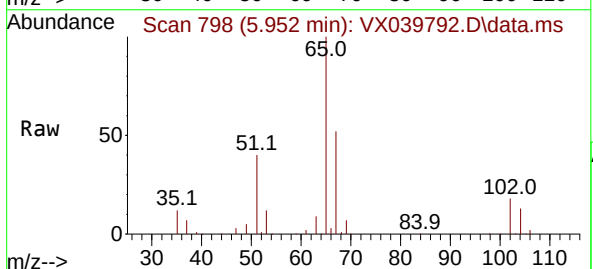


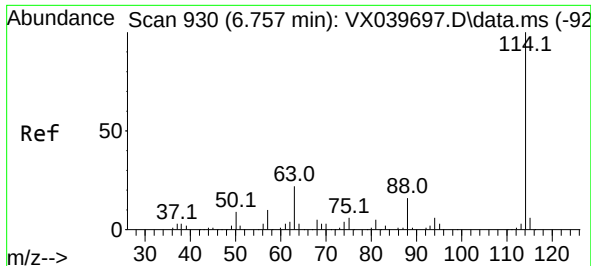

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX039792.D
Acq: 17 Jan 2024 11:22




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 167010
Ion Ratio Lower Upper
114 100
63 23.2 0.0 45.0
88 17.0 0.0 36.6

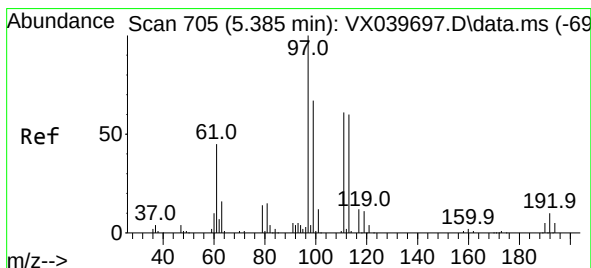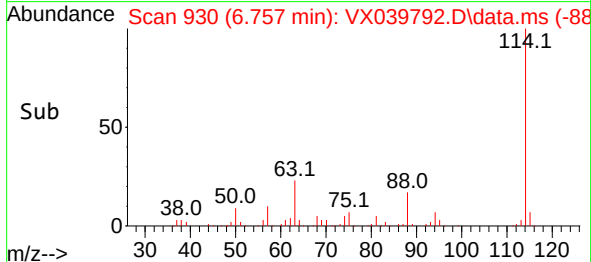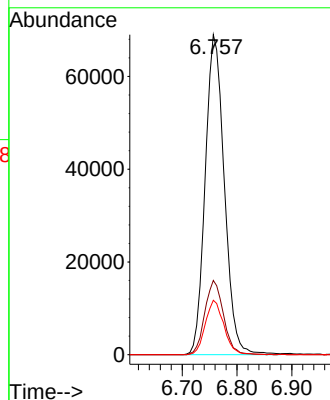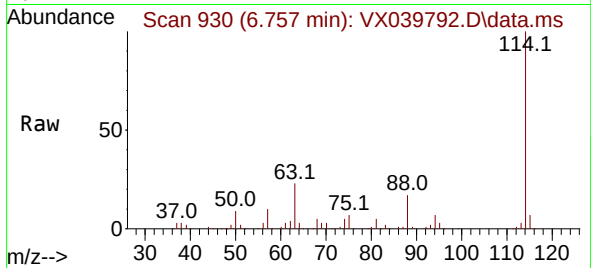

#35
Dibromofluoromethane
Concen: 48.826 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX039792.D
Acq: 17 Jan 2024 11:22

Tgt Ion:113 Resp: 54924
Ion Ratio Lower Upper
113 100
111 103.2 82.9 124.3
192 16.3 13.3 19.9


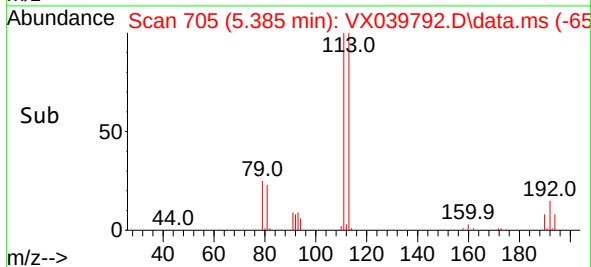
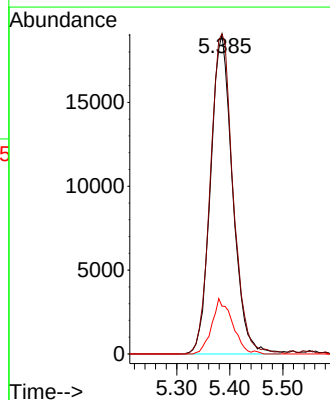
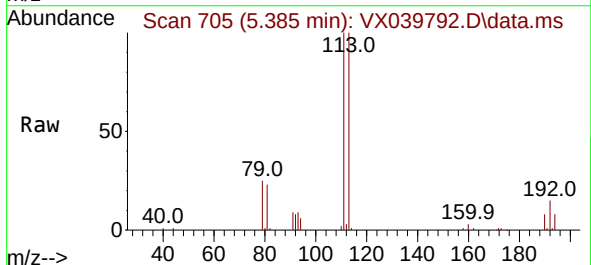


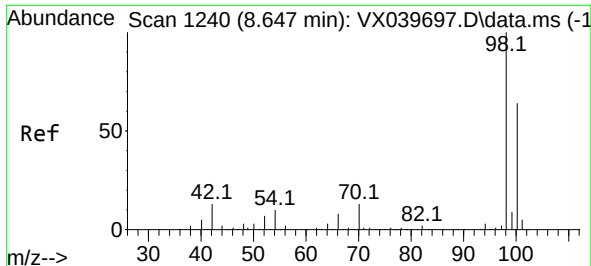

#50
Toluene-d8
Concen: 49.145 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX039792.D
Acq: 17 Jan 2024 11:22




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 208502
Ion Ratio Lower Upper
98 100
100 63.2 53.1 79.7

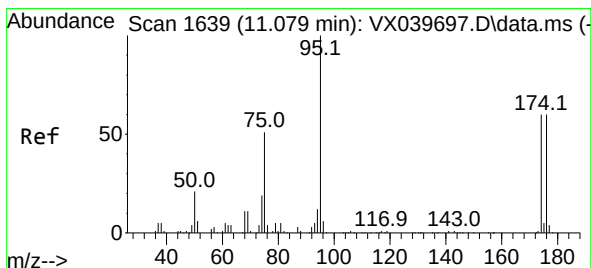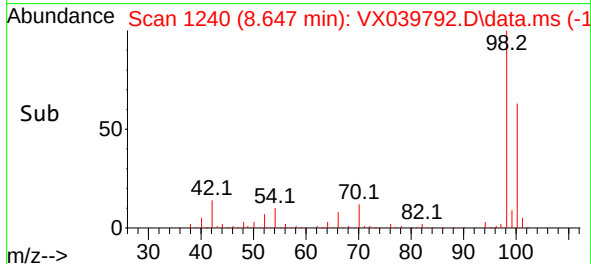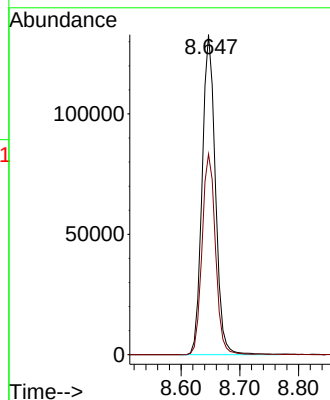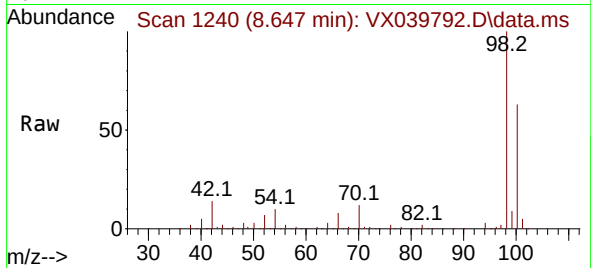

#62
4-Bromofluorobenzene
Concen: 49.490 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX039792.D
Acq: 17 Jan 2024 11:22

Tgt Ion: 95 Resp: 82107
Ion Ratio Lower Upper
95 100
174 69.2 0.0 135.6
176 67.1 0.0 131.0

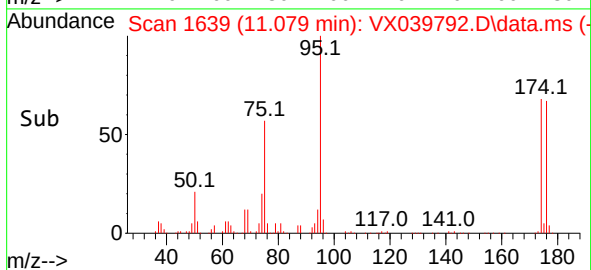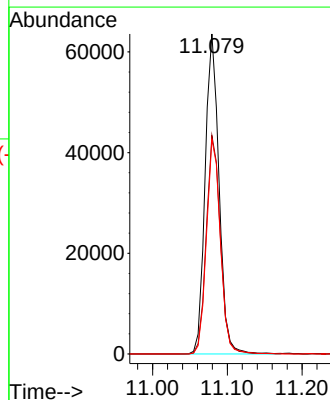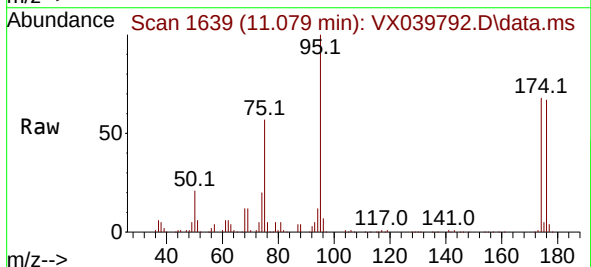

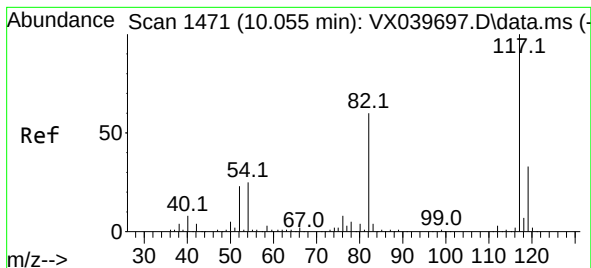

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.049 min Scan# 1471

Delta R.T. -0.006 min

Lab File: VX039792.D

Acq: 17 Jan 2024 11:22

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt Ion:117 Resp: 162190

Ion Ratio Lower Upper

117 100

82 61.6 46.2 69.4

119 31.7 25.5 38.3

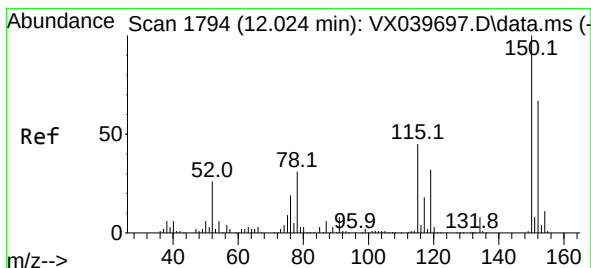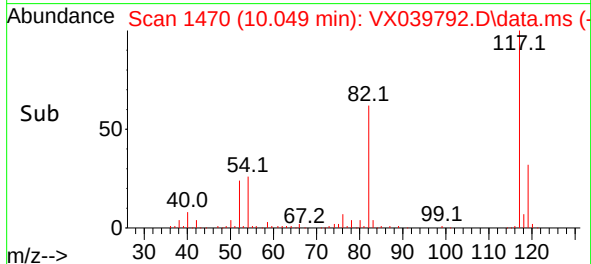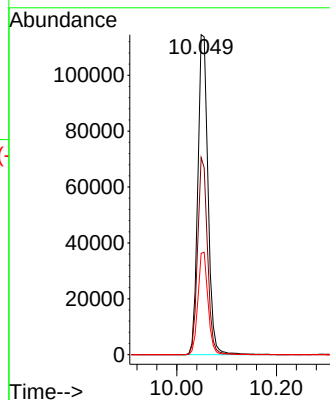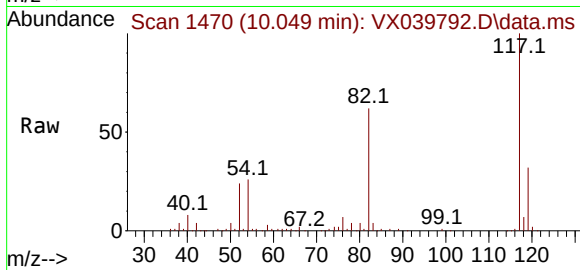

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. -0.000 min

Lab File: VX039792.D

Acq: 17 Jan 2024 11:22

Tgt Ion:152 Resp: 78463

Ion Ratio Lower Upper

152 100

115 64.5 43.3 129.9

150 157.1 0.0 345.0

