
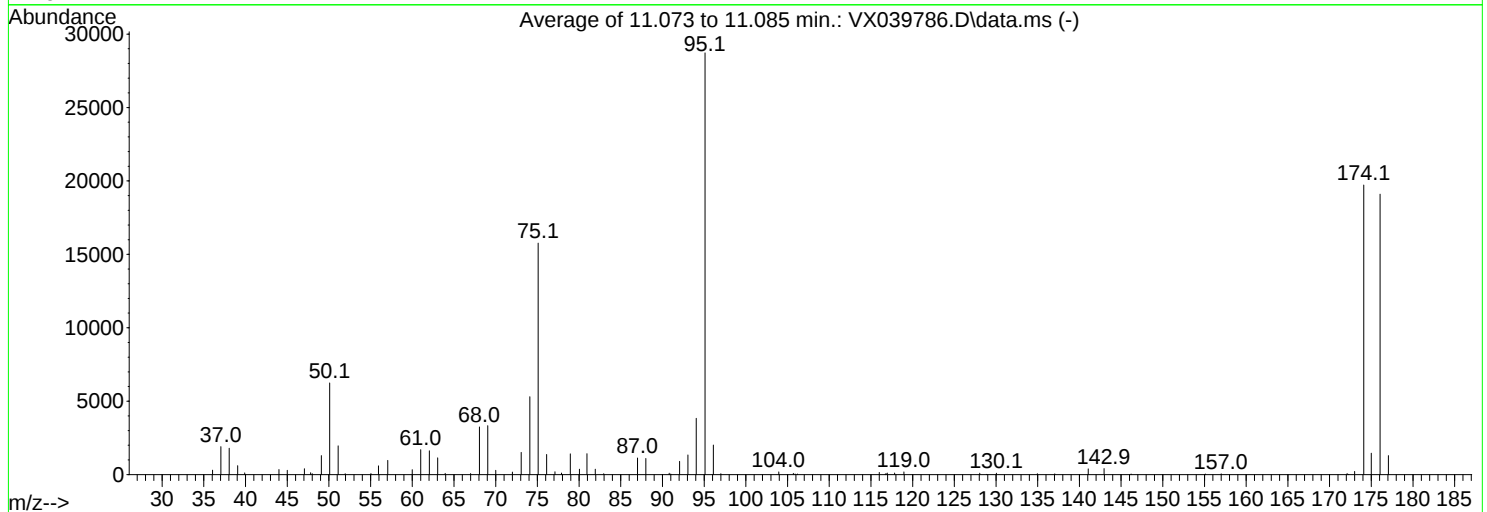


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX011724\
Data File : VX039786.D
Acq On : 17 Jan 2024 08:42
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
Title : SW846 8260
Last Update : Thu Jan 11 03:51:26 2024

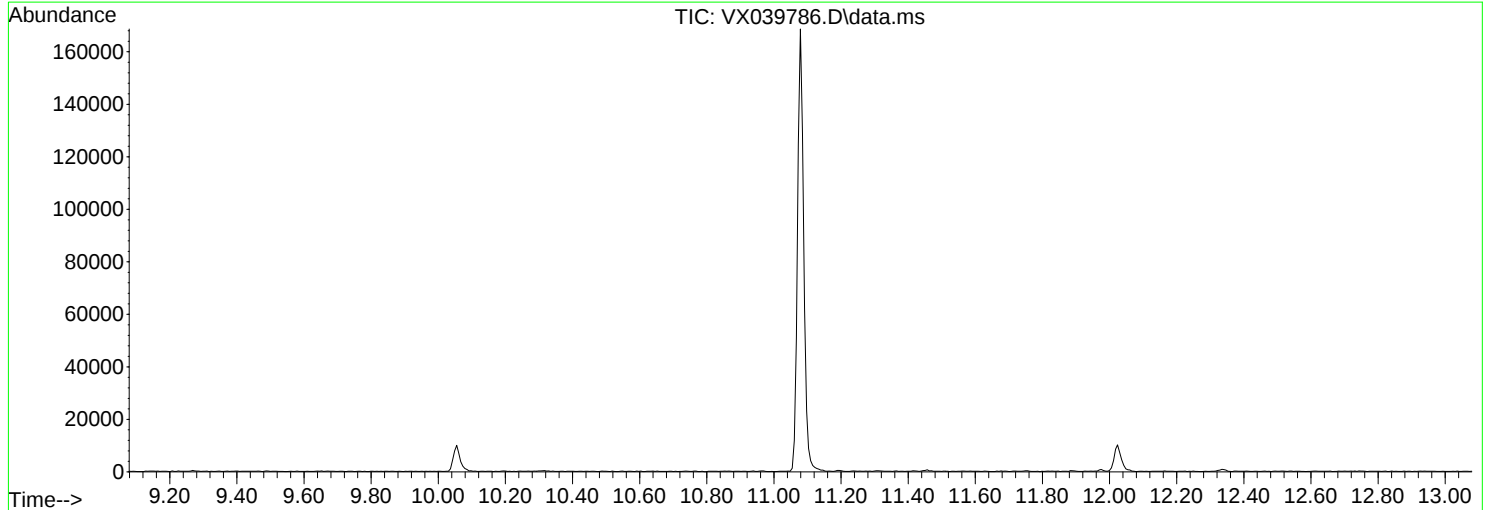

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	6244	PASS
75	95	30	60	54.9	15766	PASS
95	95	100	100	100.0	28723	PASS
96	95	5	9	7.0	2019	PASS
173	174	0.00	2	1.1	215	PASS
174	95	50	100	68.7	19726	PASS
175	174	5	9	7.4	1458	PASS
176	174	95	101	96.9	19105	PASS
177	176	5	9	6.8	1298	PASS