

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX011819\  
 Data File : VX007145.D  
 Acq On : 18 Jan 2019 19:48  
 Operator : JC/SP  
 Sample : K1199-06  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 SA-TW520-2327

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M

Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.617       | 68            | 76          | 79           | rVB4     | 32013          | 74465         | 2.94%           | 0.536%        |
| 2         | 3.026       | 301           | 307         | 314          | rVB      | 16390          | 39130         | 1.54%           | 0.282%        |
| 3         | 4.751       | 583           | 590         | 598          | rBV2     | 8733           | 27171         | 1.07%           | 0.196%        |
| 4         | 5.507       | 699           | 714         | 728          | rBV2     | 303357         | 871635        | 34.40%          | 6.276%        |
| 5         | 5.665       | 728           | 740         | 754          | rVV      | 514943         | 1446074       | 57.07%          | 10.413%       |
| 6         | 6.068       | 795           | 806         | 820          | rBV      | 317487         | 818028        | 32.28%          | 5.890%        |
| 7         | 6.860       | 927           | 936         | 950          | rBV      | 775466         | 1820353       | 71.84%          | 13.108%       |
| 8         | 8.714       | 1233          | 1240        | 1249         | rBV      | 1650437        | 2533902       | 100.00%         | 18.246%       |
| 9         | 10.110      | 1463          | 1469        | 1480         | rBV      | 1604120        | 2240010       | 88.40%          | 16.130%       |
| 10        | 11.140      | 1631          | 1638        | 1647         | rBV      | 1351372        | 1799118       | 71.00%          | 12.955%       |
| 11        | 12.079      | 1786          | 1792        | 1801         | rBV      | 1767761        | 2217731       | 87.52%          | 15.969%       |


Sum of corrected areas: 13887617

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX011819\  
Data File : VX007145.D  
Acq On : 18 Jan 2019 19:48  
Operator : JC/SP  
Sample : K1199-06  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW520-2327

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

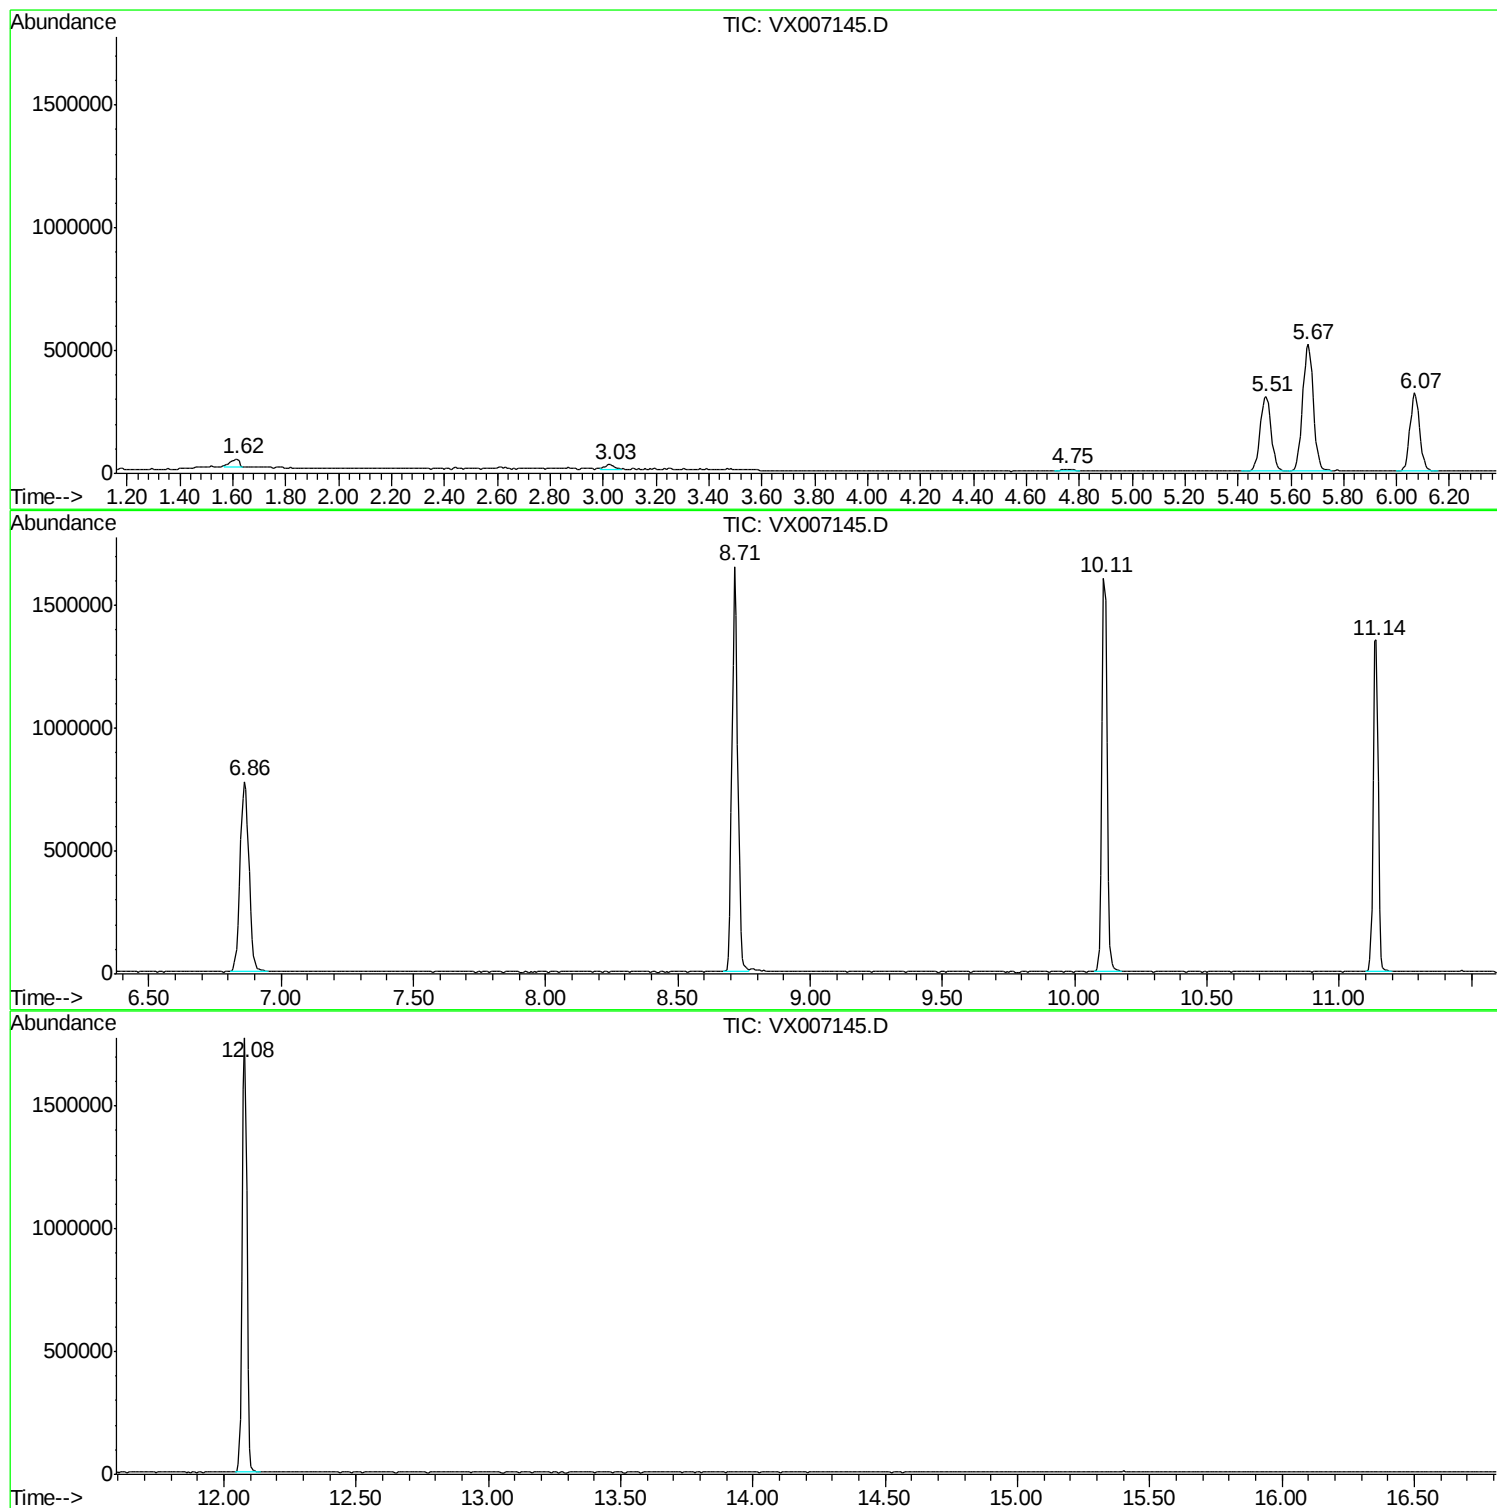

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX011819\  
Data File : VX007145.D  
Acq On : 18 Jan 2019 19:48  
Operator : JC/SP  
Sample : K1199-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW520-2327

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_X\DATA\VX011819\  
Data File : VX007145.D  
Acq On : 18 Jan 2019 19:48  
Operator : JC/SP  
Sample : K1199-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SA-TW520-2327

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X010819W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |